

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN053122\
 Data File : VN072652.D
 Acq On : 31 May 2022 14:18
 Operator : JC\MD
 Sample : N3068-01 200X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 WATER-DRUM

Quant Time: Jun 01 02:40:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N052622W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Fri May 27 05:07:24 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Bromochloromethane	7.657	128	24323	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	8.963	114	123472	30.000	ug/l	0.00
57) Chlorobenzene-d5	11.745	117	114988	30.000	ug/l	0.00
System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.434	65	71197	30.590	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	101.967%
60) 4-Bromofluorobenzene	12.727	95	43276	21.430	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	71.433%
63) Toluene-d8	10.439	98	196886	30.113	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	100.367%
Target Compounds						
					Qvalue	
3) Chloromethane	2.299	50	591	0.265	ug/l	94
47) n-amyl Acetate	12.351	43	170078	49.686	ug/l #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN053122\
Data File : VN072652.D
Acq On : 31 May 2022 14:18
Operator : JC\MD
Sample : N3068-01 200X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
WATER-DRUM

Quant Time: Jun 01 02:40:46 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N052622W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Fri May 27 05:07:24 2022
Response via : Initial Calibration




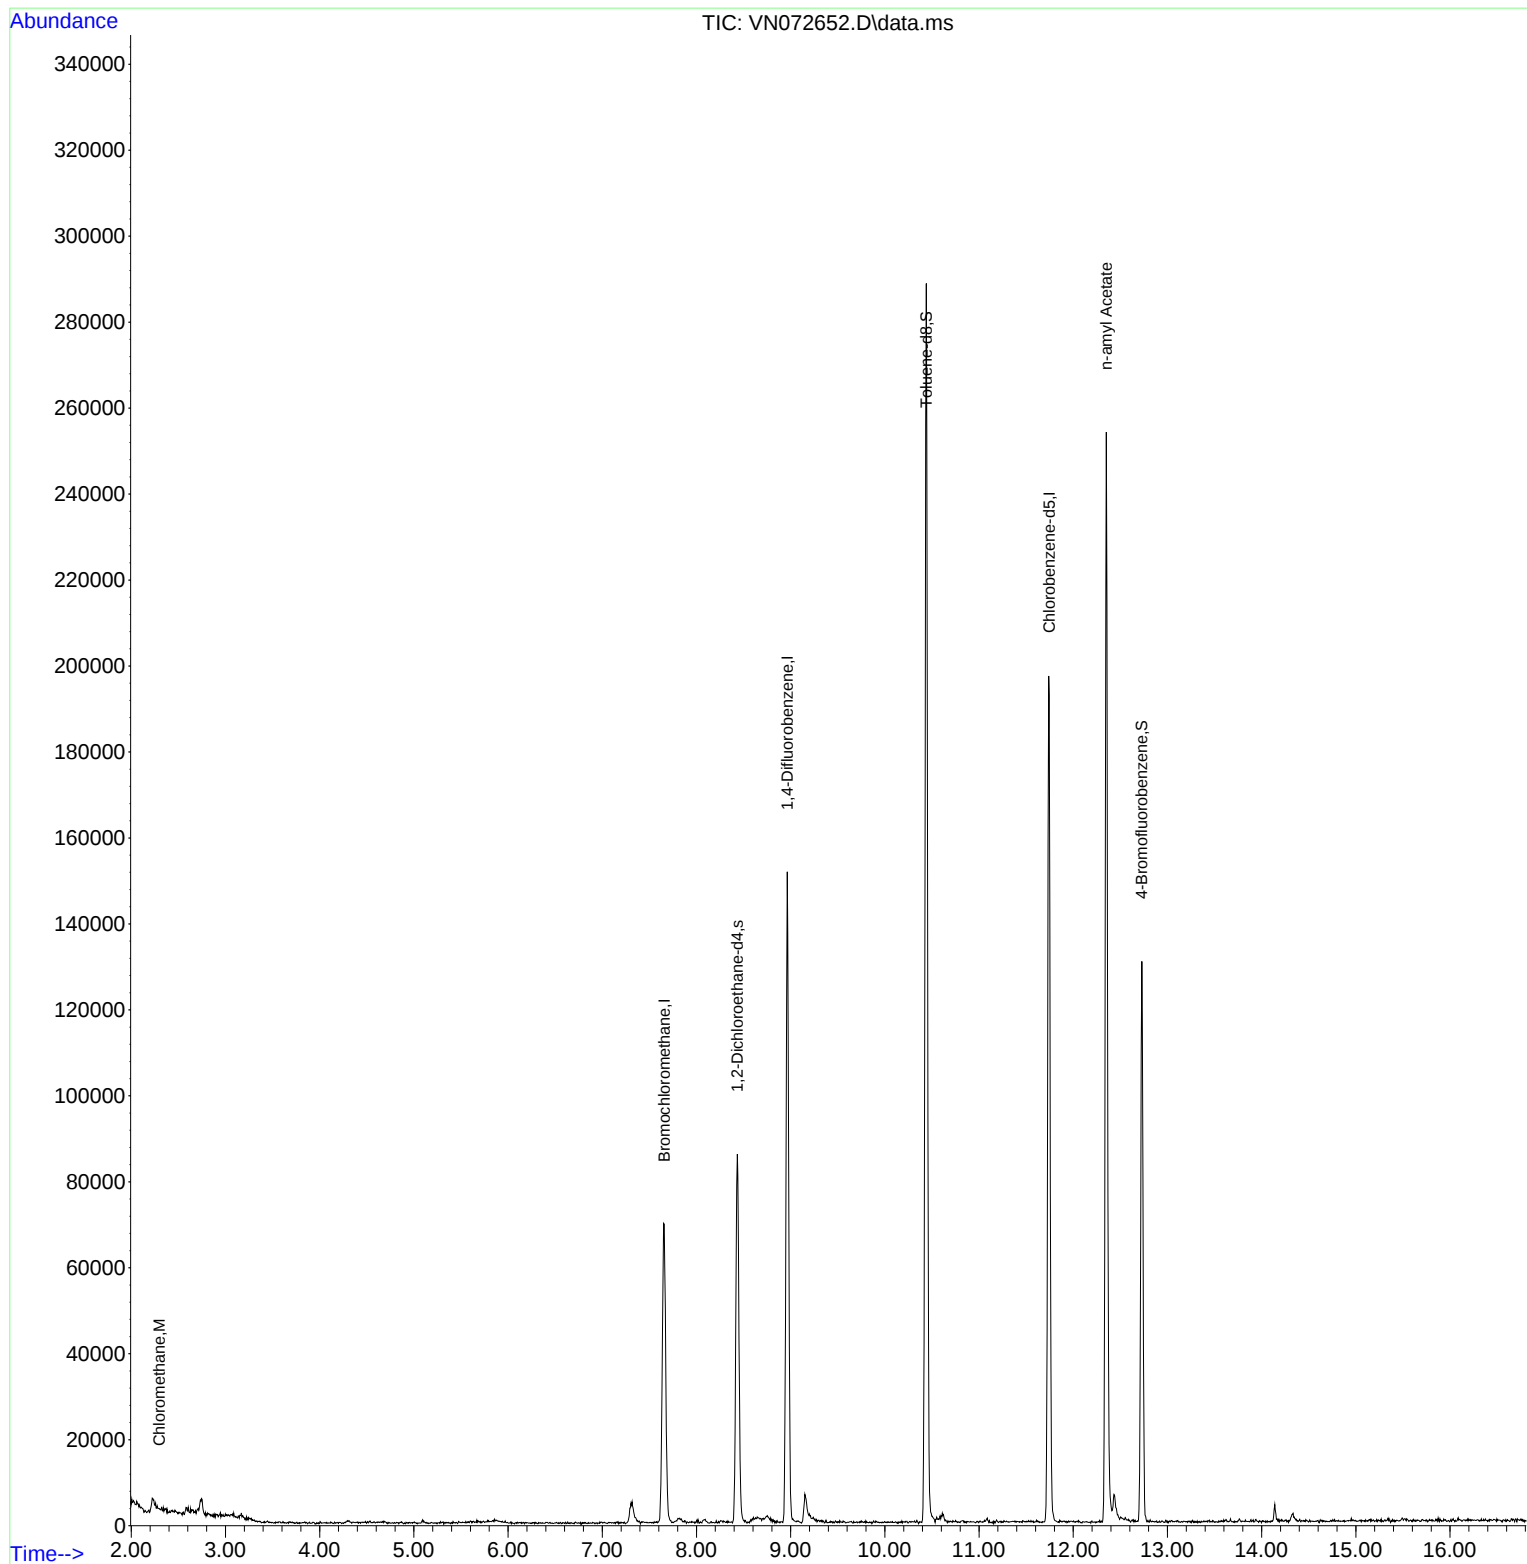


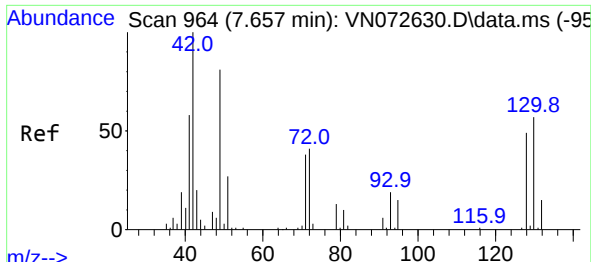

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 7.657 min Scan# 9
Delta R.T. 0.000 min
Lab File: VN072652.D
Acq: 31 May 2022 14:18




Instrument :
MSVOA_N
ClientSampleId :
WATER-DRUM


Tgt Ion:128 Resp: 24323
Ion Ratio Lower Upper
128 100
49 192.0 0.0 392.3
130 133.5 0.0 320.2

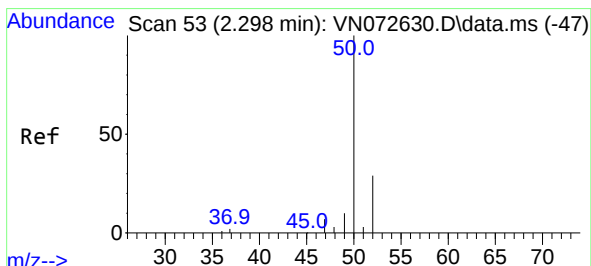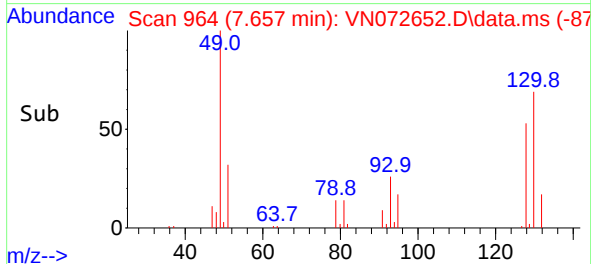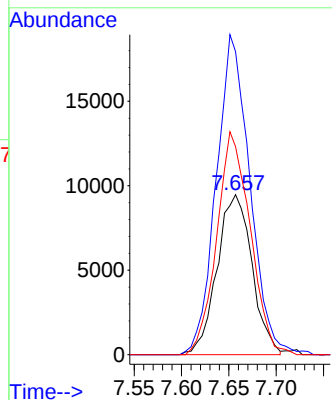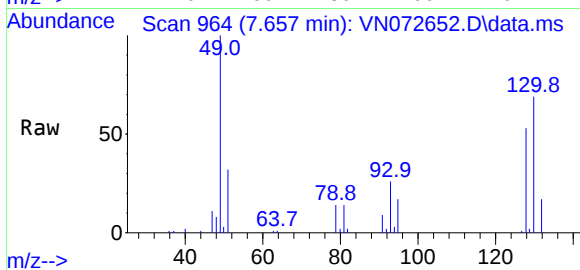

#3
Chloromethane
Concen: 0.265 ug/l
RT: 2.299 min Scan# 53
Delta R.T. 0.000 min
Lab File: VN072652.D
Acq: 31 May 2022 14:18

Tgt Ion: 50 Resp: 591
Ion Ratio Lower Upper
50 100
52 31.2 27.8 41.6


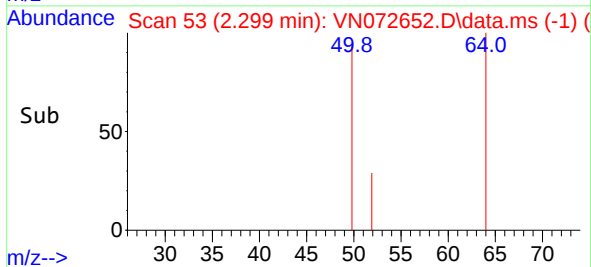
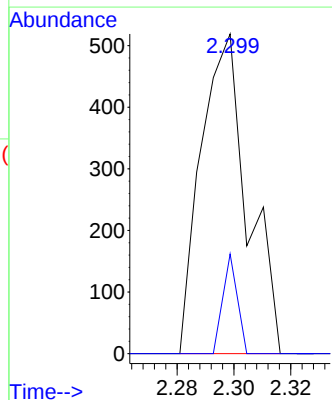
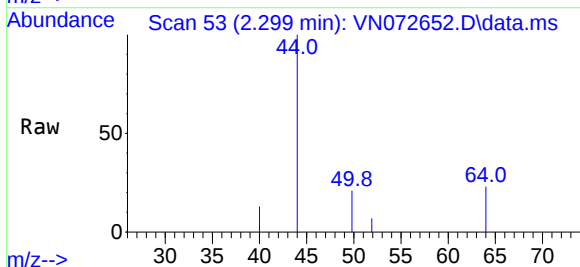


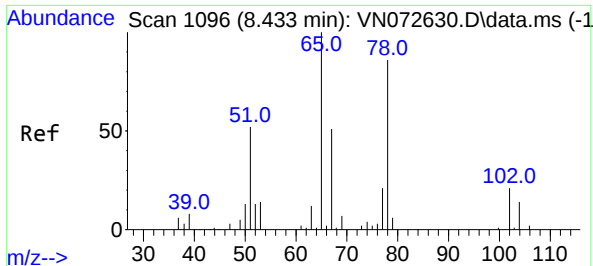

#27
1,2-Dichloroethane-d4
Concen: 30.590 ug/l
RT: 8.434 min Scan# 1096
Delta R.T. 0.000 min
Lab File: VN072652.D
Acq: 31 May 2022 14:18




Instrument :
MSVOA_N
ClientSampleId :
WATER-DRUM


Tgt Ion: 65 Resp: 71197
Ion Ratio Lower Upper
65 100
67 52.4 40.2 60.2

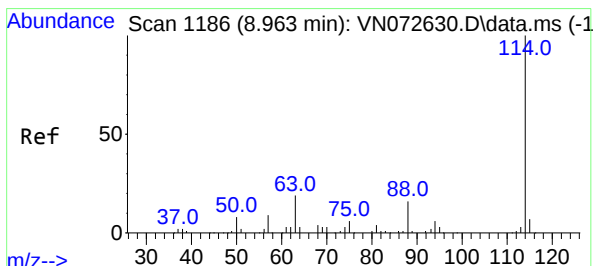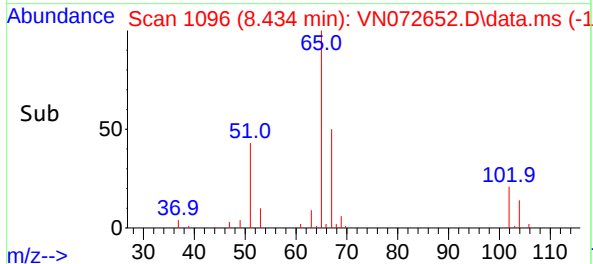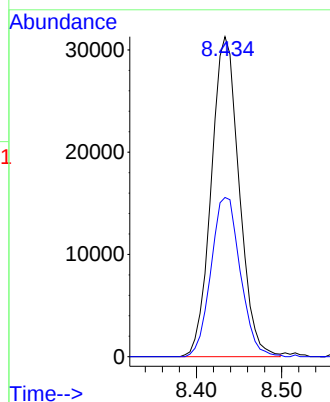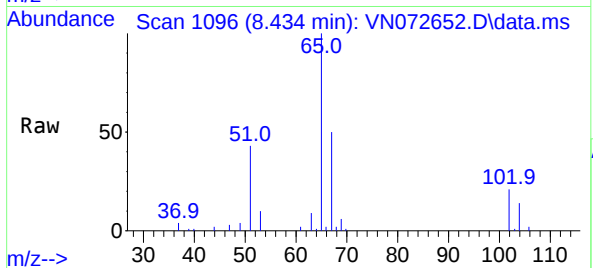

#28
1,4-Difluorobenzene
Concen: 30.000 ug/l
RT: 8.963 min Scan# 1186
Delta R.T. 0.000 min
Lab File: VN072652.D
Acq: 31 May 2022 14:18

Tgt Ion: 114 Resp: 123472
Ion Ratio Lower Upper
114 100
63 22.7 15.8 23.6
88 15.8 11.6 17.4


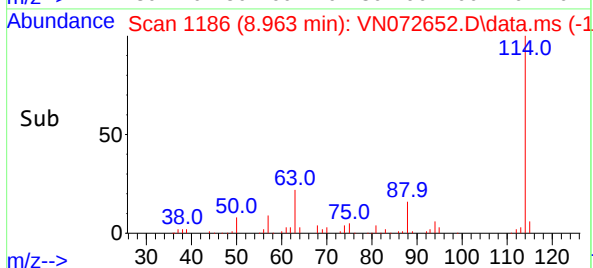
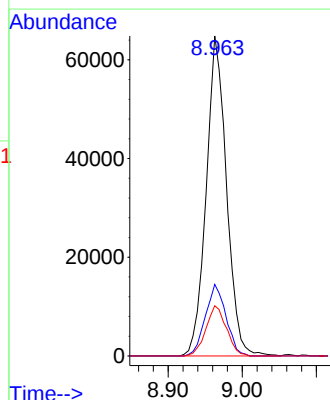
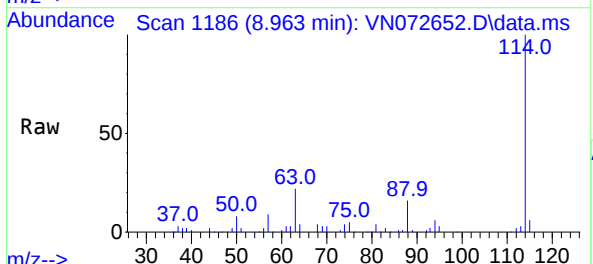


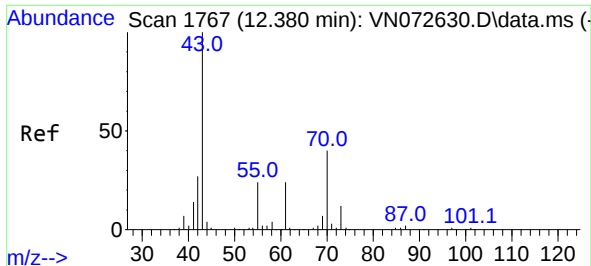

#47
n-amyl acetate
Concen: 49.686 ug/l
RT: 12.351 min Scan# 1762
Delta R.T. -0.029 min
Lab File: VN072652.D
Acq: 31 May 2022 14:18




Instrument :
MSVOA_N
ClientSampleId :
WATER-DRUM


Tgt Ion: 43 Resp: 170078
Ion Ratio Lower Upper
43 100
55 6.3 19.0 28.6#

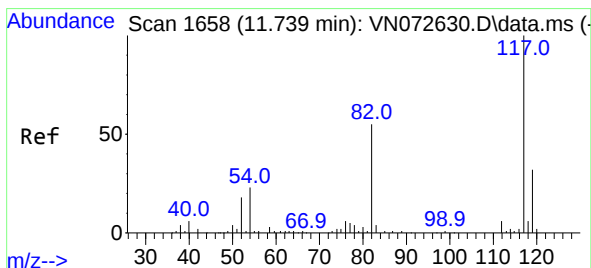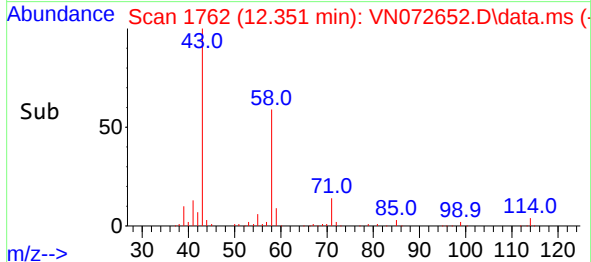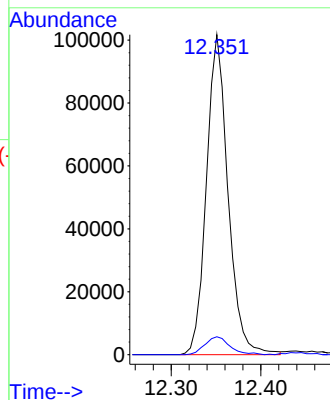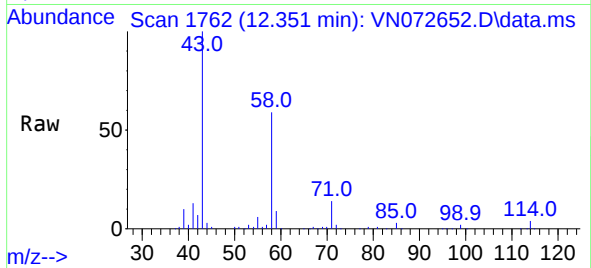

#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 11.745 min Scan# 1659
Delta R.T. 0.006 min
Lab File: VN072652.D
Acq: 31 May 2022 14:18

Tgt Ion: 117 Resp: 114988
Ion Ratio Lower Upper
117 100
82 56.4 43.6 65.4
119 32.2 25.8 38.6


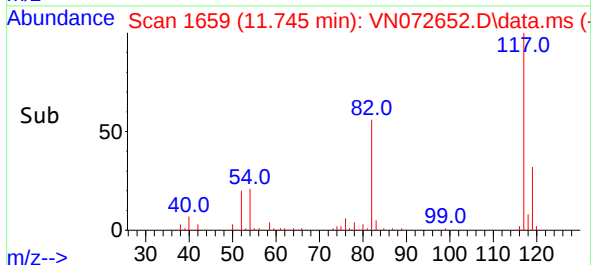
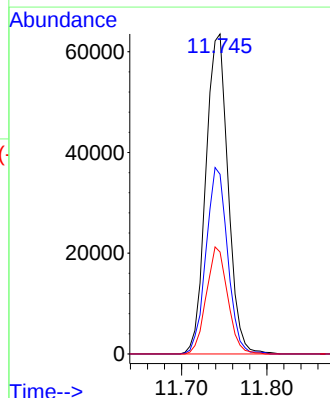
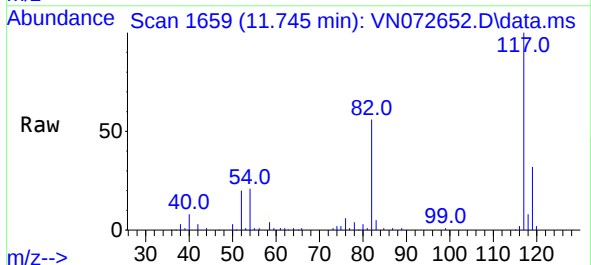


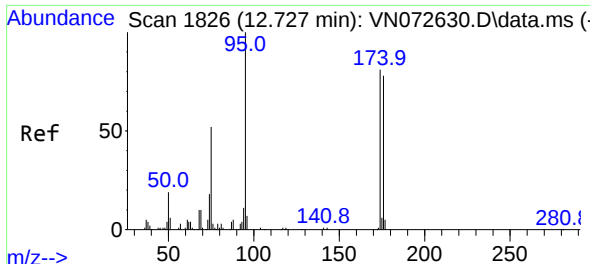

#60
4-Bromofluorobenzene
Concen: 21.430 ug/l
RT: 12.727 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN072652.D
Acq: 31 May 2022 14:18

Instrument :
MSVOA_N
ClientSampleId :
WATER-DRUM

Tgt Ion: 95 Resp: 43276
Ion Ratio Lower Upper
95 100
174 72.7 62.9 94.3
176 70.0 61.0 91.4

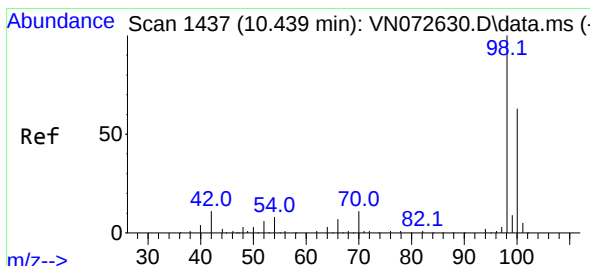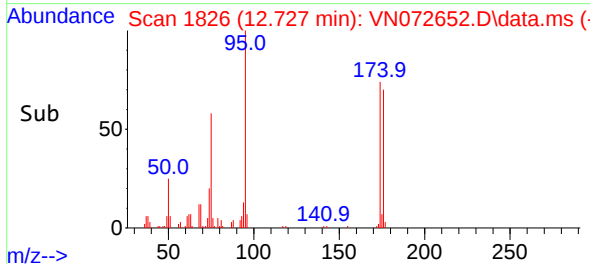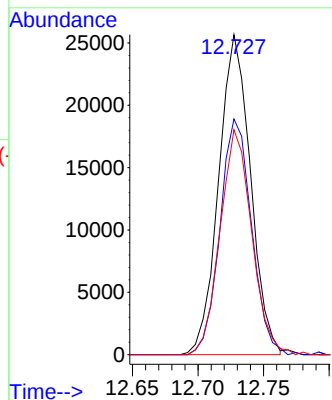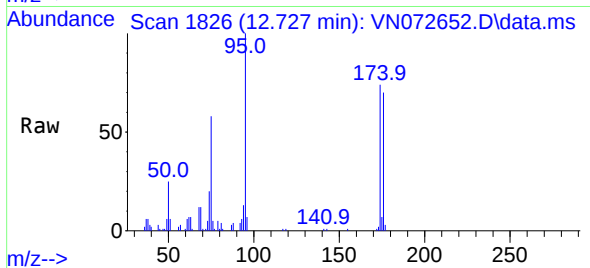

#63
Toluene-d8
Concen: 30.113 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN072652.D
Acq: 31 May 2022 14:18

Tgt Ion: 98 Resp: 196886
Ion Ratio Lower Upper
98 100
100 64.8 50.6 76.0

