


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN053122\
 Data File : VN072646.D
 Acq On : 31 May 2022 10:24
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N052622W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri May 27 05:07:24 2022

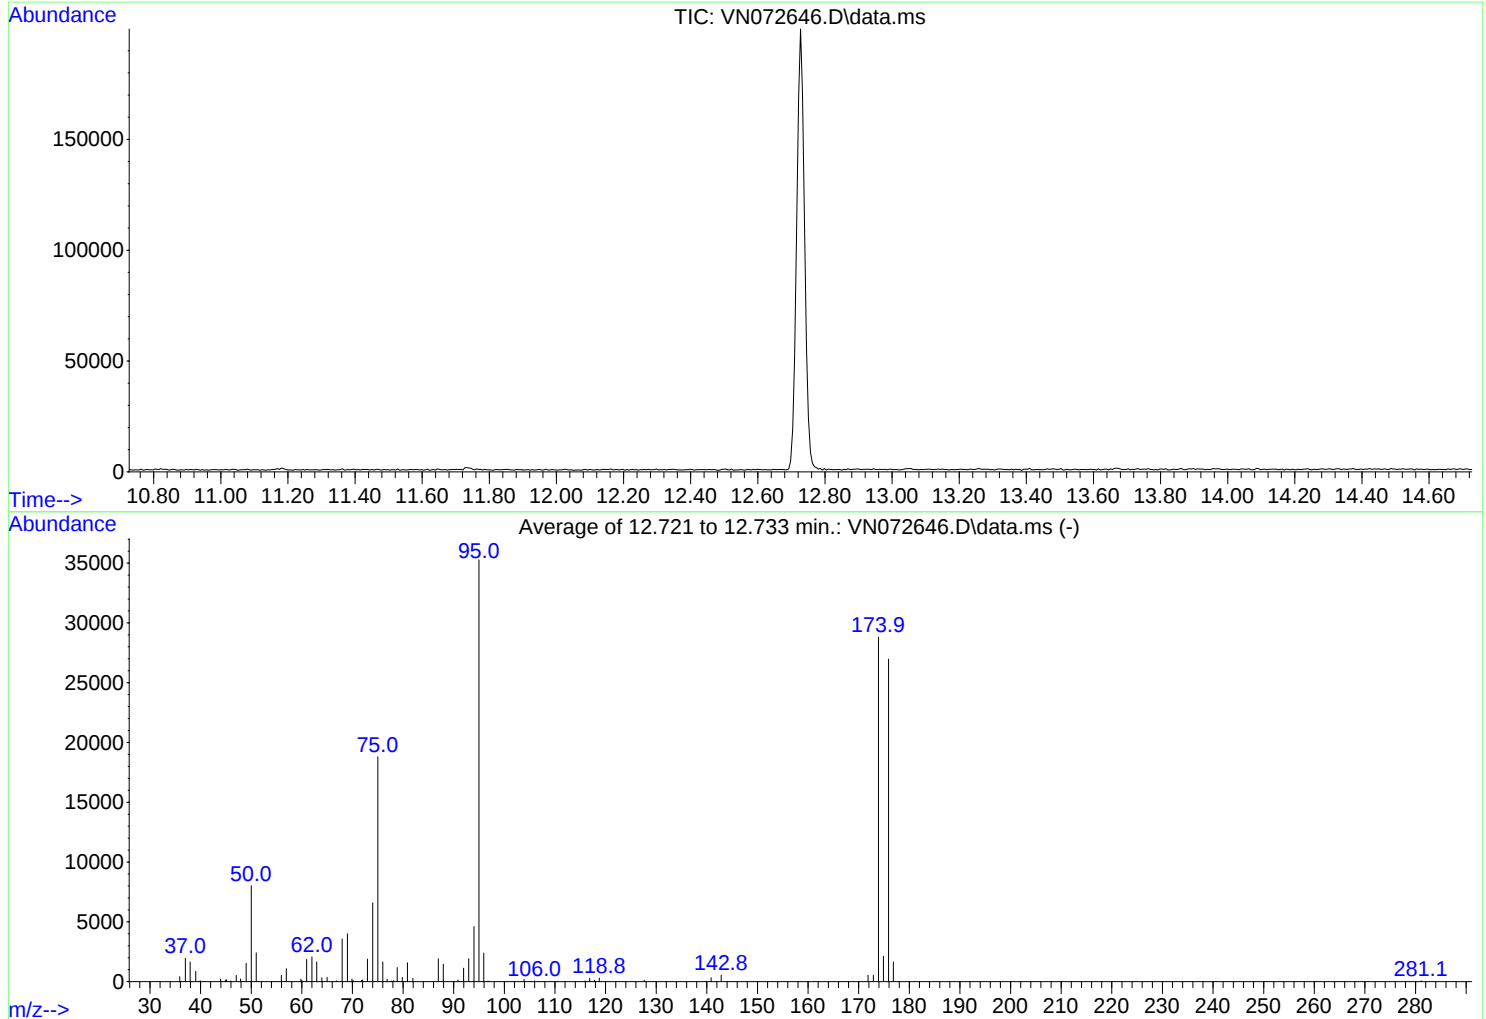

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1818

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	8014	PASS
75	95	30	60	53.3	18805	PASS
95	95	100	100	100.0	35275	PASS
96	95	5	9	6.8	2393	PASS
173	174	0.00	2	1.8	531	PASS
174	95	50	100	81.7	28811	PASS
175	174	5	9	7.4	2130	PASS
176	174	95	101	93.6	26971	FAIL*
177	176	5	9	6.1	1652	PASS