

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN053123\
 Data File : VN077985.D
 Acq On : 31 May 2023 11:30
 Operator : JC\MD
 Sample : VN0531MBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0531MBL01

Quant Time: Jun 01 01:48:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
 Quant Title : SW846 8260
 QLast Update : Tue May 16 04:07:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.229	168	358364	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	654433	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	578971	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.800	152	178532	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	253339	47.247	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	94.500%		
35) Dibromofluoromethane	8.177	113	220098	51.576	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	103.160%		
50) Toluene-d8	10.571	98	817522	49.770	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	99.540%		
62) 4-Bromofluorobenzene	12.853	95	265209	45.716	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	91.440%		
Target Compounds						
					Qvalue	
3) Chloromethane	2.371	50	973	Below Cal	#	58
13) Acrolein	4.200	56	475	Below Cal	#	70
15) Acrylonitrile	5.718	53	899	0.455	ug/l #	64
16) Acetone	4.459	43	1780	1.055	ug/l #	40
17) Carbon Disulfide	4.736	76	4369	0.430	ug/l #	75
20) Methylene Chloride	5.294	84	819	Below Cal	#	82
25) 2-Butanone	7.488	43	815	0.309	ug/l #	37
29) Tetrahydrofuran	7.877	42	744	0.431	ug/l #	25
31) Cyclohexane	8.235	56	8433	1.157	ug/l #	8
36) 1,1-Dichloropropene	8.229	75	31959	5.120	ug/l #	47
38) Carbon Tetrachloride	8.235	117	39768	6.309	ug/l #	15
49) 1,4-Dioxane	9.694	88	56	0.688	ug/l #	1
51) 4-Methyl-2-Pentanone	10.459	43	1984	0.367	ug/l #	83
59) 2-Hexanone	11.206	43	3339	0.836	ug/l	98
75) 1,1,2,2-Tetrachloroethane	12.941	83	1043	0.220	ug/l #	79
76) 1,2,3-Trichloropropane	12.853	75	139234	31.141	ug/l #	1
77) Bromobenzene	12.994	156	1159	0.330	ug/l	96
79) 2-Chlorotoluene	13.141	91	2379	0.220	ug/l	98
81) trans-1,4-Dichloro-2-b...	12.853	75	139234	99.543	ug/l #	15
82) 4-Chlorotoluene	13.229	91	3216	0.299	ug/l	98
86) p-Isopropyltoluene	13.729	119	2593	0.203	ug/l	84
87) 1,3-Dichlorobenzene	13.747	146	2737	0.421	ug/l	94
88) 1,4-Dichlorobenzene	13.747	146	2737	0.425	ug/l	96
89) n-Butylbenzene	14.059	91	4087	0.347	ug/l	91
91) 1,2-Dichlorobenzene	14.123	146	2421	0.399	ug/l	94
92) 1,2-Dibromo-3-Chloropr...	14.735	75	418	0.456	ug/l	77
93) 1,2,4-Trichlorobenzene	15.411	180	2477	0.699	ug/l	88
94) Hexachlorobutadiene	15.517	225	1432	0.973	ug/l	73
95) Naphthalene	15.647	128	12268	1.005	ug/l	96
96) 1,2,3-Trichlorobenzene	15.841	180	3041	0.876	ug/l #	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN053123\
Data File : VN077985.D
Acq On : 31 May 2023 11:30
Operator : JC\MD
Sample : VN0531MBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0531MBL01

Quant Time: Jun 01 01:48:45 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
Quant Title : SW846 8260
QLast Update : Tue May 16 04:07:42 2023
Response via : Initial Calibration




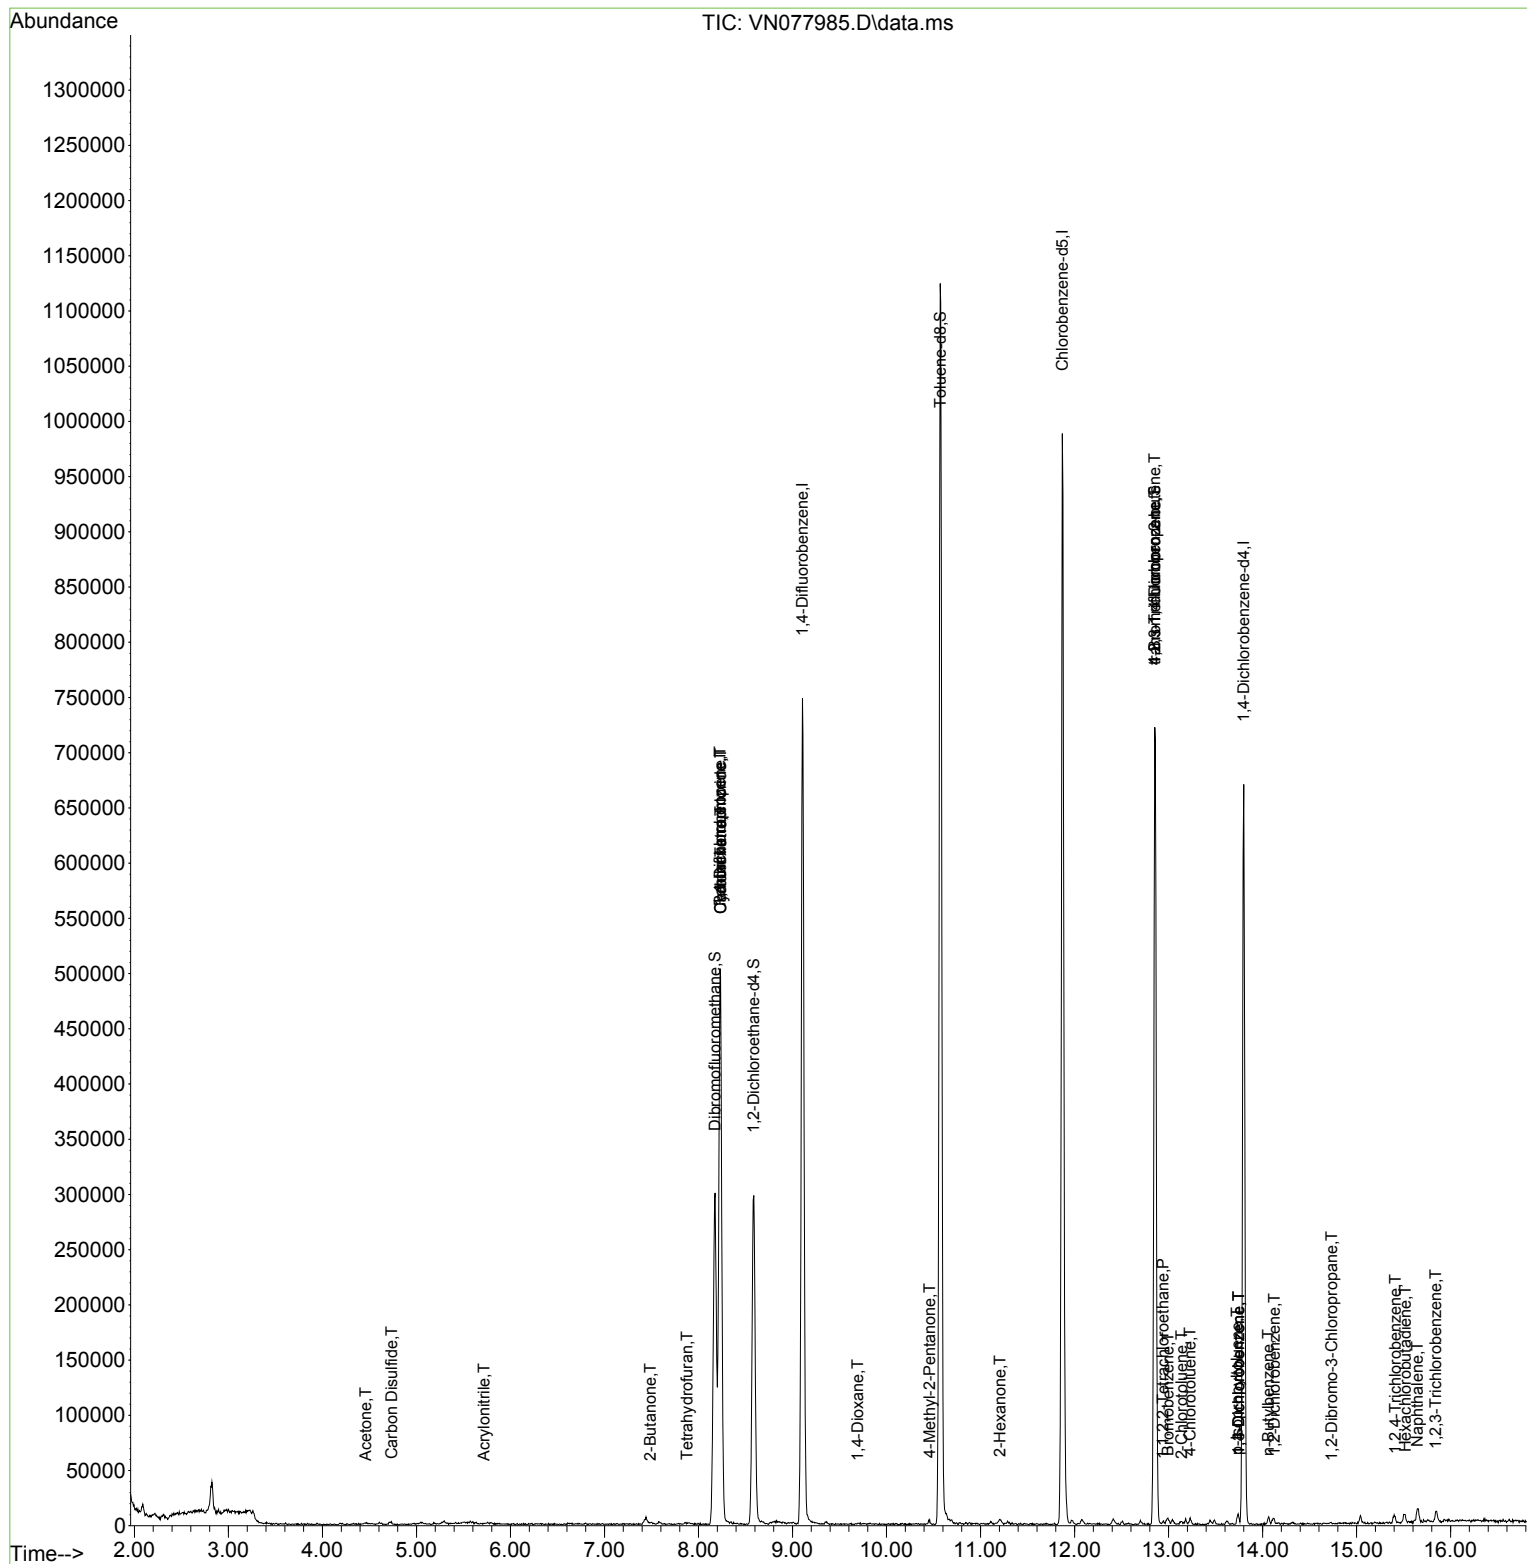




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.229 min Scan# 10
Delta R.T. -0.001 min
Lab File: VN077985.D
Acq: 31 May 2023 11:30




Instrument :
MSVOA_N
ClientSampleId :
VN0531MBL01


Tgt Ion:168 Resp: 358364
Ion Ratio Lower Upper
168 100
99 64.4 53.0 79.6



#3
Chloromethane
Concen: Below Cal
RT: 2.371 min Scan# 71
Delta R.T. 0.006 min
Lab File: VN077985.D
Acq: 31 May 2023 11:30

Tgt Ion: 50 Resp: 973
Ion Ratio Lower Upper
50 100
52 56.9 26.5 39.7#




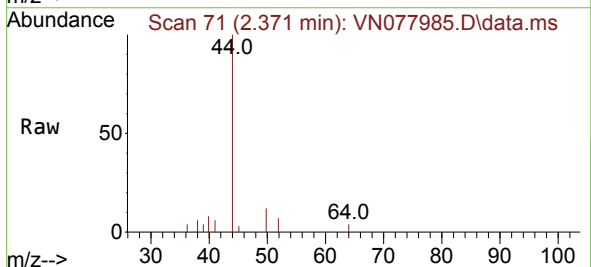




#13
Acrolein
Concen: Below Cal
RT: 4.200 min Scan# 31
Delta R.T. 0.011 min
Lab File: VN077985.D
Acq: 31 May 2023 11:30




Instrument :
MSVOA_N
ClientSampleId :
VN0531MBL01


Tgt Ion: 56 Resp: 475
Ion Ratio Lower Upper
56 100
55 92.2 54.5 81.7#



#15
Acrylonitrile
Concen: 0.455 ug/l
RT: 5.718 min Scan# 640
Delta R.T. -0.000 min
Lab File: VN077985.D
Acq: 31 May 2023 11:30

Tgt Ion: 53 Resp: 899
Ion Ratio Lower Upper
53 100
52 51.8 65.3 97.9#
51 12.0 28.9 43.3#









#16
Acetone
Concen: 1.055 ug/l
RT: 4.459 min Scan# 41
Delta R.T. 0.029 min
Lab File: VN077985.D
Acq: 31 May 2023 11:30




Instrument :
MSVOA_N
ClientSampleId :
VN0531MBL01


Tgt Ion: 43 Resp: 1780
Ion Ratio Lower Upper
43 100
58 0.0 28.0 42.0#



#17
Carbon Disulfide
Concen: 0.430 ug/l
RT: 4.736 min Scan# 473
Delta R.T. 0.024 min
Lab File: VN077985.D
Acq: 31 May 2023 11:30

Tgt Ion: 76 Resp: 4369
Ion Ratio Lower Upper
76 100
78 0.0 7.4 11.0#


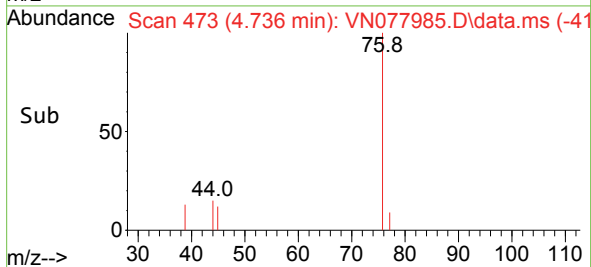

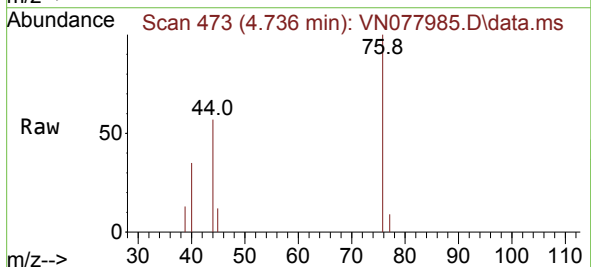




#20
Methylene Chloride
Concen: Below Cal
RT: 5.294 min Scan# 51
Delta R.T. 0.011 min
Lab File: VN077985.D
Acq: 31 May 2023 11:30




Instrument :
MSVOA_N
ClientSampleId :
VN0531MBL01


Tgt Ion: 84 Resp: 819
Ion Ratio Lower Upper
84 100
49 91.3 79.7 119.5
51 24.8 25.2 37.8#
86 38.6 53.3 79.9#



#25
2-Butanone
Concen: 0.309 ug/l
RT: 7.488 min Scan# 941
Delta R.T. 0.000 min
Lab File: VN077985.D
Acq: 31 May 2023 11:30

Tgt Ion: 43 Resp: 815
Ion Ratio Lower Upper
43 100
72 0.0 30.2 45.2#





#29

Tetrahydrofuran

Concen: 0.431 ug/l

RT: 7.877 min Scan# 1007

Delta R.T. 0.036 min

Lab File: VN077985.D

Acq: 31 May 2023 11:30

Instrument :

MSVOA_N

ClientSampleId :

VN0531MBL01





Tgt Ion: 42 Resp: 744

Ion Ratio Lower Upper

42 100

72 7.8 49.8 74.6#

71 0.0 47.4 71.2#

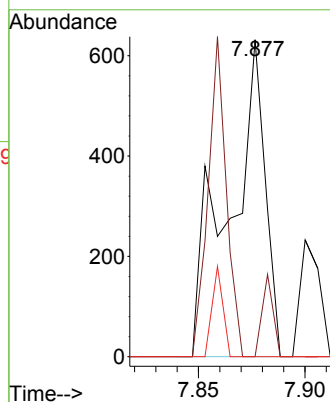

#31

Cyclohexane

Concen: 1.157 ug/l

RT: 8.235 min Scan# 1068

Delta R.T. -0.030 min

Lab File: VN077985.D

Acq: 31 May 2023 11:30




Tgt Ion: 56 Resp: 8433


Ion Ratio Lower Upper

56 100

69 156.4 26.8 40.2#

84 154.3 81.8 122.6#









#33
 1,2-Dichloroethane-d4
 Concen: 47.247 ug/l
 RT: 8.588 min Scan# 1127
 Delta R.T. 0.006 min
 Lab File: VN077985.D
 Acq: 31 May 2023 11:30




Instrument :
 MSVOA_N
 ClientSampleId :
 VN0531MBL01


Tgt Ion: 65 Resp: 253339
 Ion Ratio Lower Upper
 65 100
 67 51.5 0.0 106.6



#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 9.106 min Scan# 1216
 Delta R.T. -0.000 min
 Lab File: VN077985.D
 Acq: 31 May 2023 11:30

Tgt Ion: 114 Resp: 654433
 Ion Ratio Lower Upper
 114 100
 63 20.3 0.0 36.4
 88 16.5 0.0 30.6




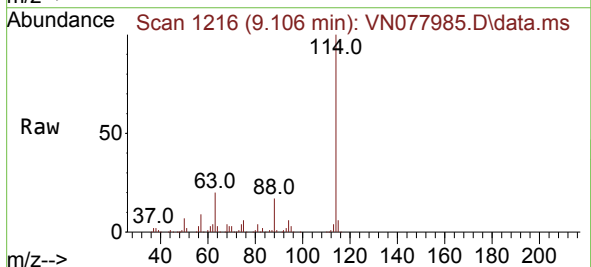




#35
Dibromofluoromethane
Concen: 51.576 ug/l
RT: 8.177 min Scan# 1057
Delta R.T. 0.006 min
Lab File: VN077985.D
Acq: 31 May 2023 11:30




Instrument :
MSVOA_N
ClientSampleId :
VN0531MBL01


Tgt Ion:113 Resp: 220098
Ion Ratio Lower Upper
113 100
111 101.2 82.6 123.8
192 16.9 12.7 19.1

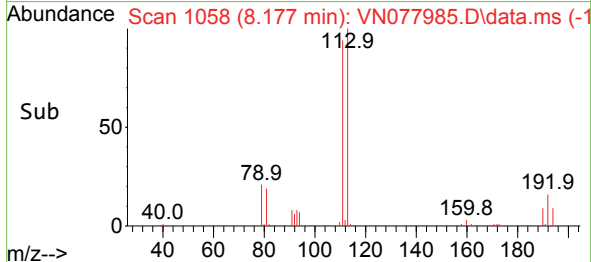

#36
1,1-Dichloropropene
Concen: 5.120 ug/l
RT: 8.229 min Scan# 1067
Delta R.T. -0.148 min
Lab File: VN077985.D
Acq: 31 May 2023 11:30

Tgt Ion: 75 Resp: 31959
Ion Ratio Lower Upper
75 100
110 8.4 19.1 57.3#
77 0.0 25.0 37.4#

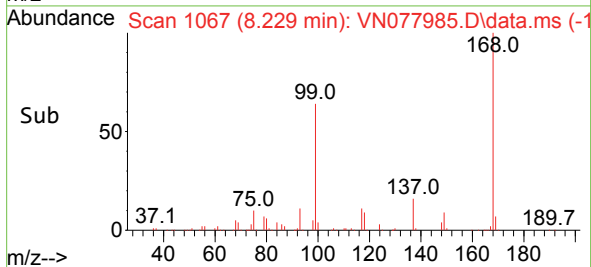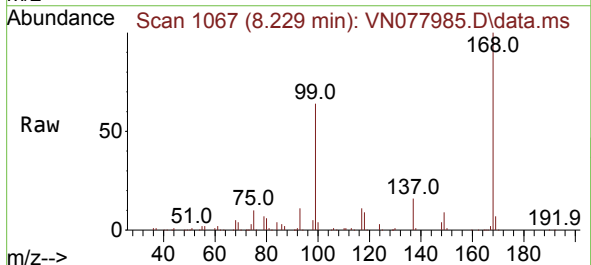



#38

Carbon Tetrachloride

Concen: 6.309 ug/l

RT: 8.235 min Scan# 1068

Delta R.T. -0.136 min

Lab File: VN077985.D

Acq: 31 May 2023 11:30

Instrument :

MSVOA_N

ClientSampleId :

VN0531MBL01





Tgt Ion:117 Resp: 39768

Ion Ratio Lower Upper

117 100

119 3.6 77.3 115.9#

121 0.0 23.3 34.9#

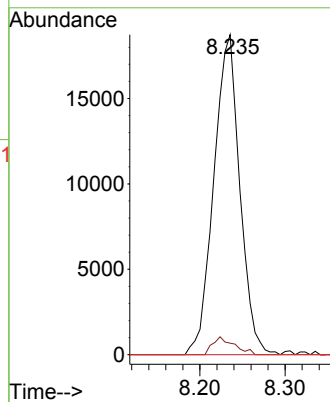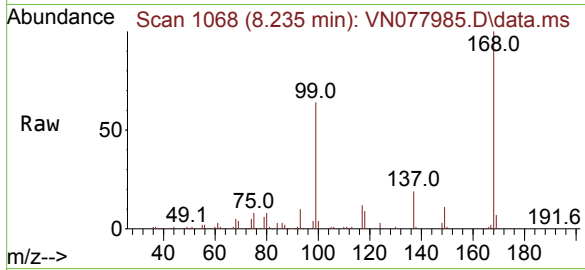

#49

1,4-Dioxane

Concen: 0.688 ug/l

RT: 9.694 min Scan# 1316

Delta R.T. 0.000 min

Lab File: VN077985.D

Acq: 31 May 2023 11:30




Tgt Ion: 88 Resp: 56


Ion Ratio Lower Upper

88 100

43 221.4 17.0 25.6#

58 119.6 47.0 70.4#




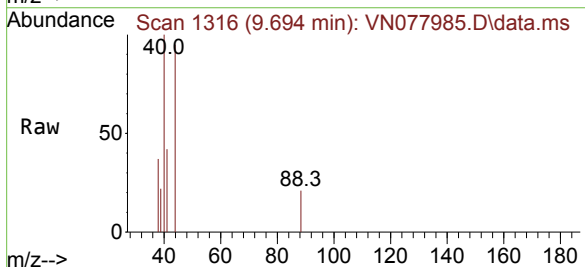


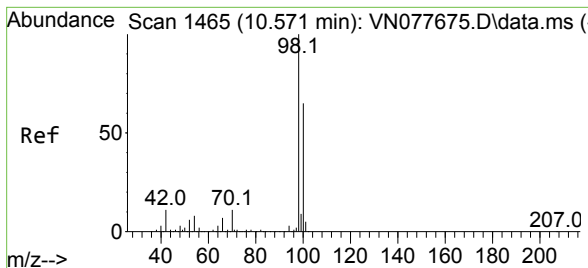

#50
Toluene-d8
Concen: 49.770 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN077985.D
Acq: 31 May 2023 11:30




Instrument :
MSVOA_N
ClientSampleId :
VN0531MBL01


Tgt Ion: 98 Resp: 817522
Ion Ratio Lower Upper
98 100
100 63.5 52.0 78.0

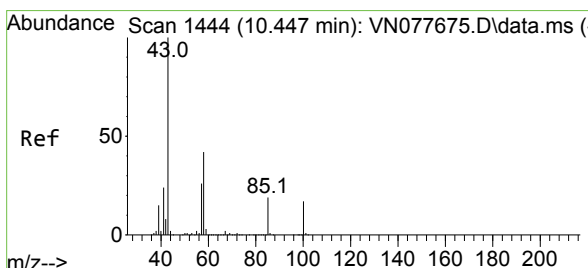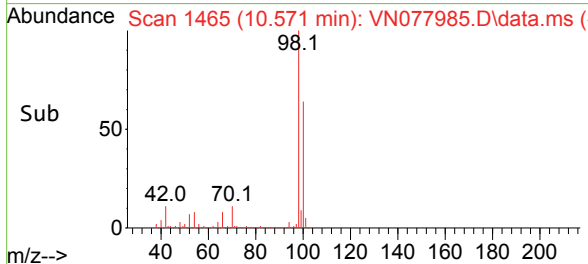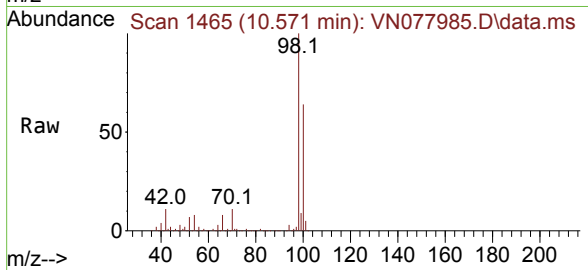

#51
4-Methyl-2-Pentanone
Concen: 0.367 ug/l
RT: 10.459 min Scan# 1446
Delta R.T. 0.012 min
Lab File: VN077985.D
Acq: 31 May 2023 11:30

Tgt Ion: 43 Resp: 1984
Ion Ratio Lower Upper
43 100
58 34.6 36.6 54.8#


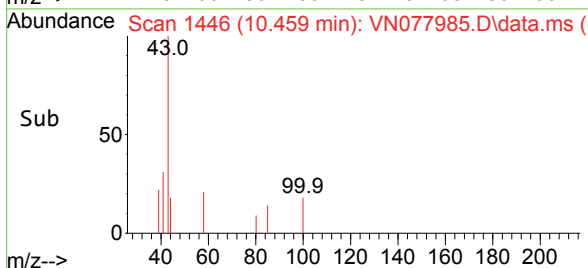

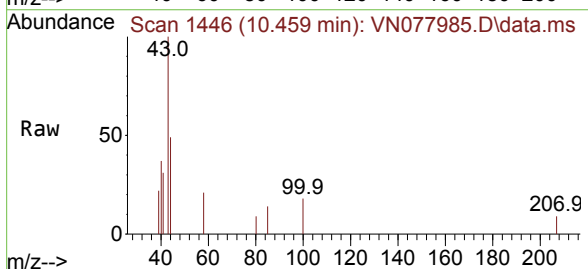


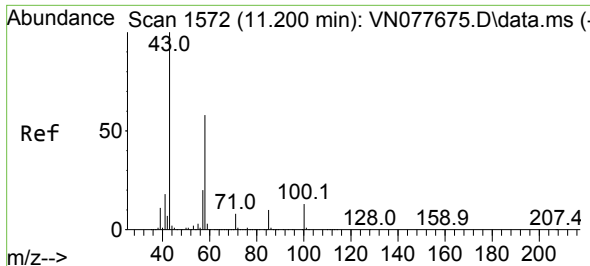

#59
2-Hexanone
Concen: 0.836 ug/l
RT: 11.206 min Scan# 1573
Delta R.T. 0.006 min
Lab File: VN077985.D
Acq: 31 May 2023 11:30




Instrument :
MSVOA_N
ClientSampleId :
VN0531MBL01


Tgt Ion: 43 Resp: 3339
Ion Ratio Lower Upper
43 100
58 61.5 31.7 95.1

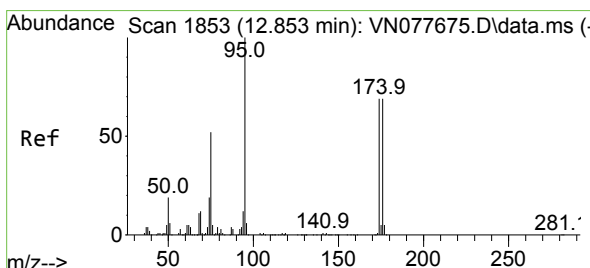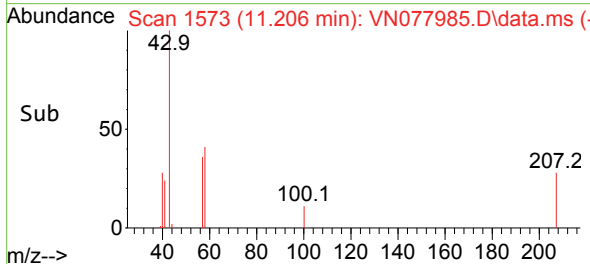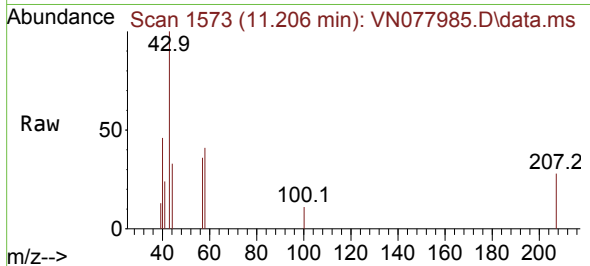

#62
4-Bromofluorobenzene
Concen: 45.716 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN077985.D
Acq: 31 May 2023 11:30

Tgt Ion: 95 Resp: 265209
Ion Ratio Lower Upper
95 100
174 73.0 0.0 143.8
176 70.6 0.0 135.8


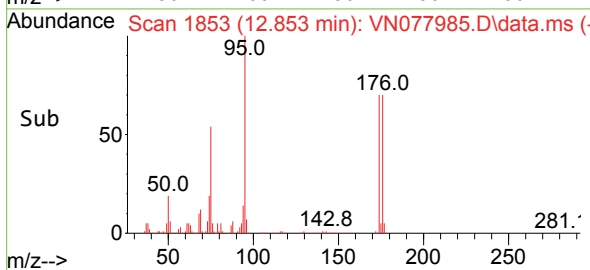

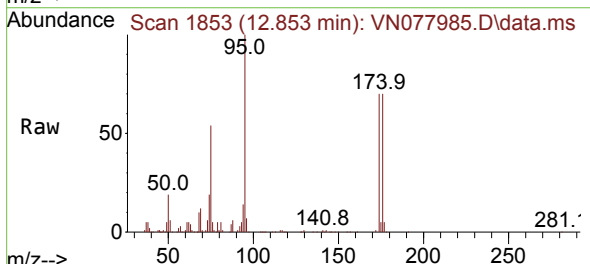




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN077985.D
Acq: 31 May 2023 11:30




Instrument :
MSVOA_N
ClientSampleId :
VN0531MBL01


Tgt Ion:117 Resp: 578971
Ion Ratio Lower Upper
117 100
82 57.3 44.0 66.0
119 31.3 25.6 38.4



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.800 min Scan# 2014
Delta R.T. -0.000 min
Lab File: VN077985.D
Acq: 31 May 2023 11:30

Tgt Ion:152 Resp: 178532
Ion Ratio Lower Upper
152 100
115 61.1 32.3 96.8
150 156.1 0.0 355.8



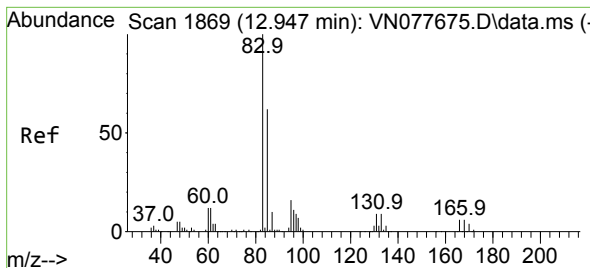

#75

1,1,2,2-Tetrachloroethane

Concen: 0.220 ug/l

RT: 12.941 min Scan# 1868

Delta R.T. -0.006 min

Lab File: VN077985.D

Acq: 31 May 2023 11:30

Instrument :

MSVOA_N

ClientSampleId :

VN0531MBL01





Tgt Ion: 83 Resp: 1043

Ion Ratio Lower Upper

83 100

131 0.0 5.0 15.0#

85 48.4 31.9 95.7

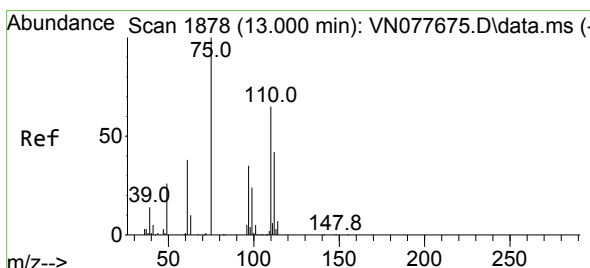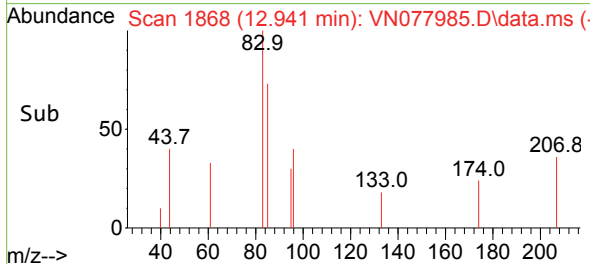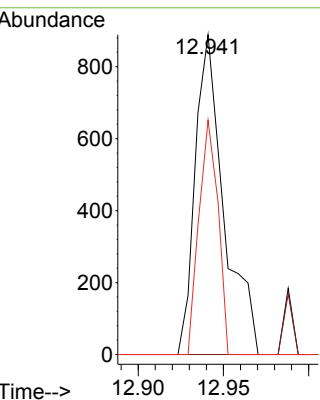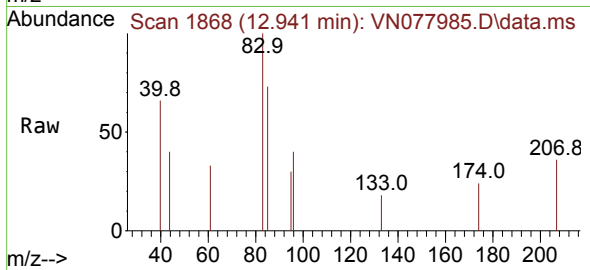

#76

1,2,3-Trichloropropane

Concen: 31.141 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. -0.147 min

Lab File: VN077985.D




Acq: 31 May 2023 11:30


Tgt Ion: 75 Resp: 139234

Ion Ratio Lower Upper

75 100

77 1.1 84.5 253.5#


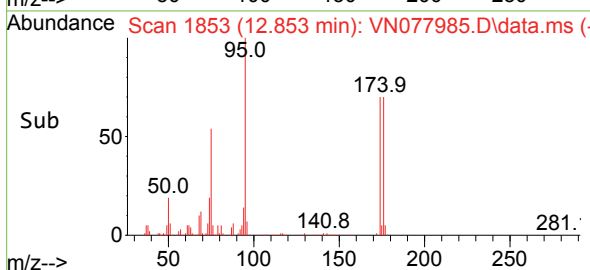
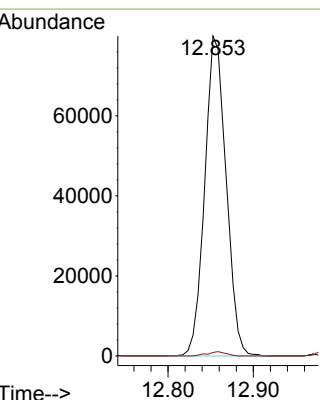
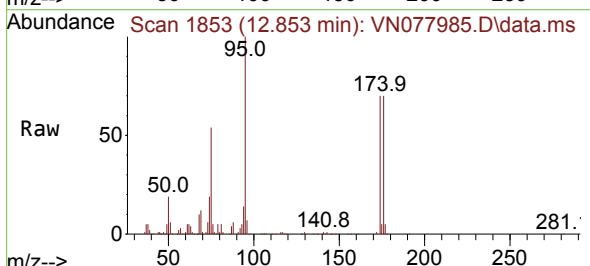




#77
Bromobenzene
Concen: 0.330 ug/l
RT: 12.994 min Scan# 1159
Delta R.T. 0.006 min
Lab File: VN077985.D
Acq: 31 May 2023 11:30




Instrument :
MSVOA_N
ClientSampleId :
VN0531MBL01


Tgt Ion:156 Resp: 1159
Ion Ratio Lower Upper
156 100
77 207.3 107.7 323.3
158 99.2 48.4 145.3

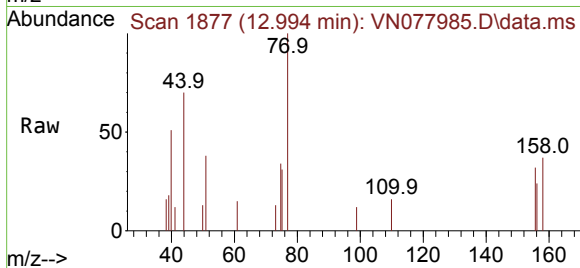

#79
2-Chlorotoluene
Concen: 0.220 ug/l
RT: 13.141 min Scan# 1902
Delta R.T. 0.012 min
Lab File: VN077985.D
Acq: 31 May 2023 11:30

Tgt Ion: 91 Resp: 2379
Ion Ratio Lower Upper
91 100
126 33.4 16.3 48.8


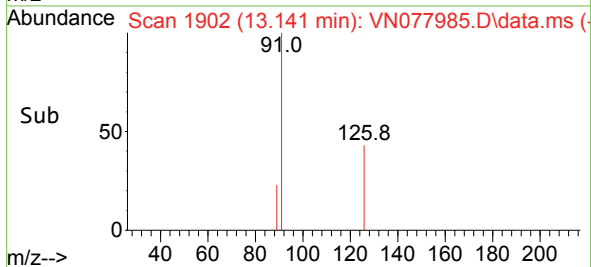

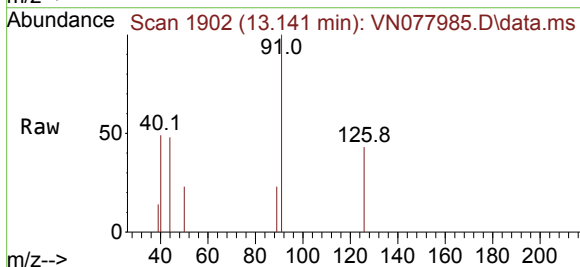




#81
trans-1,4-Dichloro-2-butene
Concen: 99.543 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.112 min
Lab File: VN077985.D
Acq: 31 May 2023 11:30




Instrument :
MSVOA_N
ClientSampleId :
VN0531MBL01


Tgt Ion: 75 Resp: 139234
Ion Ratio Lower Upper
75 100
53 0.0 67.4 101.2#
89 0.1 38.8 58.2#



#82
4-Chlorotoluene
Concen: 0.299 ug/l
RT: 13.229 min Scan# 1917
Delta R.T. 0.000 min
Lab File: VN077985.D
Acq: 31 May 2023 11:30

Tgt Ion: 91 Resp: 3216
Ion Ratio Lower Upper
91 100
126 32.0 16.7 50.0





#86

p-Isopropyltoluene

Concen: 0.203 ug/l

RT: 13.729 min Scan# 2002

Delta R.T. -0.006 min

Lab File: VN077985.D

Acq: 31 May 2023 11:30

Instrument :

MSVOA_N

ClientSampleId :

VN0531MBL01





Tgt Ion:119 Resp: 2593

Ion Ratio Lower Upper

119 100

134 15.2 12.6 37.8

91 19.0 12.4 37.2



#87

1,3-Dichlorobenzene

Concen: 0.421 ug/l

RT: 13.747 min Scan# 2005

Delta R.T. 0.006 min

Lab File: VN077985.D

Acq: 31 May 2023 11:30




Tgt Ion:146 Resp: 2737


Ion Ratio Lower Upper

146 100

111 39.8 22.1 66.3

148 59.3 32.0 96.0









#88
1,4-Dichlorobenzene
Concen: 0.425 ug/l
RT: 13.747 min Scan# 2017
Delta R.T. -0.070 min
Lab File: VN077985.D
Acq: 31 May 2023 11:30




Instrument :
MSVOA_N
ClientSampleId :
VN0531MBL01


Tgt Ion:146 Resp: 2737
Ion Ratio Lower Upper
146 100
111 39.8 20.6 61.8
148 59.3 31.6 94.8



#89
n-Butylbenzene
Concen: 0.347 ug/l
RT: 14.059 min Scan# 2058
Delta R.T. -0.005 min
Lab File: VN077985.D
Acq: 31 May 2023 11:30

Tgt Ion: 91 Resp: 4087
Ion Ratio Lower Upper
91 100
92 45.1 26.4 79.0
134 22.1 12.6 37.6









#91
 1,2-Dichlorobenzene
 Concen: 0.399 ug/l
 RT: 14.123 min Scan# 2069
 Delta R.T. 0.012 min
 Lab File: VN077985.D
 Acq: 31 May 2023 11:30




Instrument :
 MSVOA_N
 ClientSampleId :
 VN0531MBL01


Tgt Ion:	146	Resp:	2421
Ion	Ratio	Lower	Upper
146	100		
111	41.8	22.0	66.0
148	69.6	31.8	95.3

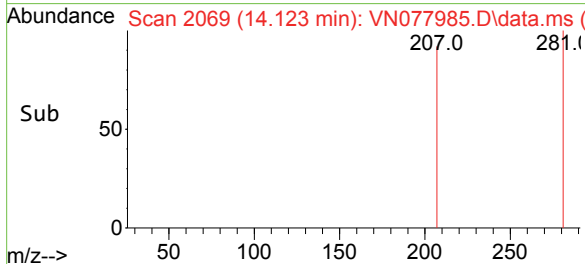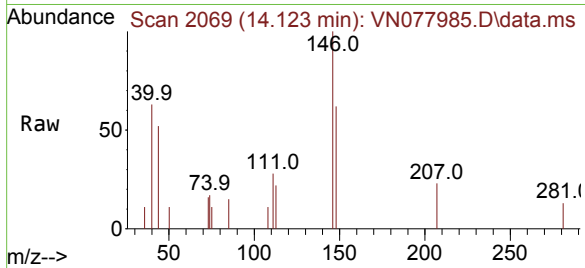

#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.456 ug/l
 RT: 14.735 min Scan# 2173
 Delta R.T. 0.012 min
 Lab File: VN077985.D
 Acq: 31 May 2023 11:30

Tgt Ion:	75	Resp:	418
Ion	Ratio	Lower	Upper
75	100		
155	63.4	39.1	117.2
157	72.2	50.3	150.9


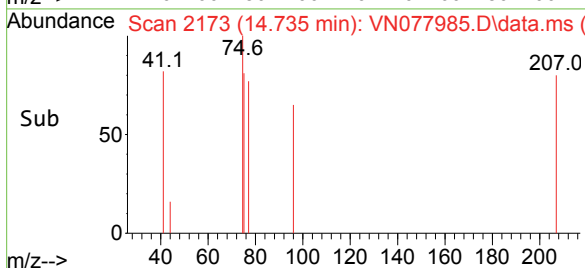
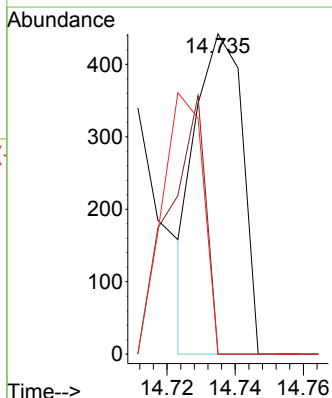
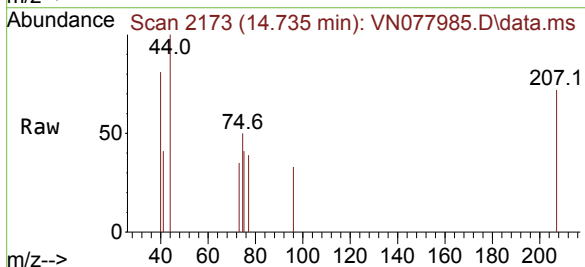




#93
1,2,4-Trichlorobenzene
Concen: 0.699 ug/l
RT: 15.411 min Scan# 21
Delta R.T. 0.011 min
Lab File: VN077985.D
Acq: 31 May 2023 11:30




Instrument :
MSVOA_N
ClientSampleId :
VN0531MBL01


Tgt Ion:180 Resp: 2477
Ion Ratio Lower Upper
180 100
182 102.3 46.1 138.2
145 43.0 16.6 49.8



#94
Hexachlorobutadiene
Concen: 0.973 ug/l
RT: 15.517 min Scan# 2306
Delta R.T. 0.011 min
Lab File: VN077985.D
Acq: 31 May 2023 11:30

Tgt Ion:225 Resp: 1432
Ion Ratio Lower Upper
225 100
223 74.4 31.3 93.8
227 33.5 31.9 95.9





#95

Naphthalene

Concen: 1.005 ug/l

RT: 15.647 min Scan# 2328

Delta R.T. -0.000 min

Lab File: VN077985.D

Acq: 31 May 2023 11:30

Instrument :

MSVOA_N

ClientSampleId :

VN0531MBL01





Tgt Ion:128 Resp: 12268

Ion Ratio Lower Upper

128 100

127 10.6 10.0 15.0

129 9.6 8.7 13.1



#96

1,2,3-Trichlorobenzene

Concen: 0.876 ug/l

RT: 15.841 min Scan# 2361

Delta R.T. -0.006 min

Lab File: VN077985.D

Acq: 31 May 2023 11:30

Tgt Ion:180 Resp: 3041

Ion Ratio Lower Upper

180 100

182 106.8 46.2 138.6

145 56.7 17.5 52.6#

