
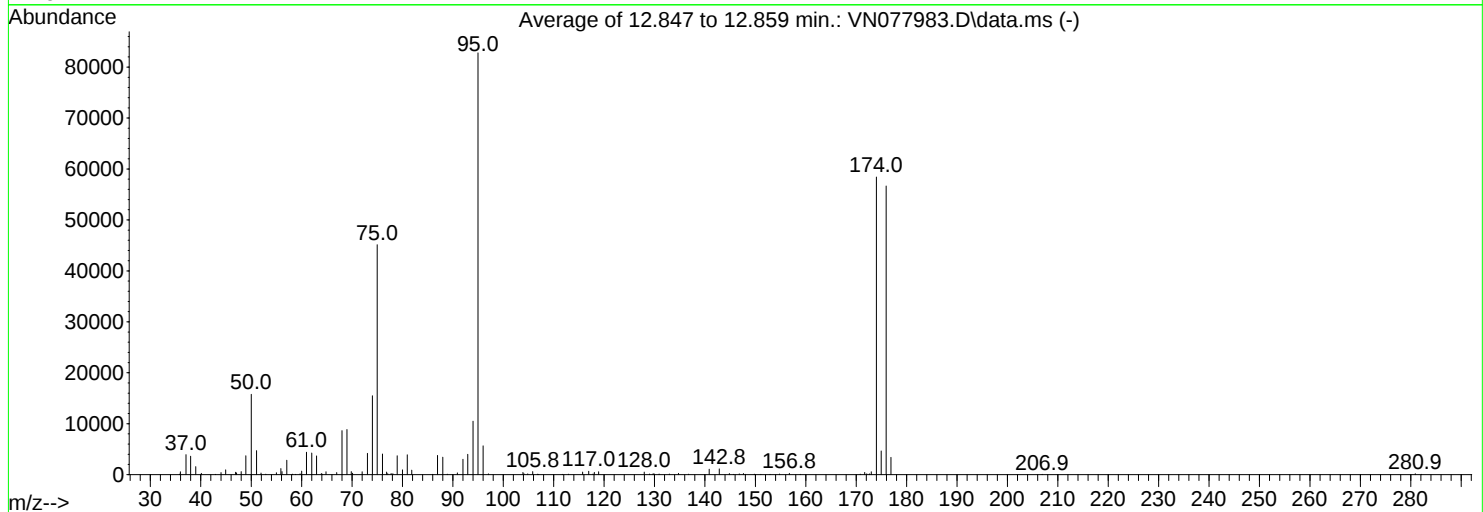


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN053123\
Data File : VN077983.D
Acq On : 31 May 2023 08:56
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
Title : SW846 8260
Last Update : Tue May 16 04:07:42 2023

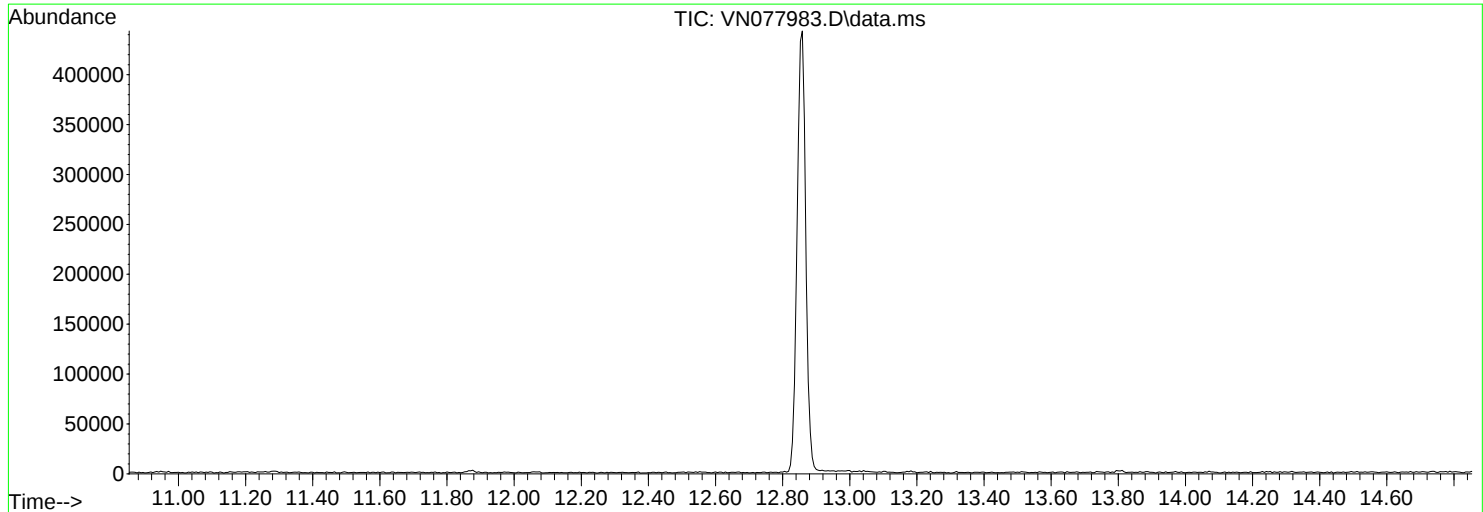

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1845

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	15779	PASS
75	95	30	60	54.5	45125	PASS
95	95	100	100	100.0	82803	PASS
96	95	5	9	6.8	5651	PASS
173	174	0.00	2	1.0	558	PASS
174	95	50	100	70.6	58437	PASS
175	174	5	9	8.0	4657	PASS
176	174	95	101	97.0	56656	PASS
177	176	5	9	6.0	3381	PASS

Average of 12.847 to 12.859 min.: VN077983.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	80	48.00	596	58.80	70	69.00	885
35.95	573	48.95	3708	59.70	148	69.85	58
37.05	3929	50.00	15779	60.00	691	70.10	28
38.00	3604	51.05	4730	60.95	4402	72.00	55
39.00	1576	51.95	304	62.00	4247	73.05	4167
40.10	261	52.90	106	62.95	3666	74.05	15474
42.90	77	55.00	390	63.90	216	75.00	45125
44.00	396	55.90	1192	64.10	98	76.05	4071
44.95	933	56.10	611	64.85	552	76.85	504
46.90	476	57.05	2839	66.95	407	77.10	199
47.10	333	58.20	99	68.00	8635	77.75	235

Average of 12.847 to 12.859 min.: VN077983.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.10	186	92.95	3979	111.70	53	130.90	142
78.95	3706	94.00	10483	112.90	89	132.95	131
80.00	931	95.00	82803	115.75	505	134.75	245
80.95	3881	96.00	5651	116.95	653	136.75	101
81.85	890	97.05	159	117.80	135	140.00	51
86.00	71	103.90	429	118.05	455	140.85	1086
86.95	3778	104.10	193	118.90	582	142.85	1137
88.00	3413	104.85	165	127.95	505	144.85	232
88.90	86	105.85	608	129.00	121	145.70	52
90.90	339	106.80	86	129.70	174	146.80	152
92.00	3026	107.00	56	129.90	195	147.65	208

Average of 12.847 to 12.859 min.: VN077983.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
148.00	55	173.00	558				
149.80	86	174.00	58437				
151.10	60	174.95	4657				
152.90	58	175.95	56656				
154.80	142	176.90	3381				
156.75	255	206.90	52				
158.90	63	280.90	177				
170.80	109	282.10	74				
171.70	437						
172.10	152						
172.60	146						