
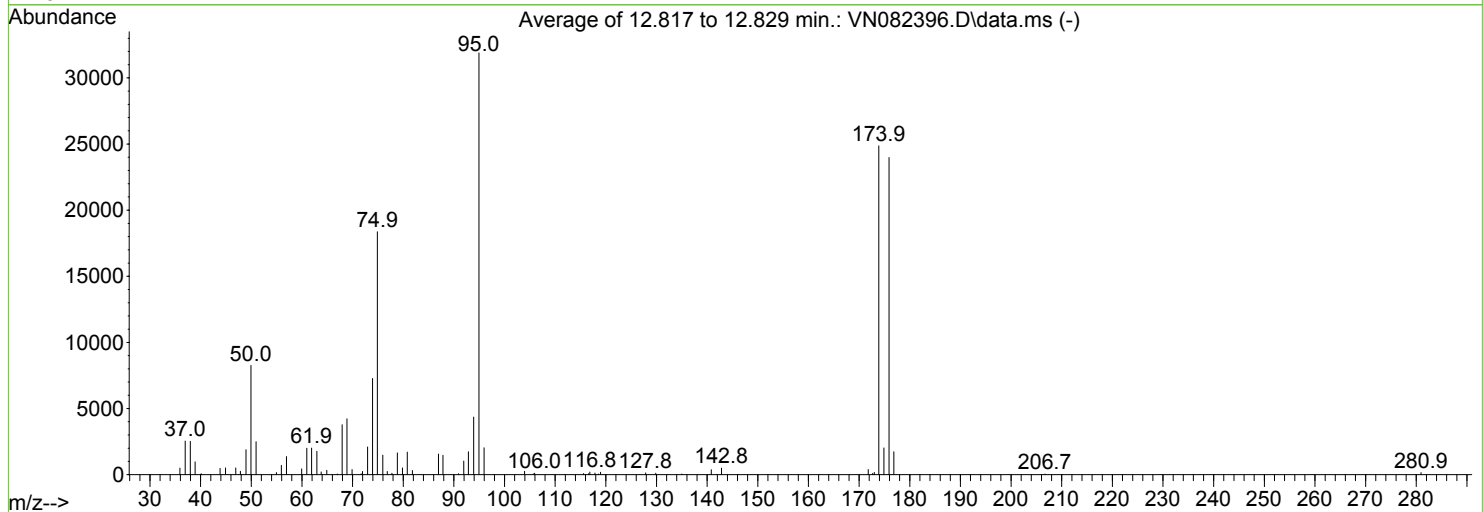


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN053124\
Data File : VN082396.D
Acq On : 31 May 2024 09:24
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Title : SW846 8260
Last Update : Thu May 16 05:21:06 2024

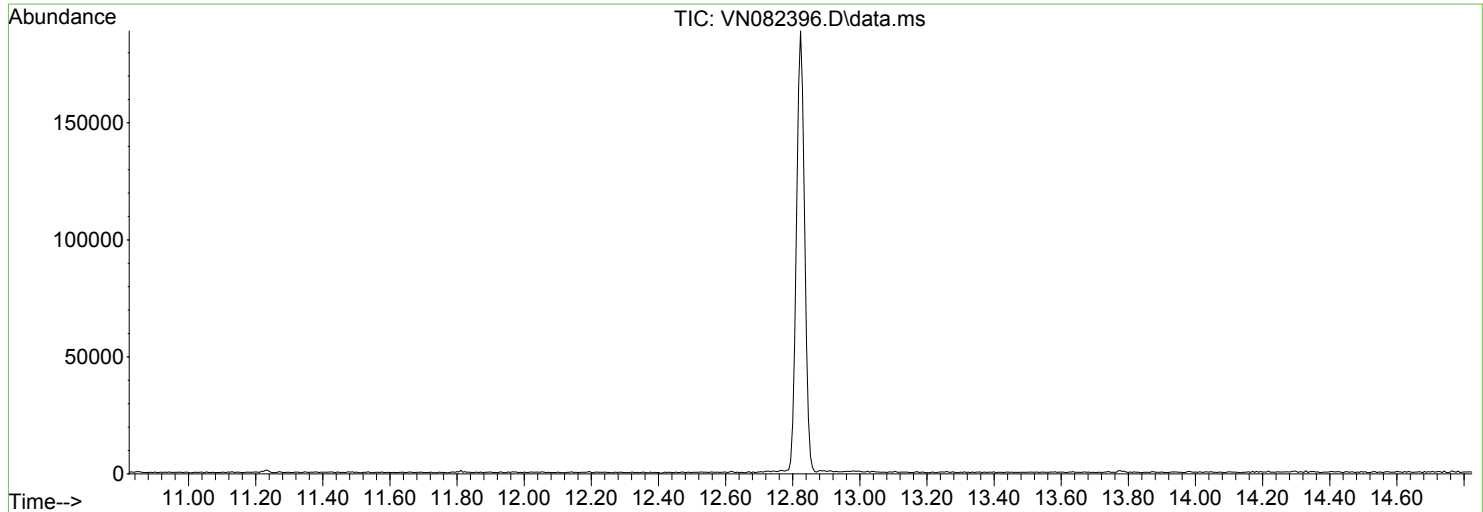

AutoFind: Scans 1847, 1848, 1849; Background Corrected with Scan 1840

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	25.9	8258	PASS
75	95	30	60	57.6	18368	PASS
95	95	100	100	100.0	31896	PASS
96	95	5	9	6.4	2031	PASS
173	174	0.00	2	0.7	170	PASS
174	95	50	100	78.0	24869	PASS
175	174	5	9	8.1	2020	PASS
176	174	95	101	96.4	23976	PASS
177	176	5	9	7.2	1728	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	500	50.95	2488	67.95	3770	78.85	1641
36.95	2543	54.95	160	68.90	4221	79.85	511
37.95	2517	55.95	702	69.90	391	80.80	170
38.90	969	56.95	1365	71.70	58	81.80	311
40.10	70	59.95	437	71.95	241	86.95	1566
43.85	474	60.95	1997	72.95	2093	87.85	1470
44.90	505	61.90	2011	73.95	7270	90.90	77
46.95	504	62.95	1766	74.90	18368	91.95	1033
47.85	257	63.80	202	75.95	1483	92.85	1728
48.95	1888	64.90	322	76.85	249	93.90	4358
49.95	8258	67.00	53	77.75	107	94.95	31896

Average of 12.817 to 12.829 min.: VN082396.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.95	2031	129.85	104	206.70	54		
103.95	258	135.00	50	280.95	155		
105.70	60	140.80	374				
105.95	113	142.85	497				
115.60	90	171.80	383				
116.60	76	172.70	95				
116.85	195	173.00	170				
117.85	119	173.90	24869				
118.50	55	174.90	2020				
118.95	180	175.90	23976				
127.85	139	176.85	1728				

Instrument :

MSVOA_N

ClientSampleId :

BFB