

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN060120\
 Data File : VN061601.D
 Acq On : 1 Jun 2020 17:43
 Operator : JC/MD
 Sample : L2813-06
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 EO-02-052920

Quant Time: Jun 02 03:56:06 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052820W.M
 Quant Title : SW846 8260
 QLast Update : Fri May 29 02:14:10 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	278958	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	491902	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	510252	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	226220	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	173100	52.08	ug/l	0.00
Spiked Amount			Recovery	=	104.16%	
35) Dibromofluoromethane	7.55	113	144769	58.02	ug/l	0.00
Spiked Amount			Recovery	=	116.04%	
50) Toluene-d8	10.06	98	615444	53.22	ug/l	0.00
Spiked Amount			Recovery	=	106.44%	
62) 4-Bromofluorobenzene	12.37	95	227526	53.93	ug/l	0.00
Spiked Amount			Recovery	=	107.86%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Tert butyl alcohol	4.73	59	100	0.226	ug/l #	72
16) Acetone	3.77	43	56661	57.073	ug/l	96
20) Methylene Chloride	4.50	84	12067	2.336	ug/l	93
25) 2-Butanone	6.79	43	3642	2.312	ug/l	89
29) Tetrahydrofuran	7.16	42	361	0.348	ug/l #	37
31) Cyclohexane	7.62	56	5277	1.127	ug/l #	12
36) 1,1-Dichloropropene	7.62	75	20929	4.806	ug/l #	47
38) Carbon Tetrachloride	7.63	117	27735	6.603	ug/l #	15
41) Methacrylonitrile	7.18	41	524	0.326	ug/l #	8
43) Isopropyl Acetate	8.13	43	35605	5.643	ug/l #	90
48) Methyl methacrylate	9.14	41	2802	0.987	ug/l #	19
51) 4-Methyl-2-Pentanone	9.96	43	6505	1.829	ug/l	100
54) cis-1,3-Dichloropropene	9.87	75	26926	4.795	ug/l #	61
56) Ethyl methacrylate	10.51	69	1075	0.220	ug/l #	1
57) 1,3-Dichloropropane	10.73	76	3198	0.572	ug/l #	42
59) 2-Hexanone	10.74	43	34894	13.664	ug/l #	48
69) o-Xylene	11.92	106	2833	0.410	ug/l	92
71) Bromoform	12.38	173	1626	0.534	ug/l #	1
74) N-amyl acetate	12.00	43	3296	0.634	ug/l #	38
76) 1,2,3-Trichloropropane	12.37	75	112392	27.322	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.71	105	9362	0.678	ug/l	90
81) trans-1,4-Dichloro-2-buten	12.37	75	112392	69.871	ug/l #	15
86) p-Isopropyltoluene	13.21	119	3370	0.233	ug/l	98
90) Hexachloroethane	13.86	117	783	0.489	ug/l #	13


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN060120\
Data File : VN061601.D
Acq On : 1 Jun 2020 17:43
Operator : JC/MD
Sample : L2813-06
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
EO-02-052920

Quant Time: Jun 02 03:56:06 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052820W.M
Quant Title : SW846 8260
QLast Update : Fri May 29 02:14:10 2020
Response via : Initial Calibration

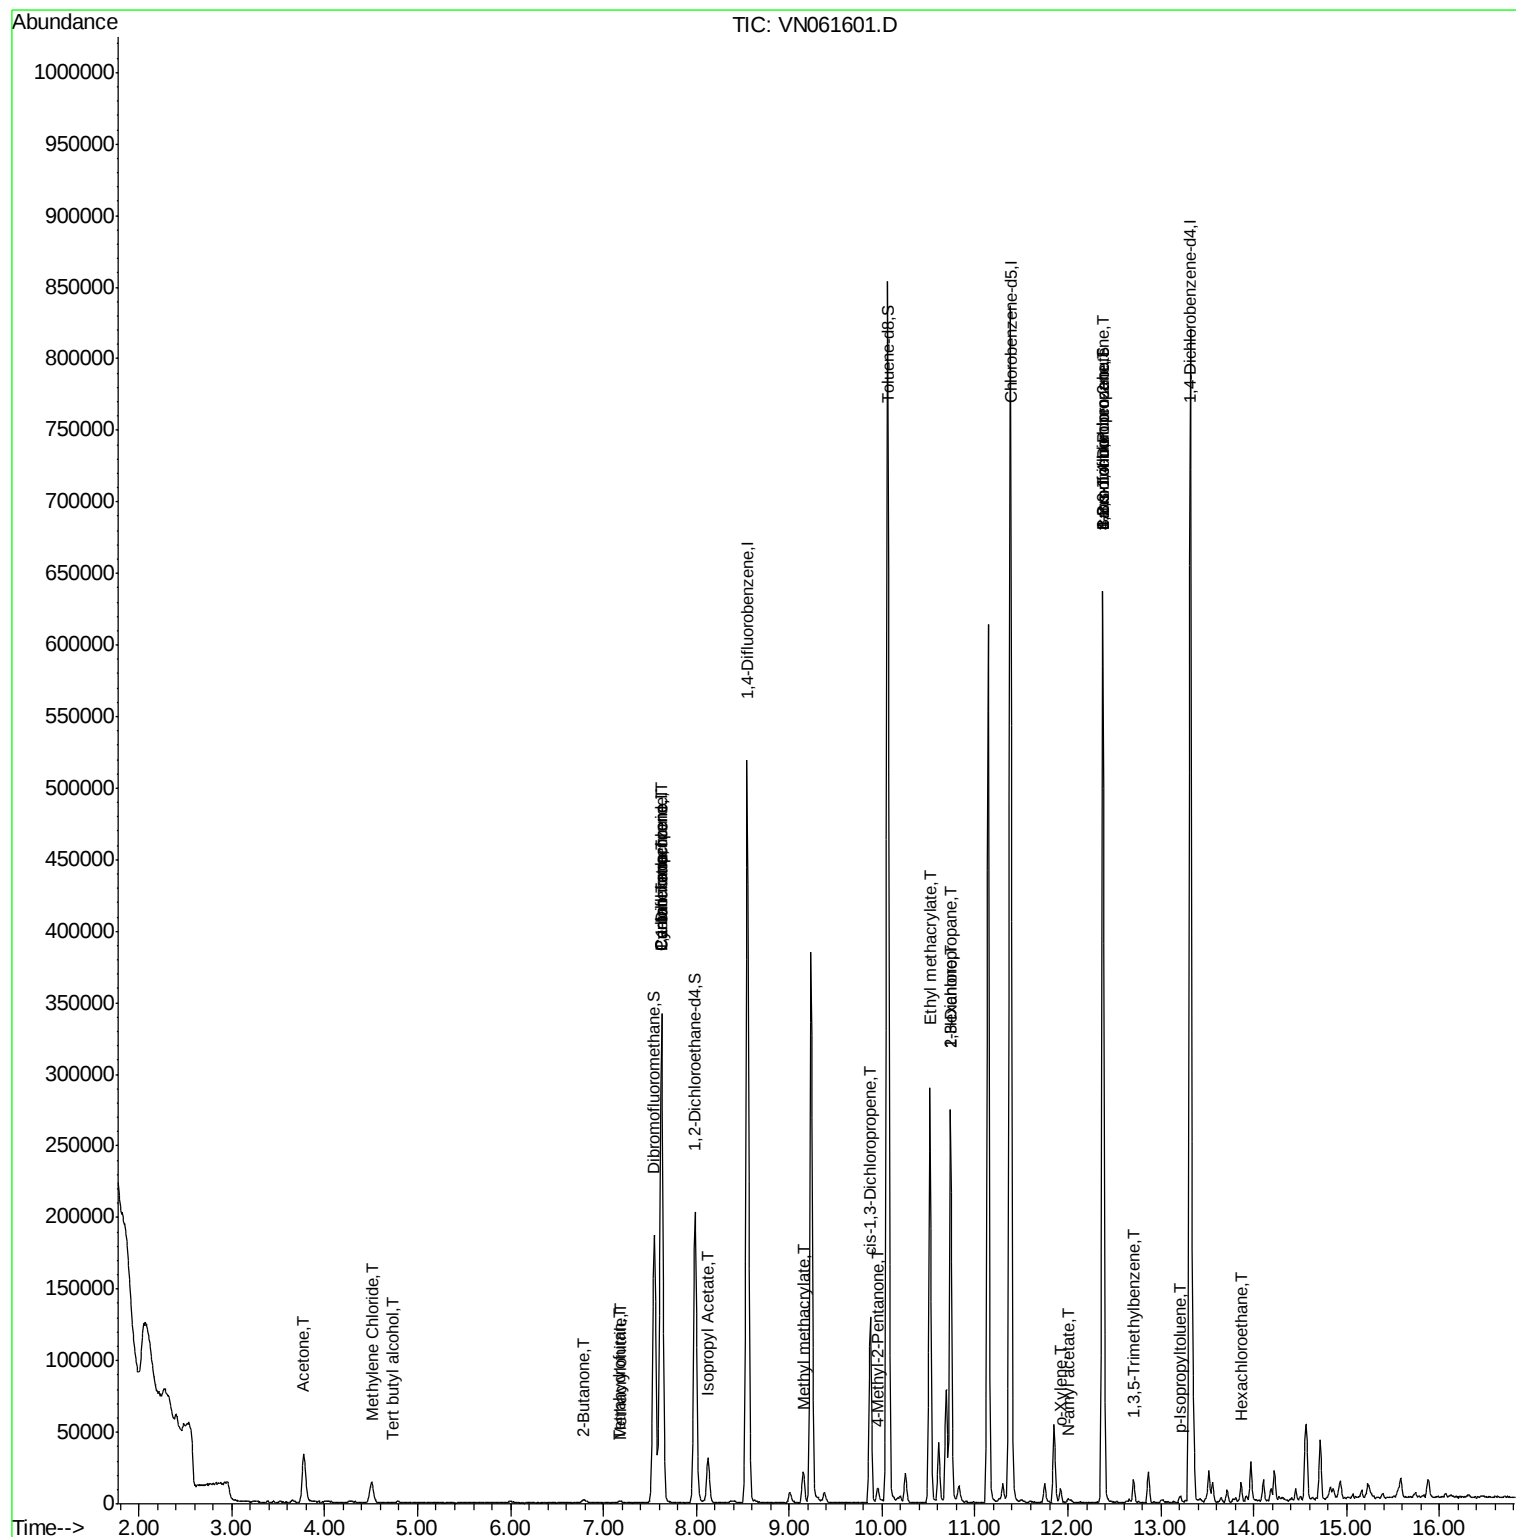



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. 0.00 min

Lab File: VN061601.D

Acq: 1 Jun 2020 17:43

Instrument :

MSVOA_N

ClientSampleId :


EO-02-052920

Tot Ion:168 Resp: 278958

Ion Ratio Lower Upper

168 100

99 58.9 45.0 67.4



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN



7.63

100000

50000

0

Time--> 7.50 7.60 7.70



#11

Tert butyl alcohol

Concen: 0.226 ug/l

RT: 4.73 min Scan# 918

Delta R.T. -0.01 min

Lab File: VN061601.D


Acq: 1 Jun 2020 17:43

Tgt Ion: 59 Resp: 100

Ion Ratio Lower Upper

59 100

57 0.0 8.4 12.6#



Abundance Ion 59.00 (58.70 to 59.70): VN

Ion 57.00 (56.70 to 57.70): VN

4.73

200


150


100

50

0

Time--> 4.71 4.72 4.73 4.74



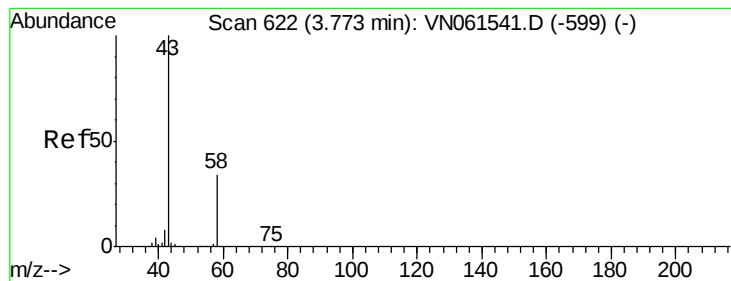

#16

Acetone

Concen: 57.073 ug/l

RT: 3.77 min Scan# 622

Delta R.T. 0.00 min

Lab File: VN061601.D

Acq: 1 Jun 2020 17:43

Instrument :

MSVOA_N

ClientSampleId :


EO-02-052920

Tot Ion: 43 Resp: 56661

Ion Ratio Lower Upper




43 100

58 36.1 27.2 40.8



Abundance Ion 43.00 (42.70 to 43.70): VN061601.D (-529) (-)

Ion 58.00 (57.70 to 58.70): VN061601.D (-529) (-)

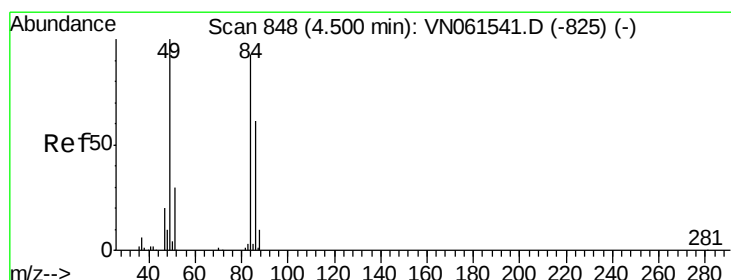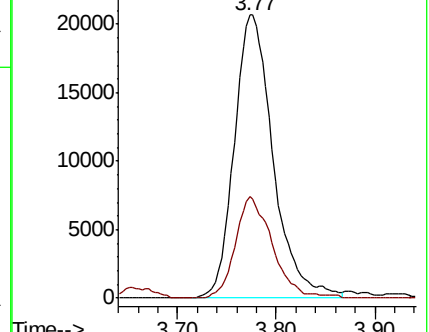

#20

Methylene Chloride

Concen: 2.336 ug/l

RT: 4.50 min Scan# 849

Delta R.T. 0.00 min

Lab File: VN061601.D

Acq: 1 Jun 2020 17:43

Tgt Ion: 84 Resp: 12067


Ion Ratio Lower Upper

84 100

49 99.4 85.8 128.8

51 31.3 26.2 39.2

86 59.5 52.6 78.8






Abundance Ion 83.90 (83.60 to 84.60): VN061601.D (-754) (-)

Ion 48.90 (48.60 to 49.60): VN061601.D (-754) (-)

Ion 50.90 (50.60 to 51.60): VN061601.D (-754) (-)

Ion 85.90 (85.60 to 86.60): VN061601.D (-754) (-)




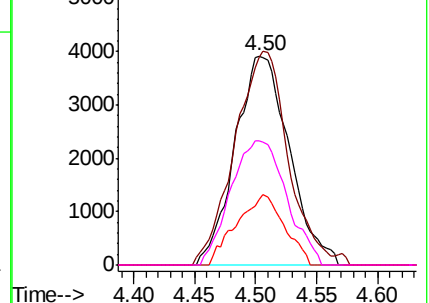




#25
2-Butanone
Concen: 2.312 ug/l
RT: 6.79 min Scan# 1559
Delta R.T. 0.00 min
Lab File: VN061601.D
Acq: 1 Jun 2020 17:43




Instrument :
MSVOA_N
ClientSampleId :
EO-02-052920


Tot Ion: 43 Resp: 3642
Ion Ratio Lower Upper
43 100
72 38.6 26.0 39.0

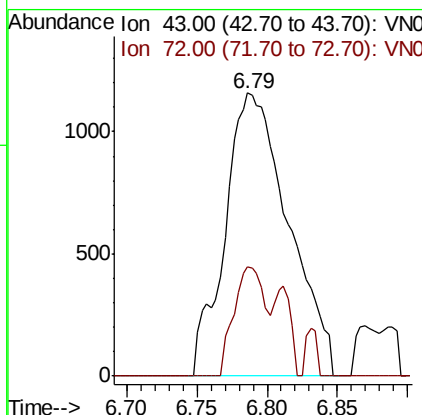

#29
Tetrahydrofuran
Concen: 0.348 ug/l
RT: 7.16 min Scan# 1676
Delta R.T. -0.00 min
Lab File: VN061601.D
Acq: 1 Jun 2020 17:43

Tgt Ion: 42 Resp: 361
Ion Ratio Lower Upper
42 100
72 0.0 43.6 65.4#
71 16.6 41.2 61.8#

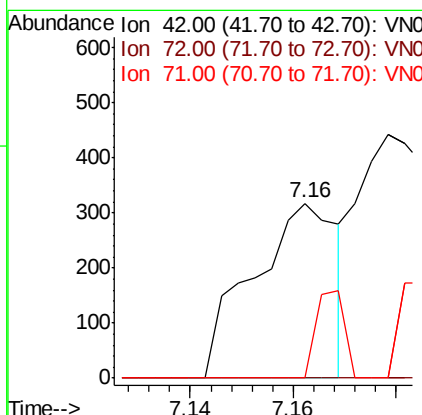

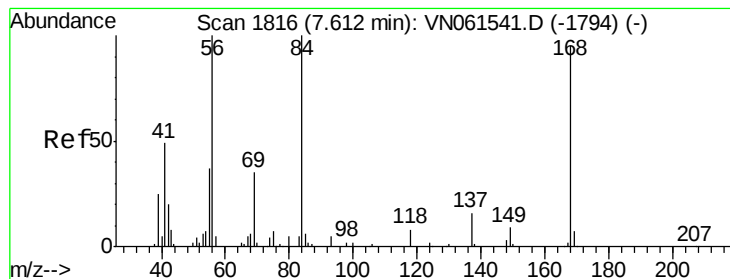

#31

Cyclohexane

Concen: 1.127 ug/l

RT: 7.62 min Scan# 1818

Delta R.T. 0.01 min

Lab File: VN061601.D

Acq: 1 Jun 2020 17:43

Instrument :

MSVOA_N

ClientSampleId :

EO-02-052920


Tot Ion: 56 Resp: 5277

Ion Ratio Lower Upper

56 100

69 165.0 27.8 41.8#




84 140.4 79.9 119.9#

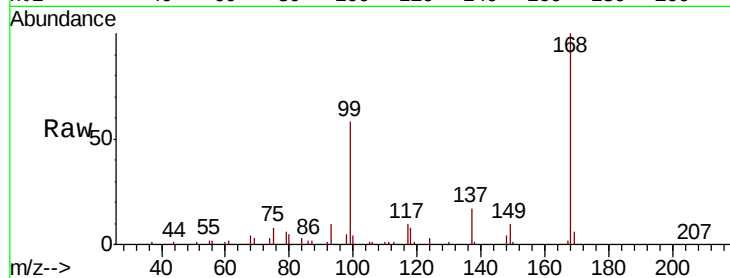

Abundance Ion 56.00 (55.70 to 56.70): VN0

Ion 69.00 (68.70 to 69.70): VN0

Ion 84.00 (83.70 to 84.70): VN0

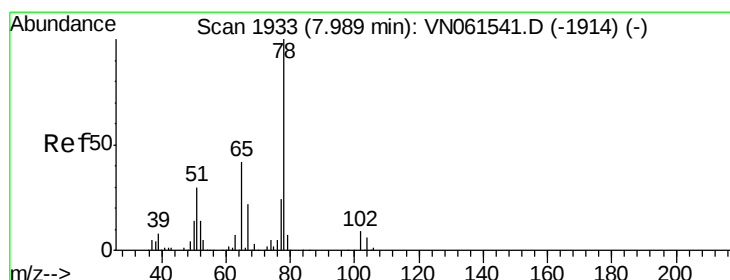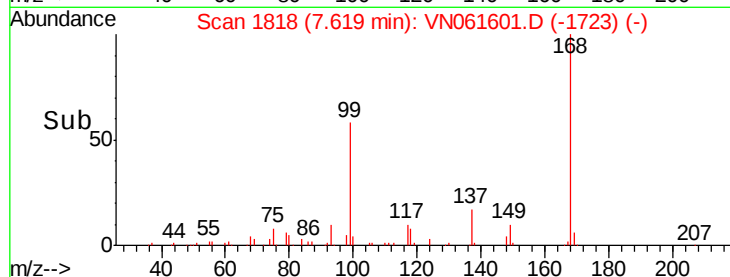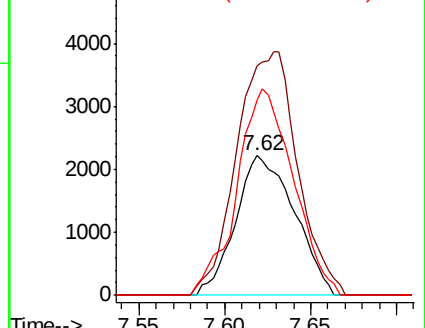

#33

1,2-Dichloroethane-d4

Concen: 52.082 ug/l

RT: 7.99 min Scan# 1932

Delta R.T. -0.00 min

Lab File: VN061601.D


Acq: 1 Jun 2020 17:43

Tgt Ion: 65 Resp: 173100

Ion Ratio Lower Upper



65 100


67 51.9 0.0 104.8

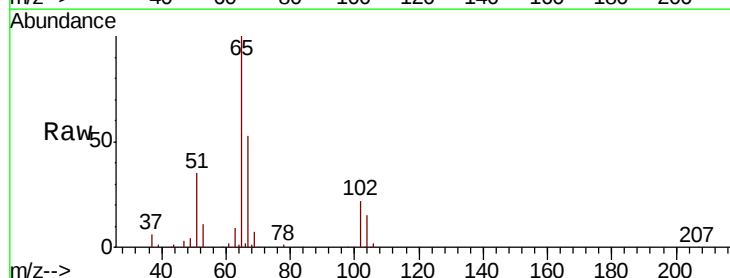

Abundance Ion 64.90 (64.60 to 65.60): VN0

Ion 66.90 (66.60 to 67.60): VN0

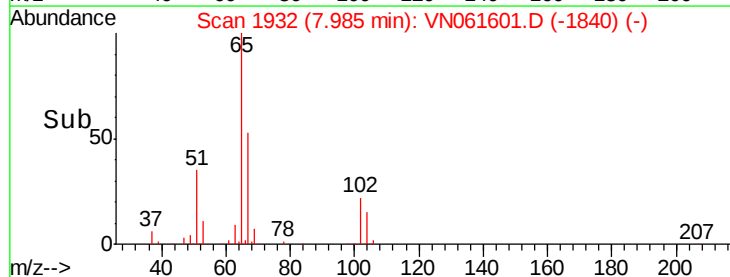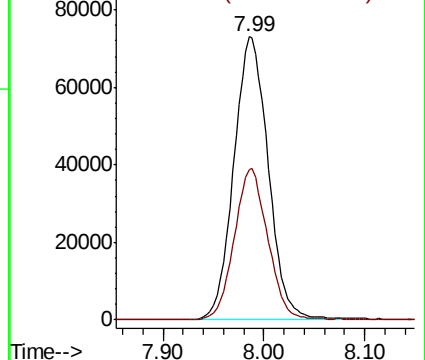







#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2108
 Delta R.T. 0.00 min
 Lab File: VN061601.D
 Acq: 1 Jun 2020 17:43

Instrument :
 MSVOA_N
 ClientSampleId :
 EO-02-052920

Tot Ion	Ratio	Lower	Upper
114	100		
63	18.4	0.0	35.8
88	15.3	0.0	31.0

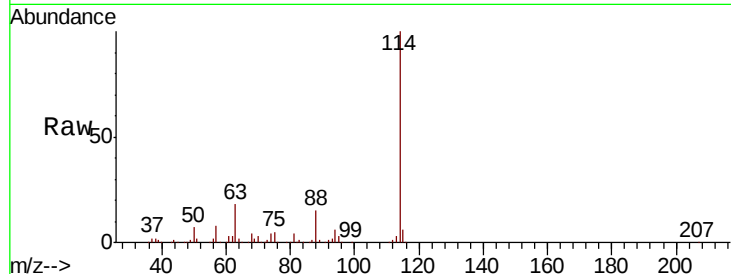


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VN
 Ion 87.90 (87.60 to 88.60): VN

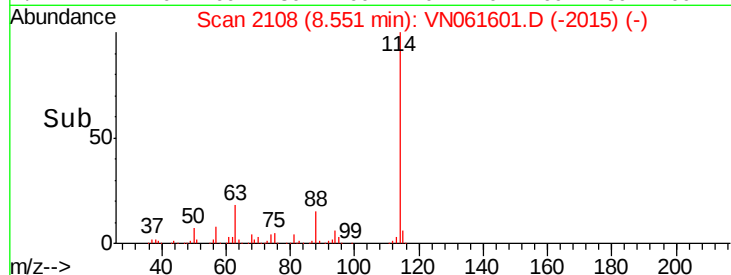
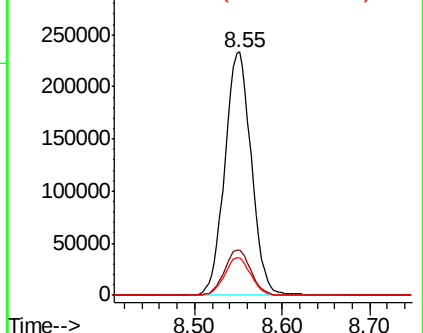



#35
 Dibromofluoromethane
 Concen: 58.016 ug/l
 RT: 7.55 min Scan# 1796
 Delta R.T. 0.00 min
 Lab File: VN061601.D
 Acq: 1 Jun 2020 17:43

Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.6	83.4	125.0
192	18.1	15.4	23.2



Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V




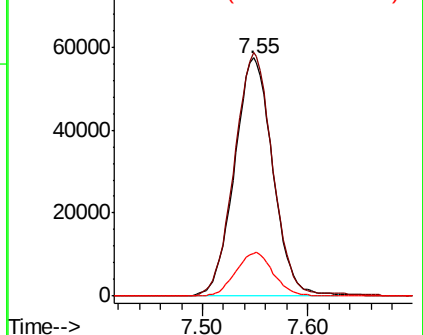




#36
 1,1-Dichloropropene
 Concen: 4.806 ug/l
 RT: 7.62 min Scan# 1819
 Delta R.T. -0.13 min
 Lab File: VN061601.D
 Acq: 1 Jun 2020 17:43




Instrument :
 MSVOA_N
 ClientSampleId :
 EO-02-052920


Tot Ion	75	Resp	20929
Ion Ratio	Lower	Upper	
75	100		
110	8.5	19.5	58.5#
77	0.0	24.7	37.1#

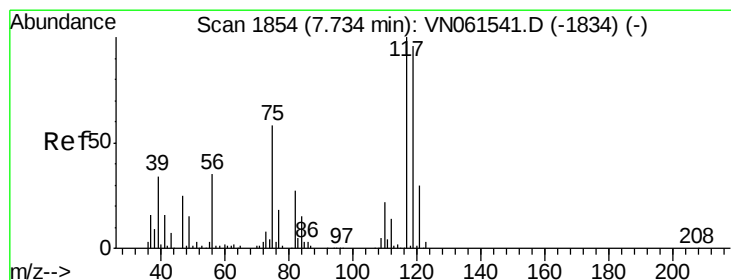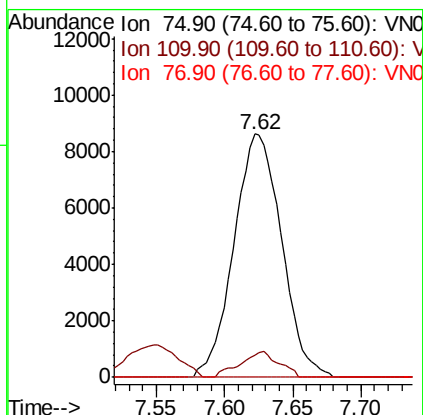

#38
 Carbon Tetrachloride
 Concen: 6.603 ug/l
 RT: 7.63 min Scan# 1820
 Delta R.T. -0.11 min
 Lab File: VN061601.D
 Acq: 1 Jun 2020 17:43

Tgt Ion	117	Resp	27735
Ion Ratio	Lower	Upper	
117	100		
119	4.0	76.5	114.7#
121	0.0	24.1	36.1#



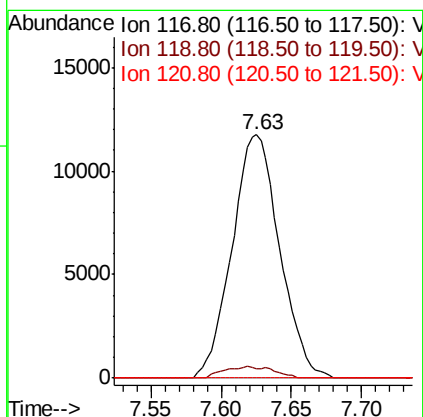





#41
Methacrylonitrile
Concen: 0.326 ug/l
RT: 7.18 min Scan# 1680
Delta R.T. 0.05 min
Lab File: VN061601.D
Acq: 1 Jun 2020 17:43




Instrument :
MSVOA_N
ClientSampled :
EO-02-052920


Tot Ion:	41	Resp:	524
Ion	Ratio	Lower	Upper
41	100		
39	0.0	53.8	80.6#
67	0.0	91.1	136.7#
52	0.0	36.0	54.0#

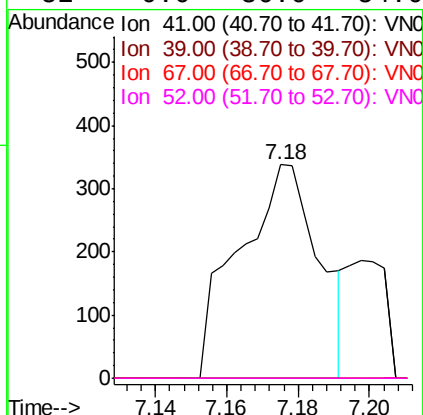

#43
Isopropyl Acetate
Concen: 5.643 ug/l
RT: 8.13 min Scan# 1976
Delta R.T. 0.00 min
Lab File: VN061601.D
Acq: 1 Jun 2020 17:43

Tgt Ion:	43	Resp:	35605
Ion	Ratio	Lower	Upper
43	100		
61	22.0	23.6	35.4#
87	16.9	13.0	19.6

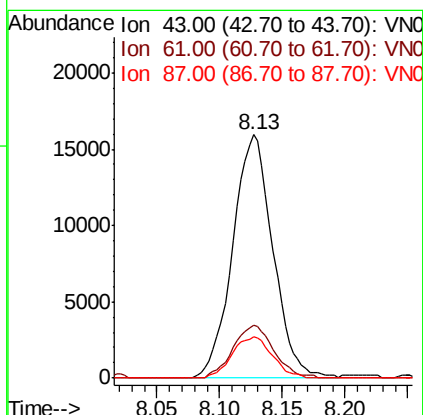







#48
Methvl methacrylate
Concen: 0.987 ug/l
RT: 9.14 min Scan# 2292
Delta R.T. -0.02 min
Lab File: VN061601.D
Acq: 1 Jun 2020 17:43

Instrument :
MSVOA_N
ClientSampleId :
EO-02-052920

Tot Ion: 41 Resp: 2802
Ion Ratio Lower Upper
41 100
69 0.0 83.9 125.9#
39 27.4 52.1 78.1#




Abundance Ion 41.00 (40.70 to 41.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 39.00 (38.70 to 39.70): VN0


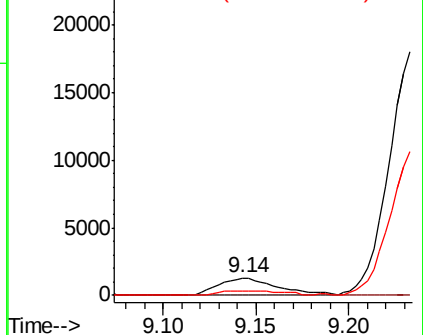



#50
Toluene-d8
Concen: 53.222 ug/l
RT: 10.06 min Scan# 2577
Delta R.T. 0.00 min
Lab File: VN061601.D
Acq: 1 Jun 2020 17:43

Tgt Ion: 98 Resp: 615444
Ion Ratio Lower Upper
98 100
100 66.0 52.8 79.2



Abundance Ion 98.00 (97.70 to 98.70): VN0
Ion 100.00 (99.70 to 100.70): VN0

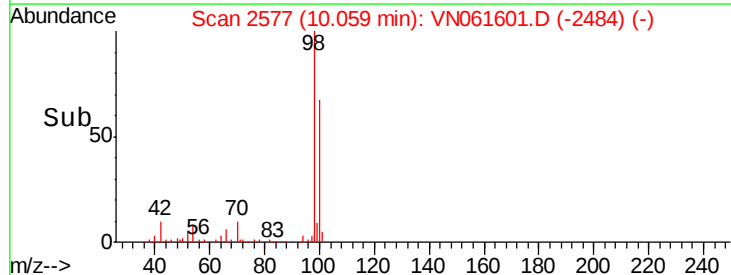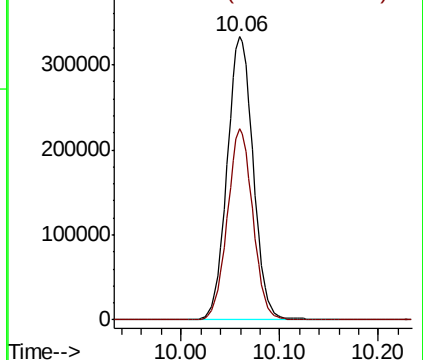



#51

4-Methyl-2-Pentanone

Concen: 1.829 ug/l

RT: 9.96 min Scan# 2545

Delta R.T. 0.00 min

Lab File: VN061601.D

Acq: 1 Jun 2020 17:43

Instrument :

MSVOA_N

ClientSampleId :


EO-02-052920

Tot Ion: 43 Resp: 6505




Ion Ratio Lower Upper

43 100

58 43.9 35.0 52.6



Abundance Ion 43.00 (42.70 to 43.70): VN061601.D (-2528) (-)

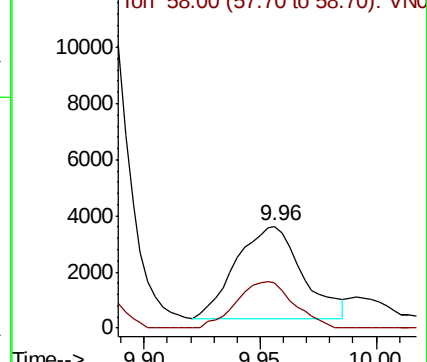

#54

cis-1,3-Dichloropropene

Concen: 4.795 ug/l

RT: 9.87 min Scan# 2519

Delta R.T. 0.06 min

Lab File: VN061601.D

Acq: 1 Jun 2020 17:43


Tgt Ion: 75 Resp: 26926

Ion Ratio Lower Upper



75 100


77 0.0 25.4 38.2#

39 26.7 33.8 50.6#



Abundance Ion 74.90 (74.60 to 75.60): VN061601.D (-2483) (-)

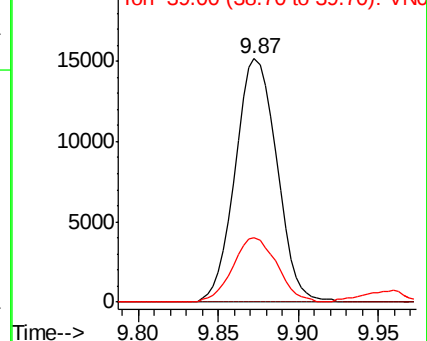



#56

Ethyl methacrylate

Concen: 0.220 ug/l

RT: 10.51 min Scan# 2718

Delta R.T. 0.11 min

Lab File: VN061601.D

Acq: 1 Jun 2020 17:43

Instrument :

MSVOA_N

ClientSampleId :

EO-02-052920


Tot Ion: 69 Resp: 1075

Ion Ratio Lower Upper

69 100

41 4671.0 43.5 65.3#




39 2118.1 27.0 40.6#



Abundance Ion 69.00 (68.70 to 69.70): VN0

Ion 41.00 (40.70 to 41.70): VN0

Ion 39.00 (38.70 to 39.70): VN0

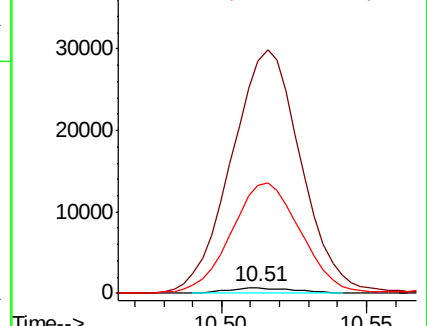

#57

1,3-Dichloropropane

Concen: 0.572 ug/l

RT: 10.73 min Scan# 2787

Delta R.T. 0.05 min

Lab File: VN061601.D


Acq: 1 Jun 2020 17:43

Tgt Ion: 76 Resp: 3198

Ion Ratio Lower Upper



76 100


78 0.0 26.3 39.5#



Abundance Ion 75.90 (75.60 to 76.60): VN0

Ion 77.90 (77.60 to 78.60): VN0




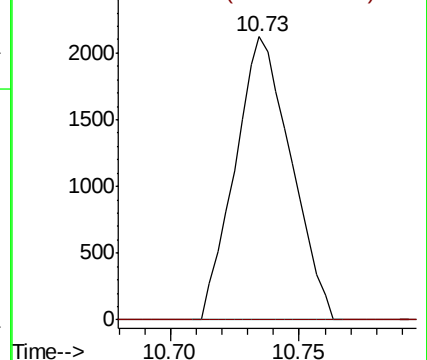




#59
2-Hexanone
Concen: 13.664 ug/l
RT: 10.74 min Scan# 2788
Delta R.T. 0.01 min
Lab File: VN061601.D
Acq: 1 Jun 2020 17:43




Instrument :
MSVOA_N
ClientSampleId :
EO-02-052920


Tot Ion: 43 Resp: 34894
Ion Ratio Lower Upper
43 100
58 21.5 30.7 92.1#

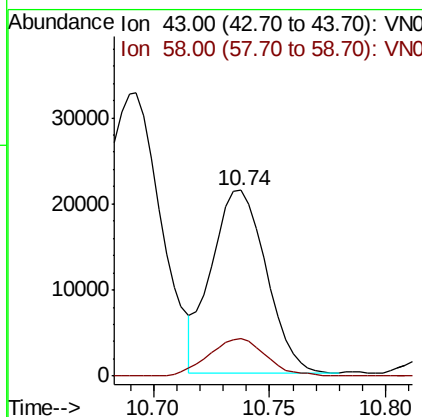

#62
4-Bromofluorobenzene
Concen: 53.931 ug/l
RT: 12.37 min Scan# 3297
Delta R.T. -0.00 min
Lab File: VN061601.D
Acq: 1 Jun 2020 17:43

Tgt Ion: 95 Resp: 227526
Ion Ratio Lower Upper
95 100
174 80.2 0.0 172.8
176 76.8 0.0 164.8

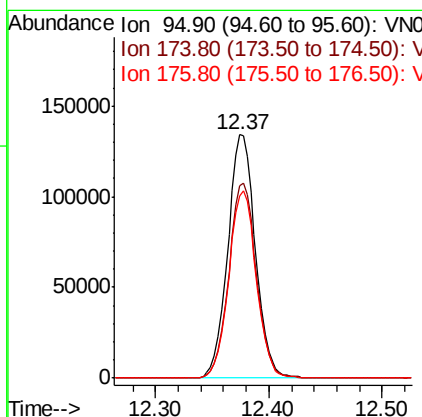







#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2988
Delta R.T. 0.00 min
Lab File: VN061601.D
Acq: 1 Jun 2020 17:43

Instrument :
MSVOA_N
ClientSampleId :
EO-02-052920

Tot Ion:117 Resp: 510252
Ion Ratio Lower Upper
117 100
82 52.5 41.5 62.3
119 32.1 25.6 38.4




Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VN
Ion 118.90 (118.60 to 119.60): V


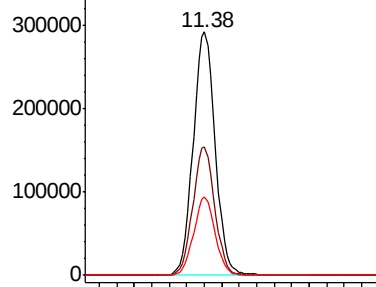



#69
o-Xylene
Concen: 0.410 ug/l
RT: 11.92 min Scan# 3156
Delta R.T. 0.00 min
Lab File: VN061601.D
Acq: 1 Jun 2020 17:43

Tgt Ion:106 Resp: 2833
Ion Ratio Lower Upper
106 100
91 219.4 103.3 309.8



Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VN

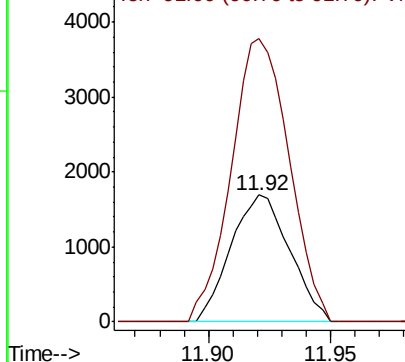

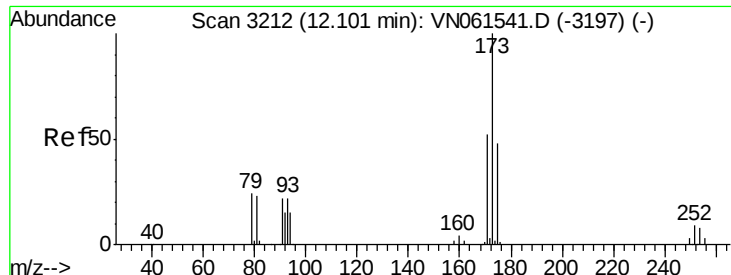

#71

Bromoform

Concen: 0.534 ug/l

RT: 12.38 min Scan# 3298

Delta R.T. 0.28 min

Lab File: VN061601.D

Acq: 1 Jun 2020 17:43

Instrument :

MSVOA_N

ClientSampleId :

EO-02-052920


Tot Ion:173 Resp: 1626

Ion Ratio Lower Upper

173 100

175 739.7 24.4 73.2#




254 0.0 0.0 0.0



Abundance Ion 172.70 (172.40 to 173.40): V

Ion 174.70 (174.40 to 175.40): V

Ion 254.40 (254.10 to 255.10): V

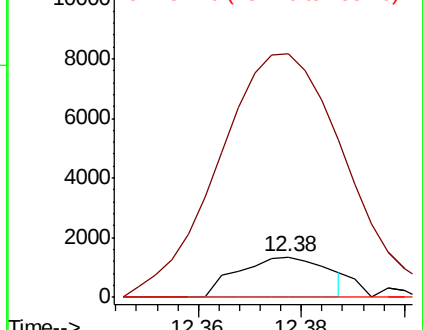

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3590

Delta R.T. 0.00 min

Lab File: VN061601.D

Acq: 1 Jun 2020 17:43


Tgt Ion:152 Resp: 226220

Ion Ratio Lower Upper

152 100

115 59.7 28.0 84.0



150 159.4 0.0 344.0




Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V



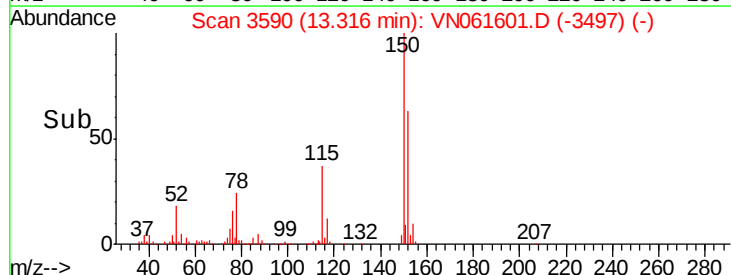
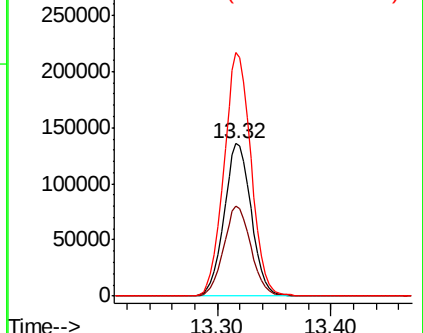




#74
N-amvl acetate
Concen: 0.634 ug/l
RT: 12.00 min Scan# 3182
Delta R.T. -0.04 min
Lab File: VN061601.D
Acq: 1 Jun 2020 17:43




Instrument :
MSVOA_N
ClientSampleId :
EO-02-052920


Tot Ion: 43 Resp: 3296
Ion Ratio Lower Upper
43 100
70 0.0 40.5 60.7#
55 0.9 20.6 31.0#
61 0.0 21.8 32.6#

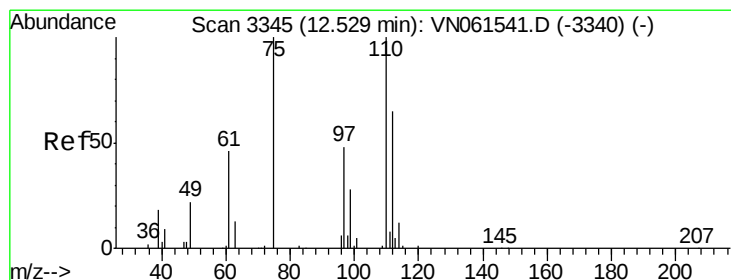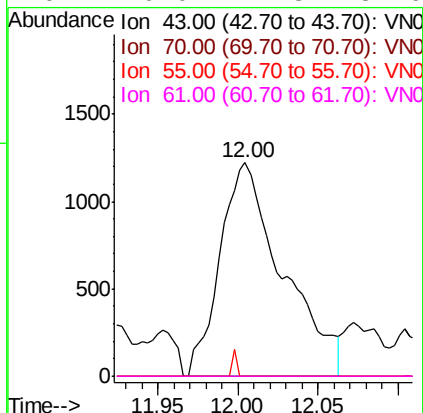

#76
1,2,3-Trichloropropane
Concen: 27.322 ug/l
RT: 12.37 min Scan# 3297
Delta R.T. -0.15 min
Lab File: VN061601.D
Acq: 1 Jun 2020 17:43

Tgt Ion: 75 Resp: 112392
Ion Ratio Lower Upper
75 100
77 1.4 0.0 0.0#

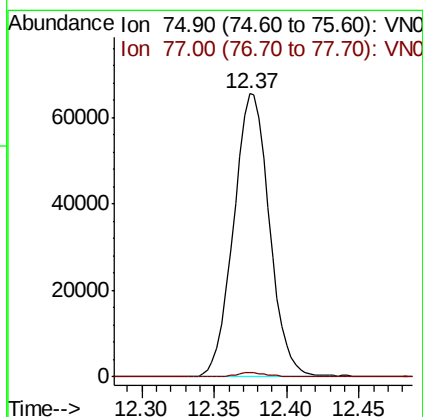



#80

1,3,5-Trimethylbenzene

Concen: 0.678 ug/l

RT: 12.71 min Scan# 3400

Delta R.T. -0.00 min

Lab File: VN061601.D

Acq: 1 Jun 2020 17:43

Instrument :

MSVOA_N

ClientSampleId :


EO-02-052920

Tot Ion:105 Resp: 9362

Ion Ratio Lower Upper




105 100

120 43.3 25.1 75.2



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

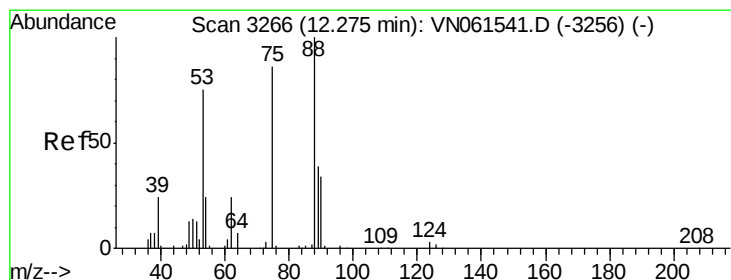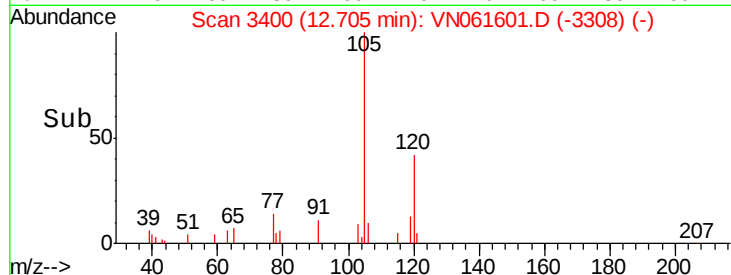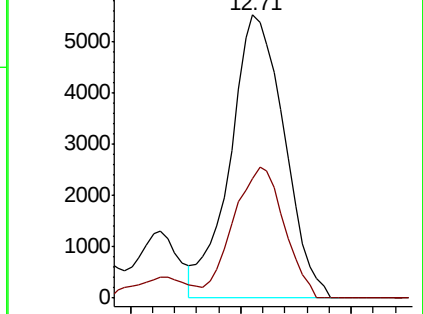

#81

trans-1,4-Dichloro-2-butene

Concen: 69.871 ug/l

RT: 12.37 min Scan# 3297

Delta R.T. 0.10 min

Lab File: VN061601.D

Acq: 1 Jun 2020 17:43


Tgt Ion: 75 Resp: 112392

Ion Ratio Lower Upper

75 100

53 0.0 67.8 101.8#



89 0.0 37.1 55.7#




Abundance Ion 74.90 (74.60 to 75.60): VNO

Ion 53.00 (52.70 to 53.70): VNO

Ion 88.90 (88.60 to 89.60): VNO

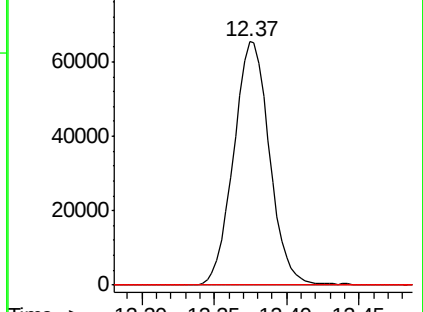


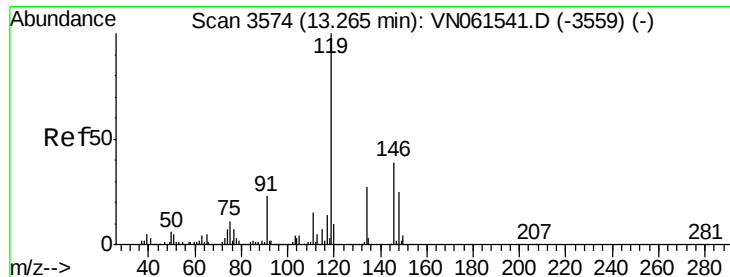




#86
 p-Isopropyltoluene
 Concen: 0.233 ug/l
 RT: 13.21 min Scan# 3556
 Delta R.T. -0.06 min
 Lab File: VN061601.D
 Acq: 1 Jun 2020 17:43

Instrument :
 MSVOA_N
 ClientSampleId :
 EO-02-052920

Tot Ion	Ratio	Lower	Upper
119	100		
134	27.3	13.5	40.5
91	24.1	11.4	34.1

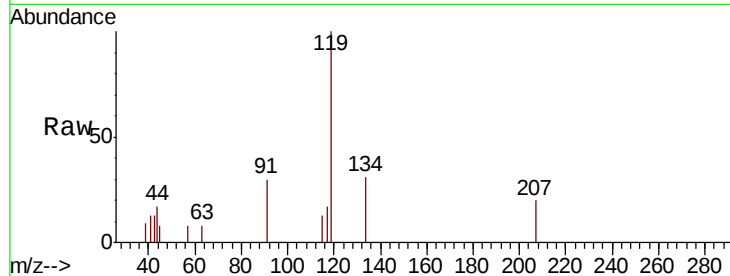


Abundance Ion 119.00 (118.70 to 119.70): V
 Ion 134.00 (133.70 to 134.70): V
 Ion 91.00 (90.70 to 91.70): V

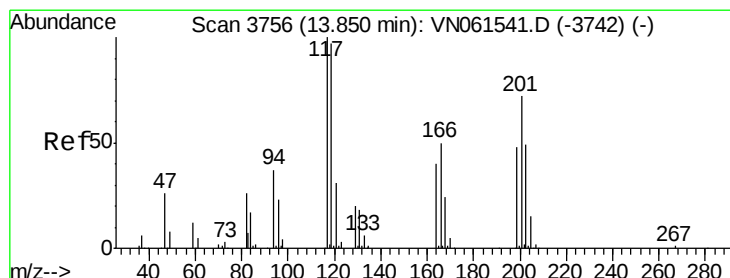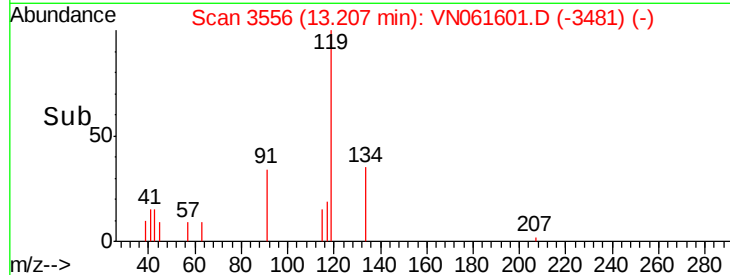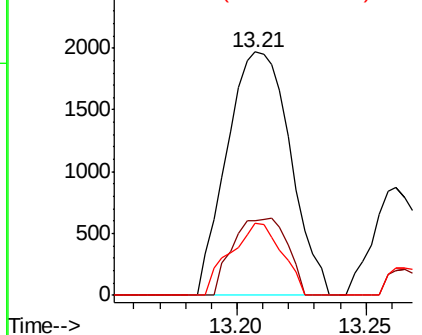

#90
 Hexachloroethane
 Concen: 0.489 ug/l
 RT: 13.86 min Scan# 3760
 Delta R.T. 0.01 min
 Lab File: VN061601.D
 Acq: 1 Jun 2020 17:43

Tgt Ion	Ratio	Lower	Upper
117	100		
201	0.0	36.7	110.1#

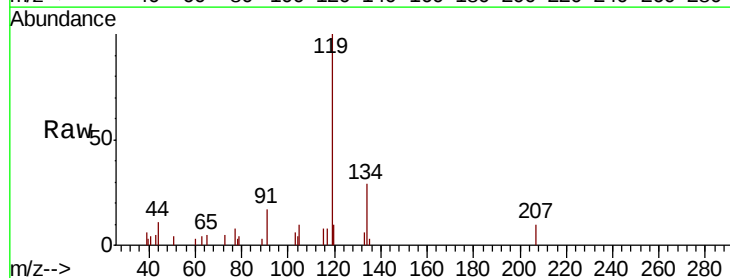

Abundance Ion 116.80 (116.50 to 117.50): V
 Ion 200.70 (200.40 to 201.40): V

