

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060123\
 Data File : VN078016.D
 Acq On : 01 Jun 2023 17:38
 Operator : JC\MD
 Sample : 02958-01MEDL 40X
 Misc : 1.09g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 11 Sample Multiplier: 1


Instrument :
 MSVOA_N
 ClientSampleId :
 ORA-0588DL

Quant Time: Jun 02 01:54:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
 Quant Title : SW846 8260
 QLast Update : Tue May 16 04:07:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.236	168	429521	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.112	114	782878	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.877	117	704576	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.800	152	238141	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.589	65	295293	45.948	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	91.900%		
35) Dibromofluoromethane	8.177	113	251150	49.196	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	98.400%		
50) Toluene-d8	10.577	98	962875	49.002	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	98.000%		
62) 4-Bromofluorobenzene	12.859	95	328158	47.286	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	94.580%		
Target Compounds						Qvalue
3) Chloromethane	2.365	50	1538	Below Cal		92
5) Bromomethane	2.965	94	1925	0.422 ug/l #		38
11) Tert butyl alcohol	5.506	59	1004	1.132 ug/l #		72
13) Acrolein	4.195	56	159	Below Cal #		82
16) Acetone	4.442	43	655	0.324 ug/l #		40
20) Methylene Chloride	5.277	84	891	Below Cal #		82
31) Cyclohexane	8.230	56	18327	2.098 ug/l #		61
36) 1,1-Dichloropropene	8.236	75	36691	4.914 ug/l #		41
38) Carbon Tetrachloride	8.236	117	47716	6.328 ug/l #		16
39) Methylcyclohexane	9.606	83	5740	0.628 ug/l		92
43) Isopropyl Acetate	8.712	43	4403	0.405 ug/l #		49
52) Toluene	10.641	92	308039	22.456 ug/l		98
55) 1,1,2-Trichloroethane	11.012	97	1191	0.219 ug/l #		36
58) 2-Chloroethyl Vinyl ether	10.171	63	3918	0.967 ug/l		93
59) 2-Hexanone	11.177	43	1241	0.260 ug/l #		19
67) Ethyl Benzene	11.977	91	17336	0.633 ug/l #		88
68) m/p-Xylenes	12.077	106	16256	1.567 ug/l		95
69) o-Xylene	12.406	106	7121	0.698 ug/l		85
73) Isopropylbenzene	12.706	105	4324	0.211 ug/l		95
74) N-amyl acetate	12.488	43	2620	0.345 ug/l #		43
76) 1,2,3-Trichloropropane	12.859	75	174198	29.209 ug/l #		1
78) n-propylbenzene	13.047	91	11091	0.458 ug/l		96
80) 1,3,5-Trimethylbenzene	13.182	105	9598	0.556 ug/l		95
81) trans-1,4-Dichloro-2-b...	12.859	75	174198	93.366 ug/l #		15
83) tert-Butylbenzene	13.482	119	5265	0.350 ug/l #		61
84) 1,2,4-Trimethylbenzene	13.488	105	32202	1.898 ug/l		99
85) sec-Butylbenzene	13.623	105	4832	0.226 ug/l		95
86) p-Isopropyltoluene	13.682	119	4591	0.269 ug/l		86
89) n-Butylbenzene	14.065	91	4194	0.267 ug/l #		76
90) Hexachloroethane	14.341	117	1474	0.526 ug/l #		21
95) Naphthalene	15.647	128	4774	0.293 ug/l #		67

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.236 min Scan# 1

Delta R.T. 0.006 min

Lab File: VN078016.D

Acq: 01 Jun 2023 17:38

Instrument :

MSVOA_N

ClientSampleId :





ORA-0588DL

Tgt Ion:168 Resp: 429521

Ion Ratio Lower Upper

168 100

99 63.6 53.0 79.6

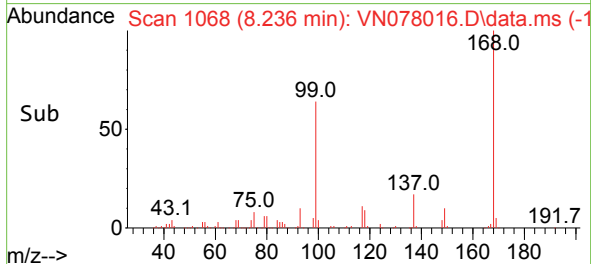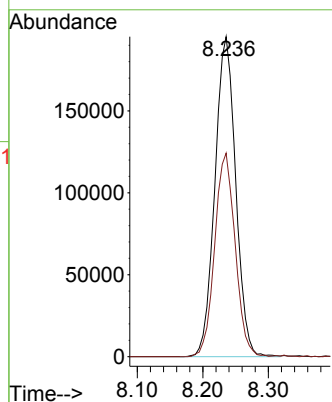

#3

Chloromethane

Concen: Below Cal

RT: 2.365 min Scan# 70

Delta R.T. 0.000 min

Lab File: VN078016.D




Acq: 01 Jun 2023 17:38


Tgt Ion: 50 Resp: 1538

Ion Ratio Lower Upper

50 100

52 37.9 26.5 39.7




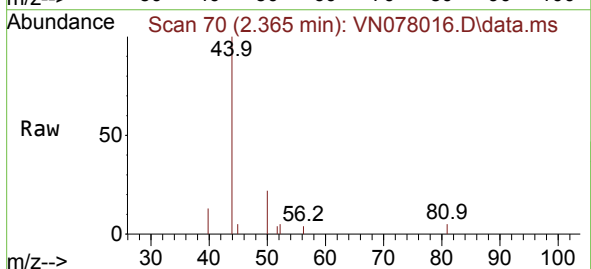




#5
Bromomethane
Concen: 0.422 ug/l
RT: 2.965 min Scan# 11
Delta R.T. 0.018 min
Lab File: VN078016.D
Acq: 01 Jun 2023 17:38




Instrument :
MSVOA_N
ClientSampleId :
ORA-0588DL


Tgt Ion: 94 Resp: 1925
Ion Ratio Lower Upper
94 100
96 32.8 73.1 109.7#

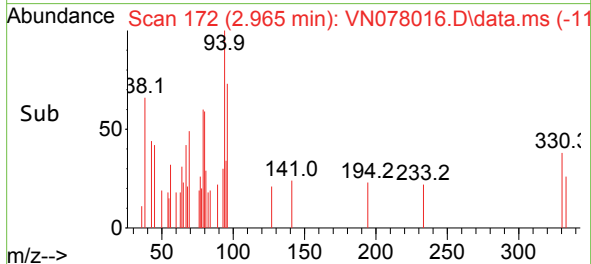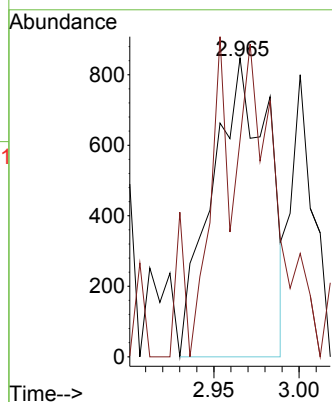

#11
Tert butyl alcohol
Concen: 1.132 ug/l
RT: 5.506 min Scan# 604
Delta R.T. -0.024 min
Lab File: VN078016.D
Acq: 01 Jun 2023 17:38

Tgt Ion: 59 Resp: 1004
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#

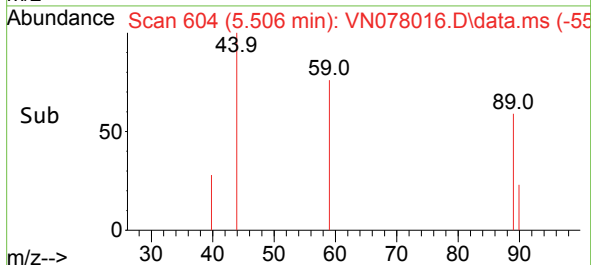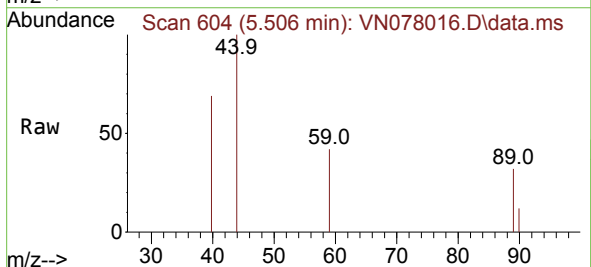



#13

Acrolein

Concen: Below Cal

RT: 4.195 min Scan# 381

Delta R.T. 0.006 min

Lab File: VN078016.D

Acq: 01 Jun 2023 17:38

Instrument :

MSVOA_N

ClientSampleId :





ORA-0588DL

Tgt Ion: 56 Resp: 159

Ion Ratio Lower Upper

56 100

55 82.4 54.5 81.7#

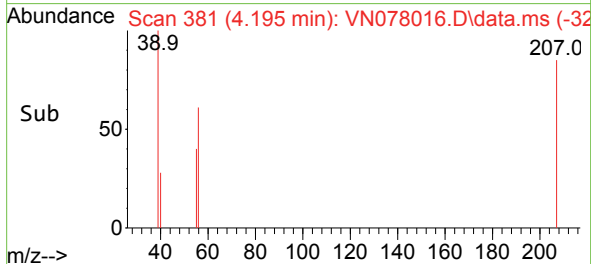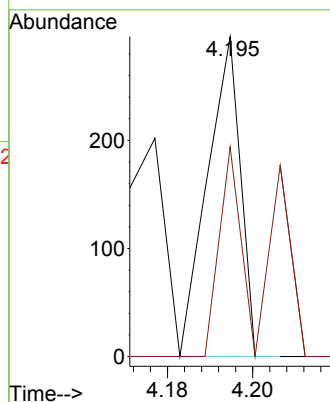

#16

Acetone

Concen: 0.324 ug/l

RT: 4.442 min Scan# 423

Delta R.T. 0.012 min

Lab File: VN078016.D




Acq: 01 Jun 2023 17:38


Tgt Ion: 43 Resp: 655

Ion Ratio Lower Upper

43 100


58 0.0 28.0 42.0#

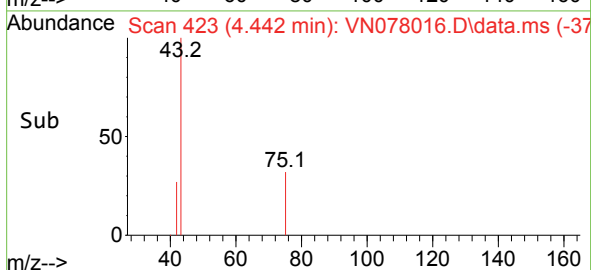






#20
Methylene Chloride
Concen: Below Cal
RT: 5.277 min Scan# 51
Delta R.T. -0.006 min
Lab File: VN078016.D
Acq: 01 Jun 2023 17:38

Instrument :
MSVOA_N
ClientSampleId :
ORA-0588DL







Tgt Ion:	84	Resp:	891
Ion	Ratio	Lower	Upper
84	100		
49	95.3	79.7	119.5
51	54.9	25.2	37.8#
86	88.2	53.3	79.9#

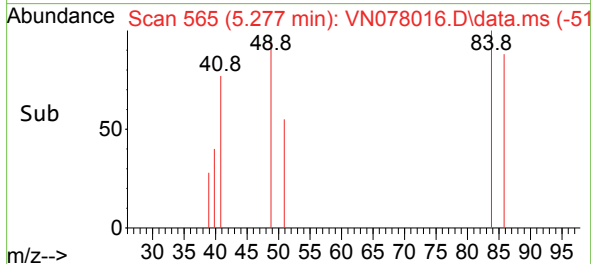

#31
Cyclohexane
Concen: 2.098 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.035 min
Lab File: VN078016.D
Acq: 01 Jun 2023 17:38

Tgt Ion:	56	Resp:	18327
Ion	Ratio	Lower	Upper
56	100		
69	73.8	26.8	40.2#
84	72.7	81.8	122.6#

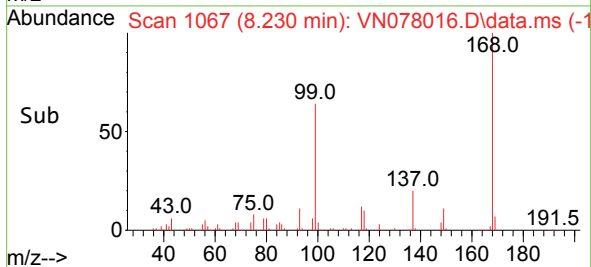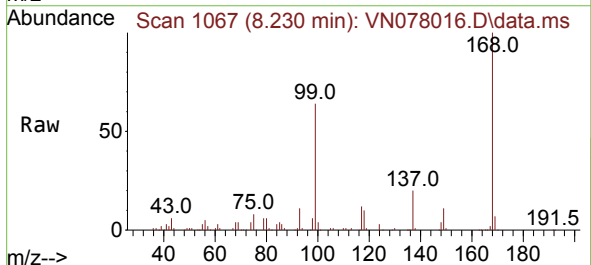



#33

1,2-Dichloroethane-d4

Concen: 45.948 ug/l

RT: 8.589 min Scan# 1128

Delta R.T. 0.007 min

Lab File: VN078016.D

Acq: 01 Jun 2023 17:38

Instrument :

MSVOA_N

ClientSampleId :





ORA-0588DL

Tgt Ion: 65 Resp: 295293

Ion Ratio Lower Upper

65 100

67 51.0 0.0 106.6

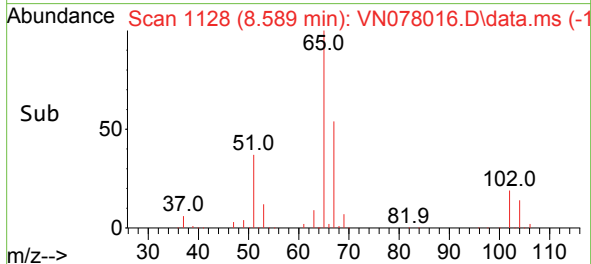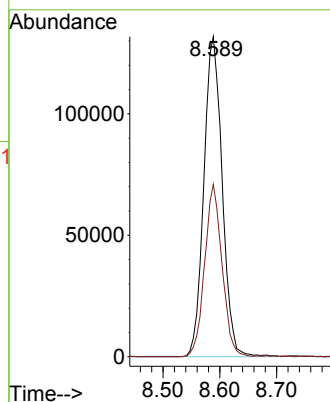

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.112 min Scan# 1217

Delta R.T. 0.006 min

Lab File: VN078016.D

Acq: 01 Jun 2023 17:38




Tgt Ion: 114 Resp: 782878


Ion Ratio Lower Upper

114 100

63 19.3 0.0 36.4

88 15.3 0.0 30.6


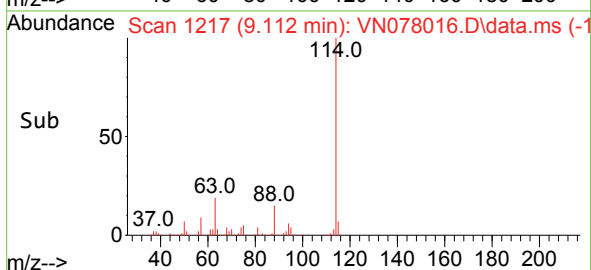






#35
 Dibromofluoromethane
 Concen: 49.196 ug/l
 RT: 8.177 min Scan# 1057
 Delta R.T. 0.006 min
 Lab File: VN078016.D
 Acq: 01 Jun 2023 17:38




Instrument :
 MSVOA_N
 ClientSampleId :
 ORA-0588DL


Tgt Ion:113 Resp: 251150
 Ion Ratio Lower Upper
 113 100
 111 102.7 82.6 123.8
 192 16.9 12.7 19.1

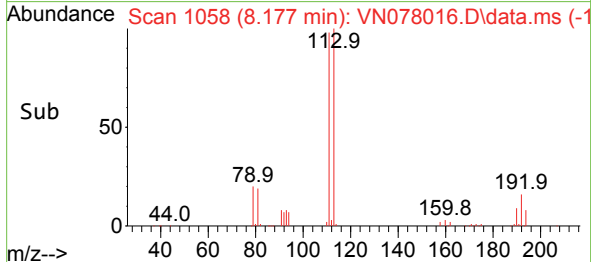

#36
 1,1-Dichloropropene
 Concen: 4.914 ug/l
 RT: 8.236 min Scan# 1068
 Delta R.T. -0.141 min
 Lab File: VN078016.D
 Acq: 01 Jun 2023 17:38

Tgt Ion: 75 Resp: 36691
 Ion Ratio Lower Upper
 75 100
 110 1.6 19.1 57.3#
 77 0.0 25.0 37.4#


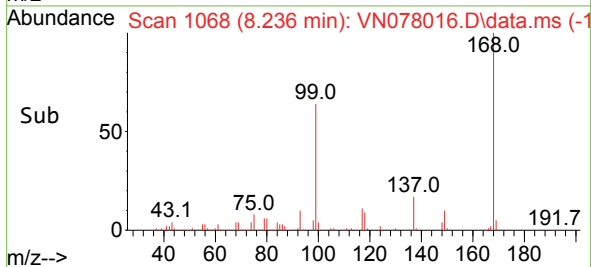

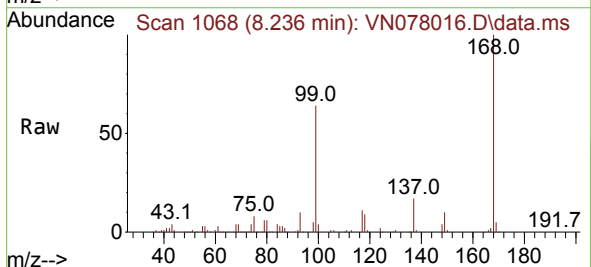




#38
Carbon Tetrachloride
Concen: 6.328 ug/l
RT: 8.236 min Scan# 1068
Delta R.T. -0.135 min
Lab File: VN078016.D
Acq: 01 Jun 2023 17:38




Instrument :
MSVOA_N
ClientSampleId :
ORA-0588DL


Tgt Ion:117 Resp: 47716
Ion Ratio Lower Upper
117 100
119 5.2 77.3 115.9#
121 0.0 23.3 34.9#

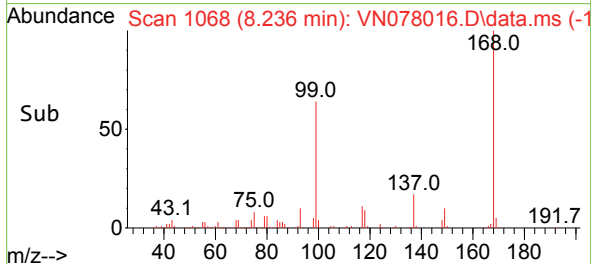

#39
Methylcyclohexane
Concen: 0.628 ug/l
RT: 9.606 min Scan# 1301
Delta R.T. 0.000 min
Lab File: VN078016.D
Acq: 01 Jun 2023 17:38

Tgt Ion: 83 Resp: 5740
Ion Ratio Lower Upper
83 100
55 54.2 49.1 73.7
98 46.2 40.6 61.0


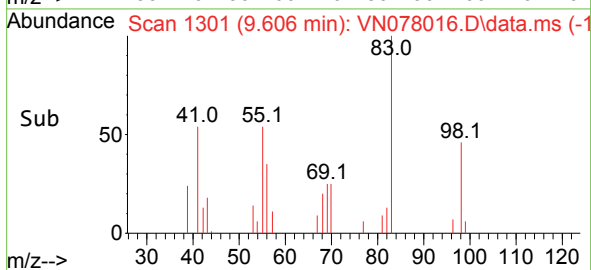

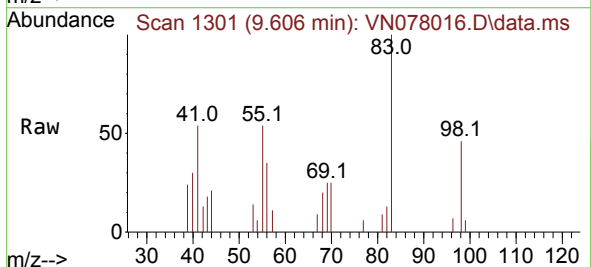




#43
Isopropyl Acetate
Concen: 0.405 ug/l
RT: 8.712 min Scan# 1149
Delta R.T. 0.018 min
Lab File: VN078016.D
Acq: 01 Jun 2023 17:38




Instrument :
MSVOA_N
ClientSampleId :
ORA-0588DL


Tgt Ion: 43 Resp: 4403
Ion Ratio Lower Upper
43 100
61 0.0 24.7 37.1#
87 0.0 14.6 21.8#

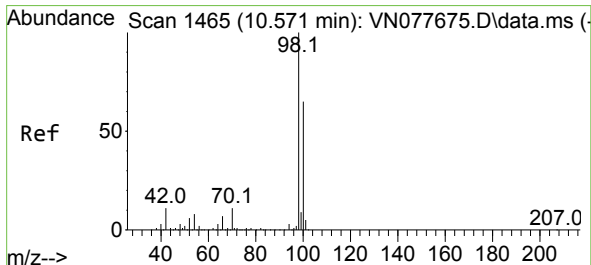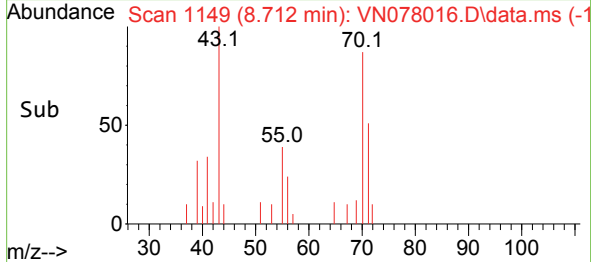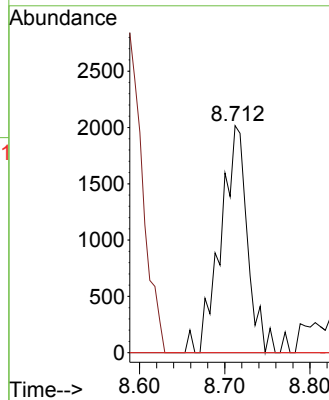

#50
Toluene-d8
Concen: 49.002 ug/l
RT: 10.577 min Scan# 1466
Delta R.T. 0.006 min
Lab File: VN078016.D
Acq: 01 Jun 2023 17:38

Tgt Ion: 98 Resp: 962875
Ion Ratio Lower Upper
98 100
100 63.5 52.0 78.0

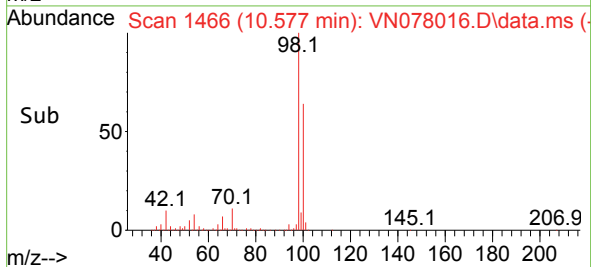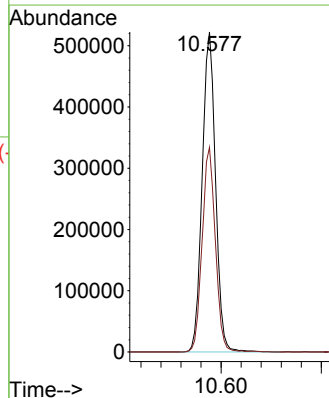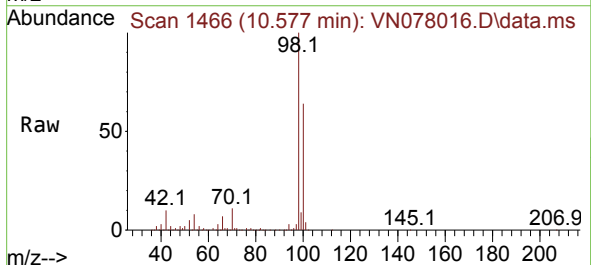



#52

Toluene

Concen: 22.456 ug/l

RT: 10.641 min Scan# 1476

Delta R.T. 0.006 min

Lab File: VN078016.D

Acq: 01 Jun 2023 17:38

Instrument :

MSVOA_N

ClientSampleId :





ORA-0588DL

Tgt Ion: 92 Resp: 308039

Ion Ratio Lower Upper

92 100

91 174.9 137.4 206.0

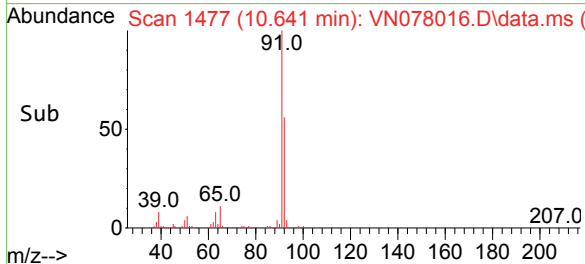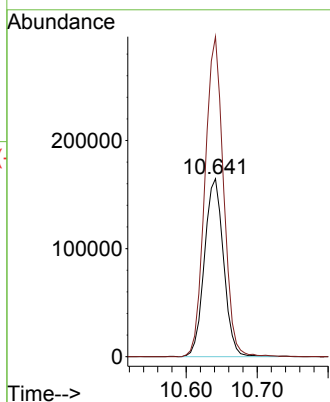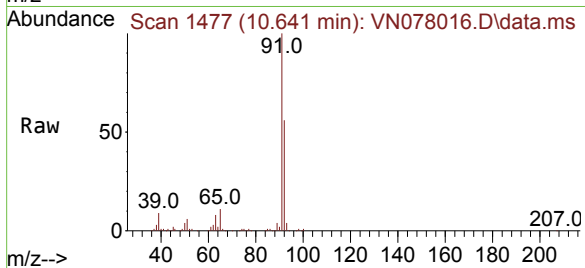

#55

1,1,2-Trichloroethane

Concen: 0.219 ug/l

RT: 11.012 min Scan# 1540

Delta R.T. -0.011 min

Lab File: VN078016.D

Acq: 01 Jun 2023 17:38

Tgt Ion: 97 Resp: 1191




Ion Ratio Lower Upper


97 100

83 43.3 65.1 97.7#

85 0.0 43.4 65.2#

99 0.0 49.2 73.8#


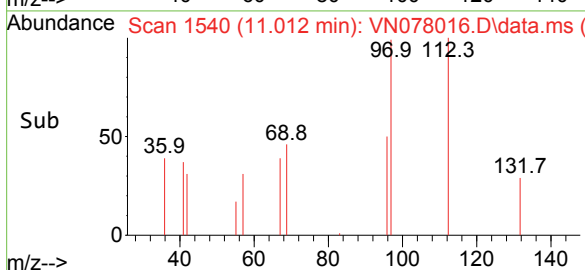

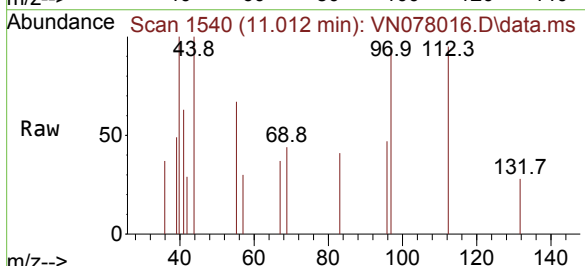




#58
2-Chloroethyl Vinyl ether
Concen: 0.967 ug/l
RT: 10.171 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN078016.D
Acq: 01 Jun 2023 17:38




Instrument :
MSVOA_N
ClientSampleId :
ORA-0588DL


Tgt Ion: 63 Resp: 3918
Ion Ratio Lower Upper
63 100
106 28.9 26.2 39.4

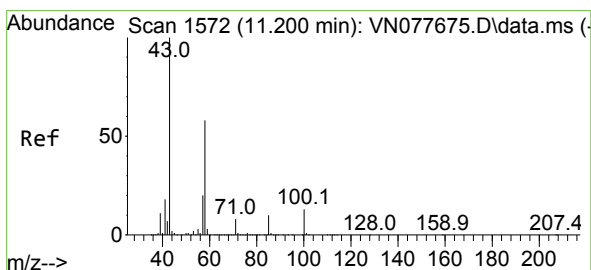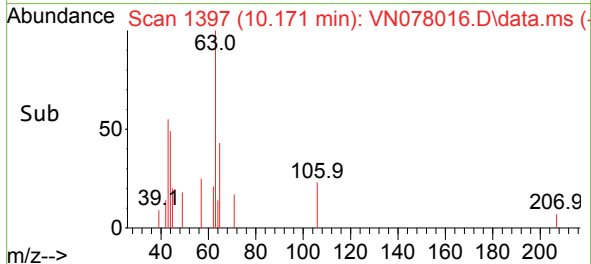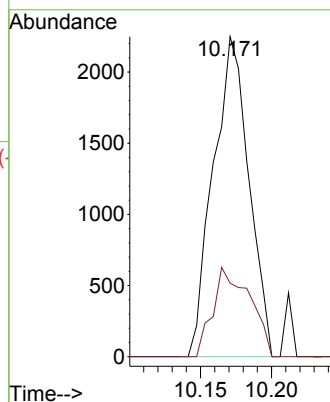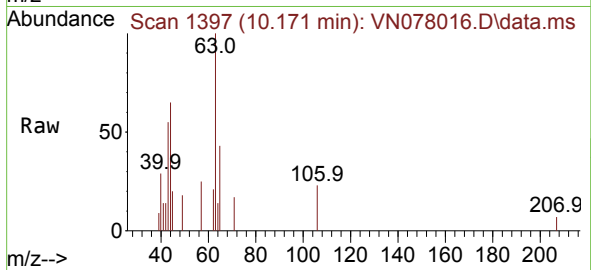

#59
2-Hexanone
Concen: 0.260 ug/l
RT: 11.177 min Scan# 1568
Delta R.T. -0.023 min
Lab File: VN078016.D
Acq: 01 Jun 2023 17:38

Tgt Ion: 43 Resp: 1241
Ion Ratio Lower Upper
43 100
58 0.0 31.7 95.1#


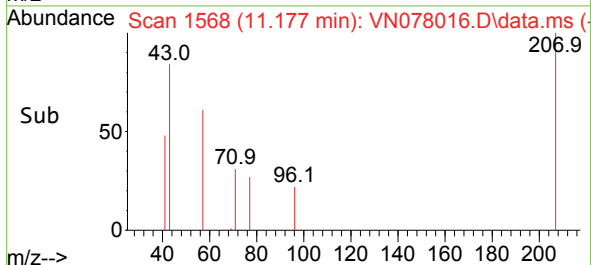

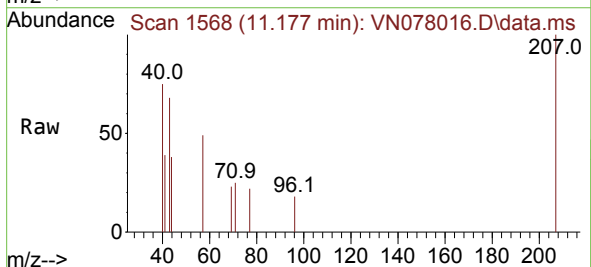


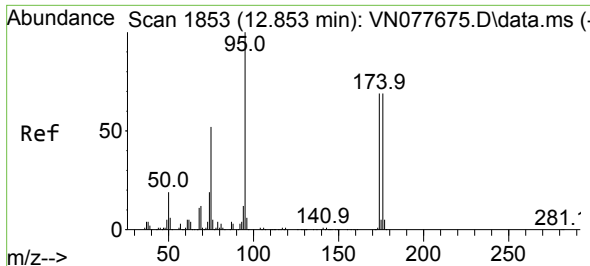

#62
4-Bromofluorobenzene
Concen: 47.286 ug/l
RT: 12.859 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN078016.D
Acq: 01 Jun 2023 17:38




Instrument :
MSVOA_N
ClientSampleId :
ORA-0588DL


Tgt Ion: 95 Resp: 328158
Ion Ratio Lower Upper
95 100
174 73.4 0.0 143.8
176 68.8 0.0 135.8

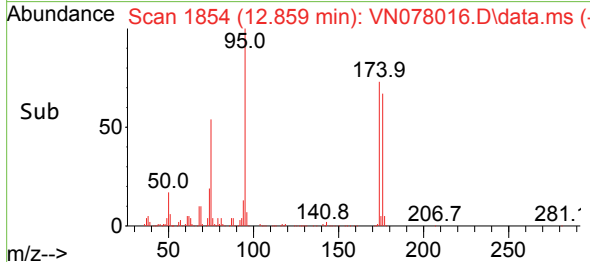

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.877 min Scan# 1687
Delta R.T. 0.007 min
Lab File: VN078016.D
Acq: 01 Jun 2023 17:38

Tgt Ion: 117 Resp: 704576
Ion Ratio Lower Upper
117 100
82 54.7 44.0 66.0
119 30.7 25.6 38.4


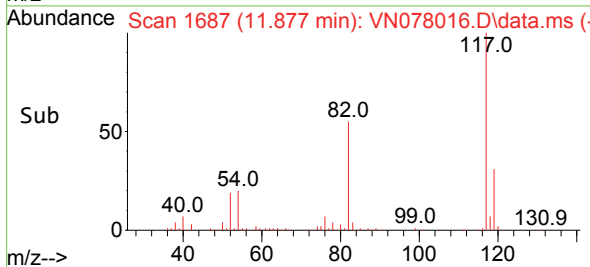

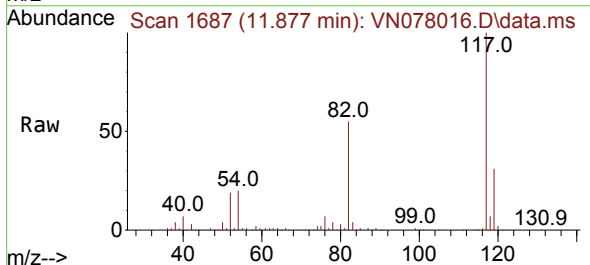


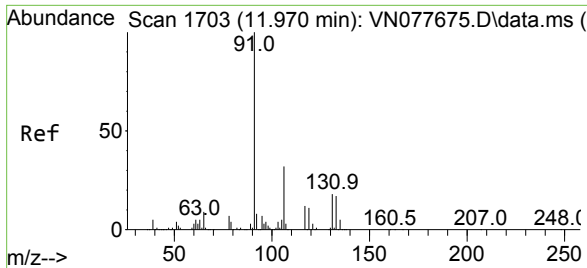

#67
Ethyl Benzene
Concen: 0.633 ug/l
RT: 11.977 min Scan# 1704
Delta R.T. 0.007 min
Lab File: VN078016.D
Acq: 01 Jun 2023 17:38




Instrument :
MSVOA_N
ClientSampleId :
ORA-0588DL


Tgt Ion: 91 Resp: 17336
Ion Ratio Lower Upper
91 100
106 25.3 25.6 38.4#

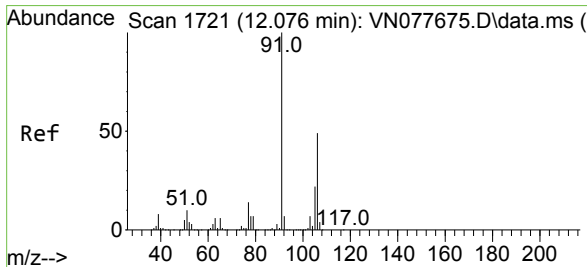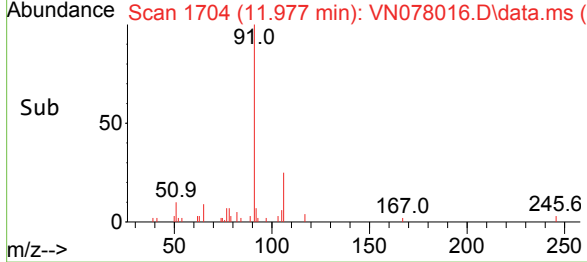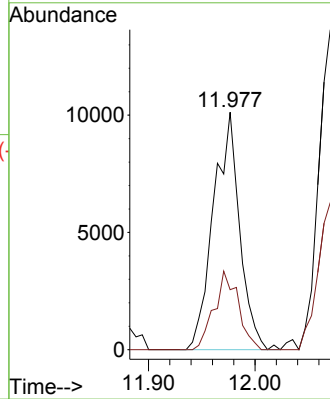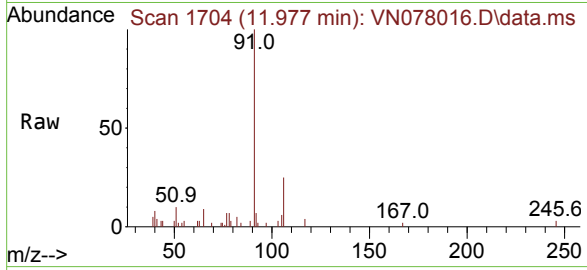

#68
m/p-Xylenes
Concen: 1.567 ug/l
RT: 12.077 min Scan# 1721
Delta R.T. 0.001 min
Lab File: VN078016.D
Acq: 01 Jun 2023 17:38

Tgt Ion: 106 Resp: 16256
Ion Ratio Lower Upper
106 100
91 206.6 159.6 239.4


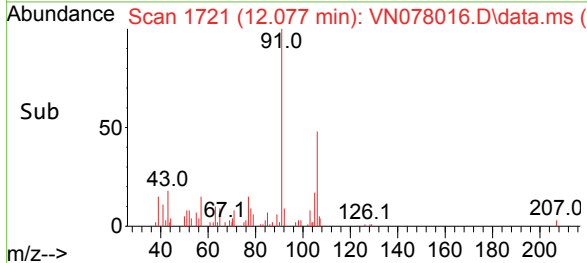
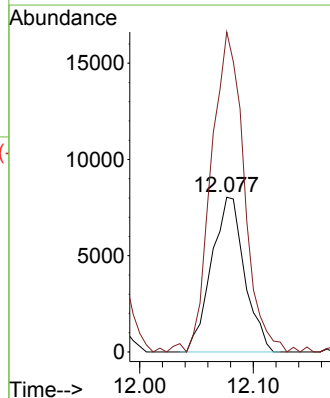
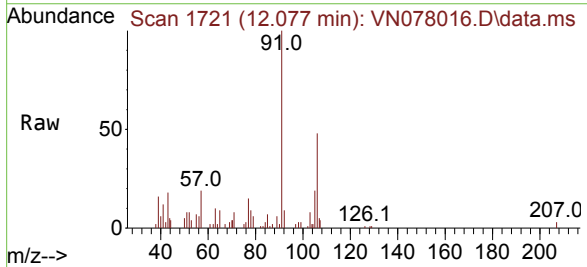


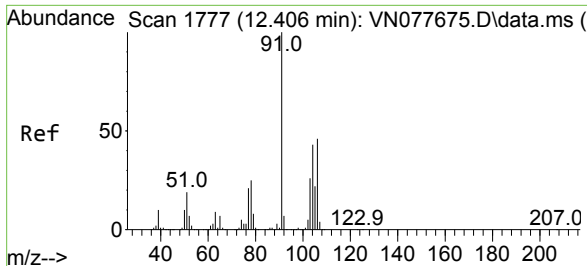

#69
o-Xylene
Concen: 0.698 ug/l
RT: 12.406 min Scan# 1777
Delta R.T. -0.000 min
Lab File: VN078016.D
Acq: 01 Jun 2023 17:38




Instrument :
MSVOA_N
ClientSampleId :
ORA-0588DL


Tgt Ion:106 Resp: 7121
Ion Ratio Lower Upper
106 100
91 234.0 105.2 315.5

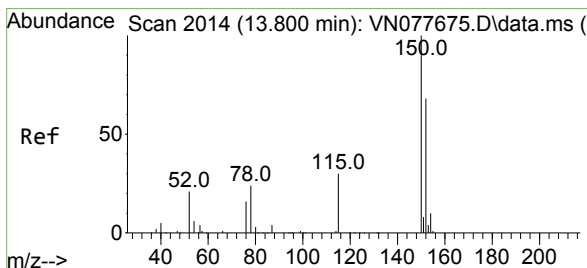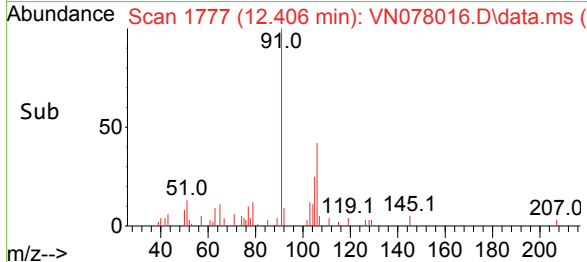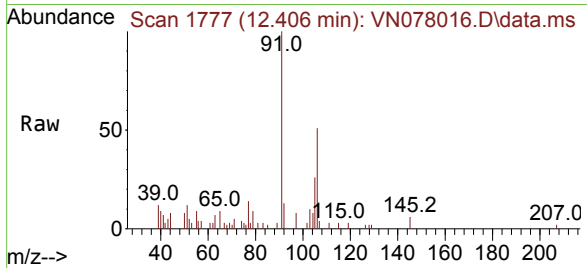

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.800 min Scan# 2014
Delta R.T. -0.000 min
Lab File: VN078016.D
Acq: 01 Jun 2023 17:38

Tgt Ion:152 Resp: 238141
Ion Ratio Lower Upper
152 100
115 63.0 32.3 96.8
150 157.9 0.0 355.8


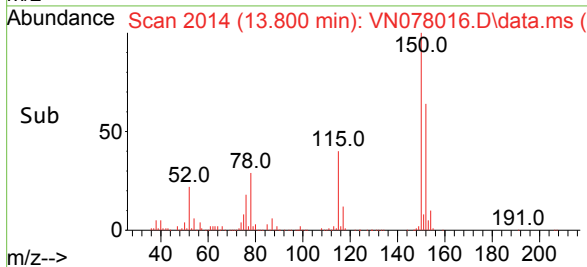

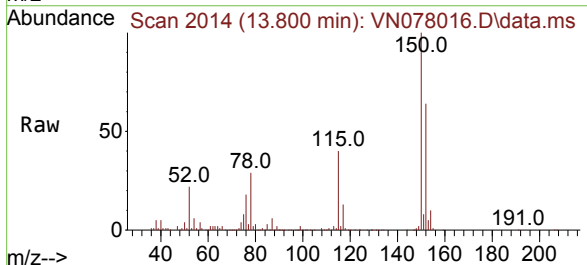




#73
Isopropylbenzene
Concen: 0.211 ug/l
RT: 12.706 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN078016.D
Acq: 01 Jun 2023 17:38




Instrument :
MSVOA_N
ClientSampleId :
ORA-0588DL


Tgt Ion:105 Resp: 4324
Ion Ratio Lower Upper
105 100
120 28.6 13.1 39.1

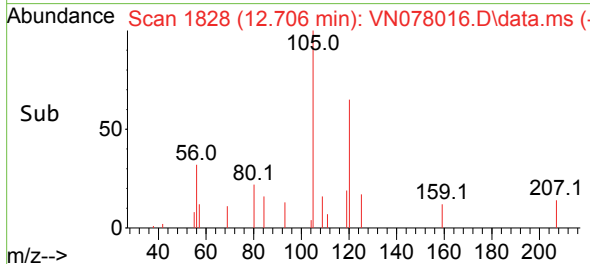

#74
N-ethyl acetate
Concen: 0.345 ug/l
RT: 12.488 min Scan# 1791
Delta R.T. -0.012 min
Lab File: VN078016.D
Acq: 01 Jun 2023 17:38

Tgt Ion: 43 Resp: 2620
Ion Ratio Lower Upper
43 100
70 8.5 43.4 65.2#
55 51.6 21.4 32.0#
61 0.0 22.8 34.2#

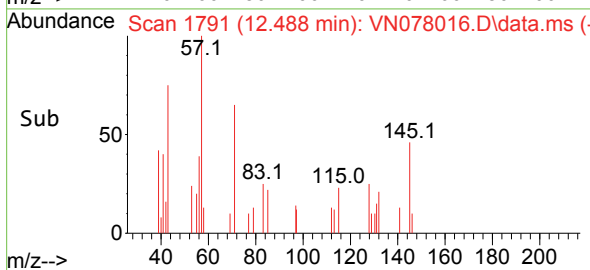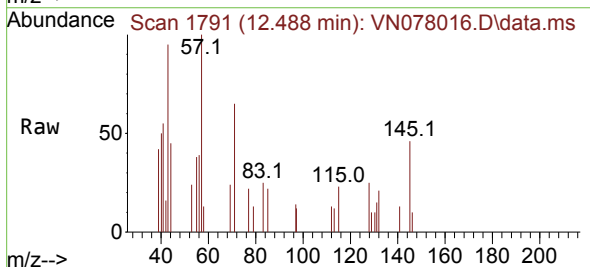



#76

1,2,3-Trichloropropane

Concen: 29.209 ug/l

RT: 12.859 min Scan# 1854

Delta R.T. -0.141 min

Lab File: VN078016.D

Acq: 01 Jun 2023 17:38

Instrument :

MSVOA_N

ClientSampleId :





ORA-0588DL

Tgt Ion: 75 Resp: 174198

Ion Ratio Lower Upper

75 100

77 1.4 84.5 253.5#

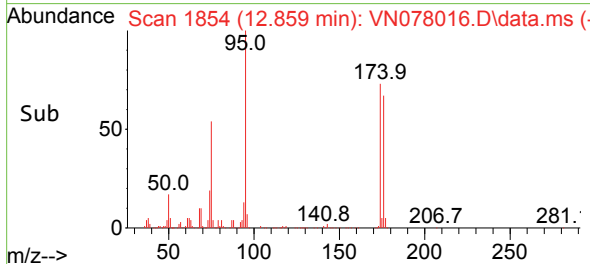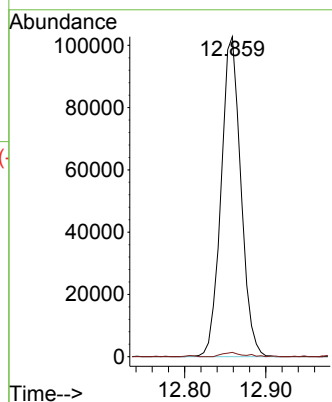

#78

n-propylbenzene

Concen: 0.458 ug/l

RT: 13.047 min Scan# 1886

Delta R.T. 0.006 min

Lab File: VN078016.D




Acq: 01 Jun 2023 17:38


Tgt Ion: 91 Resp: 11091

Ion Ratio Lower Upper

91 100

120 21.1 11.5 34.4

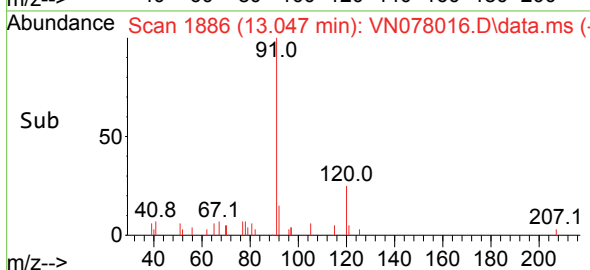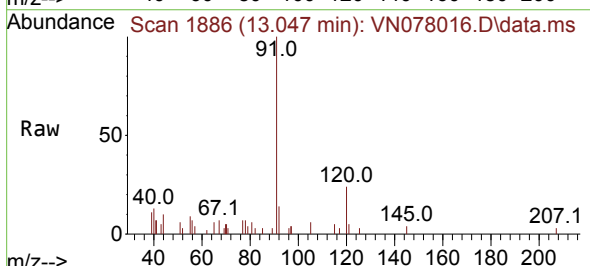

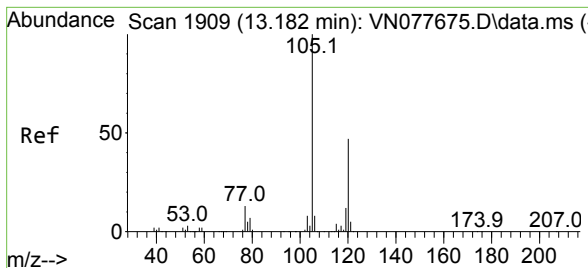

#80

1,3,5-Trimethylbenzene

Concen: 0.556 ug/l

RT: 13.182 min Scan# 1909

Delta R.T. 0.000 min

Lab File: VN078016.D

Acq: 01 Jun 2023 17:38

Instrument :

MSVOA_N

ClientSampleId :





ORA-0588DL

Tgt Ion:105 Resp: 9598

Ion Ratio Lower Upper

105 100

120 51.4 24.1 72.3

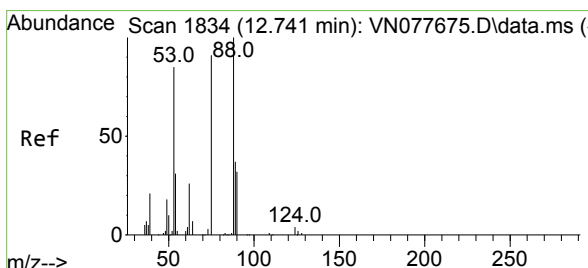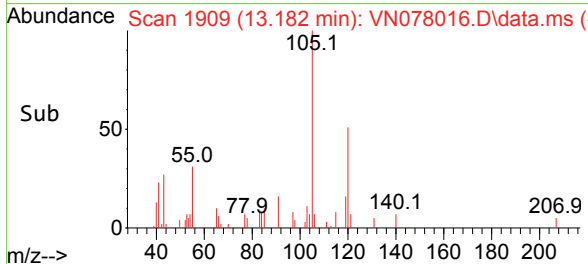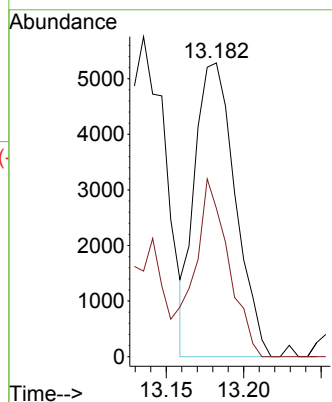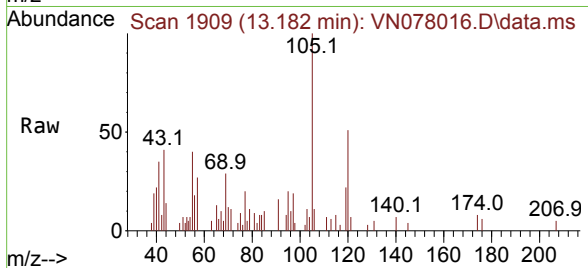

#81

trans-1,4-Dichloro-2-butene

Concen: 93.366 ug/l

RT: 12.859 min Scan# 1854

Delta R.T. 0.118 min

Lab File: VN078016.D

Acq: 01 Jun 2023 17:38




Tgt Ion: 75 Resp: 174198


Ion Ratio Lower Upper

75 100

53 0.0 67.4 101.2#

89 0.2 38.8 58.2#

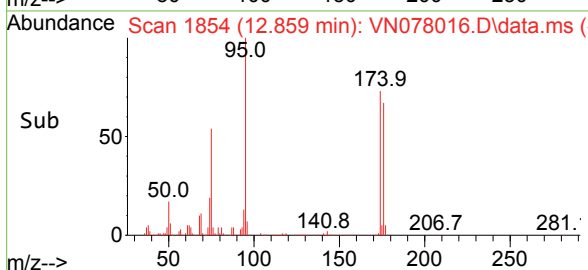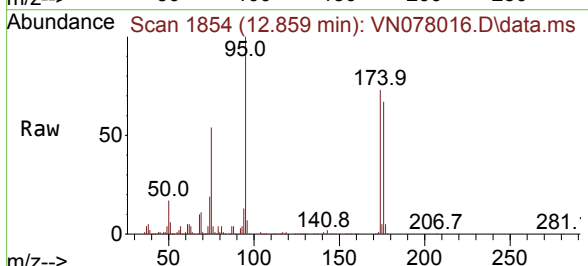



#83

tert-Butylbenzene

Concen: 0.350 ug/l

RT: 13.482 min Scan# 1954

Delta R.T. 0.035 min

Lab File: VN078016.D

Acq: 01 Jun 2023 17:38

Instrument :

MSVOA_N

ClientSampleId :

ORA-0588DL





Tgt Ion:119 Resp: 5265

Ion Ratio Lower Upper

119 100

91 95.6 33.9 101.7

134 0.0 13.2 39.6#

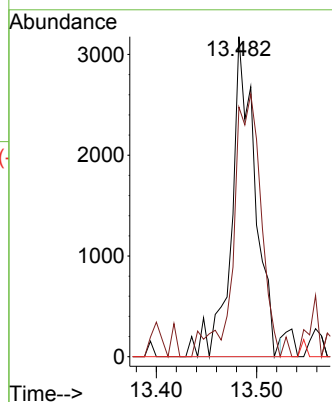

#84

1,2,4-Trimethylbenzene

Concen: 1.898 ug/l

RT: 13.488 min Scan# 1961

Delta R.T. 0.000 min

Lab File: VN078016.D




Acq: 01 Jun 2023 17:38


Tgt Ion:105 Resp: 32202

Ion Ratio Lower Upper

105 100

120 44.9 22.0 66.0

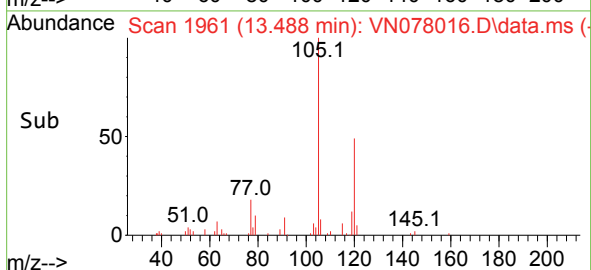



#85

sec-Butylbenzene

Concen: 0.226 ug/l

RT: 13.623 min Scan# 1984

Delta R.T. 0.000 min

Lab File: VN078016.D

Acq: 01 Jun 2023 17:38

Instrument :

MSVOA_N

ClientSampleId :





ORA-0588DL

Tgt Ion:105 Resp: 4832

Ion Ratio Lower Upper

105 100

134 17.2 9.8 29.3

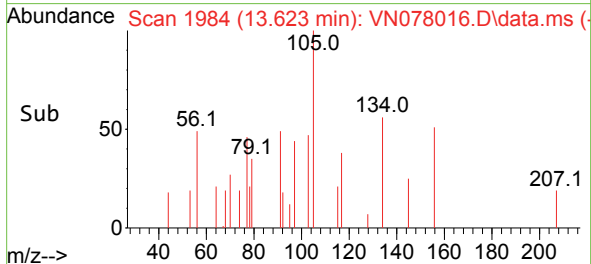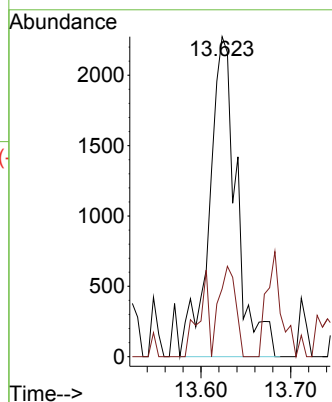

#86

p-Isopropyltoluene

Concen: 0.269 ug/l

RT: 13.682 min Scan# 1994

Delta R.T. -0.053 min

Lab File: VN078016.D

Acq: 01 Jun 2023 17:38




Tgt Ion:119 Resp: 4591


Ion Ratio Lower Upper

119 100

134 19.5 12.6 37.8

91 33.0 12.4 37.2


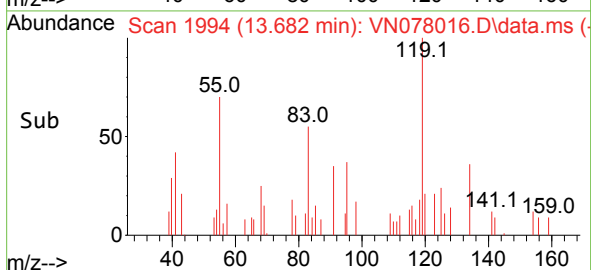






#89
n-Butylbenzene
Concen: 0.267 ug/l
RT: 14.065 min Scan# 2059
Delta R.T. 0.001 min
Lab File: VN078016.D
Acq: 01 Jun 2023 17:38




Instrument :
MSVOA_N
ClientSampleId :
ORA-0588DL


Tgt Ion: 91 Resp: 4194
Ion Ratio Lower Upper
91 100
92 61.0 26.4 79.0
134 0.0 12.6 37.6#

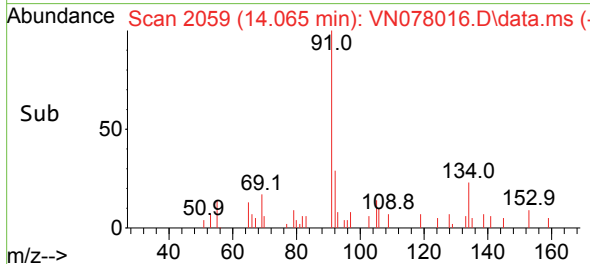

#90
Hexachloroethane
Concen: 0.526 ug/l
RT: 14.341 min Scan# 2106
Delta R.T. 0.000 min
Lab File: VN078016.D
Acq: 01 Jun 2023 17:38


Tgt Ion: 117 Resp: 1474
Ion Ratio Lower Upper
117 100
201 0.0 29.3 88.0#

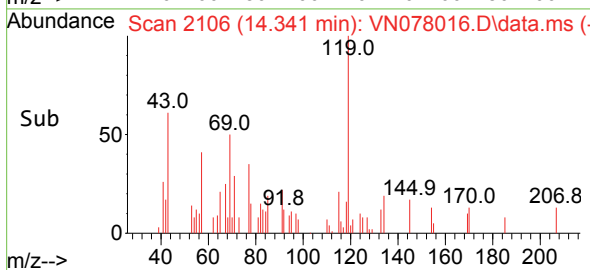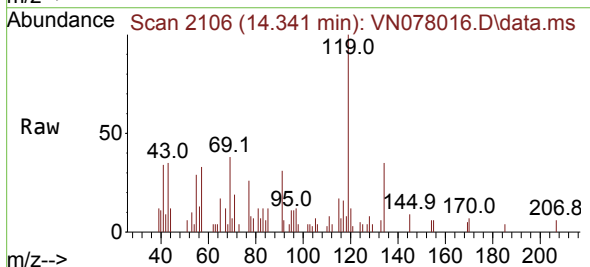

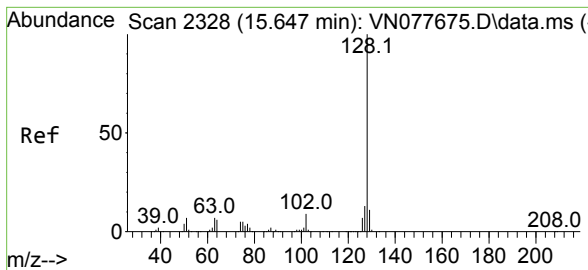

#95
Naphthalene
Concen: 0.293 ug/l
RT: 15.647 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN078016.D
Acq: 01 Jun 2023 17:38

Instrument :
MSVOA_N
ClientSampleId :
ORA-0588DL

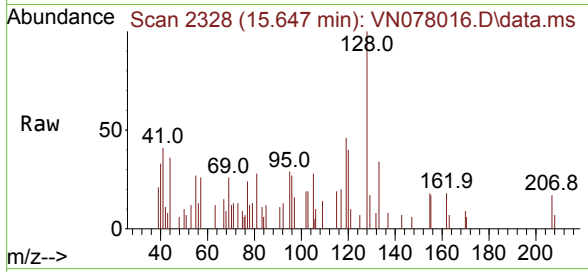

Tgt Ion:128 Resp: 4774
Ion Ratio Lower Upper
128 100
127 3.1 10.0 15.0#
129 27.3 8.7 13.1#

