

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060223\
 Data File : VN078030.D
 Acq On : 02 Jun 2023 14:33
 Operator : JC\MD
 Sample : 03001-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TP16-0A

Quant Time: Jun 05 01:12:13 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
 Quant Title : SW846 8260
 QLast Update : Tue May 16 04:07:42 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	8.235	168	367810	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.112	114	690164	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	630355	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.800	152	198568	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	254741	46.288	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	92.580%
35) Dibromofluoromethane	8.177	113	217421	48.311	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.620%
50) Toluene-d8	10.576	98	858263	49.546	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	99.100%
62) 4-Bromofluorobenzene	12.859	95	288146	47.098	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	94.200%
Target Compounds						
					Qvalue	
3) Chloromethane	2.365	50	1066	Below Cal	#	42
6) Chloroethane	3.153	64	849	0.223	ug/l #	43
11) Tert butyl alcohol	5.553	59	6754	8.892	ug/l #	82
13) Acrolein	4.194	56	57	Below Cal	#	1
16) Acetone	4.453	43	72440	41.838	ug/l	96
18) Methyl Acetate	5.036	43	2697	0.371	ug/l #	42
19) Methyl tert-butyl Ether	5.818	73	6172	0.441	ug/l #	68
20) Methylene Chloride	5.288	84	27732	4.350	ug/l	99
25) 2-Butanone	7.500	43	13827	5.105	ug/l	90
29) Tetrahydrofuran	7.865	42	1036	0.584	ug/l	92
31) Cyclohexane	8.229	56	10451	1.397	ug/l #	52
36) 1,1-Dichloropropene	8.235	75	32131	4.881	ug/l #	48
37) Ethyl Acetate	7.571	43	58512	9.973	ug/l	97
38) Carbon Tetrachloride	8.229	117	42033	6.324	ug/l #	15
39) Methylcyclohexane	9.612	83	1815	0.225	ug/l #	85
40) Benzene	8.612	78	253892	13.070	ug/l	98
43) Isopropyl Acetate	8.700	43	479779	50.063	ug/l #	67
48) Methyl methacrylate	9.671	41	6980	1.536	ug/l #	31
49) 1,4-Dioxane	9.741	88	198	2.307	ug/l #	1
51) 4-Methyl-2-Pentanone	10.459	43	17411	3.056	ug/l #	69
54) cis-1,3-Dichloropropene	10.365	75	97119	12.260	ug/l #	67
57) 1,3-Dichloropropane	11.212	76	9963	1.210	ug/l #	42
59) 2-Hexanone	11.176	43	237566	56.382	ug/l #	19
67) Ethyl Benzene	11.970	91	23867	0.975	ug/l	100
68) m/p-Xylenes	12.076	106	2433	0.262	ug/l	80
71) Bromoform	12.847	173	1692	0.538	ug/l #	1
73) Isopropylbenzene	12.706	105	17281	1.010	ug/l	98
76) 1,2,3-Trichloropropane	12.859	75	154039	30.976	ug/l #	1
78) n-propylbenzene	13.041	91	15425	0.764	ug/l	96
79) 2-Chlorotoluene	13.041	91	15425	1.281	ug/l #	42
81) trans-1,4-Dichloro-2-b...	12.859	75	154039	99.015	ug/l #	15


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060223\
Data File : VN078030.D
Acq On : 02 Jun 2023 14:33
Operator : JC\MD
Sample : 03001-02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TP16-0A

Quant Time: Jun 05 01:12:13 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
Quant Title : SW846 8260
QLast Update : Tue May 16 04:07:42 2023
Response via : Initial Calibration

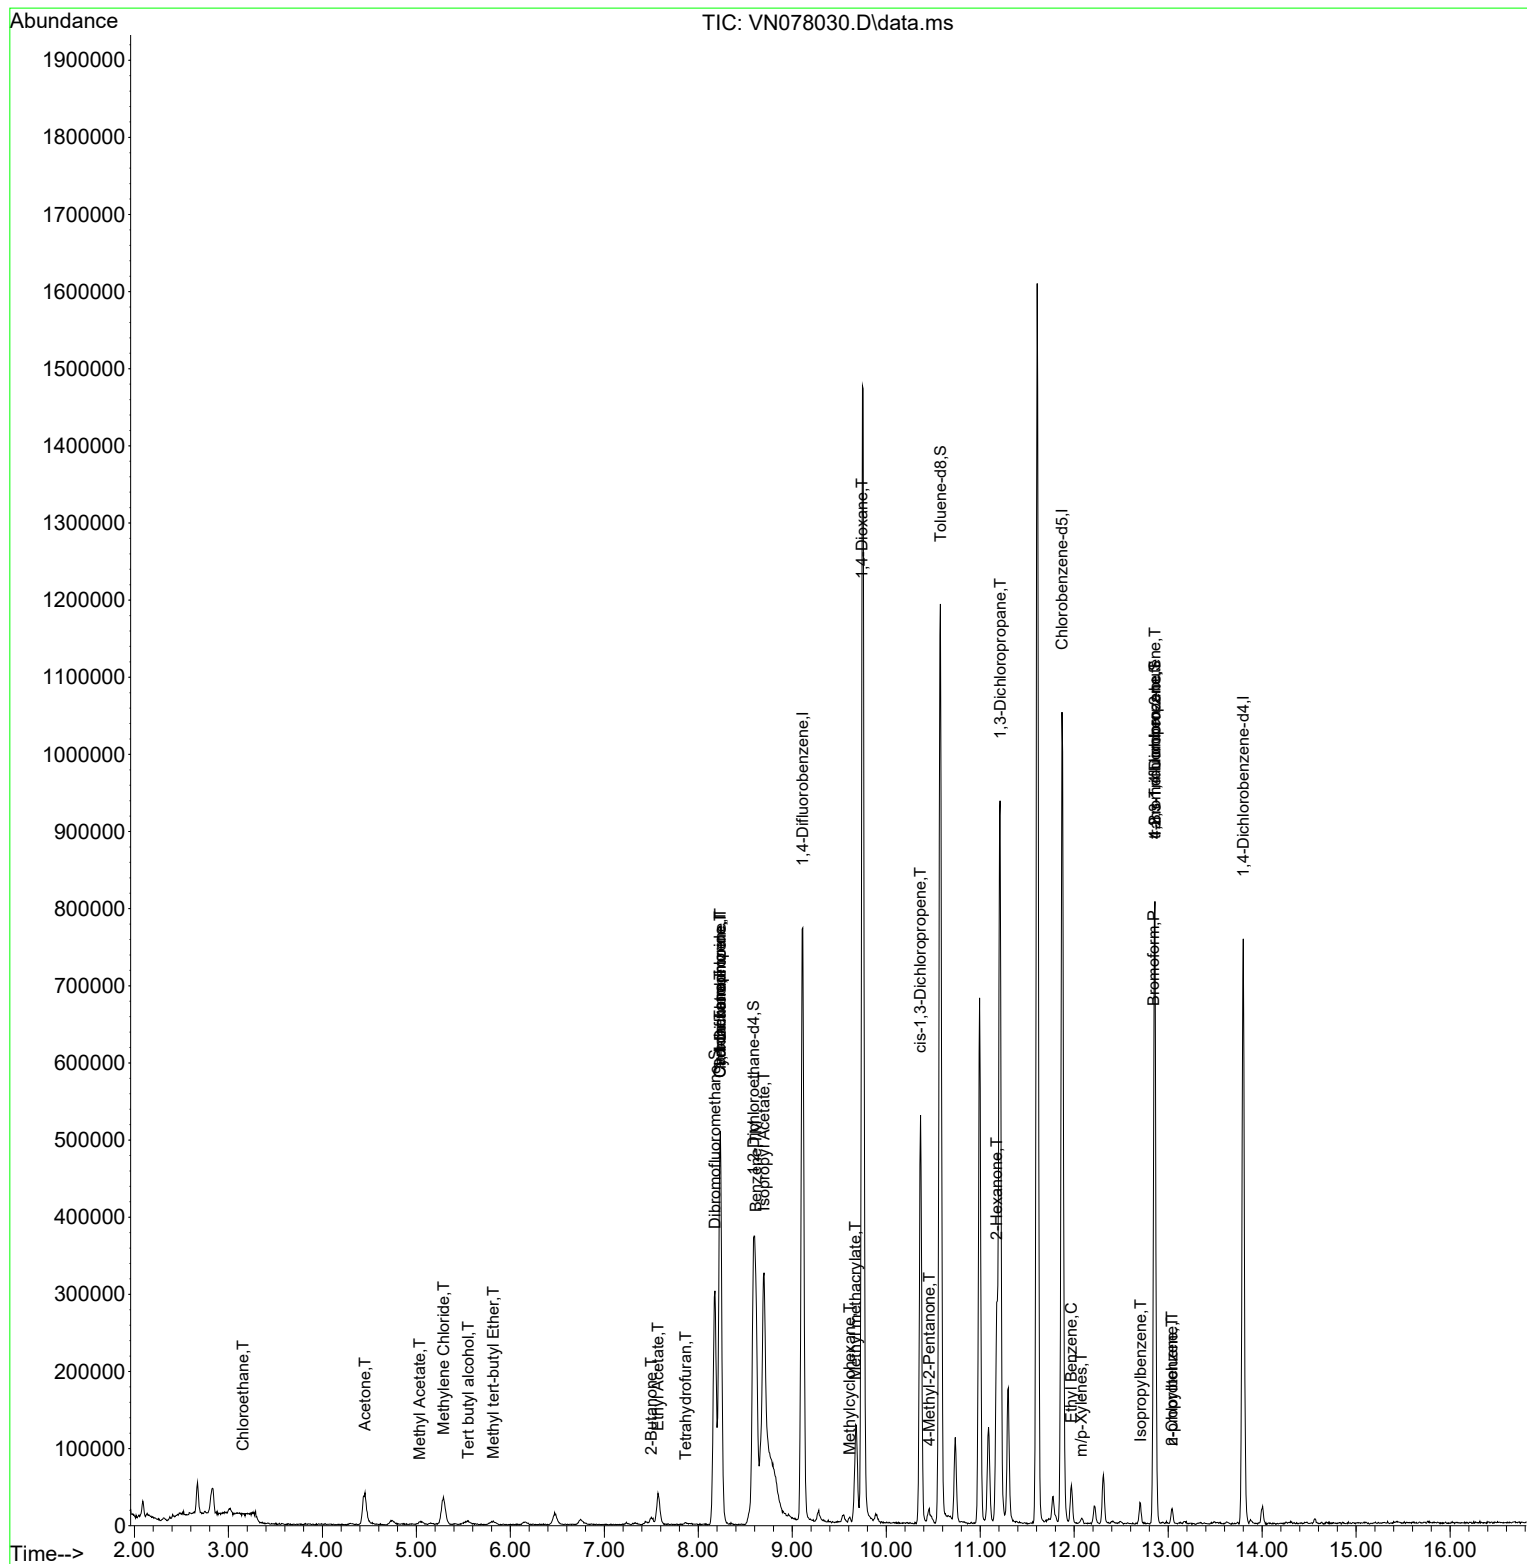

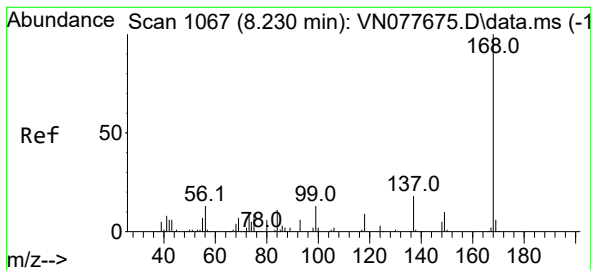

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.235 min Scan# 10

Delta R.T. 0.005 min

Lab File: VN078030.D

Acq: 02 Jun 2023 14:33

Instrument :

MSVOA_N

ClientSampleId :





TP16-0A

Tgt Ion:168 Resp: 367810

Ion Ratio Lower Upper

168 100

99 61.4 53.0 79.6

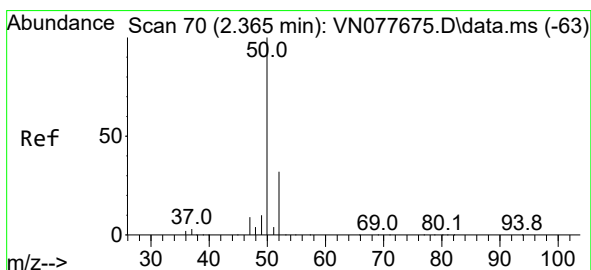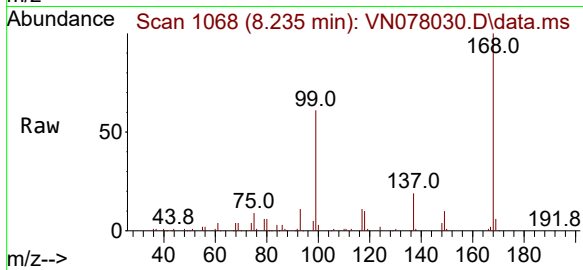

#3

Chloromethane

Concen: Below Cal

RT: 2.365 min Scan# 70

Delta R.T. 0.000 min

Lab File: VN078030.D




Acq: 02 Jun 2023 14:33


Tgt Ion: 50 Resp: 1066

Ion Ratio Lower Upper

50 100

52 0.0 26.5 39.7#


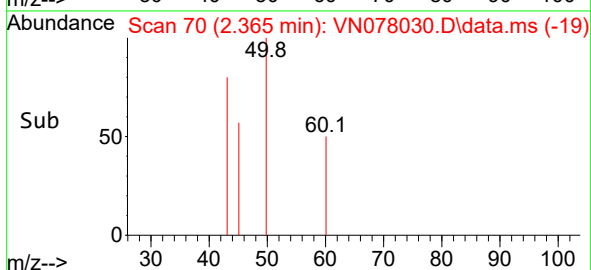

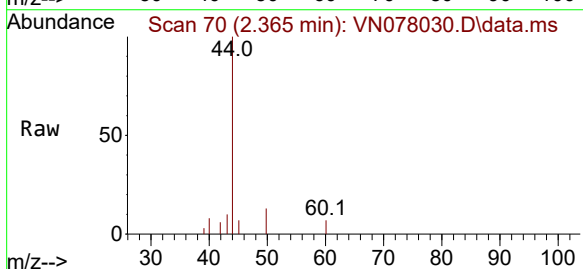


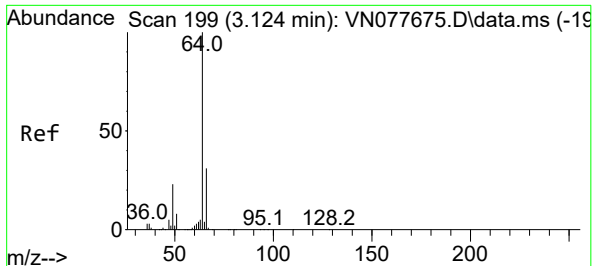

#6
Chloroethane
Concen: 0.223 ug/l
RT: 3.153 min Scan# 204
Delta R.T. 0.029 min
Lab File: VN078030.D
Acq: 02 Jun 2023 14:33




Instrument :
MSVOA_N
ClientSampleId :
TP16-0A


Tgt Ion: 64 Resp: 849
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.2#

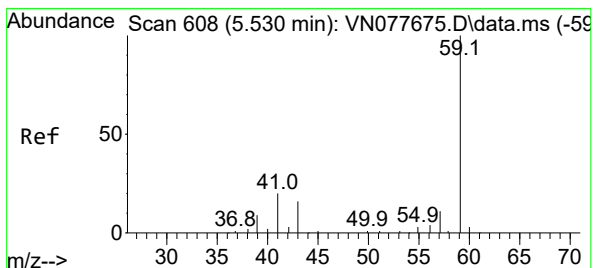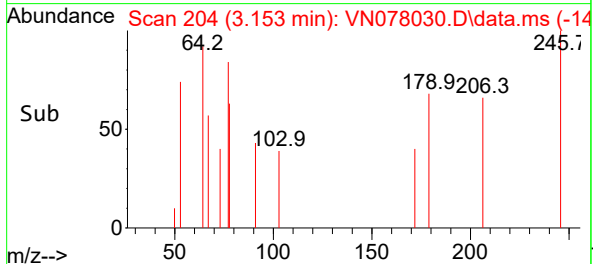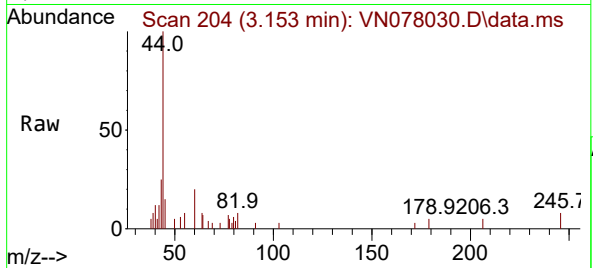

#11
Tert butyl alcohol
Concen: 8.892 ug/l
RT: 5.553 min Scan# 612
Delta R.T. 0.023 min
Lab File: VN078030.D
Acq: 02 Jun 2023 14:33

Tgt Ion: 59 Resp: 6754
Ion Ratio Lower Upper
59 100
57 3.5 8.2 12.4#


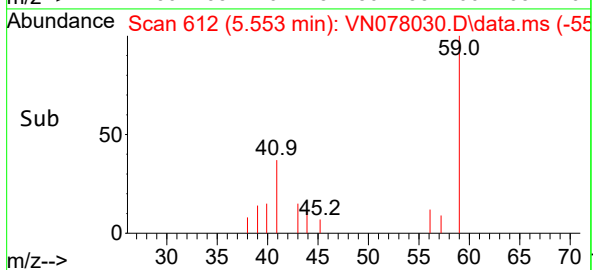

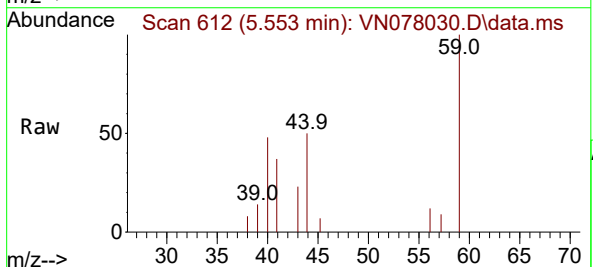




#13
Acrolein
Concen: Below Cal
RT: 4.194 min Scan# 380
Delta R.T. 0.005 min
Lab File: VN078030.D
Acq: 02 Jun 2023 14:33




Instrument :
MSVOA_N
ClientSampleId :
TP16-0A


Tgt Ion: 56 Resp: 57
Ion Ratio Lower Upper
56 100
55 443.9 54.5 81.7#



#16
Acetone
Concen: 41.838 ug/l
RT: 4.453 min Scan# 425
Delta R.T. 0.023 min
Lab File: VN078030.D
Acq: 02 Jun 2023 14:33

Tgt Ion: 43 Resp: 72440
Ion Ratio Lower Upper
43 100
58 32.4 28.0 42.0





#18

Methyl Acetate

Concen: 0.371 ug/l

RT: 5.036 min Scan# 51

Delta R.T. -0.000 min

Lab File: VN078030.D

Acq: 02 Jun 2023 14:33

Instrument :

MSVOA_N

ClientSampleId :





TP16-0A

Tgt Ion: 43 Resp: 2697

Ion Ratio Lower Upper

43 100

74 0.0 26.2 39.4#

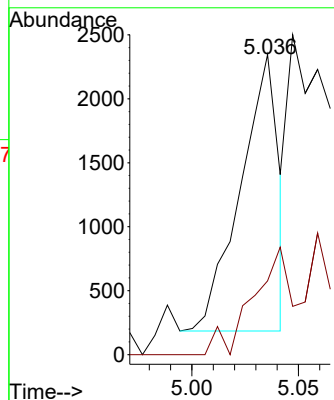

#19

Methyl tert-butyl Ether

Concen: 0.441 ug/l

RT: 5.818 min Scan# 657

Delta R.T. 0.018 min

Lab File: VN078030.D




Acq: 02 Jun 2023 14:33


Tgt Ion: 73 Resp: 6172

Ion Ratio Lower Upper

73 100

57 33.9 15.6 23.4#



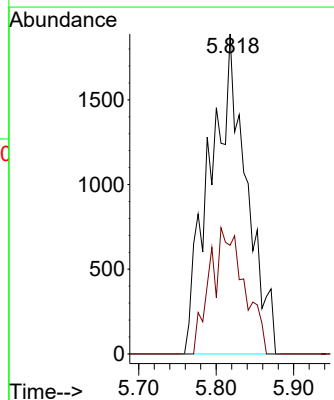
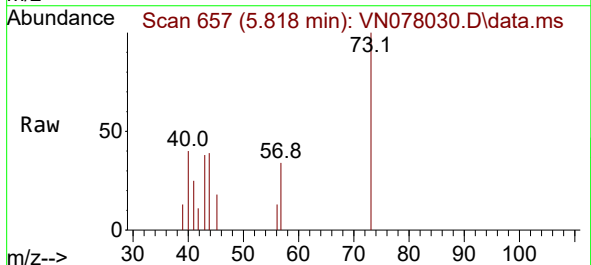




#20
Methylene Chloride
Concen: 4.350 ug/l
RT: 5.288 min Scan# 501
Delta R.T. 0.005 min
Lab File: VN078030.D
Acq: 02 Jun 2023 14:33




Instrument :
MSVOA_N
ClientSampleId :
TP16-0A


Tgt Ion:	84	Resp:	27732
Ion	Ratio	Lower	Upper
84	100		
49	99.4	79.7	119.5
51	32.8	25.2	37.8
86	67.7	53.3	79.9

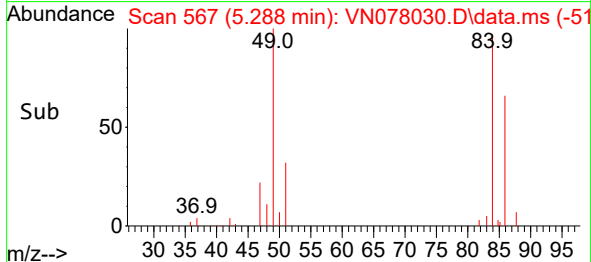

#25
2-Butanone
Concen: 5.105 ug/l
RT: 7.500 min Scan# 943
Delta R.T. 0.012 min
Lab File: VN078030.D
Acq: 02 Jun 2023 14:33

Tgt Ion:	43	Resp:	13827
Ion	Ratio	Lower	Upper
43	100		
72	31.6	30.2	45.2

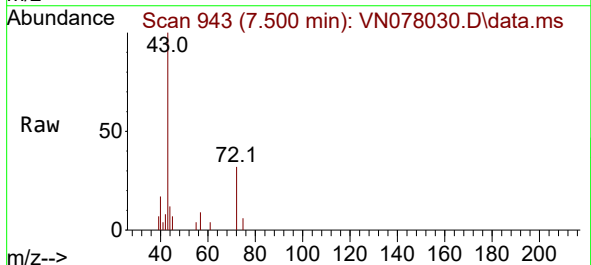



#29

Tetrahydrofuran

Concen: 0.584 ug/l

RT: 7.865 min Scan# 1005

Delta R.T. 0.024 min

Lab File: VN078030.D

Acq: 02 Jun 2023 14:33

Instrument :

MSVOA_N

ClientSampleId :

TP16-0A





Tgt Ion: 42 Resp: 1036

Ion Ratio Lower Upper

42 100

72 58.1 49.8 74.6

71 51.8 47.4 71.2

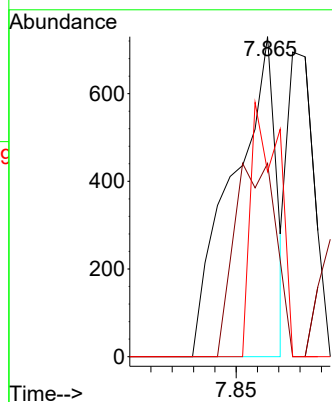

#31

Cyclohexane

Concen: 1.397 ug/l

RT: 8.229 min Scan# 1067

Delta R.T. -0.036 min

Lab File: VN078030.D

Acq: 02 Jun 2023 14:33




Tgt Ion: 56 Resp: 10451


Ion Ratio Lower Upper

56 100

69 137.7 26.8 40.2#

84 106.5 81.8 122.6

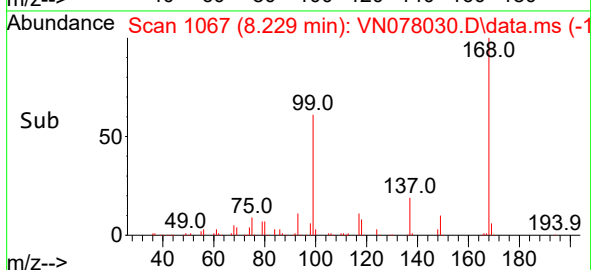



#33

1,2-Dichloroethane-d4

Concen: 46.288 ug/l

RT: 8.588 min Scan# 1128

Delta R.T. 0.006 min

Lab File: VN078030.D

Acq: 02 Jun 2023 14:33

Instrument :

MSVOA_N

ClientSampleId :





TP16-0A

Tgt Ion: 65 Resp: 254741

Ion Ratio Lower Upper

65 100

67 52.0 0.0 106.6



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.112 min Scan# 1217

Delta R.T. 0.006 min

Lab File: VN078030.D

Acq: 02 Jun 2023 14:33




Tgt Ion: 114 Resp: 690164


Ion Ratio Lower Upper

114 100

63 19.8 0.0 36.4

88 14.4 0.0 30.6


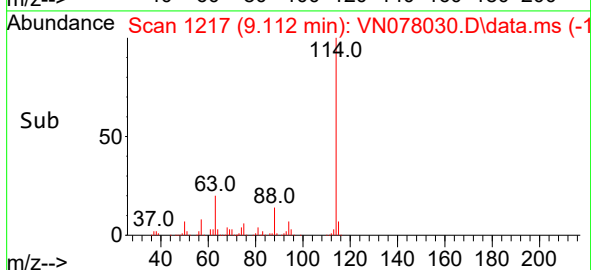






#35
Dibromofluoromethane
Concen: 48.311 ug/l
RT: 8.177 min Scan# 1057
Delta R.T. 0.006 min
Lab File: VN078030.D
Acq: 02 Jun 2023 14:33




Instrument :
MSVOA_N
ClientSampleId :
TP16-0A


Tgt Ion:113 Resp: 217421
Ion Ratio Lower Upper
113 100
111 104.7 82.6 123.8
192 17.1 12.7 19.1

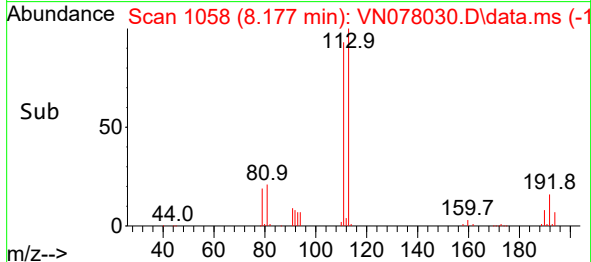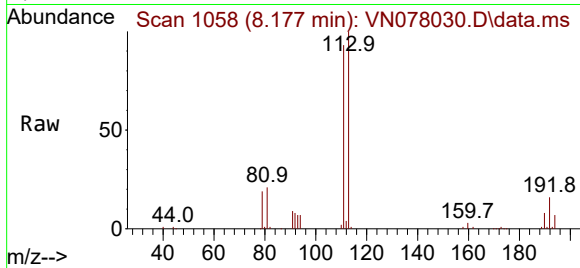

#36
1,1-Dichloropropene
Concen: 4.881 ug/l
RT: 8.235 min Scan# 1068
Delta R.T. -0.142 min
Lab File: VN078030.D
Acq: 02 Jun 2023 14:33

Tgt Ion: 75 Resp: 32131
Ion Ratio Lower Upper
75 100
110 8.9 19.1 57.3#
77 0.0 25.0 37.4#

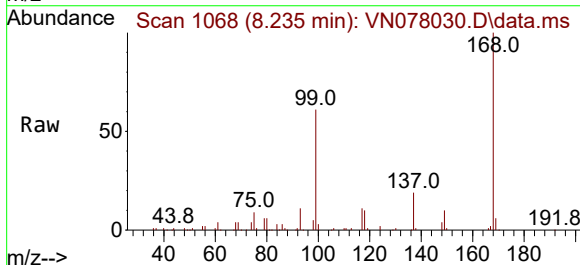



#37

Ethyl Acetate

Concen: 9.973 ug/l

RT: 7.571 min Scan# 91

Delta R.T. 0.006 min

Lab File: VN078030.D

Acq: 02 Jun 2023 14:33





Instrument :

MSVOA_N

ClientSampleId :

TP16-0A

Tgt Ion:	43	Resp:	58512
Ion	Ratio	Lower	Upper
43	100		
61	16.4	13.2	19.8
70	11.6	11.3	16.9



#38

Carbon Tetrachloride

Concen: 6.324 ug/l




RT: 8.229 min Scan# 1067


Delta R.T. -0.142 min

Lab File: VN078030.D

Acq: 02 Jun 2023 14:33

Tgt Ion:	117	Resp:	42033
Ion	Ratio	Lower	Upper
117	100		
119	4.4	77.3	115.9#
121	0.0	23.3	34.9#

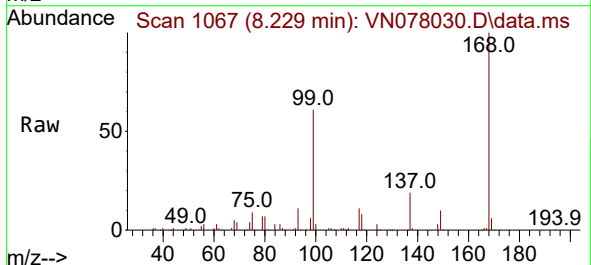



#39

Methylcyclohexane

Concen: 0.225 ug/l

RT: 9.612 min Scan# 1130

Delta R.T. 0.006 min

Lab File: VN078030.D

Acq: 02 Jun 2023 14:33

Instrument :

MSVOA_N

ClientSampleId :

TP16-0A





Tgt Ion: 83 Resp: 1815

Ion Ratio Lower Upper

83 100

55 79.7 49.1 73.7#

98 48.0 40.6 61.0

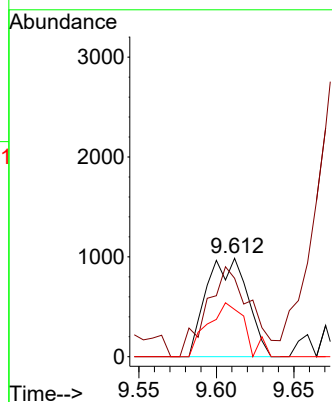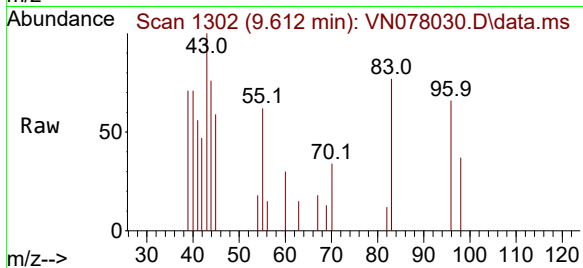

#40

Benzene

Concen: 13.070 ug/l

RT: 8.612 min Scan# 1132

Delta R.T. -0.000 min

Lab File: VN078030.D




Acq: 02 Jun 2023 14:33


Tgt Ion: 78 Resp: 253892

Ion Ratio Lower Upper

78 100

77 22.7 19.0 28.6




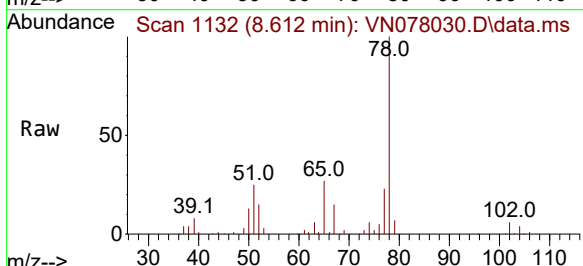




#43
Isopropyl Acetate
Concen: 50.063 ug/l
RT: 8.700 min Scan# 1146
Delta R.T. 0.006 min
Lab File: VN078030.D
Acq: 02 Jun 2023 14:33




Instrument :
MSVOA_N
ClientSampleId :
TP16-0A


Tgt Ion: 43 Resp: 479779
Ion Ratio Lower Upper
43 100
61 10.2 24.7 37.1#
87 7.6 14.6 21.8#

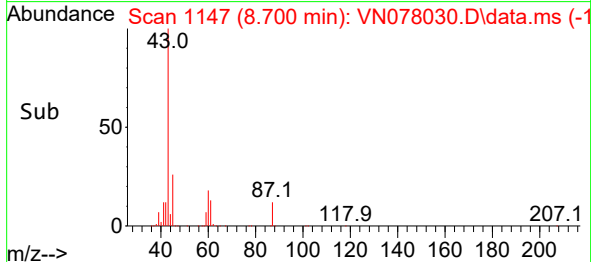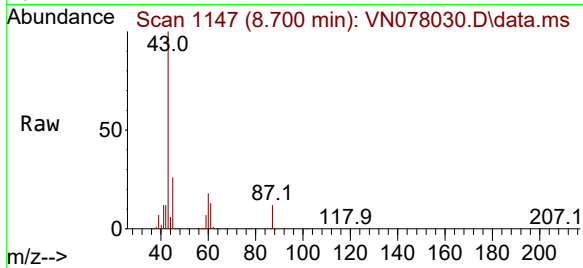

#48
Methyl methacrylate
Concen: 1.536 ug/l
RT: 9.671 min Scan# 1312
Delta R.T. -0.017 min
Lab File: VN078030.D
Acq: 02 Jun 2023 14:33

Tgt Ion: 41 Resp: 6980
Ion Ratio Lower Upper
41 100
69 0.0 90.4 135.6#
39 76.3 54.6 81.8




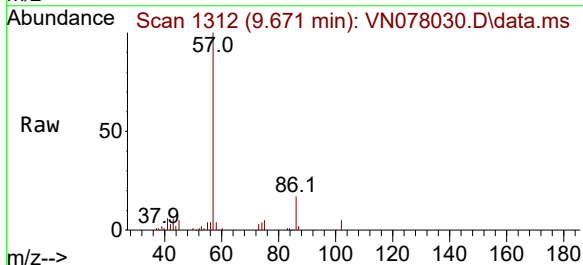




#49
1,4-Dioxane
Concen: 2.307 ug/l
RT: 9.741 min Scan# 1316
Delta R.T. 0.047 min
Lab File: VN078030.D
Acq: 02 Jun 2023 14:33




Instrument :
MSVOA_N
ClientSampleId :
TP16-0A


Tgt Ion: 88 Resp: 198
Ion Ratio Lower Upper
88 100
43 713931.8 17.0 25.6#
58 3704.0 47.0 70.4#

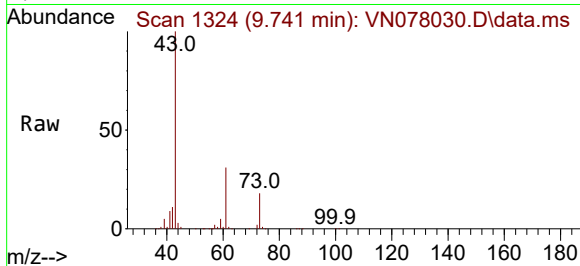

#50
Toluene-d8
Concen: 49.546 ug/l
RT: 10.576 min Scan# 1466
Delta R.T. 0.005 min
Lab File: VN078030.D
Acq: 02 Jun 2023 14:33

Tgt Ion: 98 Resp: 858263
Ion Ratio Lower Upper
98 100
100 63.2 52.0 78.0




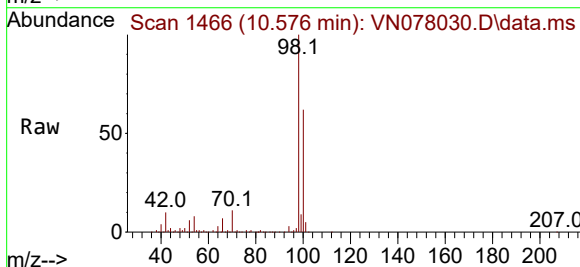




#51
4-Methyl-2-Pentanone
Concen: 3.056 ug/l
RT: 10.459 min Scan# 1446
Delta R.T. 0.012 min
Lab File: VN078030.D
Acq: 02 Jun 2023 14:33




Instrument :
MSVOA_N
ClientSampleId :
TP16-0A


Tgt Ion: 43 Resp: 17411
Ion Ratio Lower Upper
43 100
58 25.5 36.6 54.8#

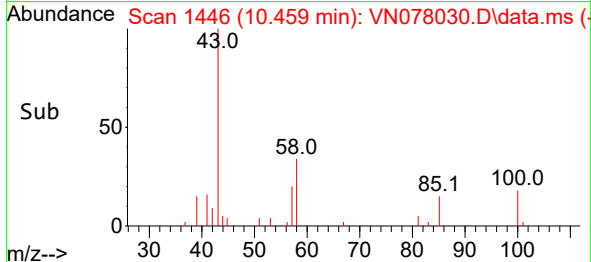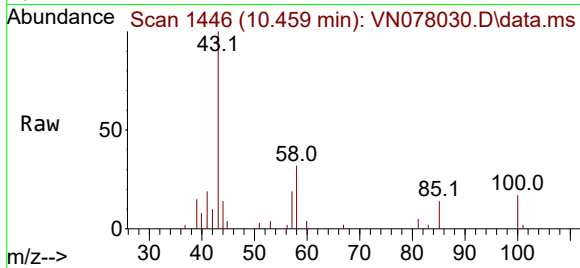

#54
cis-1,3-Dichloropropene
Concen: 12.260 ug/l
RT: 10.365 min Scan# 1430
Delta R.T. 0.047 min
Lab File: VN078030.D
Acq: 02 Jun 2023 14:33

Tgt Ion: 75 Resp: 97119
Ion Ratio Lower Upper
75 100
77 0.6 26.1 39.1#
39 31.7 31.6 47.4




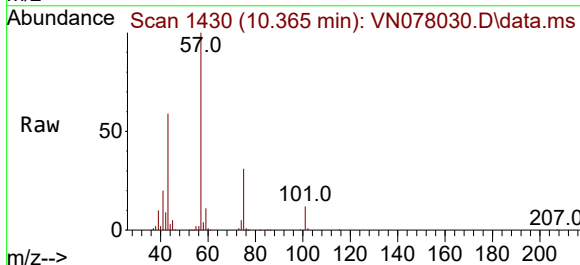




#57
1,3-Dichloropropane
Concen: 1.210 ug/l
RT: 11.212 min Scan# 1574
Delta R.T. 0.041 min
Lab File: VN078030.D
Acq: 02 Jun 2023 14:33




Instrument :
MSVOA_N
ClientSampleId :
TP16-0A


Tgt Ion: 76 Resp: 9963
Ion Ratio Lower Upper
76 100
78 0.0 26.1 39.1#

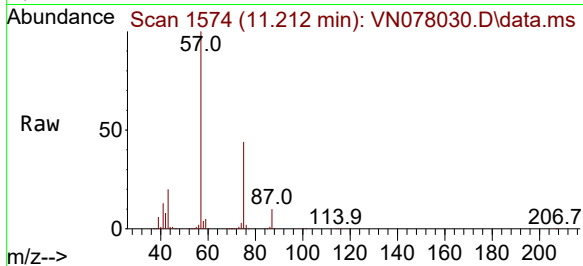

#59
2-Hexanone
Concen: 56.382 ug/l
RT: 11.176 min Scan# 1568
Delta R.T. -0.024 min
Lab File: VN078030.D
Acq: 02 Jun 2023 14:33

Tgt Ion: 43 Resp: 237566
Ion Ratio Lower Upper
43 100
58 0.0 31.7 95.1#




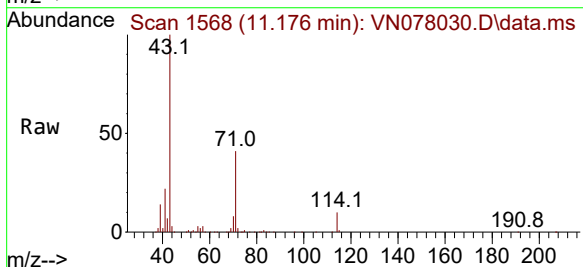




#62
4-Bromofluorobenzene
Concen: 47.098 ug/l
RT: 12.859 min Scan# 1854
Delta R.T. 0.006 min
Lab File: VN078030.D
Acq: 02 Jun 2023 14:33




Instrument :
MSVOA_N
ClientSampleId :
TP16-0A


Tgt Ion: 95 Resp: 288146
Ion Ratio Lower Upper
95 100
174 74.9 0.0 143.8
176 70.3 0.0 135.8

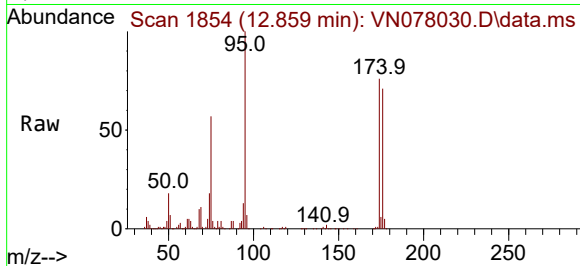

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 1686
Delta R.T. 0.000 min
Lab File: VN078030.D
Acq: 02 Jun 2023 14:33

Tgt Ion: 117 Resp: 630355
Ion Ratio Lower Upper
117 100
82 54.9 44.0 66.0
119 32.3 25.6 38.4


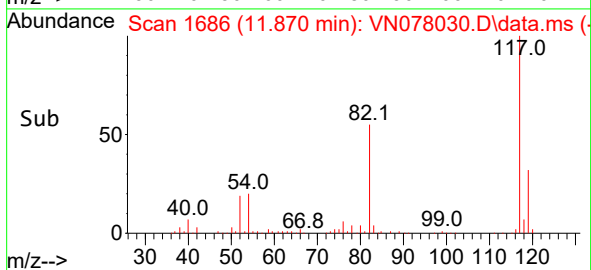

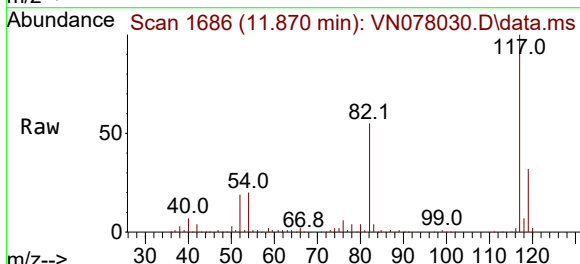


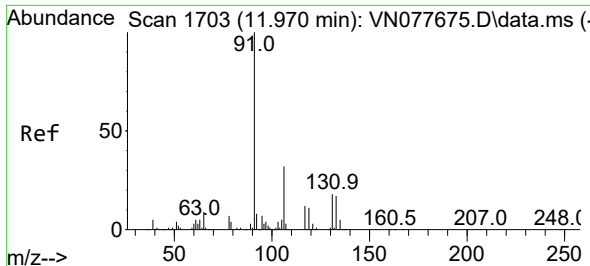

#67
Ethyl Benzene
Concen: 0.975 ug/l
RT: 11.970 min Scan# 1703
Delta R.T. 0.000 min
Lab File: VN078030.D
Acq: 02 Jun 2023 14:33




Instrument :
MSVOA_N
ClientSampleId :
TP16-0A


Tgt Ion: 91 Resp: 23867
Ion Ratio Lower Upper
91 100
106 32.2 25.6 38.4

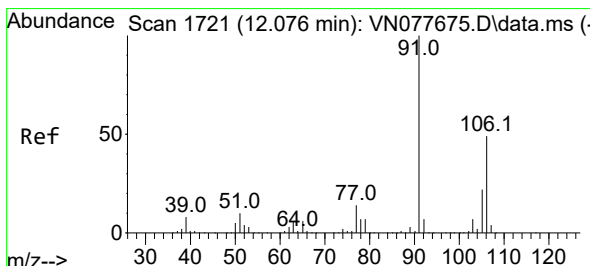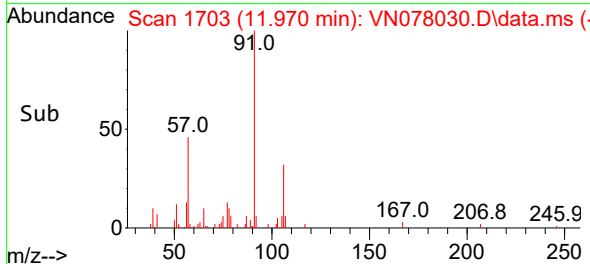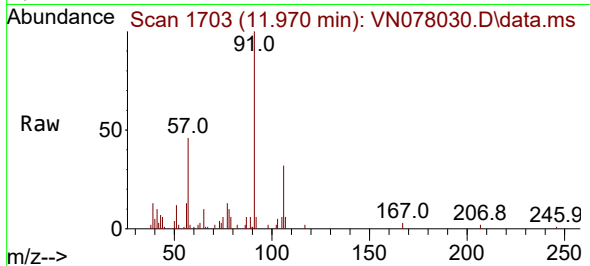

#68
m/p-Xylenes
Concen: 0.262 ug/l
RT: 12.076 min Scan# 1721
Delta R.T. 0.000 min
Lab File: VN078030.D
Acq: 02 Jun 2023 14:33

Tgt Ion: 106 Resp: 2433
Ion Ratio Lower Upper
106 100
91 230.4 159.6 239.4

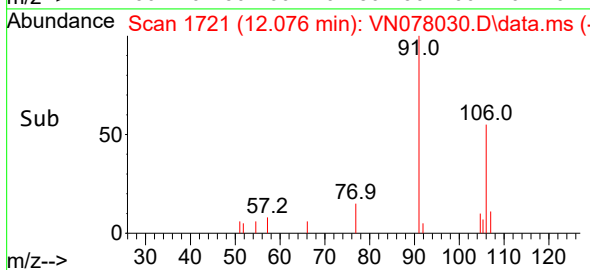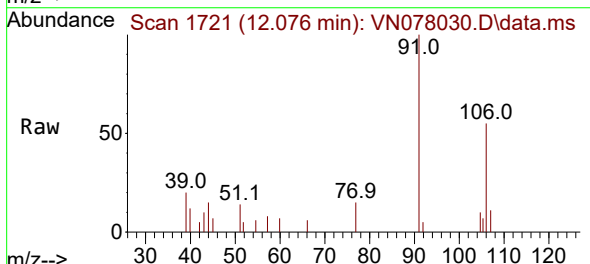



#71

Bromoform

Concen: 0.538 ug/l

RT: 12.847 min Scan# 1852

Delta R.T. 0.265 min

Lab File: VN078030.D

Acq: 02 Jun 2023 14:33

Instrument :

MSVOA_N

ClientSampleId :

TP16-0A





Tgt Ion:173 Resp: 1692

Ion Ratio Lower Upper

173 100

175 709.4 24.3 73.0#

254 0.0 0.0 0.0

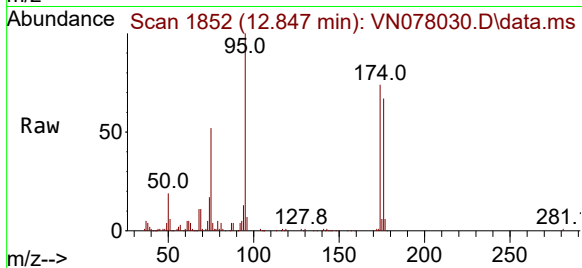

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.800 min Scan# 2014

Delta R.T. -0.000 min

Lab File: VN078030.D

Acq: 02 Jun 2023 14:33




Tgt Ion:152 Resp: 198568


Ion Ratio Lower Upper

152 100

115 64.0 32.3 96.8

150 159.3 0.0 355.8


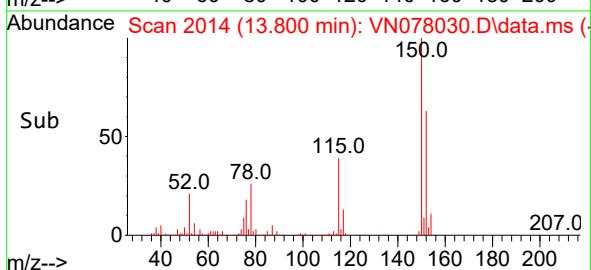

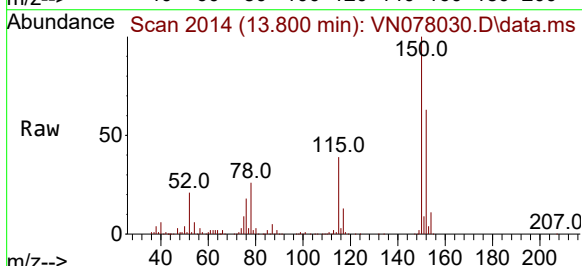


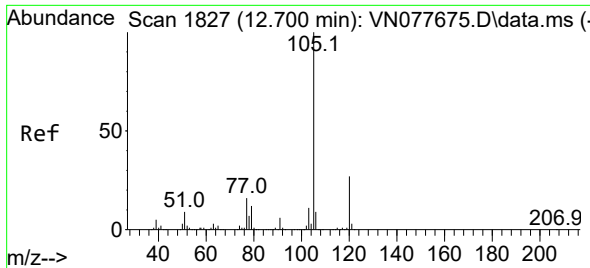

#73
Isopropylbenzene
Concen: 1.010 ug/l
RT: 12.706 min Scan# 1854
Delta R.T. 0.006 min
Lab File: VN078030.D
Acq: 02 Jun 2023 14:33




Instrument :
MSVOA_N
ClientSampleId :
TP16-0A


Tgt Ion:105 Resp: 17281
Ion Ratio Lower Upper
105 100
120 27.3 13.1 39.1

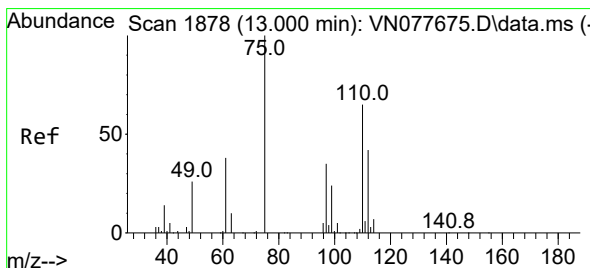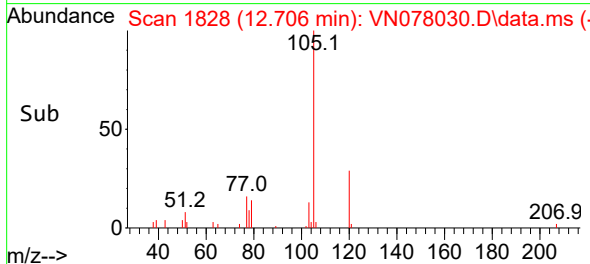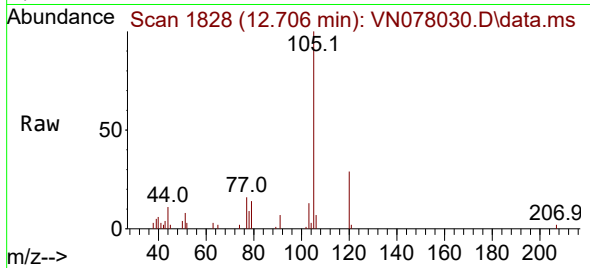

#76
1,2,3-Trichloropropane
Concen: 30.976 ug/l
RT: 12.859 min Scan# 1854
Delta R.T. -0.141 min
Lab File: VN078030.D
Acq: 02 Jun 2023 14:33

Tgt Ion: 75 Resp: 154039
Ion Ratio Lower Upper
75 100
77 1.4 84.5 253.5#


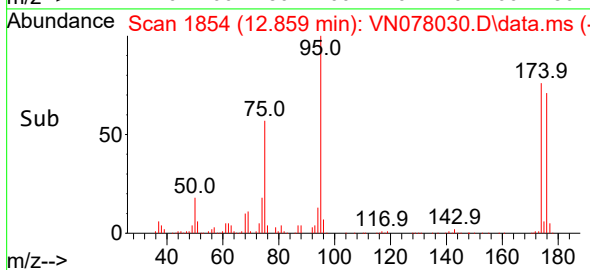

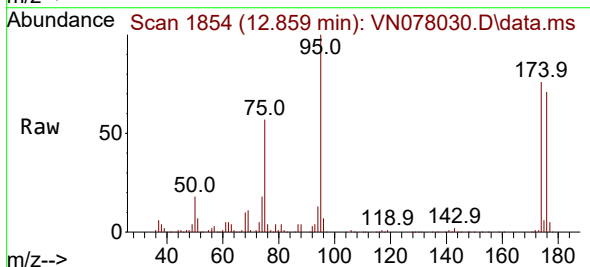




#78
n-propylbenzene
Concen: 0.764 ug/l
RT: 13.041 min Scan# 1885
Delta R.T. -0.000 min
Lab File: VN078030.D
Acq: 02 Jun 2023 14:33




Instrument :
MSVOA_N
ClientSampleId :
TP16-0A


Tgt Ion: 91 Resp: 15425
Ion Ratio Lower Upper
91 100
120 21.1 11.5 34.4

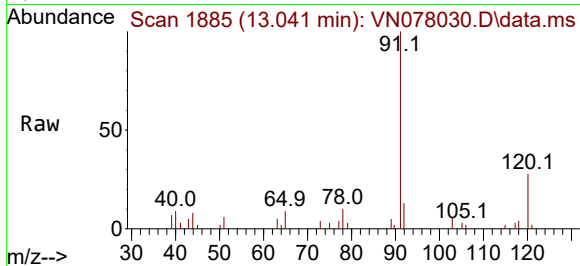

#79
2-Chlorotoluene
Concen: 1.281 ug/l
RT: 13.041 min Scan# 1885
Delta R.T. -0.088 min
Lab File: VN078030.D
Acq: 02 Jun 2023 14:33

Tgt Ion: 91 Resp: 15425
Ion Ratio Lower Upper
91 100
126 0.0 16.3 48.8#

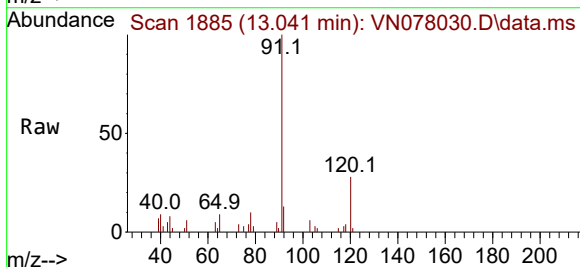



#81
 trans-1,4-Dichloro-2-butene
 Concen: 99.015 ug/l
 RT: 12.859 min Scan# 11
 Delta R.T. 0.118 min
 Lab File: VN078030.D
 Acq: 02 Jun 2023 14:33

Instrument :
 MSVOA_N
 ClientSampleId :
 TP16-0A

Tgt Ion: 75 Resp: 154039
 Ion Ratio Lower Upper
 75 100
 53 0.1 67.4 101.2#
 89 0.0 38.8 58.2#

