


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN060320\
Data File : VN061626.D
Acq On : 3 Jun 2020 9:51
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052820W.M
Title : SW846 8260
Last Update : Fri May 29 02:14:10 2020

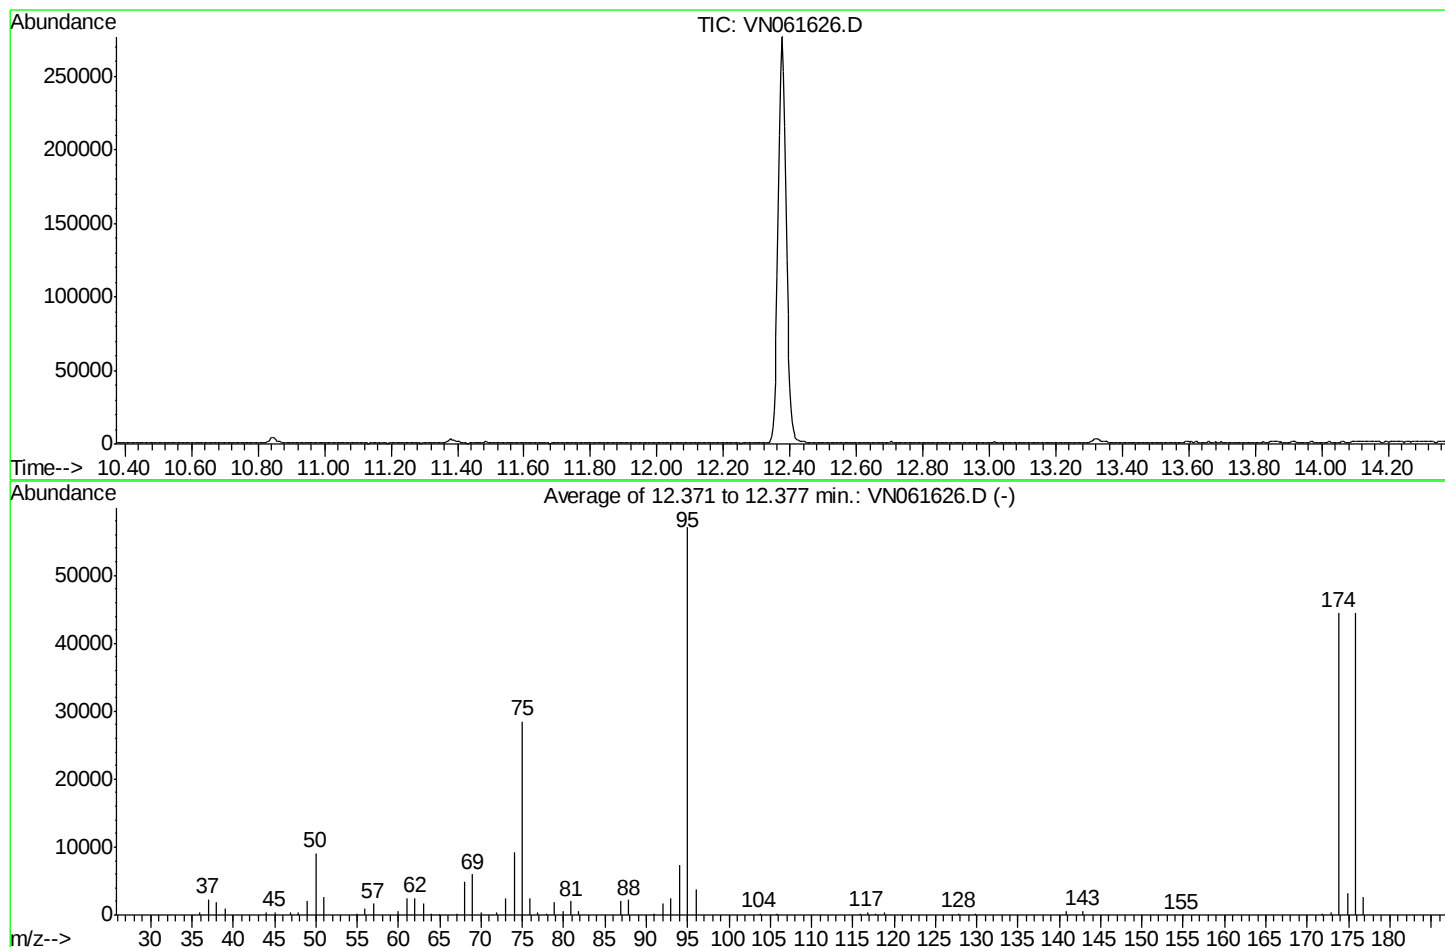

AutoFind: Scans 3296, 3297, 3298; Background Corrected with Scan 3283

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	9076	PASS
75	95	30	60	49.9	28477	PASS
95	95	100	100	100.0	57064	PASS
96	95	5	9	6.6	3790	PASS
173	174	0.00	2	0.8	341	PASS
174	95	50	100	78.1	44565	PASS
175	174	5	9	7.2	3212	PASS
176	174	95	101	99.7	44429	PASS
177	176	5	9	6.1	2697	PASS