
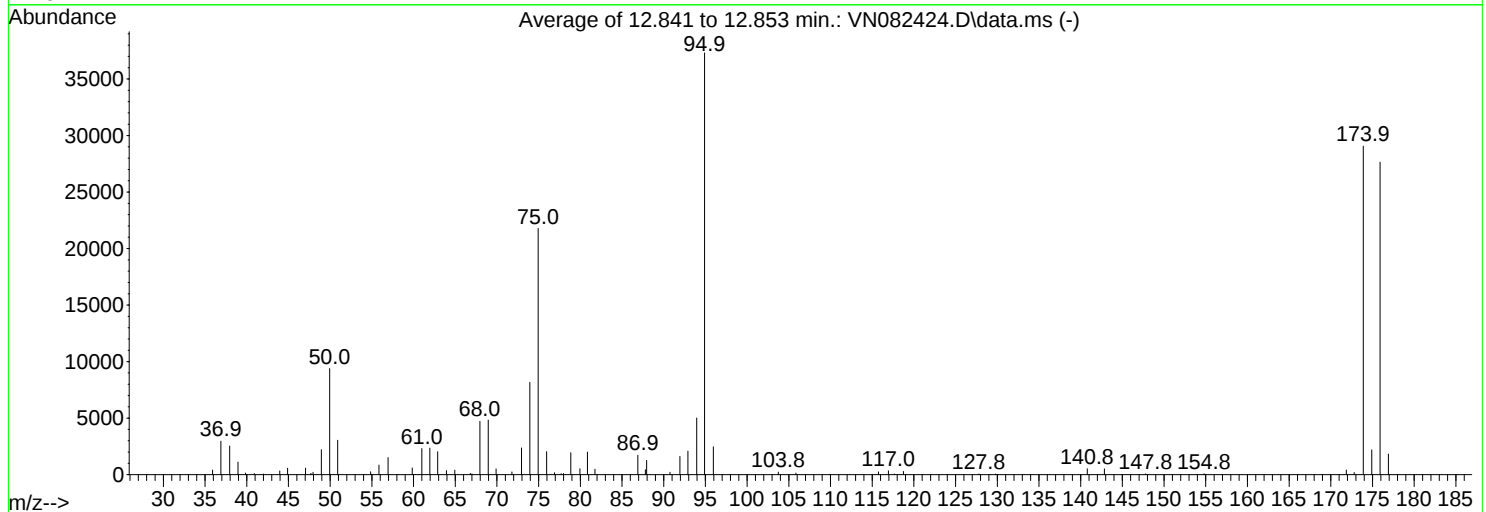


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060324\
Data File : VN082424.D
Acq On : 03 Jun 2024 09:33
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Title : SW846 8260
Last Update : Thu May 16 05:21:06 2024

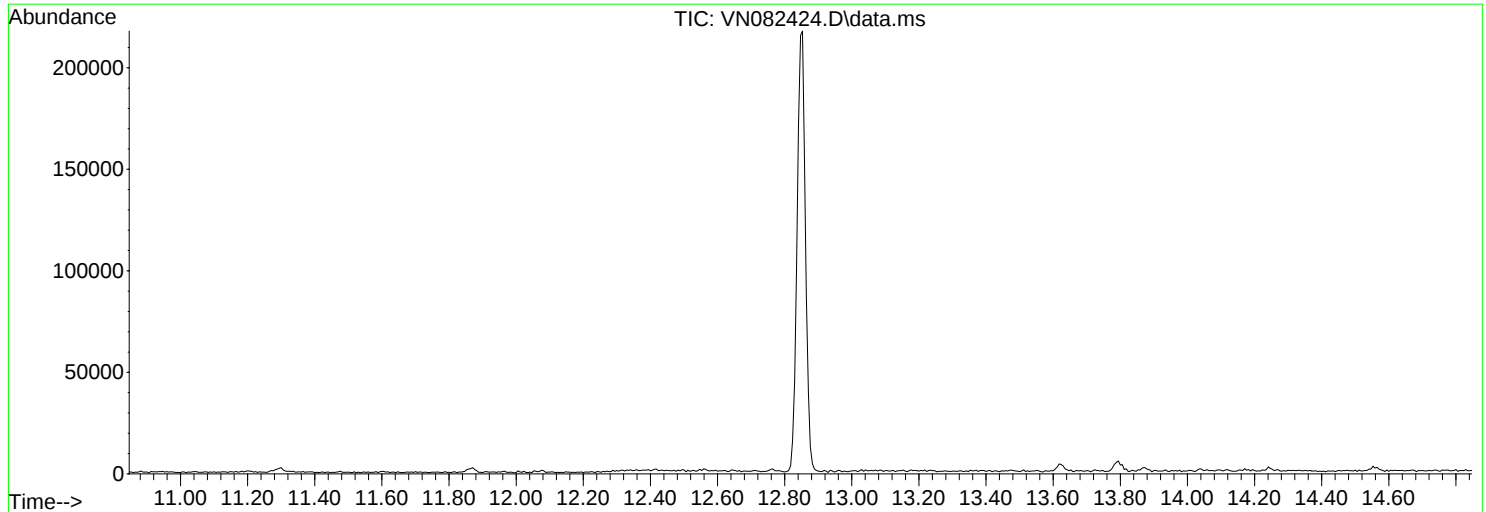

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.1	9384	PASS
75	95	30	60	58.4	21784	PASS
95	95	100	100	100.0	37317	PASS
96	95	5	9	6.6	2465	PASS
173	174	0.00	2	0.6	188	PASS
174	95	50	100	77.9	29059	PASS
175	174	5	9	7.6	2194	PASS
176	174	95	101	95.1	27640	PASS
177	176	5	9	6.6	1820	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	410	47.95	209	63.95	356	75.95	203
36.90	2953	48.95	2212	64.95	403	76.90	16
37.95	2538	49.95	9384	66.80	110	77.70	9
38.95	1103	50.90	3042	67.00	62	78.00	9
39.85	146	54.85	261	67.95	4715	78.85	1935
40.90	104	55.85	850	68.95	4822	79.95	524
42.00	60	56.95	1512	69.90	514	80.85	1996
43.95	329	59.85	594	71.80	241	81.75	476
44.90	565	61.00	2312	72.95	2362	86.90	1718
47.05	584	61.95	2351	73.95	8165	87.80	437
47.70	119	62.90	2030	74.95	21784	87.95	1256

Average of 12.841 to 12.853 min.: VN082424.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.75	214	118.75	286	175.90	27640		
91.95	1620	127.80	56	176.90	1820		
92.90	2088	129.80	52				
93.95	5007	140.80	521				
94.90	37317	142.85	513				
95.95	2465	147.80	76				
103.75	225	154.80	91				
105.85	139	171.85	410				
115.75	248	172.80	188				
116.95	342	173.90	29059				
117.70	54	174.90	2194				