


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060325\
Data File : VN086834.D
Acq On : 03 Jun 2025 10:47
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051625W.M
Title : SW846 8260
Last Update : Sat May 17 00:46:13 2025

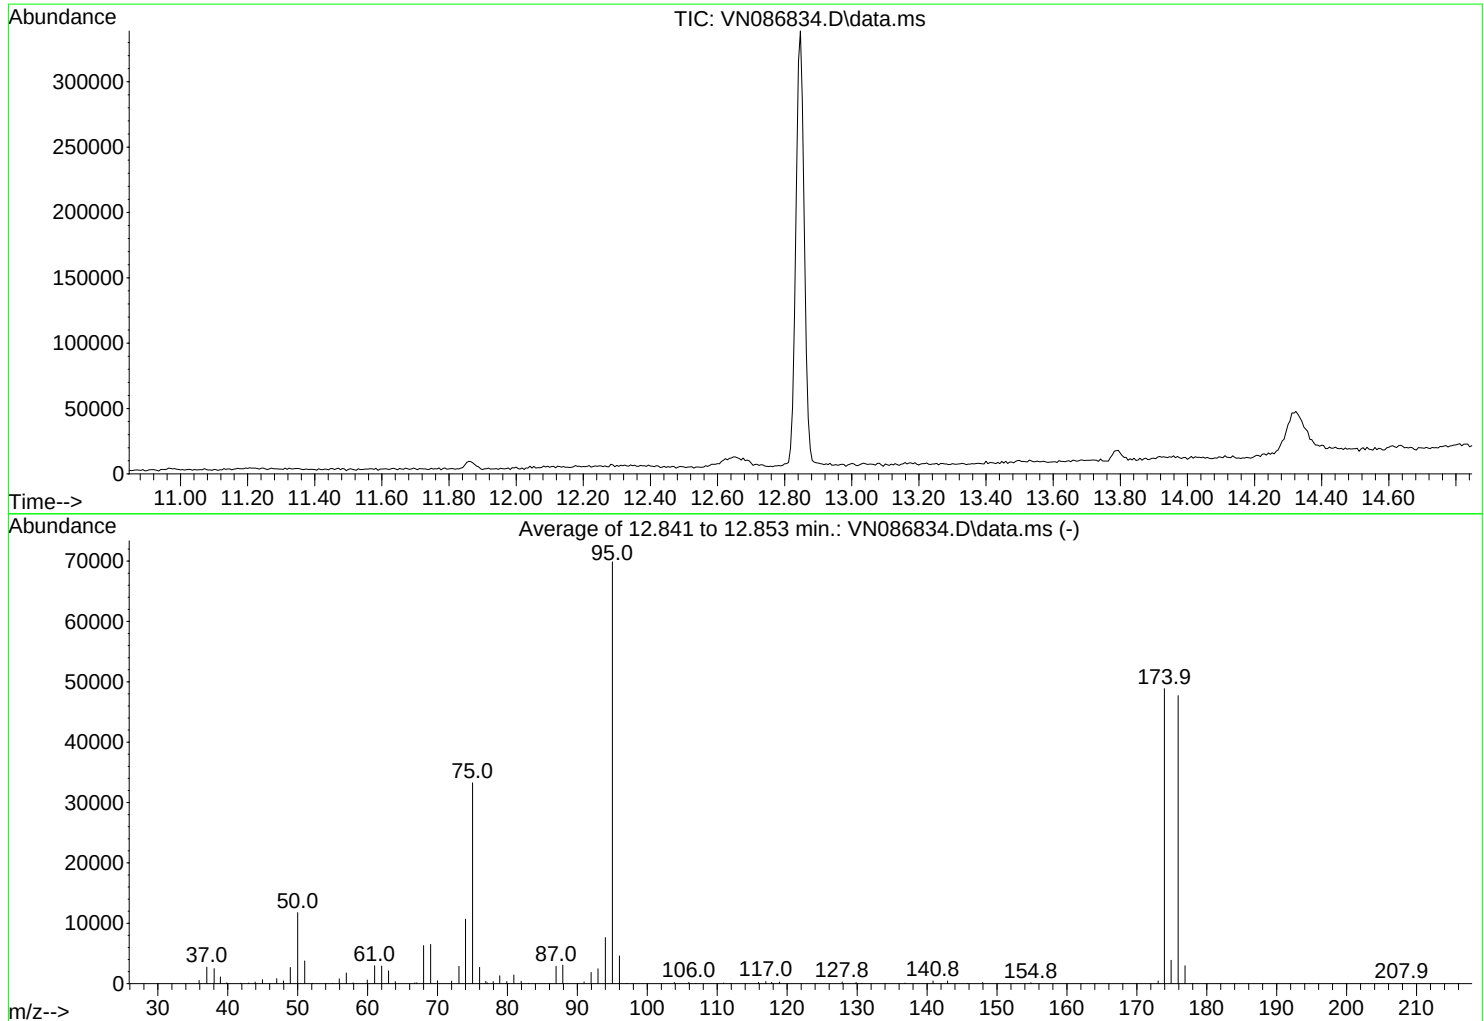

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1842

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	11764	PASS
75	95	30	60	47.6	33277	PASS
95	95	100	100	100.0	69877	PASS
96	95	5	9	6.6	4594	PASS
173	174	0.00	2	0.9	441	PASS
174	95	50	100	69.9	48877	PASS
175	174	5	9	7.9	3863	PASS
176	174	95	101	97.6	47701	PASS
177	176	5	9	6.2	2978	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	536	48.95	2681	63.00	2132	76.00	2711
37.00	2747	50.00	11764	63.95	342	76.90	360
38.05	2501	51.00	3775	66.75	147	77.10	14
38.95	1113	52.10	60	67.05	174	77.95	34
39.85	130	54.95	57	68.00	6320	78.90	1299
41.80	74	55.95	809	69.00	6498	79.90	356
43.00	103	56.95	1780	70.00	477	80.90	1437
43.90	263	57.90	128	72.00	435	81.95	401
44.95	630	59.95	611	73.05	2875	83.00	50
47.00	814	61.00	2974	74.00	10695	86.95	2901
47.95	463	62.00	2917	75.00	33277	87.90	3075

Average of 12.841 to 12.853 min.: VN086834.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.95	293	111.90	62	145.80	51		
91.95	1844	115.90	219	147.95	187		
92.95	2466	116.95	377	154.85	154		
94.00	7644	117.80	220	173.05	441		
95.00	69877	118.90	258	173.95	48877		
96.00	4594	127.85	292	174.90	3863		
97.05	38	129.85	202	175.90	47701		
103.85	182	130.70	51	176.90	2978		
105.95	227	136.85	120	177.90	57		
106.90	63	140.85	466	207.90	61		
110.90	104	142.95	465				

Instrument :

MSVOA_N

ClientSampleId :

BFB