

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN060420\
 Data File : VN061652.D
 Acq On : 4 Jun 2020 14:51
 Operator : JC/MD
 Sample : PB129284ZHE#01
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB129284ZHE#01

Quant Time: Jun 05 08:03:48 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052820W.M
 Quant Title : SW846 8260
 QLast Update : Fri May 29 02:14:10 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	309722	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	529777	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	530720	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	247632	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.99	65	176404	47.80	ug/l	0.00
Spiked Amount 50.000			Recovery	=	95.60%	
35) Dibromofluoromethane	7.55	113	132418	49.27	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.54%	
50) Toluene-d8	10.06	98	634235	50.93	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.86%	
62) 4-Bromofluorobenzene	12.38	95	245834	54.10	ug/l	0.00
Spiked Amount 50.000			Recovery	=	108.20%	
Target Compounds						
16) Acetone	3.78	43	22061	15.885	ug/l	99
20) Methylene Chloride	4.50	84	12896	2.181	ug/l	93
43) Isopropyl Acetate	8.13	43	71057	10.456	ug/l #	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN060420\
Data File : VN061652.D
Acq On : 4 Jun 2020 14:51
Operator : JC/MD
Sample : PB129284ZHE#01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB129284ZHE#01

Quant Time: Jun 05 08:03:48 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N052820W.M
Quant Title : SW846 8260
QLast Update : Fri May 29 02:14:10 2020
Response via : Initial Calibration

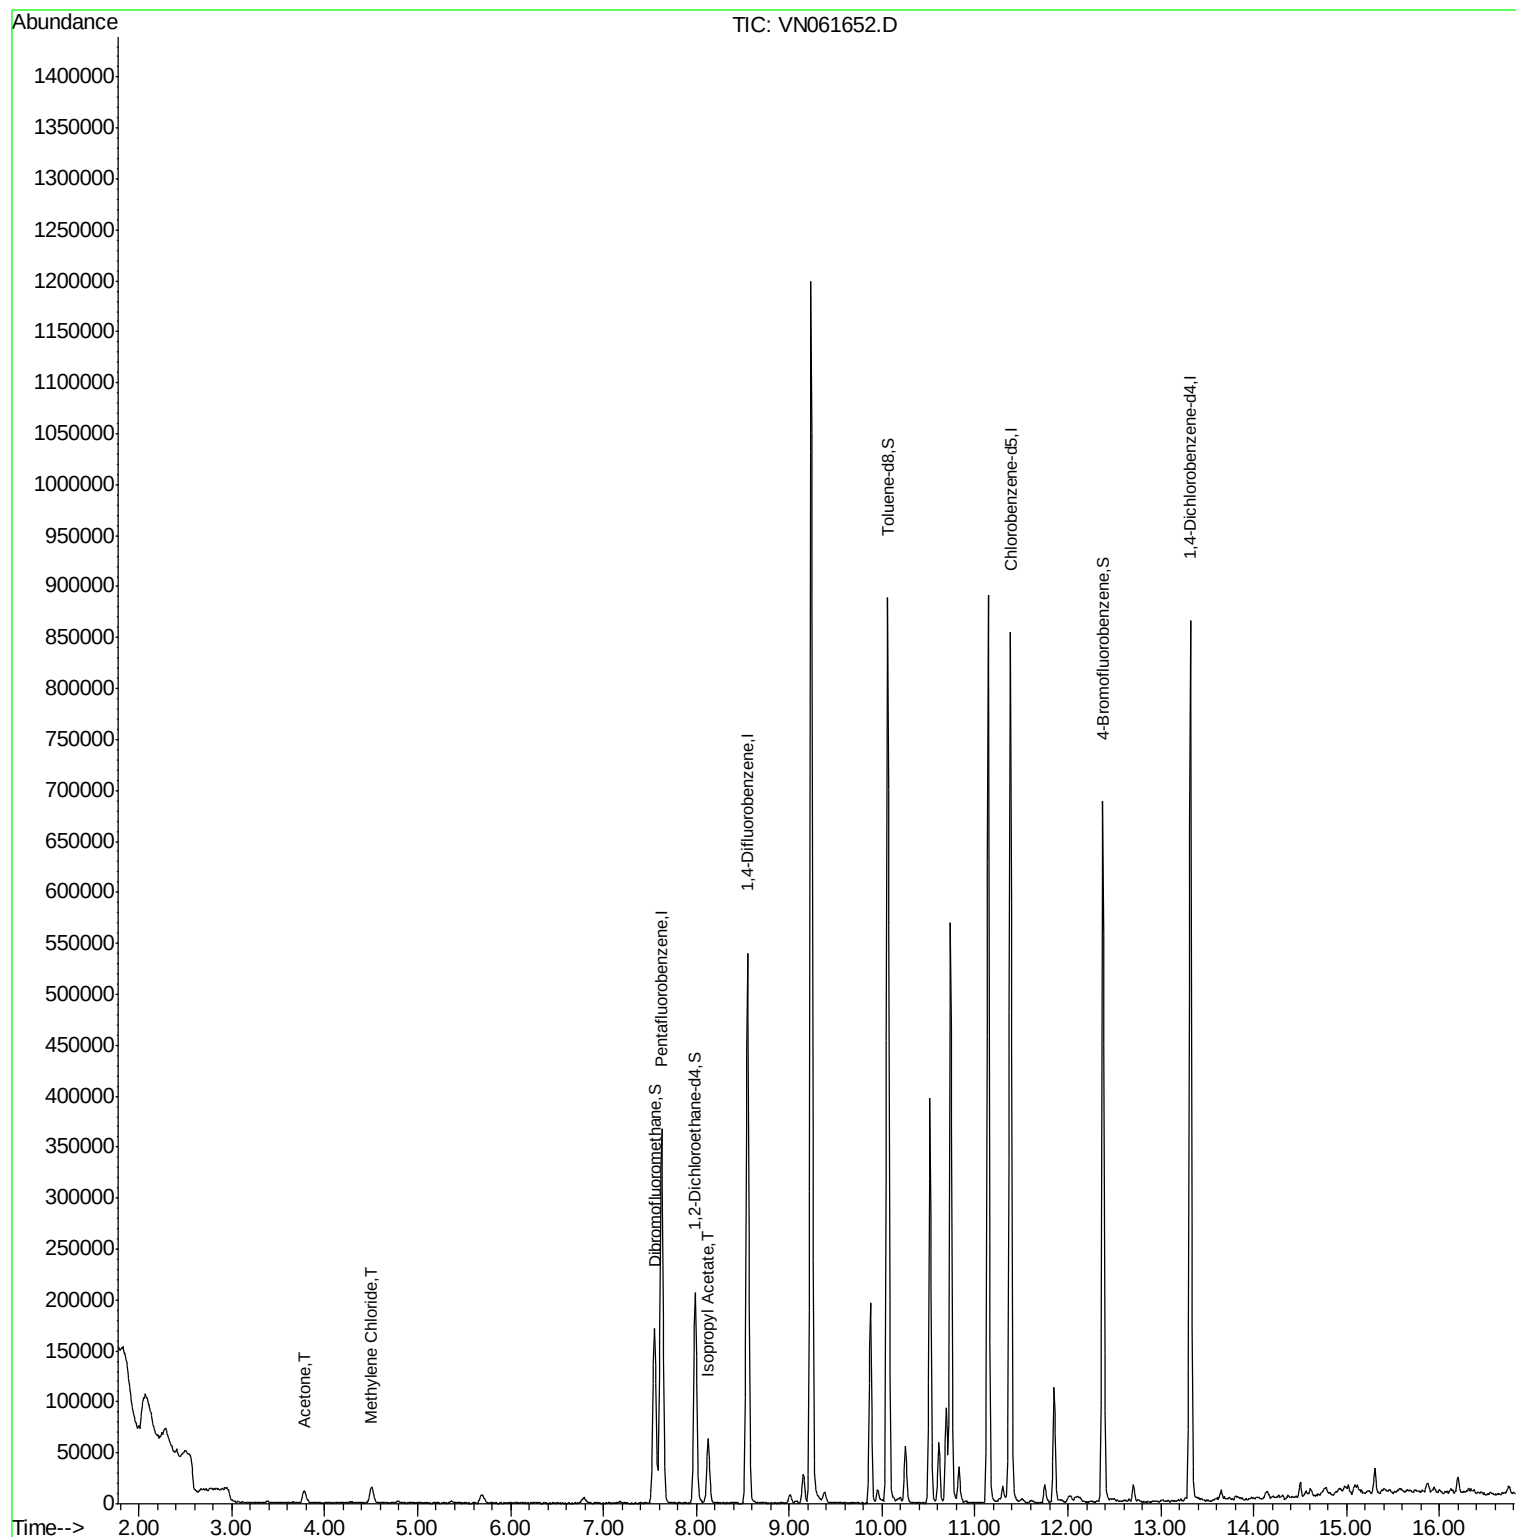

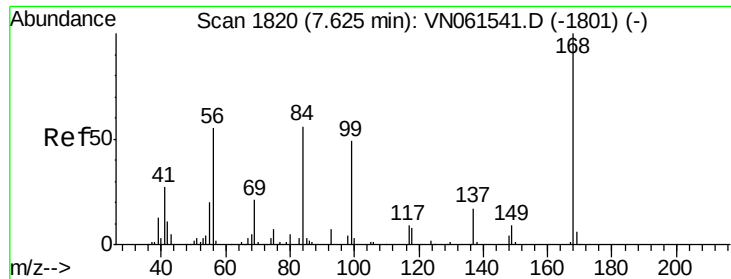

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. 0.00 min

Lab File: VN061652.D

Acq: 4 Jun 2020 14:51

Instrument :

MSVOA_N

ClientSampleId :


PB129284ZHE#01

Tot Ion:168 Resp: 309722

Ion Ratio Lower Upper

168 100

99 54.2 45.0 67.4

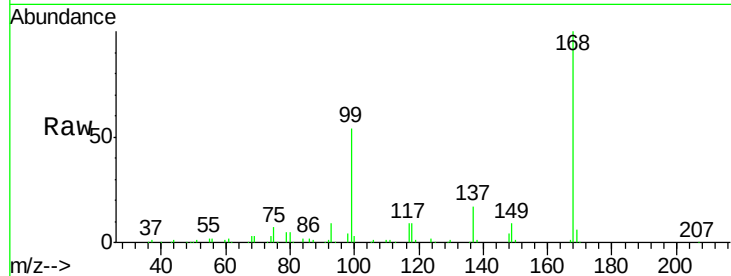

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

7.63



150000

100000

50000

0

Time--> 7.50 7.60 7.70

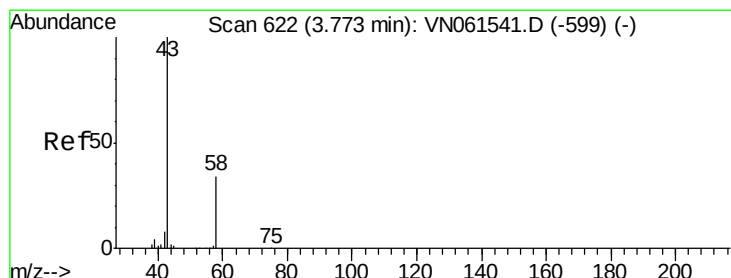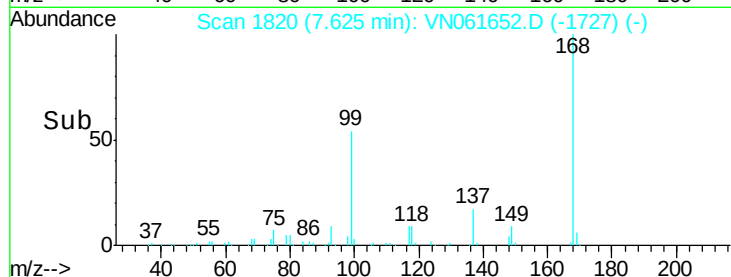

#16

Acetone

Concen: 15.885 ug/l

RT: 3.78 min Scan# 624

Delta R.T. 0.01 min

Lab File: VN061652.D


Acq: 4 Jun 2020 14:51

Tgt Ion: 43 Resp: 22061

Ion Ratio Lower Upper

43 100

58 34.8 27.2 40.8

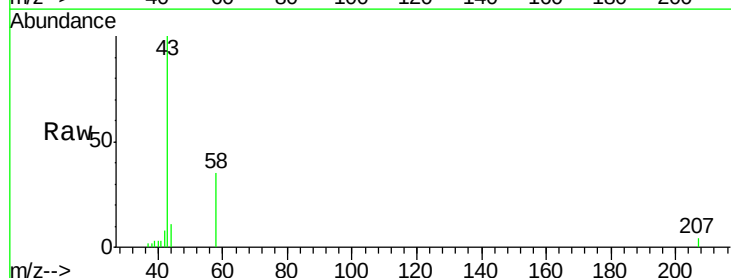

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

3.78

8000


6000


4000

2000

0

Time--> 3.70 3.80 3.90




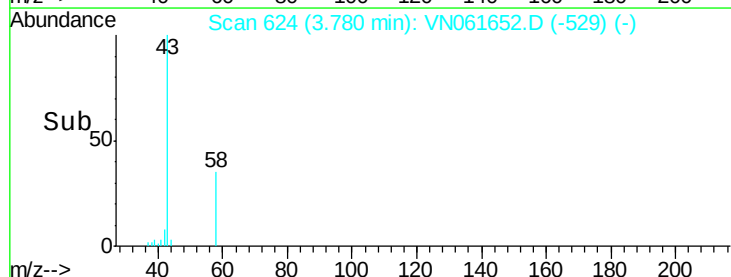


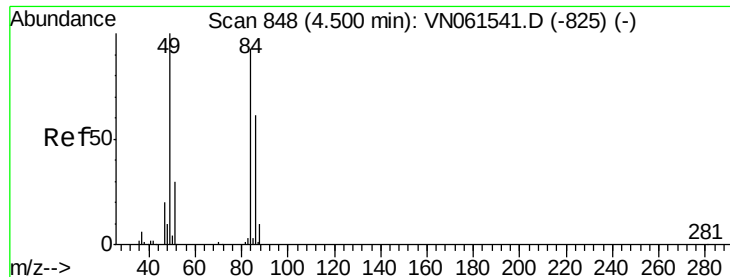

#20
Methylene Chloride
Concen: 2.181 ug/l
RT: 4.50 min Scan# 849
Delta R.T. 0.00 min
Lab File: VN061652.D
Acq: 4 Jun 2020 14:51




Instrument :
MSVOA_N
ClientSampleId :
PB129284ZHE#01


Tot Ion: 84 Resp: 12896
Ion Ratio Lower Upper
84 100
49 98.4 85.8 128.8
51 30.7 26.2 39.2
86 61.8 52.6 78.8

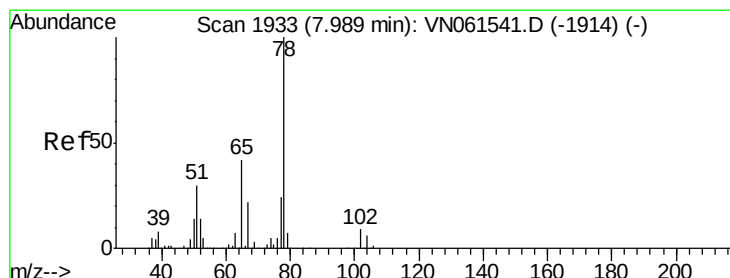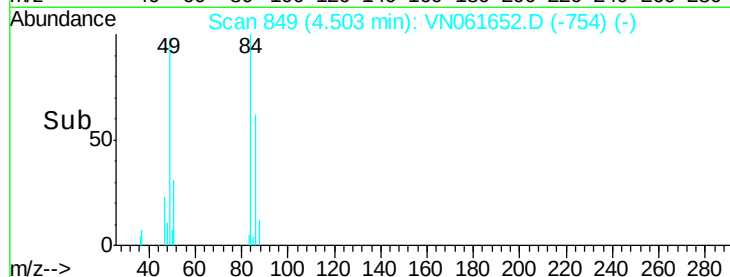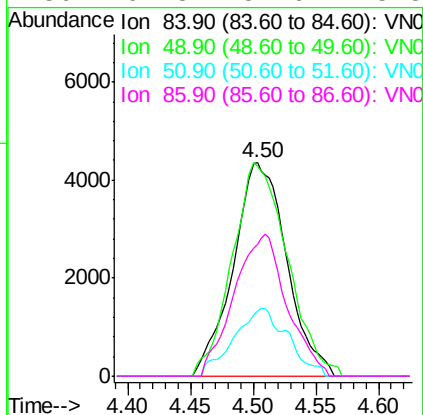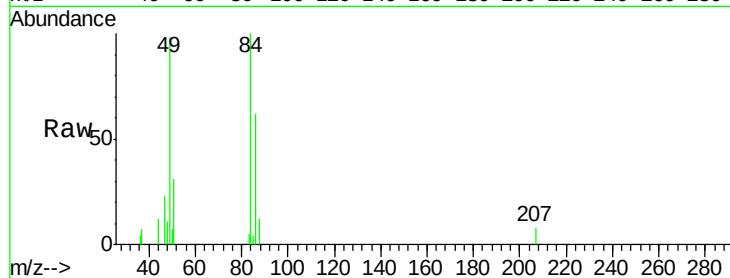

#33
1,2-Dichloroethane-d4
Concen: 47.804 ug/l
RT: 7.99 min Scan# 1933
Delta R.T. 0.00 min
Lab File: VN061652.D
Acq: 4 Jun 2020 14:51

Tgt Ion: 65 Resp: 176404
Ion Ratio Lower Upper
65 100
67 52.4 0.0 104.8

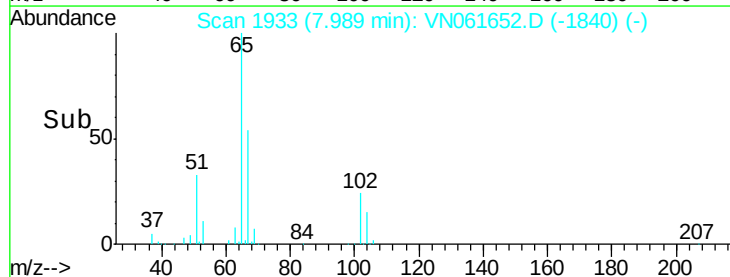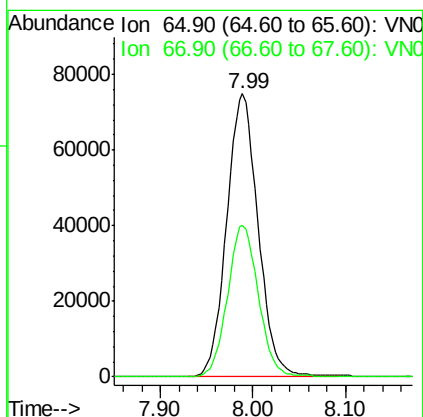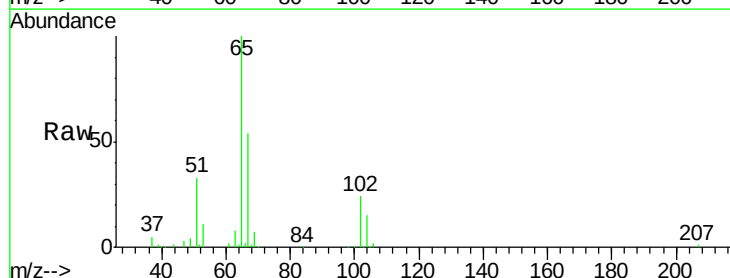

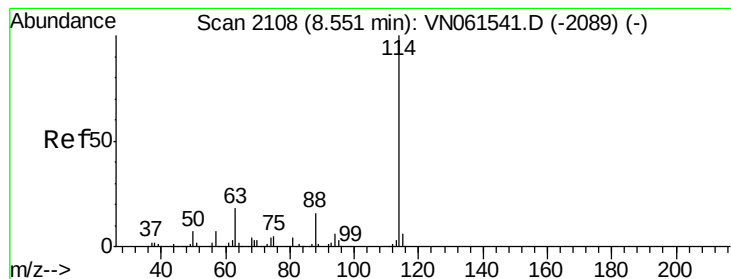

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.55 min Scan# 2108

Delta R.T. 0.00 min

Lab File: VN061652.D

Acq: 4 Jun 2020 14:51

Instrument :

MSVOA_N

ClientSampleId :

PB129284ZHE#01


Tot Ion:114 Resp: 529777

Ion Ratio Lower Upper

114 100

63 17.5 0.0 35.8




88 14.9 0.0 31.0

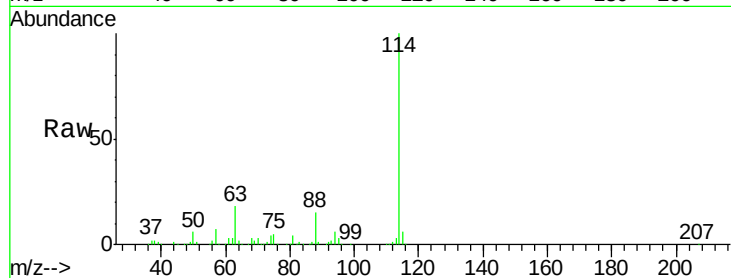

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN

Ion 87.90 (87.60 to 88.60): VN

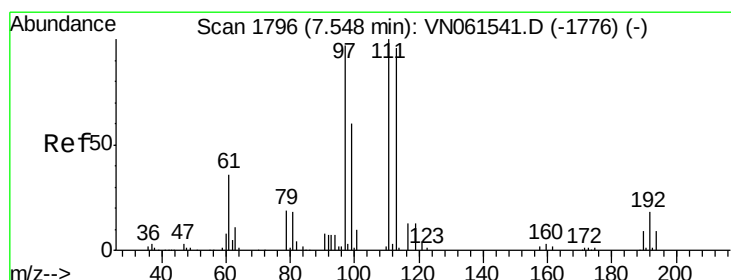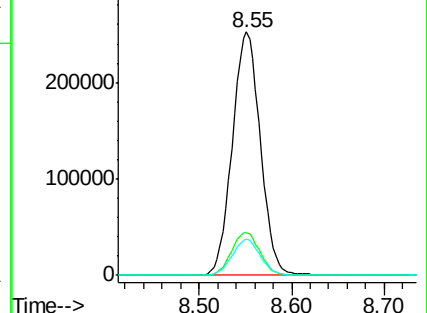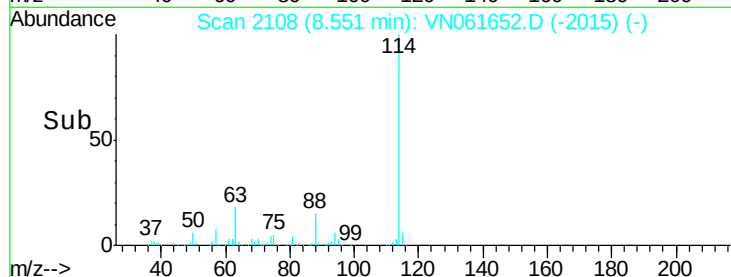

#35

Dibromofluoromethane

Concen: 49.273 ug/l

RT: 7.55 min Scan# 1797

Delta R.T. 0.00 min

Lab File: VN061652.D

Acq: 4 Jun 2020 14:51


Tgt Ion:113 Resp: 132418

Ion Ratio Lower Upper

113 100

111 103.5 83.4 125.0



192 19.4 15.4 23.2

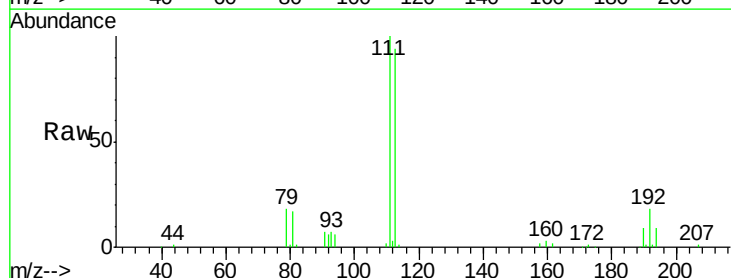


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

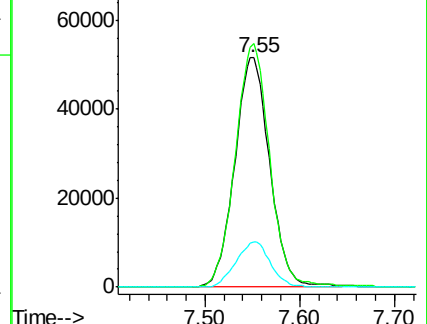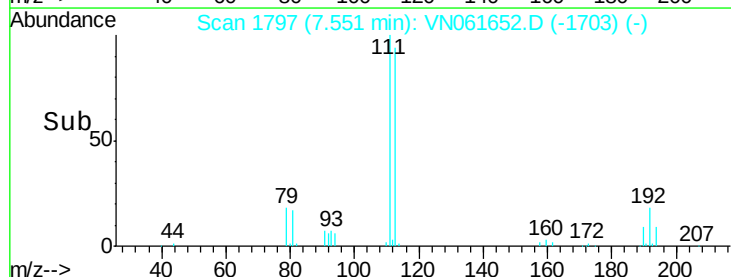

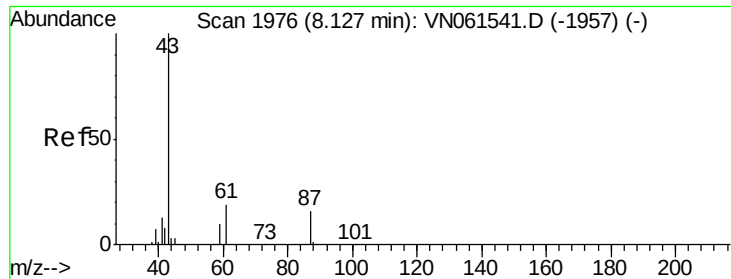

#43

Isopropyl Acetate

Concen: 10.456 ug/l

RT: 8.13 min Scan# 1976

Delta R.T. 0.00 min

Lab File: VN061652.D

Acq: 4 Jun 2020 14:51

Instrument :

MSVOA_N

ClientSampleId :

PB129284ZHE#01


Tot Ion: 43 Resp: 71057

Ion Ratio Lower Upper

43 100

61 22.0 23.6 35.4#




87 17.2 13.0 19.6

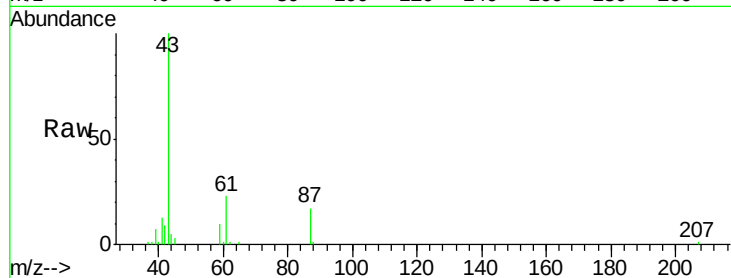

Abundance Ion 43.00 (42.70 to 43.70): VN061541.D (-1957) (-)

Ion 61.00 (60.70 to 61.70): VN061541.D (-1957) (-)

Ion 87.00 (86.70 to 87.70): VN061541.D (-1957) (-)

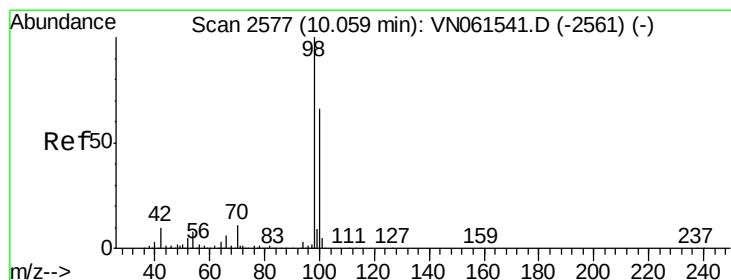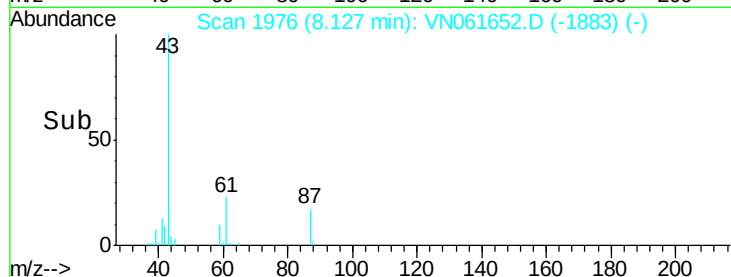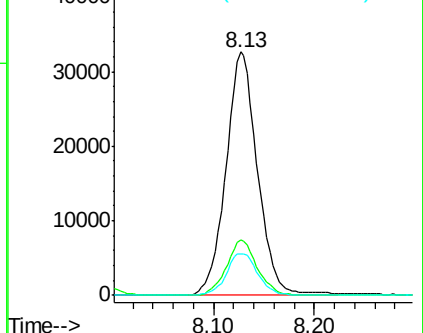

#50

Toluene-d8

Concen: 50.926 ug/l

RT: 10.06 min Scan# 2577

Delta R.T. 0.00 min

Lab File: VN061652.D


Acq: 4 Jun 2020 14:51

Tgt Ion: 98 Resp: 634235

Ion Ratio Lower Upper



98 100


100 66.1 52.8 79.2

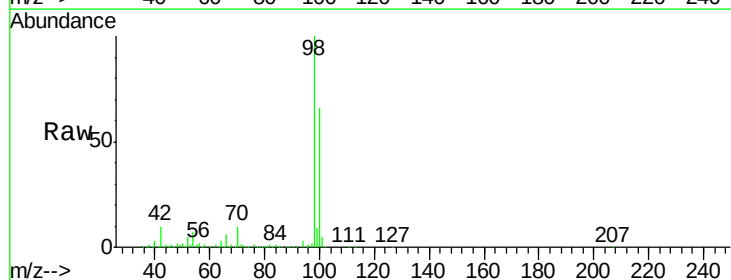

Abundance Ion 98.00 (97.70 to 98.70): VN061541.D (-2561) (-)

Ion 100.00 (99.70 to 100.70): VN061541.D (-2561) (-)



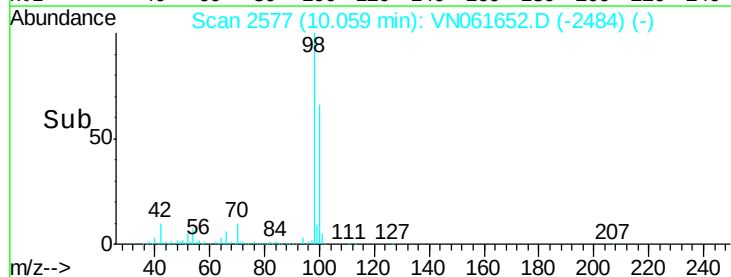
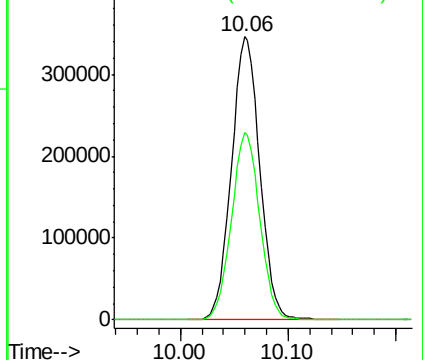


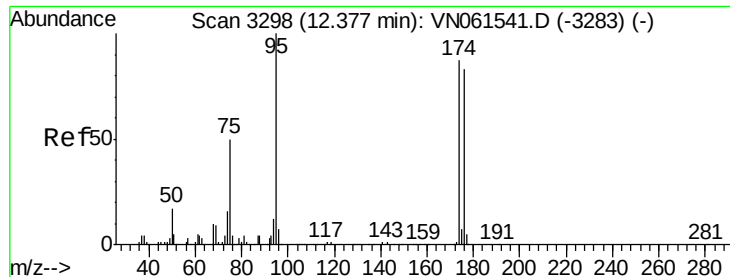

#62
 4-Bromofluorobenzene
 Concen: 54.105 ug/l
 RT: 12.38 min Scan# 3298
 Delta R.T. 0.00 min
 Lab File: VN061652.D
 Acq: 4 Jun 2020 14:51




Instrument :
 MSVOA_N
 ClientSampleId :
 PB129284ZHE#01


Tot Ion: 95 Resp: 245834
 Ion Ratio Lower Upper
 95 100
 174 84.8 0.0 172.8
 176 79.9 0.0 164.8

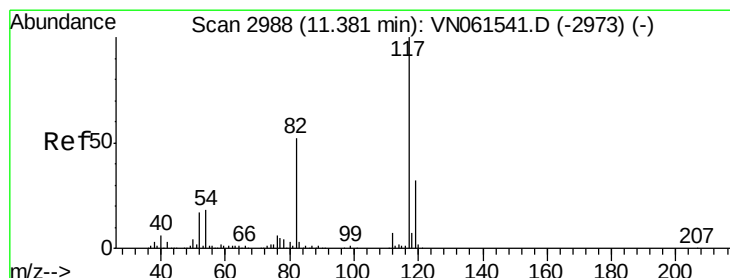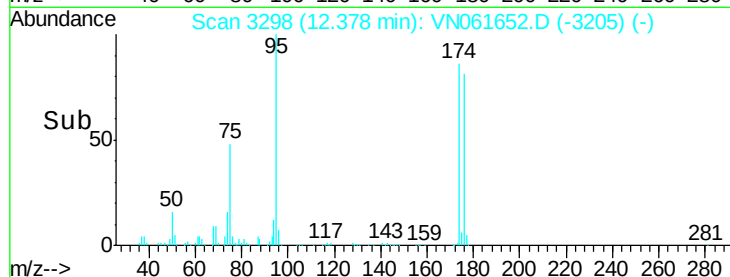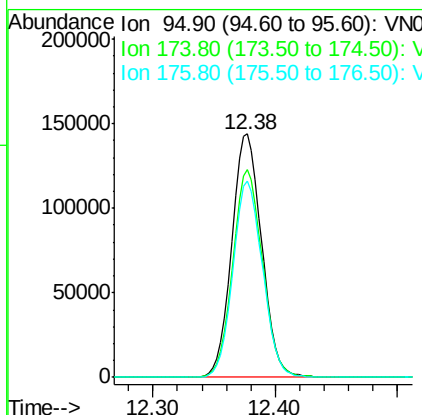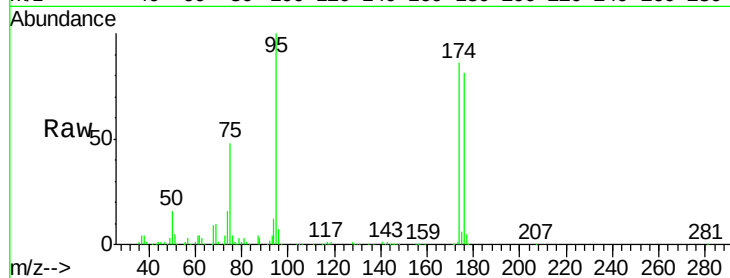

#63
 Chlorobenzene-d5
 Concen: 50.000 ug/l
 RT: 11.38 min Scan# 2988
 Delta R.T. 0.00 min
 Lab File: VN061652.D
 Acq: 4 Jun 2020 14:51

Tgt Ion: 117 Resp: 530720
 Ion Ratio Lower Upper
 117 100
 82 52.3 41.5 62.3
 119 31.8 25.6 38.4

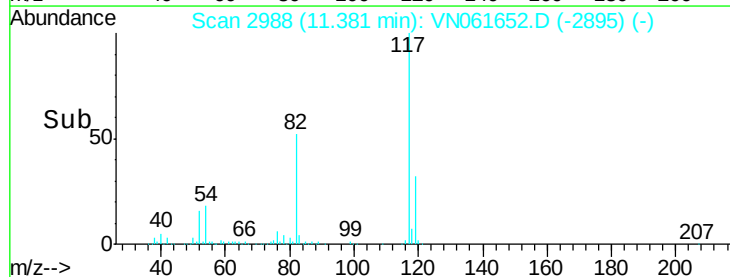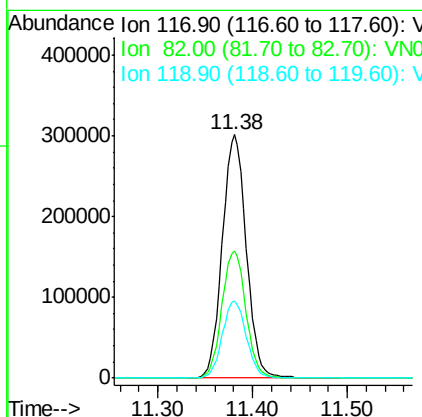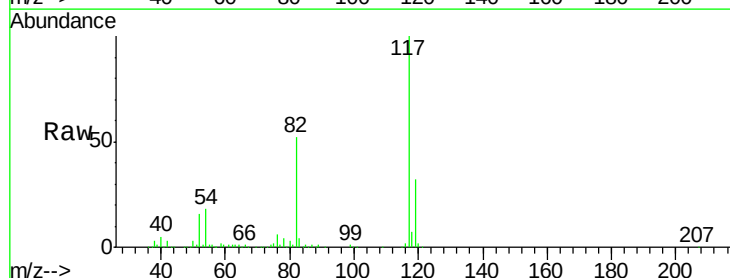

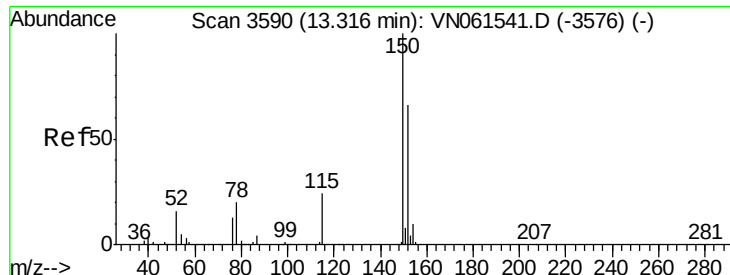

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3590

Delta R.T. 0.00 min

Lab File: VN061652.D

Acq: 4 Jun 2020 14:51

Instrument :

MSVOA_N

ClientSampleId :

PB129284ZHE#01



Tot Ion:152 Resp: 247632

Ion Ratio Lower Upper

152 100

115 57.5 28.0 84.0

150 160.1 0.0 344.0

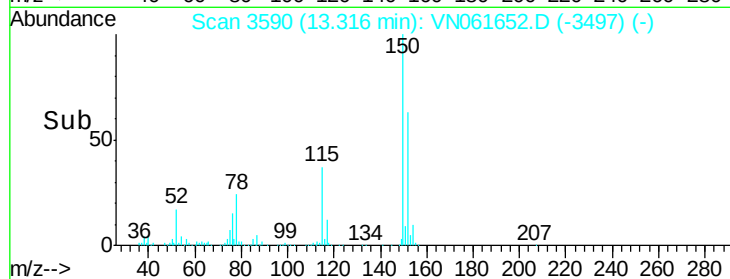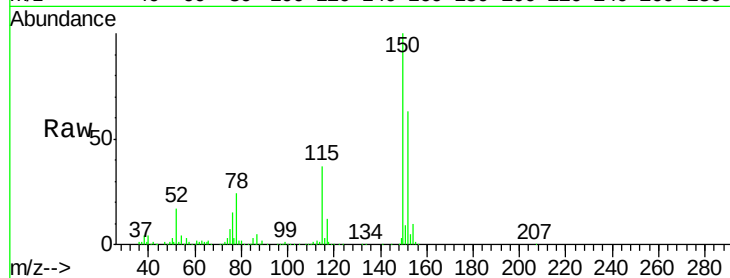

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

