


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN060420\
 Data File : VN061643.D
 Acq On : 4 Jun 2020 10:32
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052820W.M
 Title : SW846 8260
 Last Update : Fri May 29 02:14:10 2020

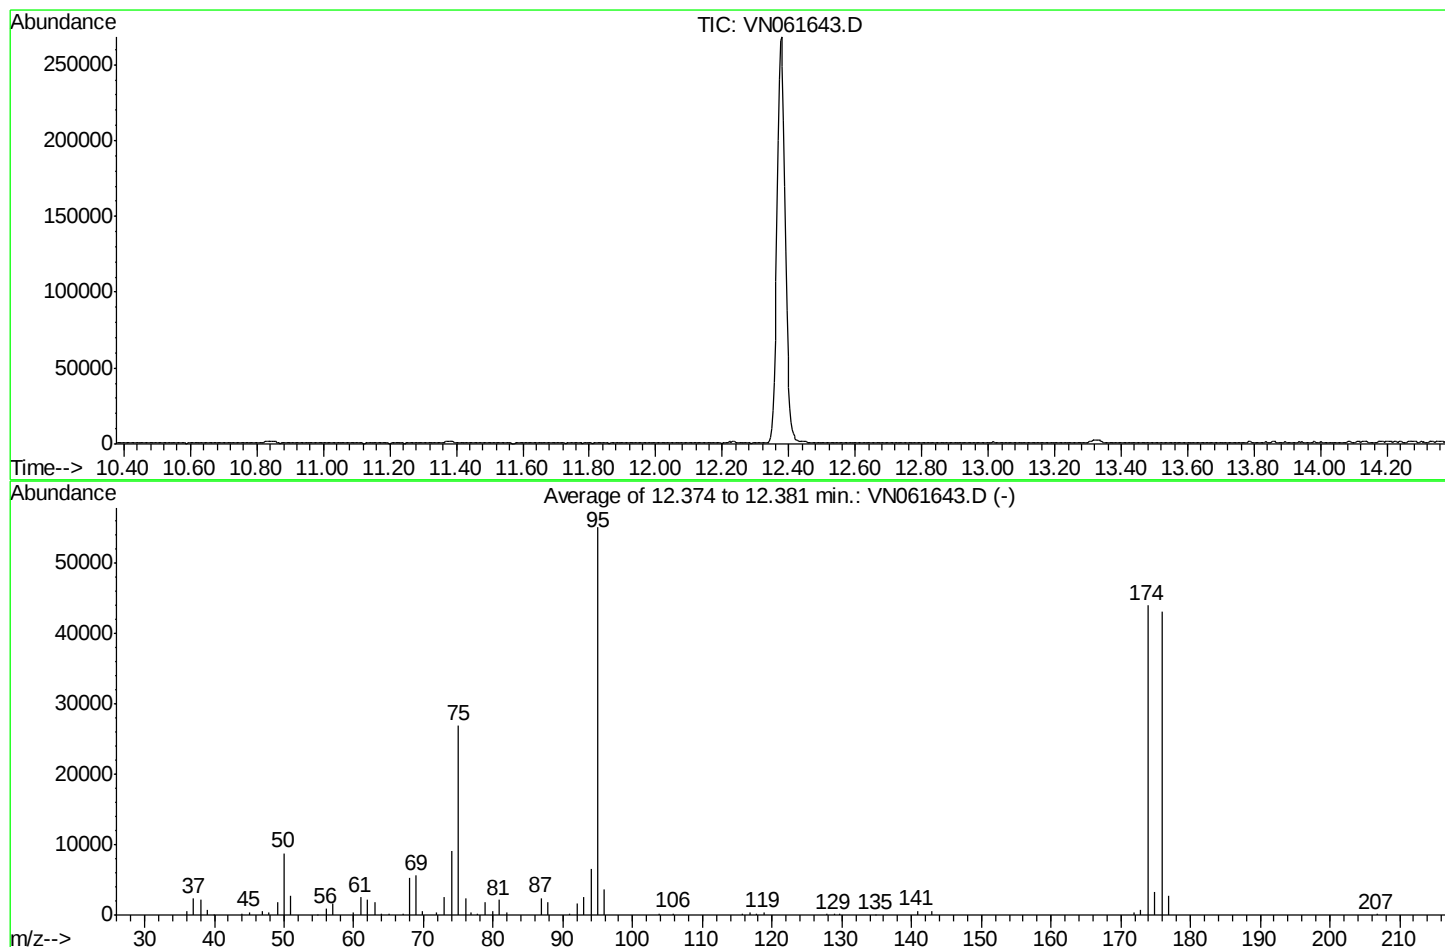

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3284

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	8760	PASS
75	95	30	60	48.8	26853	PASS
95	95	100	100	100.0	55032	PASS
96	95	5	9	6.8	3726	PASS
173	174	0.00	2	1.5	642	PASS
174	95	50	100	79.8	43941	PASS
175	174	5	9	7.5	3275	PASS
176	174	95	101	98.1	43085	PASS
177	176	5	9	6.6	2823	PASS