

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060421\
 Data File : VN067215.D
 Acq On : 4 Jun 2021 23:11
 Operator : JC/MD
 Sample : M2589-33
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 18-B10(4-6)

Quant Time: Jun 05 05:34:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060421W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 04 19:00:20 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.091	168	138345	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.973	114	230530	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.749	117	220816	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.680	152	102134	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.442	65	84559	44.839	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	89.680%		
35) Dibromofluoromethane	8.029	113	69759	48.812	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	97.620%		
50) Toluene-d8	10.446	98	297886	51.179	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	102.360%		
62) 4-Bromofluorobenzene	12.736	95	98472	43.928	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	87.860%		
Target Compounds						Qvalue
3) Chloromethane	2.303	50	549	0.280	ug/l #	42
13) Acrolein	4.065	56	376	Below Cal	#	56
16) Acetone	4.307	43	17063	26.222	ug/l	100
17) Carbon Disulfide	4.535	76	1405	0.365	ug/l #	86
20) Methylene Chloride	5.111	84	6986	4.263	ug/l	97
25) 2-Butanone	7.351	43	4050	3.887	ug/l	95
31) Cyclohexane	8.094	56	3480	1.374	ug/l #	43
36) 1,1-Dichloropropene	8.088	75	10659	5.006	ug/l #	48
38) Carbon Tetrachloride	8.091	117	13181	5.669	ug/l #	15
42) 1,2-Dichloroethane	8.536	62	843	0.372	ug/l #	73
43) Isopropyl Acetate	8.568	43	7835	2.008	ug/l #	81
48) Methyl methacrylate	9.553	41	4478	2.648	ug/l #	25
51) 4-Methyl-2-Pentanone	10.336	43	3577	1.564	ug/l	99
52) Toluene	10.513	92	4105	0.942	ug/l	85
54) cis-1,3-Dichloropropene	10.247	75	14047	4.982	ug/l #	70
57) 1,3-Dichloropropane	11.095	76	1187	0.435	ug/l #	42
59) 2-Hexanone	11.098	43	19786	11.904	ug/l #	49
67) Ethyl Benzene	11.851	91	2101	0.243	ug/l	98
68) m/p-Xylenes	11.956	106	2528	0.744	ug/l	85
69) o-Xylene	12.286	106	2183	0.657	ug/l	93
70) Styrene	12.299	104	3616	0.637	ug/l	95
74) N-amyl acetate	12.358	43	1647	0.526	ug/l #	50
76) 1,2,3-Trichloropropane	12.736	75	55553	28.284	ug/l #	100
80) 1,3,5-Trimethylbenzene	13.063	105	2256	0.335	ug/l	98
81) trans-1,4-Dichloro-2-b...	12.736	75	55553	69.203	ug/l #	15
84) 1,2,4-Trimethylbenzene	13.369	105	4792	0.716	ug/l	79
88) 1,4-Dichlorobenzene	13.702	146	836	0.245	ug/l #	65
90) Hexachloroethane	14.329	117	833	0.684	ug/l #	4
95) Naphthalene	15.512	128	23663	9.174	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060421\
Data File : VN067215.D
Acq On : 4 Jun 2021 23:11
Operator : JC/MD
Sample : M2589-33
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
18-B10(4-6)

Quant Time: Jun 05 05:34:24 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060421W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 04 19:00:20 2021
Response via : Initial Calibration




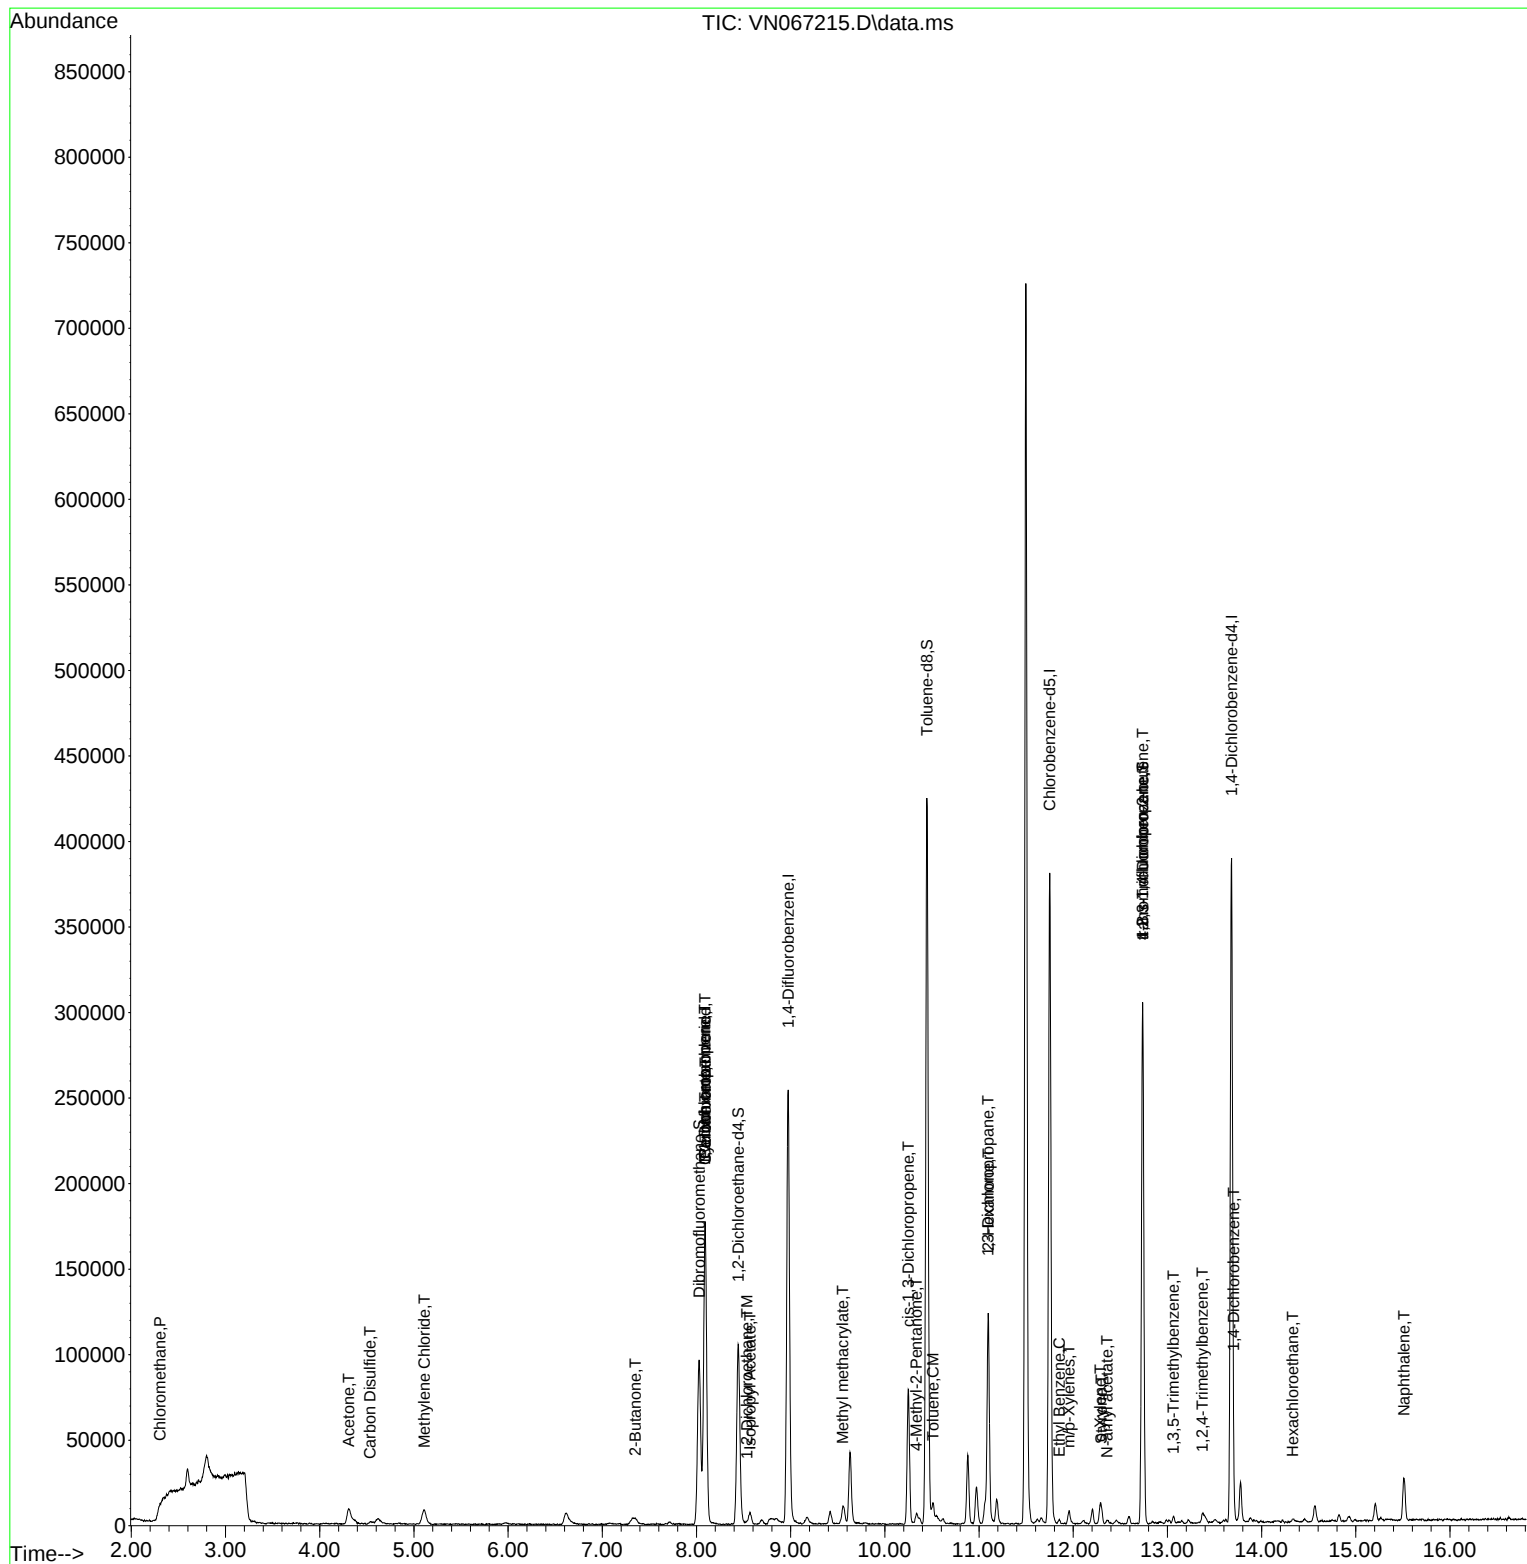




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.091 min Scan# 2275
Delta R.T. 0.000 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11




Instrument :
MSVOA_N
ClientSampleId :
18-B10(4-6)


Tgt Ion:168 Resp: 138345
Ion Ratio Lower Upper
168 100
99 52.6 38.5 57.7

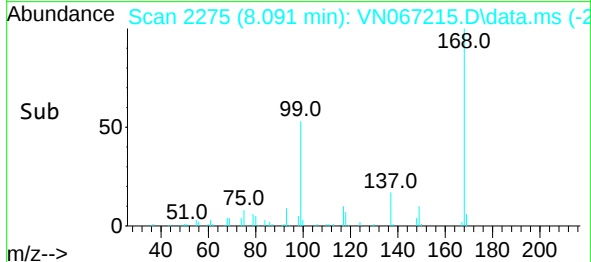

#3
Chloromethane
Concen: 0.280 ug/l
RT: 2.303 min Scan# 117
Delta R.T. 0.008 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11

Tgt Ion: 50 Resp: 549
Ion Ratio Lower Upper
50 100
52 0.0 26.5 39.7#


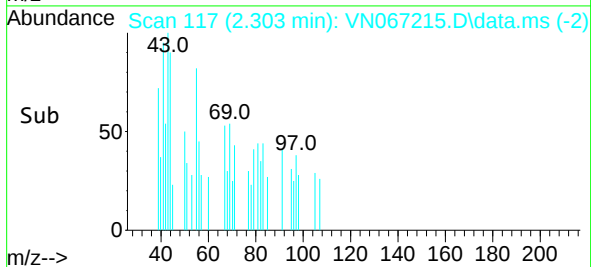

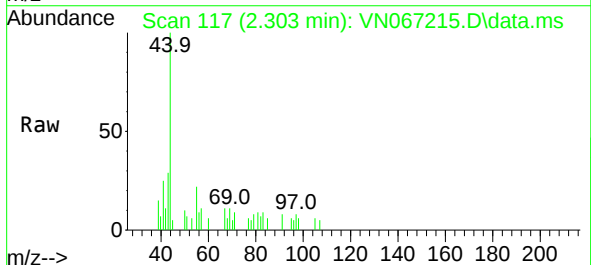




#13
Acrolein
Concen: Below Cal
RT: 4.065 min Scan# 774
Delta R.T. 0.018 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11




Instrument :
MSVOA_N
ClientSampleId :
18-B10(4-6)


Tgt Ion: 56 Resp: 376
Ion Ratio Lower Upper
56 100
55 31.6 53.8 80.6#

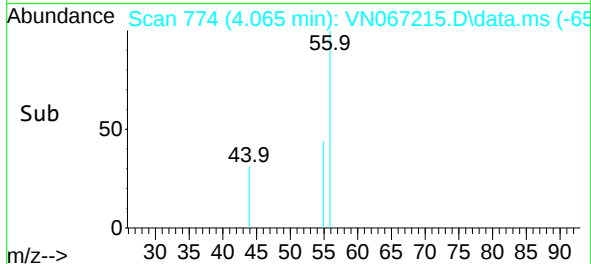

#16
Acetone
Concen: 26.222 ug/l
RT: 4.307 min Scan# 864
Delta R.T. 0.016 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11

Tgt Ion: 43 Resp: 17063
Ion Ratio Lower Upper
43 100
58 33.9 27.2 40.8


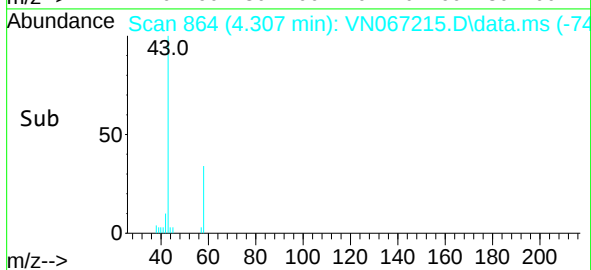

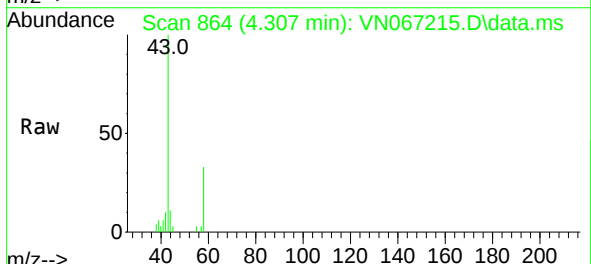




#17
Carbon Disulfide
Concen: 0.365 ug/l
RT: 4.535 min Scan# 949
Delta R.T. -0.005 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11




Instrument :
MSVOA_N
ClientSampleId :
18-B10(4-6)


Tgt Ion: 76 Resp: 1405
Ion Ratio Lower Upper
76 100
78 14.6 7.5 11.3#

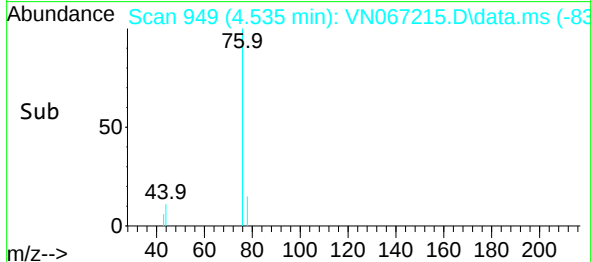

#20
Methylene Chloride
Concen: 4.263 ug/l
RT: 5.111 min Scan# 1164
Delta R.T. 0.008 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11

Tgt Ion: 84 Resp: 6986
Ion Ratio Lower Upper
84 100
49 113.7 88.3 132.5
51 32.8 26.7 40.1
86 59.7 51.1 76.7


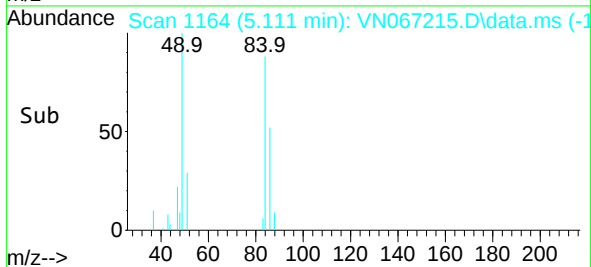

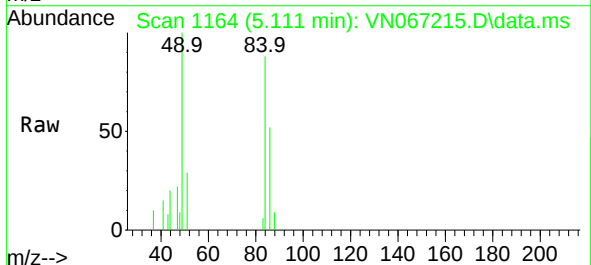


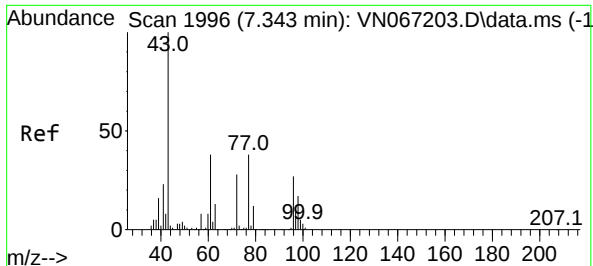

#25
2-Butanone
Concen: 3.887 ug/l
RT: 7.351 min Scan# 1999
Delta R.T. 0.008 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11




Instrument :
MSVOA_N
ClientSampleId :
18-B10(4-6)


Tgt Ion: 43 Resp: 4050
Ion Ratio Lower Upper
43 100
72 27.6 24.4 36.6

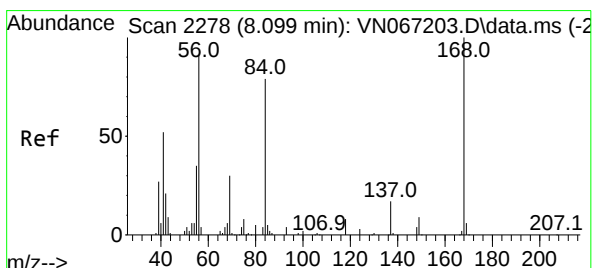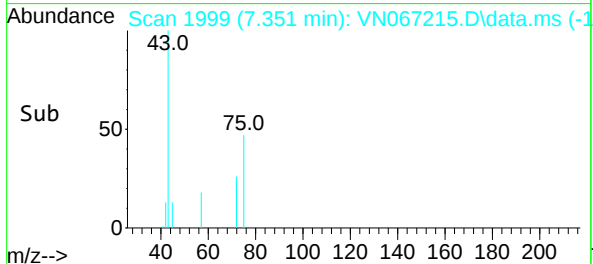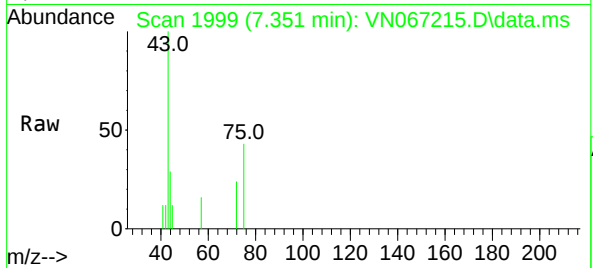

#31
Cyclohexane
Concen: 1.374 ug/l
RT: 8.094 min Scan# 2276
Delta R.T. -0.005 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11

Tgt Ion: 56 Resp: 3480
Ion Ratio Lower Upper
56 100
69 144.7 28.0 42.0#
84 99.4 74.2 111.2


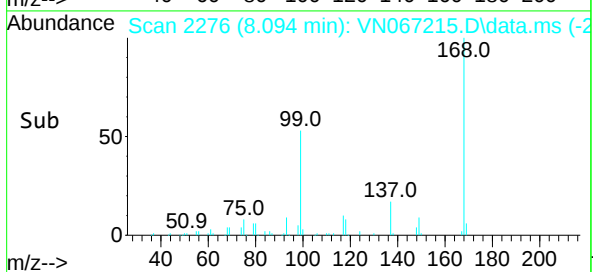

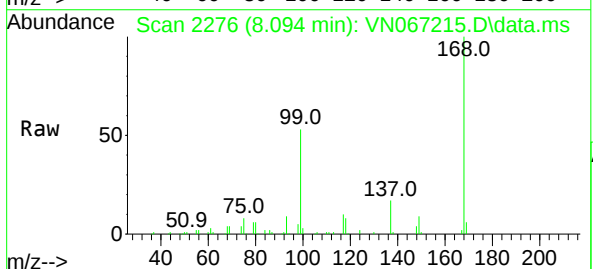




#33
 1,2-Dichloroethane-d4
 Concen: 44.839 ug/l
 RT: 8.442 min Scan# 2406
 Delta R.T. 0.000 min
 Lab File: VN067215.D
 Acq: 4 Jun 2021 23:11




Instrument :
 MSVOA_N
 ClientSampled :
 18-B10(4-6)


Tgt Ion: 65 Resp: 84559
 Ion Ratio Lower Upper
 65 100
 67 53.4 0.0 110.4

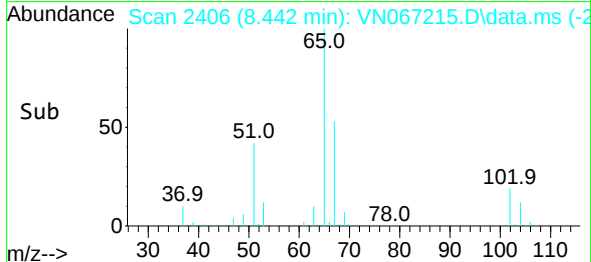

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.973 min Scan# 2604
 Delta R.T. 0.003 min
 Lab File: VN067215.D
 Acq: 4 Jun 2021 23:11

Tgt Ion: 114 Resp: 230530
 Ion Ratio Lower Upper
 114 100
 63 20.1 0.0 35.8
 88 14.1 0.0 30.4


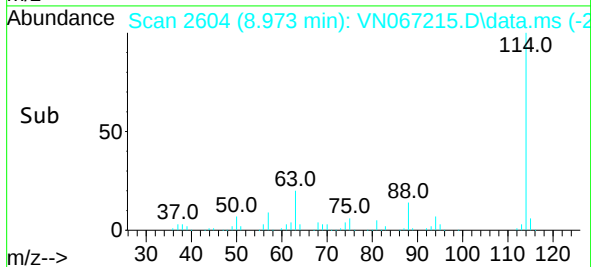

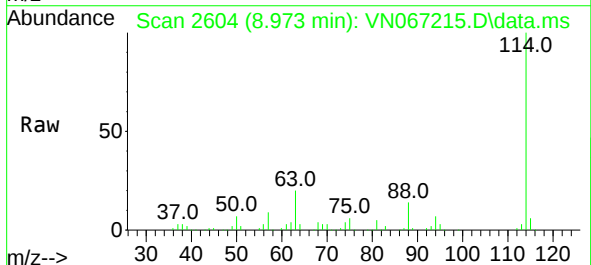




#35
Dibromofluoromethane
Concen: 48.812 ug/l
RT: 8.029 min Scan# 2252
Delta R.T. 0.003 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11




Instrument :
MSVOA_N
ClientSampleId :
18-B10(4-6)


Tgt Ion:113 Resp: 69759
Ion Ratio Lower Upper
113 100
111 104.8 82.6 124.0
192 18.5 18.2 27.4

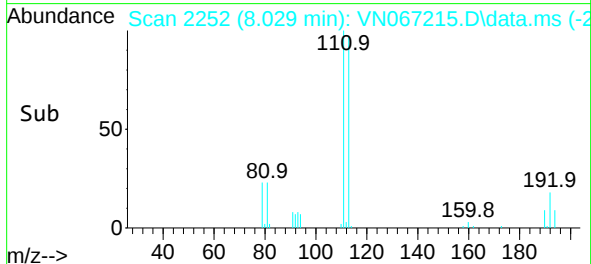

#36
1,1-Dichloropropene
Concen: 5.006 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.139 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11


Tgt Ion: 75 Resp: 10659
Ion Ratio Lower Upper
75 100
110 8.7 19.1 57.3#
77 0.0 24.8 37.2#

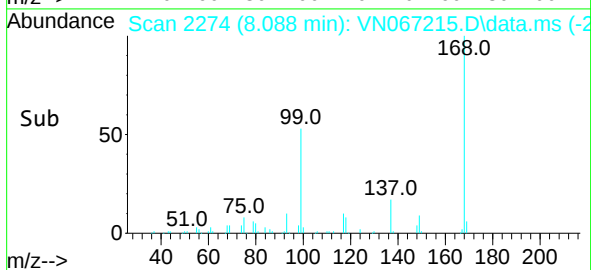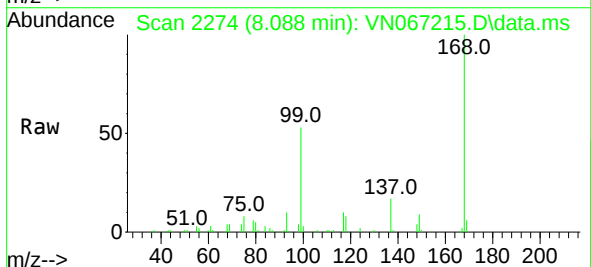






#38
Carbon Tetrachloride
Concen: 5.669 ug/l
RT: 8.091 min Scan# 2275
Delta R.T. -0.121 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11


Instrument :
MSVOA_N
ClientSampleId :
18-B10(4-6)





Tgt Ion:117 Resp: 13181
Ion Ratio Lower Upper
117 100
119 4.4 78.2 117.2#
121 0.0 24.7 37.1#




#42
1,2-Dichloroethane
Concen: 0.372 ug/l
RT: 8.536 min Scan# 2441
Delta R.T. 0.000 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11




Tgt Ion: 62 Resp: 843
Ion Ratio Lower Upper
62 100
98 0.0 0.0 20.2

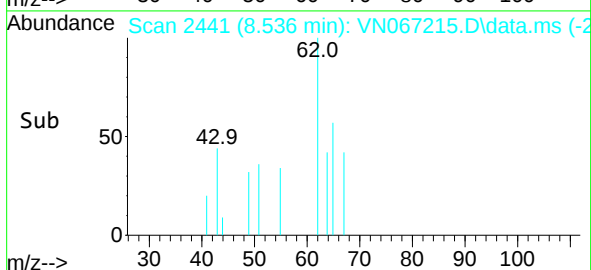






#43
Isopropyl Acetate
Concen: 2.008 ug/l
RT: 8.568 min Scan# 2453
Delta R.T. 0.003 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11


Instrument :
MSVOA_N
ClientSampleId :
18-B10(4-6)





Tgt Ion: 43	Resp: 7835
Ion Ratio	Lower Upper
43 100	
61 17.3	23.4 35.0#
87 9.6	12.2 18.2#




#48
Methyl methacrylate
Concen: 2.648 ug/l
RT: 9.553 min Scan# 2820
Delta R.T. -0.011 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11



Tgt Ion: 41	Resp: 4478
Ion Ratio	Lower Upper
41 100	
69 0.0	80.5 120.7#
39 34.5	41.4 62.0#



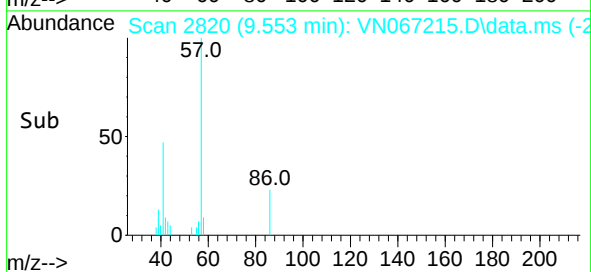





#50
Toluene-d8
Concen: 51.179 ug/l
RT: 10.446 min Scan# 3153
Delta R.T. 0.000 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11




Instrument :
MSVOA_N
ClientSampleId :
18-B10(4-6)


Tgt Ion: 98 Resp: 297886
Ion Ratio Lower Upper
98 100
100 62.4 51.8 77.8

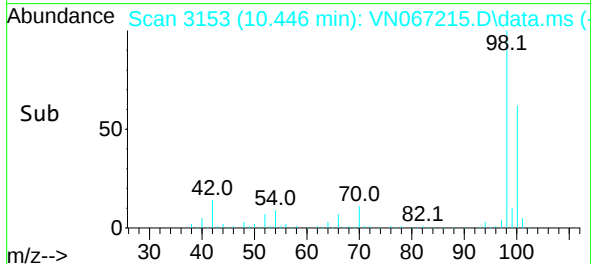

#51
4-Methyl-2-Pentanone
Concen: 1.564 ug/l
RT: 10.336 min Scan# 3112
Delta R.T. -0.000 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11

Tgt Ion: 43 Resp: 3577
Ion Ratio Lower Upper
43 100
58 43.5 34.5 51.7


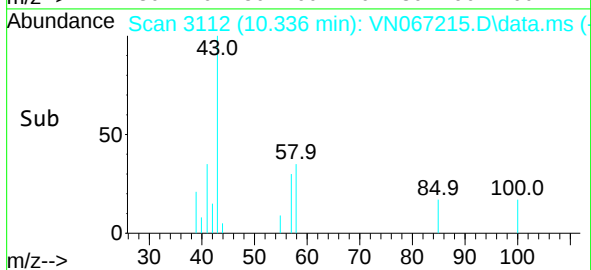

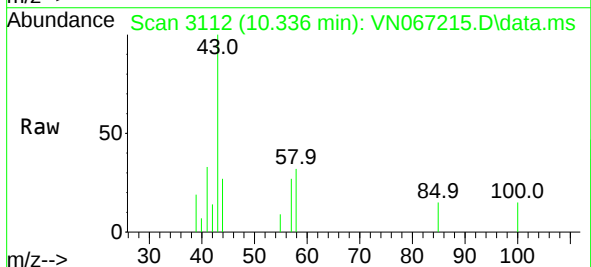




#52
Toluene
Concen: 0.942 ug/l
RT: 10.513 min Scan# 3178
Delta R.T. 0.003 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11




Instrument :
MSVOA_N
ClientSampleId :
18-B10(4-6)


Tgt Ion: 92 Resp: 4105
Ion Ratio Lower Upper
92 100
91 193.6 138.7 208.1

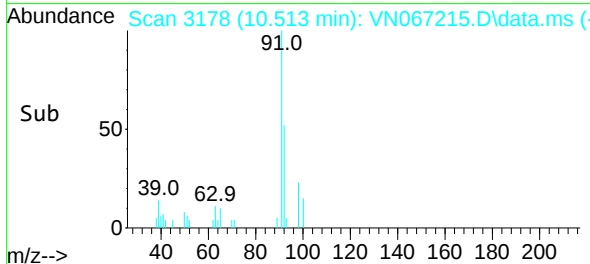

#54
cis-1,3-Dichloropropene
Concen: 4.982 ug/l
RT: 10.247 min Scan# 3079
Delta R.T. 0.054 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11

Tgt Ion: 75 Resp: 14047
Ion Ratio Lower Upper
75 100
77 0.0 25.1 37.7#
39 33.1 30.9 46.3


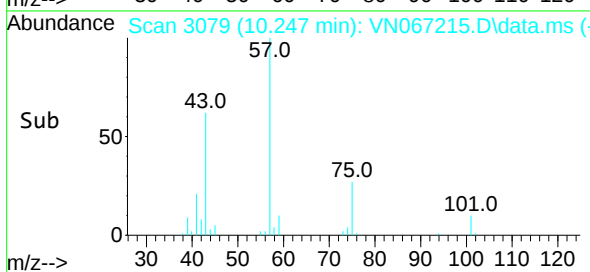

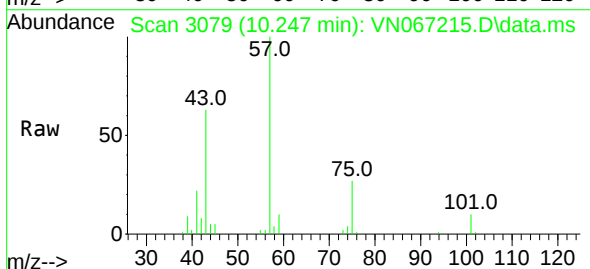




#57
1,3-Dichloropropane
Concen: 0.435 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.046 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11




Instrument :
MSVOA_N
ClientSampleId :
18-B10(4-6)


Tgt Ion: 76 Resp: 1187
Ion Ratio Lower Upper
76 100
78 0.0 26.3 39.5#



#59
2-Hexanone
Concen: 11.904 ug/l
RT: 11.098 min Scan# 3396
Delta R.T. 0.006 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11

Tgt Ion: 43 Resp: 19786
Ion Ratio Lower Upper
43 100
58 20.9 29.8 89.5#


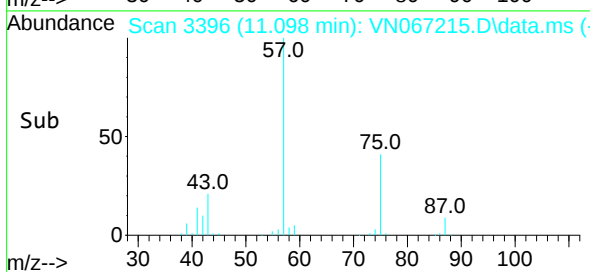




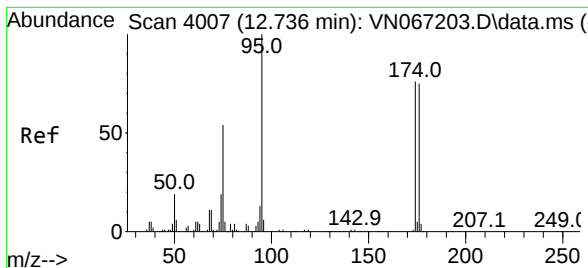

#62
4-Bromofluorobenzene
Concen: 43.928 ug/l
RT: 12.736 min Scan# 4007
Delta R.T. 0.000 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11




Instrument :
MSVOA_N
ClientSampleId :
18-B10(4-6)


Tgt Ion: 95	Resp: 98472
Ion Ratio	Lower Upper
95 100	
174 84.3	0.0 182.8
176 81.4	0.0 176.6

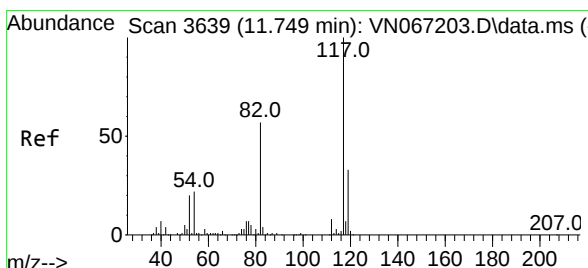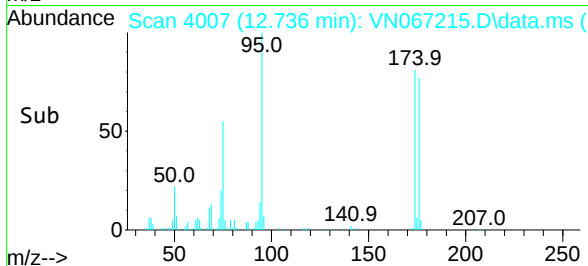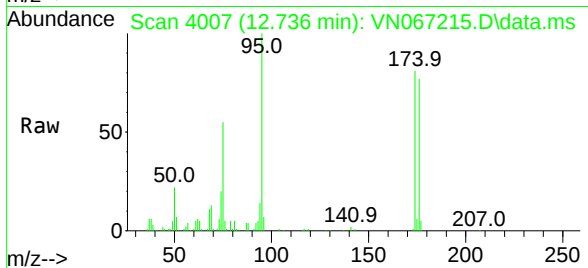

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.749 min Scan# 3639
Delta R.T. 0.000 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11

Tgt Ion: 117	Resp: 220816
Ion Ratio	Lower Upper
117 100	
82 55.7	42.2 63.2
119 31.3	25.8 38.6


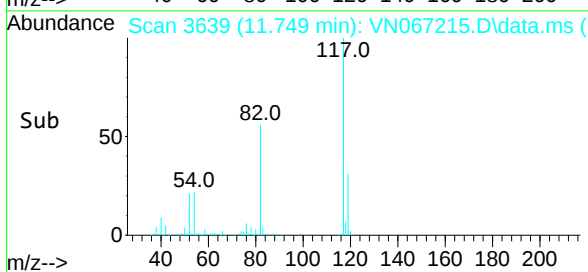

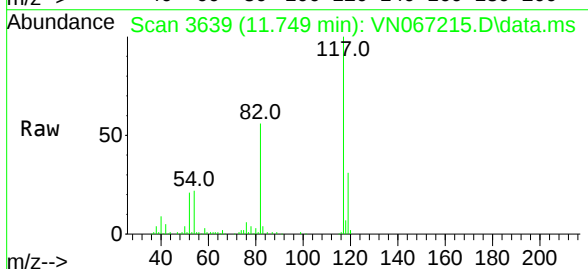




#67
Ethyl Benzene
Concen: 0.243 ug/l
RT: 11.851 min Scan# 3677
Delta R.T. 0.003 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11




Instrument :
MSVOA_N
ClientSampleId :
18-B10(4-6)


Tgt Ion: 91 Resp: 2101
Ion Ratio Lower Upper
91 100
106 31.3 26.2 39.2



#68
m/p-Xylenes
Concen: 0.744 ug/l
RT: 11.956 min Scan# 3716
Delta R.T. -0.002 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11

Tgt Ion: 106 Resp: 2528
Ion Ratio Lower Upper
106 100
91 216.4 155.2 232.8


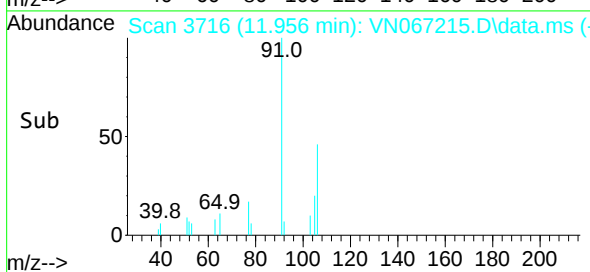






#69
o-Xylene
Concen: 0.657 ug/l
RT: 12.286 min Scan# 3839
Delta R.T. 0.000 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11




Instrument :
MSVOA_N
ClientSampleId :
18-B10(4-6)


Tgt Ion:106 Resp: 2183
Ion Ratio Lower Upper
106 100
91 214.8 102.3 306.8

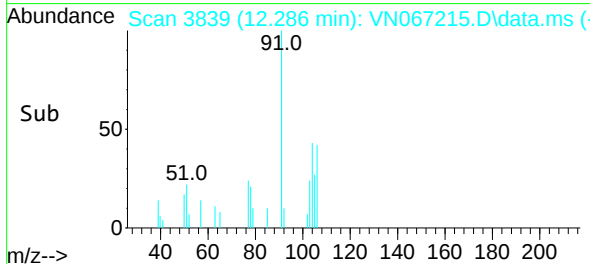

#70
Styrene
Concen: 0.637 ug/l
RT: 12.299 min Scan# 3844
Delta R.T. 0.000 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11

Tgt Ion:104 Resp: 3616
Ion Ratio Lower Upper
104 100
78 45.1 37.7 56.5
103 60.6 44.2 66.4


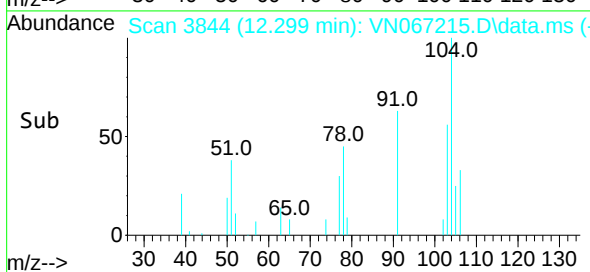

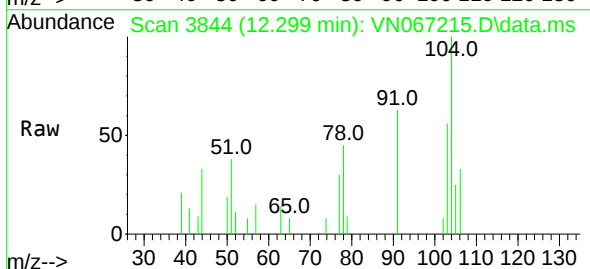




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.680 min Scan# 4359
Delta R.T. 0.000 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11




Instrument :
MSVOA_N
ClientSampleId :
18-B10(4-6)


Tgt Ion:152 Resp: 102134
Ion Ratio Lower Upper
152 100
115 58.9 27.0 80.8
150 156.3 0.0 350.2

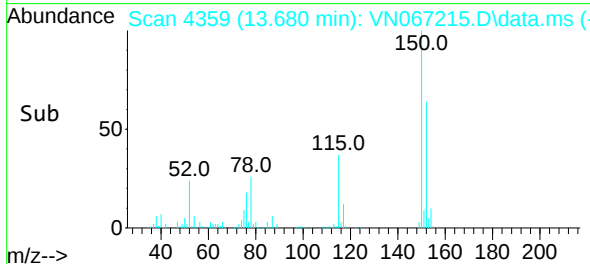

#74
N-ethyl acetate
Concen: 0.526 ug/l
RT: 12.358 min Scan# 3866
Delta R.T. -0.035 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11

Tgt Ion: 43 Resp: 1647
Ion Ratio Lower Upper
43 100
70 0.0 36.7 55.1#
55 15.8 17.6 26.4#
61 0.0 18.9 28.3#


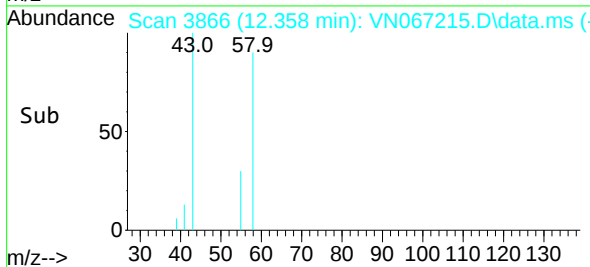

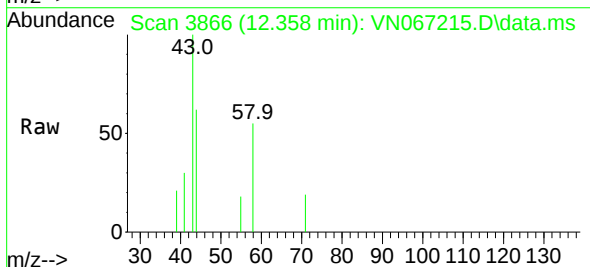




#76
1,2,3-Trichloropropane
Concen: 28.284 ug/l
RT: 12.736 min Scan# 4007
Delta R.T. -0.150 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11




Instrument :
MSVOA_N
ClientSampleId :
18-B10(4-6)


Tgt Ion: 75 Resp: 55553
Ion Ratio Lower Upper
75 100
77 0.7 0.0 0.0#

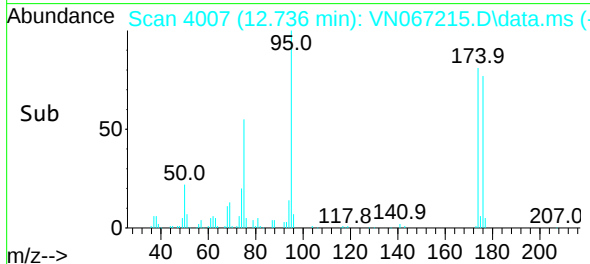

#80
1,3,5-Trimethylbenzene
Concen: 0.335 ug/l
RT: 13.063 min Scan# 4129
Delta R.T. 0.000 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11

Tgt Ion:105 Resp: 2256
Ion Ratio Lower Upper
105 100
120 51.2 25.0 75.0


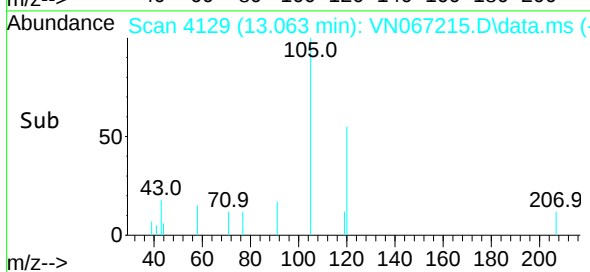






#81
trans-1,4-Dichloro-2-butene
Concen: 69.203 ug/l
RT: 12.736 min Scan# 4007
Delta R.T. 0.105 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11




Instrument :
MSVOA_N
ClientSampleId :
18-B10(4-6)


Tgt Ion: 75 Resp: 55553
Ion Ratio Lower Upper
75 100
53 0.0 66.3 99.5#
89 0.0 39.5 59.3#

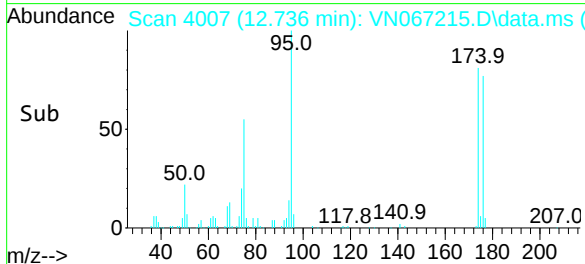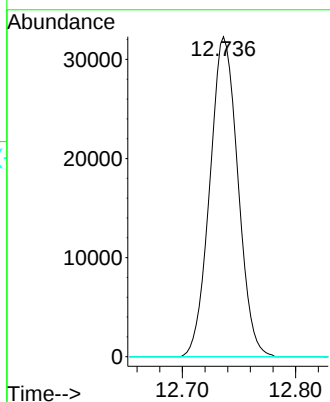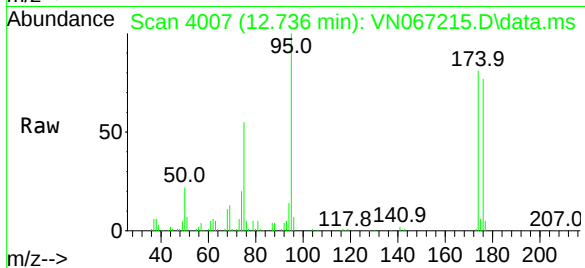

#84
1,2,4-Trimethylbenzene
Concen: 0.716 ug/l
RT: 13.369 min Scan# 4243
Delta R.T. -0.003 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11

Tgt Ion: 105 Resp: 4792
Ion Ratio Lower Upper
105 100
120 33.5 23.8 71.2

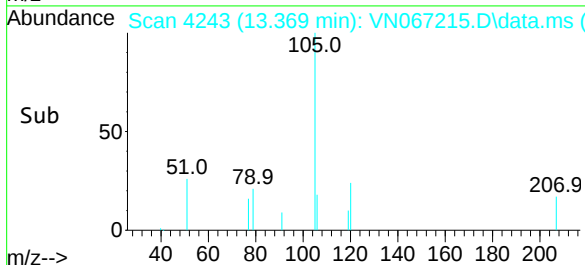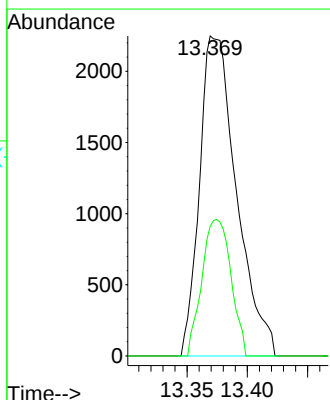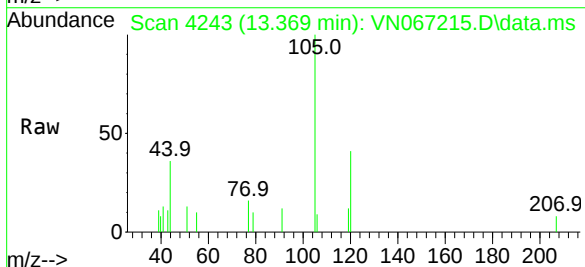



#88

1,4-Dichlorobenzene

Concen: 0.245 ug/l

RT: 13.702 min Scan# 4367

Delta R.T. 0.003 min

Lab File: VN067215.D

Acq: 4 Jun 2021 23:11





Tgt Ion:146 Resp: 836

Ion Ratio Lower Upper

146 100

111 0.0 18.5 55.5#

148 77.4 31.4 94.3

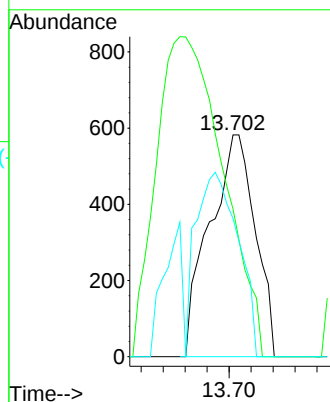

#90

Hexachloroethane

Concen: 0.684 ug/l

RT: 14.329 min Scan# 4601

Delta R.T. 0.113 min

Lab File: VN067215.D




Acq: 4 Jun 2021 23:11


Tgt Ion:117 Resp: 833

Ion Ratio Lower Upper

117 100


201 0.0 45.5 136.5#

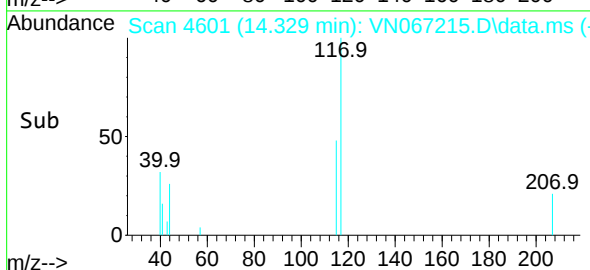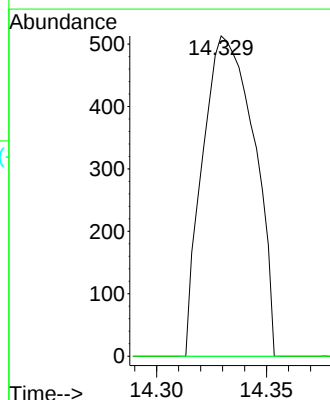

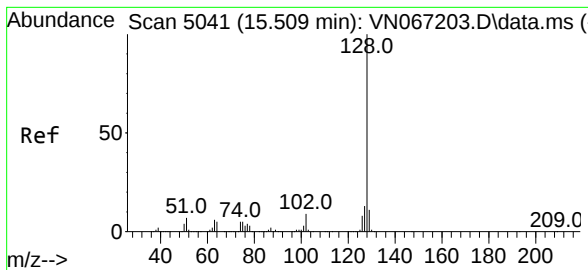

#95
Naphthalene
Concen: 9.174 ug/l
RT: 15.512 min Scan# 5042
Delta R.T. 0.003 min
Lab File: VN067215.D
Acq: 4 Jun 2021 23:11

Instrument :
MSVOA_N
ClientSampleId :
18-B10(4-6)

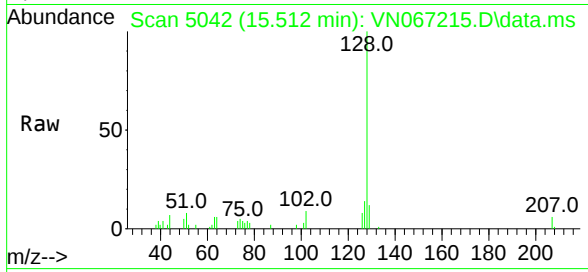

Tgt Ion:	128	Resp:	23663
Ion Ratio	Lower	Upper	
128	100		
127	13.1	10.2	15.2
129	10.6	8.6	13.0

