
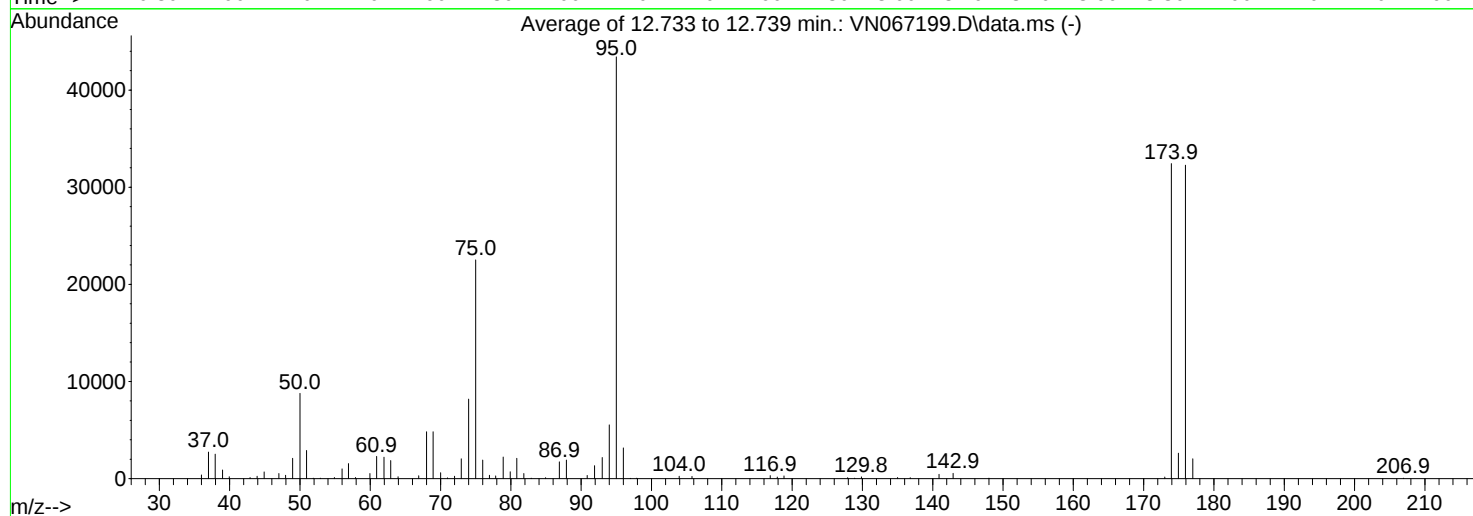


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060421\
Data File : VN067199.D
Acq On : 4 Jun 2021 16:02
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060421W.M
Title : SW846 8260
Last Update : Fri Jun 04 19:00:20 2021

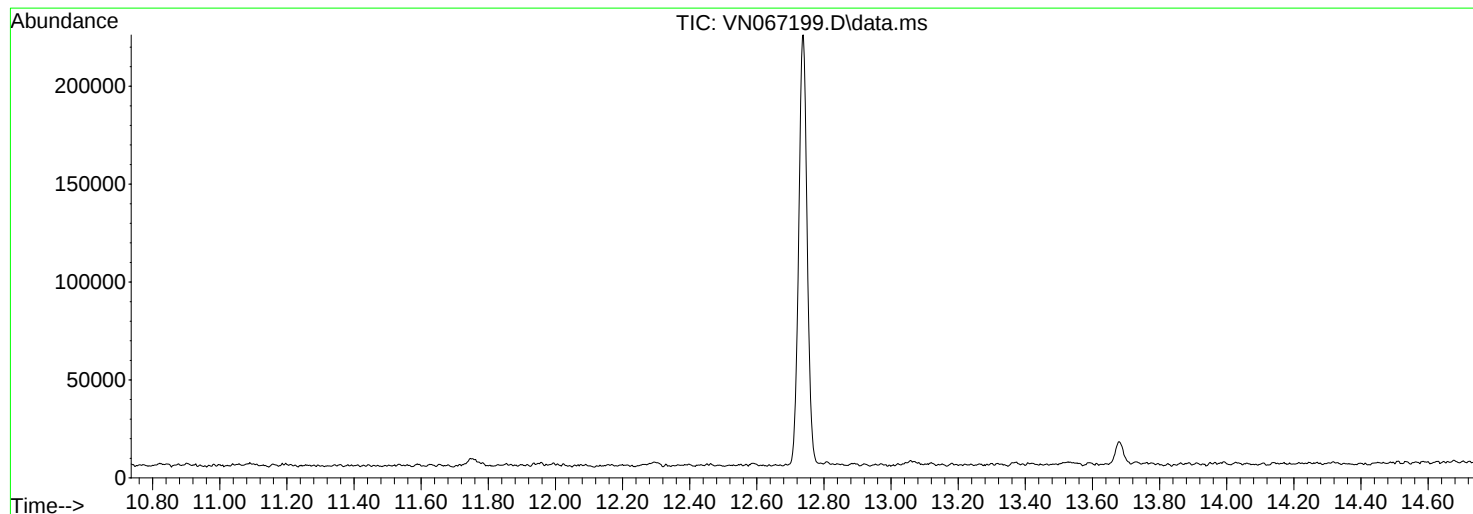

AutoFind: Scans 4006, 4007, 4008; Background Corrected with Scan 3985

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	8778	PASS
75	95	30	60	51.9	22523	PASS
95	95	100	100	100.0	43421	PASS
96	95	5	9	7.3	3170	PASS
173	174	0.00	2	0.5	164	PASS
174	95	50	100	74.7	32440	PASS
175	174	5	9	8.1	2612	PASS
176	174	95	101	99.5	32275	PASS
177	176	5	9	6.3	2047	PASS