

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060424\
 Data File : VN082452.D
 Acq On : 04 Jun 2024 10:59
 Operator : JC\MD
 Sample : VN0604MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0604MBL01

Quant Time: Jun 05 03:17:53 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 16 05:21:06 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	155032	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	278612	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	264536	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	112638	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	131558	53.741	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	107.480%
35) Dibromofluoromethane	8.165	113	93479	54.542	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	109.080%
50) Toluene-d8	10.571	98	357032	54.335	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	108.680%
62) 4-Bromofluorobenzene	12.853	95	121065	51.620	ug/l	0.00
Spiked Amount	50.000	Range	64 - 133	Recovery	=	103.240%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060424\
Data File : VN082452.D
Acq On : 04 Jun 2024 10:59
Operator : JC\MD
Sample : VN0604MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0604MBL01

Quant Time: Jun 05 03:17:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Quant Title : SW846 8260
QLast Update : Thu May 16 05:21:06 2024
Response via : Initial Calibration




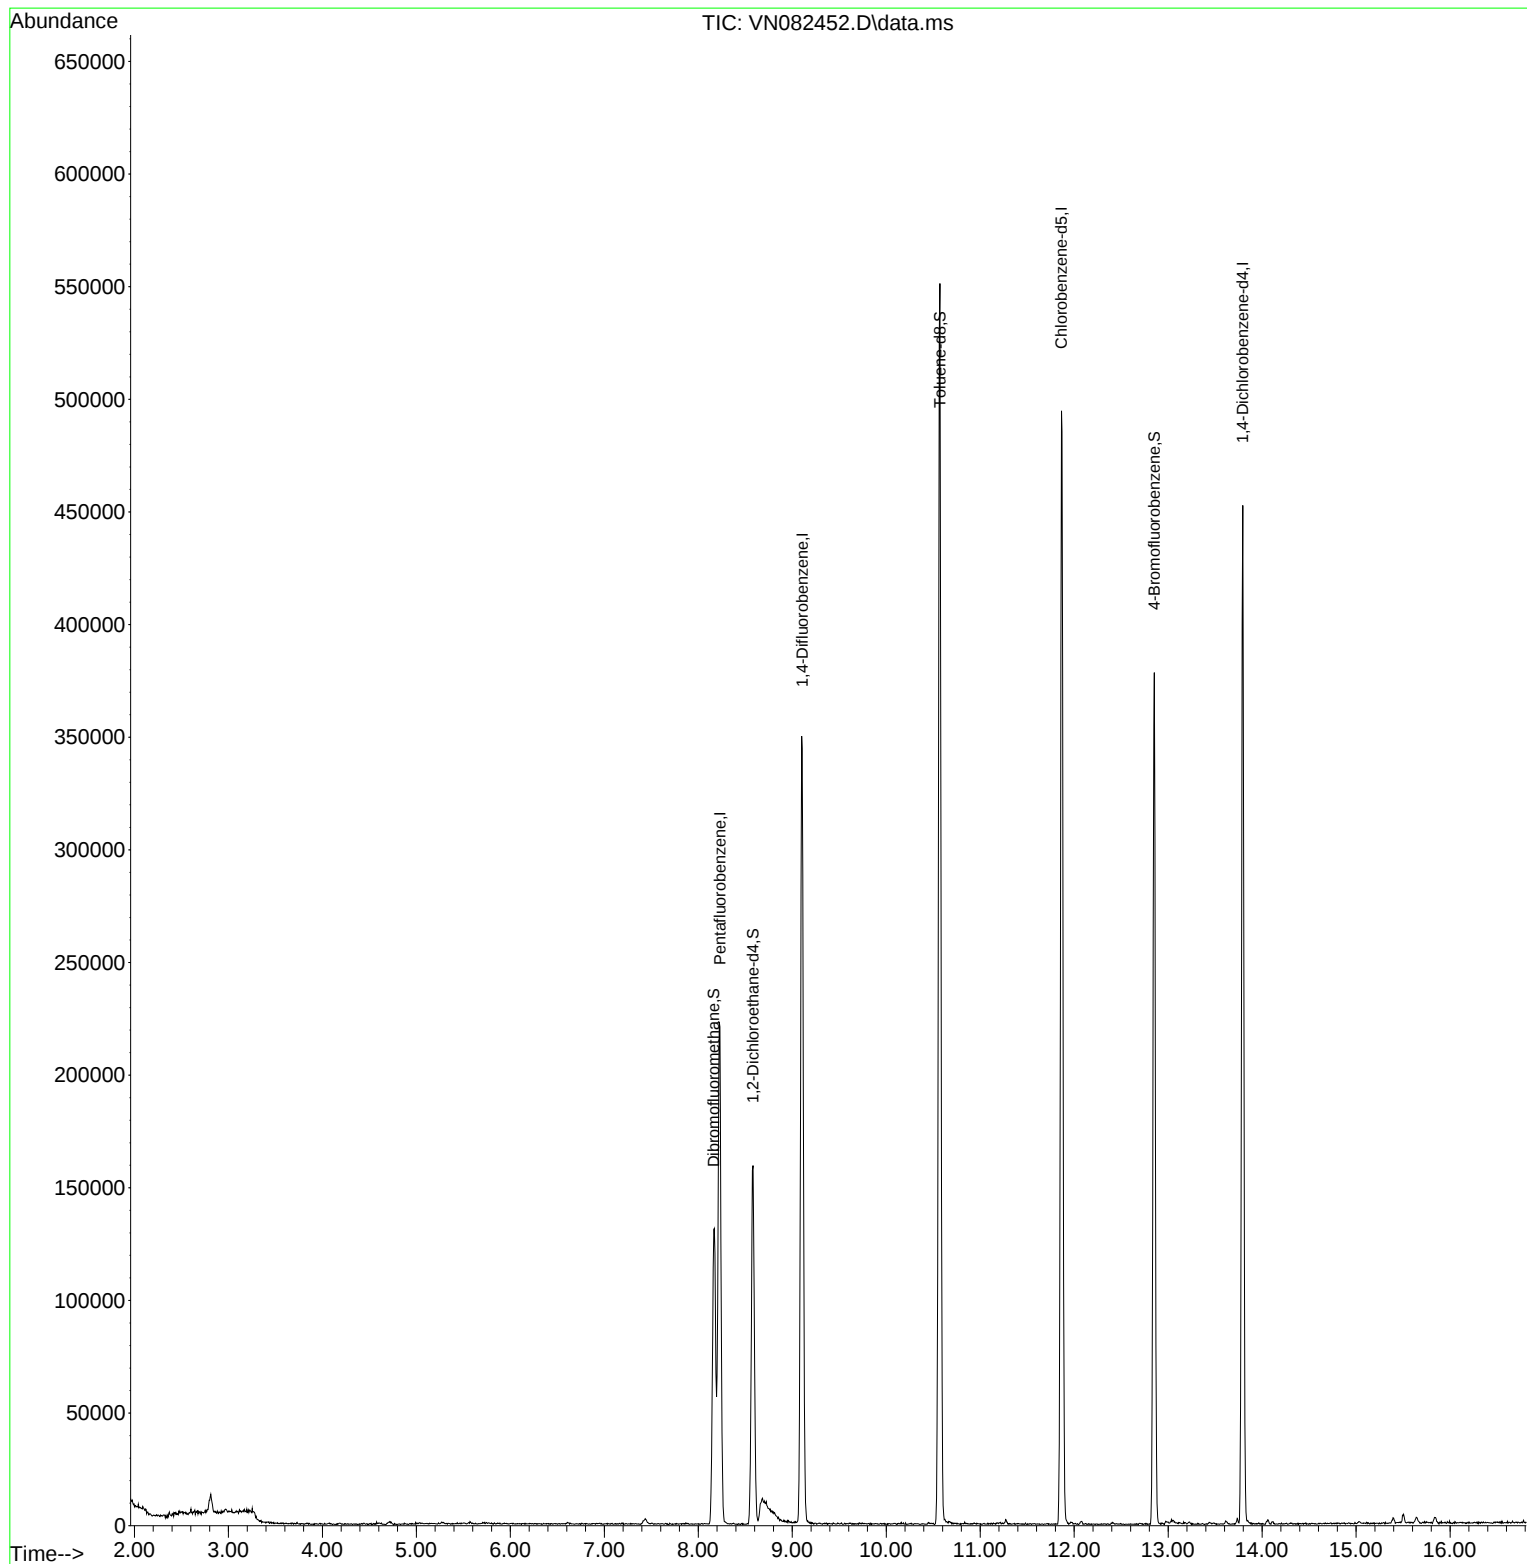


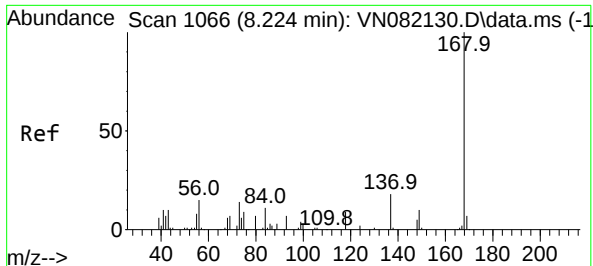

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1066
Delta R.T. 0.006 min
Lab File: VN082452.D
Acq: 04 Jun 2024 10:59




Instrument :
MSVOA_N
ClientSampleId :
VN0604MBL01


Tgt Ion:168 Resp: 155032
Ion Ratio Lower Upper
168 100
99 60.4 48.2 72.4

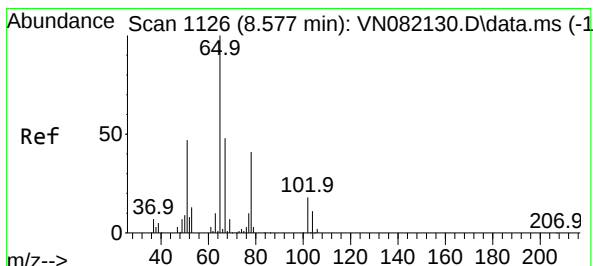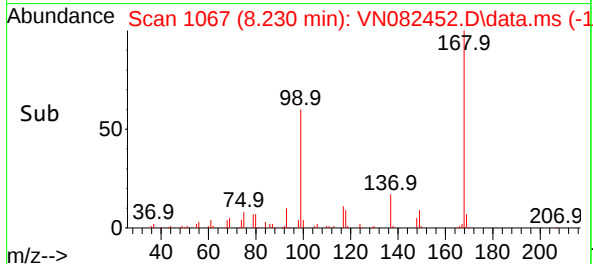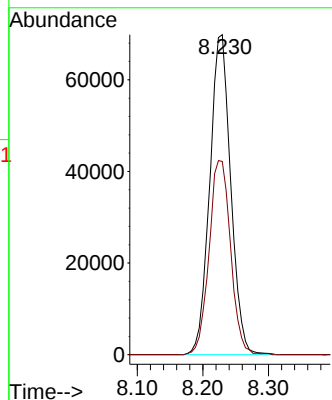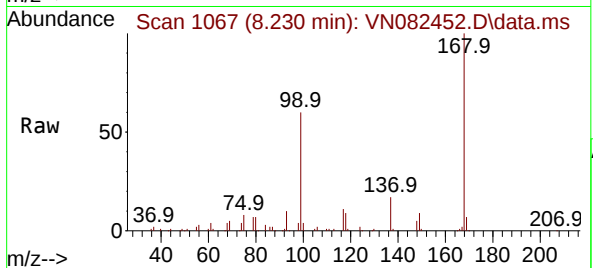

#33
1,2-Dichloroethane-d4
Concen: 53.741 ug/l
RT: 8.583 min Scan# 1127
Delta R.T. 0.006 min
Lab File: VN082452.D
Acq: 04 Jun 2024 10:59

Tgt Ion: 65 Resp: 131558
Ion Ratio Lower Upper
65 100
67 51.3 0.0 103.0


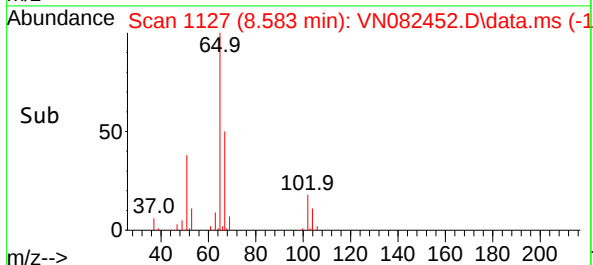
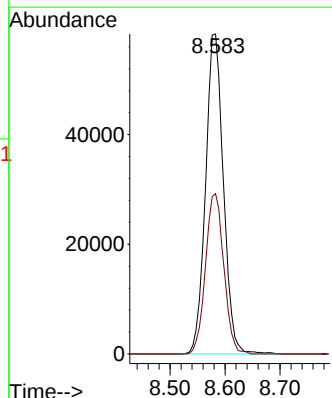
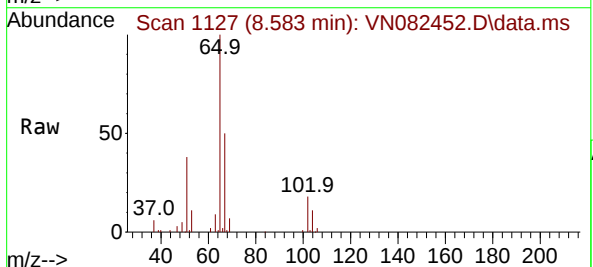


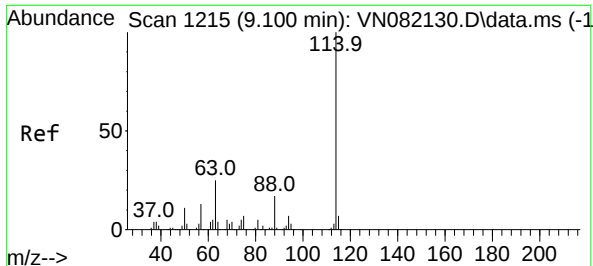

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN082452.D
Acq: 04 Jun 2024 10:59




Instrument :
MSVOA_N
ClientSampleId :
VN0604MBL01


Tgt Ion:114 Resp: 278612
Ion Ratio Lower Upper
114 100
63 22.8 0.0 41.0
88 16.5 0.0 31.4

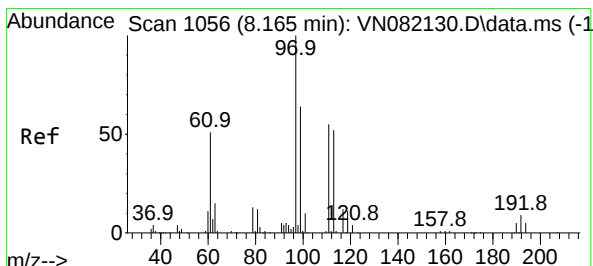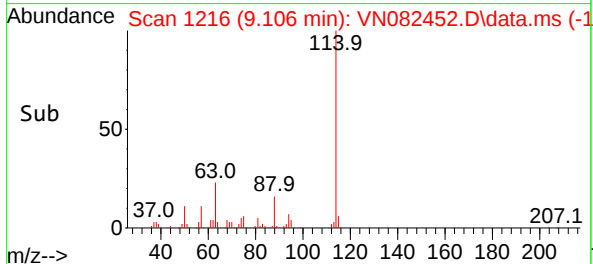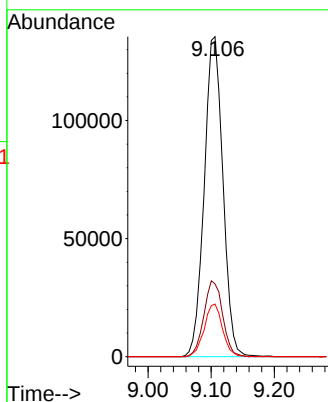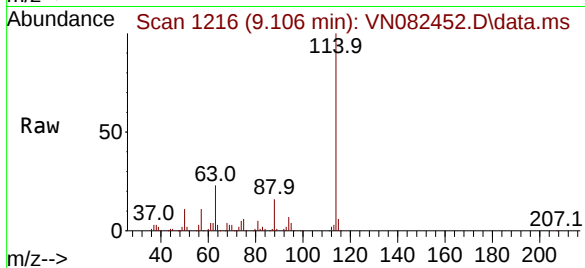

#35
Dibromofluoromethane
Concen: 54.542 ug/l
RT: 8.165 min Scan# 1056
Delta R.T. 0.000 min
Lab File: VN082452.D
Acq: 04 Jun 2024 10:59

Tgt Ion:113 Resp: 93479
Ion Ratio Lower Upper
113 100
111 104.6 83.4 125.2
192 17.9 14.0 21.0


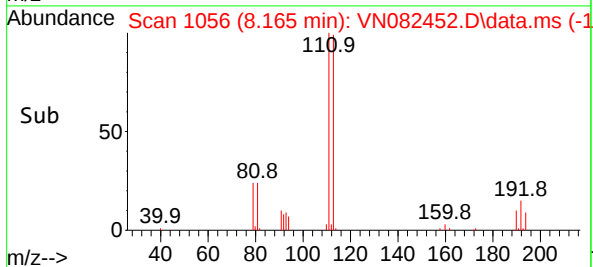
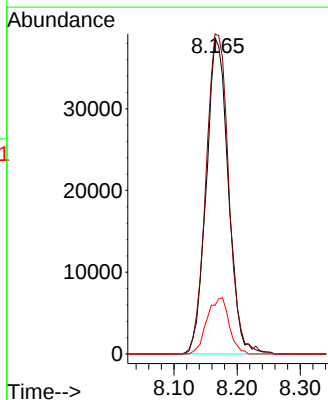
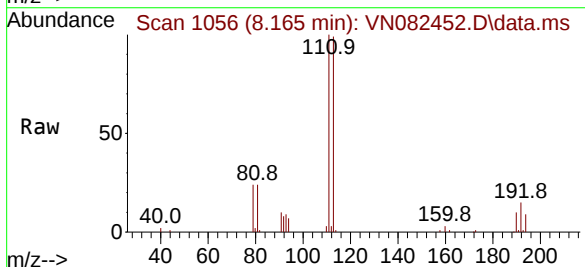


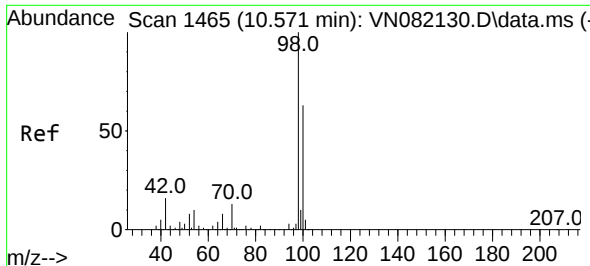

#50
Toluene-d8
Concen: 54.335 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.000 min
Lab File: VN082452.D
Acq: 04 Jun 2024 10:59




Instrument :
MSVOA_N
ClientSampleId :
VN0604MBL01


Tgt Ion: 98 Resp: 357032
Ion Ratio Lower Upper
98 100
100 64.5 51.8 77.6

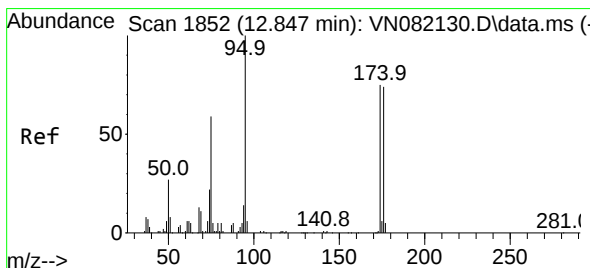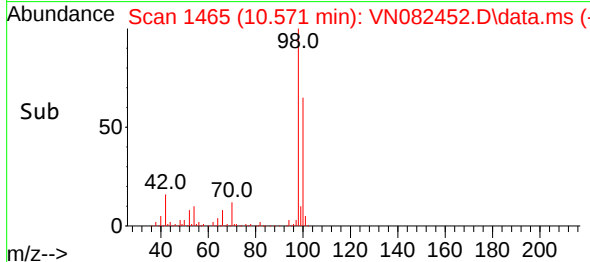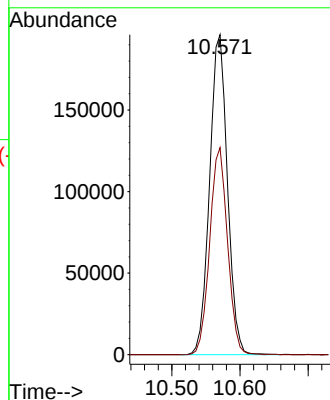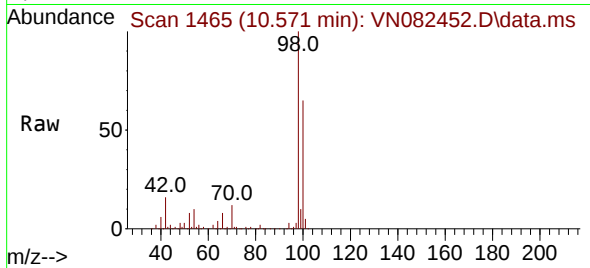

#62
4-Bromofluorobenzene
Concen: 51.620 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.006 min
Lab File: VN082452.D
Acq: 04 Jun 2024 10:59

Tgt Ion: 95 Resp: 121065
Ion Ratio Lower Upper
95 100
174 76.2 0.0 160.6
176 73.5 0.0 152.8

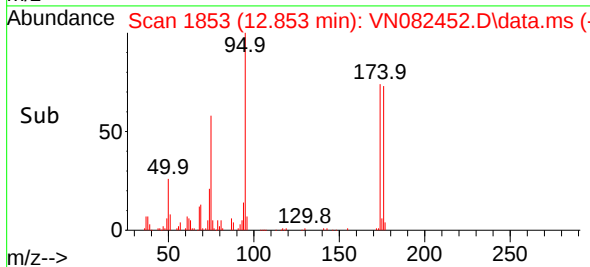
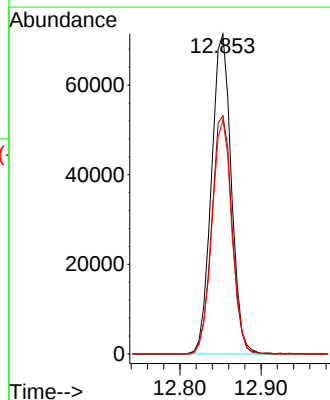
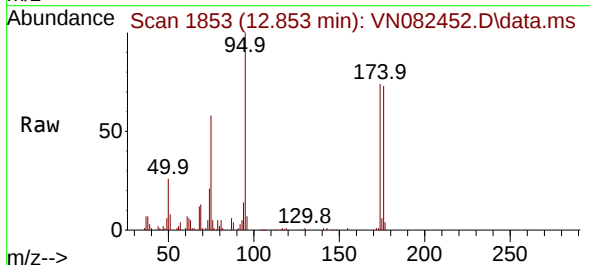


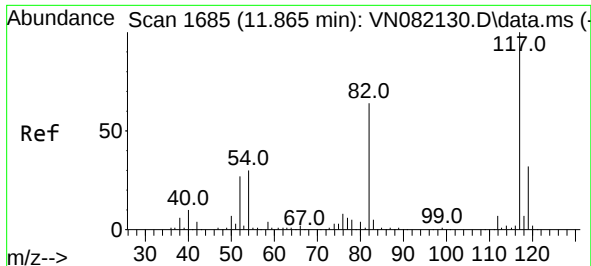

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN082452.D
Acq: 04 Jun 2024 10:59

Instrument :
MSVOA_N
ClientSampleId :
VN0604MBL01

Tgt Ion:117 Resp: 264536
Ion Ratio Lower Upper
117 100
82 60.4 44.6 66.8
119 33.1 25.9 38.9

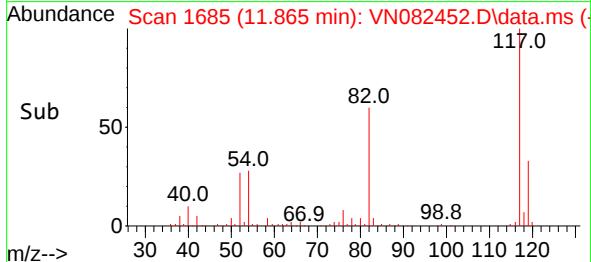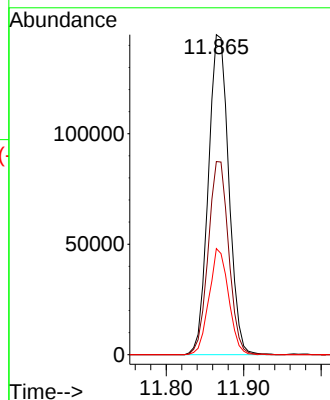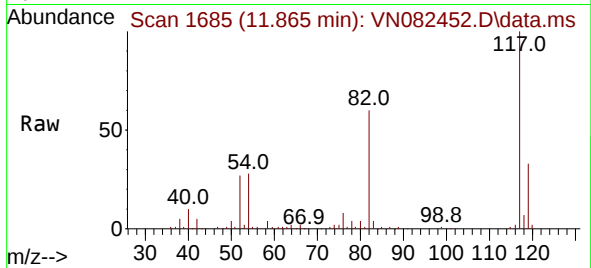

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. 0.000 min
Lab File: VN082452.D
Acq: 04 Jun 2024 10:59

Tgt Ion:152 Resp: 112638
Ion Ratio Lower Upper
152 100
115 60.0 30.4 91.3
150 156.1 0.0 353.2

