
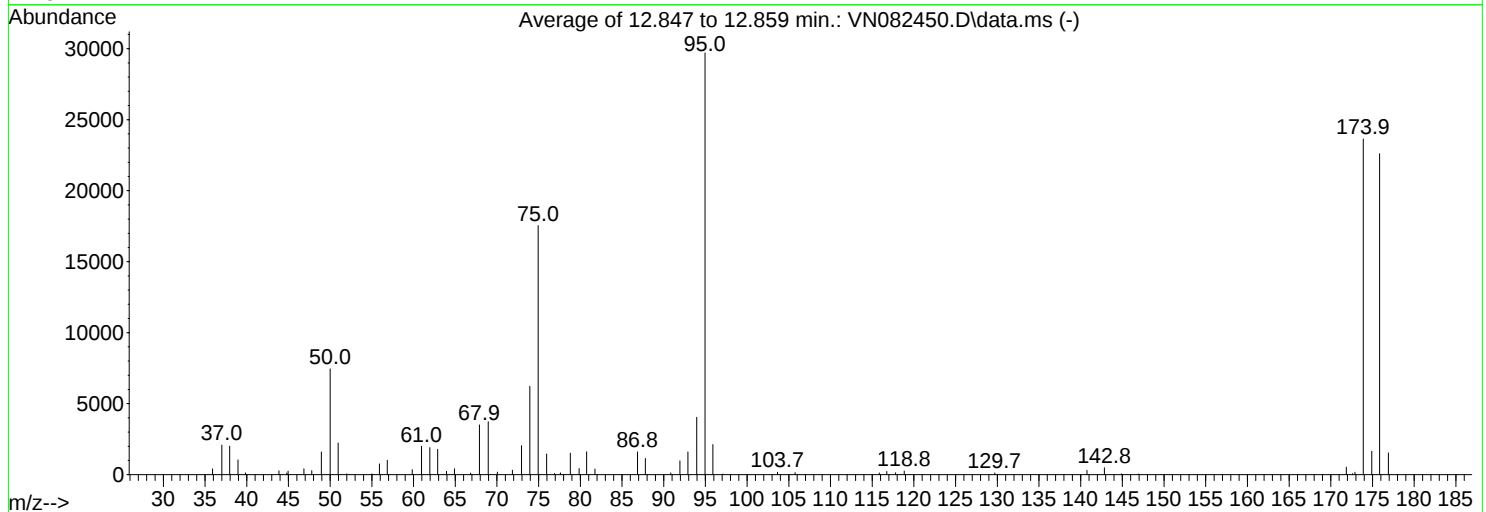


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060424\
Data File : VN082450.D
Acq On : 04 Jun 2024 09:16
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Title : SW846 8260
Last Update : Thu May 16 05:21:06 2024

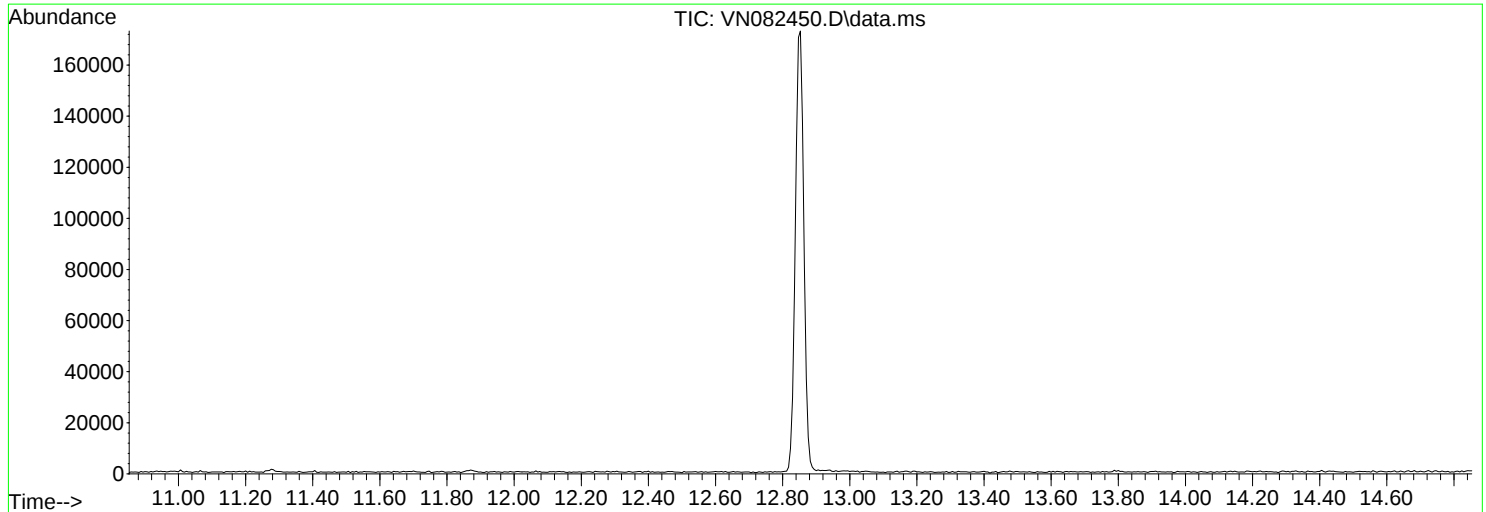

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.1	7451	PASS
75	95	30	60	59.1	17549	PASS
95	95	100	100	100.0	29709	PASS
96	95	5	9	7.1	2124	PASS
173	174	0.00	2	0.7	169	PASS
174	95	50	100	79.6	23645	PASS
175	174	5	9	6.9	1643	PASS
176	174	95	101	95.6	22608	PASS
177	176	5	9	6.8	1535	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	404	50.00	7451	64.90	416	77.60	124
37.00	2090	50.95	2233	66.85	115	78.80	150
37.95	2005	52.00	60	67.90	3509	79.85	42
38.95	1035	55.00	55	68.95	3726	80.75	161
39.85	125	55.90	760	70.05	176	81.75	394
43.85	267	56.85	1011	71.85	316	86.85	1596
44.80	109	59.85	347	72.95	2039	87.80	1136
44.95	243	60.95	1991	73.95	6223	90.85	124
46.85	422	61.95	1906	74.95	17549	91.95	969
47.80	279	62.90	1784	75.95	1453	92.90	1601
48.95	1602	63.95	239	76.90	82	93.95	4036

Average of 12.847 to 12.859 min.: VN082450.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.95	29709	142.85	482				
95.90	2124	144.90	54				
97.10	50	146.90	50				
103.65	171	171.85	528				
105.75	146	172.60	68				
115.85	125	172.90	169				
116.75	229	173.90	23645				
117.80	130	174.90	1643				
118.85	262	175.85	22608				
129.70	125	176.90	1535				
140.75	310						

Instrument :

MSVOA_N

ClientSampleId :

BFB