


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN060519\
 Data File : VN055994.D
 Acq On : 5 Jun 2019 8:30
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N060419W.M
 Title : SW846 8260
 Last Update : Tue Jun 04 11:02:09 2019

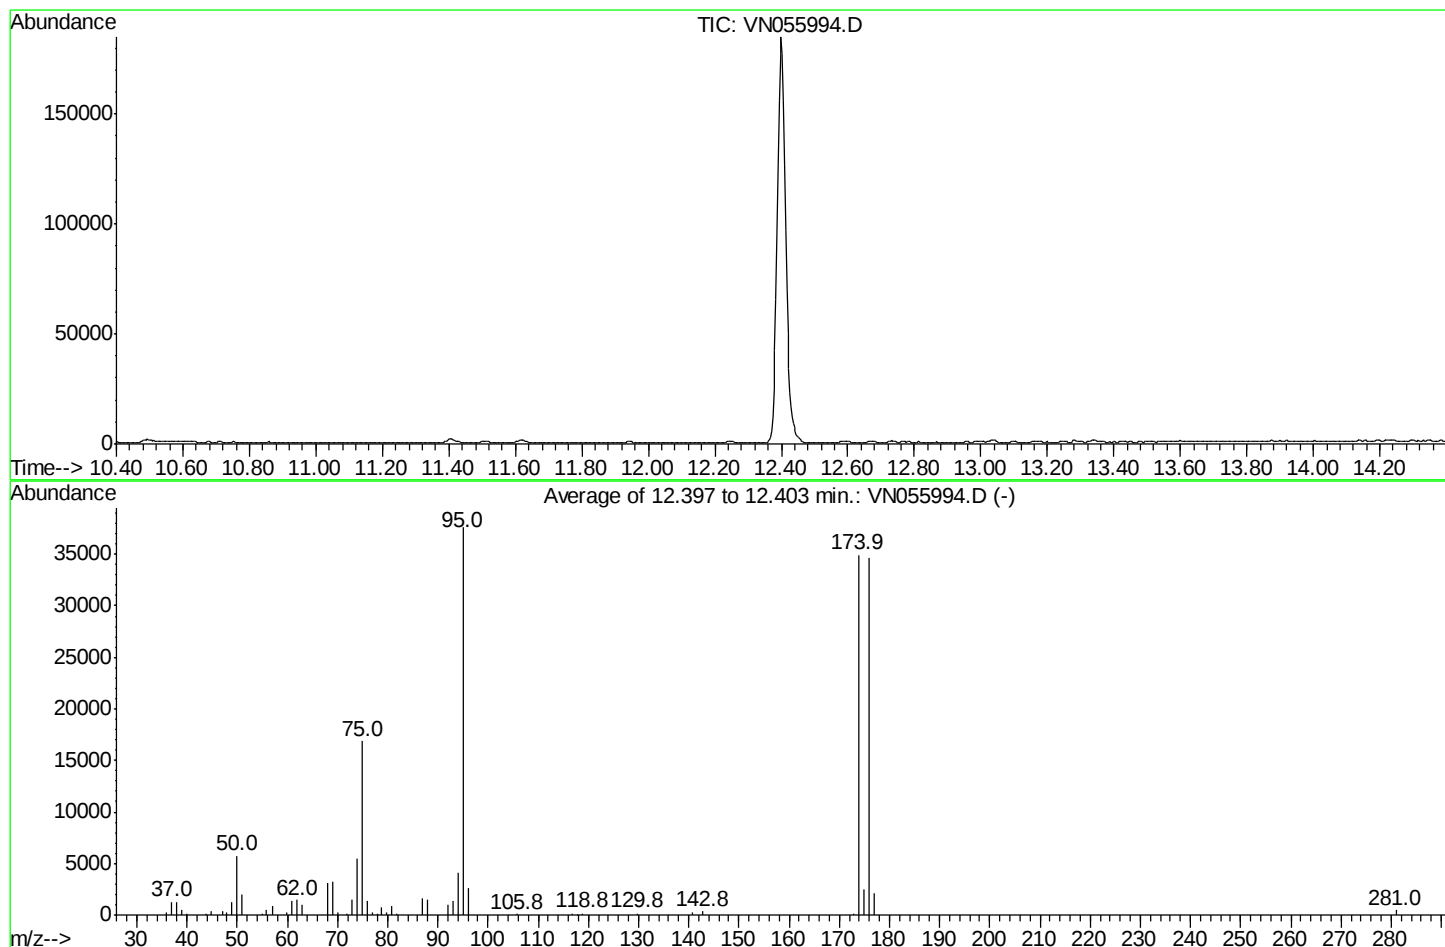

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	5730	PASS
75	95	30	60	44.8	16869	PASS
95	95	100	100	100.0	37616	PASS
96	95	5	9	7.0	2628	PASS
173	174	0.00	2	0.4	136	PASS
174	95	50	100	92.9	34930	PASS
175	174	5	9	7.2	2514	PASS
176	174	95	101	99.1	34629	PASS
177	176	5	9	6.3	2165	PASS