
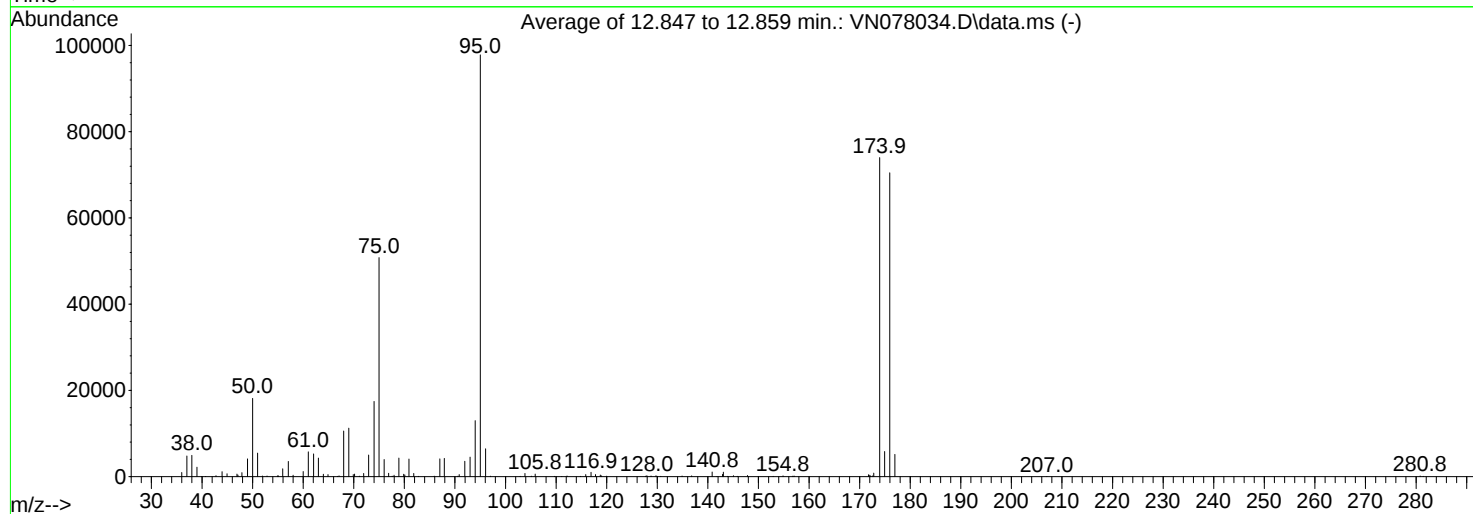


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060523\
Data File : VN078034.D
Acq On : 05 Jun 2023 10:38
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
Title : SW846 8260
Last Update : Tue May 16 04:07:42 2023

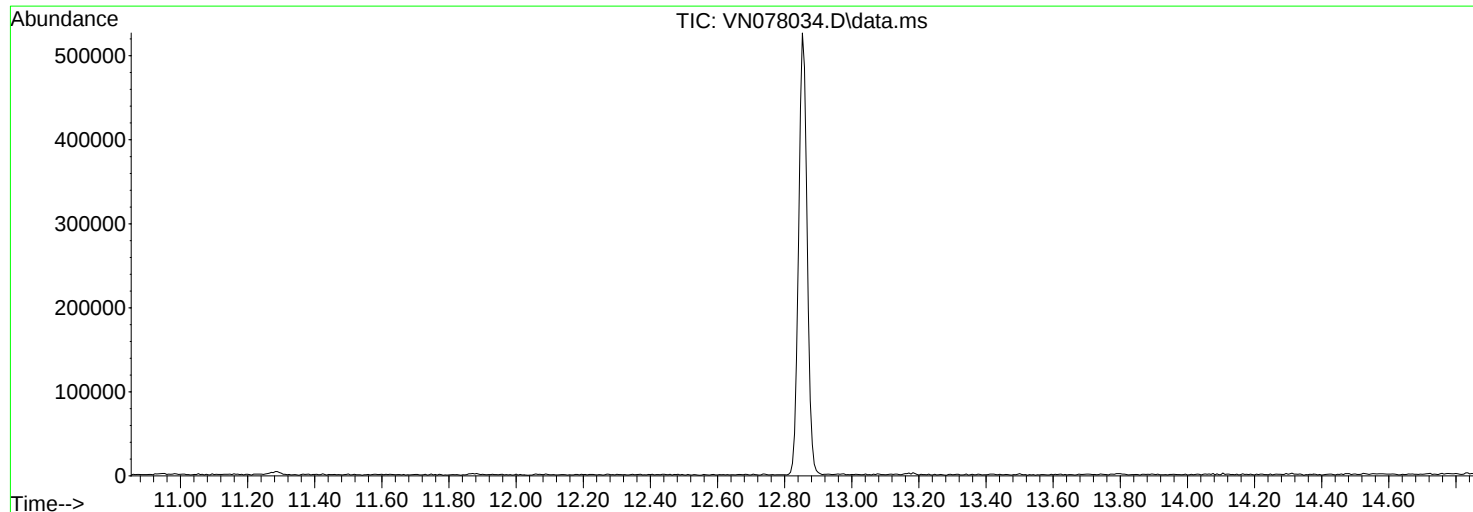

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.6	18152	PASS
75	95	30	60	51.9	50792	PASS
95	95	100	100	100.0	97819	PASS
96	95	5	9	6.6	6473	PASS
173	174	0.00	2	1.1	803	PASS
174	95	50	100	75.6	73973	PASS
175	174	5	9	7.9	5844	PASS
176	174	95	101	95.2	70451	PASS
177	176	5	9	7.3	5161	PASS

Average of 12.847 to 12.859 min.: VN078034.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	980	47.90	927	60.00	1176	70.15	611
37.00	4796	49.00	4136	61.00	5737	71.10	111
38.00	4949	50.00	18152	62.05	5260	71.95	76
39.00	2181	51.00	5448	63.00	4316	72.95	499
39.95	22	51.95	168	64.00	569	74.00	17440
40.70	55	52.85	150	64.90	492	75.00	50792
42.75	225	54.90	174	66.80	74	76.00	3966
43.95	1168	55.10	185	67.10	186	76.90	791
44.95	672	55.95	1836	68.00	10594	77.60	105
46.90	588	57.05	3513	69.00	11247	77.95	323
47.10	368	58.00	336	69.90	482	78.90	4306

Average of 12.847 to 12.859 min.: VN078034.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.85	564	93.00	4513	112.15	139	129.75	227
80.10	426	94.00	13005	114.80	67	130.00	95
80.90	4098	95.00	97819	115.85	485	130.70	85
81.85	745	96.05	6473	116.90	998	134.90	141
82.80	69	97.00	123	117.80	487	136.80	175
85.90	114	102.90	63	118.75	361	140.85	1081
87.00	4132	103.85	745	119.00	204	141.80	56
87.90	4244	105.10	121	120.00	114	142.90	513
90.60	130	105.85	603	127.70	131	143.05	1045
90.85	478	109.70	77	127.95	234	143.90	82
91.95	3553	111.10	53	128.75	171	145.05	210

Average of 12.847 to 12.859 min.: VN078034.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
145.80	72	173.95	73973				
147.85	257	174.95	5844				
152.90	83	175.95	70451				
154.85	186	176.95	5161				
156.80	131	207.00	51				
157.05	166	280.80	149				
171.75	444	281.40	61				
172.00	336						
172.20	151						
172.60	203						
172.80	803						