
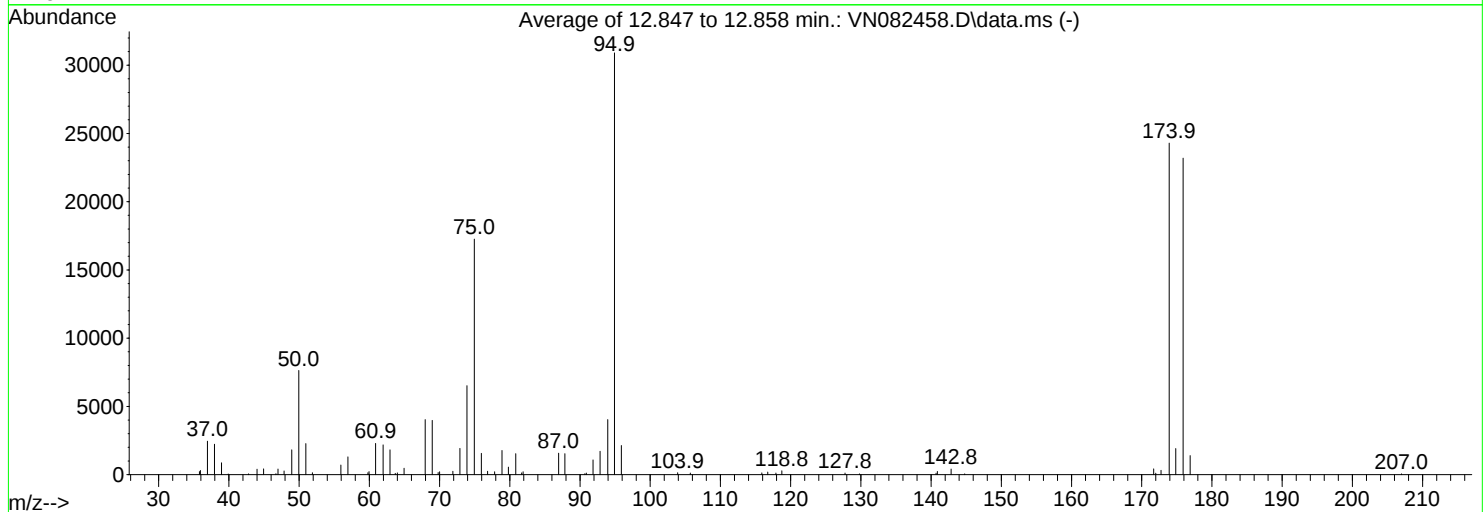


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060524\
Data File : VN082458.D
Acq On : 05 Jun 2024 08:37
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Title : SW846 8260
Last Update : Thu May 16 05:21:06 2024

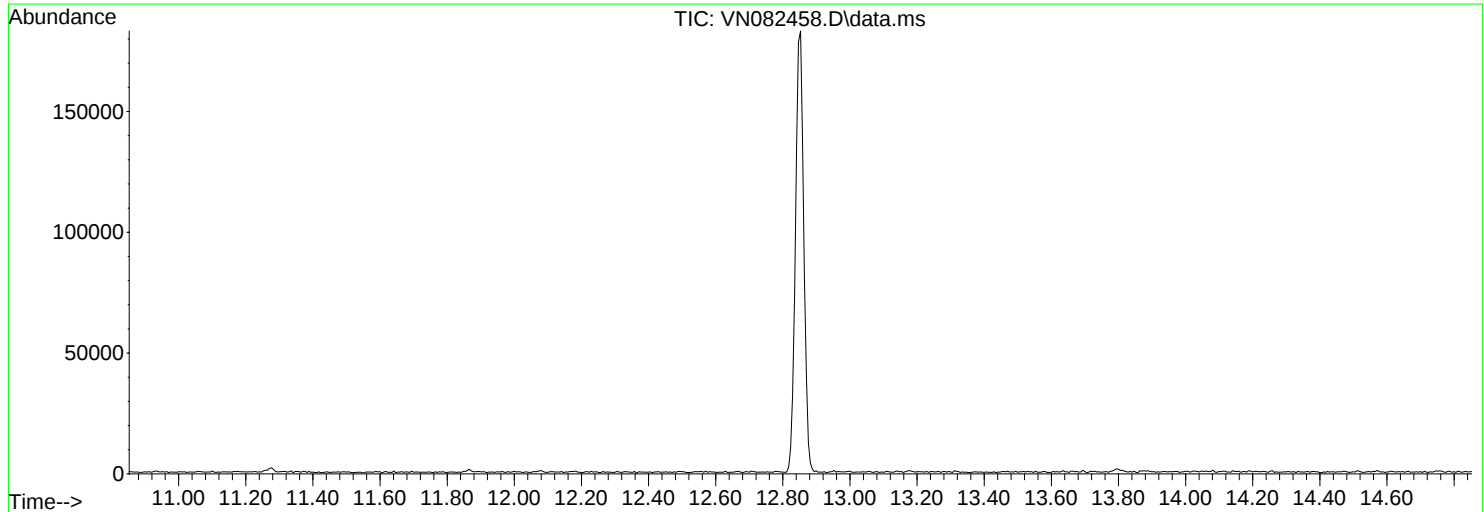

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.7	7638	PASS
75	95	30	60	55.9	17263	PASS
95	95	100	100	100.0	30907	PASS
96	95	5	9	6.9	2139	PASS
173	174	0.00	2	1.3	321	PASS
174	95	50	100	78.6	24293	PASS
175	174	5	9	7.9	1912	PASS
176	174	95	101	95.5	23195	PASS
177	176	5	9	6.0	1401	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	218	47.85	271	62.95	1823	74.95	1726
35.95	308	48.95	1822	63.70	93	75.95	155
36.95	2446	49.95	7638	64.00	132	76.85	24
37.95	2225	50.95	2279	64.95	471	77.85	21
38.95	865	51.90	142	67.95	4029	78.90	1765
39.90	45	55.95	704	68.95	3971	79.80	554
42.80	56	56.95	1305	69.80	158	80.85	1536
44.00	396	59.80	141	70.00	207	81.70	124
44.95	420	59.95	224	71.90	241	81.90	208
46.70	72	60.90	2291	72.90	1918	86.95	1566
47.00	413	61.95	2180	73.90	6517	87.85	1531

Average of 12.847 to 12.858 min.: VN082458.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.70	67	117.90	119	173.90	24293		
90.90	121	118.75	278	174.85	1912		
91.85	1076	127.75	120	175.90	23195		
92.85	1709	129.80	62	176.90	1401		
93.95	4031	140.70	101	207.00	58		
94.90	30907	140.90	239				
95.90	2139	142.85	414				
103.90	144	144.80	55				
105.70	120	171.70	419				
115.90	130	172.00	105				
116.75	192	172.75	321				

Instrument :

MSVOA_N

ClientSampleId :

BFB