


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN060619\
 Data File : VN056014.D
 Acq On : 5 Jun 2019 18:03
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N060619W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Thu Jun 06 04:02:53 2019

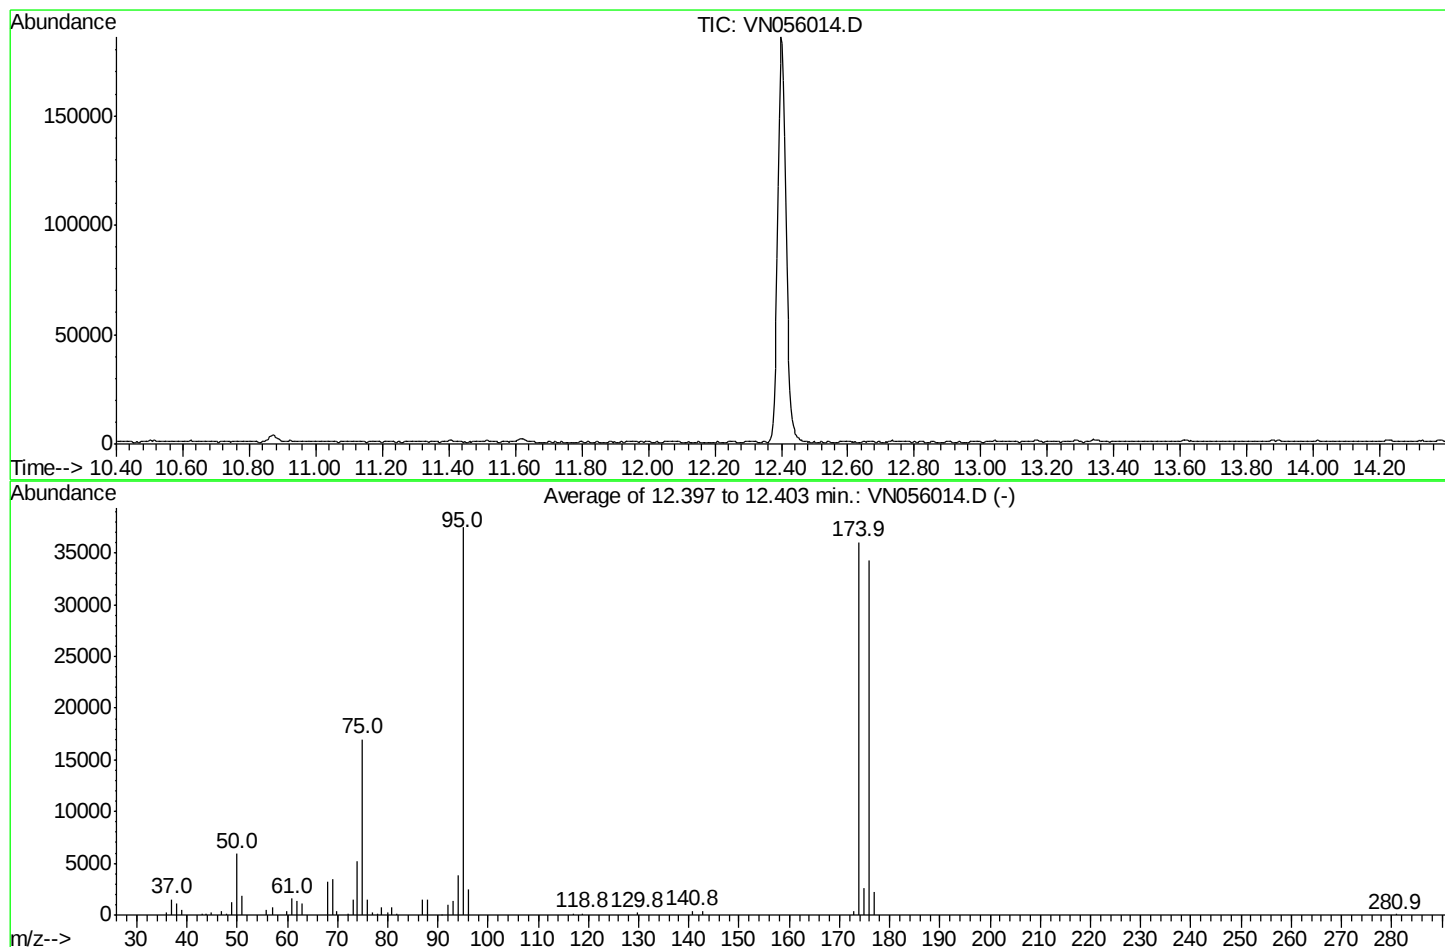

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	5916	PASS
75	95	30	60	45.3	16989	PASS
95	95	100	100	100.0	37493	PASS
96	95	5	9	6.5	2455	PASS
173	174	0.00	2	0.9	338	PASS
174	95	50	100	96.1	36026	PASS
175	174	5	9	7.4	2651	PASS
176	174	95	101	95.1	34253	PASS
177	176	5	9	6.4	2200	PASS