

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060622\
 Data File : VN072666.D
 Acq On : 06 Jun 2022 16:24
 Operator : JC\MD
 Sample : VN0606WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0606WBL01

Quant Time: Jun 07 06:27:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N060622W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Mon Jun 06 14:10:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	7.651	128	41549	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	8.963	114	255057	30.000	ug/l	0.00
57) Chlorobenzene-d5	11.739	117	218149	30.000	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.434	65	148043	31.242	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	104.133%
60) 4-Bromofluorobenzene	12.733	95	113379	25.269	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	84.233%
63) Toluene-d8	10.439	98	371737	30.762	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	102.533%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060622\
Data File : VN072666.D
Acq On : 06 Jun 2022 16:24
Operator : JC\MD
Sample : VN0606WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0606WBL01

Quant Time: Jun 07 06:27:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N060622W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Mon Jun 06 14:10:15 2022
Response via : Initial Calibration




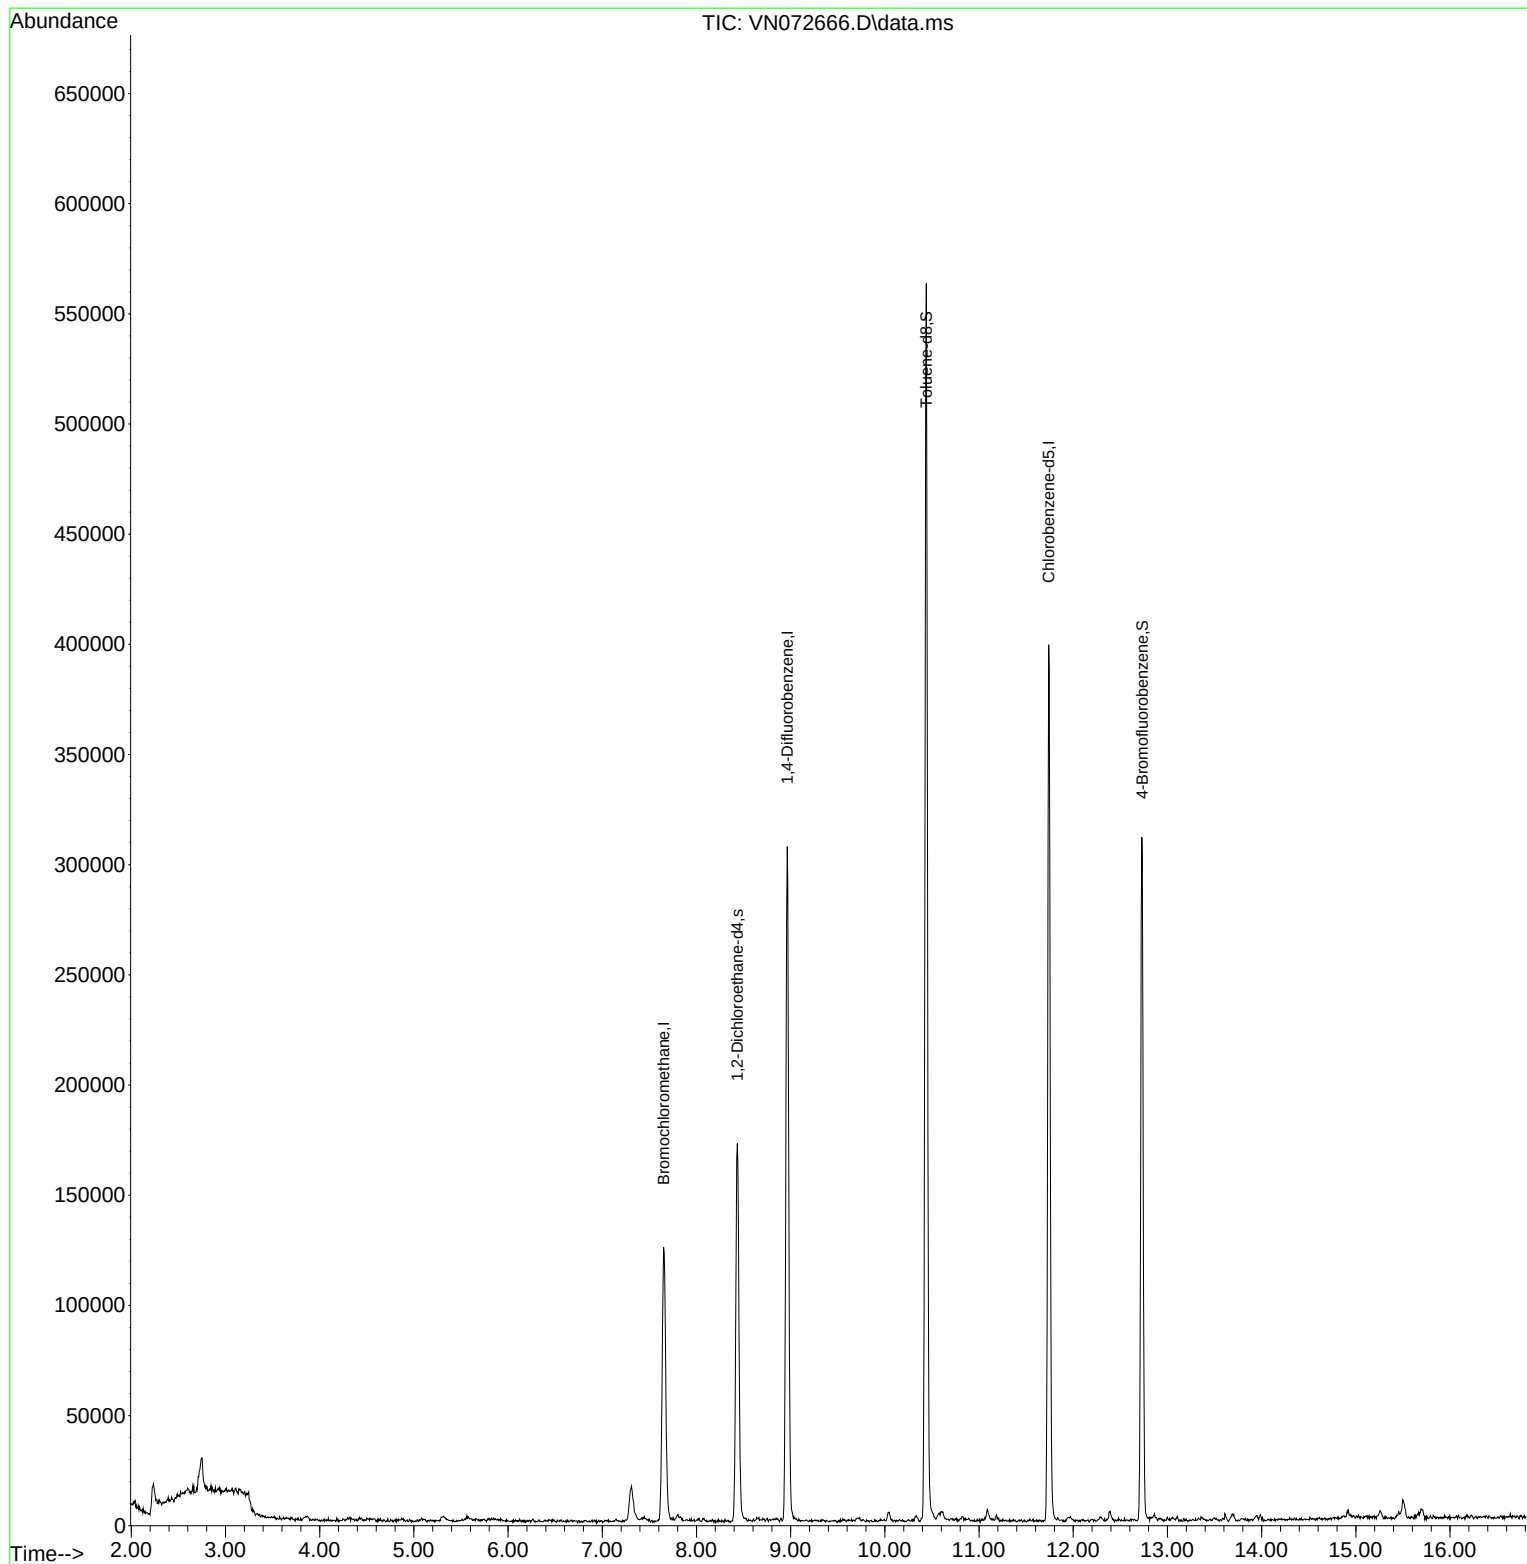


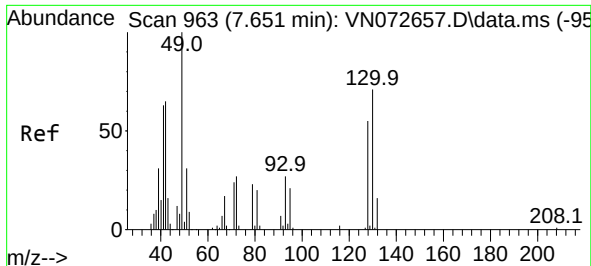

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 7.651 min Scan# 90
Delta R.T. 0.000 min
Lab File: VN072666.D
Acq: 06 Jun 2022 16:24




Instrument :
MSVOA_N
ClientSampleId :
VN0606WBL01


Tgt Ion:128 Resp: 41549
Ion Ratio Lower Upper
128 100
49 189.1 0.0 392.3
130 130.1 0.0 320.2

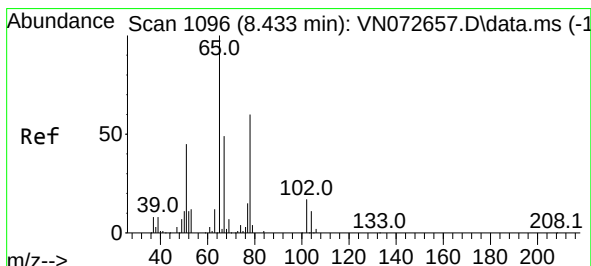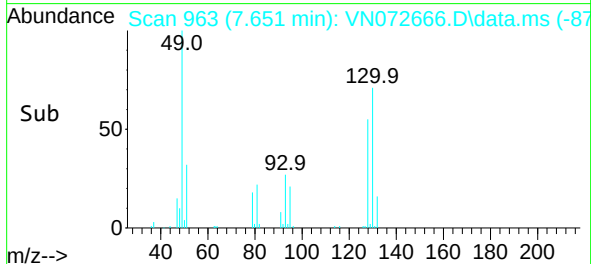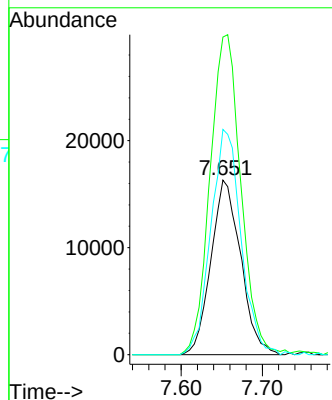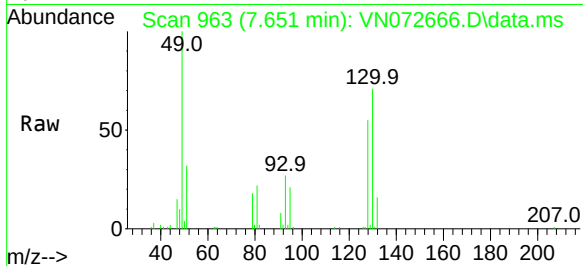

#27
1,2-Dichloroethane-d4
Concen: 31.242 ug/l
RT: 8.434 min Scan# 1096
Delta R.T. 0.000 min
Lab File: VN072666.D
Acq: 06 Jun 2022 16:24

Tgt Ion: 65 Resp: 148043
Ion Ratio Lower Upper
65 100
67 50.4 40.2 60.2

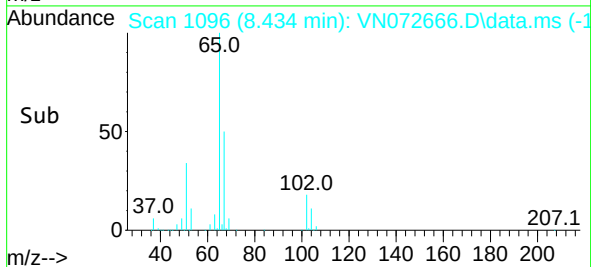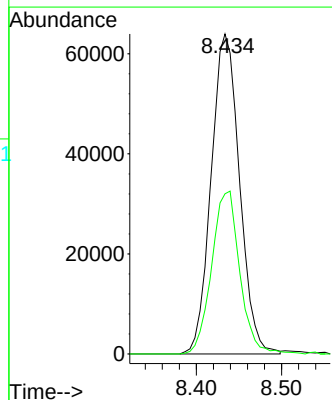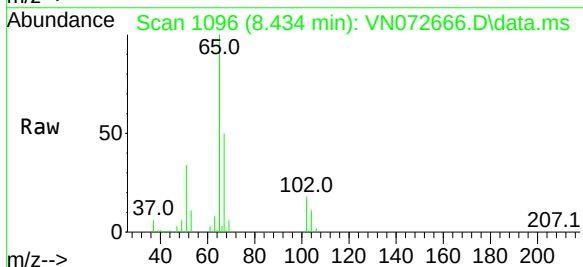

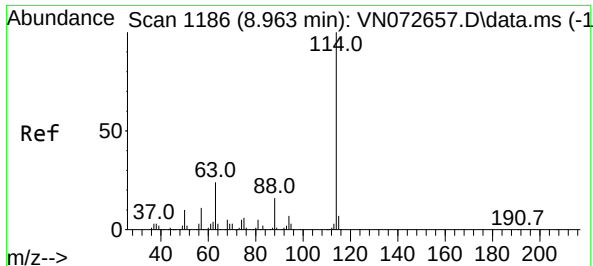

#28

1,4-Difluorobenzene

Concen: 30.000 ug/l

RT: 8.963 min Scan# 1186

Delta R.T. 0.000 min

Lab File: VN072666.D

Acq: 06 Jun 2022 16:24

Instrument :

MSVOA_N

ClientSampleId :

VN0606WBL01





Tgt Ion:114 Resp: 255057

Ion Ratio Lower Upper

114 100

63 22.9 15.8 23.6

88 17.1 11.6 17.4

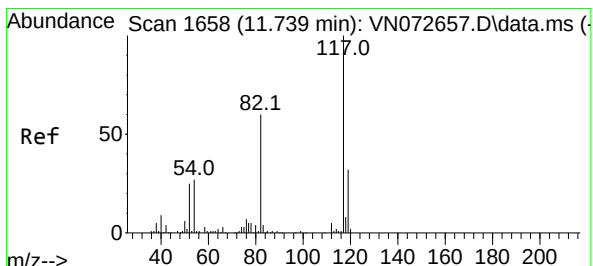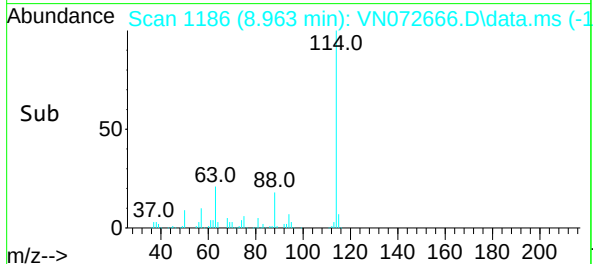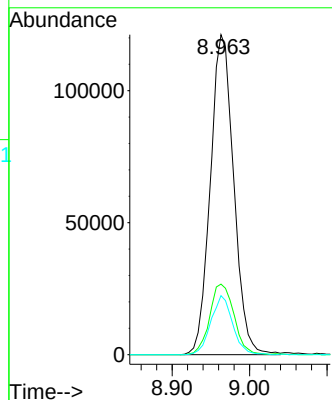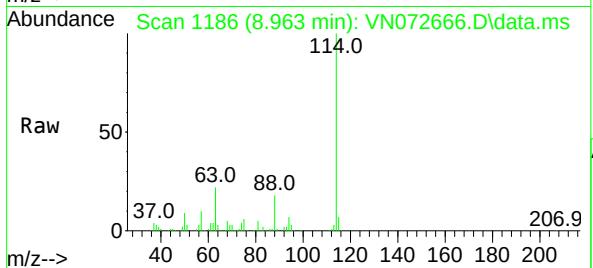

#57

Chlorobenzene-d5

Concen: 30.000 ug/l

RT: 11.739 min Scan# 1658

Delta R.T. 0.000 min

Lab File: VN072666.D

Acq: 06 Jun 2022 16:24




Tgt Ion:117 Resp: 218149


Ion Ratio Lower Upper

117 100

82 60.2 43.6 65.4

119 32.0 25.8 38.6


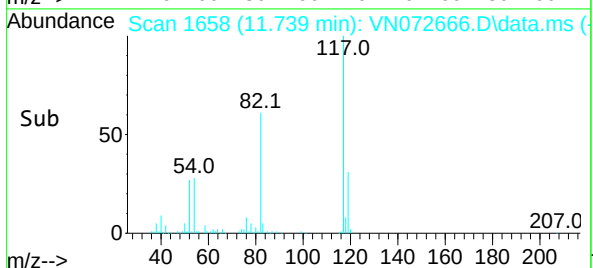
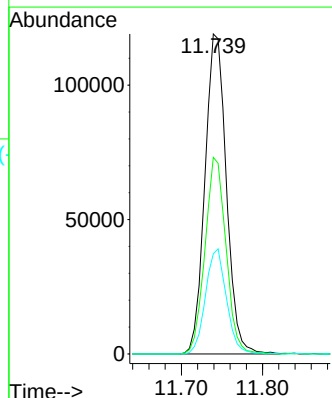
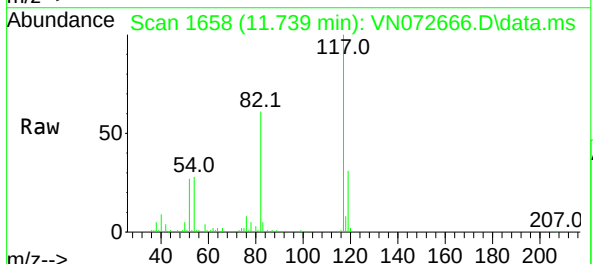


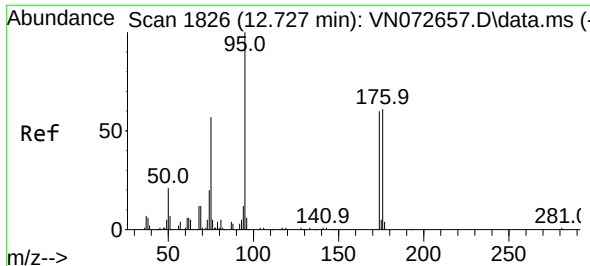

#60
4-Bromofluorobenzene
Concen: 25.269 ug/l
RT: 12.733 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN072666.D
Acq: 06 Jun 2022 16:24

Instrument :
MSVOA_N
ClientSampleId :
VN0606WBL01

Tgt Ion: 95 Resp: 113379
Ion Ratio Lower Upper
95 100
174 64.8 62.9 94.3
176 62.5 61.0 91.4

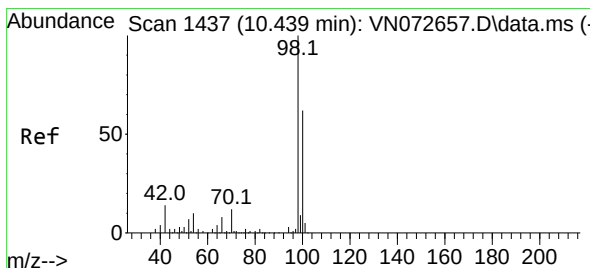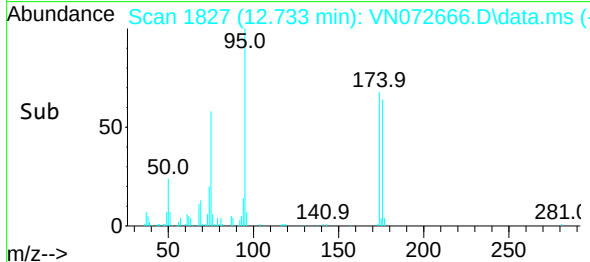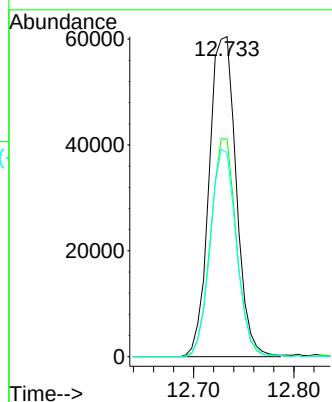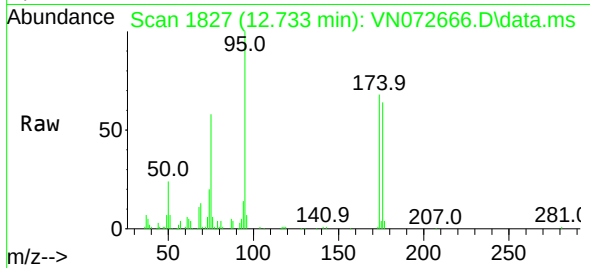

#63
Toluene-d8
Concen: 30.762 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN072666.D
Acq: 06 Jun 2022 16:24

Tgt Ion: 98 Resp: 371737
Ion Ratio Lower Upper
98 100
100 65.6 50.6 76.0

