
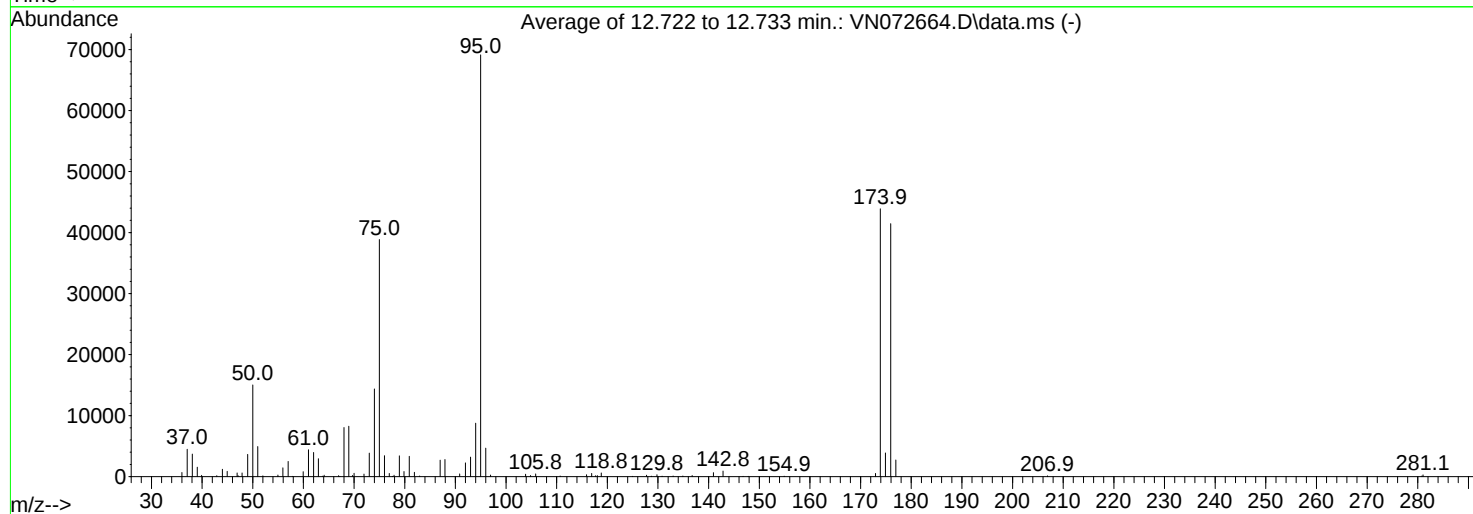


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060622\
 Data File : VN072664.D
 Acq On : 06 Jun 2022 15:16
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N060622W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Mon Jun 06 14:10:15 2022

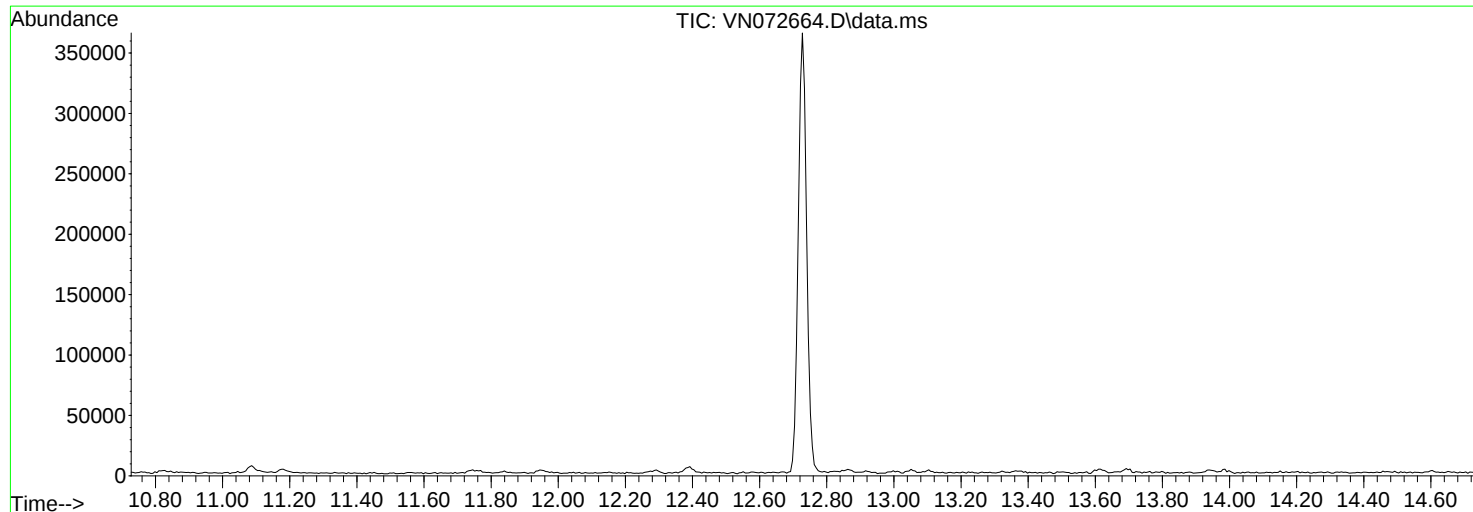

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1818

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	15036	PASS
75	95	30	60	56.2	38869	PASS
95	95	100	100	100.0	69131	PASS
96	95	5	9	6.7	4662	PASS
173	174	0.00	2	1.2	523	PASS
174	95	50	100	63.5	43915	PASS
175	174	5	9	8.8	3875	PASS
176	174	95	101	94.4	41461	FAIL*
177	176	5	9	6.6	2721	PASS