

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060623\
 Data File : VN078073.D
 Acq On : 06 Jun 2023 16:24
 Operator : JC\MD
 Sample : 03029-14
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TP-10

Quant Time: Jun 07 01:22:58 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
 Quant Title : SW846 8260
 QLast Update : Tue May 16 04:07:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.235	168	445080	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	813468	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	742707	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.800	152	243497	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	290267	43.587	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	87.180%		
35) Dibromofluoromethane	8.171	113	251945	47.496	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	95.000%		
50) Toluene-d8	10.571	98	1008114	49.375	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	98.740%		
62) 4-Bromofluorobenzene	12.853	95	336513	46.666	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	93.340%		
Target Compounds						
					Qvalue	
3) Chloromethane	2.371	50	1194	Below Cal		99
5) Bromomethane	2.977	94	2676	0.567 ug/l #		40
11) Tert butyl alcohol	5.536	59	834	0.907 ug/l #		72
13) Acrolein	4.195	56	64	Below Cal #		16
16) Acetone	4.453	43	28323	13.518 ug/l		97
18) Methyl Acetate	5.047	43	4474	0.509 ug/l #		59
20) Methylene Chloride	5.289	84	22274	2.195 ug/l		90
25) 2-Butanone	7.518	43	6781	2.069 ug/l #		77
29) Tetrahydrofuran	7.847	42	686	0.320 ug/l #		68
31) Cyclohexane	8.235	56	9220	1.019 ug/l #		7
36) 1,1-Dichloropropene	8.230	75	35443	4.568 ug/l #		41
37) Ethyl Acetate	7.577	43	76966	11.130 ug/l		97
38) Carbon Tetrachloride	8.230	117	46674	5.957 ug/l #		15
42) 1,2-Dichloroethane	8.688	62	2547	0.306 ug/l #		73
43) Isopropyl Acetate	8.694	43	326362	28.893 ug/l #		86
48) Methyl methacrylate	9.671	41	8057	1.504 ug/l #		32
49) 1,4-Dioxane	9.677	88	66	0.652 ug/l #		1
51) 4-Methyl-2-Pentanone	10.447	43	11878	1.769 ug/l		92
54) cis-1,3-Dichloropropene	10.365	75	129876	13.910 ug/l #		66
57) 1,3-Dichloropropane	11.212	76	16588	1.710 ug/l #		44
59) 2-Hexanone	11.176	43	277956	55.969 ug/l #		19
74) N-amyl acetate	12.488	43	4540	0.585 ug/l #		43
76) 1,2,3-Trichloropropane	12.853	75	175298	28.747 ug/l #		1
81) trans-1,4-Dichloro-2-b...	12.853	75	175298	91.889 ug/l #		15
87) 1,3-Dichlorobenzene	13.747	146	2411	0.272 ug/l #		59
89) n-Butylbenzene	14.059	91	4556	0.284 ug/l		89
93) 1,2,4-Trichlorobenzene	15.406	180	1296	0.268 ug/l #		1
94) Hexachlorobutadiene	15.511	225	487	0.243 ug/l #		54
95) Naphthalene	15.647	128	7290	0.438 ug/l #		68
96) 1,2,3-Trichlorobenzene	15.841	180	1186	0.250 ug/l #		1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060623\
Data File : VN078073.D
Acq On : 06 Jun 2023 16:24
Operator : JC\MD
Sample : 03029-14
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TP-10

Quant Time: Jun 07 01:22:58 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
Quant Title : SW846 8260
QLast Update : Tue May 16 04:07:42 2023
Response via : Initial Calibration




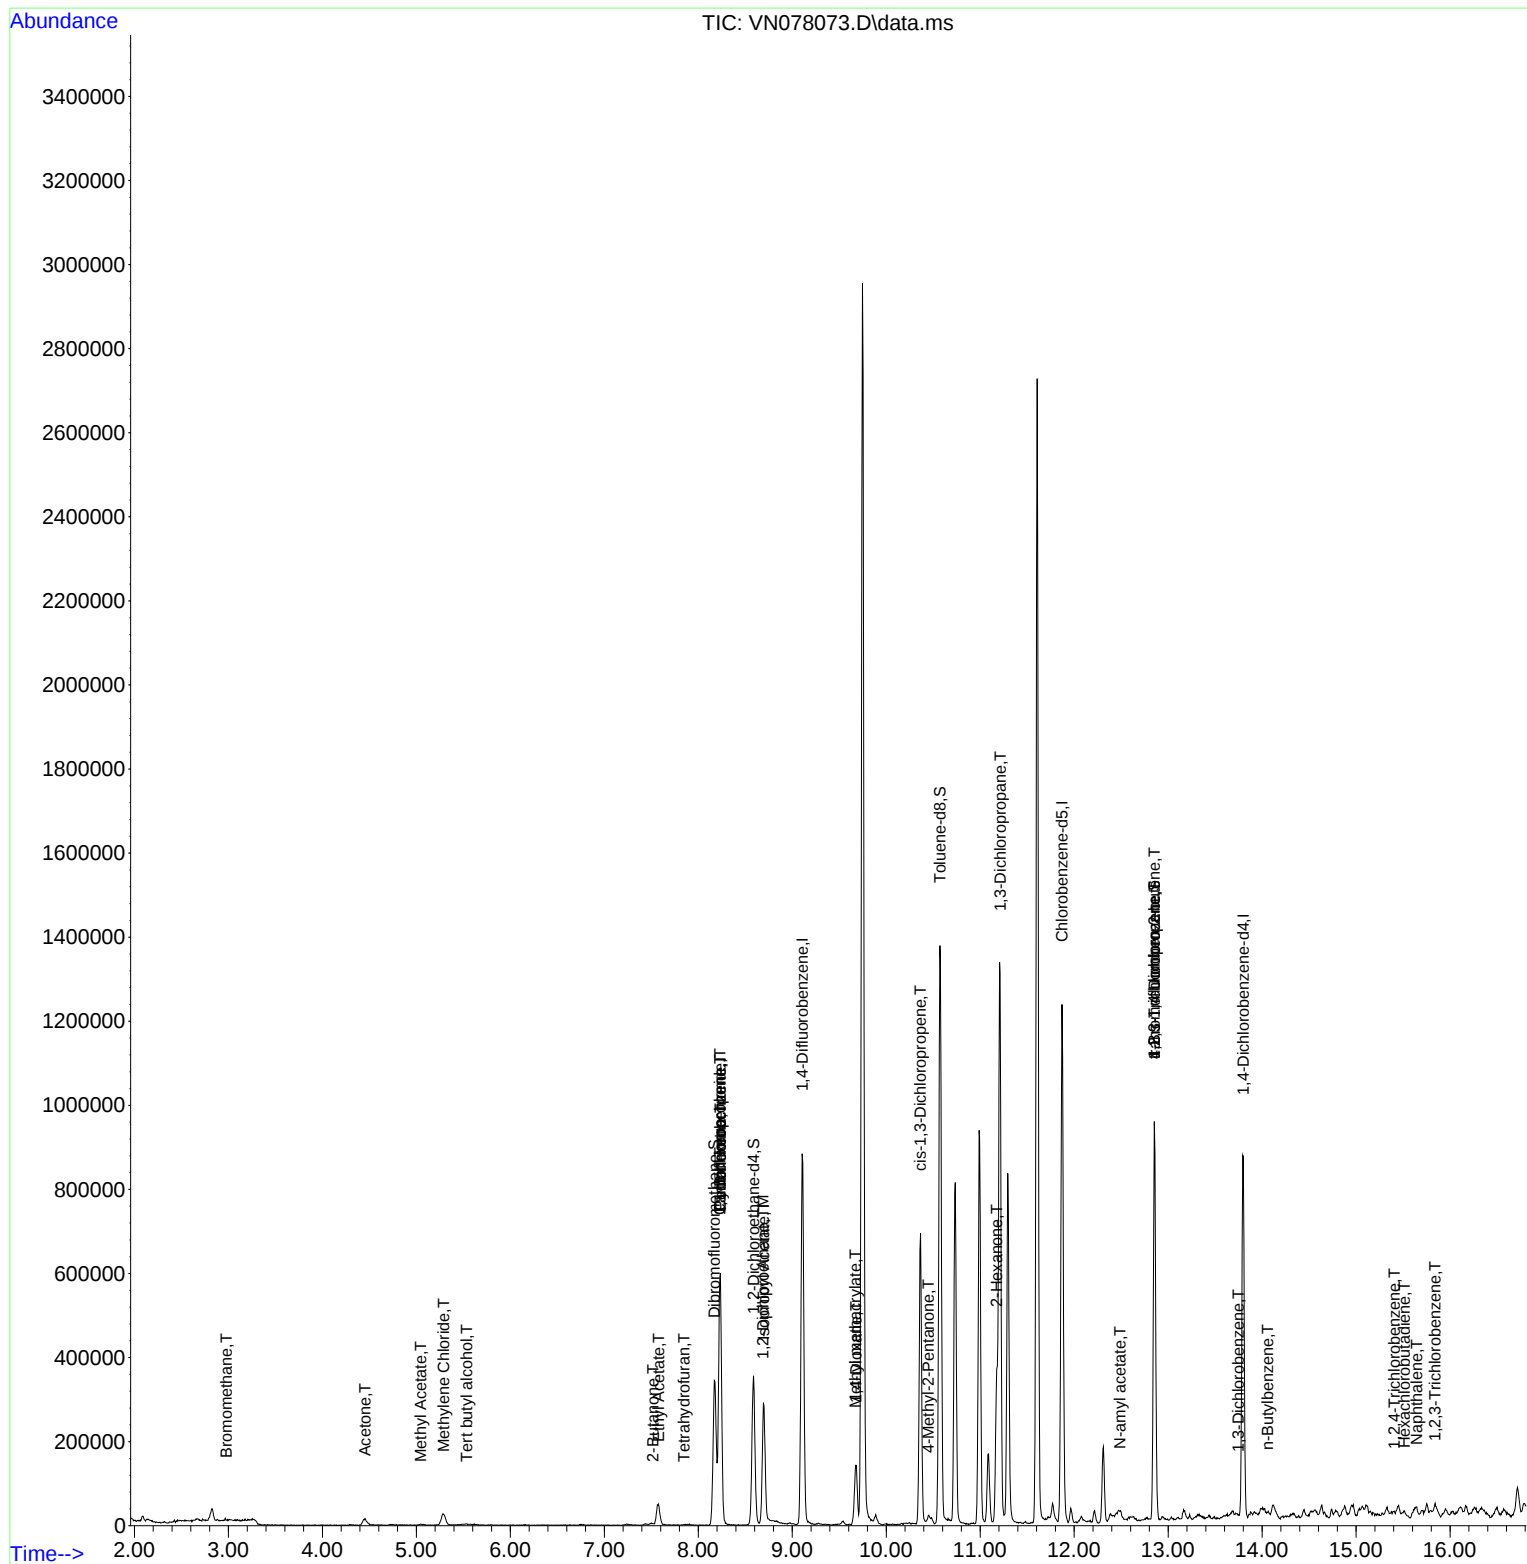




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.235 min Scan# 10
Delta R.T. 0.005 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24




Instrument :
MSVOA_N
ClientSampleId :
TP-10


Tgt Ion:168 Resp: 445080
Ion Ratio Lower Upper
168 100
99 60.9 53.0 79.6



#3
Chloromethane
Concen: Below Cal
RT: 2.371 min Scan# 71
Delta R.T. 0.006 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24

Tgt Ion: 50 Resp: 1194
Ion Ratio Lower Upper
50 100
52 33.7 26.5 39.7



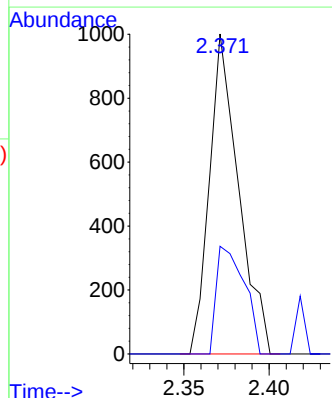





#5
Bromomethane
Concen: 0.567 ug/l
RT: 2.977 min Scan# 11
Delta R.T. 0.030 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24




Instrument :
MSVOA_N
ClientSampleId :
TP-10


Tgt Ion: 94 Resp: 2676
Ion Ratio Lower Upper
94 100
96 34.1 73.1 109.7#



#11
Tert butyl alcohol
Concen: 0.907 ug/l
RT: 5.536 min Scan# 609
Delta R.T. 0.006 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24

Tgt Ion: 59 Resp: 834
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#









#13
Acrolein
Concen: Below Cal
RT: 4.195 min Scan# 381
Delta R.T. 0.006 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24




Instrument :
MSVOA_N
ClientSampleId :
TP-10


Tgt Ion: 56 Resp: 64
Ion Ratio Lower Upper
56 100
55 0.0 54.5 81.7#



#16
Acetone
Concen: 13.518 ug/l
RT: 4.453 min Scan# 425
Delta R.T. 0.023 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24

Tgt Ion: 43 Resp: 28323
Ion Ratio Lower Upper
43 100
58 36.8 28.0 42.0



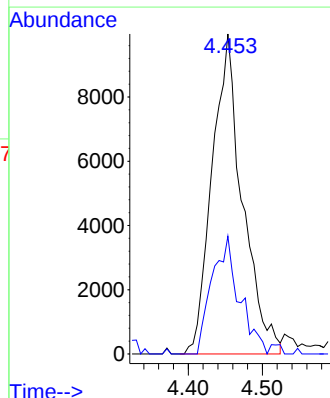





#18
Methyl Acetate
Concen: 0.509 ug/l
RT: 5.047 min Scan# 51
Delta R.T. 0.011 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24




Instrument :
MSVOA_N
ClientSampleId :
TP-10


Tgt Ion: 43 Resp: 4474
Ion Ratio Lower Upper
43 100
74 9.5 26.2 39.4#

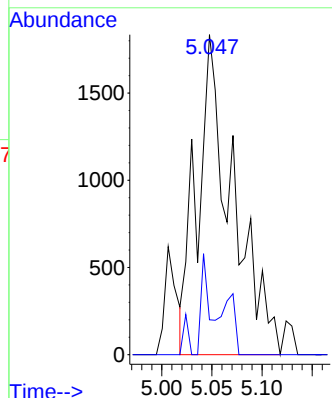

#20
Methylene Chloride
Concen: 2.195 ug/l
RT: 5.289 min Scan# 567
Delta R.T. 0.006 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24

Tgt Ion: 84 Resp: 22274
Ion Ratio Lower Upper
84 100
49 109.8 79.7 119.5
51 27.2 25.2 37.8
86 58.8 53.3 79.9


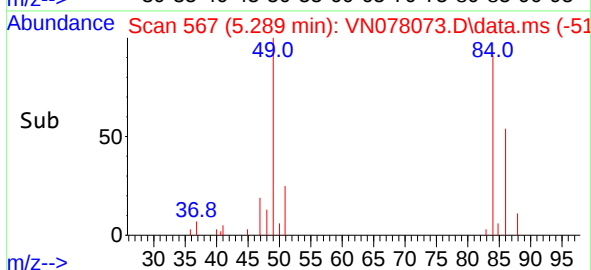
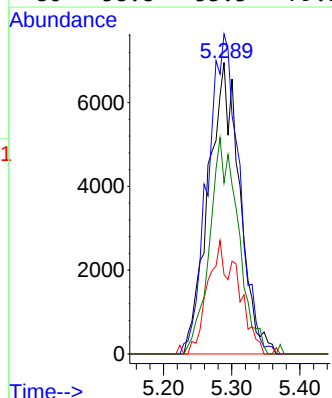





#25
2-Butanone
Concen: 2.069 ug/l
RT: 7.518 min Scan# 941
Delta R.T. 0.030 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24




Instrument :
MSVOA_N
ClientSampleId :
TP-10


Tgt Ion: 43 Resp: 6781
Ion Ratio Lower Upper
43 100
72 24.0 30.2 45.2#

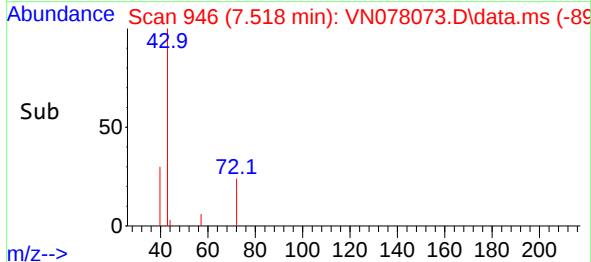

#29
Tetrahydrofuran
Concen: 0.320 ug/l
RT: 7.847 min Scan# 1002
Delta R.T. 0.006 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24


Tgt Ion: 42 Resp: 686
Ion Ratio Lower Upper
42 100
72 24.6 49.8 74.6#
71 48.7 47.4 71.2

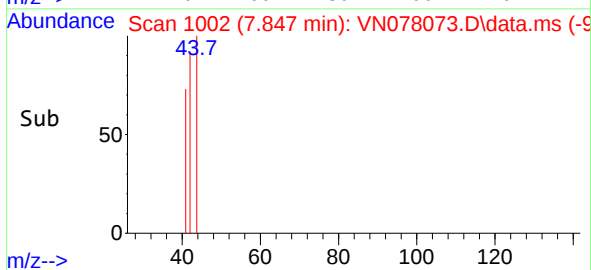



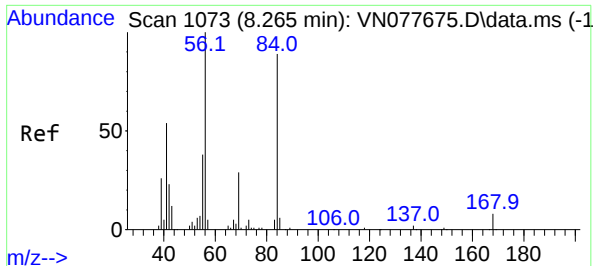


#31
Cyclohexane
Concen: 1.019 ug/l
RT: 8.235 min Scan# 1068
Delta R.T. -0.030 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24

Instrument :
MSVOA_N
ClientSampleId :
TP-10







Tgt Ion: 56 Resp: 9220
Ion Ratio Lower Upper
56 100
69 171.1 26.8 40.2#
84 146.9 81.8 122.6#

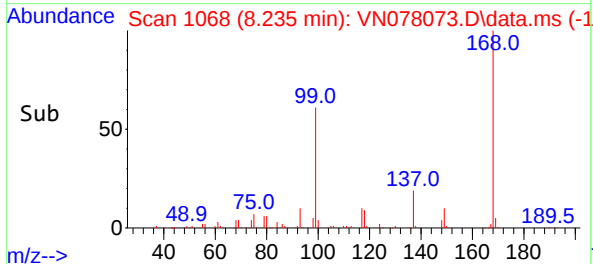

#33
1,2-Dichloroethane-d4
Concen: 43.587 ug/l
RT: 8.588 min Scan# 1128
Delta R.T. 0.006 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24

Tgt Ion: 65 Resp: 290267
Ion Ratio Lower Upper
65 100
67 52.6 0.0 106.6


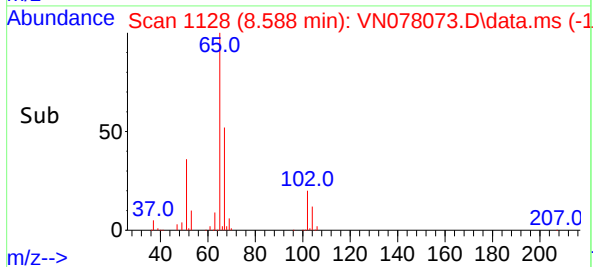

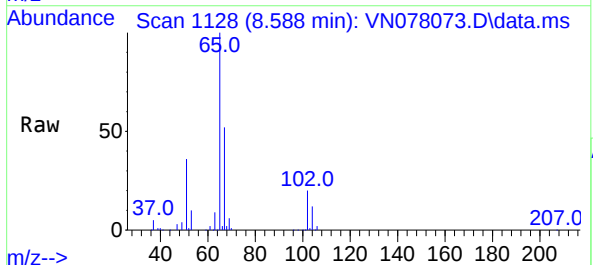


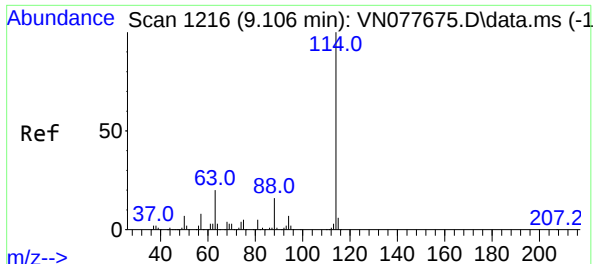

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24




Instrument :
MSVOA_N
ClientSampleId :
TP-10


Tgt Ion:114 Resp: 813468
Ion Ratio Lower Upper
114 100
63 18.9 0.0 36.4
88 14.3 0.0 30.6

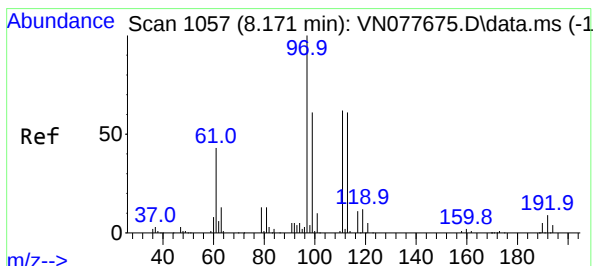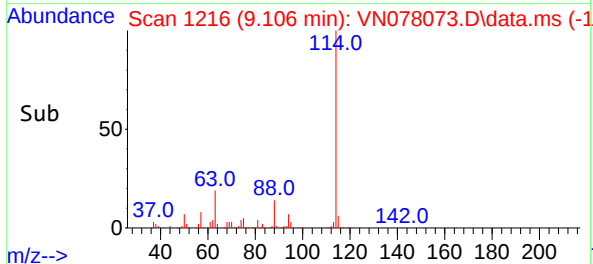

#35
Dibromofluoromethane
Concen: 47.496 ug/l
RT: 8.171 min Scan# 1057
Delta R.T. -0.000 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24

Tgt Ion:113 Resp: 251945
Ion Ratio Lower Upper
113 100
111 102.7 82.6 123.8
192 17.0 12.7 19.1



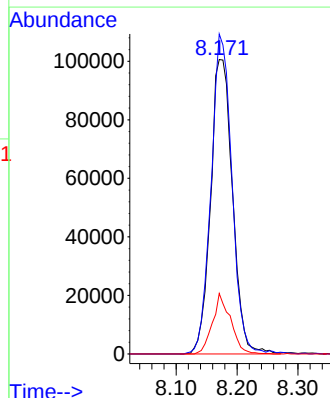
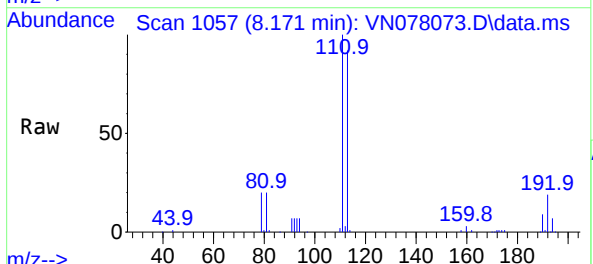


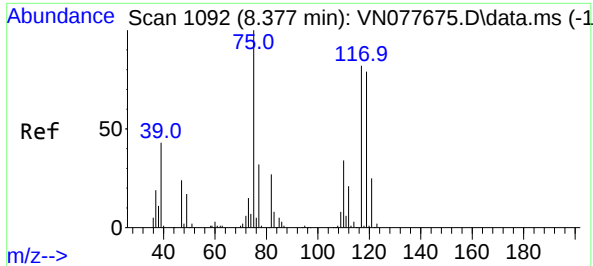

#36
1,1-Dichloropropene
Concen: 4.568 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.147 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24




Instrument :
MSVOA_N
ClientSampleId :
TP-10


Tgt Ion: 75 Resp: 35443
Ion Ratio Lower Upper
75 100
110 1.6 19.1 57.3#
77 0.0 25.0 37.4#

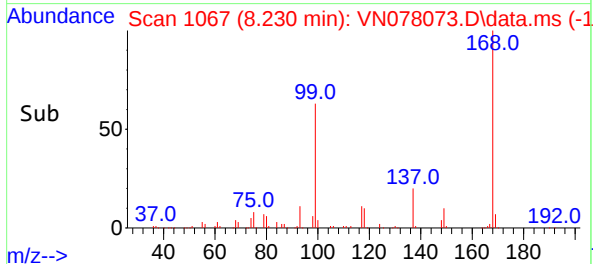

#37
Ethyl Acetate
Concen: 11.130 ug/l
RT: 7.577 min Scan# 956
Delta R.T. 0.012 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24

Tgt Ion: 43 Resp: 76966
Ion Ratio Lower Upper
43 100
61 15.5 13.2 19.8
70 12.2 11.3 16.9


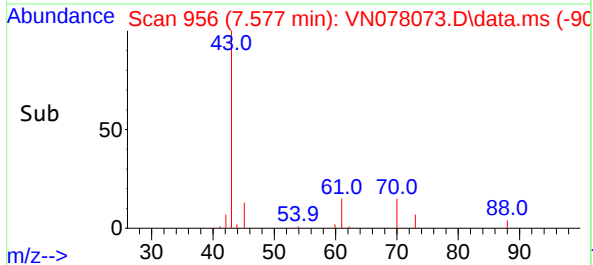

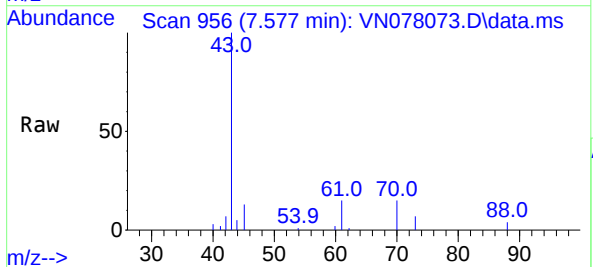


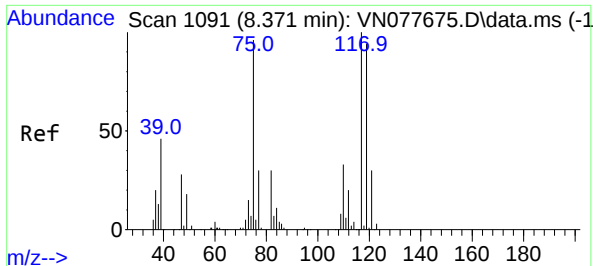

#38
Carbon Tetrachloride
Concen: 5.957 ug/l
RT: 8.230 min Scan# 1107
Delta R.T. -0.141 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24




Instrument :
MSVOA_N
ClientSampleId :
TP-10


Tgt Ion:117 Resp: 46674
Ion Ratio Lower Upper
117 100
119 3.9 77.3 115.9#
121 0.0 23.3 34.9#

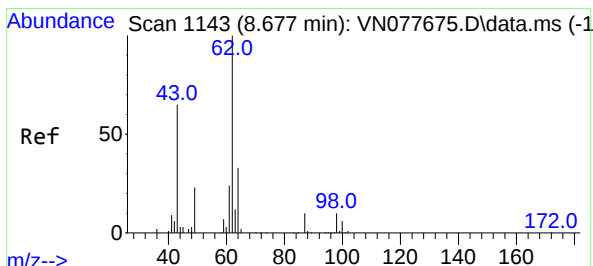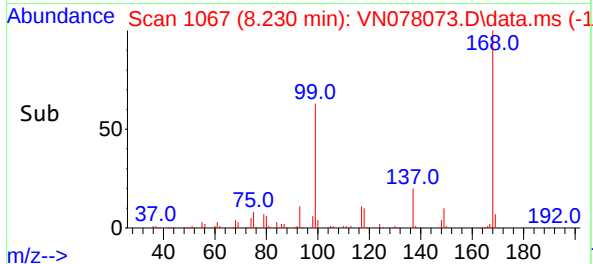

#42
1,2-Dichloroethane
Concen: 0.306 ug/l
RT: 8.688 min Scan# 1145
Delta R.T. 0.011 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24

Tgt Ion: 62 Resp: 2547
Ion Ratio Lower Upper
62 100
98 0.0 0.0 19.8


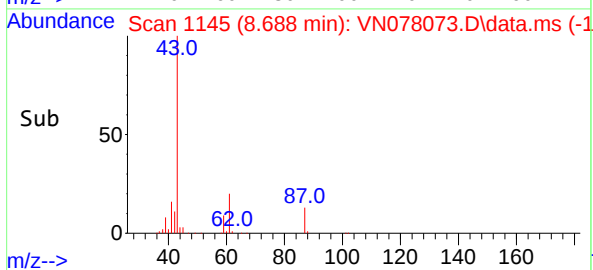

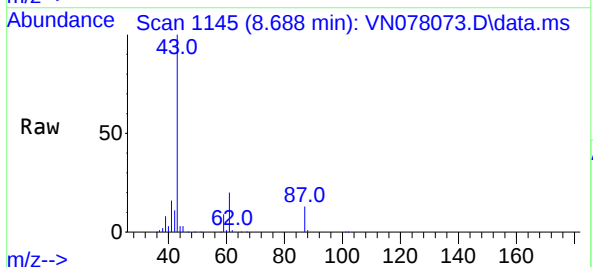


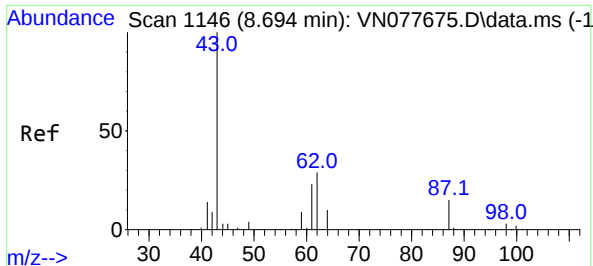

#43
Isopropyl Acetate
Concen: 28.893 ug/l
RT: 8.694 min Scan# 1146
Delta R.T. 0.000 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24




Instrument :
MSVOA_N
ClientSampleId :
TP-10


Tgt Ion: 43 Resp: 326362
Ion Ratio Lower Upper
43 100
61 20.6 24.7 37.1#
87 15.4 14.6 21.8

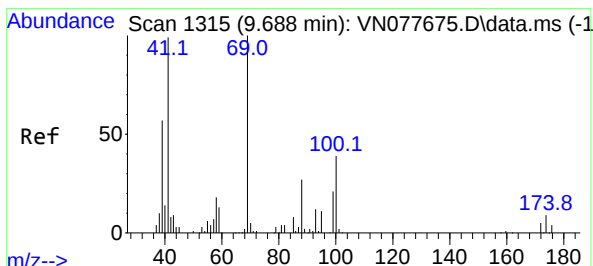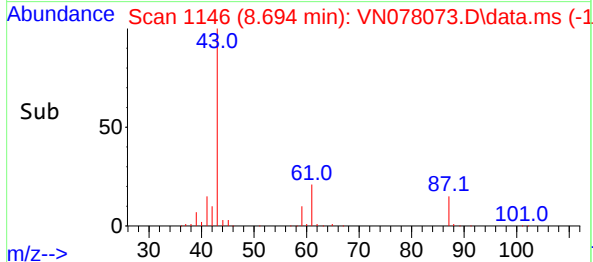

#48
Methyl methacrylate
Concen: 1.504 ug/l
RT: 9.671 min Scan# 1312
Delta R.T. -0.017 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24

Tgt Ion: 41 Resp: 8057
Ion Ratio Lower Upper
41 100
69 1.8 90.4 135.6#
39 61.4 54.6 81.8


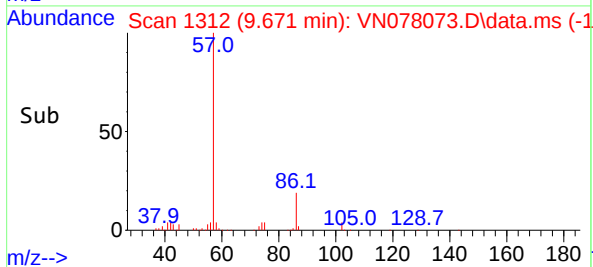

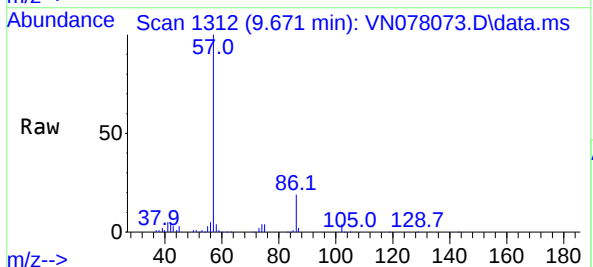


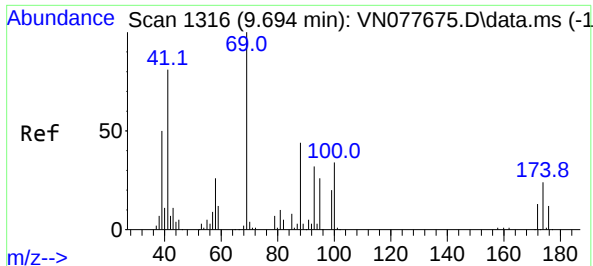

#49
1,4-Dioxane
Concen: 0.652 ug/l
RT: 9.677 min Scan# 11
Delta R.T. -0.017 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24




Instrument :
MSVOA_N
ClientSampleId :
TP-10


Tgt Ion: 88 Resp: 66
Ion Ratio Lower Upper
88 100
43 0.0 17.0 25.6#
58 11507.6 47.0 70.4#

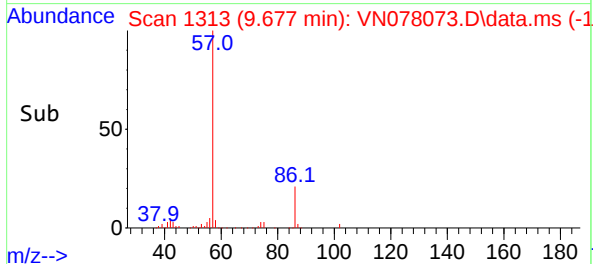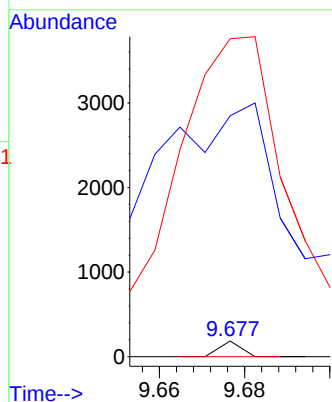

#50
Toluene-d8
Concen: 49.375 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24

Tgt Ion: 98 Resp: 1008114
Ion Ratio Lower Upper
98 100
100 64.3 52.0 78.0


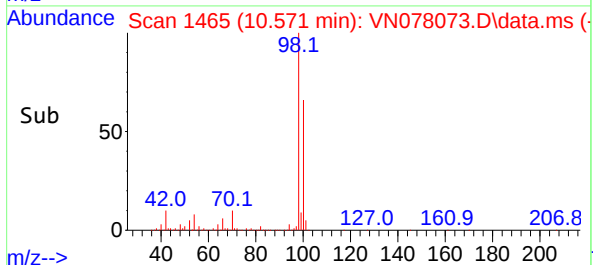

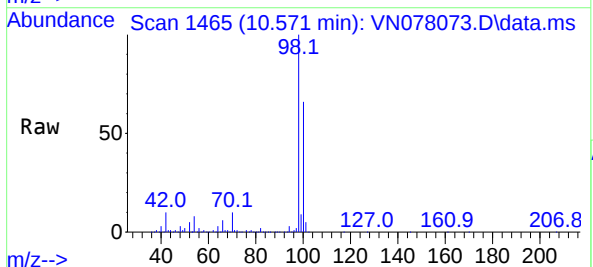


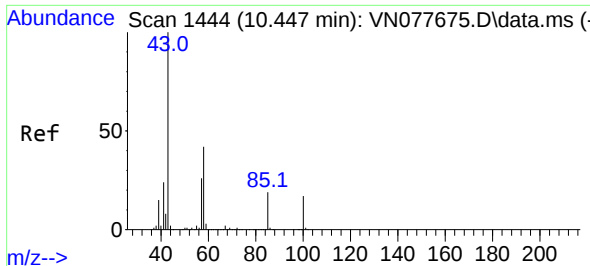

#51
4-Methyl-2-Pentanone
Concen: 1.769 ug/l
RT: 10.447 min Scan# 1444
Delta R.T. 0.000 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24




Instrument :
MSVOA_N
ClientSampleId :
TP-10


Tgt Ion: 43 Resp: 11878
Ion Ratio Lower Upper
43 100
58 40.3 36.6 54.8

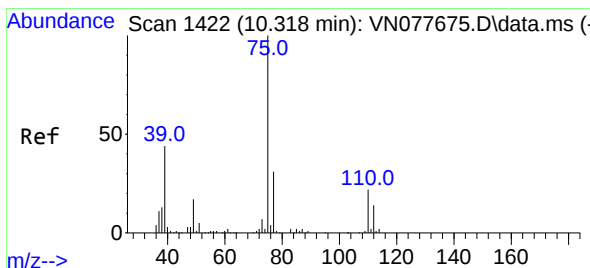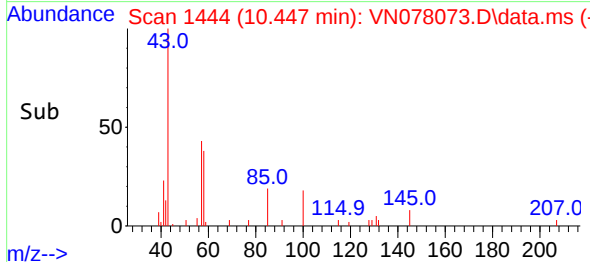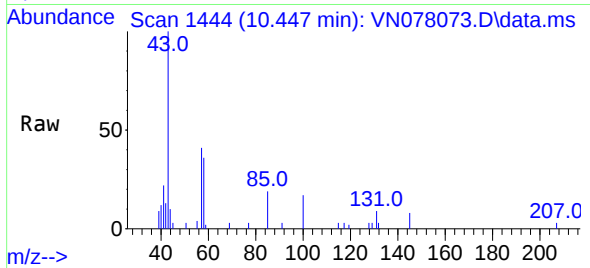

#54
cis-1,3-Dichloropropene
Concen: 13.910 ug/l
RT: 10.365 min Scan# 1430
Delta R.T. 0.047 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24

Tgt Ion: 75 Resp: 129876
Ion Ratio Lower Upper
75 100
77 0.2 26.1 39.1#
39 30.9 31.6 47.4#

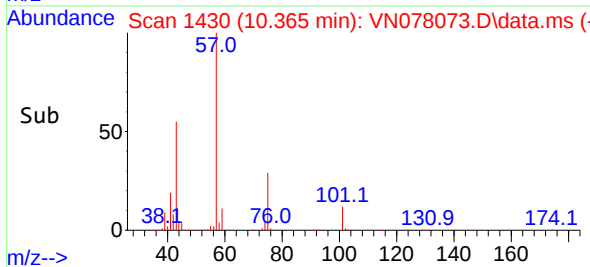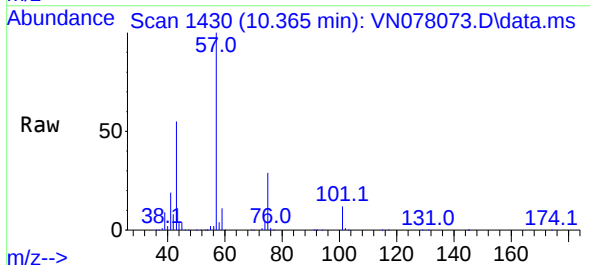



#57

1,3-Dichloropropane

Concen: 1.710 ug/l

RT: 11.212 min Scan# 11

Delta R.T. 0.041 min

Lab File: VN078073.D

Acq: 06 Jun 2023 16:24

Instrument :

MSVOA_N

ClientSampleId :





TP-10

Tgt Ion: 76 Resp: 16588

Ion Ratio Lower Upper

76 100

78 0.9 26.1 39.1#

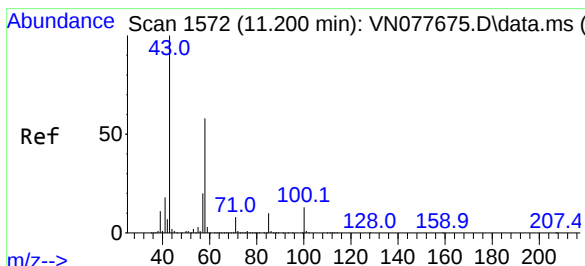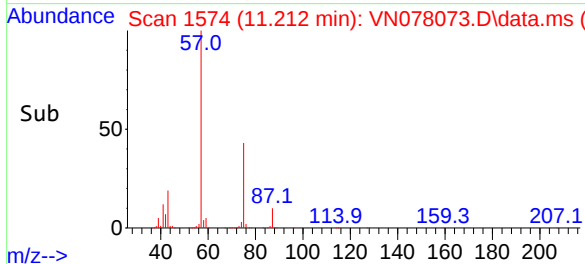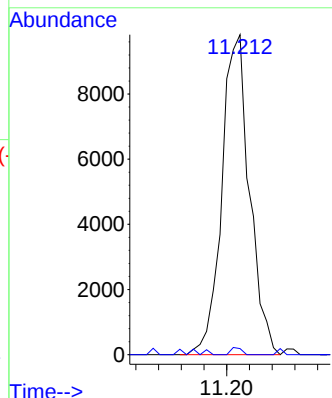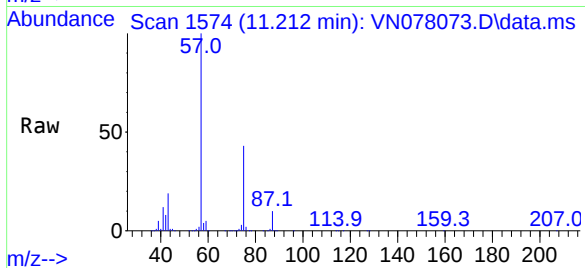

#59

2-Hexanone

Concen: 55.969 ug/l

RT: 11.176 min Scan# 1568

Delta R.T. -0.024 min

Lab File: VN078073.D




Acq: 06 Jun 2023 16:24


Tgt Ion: 43 Resp: 277956

Ion Ratio Lower Upper

43 100

58 0.0 31.7 95.1#


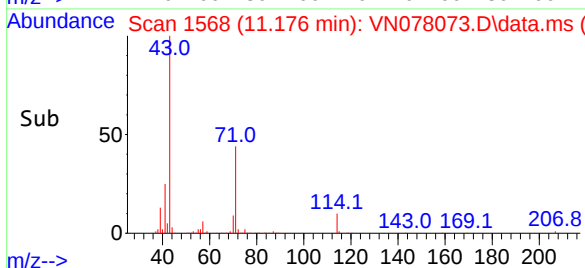
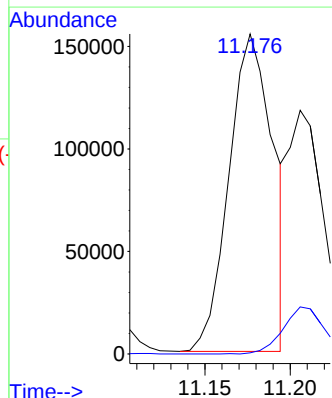
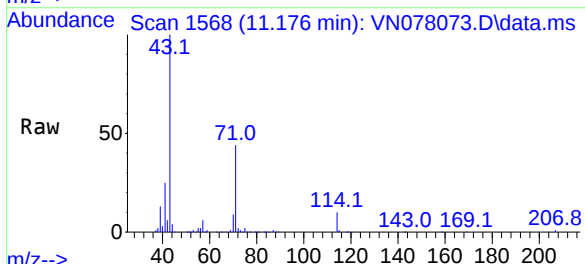




#62
4-Bromofluorobenzene
Concen: 46.666 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24




Instrument :
MSVOA_N
ClientSampleId :
TP-10


Tgt Ion: 95 Resp: 336513
Ion Ratio Lower Upper
95 100
174 76.7 0.0 143.8
176 73.1 0.0 135.8



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1686
Delta R.T. 0.001 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24

Tgt Ion: 117 Resp: 742707
Ion Ratio Lower Upper
117 100
82 53.7 44.0 66.0
119 31.2 25.6 38.4


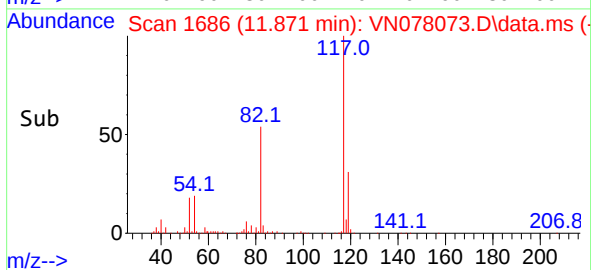






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.800 min Scan# 2014
Delta R.T. -0.000 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24




Instrument :
MSVOA_N
ClientSampleId :
TP-10


Tgt Ion:152 Resp: 243497
Ion Ratio Lower Upper
152 100
115 61.9 32.3 96.8
150 155.4 0.0 355.8

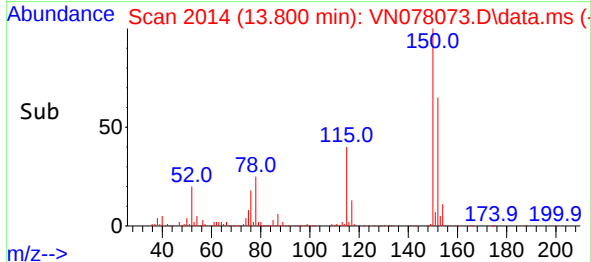

#74
N-ethyl acetate
Concen: 0.585 ug/l
RT: 12.488 min Scan# 1791
Delta R.T. -0.012 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24

Tgt Ion: 43 Resp: 4540
Ion Ratio Lower Upper
43 100
70 10.8 43.4 65.2#
55 0.0 21.4 32.0#
61 0.0 22.8 34.2#


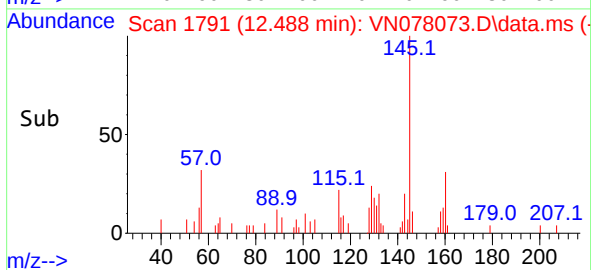






#76
1,2,3-Trichloropropane
Concen: 28.747 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.147 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24




Instrument :
MSVOA_N
ClientSampleId :
TP-10


Tgt Ion: 75 Resp: 175298
Ion Ratio Lower Upper
75 100
77 1.9 84.5 253.5#

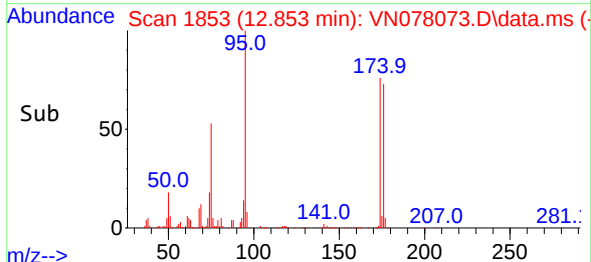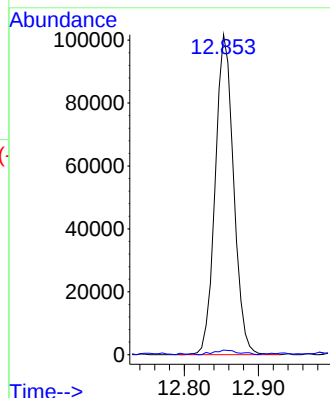

#81
trans-1,4-Dichloro-2-butene
Concen: 91.889 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.112 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24

Tgt Ion: 75 Resp: 175298
Ion Ratio Lower Upper
75 100
53 0.1 67.4 101.2#
89 0.2 38.8 58.2#

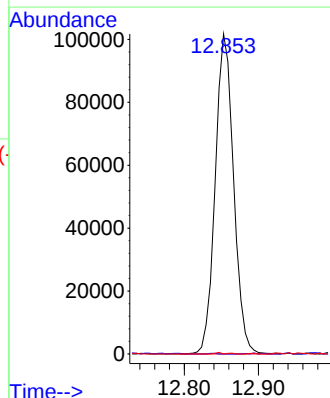



#87

1,3-Dichlorobenzene

Concen: 0.272 ug/l

RT: 13.747 min Scan# 2004

Delta R.T. 0.006 min

Lab File: VN078073.D

Acq: 06 Jun 2023 16:24

Instrument :

MSVOA_N

ClientSampleId :

TP-10





Tgt Ion:146 Resp: 2411

Ion Ratio Lower Upper

146 100

111 32.0 22.1 66.3

148 20.0 32.0 96.0#

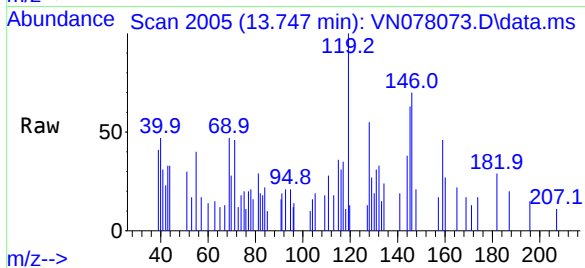

#89

n-Butylbenzene

Concen: 0.284 ug/l

RT: 14.059 min Scan# 2058

Delta R.T. -0.005 min

Lab File: VN078073.D

Acq: 06 Jun 2023 16:24




Tgt Ion: 91 Resp: 4556


Ion Ratio Lower Upper

91 100

92 42.9 26.4 79.0

134 23.0 12.6 37.6



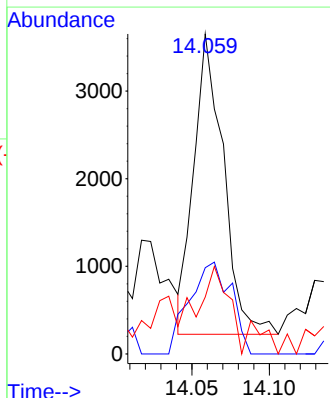
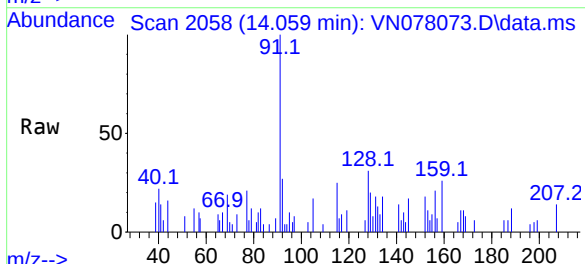




#93
1,2,4-Trichlorobenzene
Concen: 0.268 ug/l
RT: 15.406 min Scan# 21
Delta R.T. 0.006 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24




Instrument :
MSVOA_N
ClientSampleId :
TP-10


Tgt Ion:180 Resp: 1296
Ion Ratio Lower Upper
180 100
182 99.2 46.1 138.2
145 292.0 16.6 49.8#

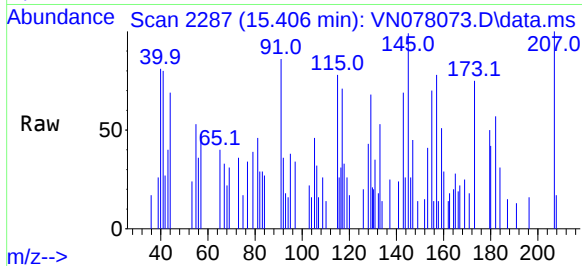

#94
Hexachlorobutadiene
Concen: 0.243 ug/l
RT: 15.511 min Scan# 2305
Delta R.T. 0.005 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24

Tgt Ion:225 Resp: 487
Ion Ratio Lower Upper
225 100
223 31.6 31.3 93.8
227 23.8 31.9 95.9#



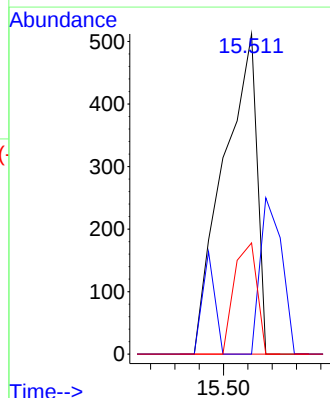
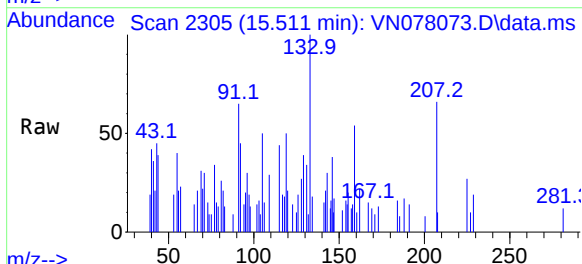




#95
Naphthalene
Concen: 0.438 ug/l
RT: 15.647 min Scan# 2328
Delta R.T. -0.000 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24

Instrument :
MSVOA_N
ClientSampleId :
TP-10

Tgt Ion:128 Resp: 7290
Ion Ratio Lower Upper
128 100
127 35.1 10.0 15.0#
129 9.7 8.7 13.1

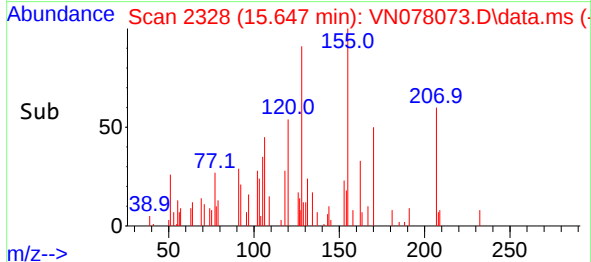

#96
1,2,3-Trichlorobenzene
Concen: 0.250 ug/l
RT: 15.841 min Scan# 2361
Delta R.T. -0.006 min
Lab File: VN078073.D
Acq: 06 Jun 2023 16:24

Tgt Ion:180 Resp: 1186
Ion Ratio Lower Upper
180 100
182 104.9 46.2 138.6
145 287.4 17.5 52.6#

