
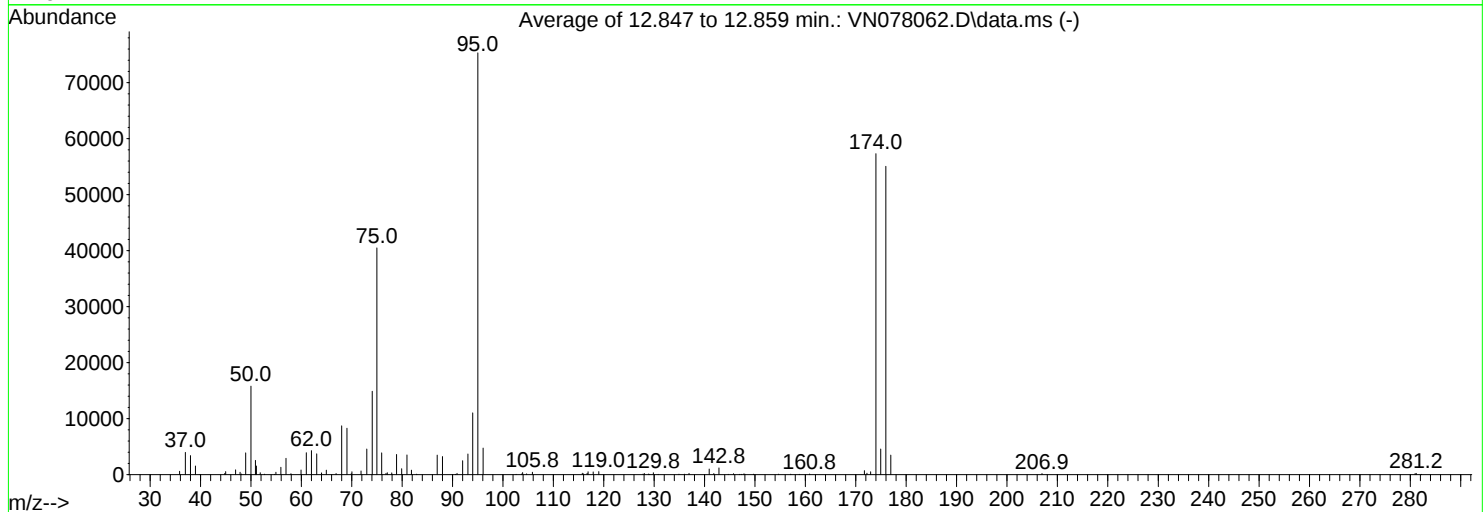


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060623\
Data File : VN078062.D
Acq On : 06 Jun 2023 09:09
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
Title : SW846 8260
Last Update : Tue May 16 04:07:42 2023

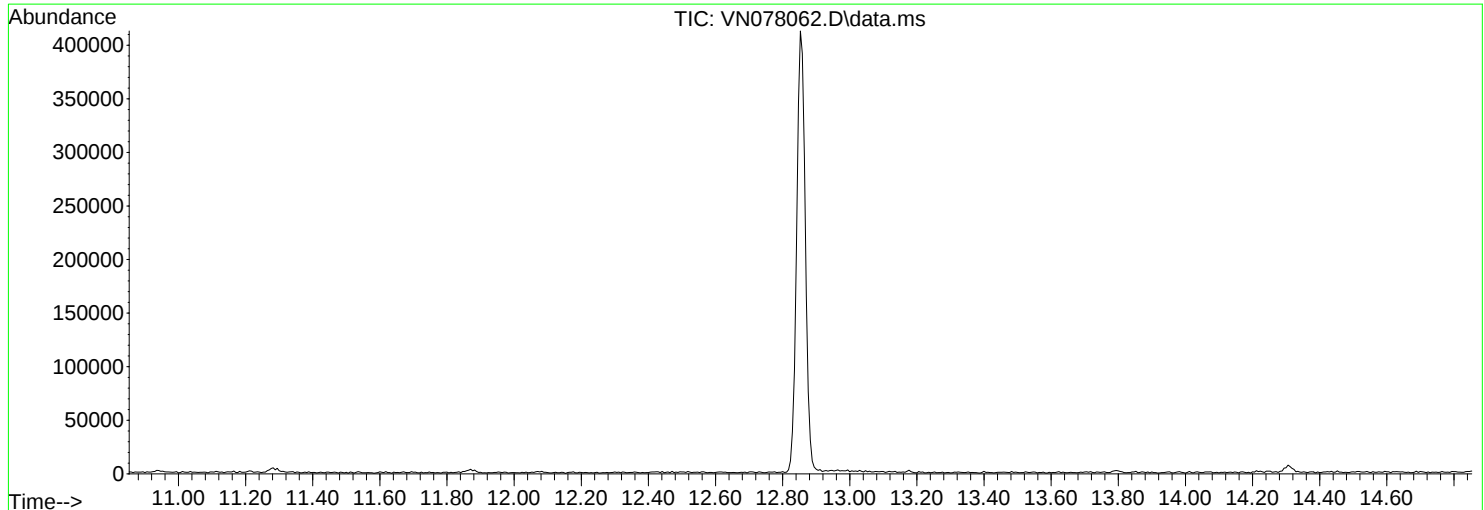

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	15802	PASS
75	95	30	60	53.8	40491	PASS
95	95	100	100	100.0	75309	PASS
96	95	5	9	6.3	4748	PASS
173	174	0.00	2	0.9	504	PASS
174	95	50	100	76.1	57296	PASS
175	174	5	9	8.0	4587	PASS
176	174	95	101	96.1	55045	PASS
177	176	5	9	6.3	3484	PASS

Average of 12.847 to 12.859 min.: VN078062.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	600	50.00	15802	61.00	3926	73.00	4581
37.00	3978	50.90	2538	62.00	4282	74.05	1488
38.00	3390	51.10	1557	63.05	3713	75.00	4049
39.00	1536	51.85	355	64.00	318	75.95	388
39.90	27	52.70	77	64.95	798	76.80	216
44.80	200	54.70	53	66.90	195	77.05	359
45.00	543	54.95	435	68.00	8721	77.95	320
46.95	875	55.95	1320	69.05	8291	78.90	3614
47.85	441	56.95	2912	69.90	168	79.90	1057
48.10	114	57.95	177	70.05	513	80.95	3526
48.95	3878	59.95	839	71.85	657	81.85	810

Average of 12.847 to 12.859 min.: VN078062.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
82.90	83	103.70	117	128.05	191	144.70	54
86.95	3480	103.90	364	128.85	128	145.75	163
88.00	3227	104.70	159	129.10	70	146.90	52
90.60	58	105.85	442	129.85	336	147.30	51
90.90	221	115.75	266	130.80	74	147.80	157
92.00	2503	116.00	153	134.90	84	148.00	94
93.05	3697	116.70	225	136.00	86	149.70	84
94.00	11036	116.90	528	136.90	242	154.70	78
95.00	75309	117.90	490	140.90	1011	157.10	93
96.05	4748	119.00	554	141.85	208	158.80	69
102.60	66	127.80	105	142.85	1206	160.85	122

Average of 12.847 to 12.859 min.: VN078062.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
171.70	729						
172.20	262						
172.95	504						
174.00	57296						
174.95	4587						
175.95	55045						
176.95	3484						
206.95	190						
280.95	213						
281.20	235						
282.20	64						

Instrument :

MSVOA_N

ClientSampleId :

BFB