
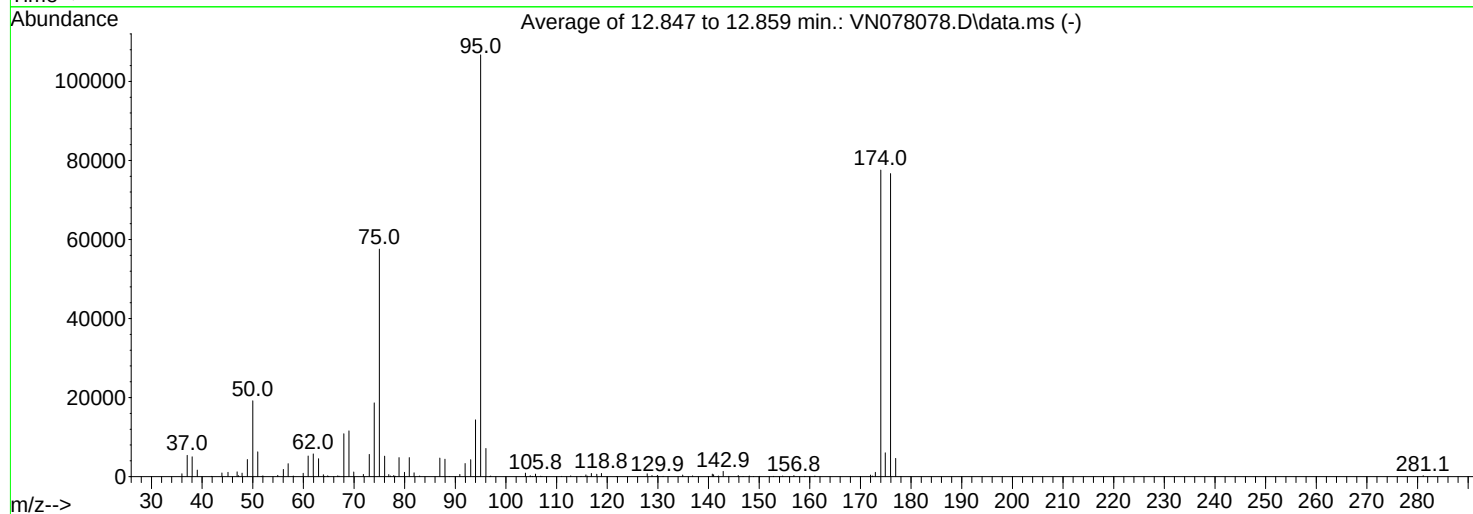


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060623\
Data File : VN078078.D
Acq On : 06 Jun 2023 20:35
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
Title : SW846 8260
Last Update : Tue May 16 04:07:42 2023

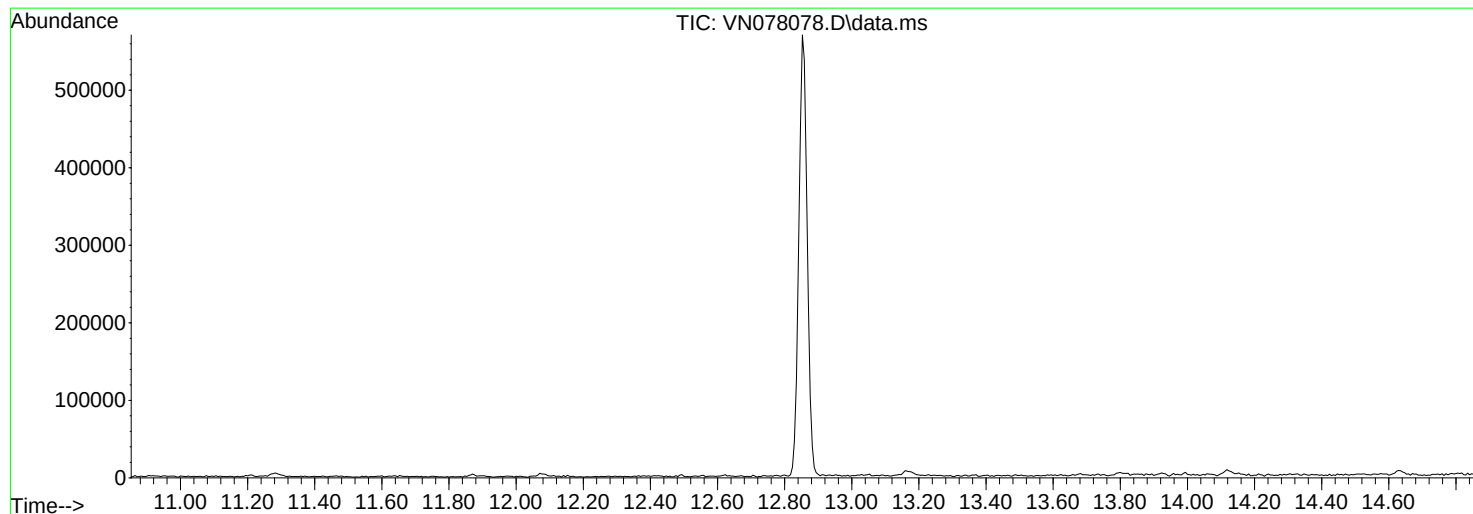

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	19211	PASS
75	95	30	60	53.9	57573	PASS
95	95	100	100	100.0	106720	PASS
96	95	5	9	6.7	7111	PASS
173	174	0.00	2	1.4	1078	PASS
174	95	50	100	72.7	77565	PASS
175	174	5	9	7.8	6037	PASS
176	174	95	101	98.8	76669	PASS
177	176	5	9	6.0	4638	PASS

Average of 12.847 to 12.859 min.: VN078078.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	750	50.00	19211	63.00	4555	73.00	5611
37.05	5404	51.00	6277	63.95	493	74.00	1868
38.05	5016	51.80	67	64.20	89	75.00	5757
39.05	1672	52.00	209	64.80	205	76.05	516
41.90	69	54.95	334	65.00	86	76.85	510
43.90	920	56.05	1832	66.80	222	77.20	174
45.10	1095	57.00	3275	67.05	119	77.85	290
46.90	1231	58.00	169	68.00	10869	78.10	139
47.20	240	59.95	868	69.00	11567	78.90	4818
47.90	881	60.95	5218	69.95	1186	79.95	1092
48.95	4349	61.95	5751	71.85	579	80.90	4832

Average of 12.847 to 12.859 min.: VN078078.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.85	977	96.80	52	115.80	439	134.90	400
82.95	182	97.00	145	116.10	140	136.85	215
86.95	4713	103.85	886	116.85	810	140.75	648
87.95	4424	104.80	254	117.95	598	141.00	487
88.80	51	105.20	81	118.85	823	141.80	53
90.90	568	105.85	671	121.90	55	141.95	157
91.95	3312	106.85	131	127.90	719	142.90	1327
93.05	4312	107.10	72	128.85	280	144.00	85
94.00	14371	111.00	66	129.80	134	145.85	302
95.00	106720	112.80	206	129.95	308	146.80	57
96.05	7111	114.80	92	131.00	76	148.05	161

Average of 12.847 to 12.859 min.: VN078078.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
148.90	50	174.90	6037				
150.10	103	175.95	76669				
152.80	76	176.95	4638				
154.65	179	178.00	62				
156.85	302	281.10	261				
159.00	79						
161.00	154						
172.00	406						
172.40	151						
172.95	1078						
174.00	77565						

Instrument :

MSVOA_N

ClientSampleId :

BFB