


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060625\
Data File : VN086861.D
Acq On : 06 Jun 2025 07:59
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060625W.M
Title : SW846 8260
Last Update : Sat Jun 07 02:12:50 2025

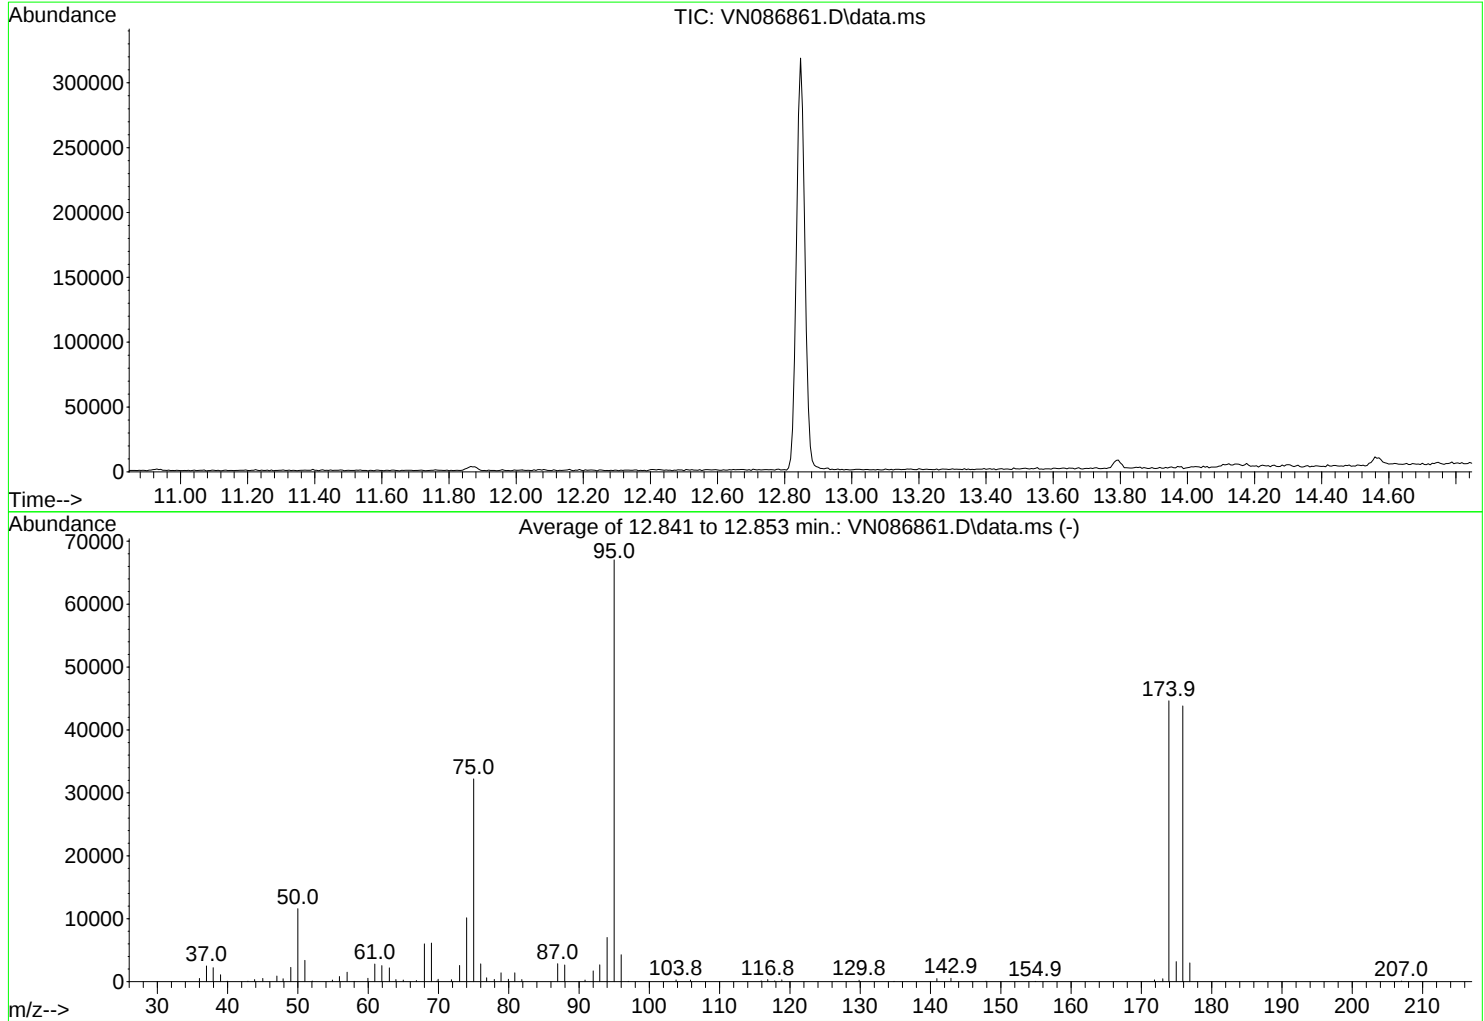

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.3	11610	PASS
75	95	30	60	48.1	32235	PASS
95	95	100	100	100.0	67037	PASS
96	95	5	9	6.4	4284	PASS
173	174	0.00	2	1.0	453	PASS
174	95	50	100	66.6	44632	PASS
175	174	5	9	7.1	3184	PASS
176	174	95	101	98.1	43805	PASS
177	176	5	9	6.8	2979	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	508	50.00	11610	63.95	331	76.00	281
37.00	2495	51.00	3387	65.00	260	76.85	60
37.95	2209	52.05	112	66.85	177	77.95	34
39.00	1096	54.90	253	68.00	6008	78.90	141
39.95	84	55.90	806	69.00	6141	79.95	395
42.90	88	57.00	1501	69.80	100	80.85	1397
43.85	329	58.00	50	69.95	383	81.85	328
45.00	512	59.95	526	71.85	297	86.95	2851
47.00	882	60.95	2806	73.00	2562	87.95	2646
47.90	460	61.95	2535	74.00	10138	90.85	264
49.00	2276	63.00	2195	75.00	32235	92.00	1704

Average of 12.841 to 12.853 min.: VN086861.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.95	2660	129.85	228	175.90	43805		
94.00	7029	134.80	66	176.90	2979		
95.00	67037	140.90	488	207.00	111		
96.00	4284	142.90	542				
97.00	57	145.90	54				
103.80	279	147.90	82				
105.85	267	154.90	64				
115.90	128	171.85	288				
116.85	345	173.05	453				
117.85	116	173.90	44632				
118.85	274	174.95	3184				

Instrument :

MSVOA_N

ClientSampleId :

BFB