

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN060719\  
Data File : VN056070.D  
Acq On : 7 Jun 2019 2:14  
Operator : JC/SP  
Sample : K3190-22  
Misc : 5.00mL/MSVOA N/WATER  
ALS Vial : 43 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BPS1-TT-MW307I-20190604

## Integration Parameters: RTEINT.P

Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N060419W.M  
Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 7.590       | 1790          | 1809        | 1820         | rBV      | 202757         | 499388        | 30.51%          | 6.354%        |
| 2         | 7.664       | 1820          | 1832        | 1863         | rVB      | 359295         | 858513        | 52.45%          | 10.923%       |
| 3         | 8.027       | 1928          | 1945        | 1971         | rBV      | 211517         | 493356        | 30.14%          | 6.277%        |
| 4         | 8.583       | 2102          | 2118        | 2150         | rBV      | 521570         | 1098312       | 67.10%          | 13.974%       |
| 5         | 10.088      | 2571          | 2586        | 2618         | rBV      | 858726         | 1636879       | 100.00%         | 20.827%       |
| 6         | 11.406      | 2982          | 2996        | 3033         | rBV      | 758439         | 1359890       | 83.08%          | 17.303%       |
| 7         | 12.400      | 3292          | 3305        | 3327         | rBV      | 585352         | 1017725       | 62.17%          | 12.949%       |
| 8         | 13.342      | 3584          | 3598        | 3620         | rBV      | 524376         | 895388        | 54.70%          | 11.393%       |


Sum of corrected areas: 7859451

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN060719\  
Data File : VN056070.D  
Acq On : 7 Jun 2019 2:14  
Operator : JC/SP  
Sample : K3190-22  
Misc : 5.00mL/MSVOA N/WATER  
ALS Vial : 43 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BPS1-TT-MW307I-20190604

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_N\METHODS\82N060419W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

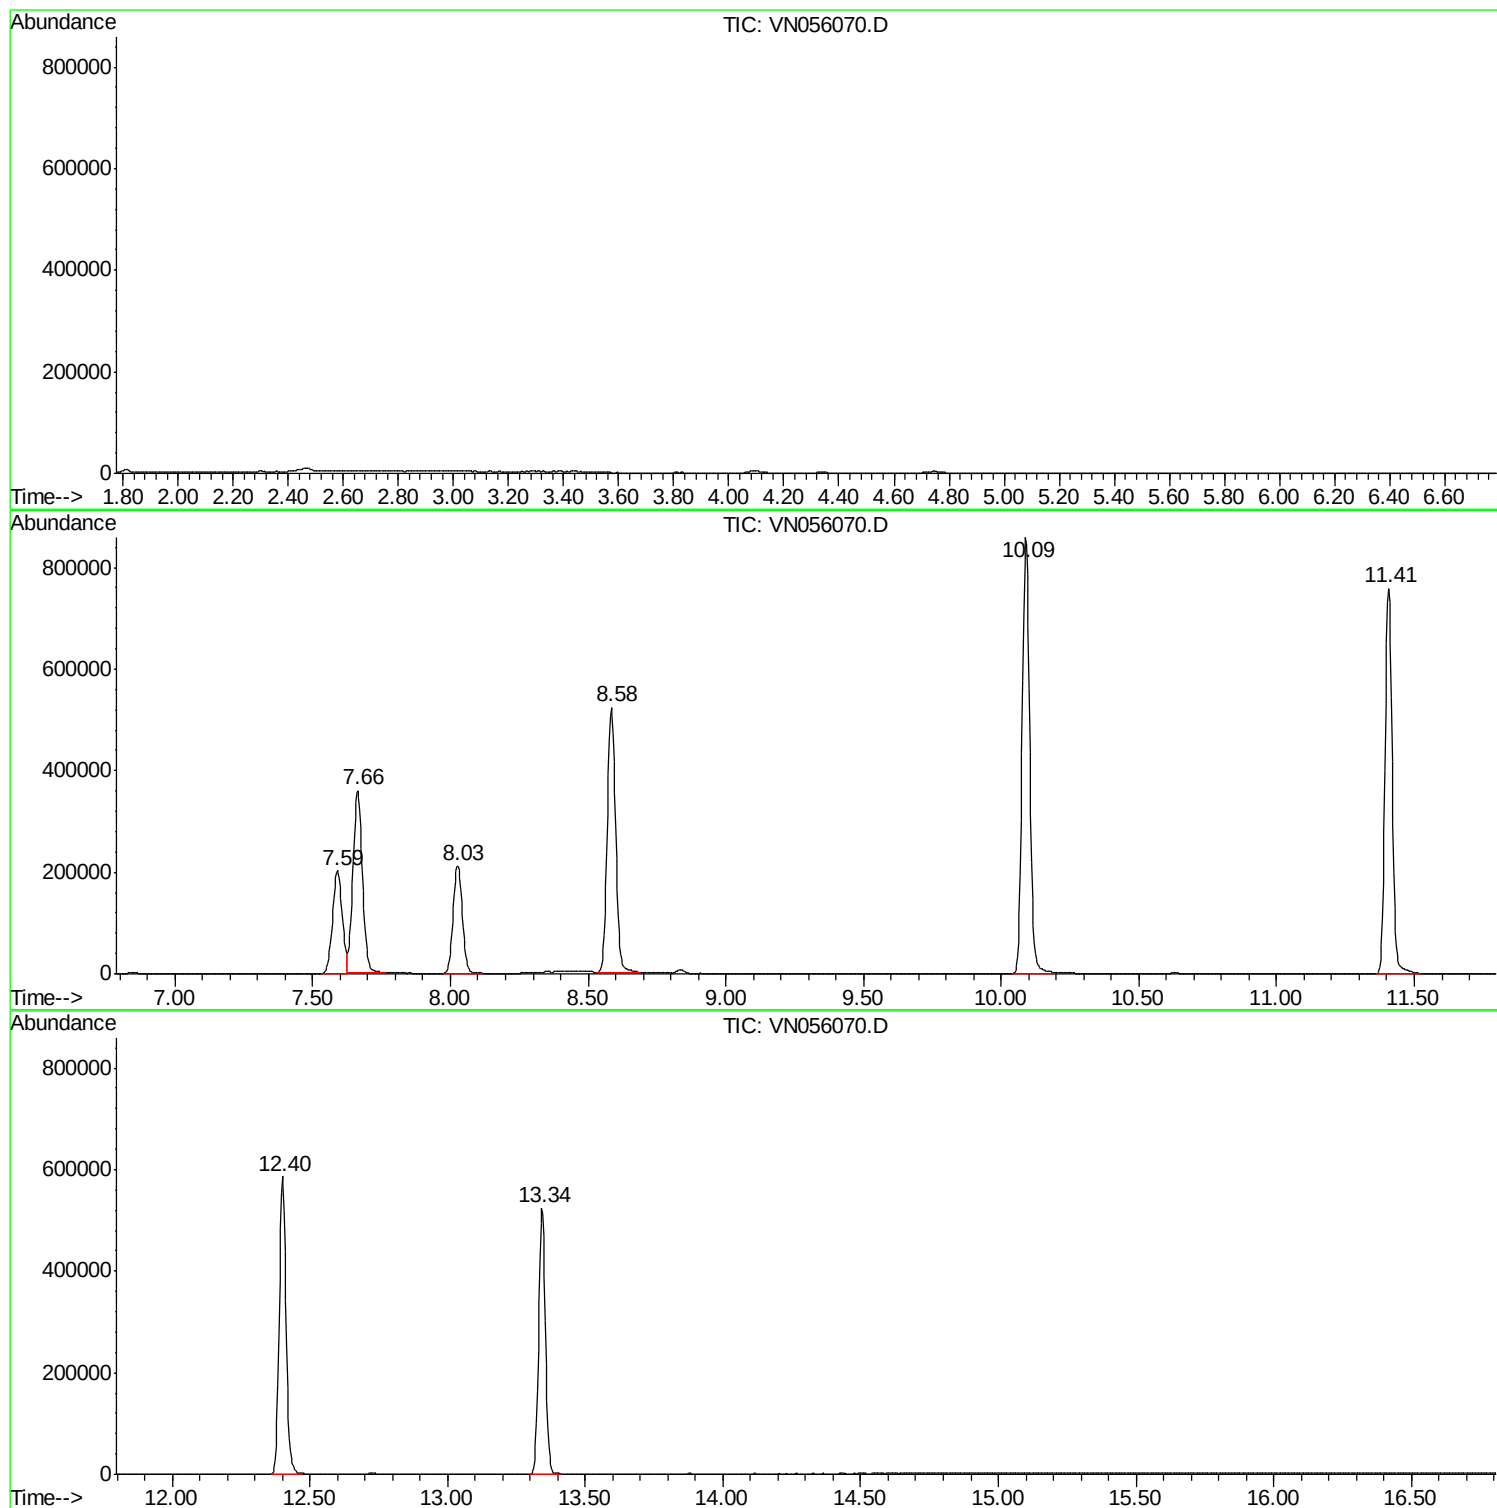

Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_N\DATA\VN060719\  
Data File : VN056070.D  
Acq On : 7 Jun 2019 2:14  
Operator : JC/SP  
Sample : K3190-22  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 43 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BPS1-TT-MW307I-20190604

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N060419W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_N\DATA\VN060719\  
Data File : VN056070.D  
Acq On : 7 Jun 2019 2:14  
Operator : JC/SP  
Sample : K3190-22  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 43 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BPS1-TT-MW307I-20190604

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N060419W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |