


Bromomethane


Response Ratio

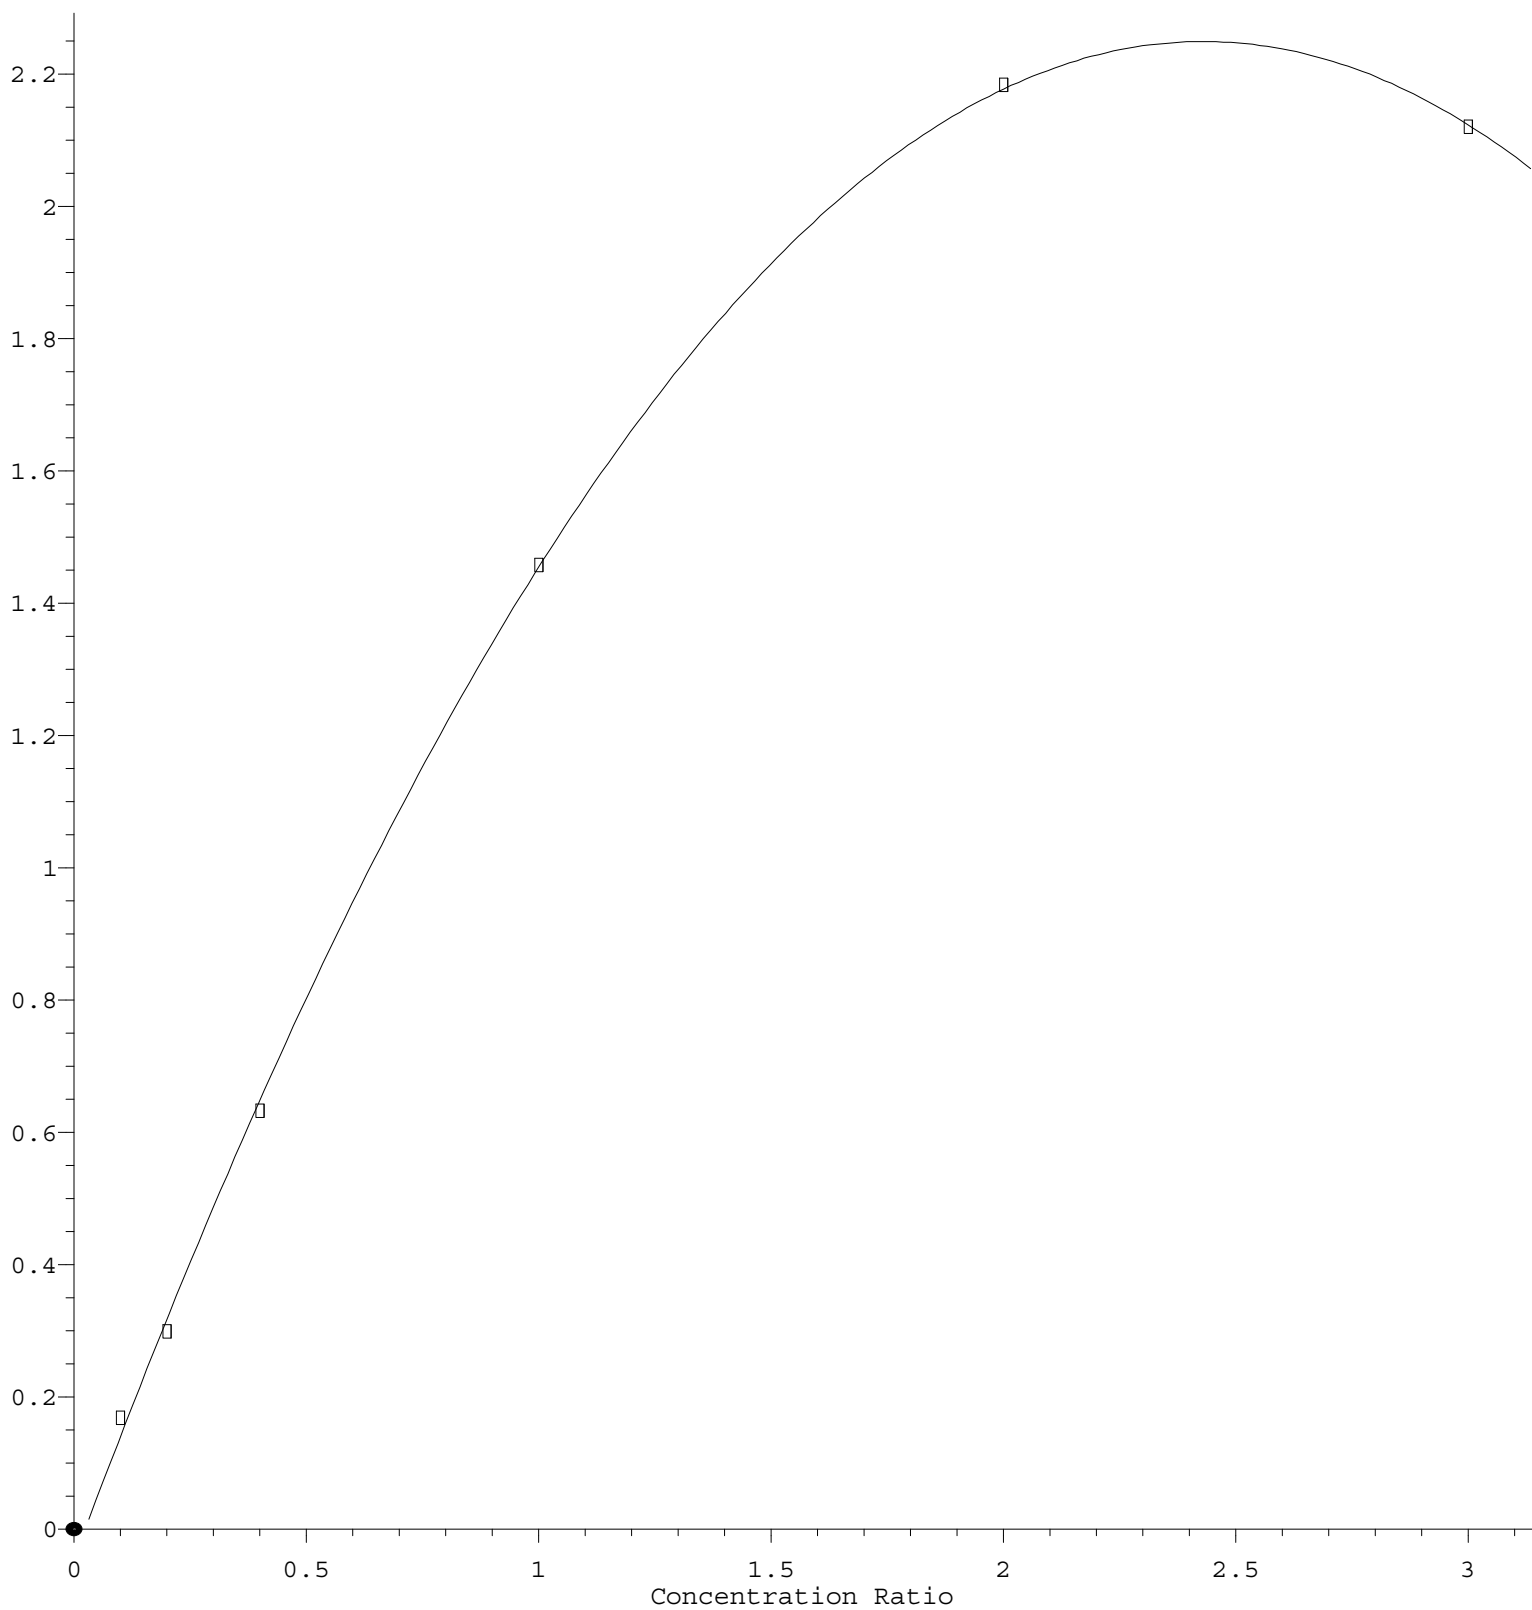

$R = -3.883e-001 A^2 + 1.888e+000 A - 4.442e-002$
 Coef of Det (r^2) = 0.999647 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N060721W.M
 Calibration Table Last Updated: Mon Jun 07 16:11:37 2021

Chloroethane


Response Ratio

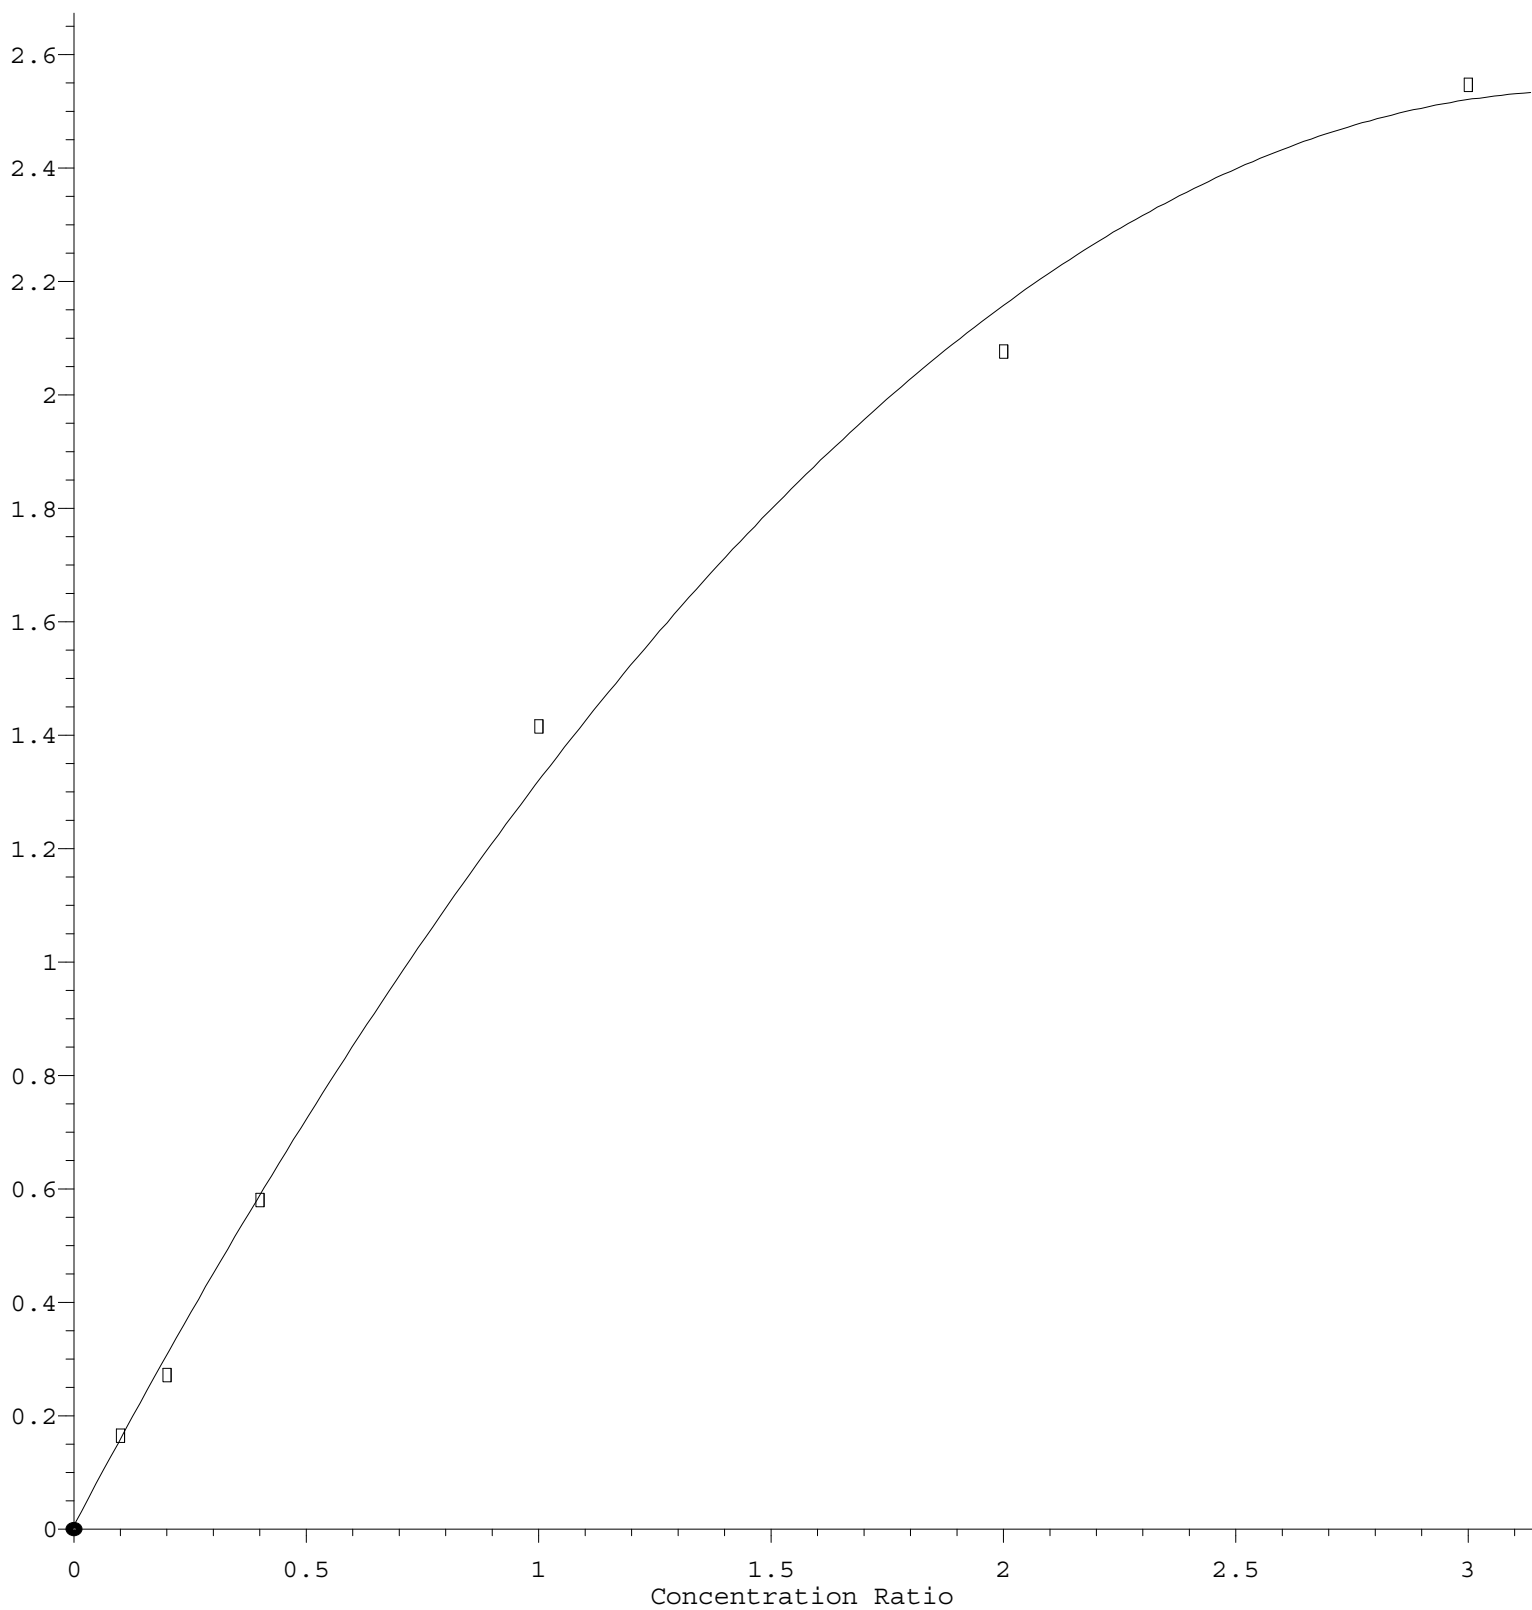

$R = -2.375e-001 A^2 + 1.550e+000 A + 7.037e-003$
Coef of Det (r^2) = 0.996399 Curve Fit: Quadratic
Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N060721W.M
Calibration Table Last Updated: Mon Jun 07 16:11:37 2021

Trichlorofluoromethane


Response Ratio

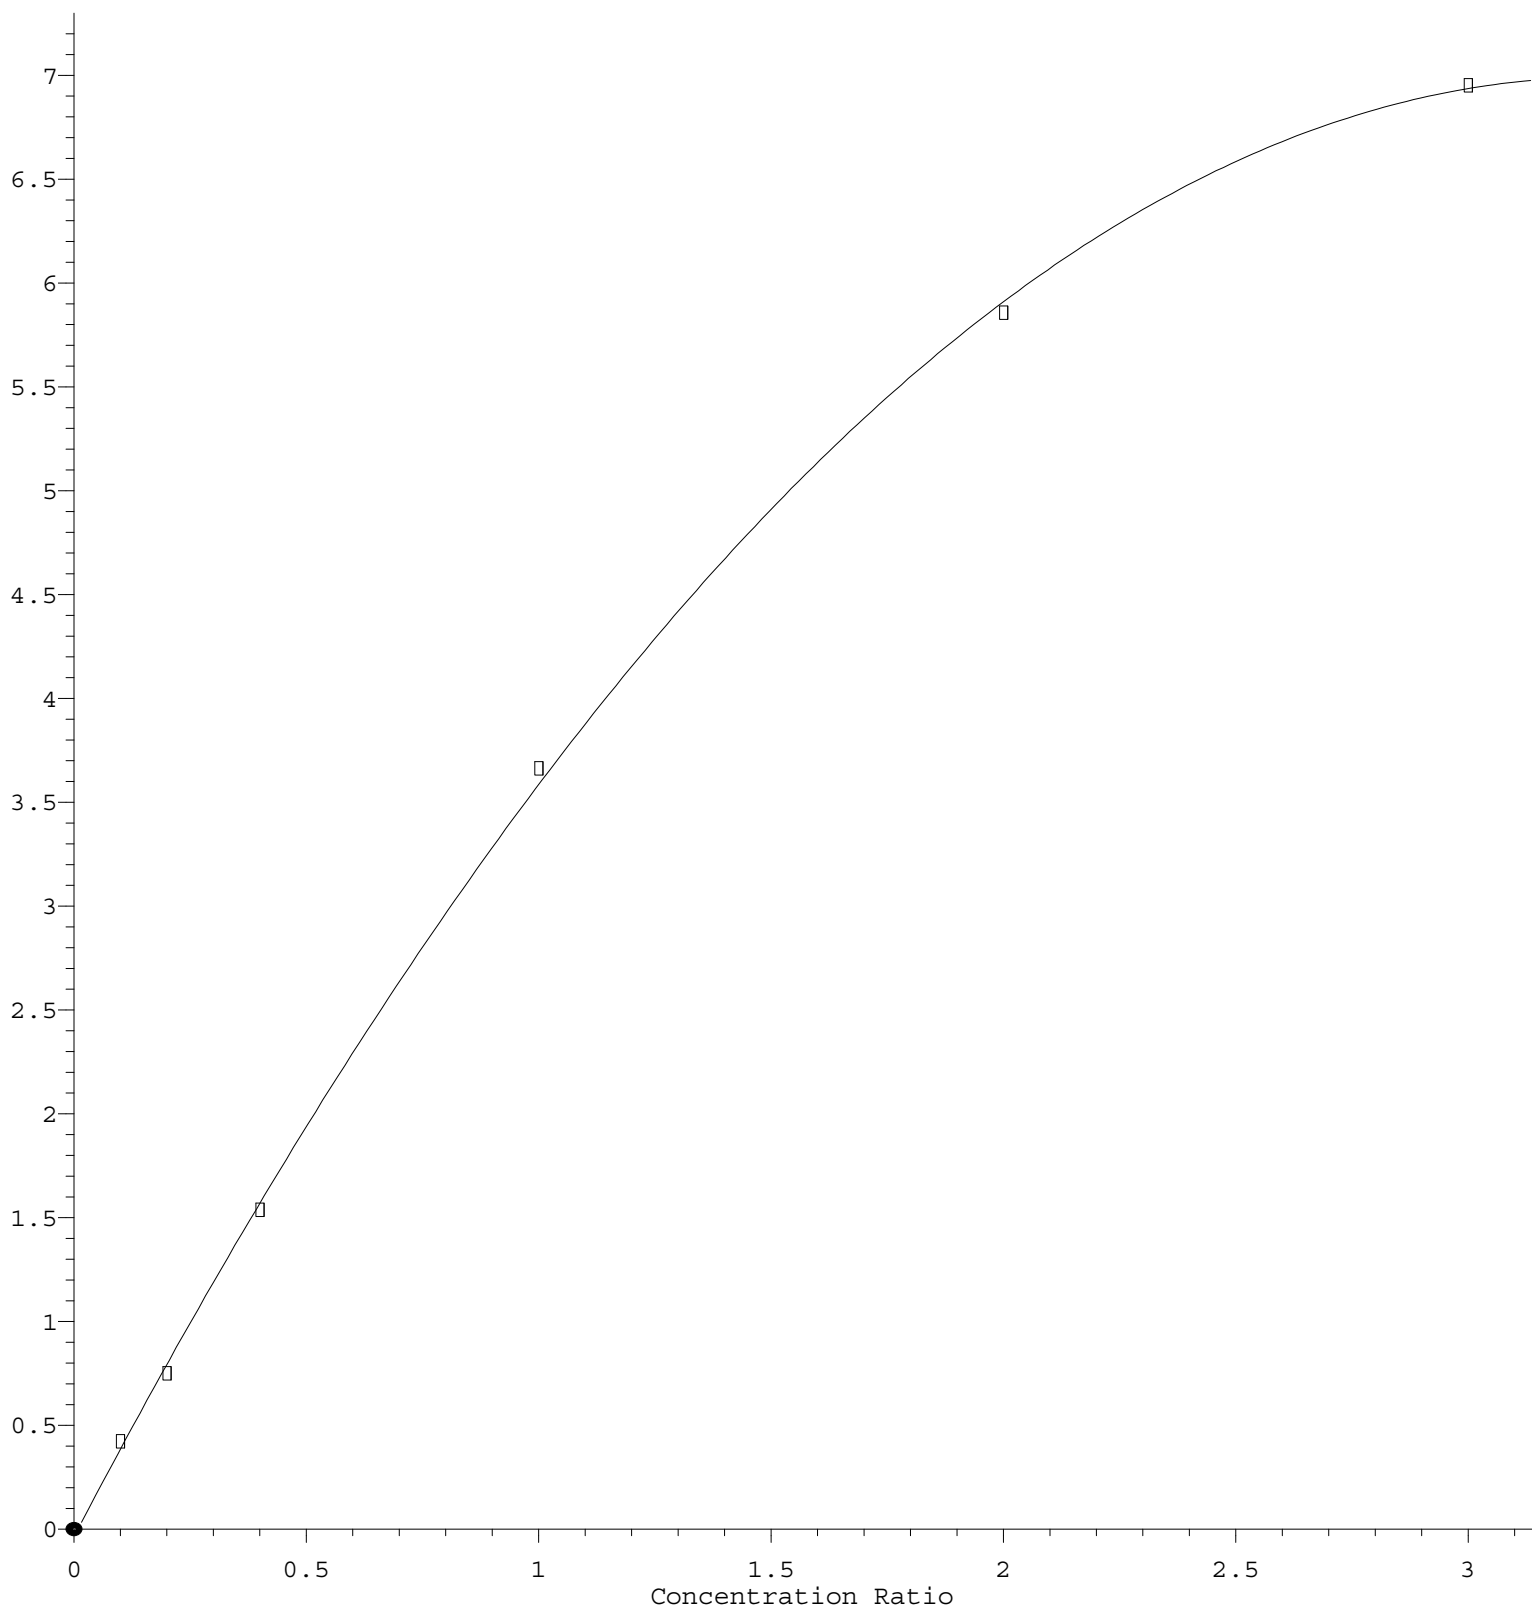

$R = -6.484e-001 A^2 + 4.269e+000 A - 3.404e-002$
 Coef of Det (r^2) = 0.999652 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N060721W.M
 Calibration Table Last Updated: Mon Jun 07 16:11:37 2021

Diethyl Ether


Response Ratio

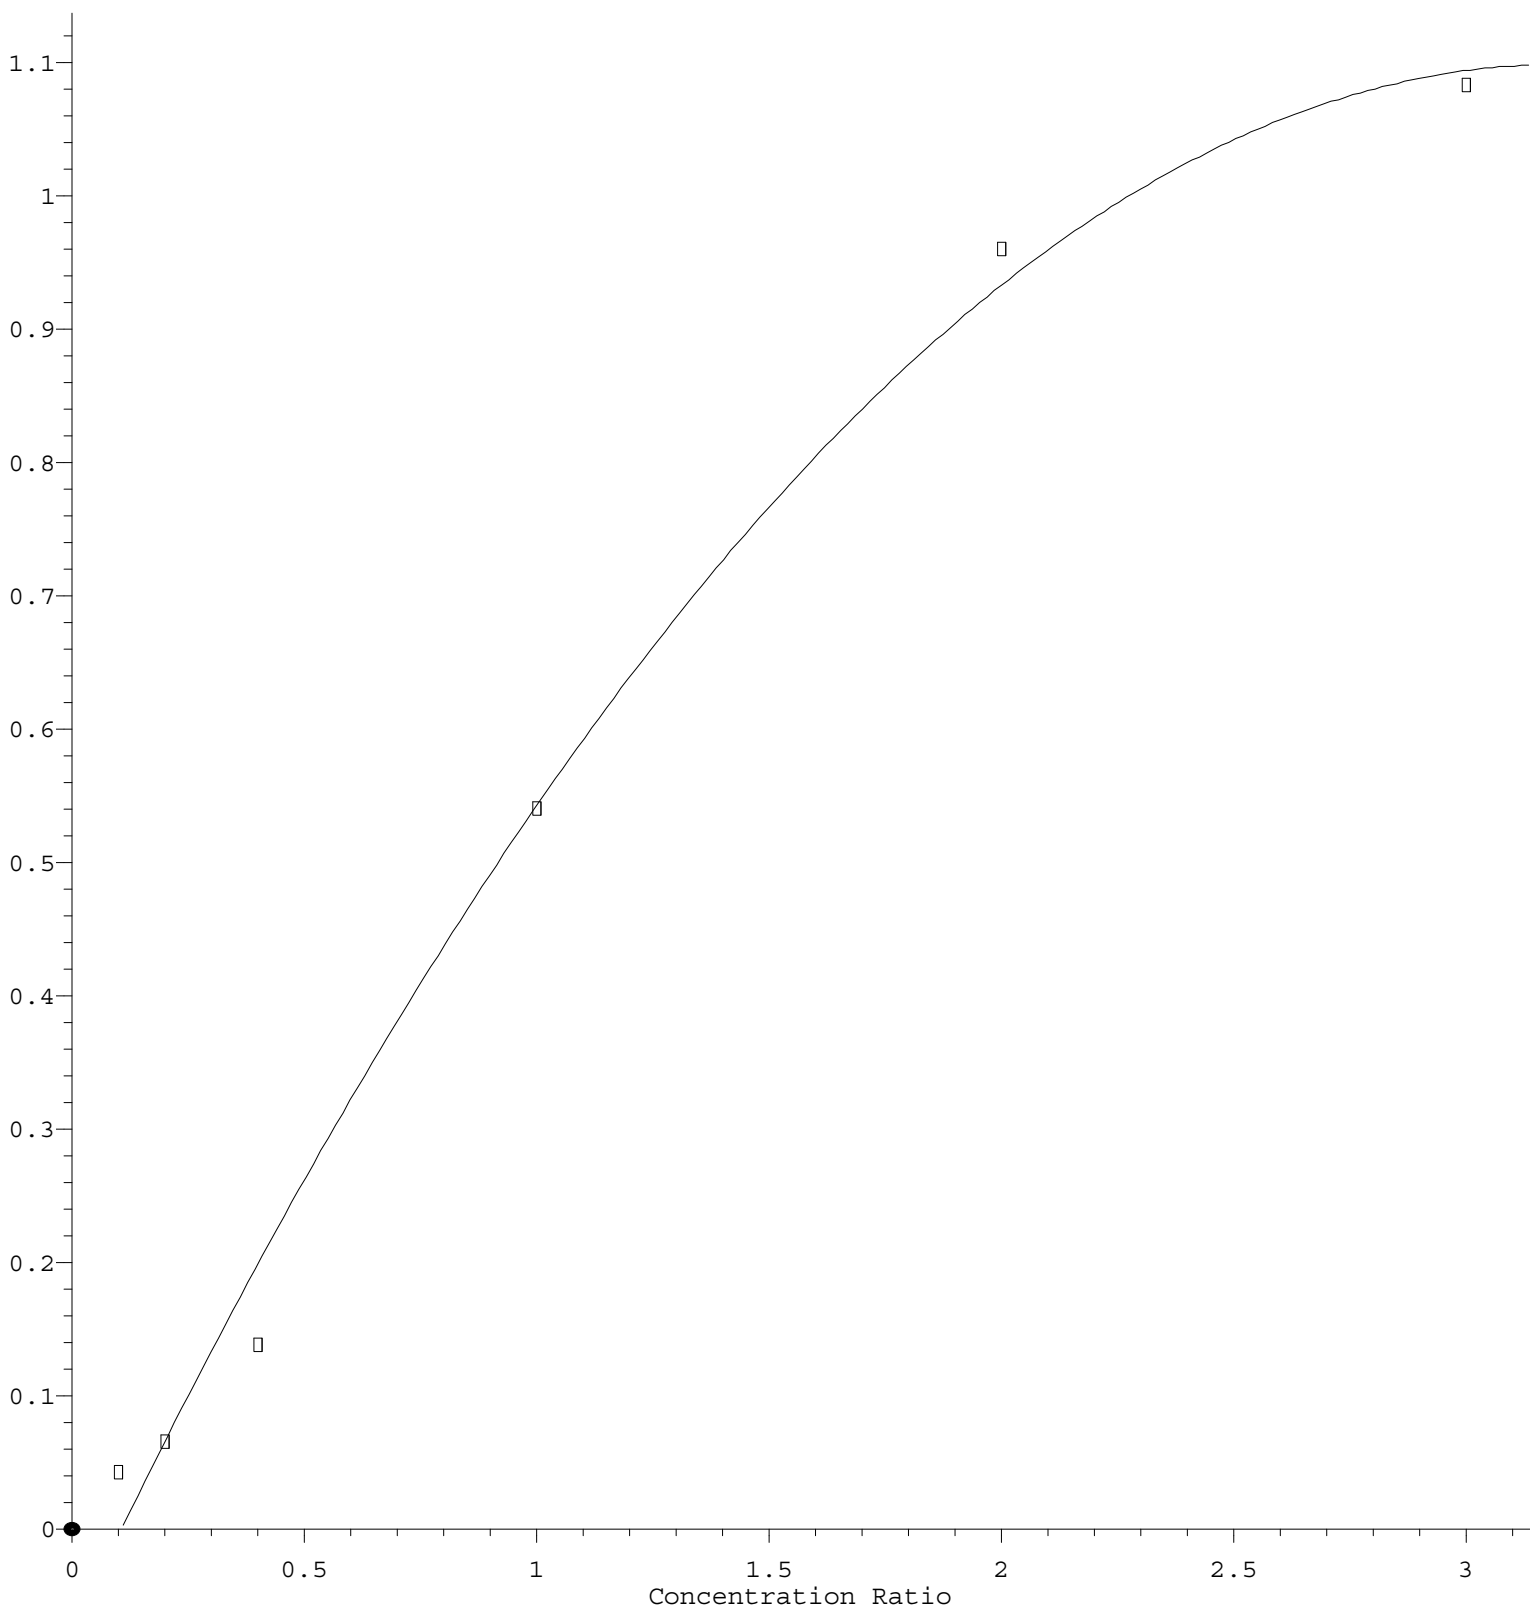

$R = -1.146e-001 A^2 + 7.337e-001 A - 7.632e-002$
 Coef of Det (r^2) = 0.993766 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N060721W.M
 Calibration Table Last Updated: Mon Jun 07 16:11:37 2021

Toluene-d8

Response Ratio

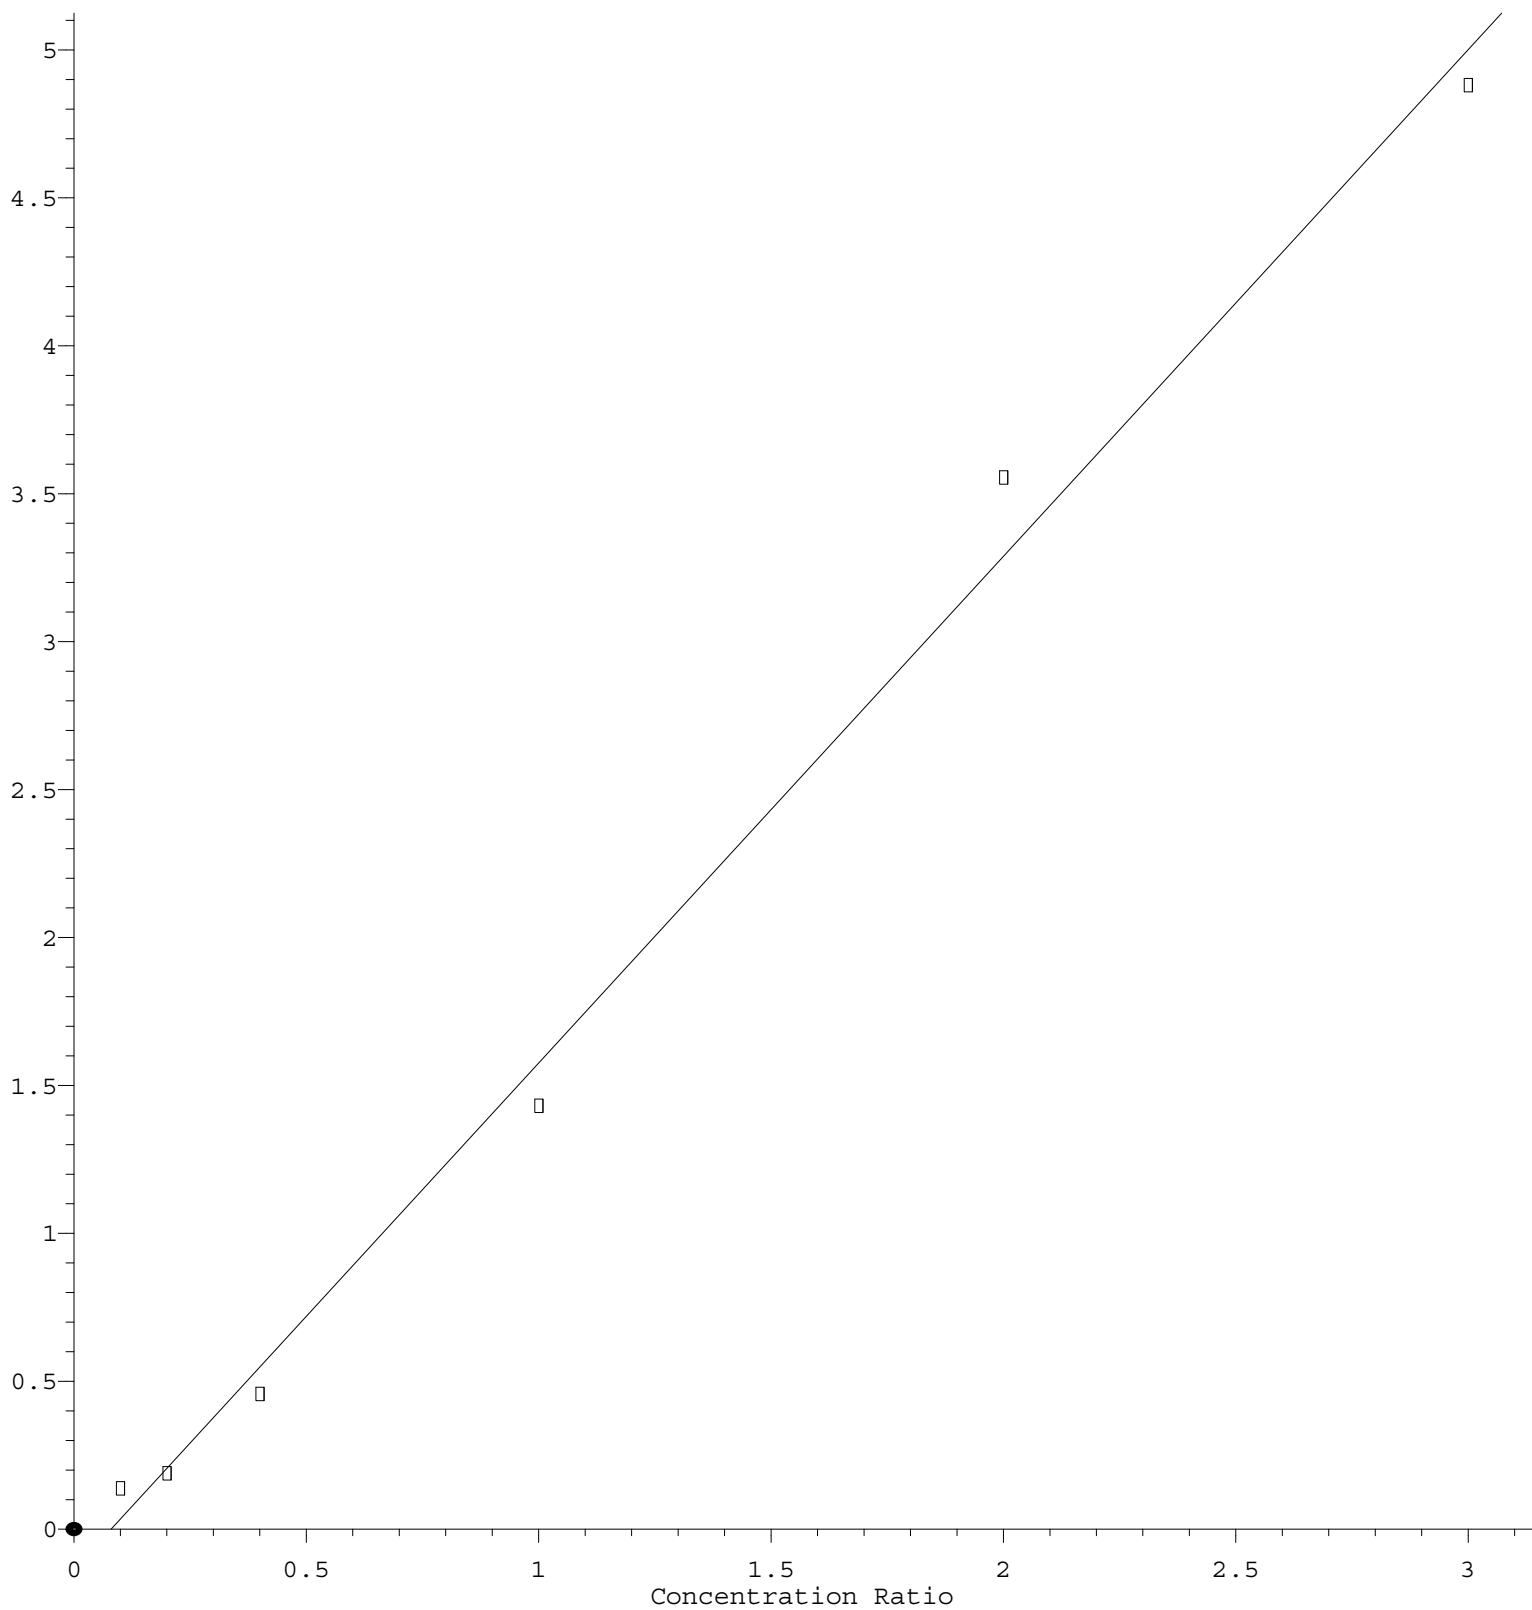

$$\text{Response} = 1.713\text{e}+000 * \text{Amt} - 1.376\text{e}-001$$


Coef of Det (r^2) = 0.993668 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N060721W.M

Calibration Table Last Updated: Mon Jun 07 16:11:37 2021

Toluene


Response Ratio

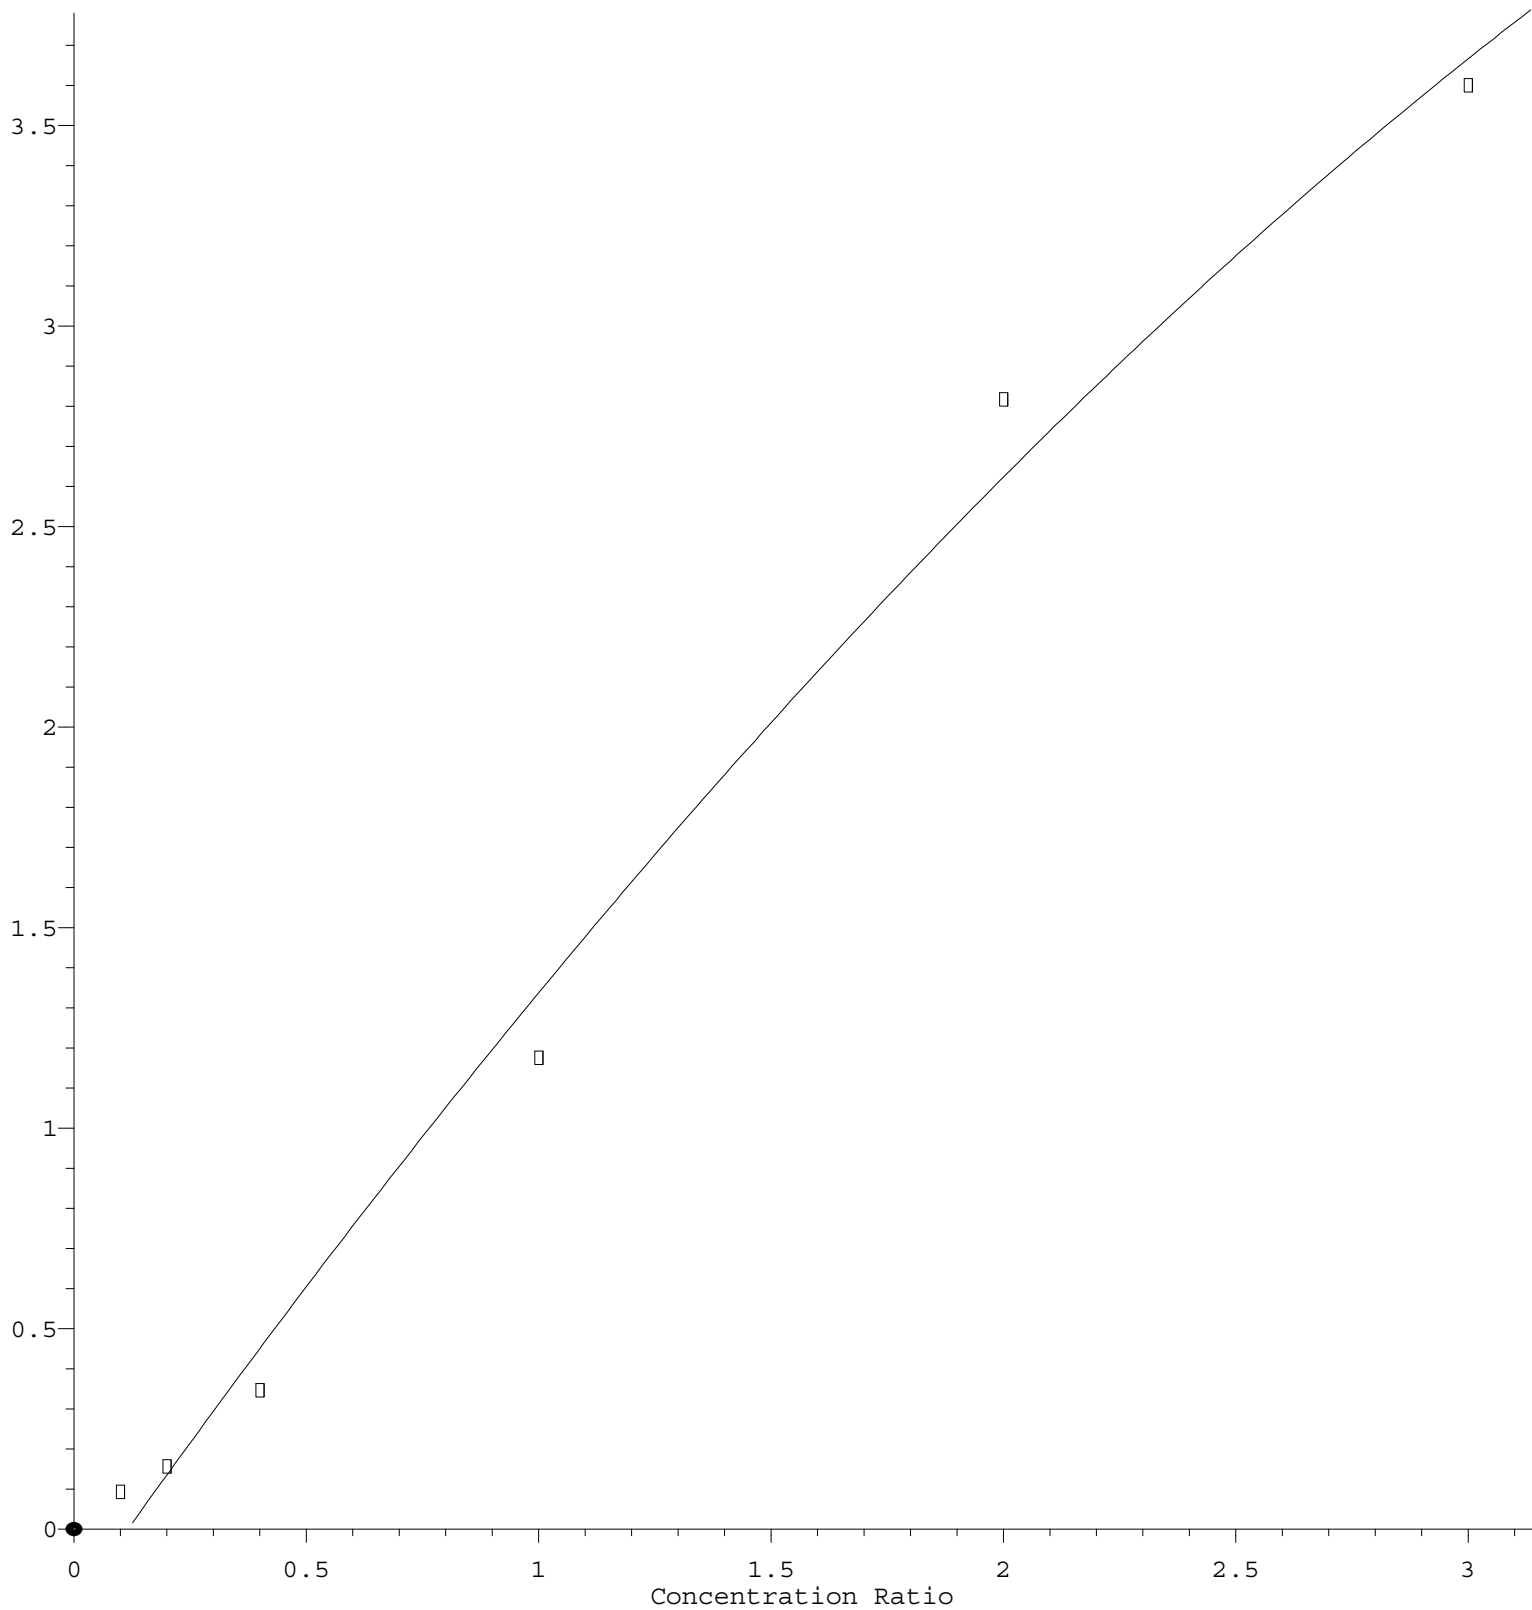

$R = -1.210e-001 A^2 + 1.648e+000 A - 1.894e-001$
 Coef of Det (r^2) = 0.991673 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N060721W.M
 Calibration Table Last Updated: Mon Jun 07 16:11:37 2021

Ethyl methacrylate


Response Ratio

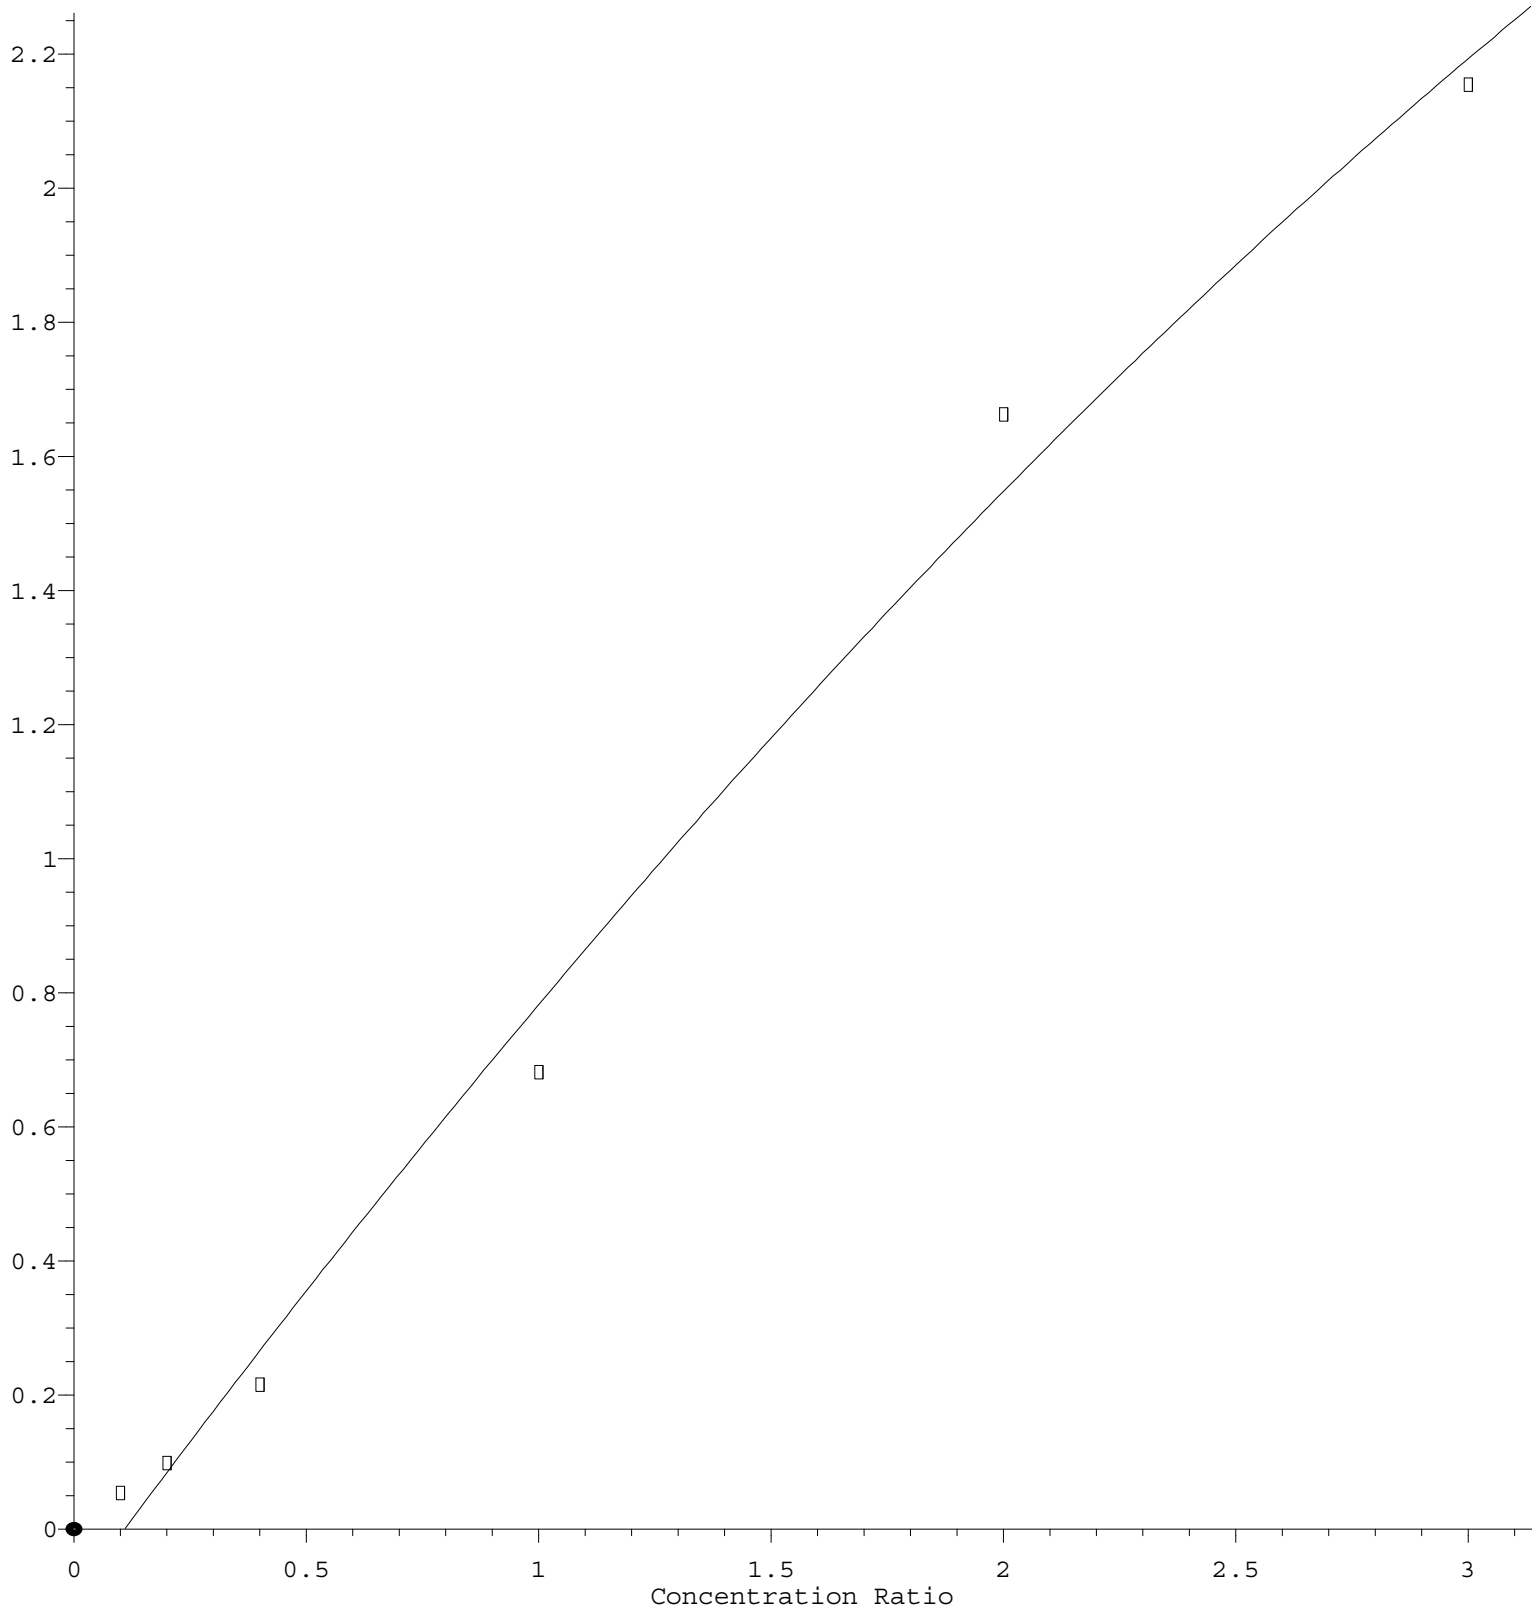

$R = -5.989e-002 A^2 + 9.448e-001 A - 1.021e-001$
Coef of Det (r^2) = 0.992077 Curve Fit: Quadratic
Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N060721W.M
Calibration Table Last Updated: Mon Jun 07 16:11:37 2021

2-Chloroethyl Vinyl ether

Response Ratio

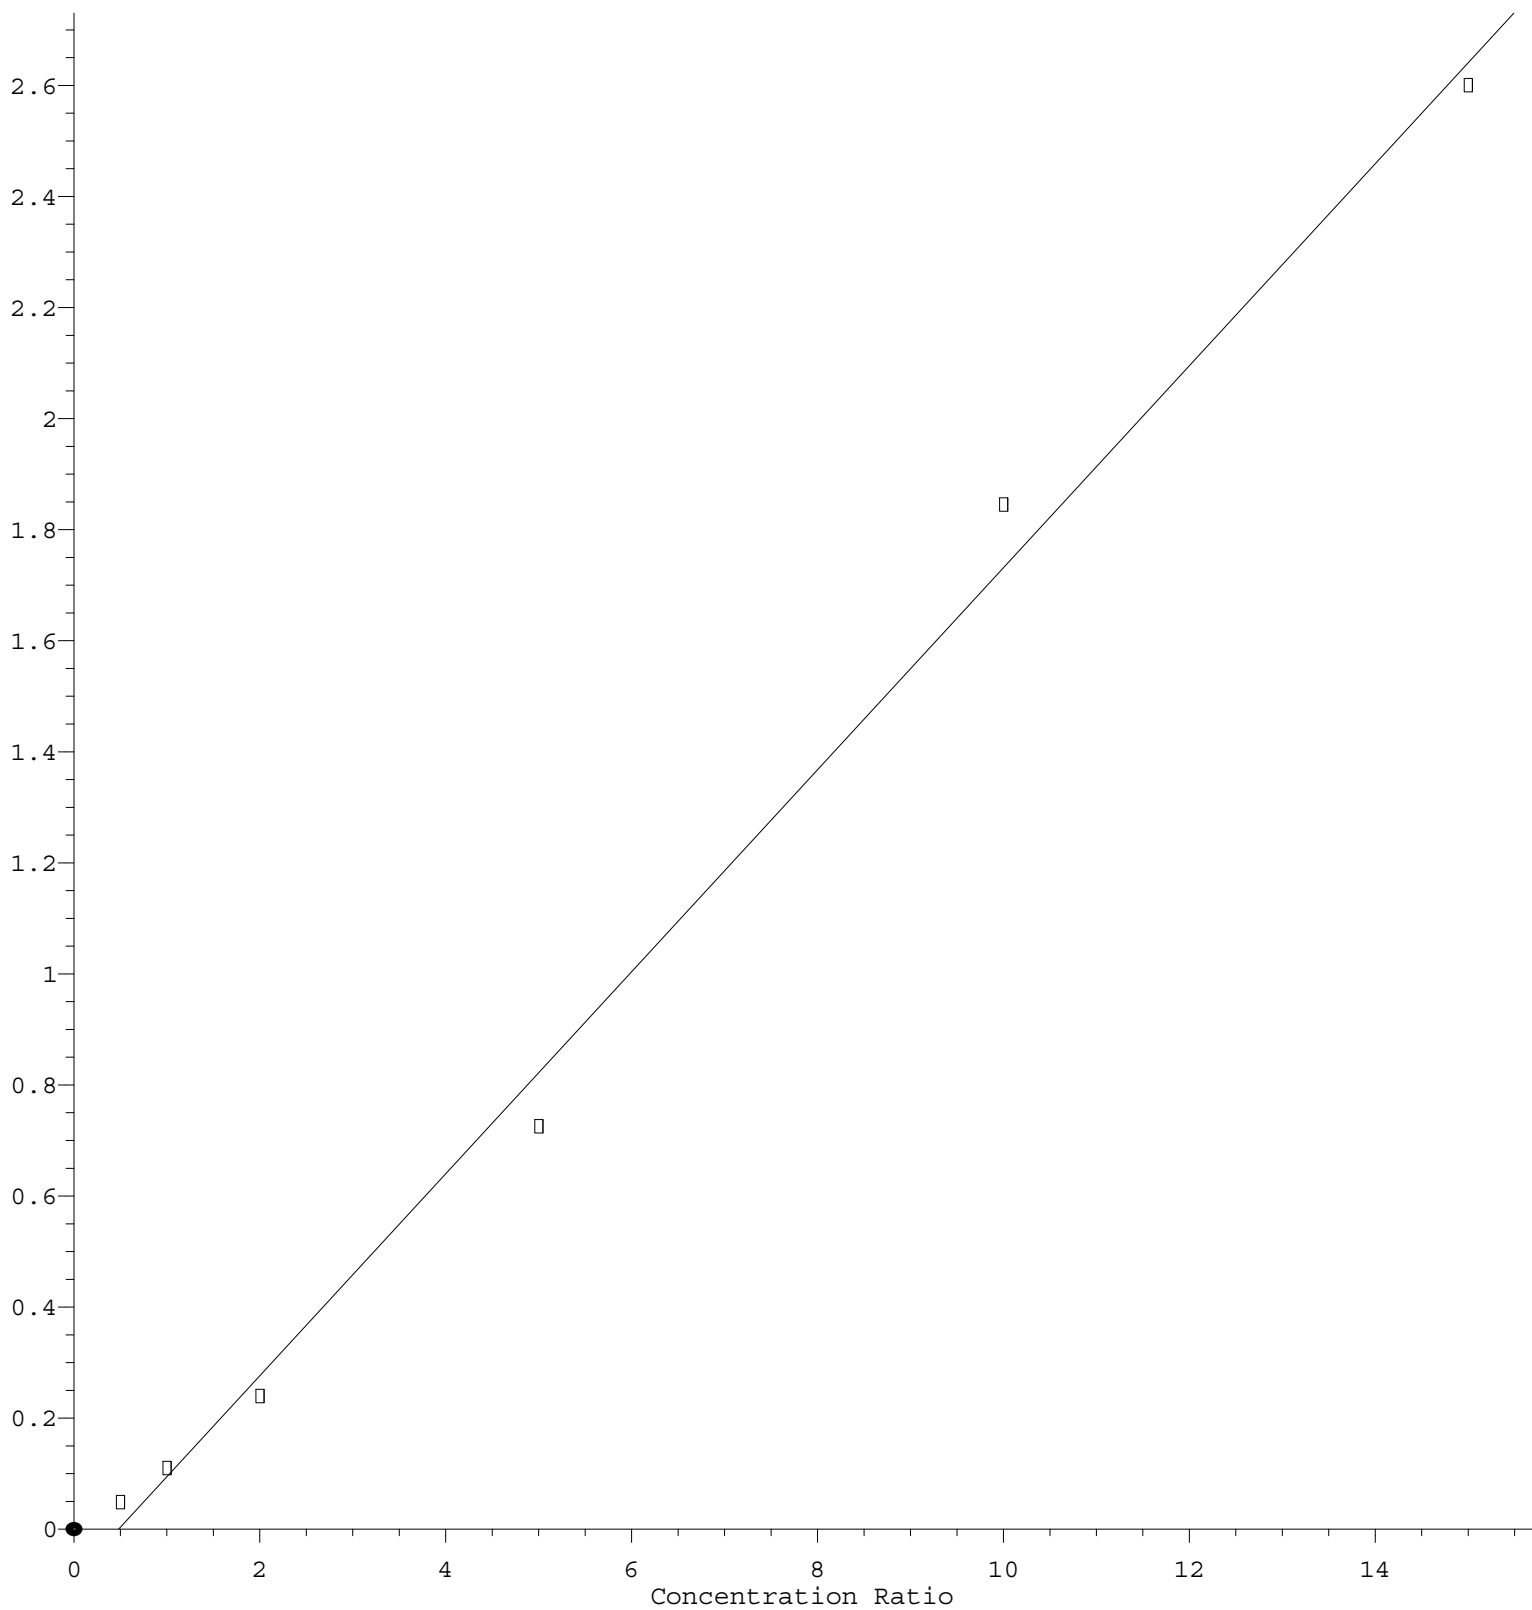

$$\text{Response} = 1.819\text{e-}001 * \text{Amt} - 8.758\text{e-}002$$


Coef of Det (r^2) = 0.995084 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N060721W.M

Calibration Table Last Updated: Mon Jun 07 16:11:37 2021

Dibromochloromethane


Response Ratio

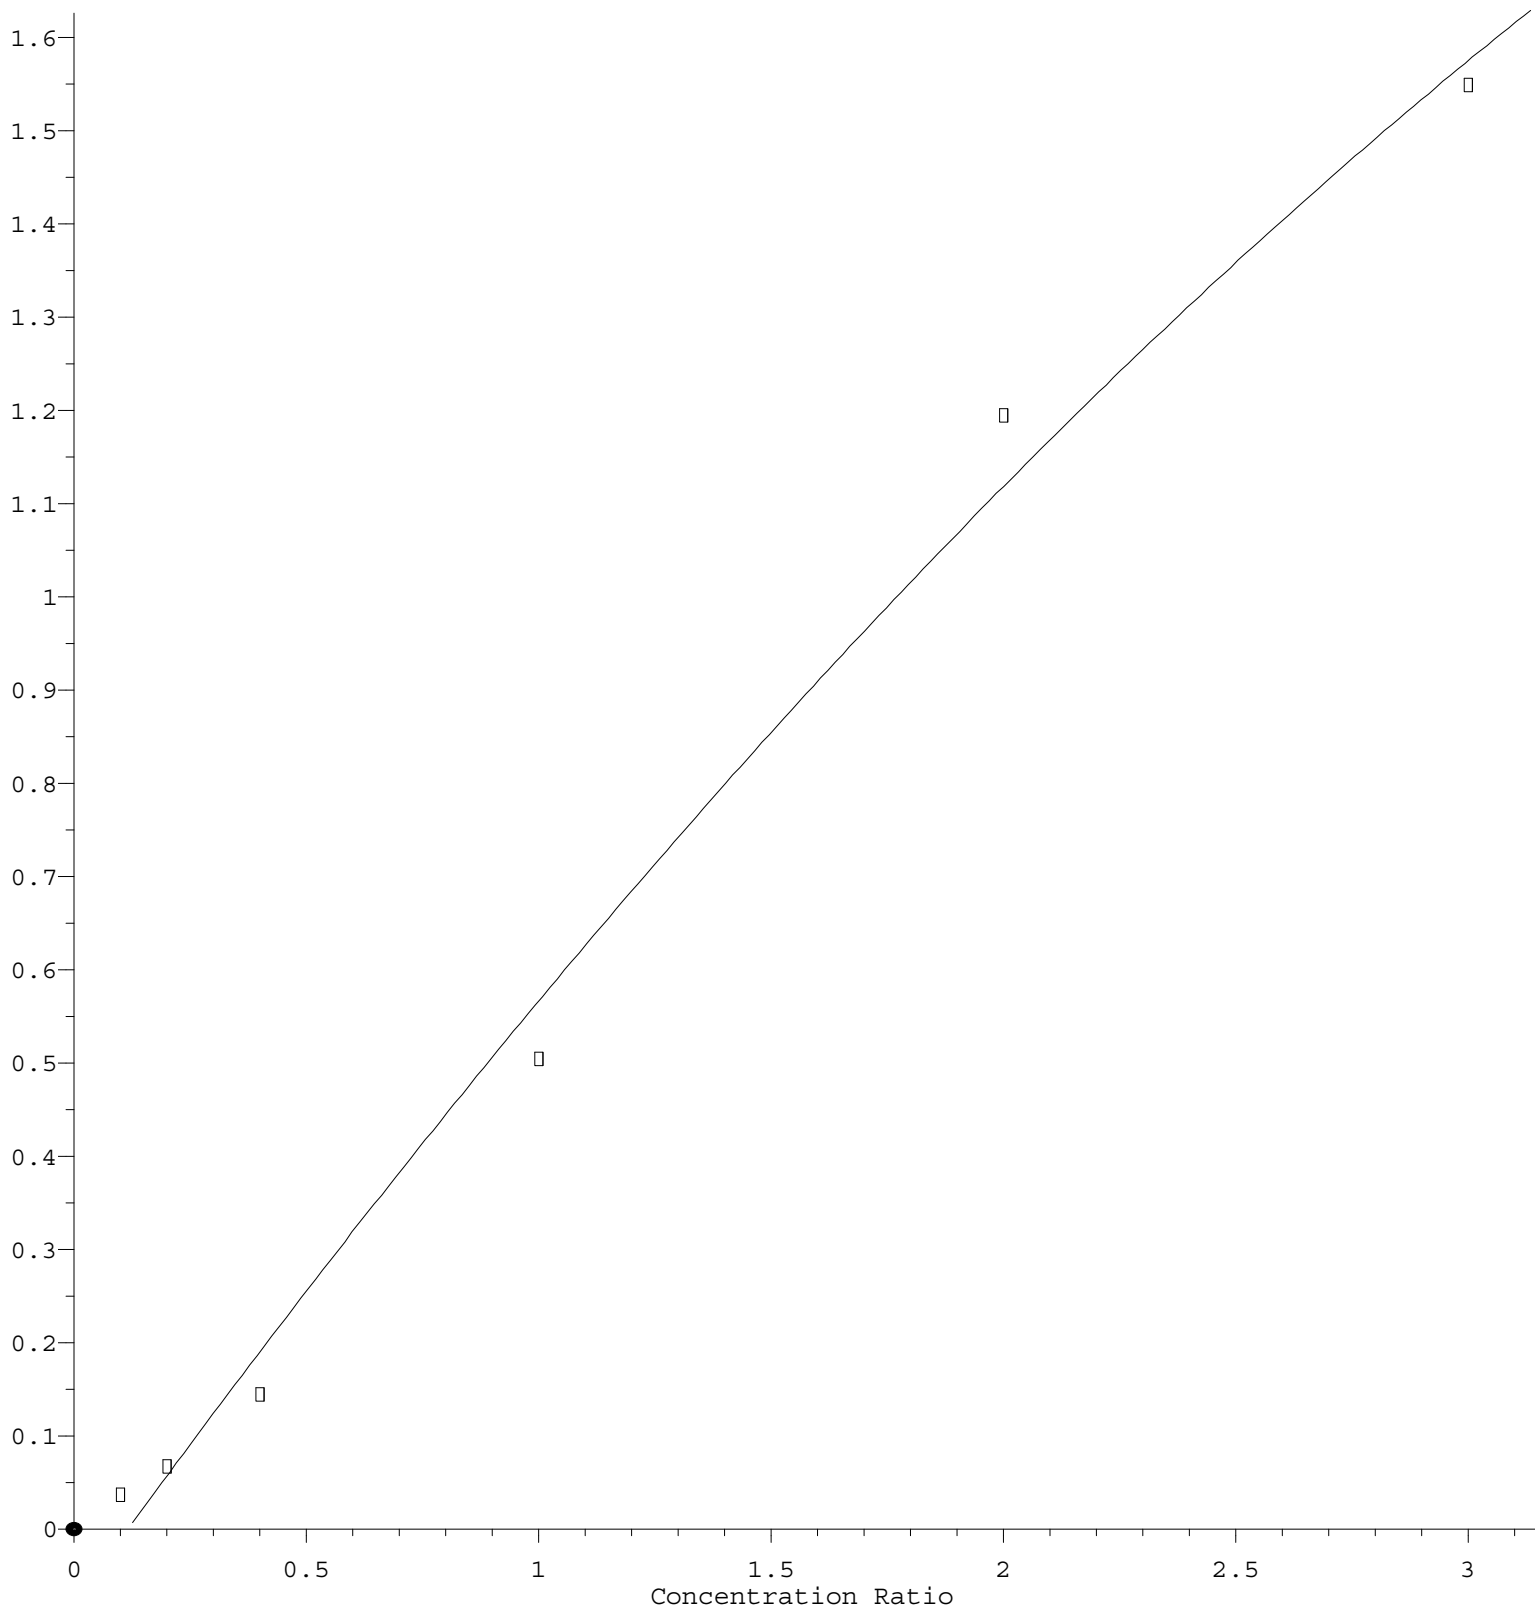

$R = -4.743e-002 A^2 + 6.940e-001 A - 7.981e-002$
 Coef of Det (r^2) = 0.992816 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N060721W.M
 Calibration Table Last Updated: Mon Jun 07 16:11:37 2021

4-Bromofluorobenzene

Response Ratio

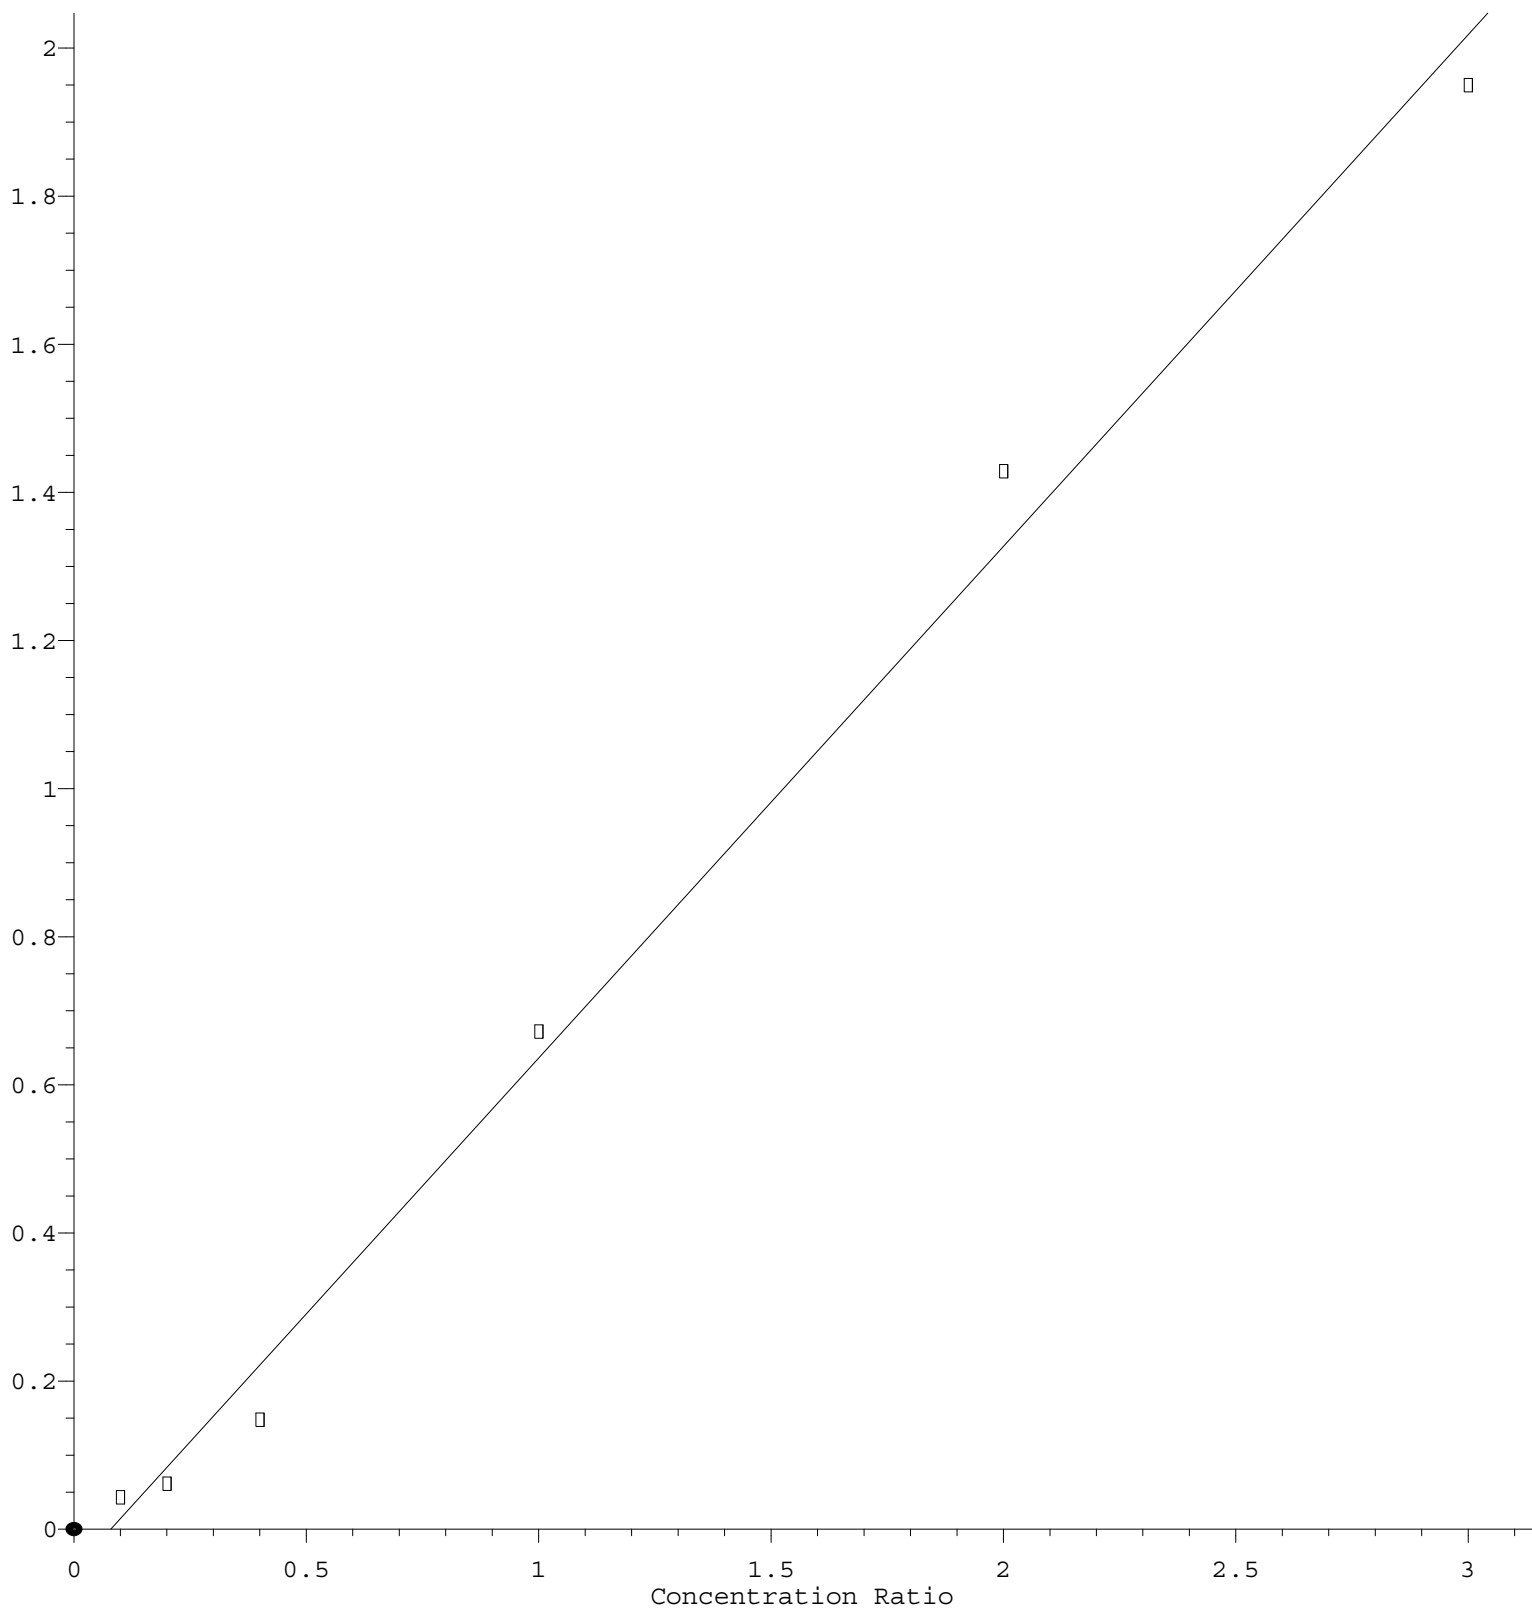

$$\text{Response} = 6.911\text{e-}001 * \text{Amt} - 5.465\text{e-}002$$


Coef of Det (r^2) = 0.992918 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N060721W.M

Calibration Table Last Updated: Mon Jun 07 16:11:37 2021

Styrene

Response Ratio

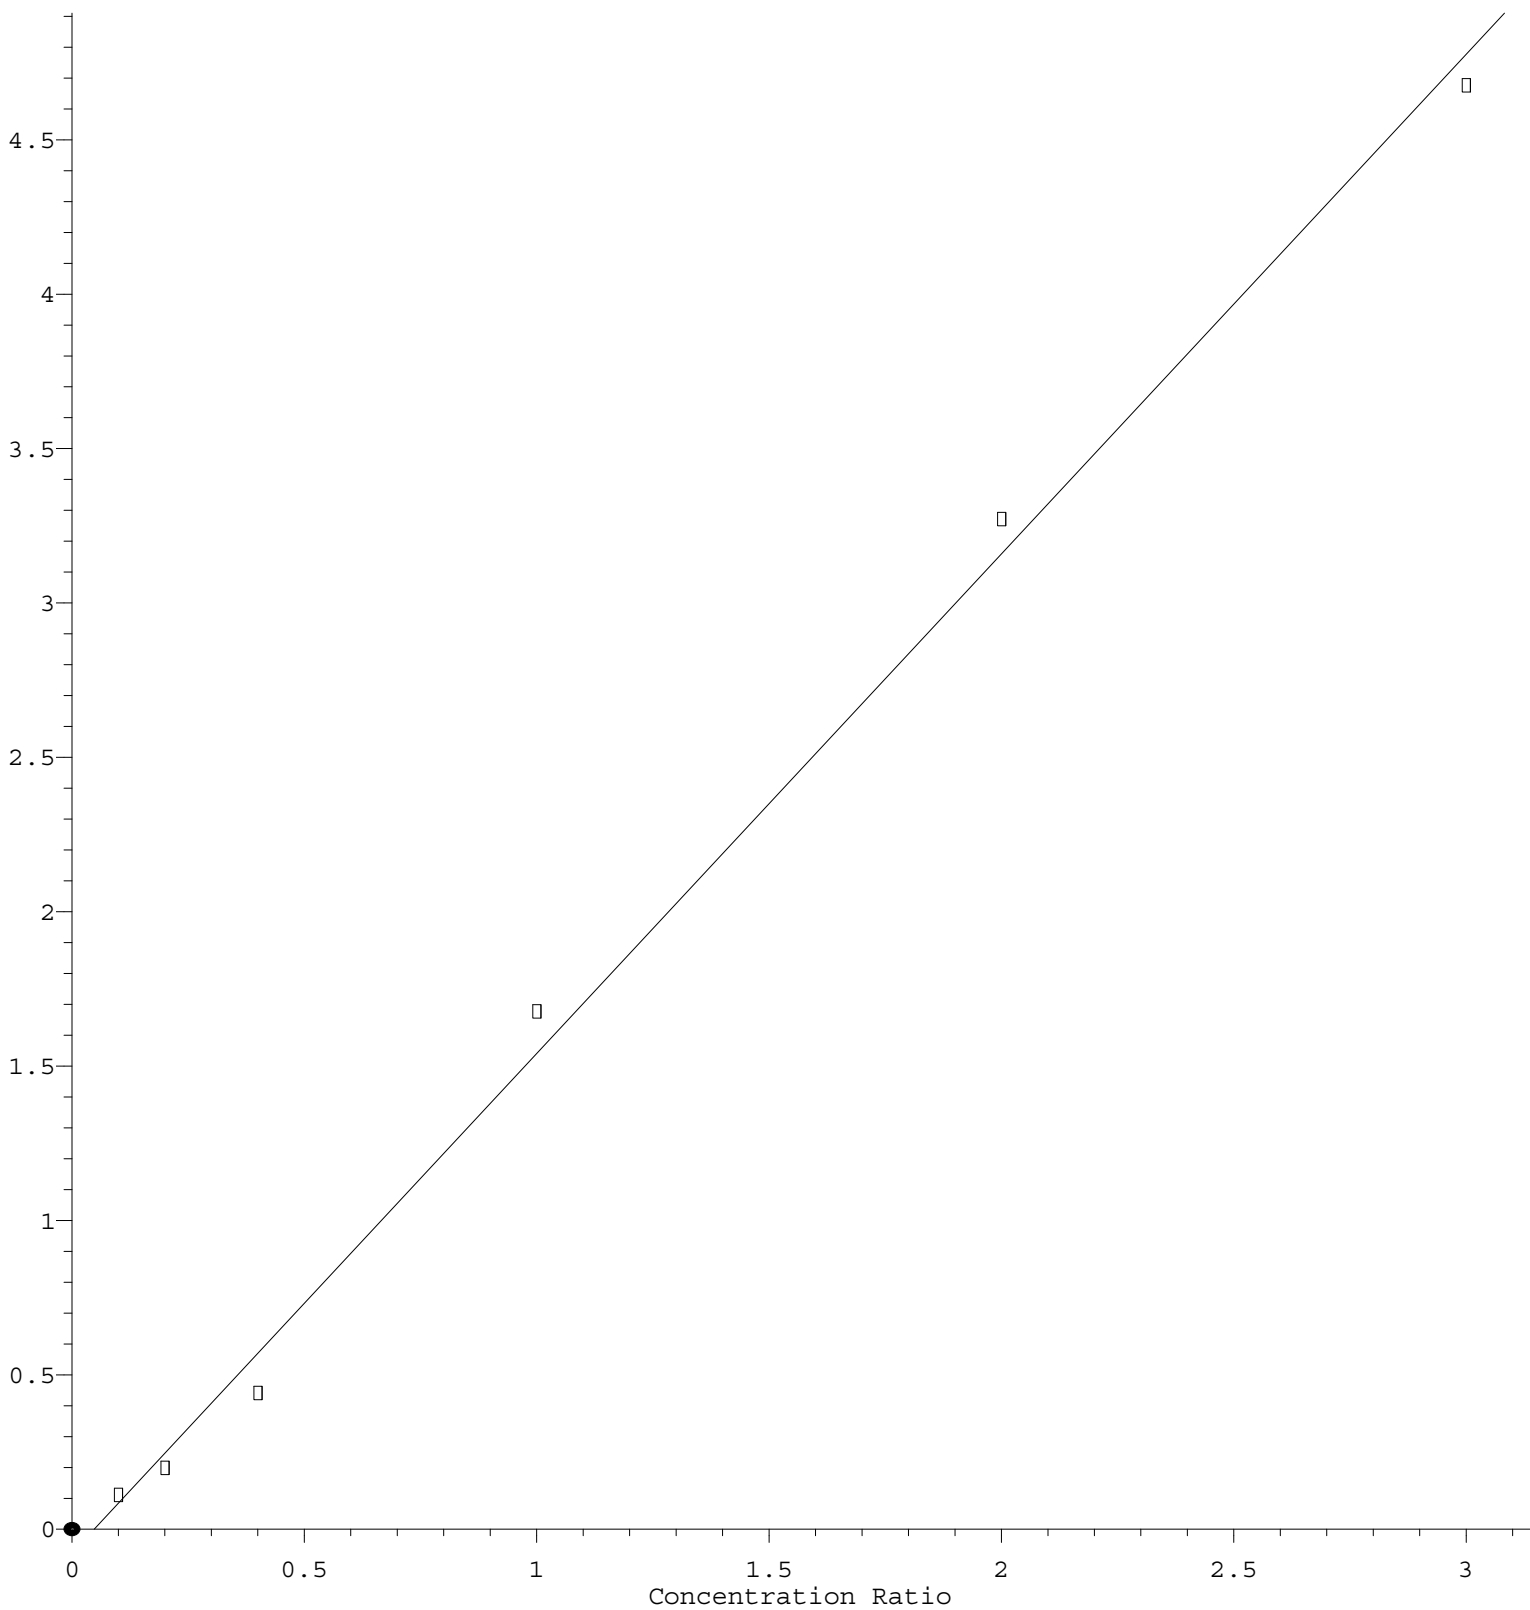

$$\text{Response} = 1.619\text{e}+000 * \text{Amt} - 7.835\text{e}-002$$


Coef of Det (r^2) = 0.996558 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N060721W.M

Calibration Table Last Updated: Mon Jun 07 16:11:37 2021

Bromoform

Response Ratio

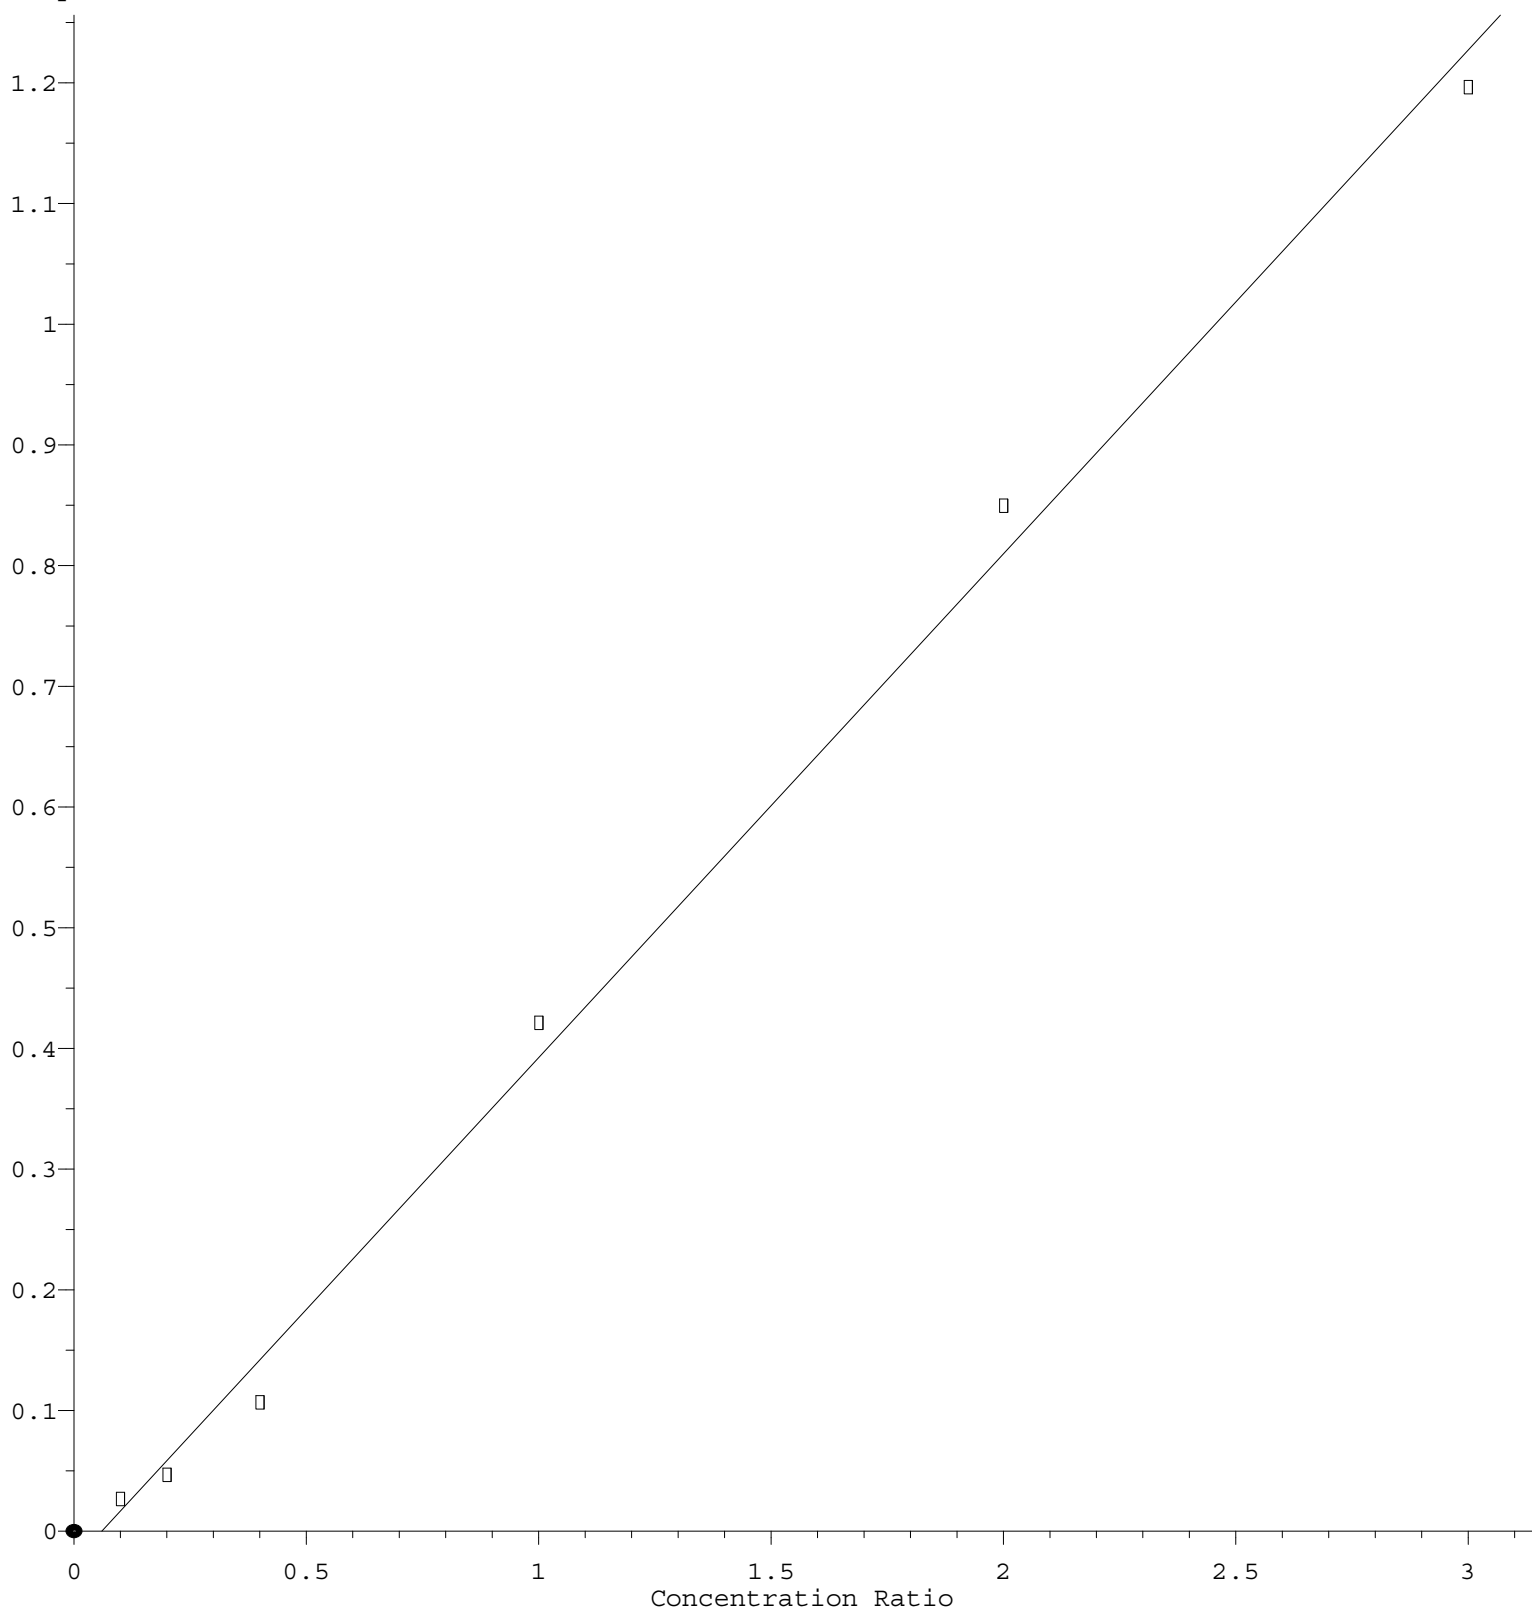

$$\text{Response} = 4.174\text{e-}001 * \text{Amt} - 2.492\text{e-}002$$

Coef of Det (r^2) = 0.995893 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N060721W.M

Calibration Table Last Updated: Mon Jun 07 16:11:37 2021