
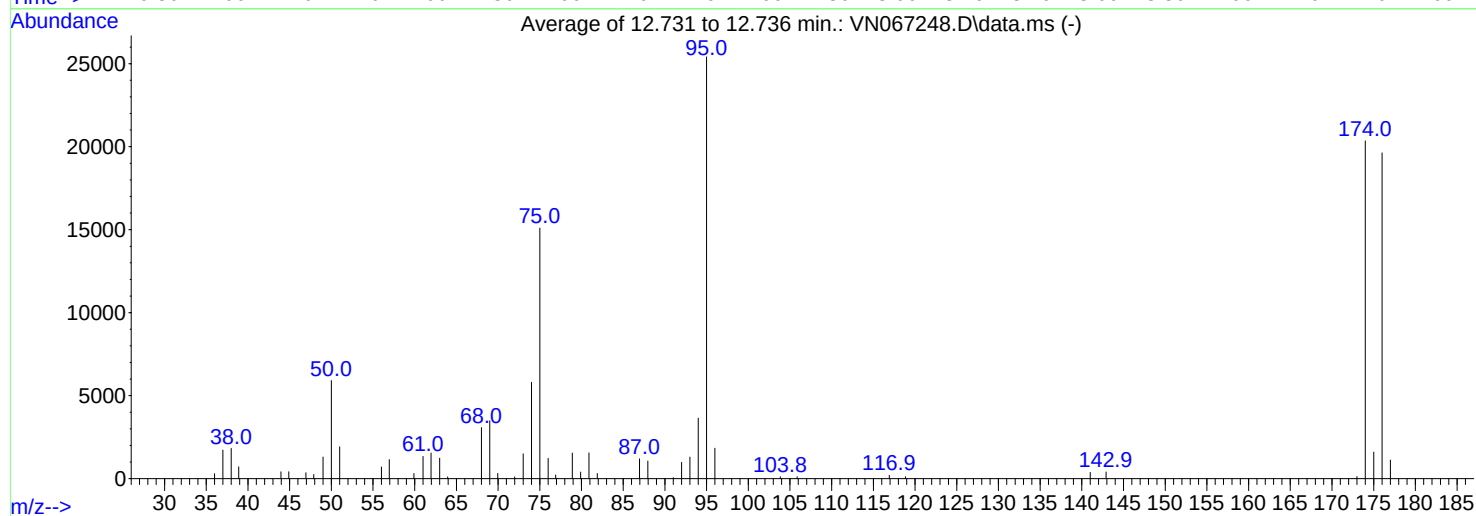


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060721\
 Data File : VN067248.D
 Acq On : 7 Jun 2021 10:09
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060721W.M
 Title : SW846 8260
 Last Update : Mon Jun 07 16:11:37 2021

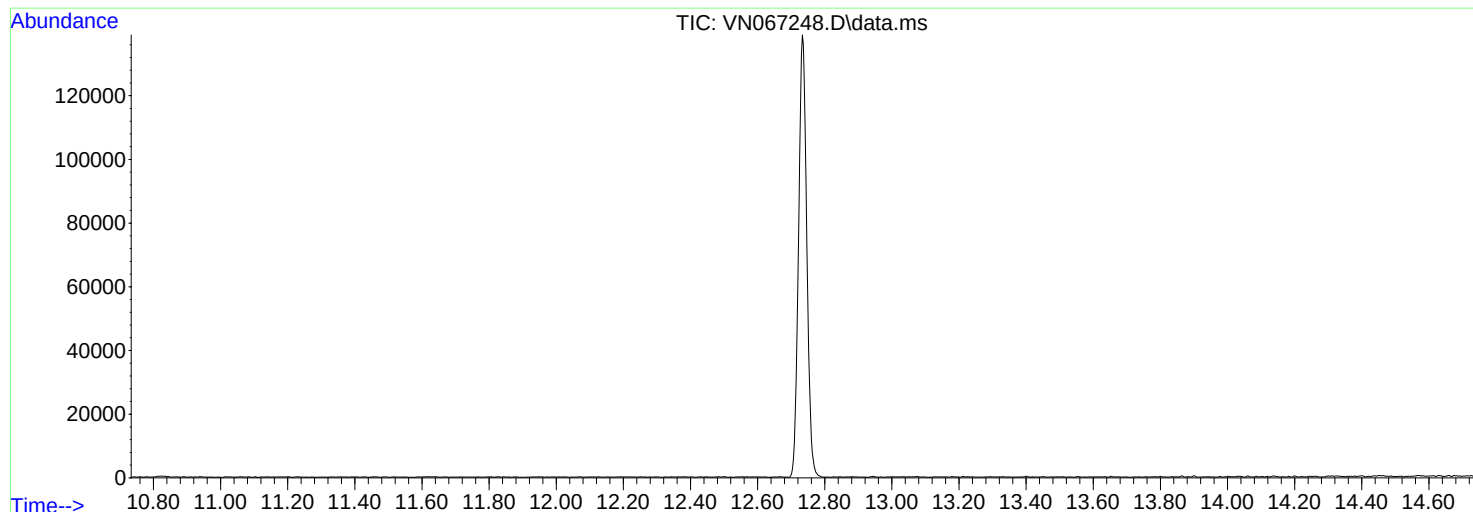

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3990

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.3	5911	PASS
75	95	30	60	59.4	15097	PASS
95	95	100	100	100.0	25411	PASS
96	95	5	9	7.2	1830	PASS
173	174	0.00	2	0.6	124	PASS
174	95	50	100	80.1	20347	PASS
175	174	5	9	7.8	1597	PASS
176	174	95	101	96.5	19627	PASS
177	176	5	9	5.7	1121	PASS