

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060723\
 Data File : VN078100.D
 Acq On : 07 Jun 2023 13:52
 Operator : JC\MD
 Sample : 03037-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-1

Quant Time: Jun 08 05:28:00 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 07 05:05:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.235	168	375924	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	691377	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	588849	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.800	152	173944	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	253856	50.647	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	101.300%
35) Dibromofluoromethane	8.177	113	223160	51.049	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	102.100%
50) Toluene-d8	10.571	98	834502	49.518	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	99.040%
62) 4-Bromofluorobenzene	12.853	95	237026	45.242	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	90.480%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060723\
Data File : VN078100.D
Acq On : 07 Jun 2023 13:52
Operator : JC\MD
Sample : 03037-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-1

Quant Time: Jun 08 05:28:00 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 07 05:05:00 2023
Response via : Initial Calibration




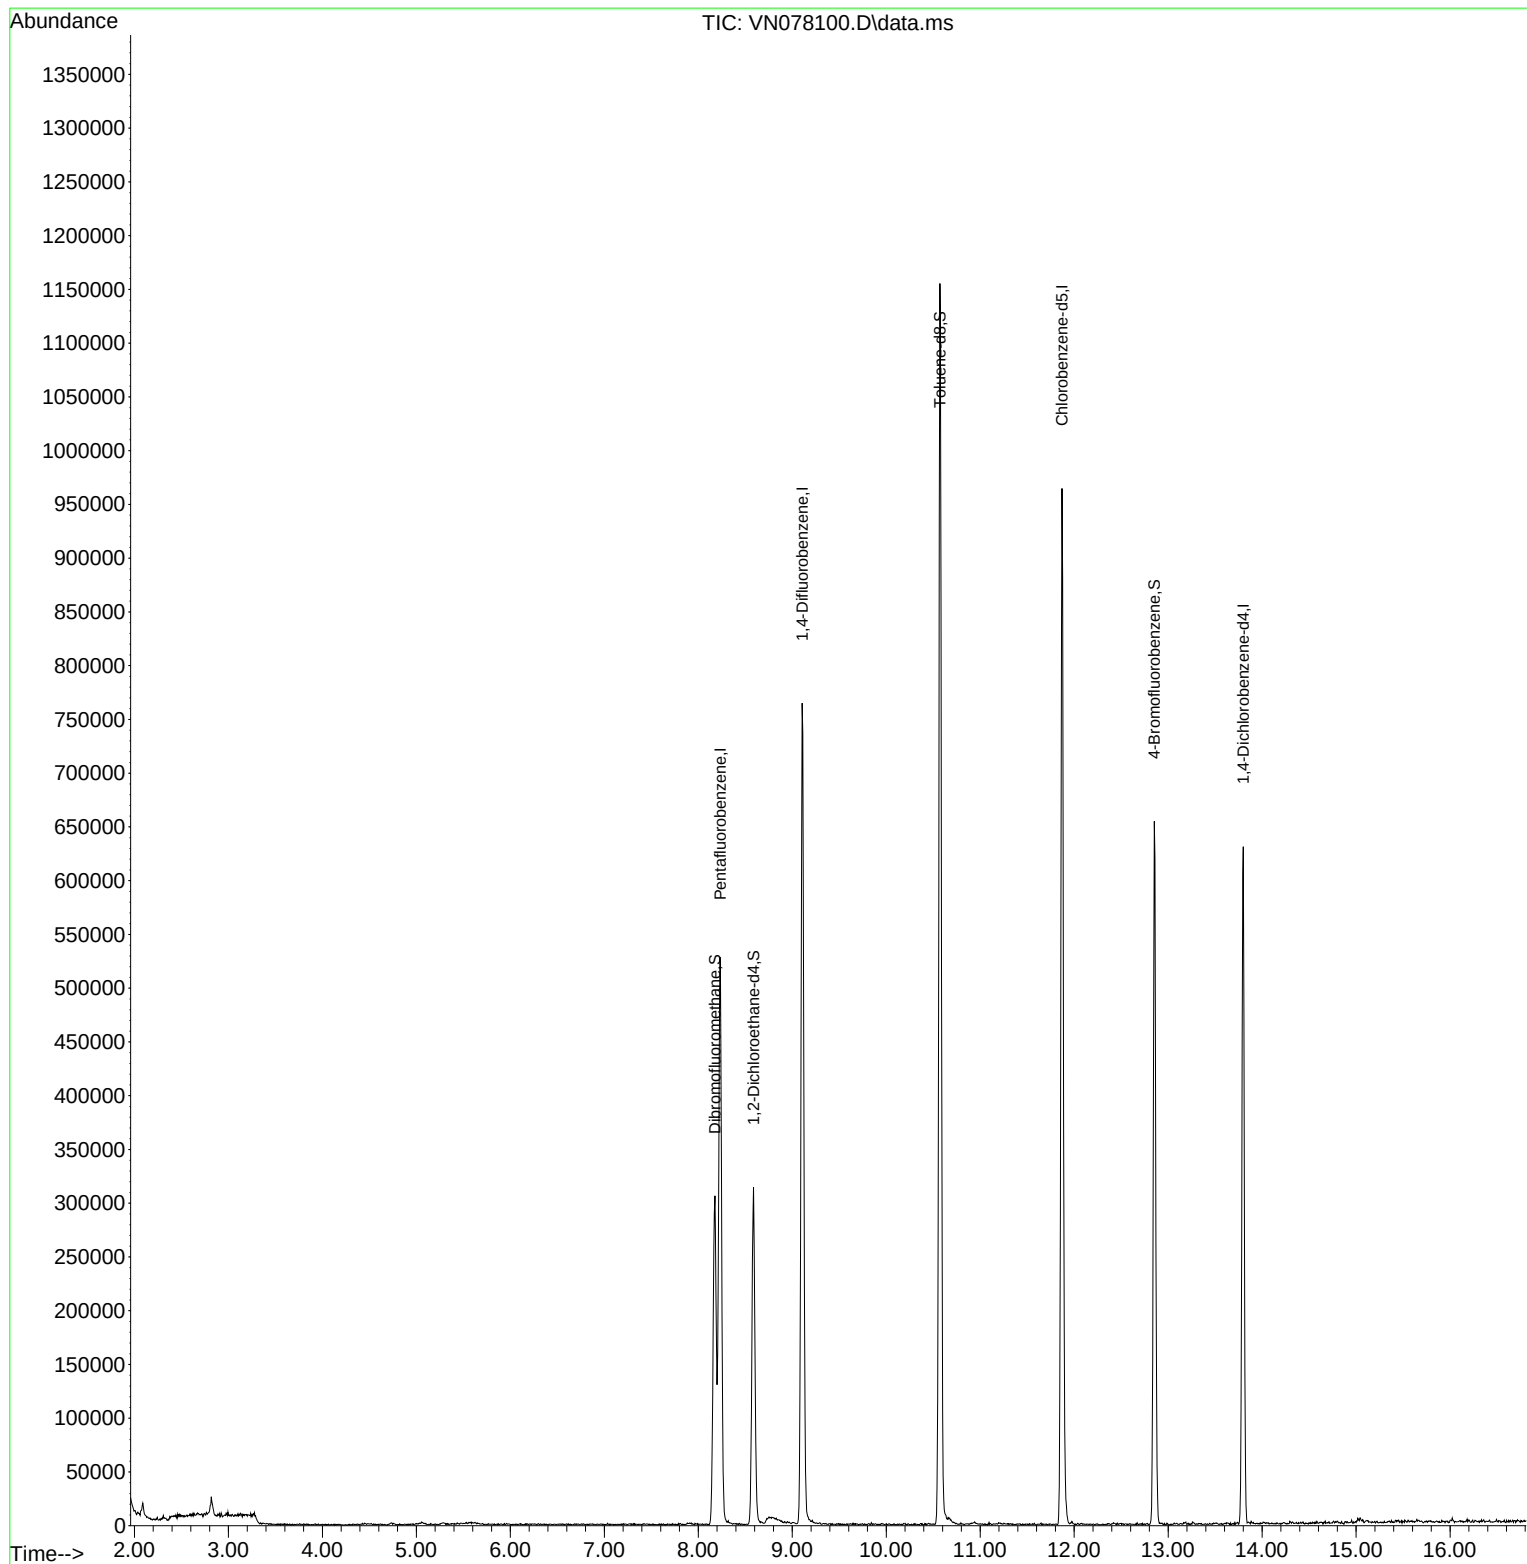


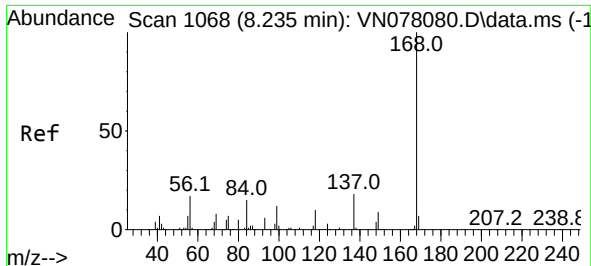

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.235 min Scan# 1068
Delta R.T. 0.000 min
Lab File: VN078100.D
Acq: 07 Jun 2023 13:52




Instrument :
MSVOA_N
ClientSampleId :
MW-1


Tgt Ion:168 Resp: 375924
Ion Ratio Lower Upper
168 100
99 62.8 53.0 79.6

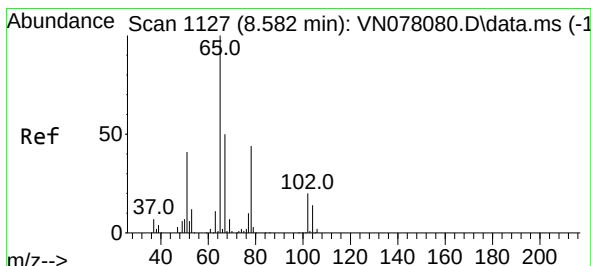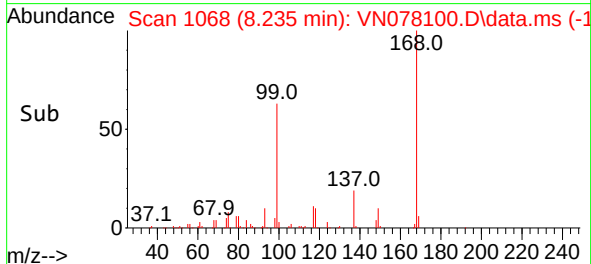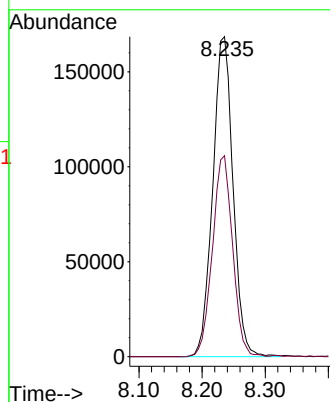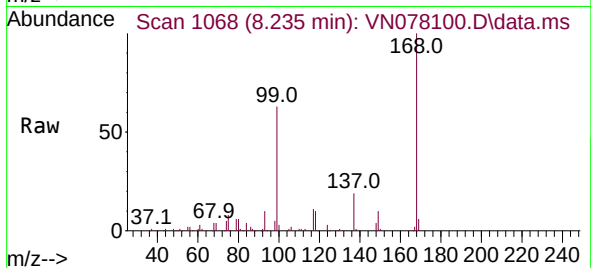

#33
1,2-Dichloroethane-d4
Concen: 50.647 ug/l
RT: 8.588 min Scan# 1128
Delta R.T. 0.006 min
Lab File: VN078100.D
Acq: 07 Jun 2023 13:52

Tgt Ion: 65 Resp: 253856
Ion Ratio Lower Upper
65 100
67 52.5 0.0 106.6

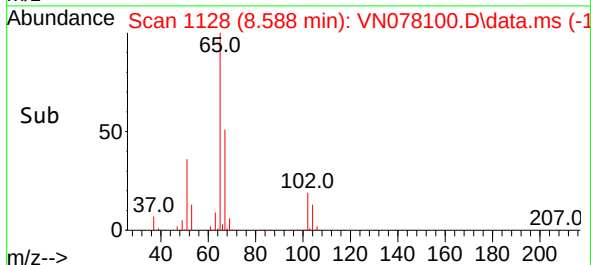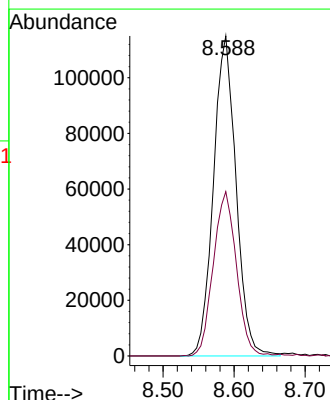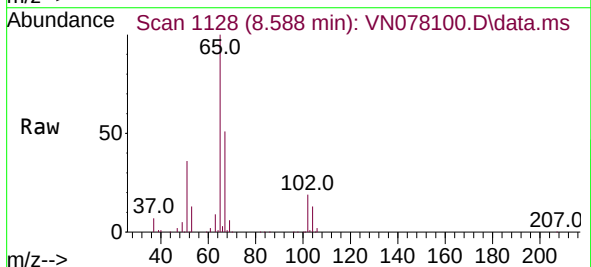

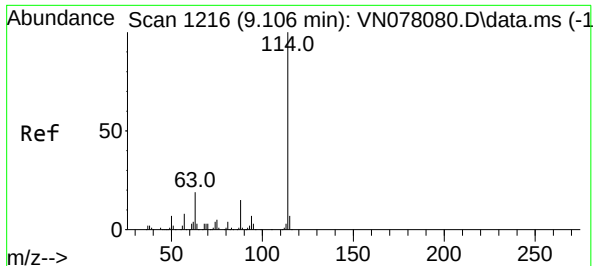

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN078100.D

Acq: 07 Jun 2023 13:52

Instrument :

MSVOA_N

ClientSampleId :

MW-1





Tgt Ion:114 Resp: 691377

Ion Ratio Lower Upper

114 100

63 19.1 0.0 36.4

88 15.4 0.0 30.6

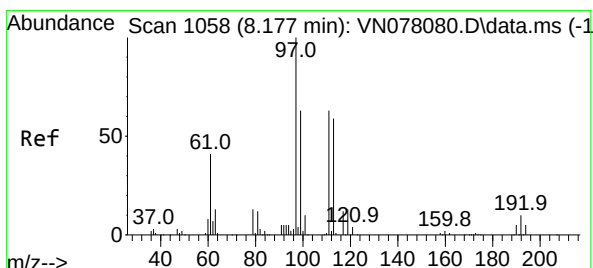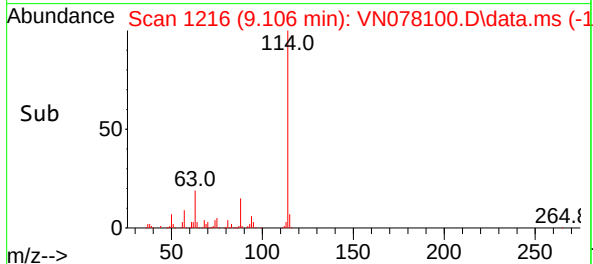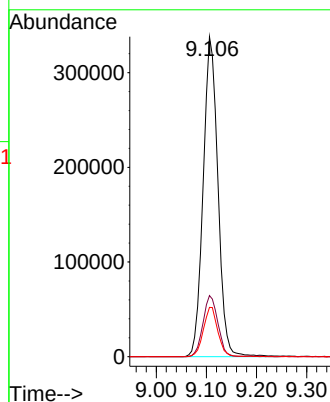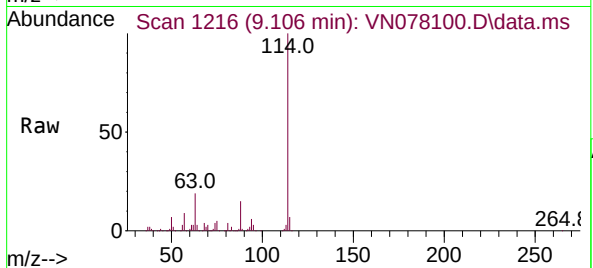

#35

Dibromofluoromethane

Concen: 51.049 ug/l

RT: 8.177 min Scan# 1058

Delta R.T. -0.000 min

Lab File: VN078100.D

Acq: 07 Jun 2023 13:52




Tgt Ion:113 Resp: 223160


Ion Ratio Lower Upper

113 100

111 104.7 82.6 123.8

192 16.5 12.7 19.1


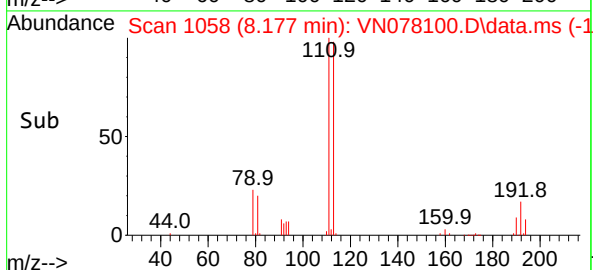
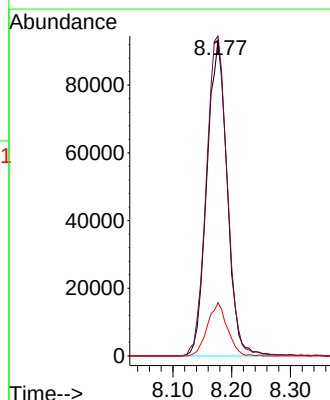
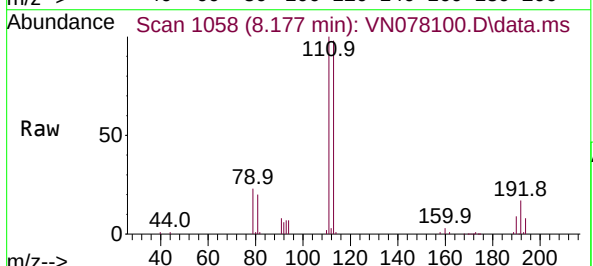


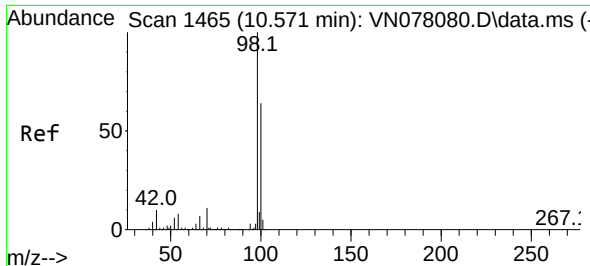

#50
Toluene-d8
Concen: 49.518 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN078100.D
Acq: 07 Jun 2023 13:52




Instrument :
MSVOA_N
ClientSampleId :
MW-1


Tgt Ion: 98 Resp: 834502
Ion Ratio Lower Upper
98 100
100 62.7 52.0 78.0

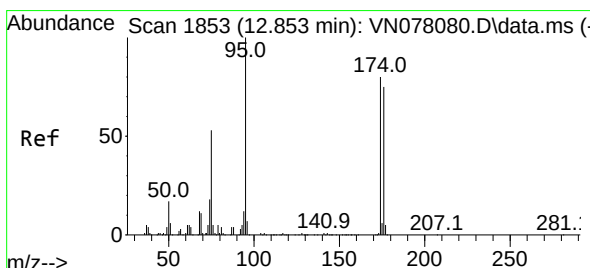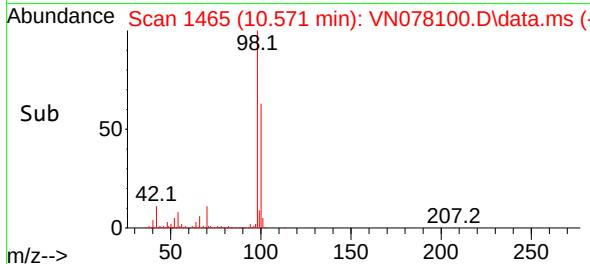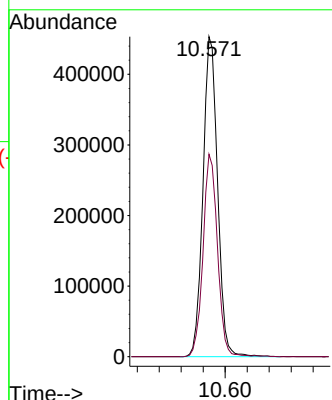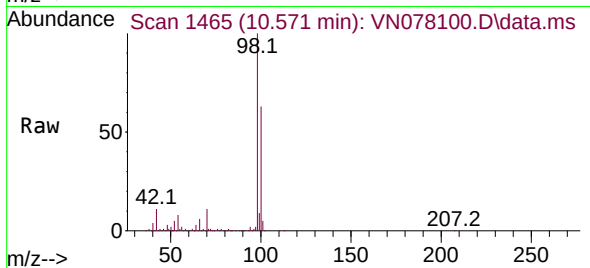

#62
4-Bromofluorobenzene
Concen: 45.242 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN078100.D
Acq: 07 Jun 2023 13:52

Tgt Ion: 95 Resp: 237026
Ion Ratio Lower Upper
95 100
174 73.7 0.0 143.8
176 71.4 0.0 135.8


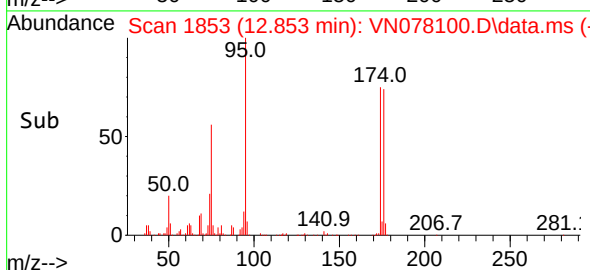
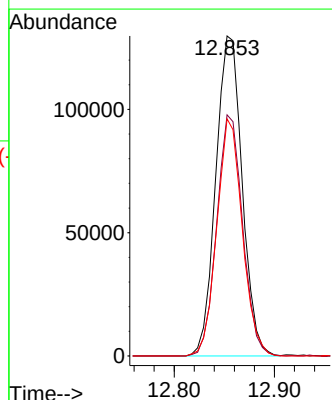
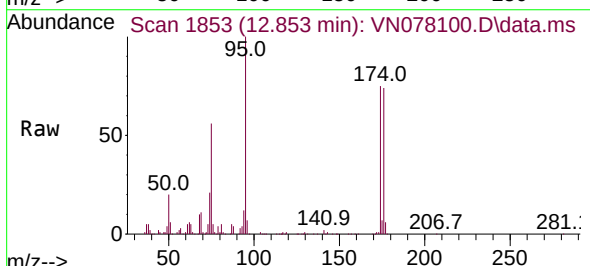


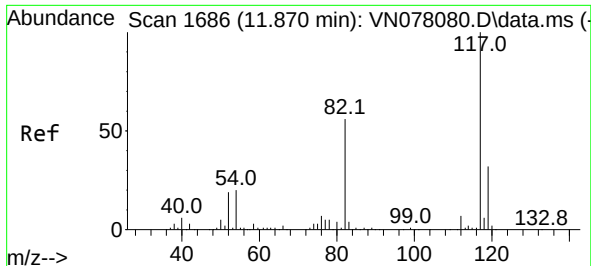

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN078100.D
Acq: 07 Jun 2023 13:52

Instrument :
MSVOA_N
ClientSampleId :
MW-1

Tgt Ion:117 Resp: 588849
Ion Ratio Lower Upper
117 100
82 55.8 44.0 66.0
119 32.0 25.6 38.4

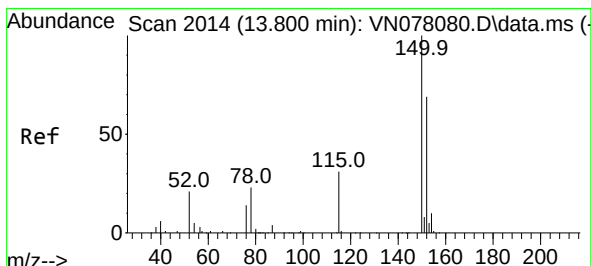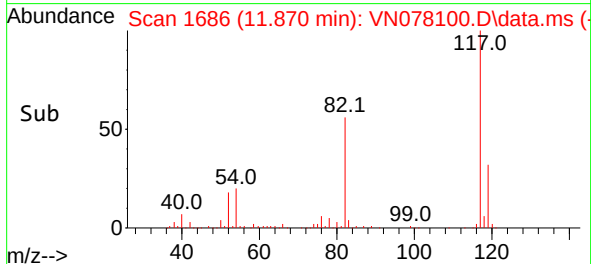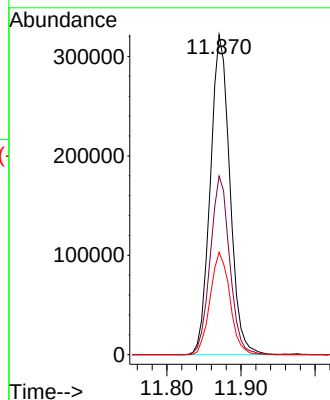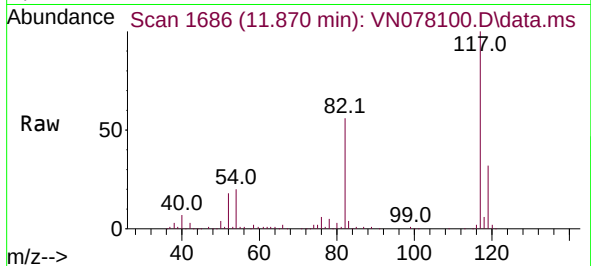

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.800 min Scan# 2014
Delta R.T. -0.000 min
Lab File: VN078100.D
Acq: 07 Jun 2023 13:52

Tgt Ion:152 Resp: 173944
Ion Ratio Lower Upper
152 100
115 61.7 32.3 96.8
150 156.6 0.0 355.8

