
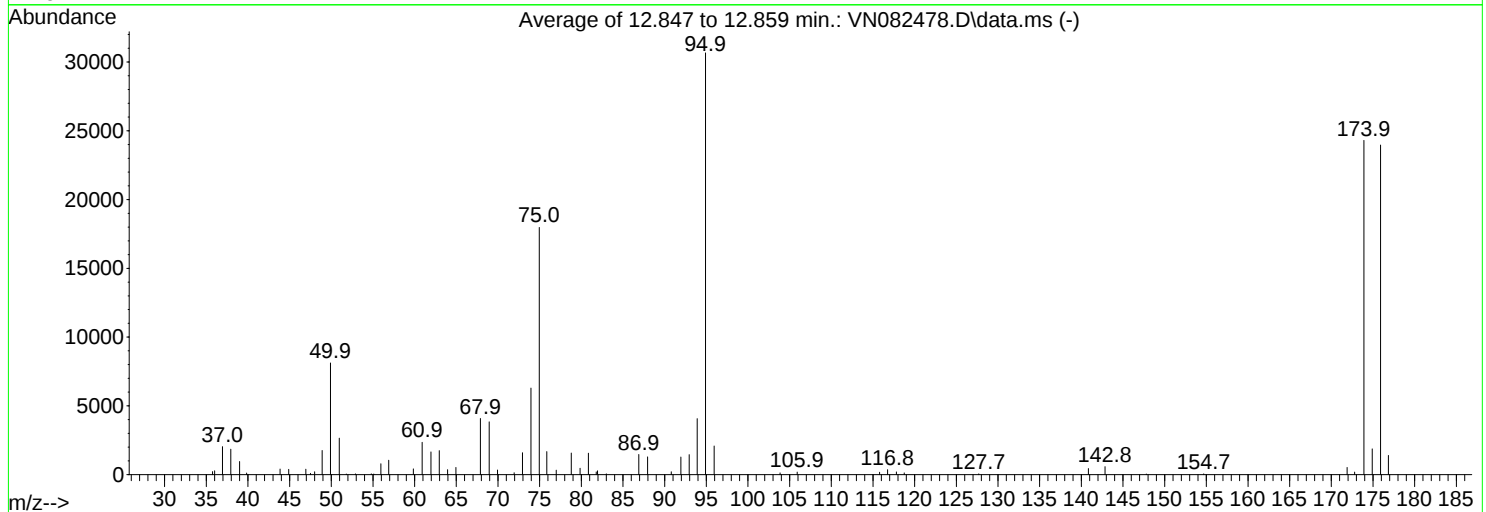


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060724\
Data File : VN082478.D
Acq On : 07 Jun 2024 08:25
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Title : SW846 8260
Last Update : Thu May 16 05:21:06 2024

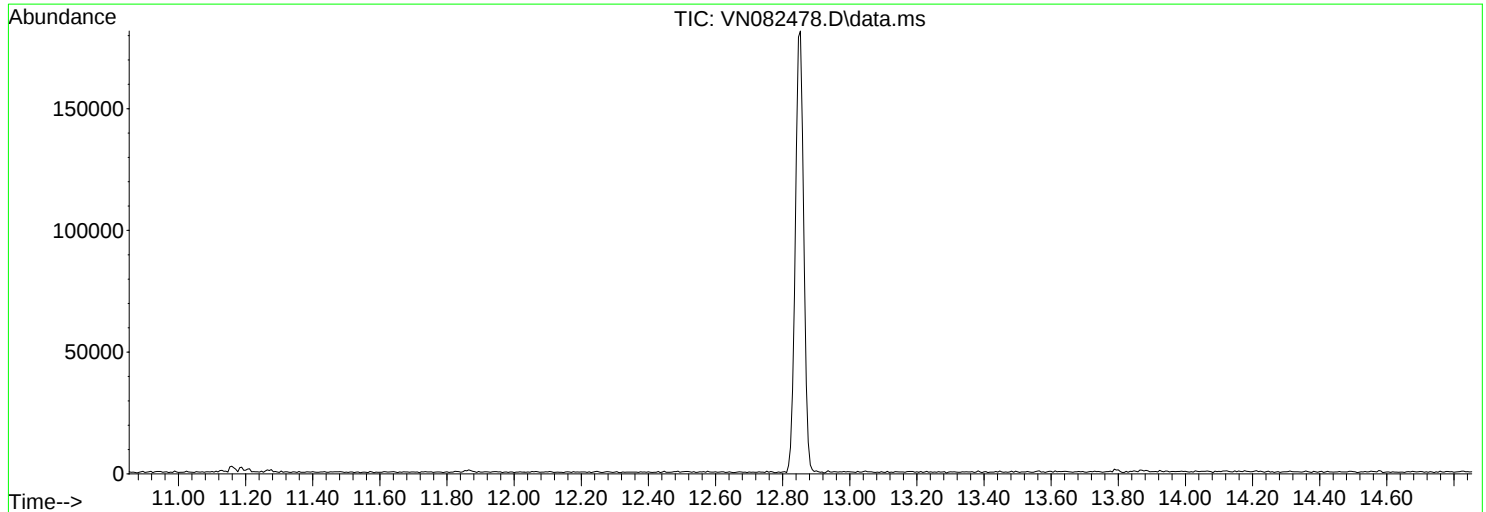

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	26.5	8125	PASS
75	95	30	60	58.6	17975	PASS
95	95	100	100	100.0	30667	PASS
96	95	5	9	6.8	2082	PASS
173	174	0.00	2	0.7	182	PASS
174	95	50	100	79.2	24299	PASS
175	174	5	9	7.7	1873	PASS
176	174	95	101	98.6	23965	PASS
177	176	5	9	5.8	1399	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.75	223	48.90	1760	61.95	1654	75.85	1670
36.00	281	49.90	8125	62.95	1744	77.00	321
36.95	2031	50.95	2658	63.95	359	78.80	156
37.95	1854	51.80	52	64.95	524	79.85	46
39.00	951	52.90	59	67.90	4084	80.85	1557
39.85	111	54.80	61	68.95	3841	81.80	200
43.85	406	55.10	52	69.95	339	81.95	279
44.90	387	55.95	795	71.95	142	83.00	55
46.95	398	56.90	1047	72.95	1590	86.90	1468
47.50	93	59.85	420	73.95	6299	87.95	1297
48.00	213	60.90	2356	74.95	17975	90.80	206

Average of 12.847 to 12.859 min.: VN082478.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
91.95	1276	127.70	56				
92.95	1454	140.85	438				
93.90	4069	142.85	582				
94.90	30667	147.80	50				
95.95	2082	154.70	60				
103.85	129	171.90	527				
105.90	188	172.80	182				
115.80	179	173.90	24299				
116.75	366	174.90	1873				
117.80	194	175.90	23965				
118.75	133	176.85	1399				

Instrument :

MSVOA_N

ClientSampleId :

BFB