


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN060819\
 Data File : VN056084.D
 Acq On : 7 Jun 2019 8:19
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N060619W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Thu Jun 06 04:02:53 2019

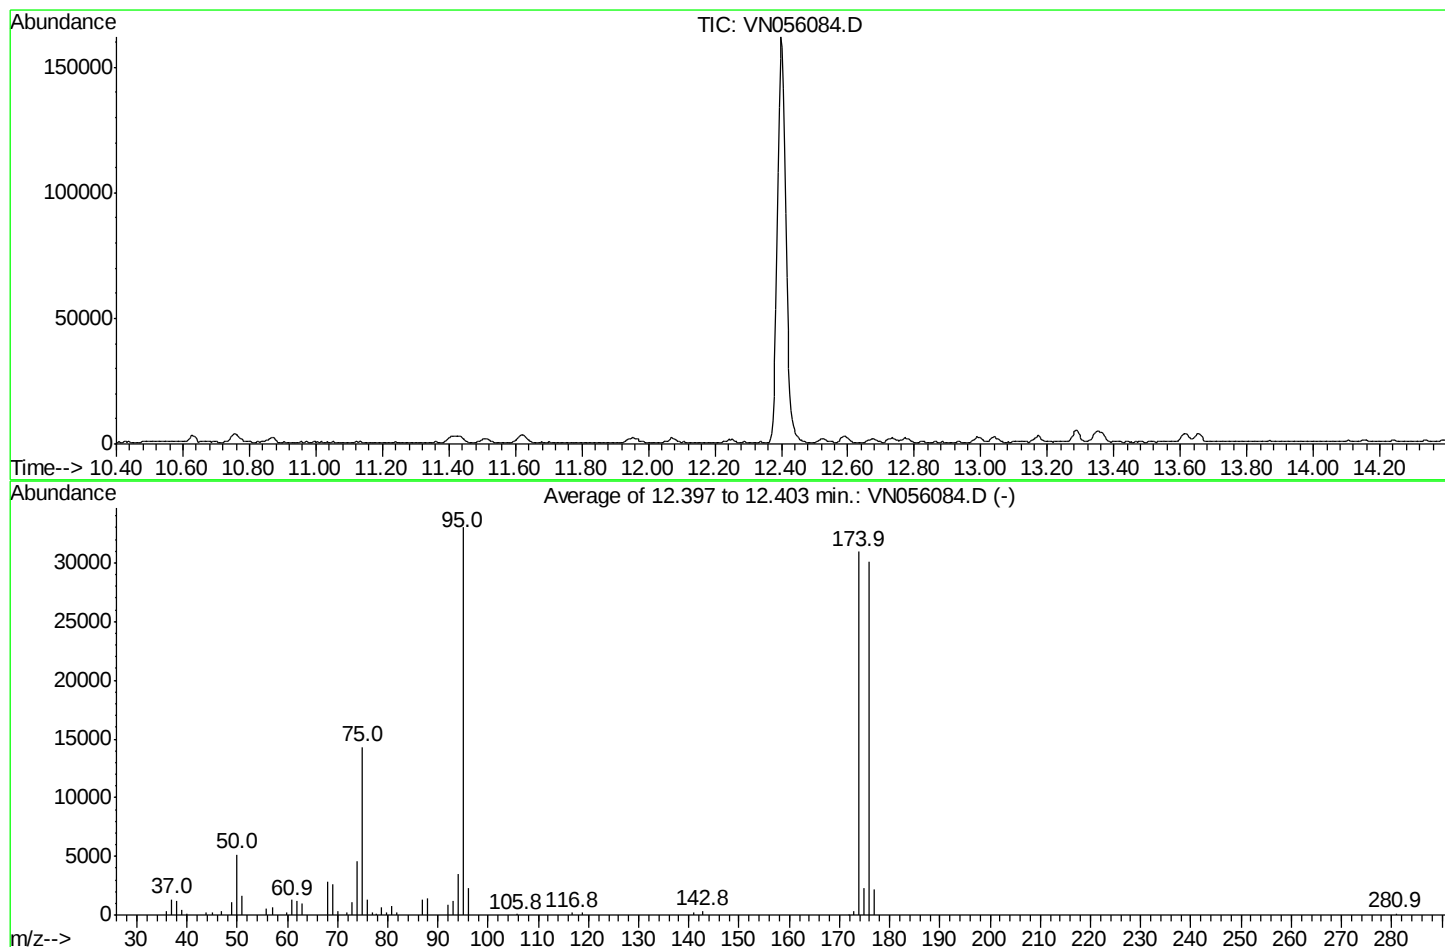

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	5140	PASS
75	95	30	60	43.4	14345	PASS
95	95	100	100	100.0	33032	PASS
96	95	5	9	6.9	2266	PASS
173	174	0.00	2	1.2	364	PASS
174	95	50	100	93.7	30965	PASS
175	174	5	9	7.5	2318	PASS
176	174	95	101	97.4	30157	PASS
177	176	5	9	7.1	2142	PASS