


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN060819\
 Data File : VN056128.D
 Acq On : 8 Jun 2019 4:06
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N060419W.M
 Title : SW846 8260
 Last Update : Tue Jun 04 11:02:09 2019

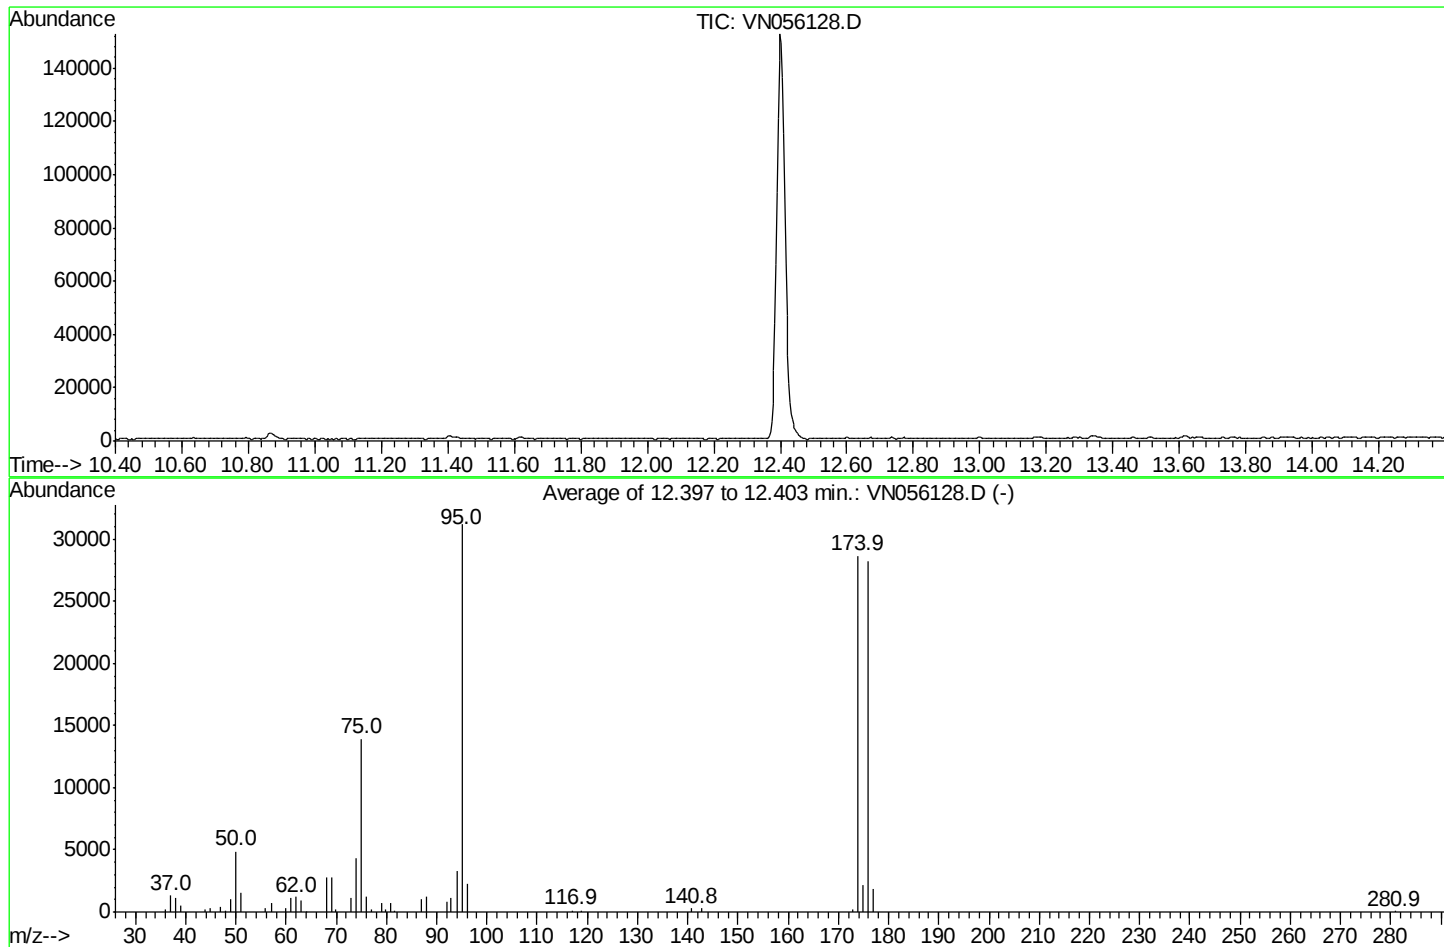

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	4883	PASS
75	95	30	60	44.7	13950	PASS
95	95	100	100	100.0	31184	PASS
96	95	5	9	7.3	2263	PASS
173	174	0.00	2	0.7	196	PASS
174	95	50	100	91.8	28629	PASS
175	174	5	9	7.7	2199	PASS
176	174	95	101	98.5	28197	PASS
177	176	5	9	6.6	1865	PASS