

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN060820\
 Data File : VN061707.D
 Acq On : 8 Jun 2020 19:39
 Operator : JC/MD
 Sample : PB129340ZHE#02
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB129340ZHE#02

Quant Time: Jun 09 04:34:11 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052820W.M
 Quant Title : SW846 8260
 QLast Update : Fri May 29 02:14:10 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	296704	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	513804	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	520688	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	237911	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.99	65	166451	47.09	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.18%	
35) Dibromofluoromethane	7.55	113	131553	50.47	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.94%	
50) Toluene-d8	10.06	98	624105	51.67	ug/l	0.00
Spiked Amount 50.000			Recovery	=	103.34%	
62) 4-Bromofluorobenzene	12.38	95	225167	51.10	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.20%	
Target Compounds						
16) Acetone	3.78	43	21270	16.029	ug/l	90
20) Methylene Chloride	4.51	84	16707	3.585	ug/l	94
43) Isopropyl Acetate	8.13	43	60703	9.210	ug/l #	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN060820\
Data File : VN061707.D
Acq On : 8 Jun 2020 19:39
Operator : JC/MD
Sample : PB129340ZHE#02
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB129340ZHE#02

Quant Time: Jun 09 04:34:11 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052820W.M
Quant Title : SW846 8260
QLast Update : Fri May 29 02:14:10 2020
Response via : Initial Calibration

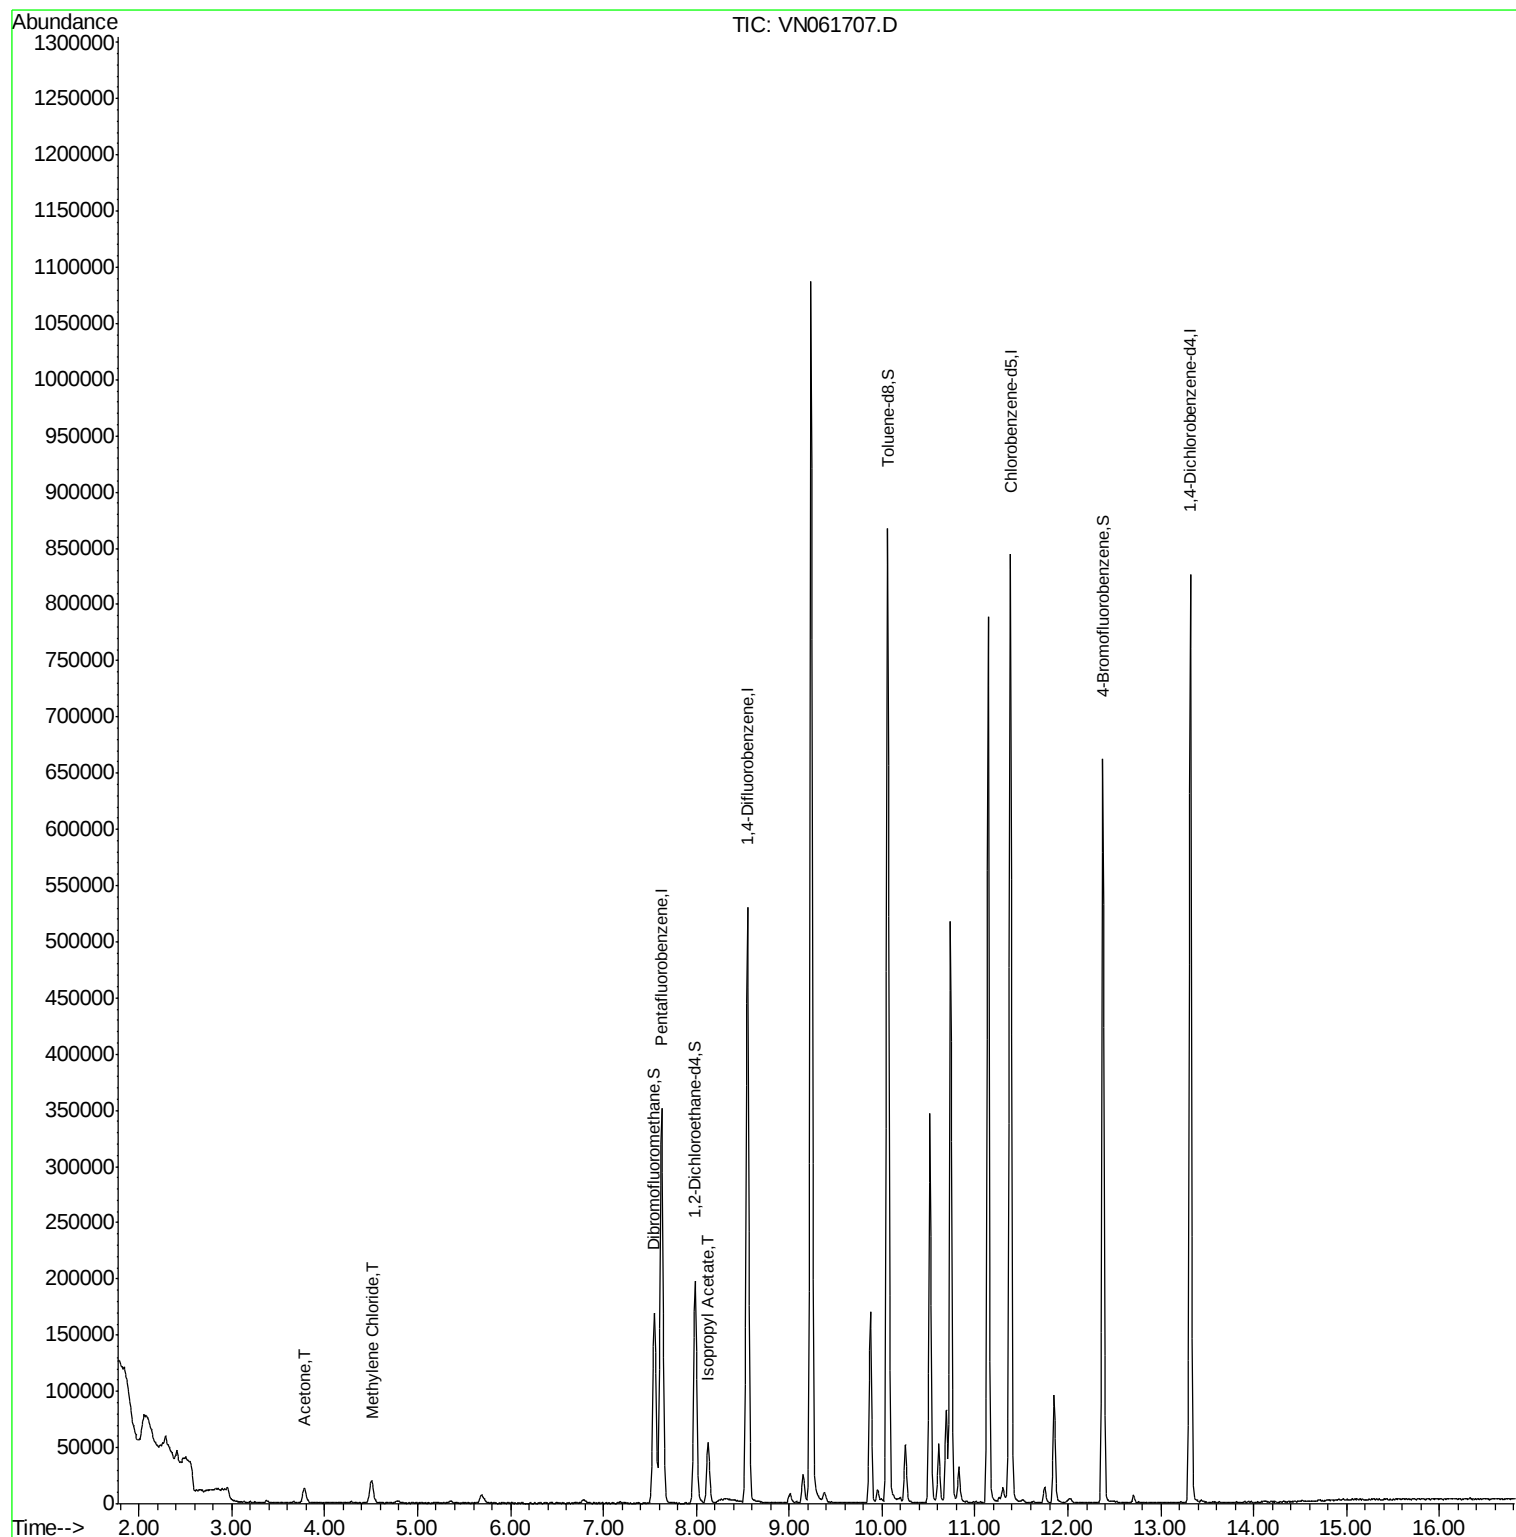

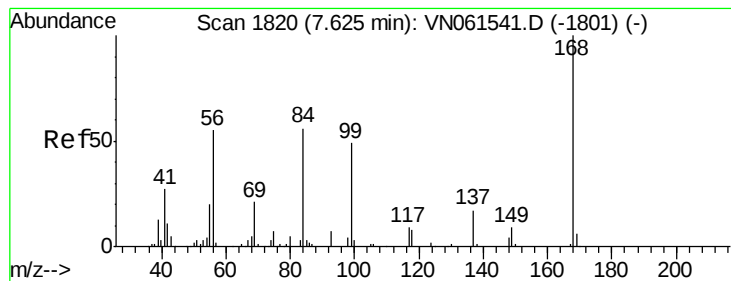

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1820

Delta R.T. 0.00 min

Lab File: VN061707.D

Acq: 8 Jun 2020 19:39

Instrument :

MSVOA_N

ClientSampleId :


PB129340ZHE#02

Tot Ion:168 Resp: 296704

Ion Ratio Lower Upper

168 100

99 53.7 45.0 67.4

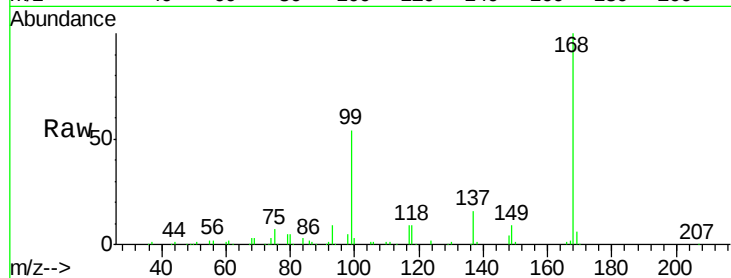

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.63



150000

100000

50000

0

Time-->

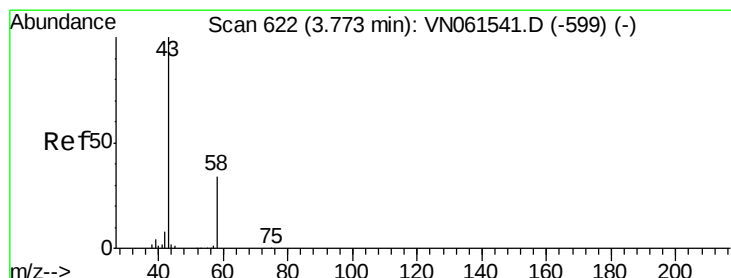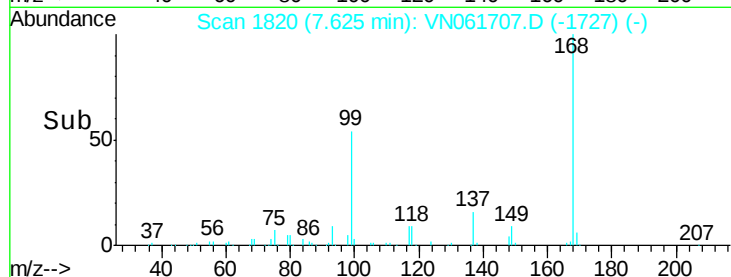

#16

Acetone

Concen: 16.029 ug/l

RT: 3.78 min Scan# 624

Delta R.T. 0.01 min

Lab File: VN061707.D


Acq: 8 Jun 2020 19:39

Tgt Ion: 43 Resp: 21270

Ion Ratio Lower Upper

43 100

58 39.7 27.2 40.8

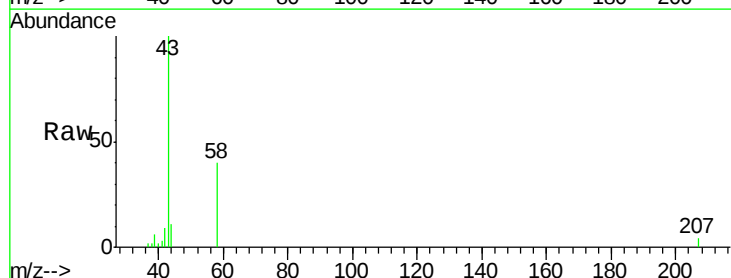

Abundance Ion 43.00 (42.70 to 43.70): VN

Ion 58.00 (57.70 to 58.70): VN

3.78

8000


6000




4000

2000

0

Time-->




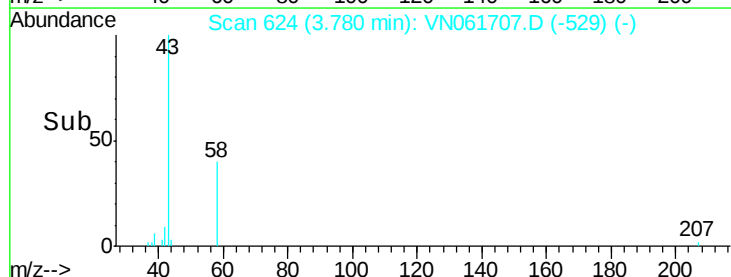


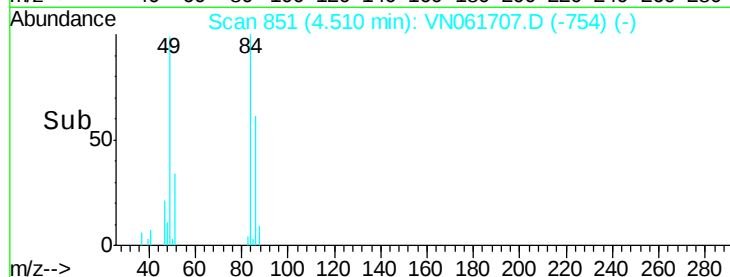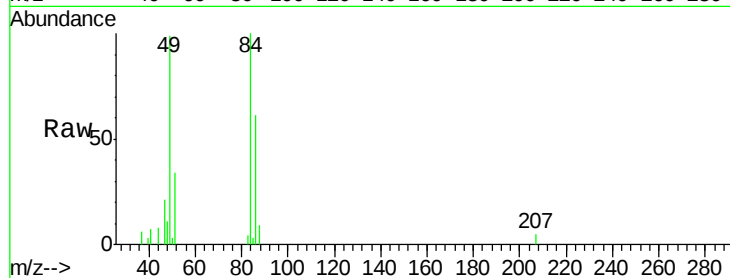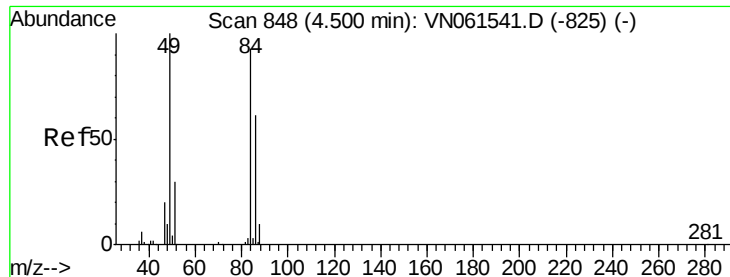

#20
Methylene Chloride
Concen: 3.585 ug/l
RT: 4.51 min Scan# 851
Delta R.T. 0.01 min
Lab File: VN061707.D
Acq: 8 Jun 2020 19:39


Instrument :
MSVOA_N
ClientSampleId :
PB129340ZHE#02


Tot Ion:	84	Resp:	16707
Ion	Ratio	Lower	Upper
84	100		
49	99.4	85.8	128.8
51	34.1	26.2	39.2
86	61.3	52.6	78.8

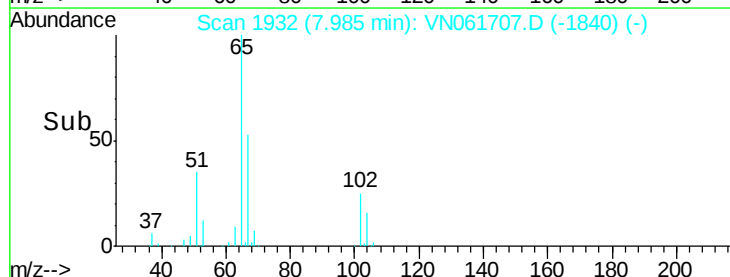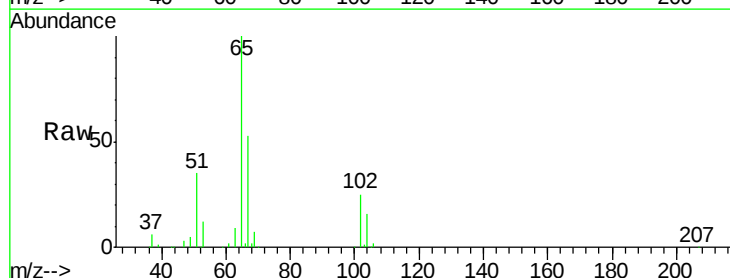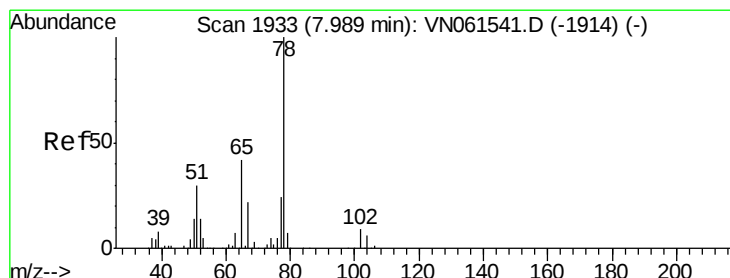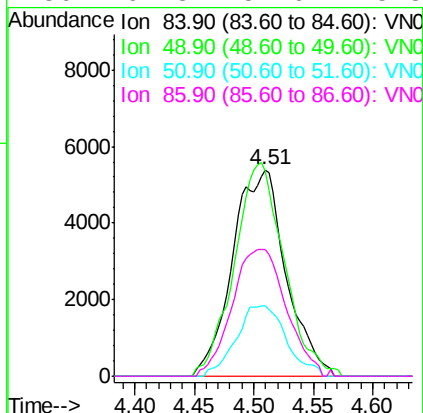

#33
1,2-Dichloroethane-d4
Concen: 47.086 ug/l
RT: 7.99 min Scan# 1932
Delta R.T. -0.00 min
Lab File: VN061707.D
Acq: 8 Jun 2020 19:39

Tgt Ion:	65	Resp:	166451
Ion	Ratio	Lower	Upper
65	100		
67	53.2	0.0	104.8

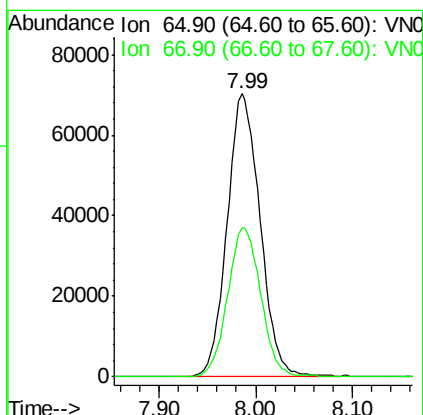

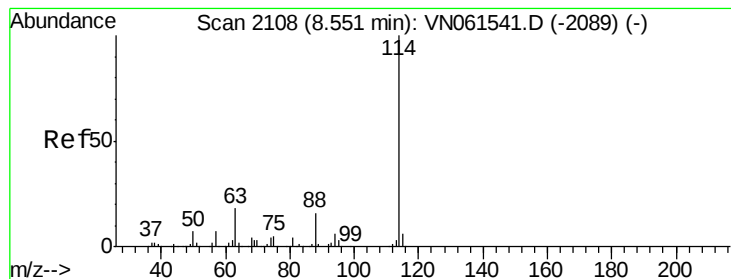

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.55 min Scan# 2108

Delta R.T. 0.00 min

Lab File: VN061707.D

Acq: 8 Jun 2020 19:39

Instrument :

MSVOA_N

ClientSampleId :

PB129340ZHE#02


Tot Ion:114 Resp: 513804

Ion Ratio Lower Upper

114 100

63 16.5 0.0 35.8




88 14.4 0.0 31.0

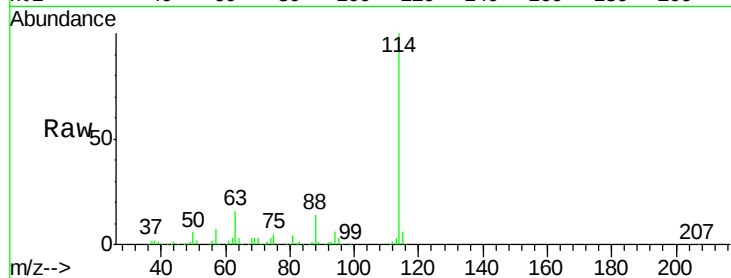

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN

Ion 87.90 (87.60 to 88.60): VN

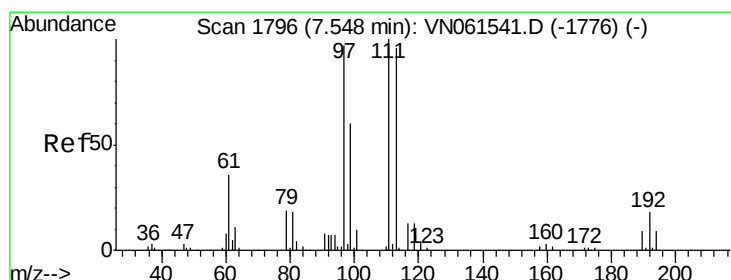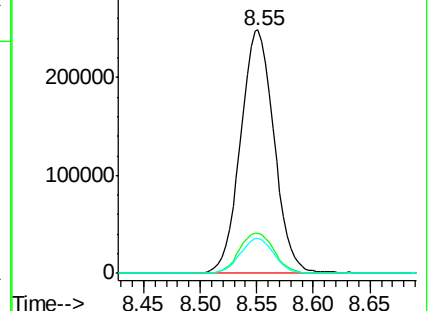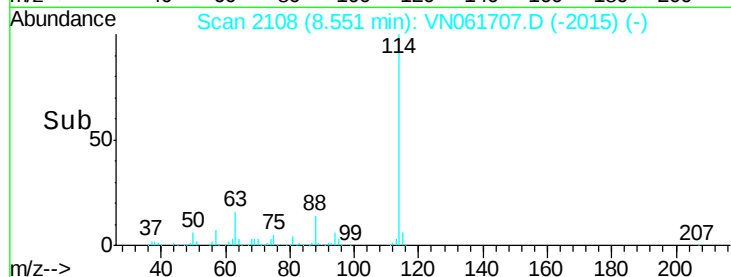

#35

Dibromofluoromethane

Concen: 50.472 ug/l

RT: 7.55 min Scan# 1796

Delta R.T. 0.00 min

Lab File: VN061707.D

Acq: 8 Jun 2020 19:39


Tgt Ion:113 Resp: 131553

Ion Ratio Lower Upper

113 100

111 103.4 83.4 125.0



192 19.9 15.4 23.2

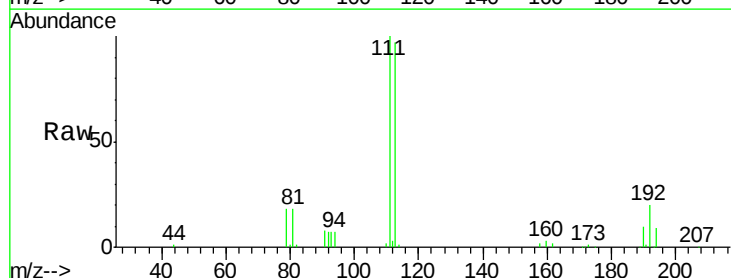


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

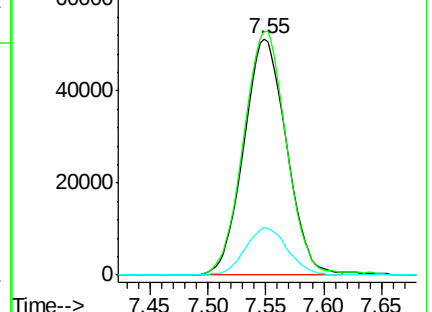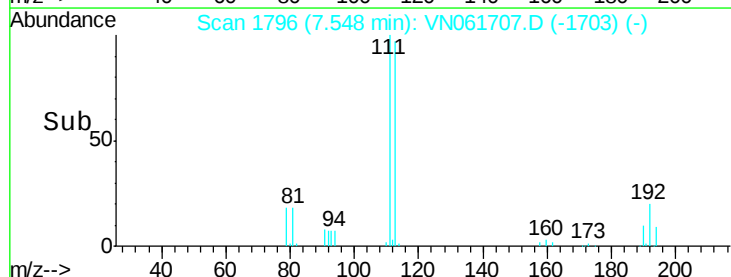

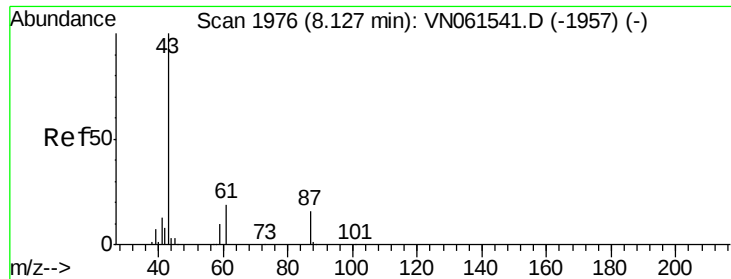

#43

Isopropyl Acetate

Concen: 9.210 ug/l

RT: 8.13 min Scan# 1976

Delta R.T. 0.00 min

Lab File: VN061707.D

Acq: 8 Jun 2020 19:39

Instrument :

MSVOA_N

ClientSampleId :

PB129340ZHE#02


Tot Ion: 43 Resp: 60703

Ion Ratio Lower Upper

43 100

61 22.4 23.6 35.4#




87 16.0 13.0 19.6

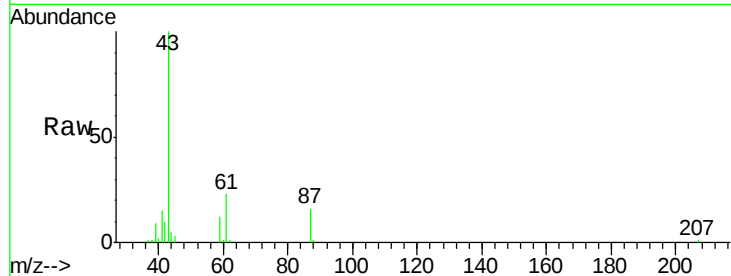

Abundance Ion 43.00 (42.70 to 43.70): VN061707.D (-1883) (-)

Ion 61.00 (60.70 to 61.70): VN061707.D (-1883) (-)

Ion 87.00 (86.70 to 87.70): VN061707.D (-1883) (-)

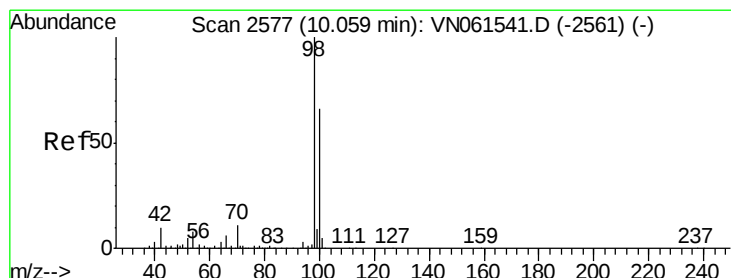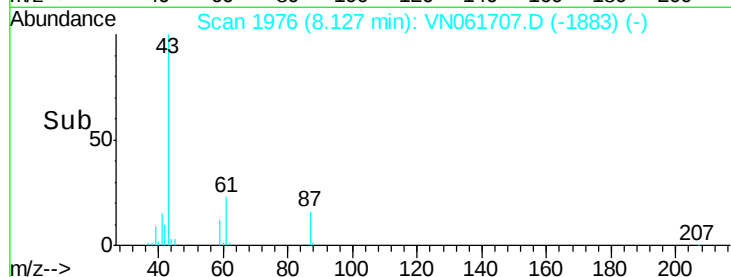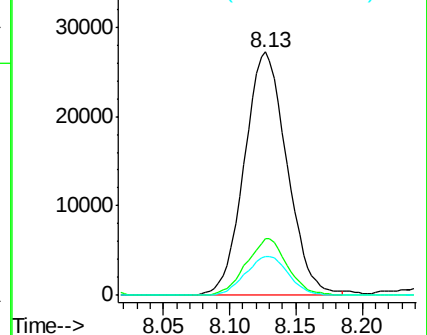

#50

Toluene-d8

Concen: 51.671 ug/l

RT: 10.06 min Scan# 2577

Delta R.T. 0.00 min

Lab File: VN061707.D


Acq: 8 Jun 2020 19:39

Tgt Ion: 98 Resp: 624105

Ion Ratio Lower Upper



98 100


100 65.2 52.8 79.2

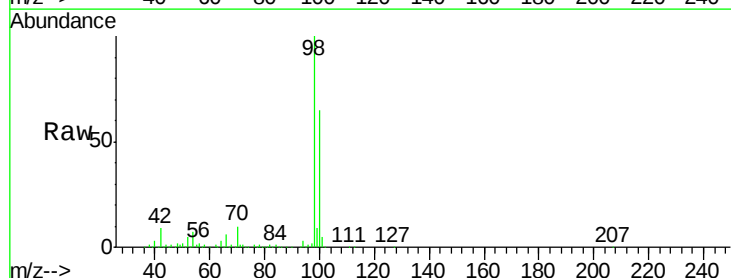

Abundance Ion 98.00 (97.70 to 98.70): VN061707.D (-2484) (-)

Ion 100.00 (99.70 to 100.70): VN061707.D (-2484) (-)



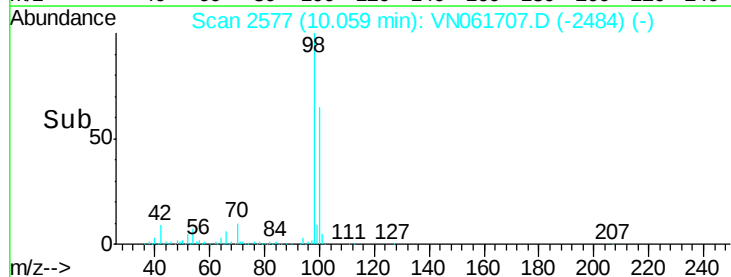
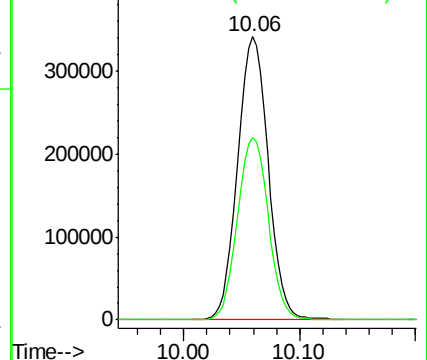


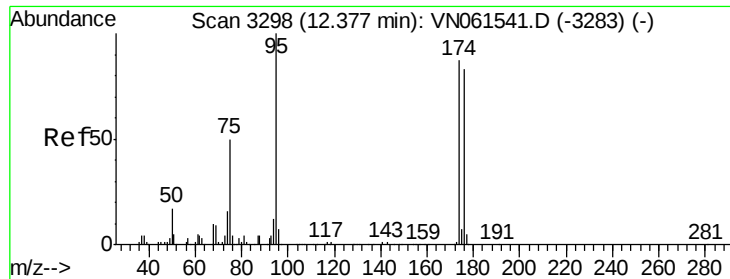

#62
4-Bromofluorobenzene
Concen: 51.097 ug/l
RT: 12.38 min Scan# 3298
Delta R.T. 0.00 min
Lab File: VN061707.D
Acq: 8 Jun 2020 19:39




Instrument :
MSVOA_N
ClientSampleId :
PB129340ZHE#02


Tot Ion	Ratio	Lower	Upper
95	100		
174	86.7	0.0	172.8
176	83.3	0.0	164.8

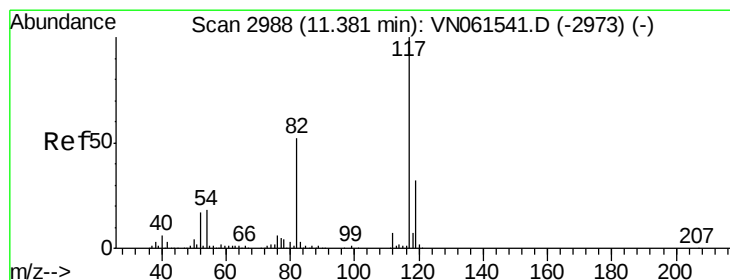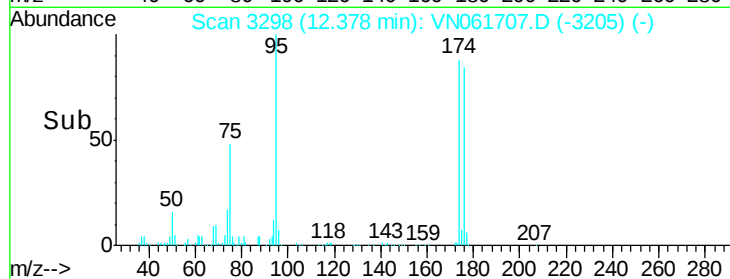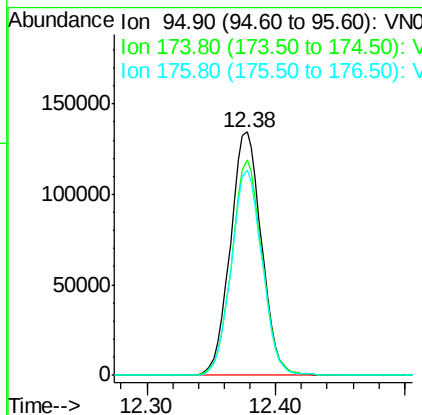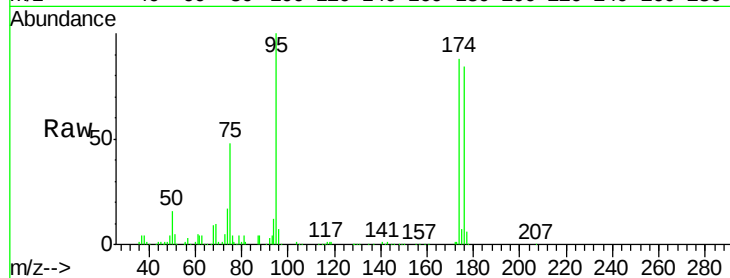

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2988
Delta R.T. 0.00 min
Lab File: VN061707.D
Acq: 8 Jun 2020 19:39

Tgt Ion	Ratio	Lower	Upper
117	100		
82	51.9	41.5	62.3
119	32.2	25.6	38.4

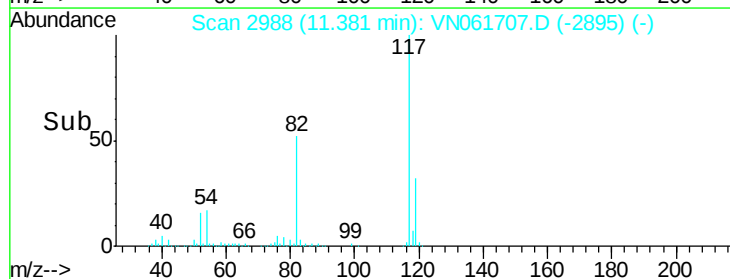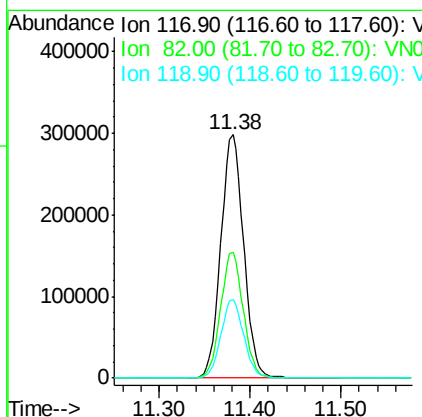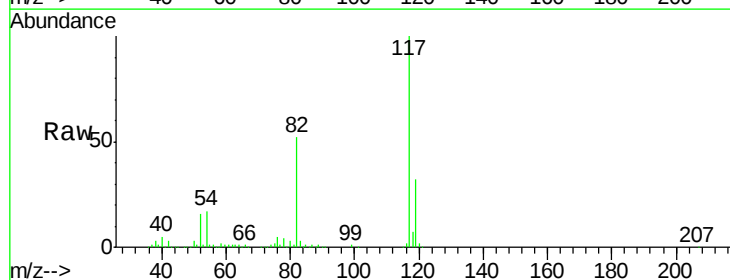

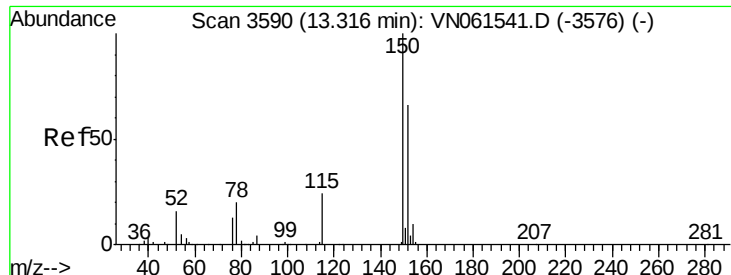

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3591

Delta R.T. 0.00 min

Lab File: VN061707.D

Acq: 8 Jun 2020 19:39

Instrument :

MSVOA_N

ClientSampleId :

PB129340ZHE#02

Tot Ion:152 Resp: 237911

Ion Ratio Lower Upper

152 100

115 56.5 28.0 84.0

150 157.8 0.0 344.0

