
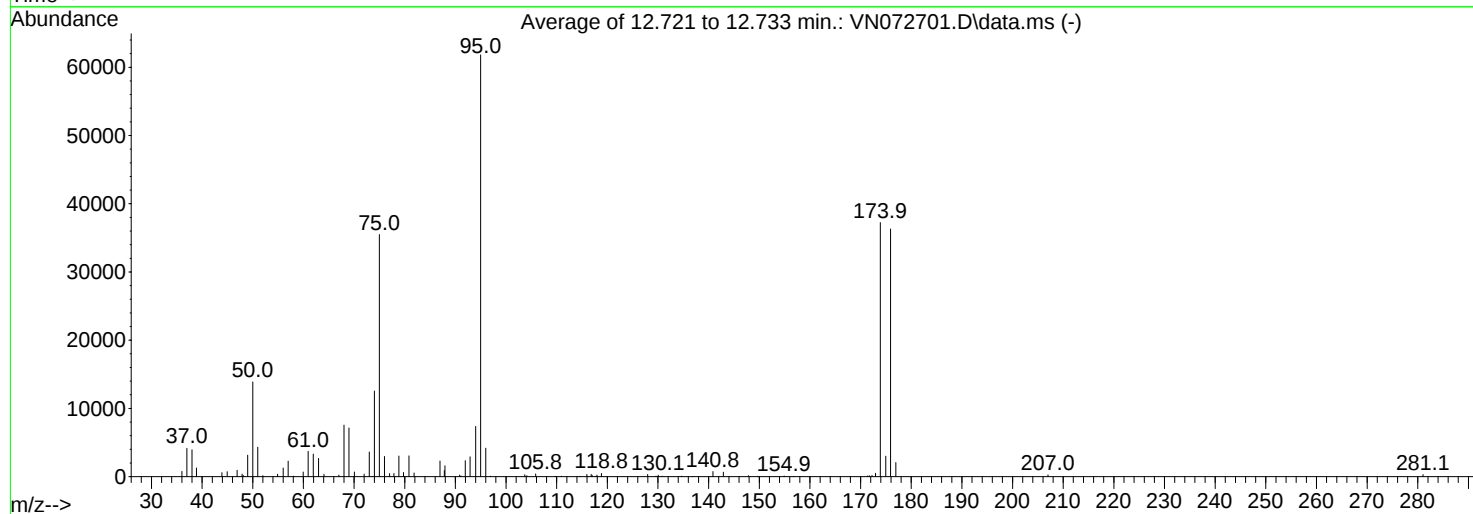


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060822\
Data File : VN072701.D
Acq On : 08 Jun 2022 15:40
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060822W.M
Title : SW846 8260
Last Update : Thu Jun 09 05:17:31 2022

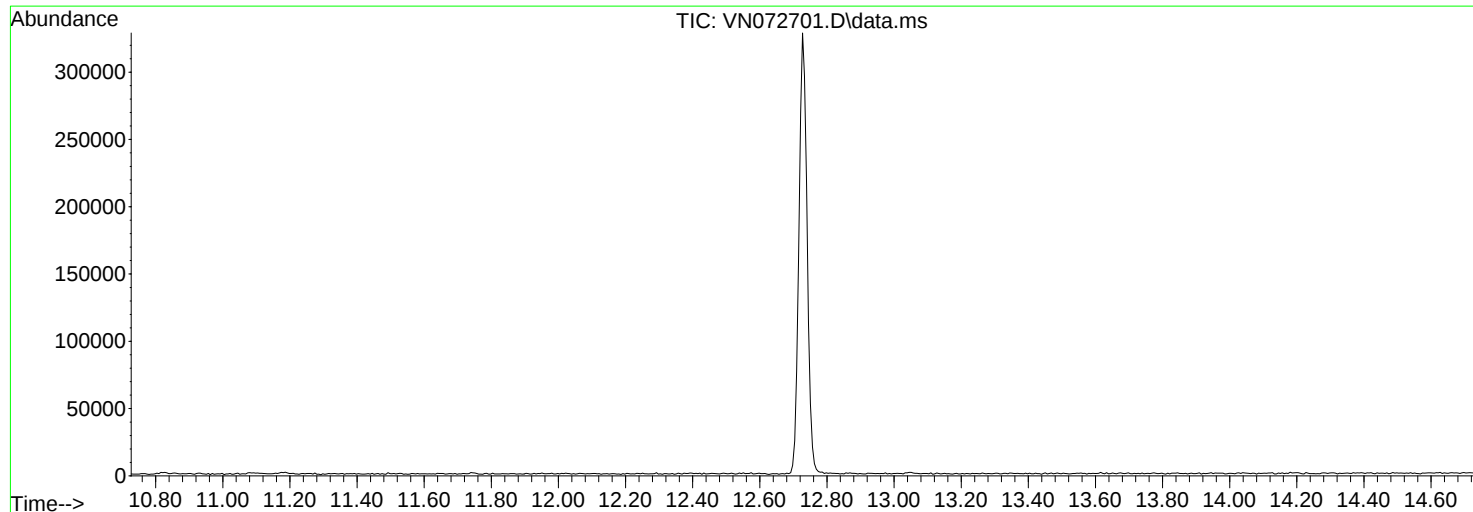

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1816

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.5	13894	PASS
75	95	30	60	57.4	35477	PASS
95	95	100	100	100.0	61824	PASS
96	95	5	9	6.7	4166	PASS
173	174	0.00	2	1.3	495	PASS
174	95	50	100	60.2	37240	PASS
175	174	5	9	8.1	3003	PASS
176	174	95	101	97.5	36299	PASS
177	176	5	9	5.7	2071	PASS