

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060823\
 Data File : VN078117.D
 Acq On : 08 Jun 2023 09:47
 Operator : JC\MD
 Sample : VN0608MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0608MBL01

Quant Time: Jun 09 01:21:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 07 05:05:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	348410	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	626439	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	552987	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.800	152	161210	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	237590	51.146	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	102.300%
35) Dibromofluoromethane	8.171	113	209974	53.012	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	106.020%
50) Toluene-d8	10.571	98	773988	50.688	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	101.380%
62) 4-Bromofluorobenzene	12.853	95	217564	45.832	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	91.660%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060823\
Data File : VN078117.D
Acq On : 08 Jun 2023 09:47
Operator : JC\MD
Sample : VN0608MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0608MBL01

Quant Time: Jun 09 01:21:38 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 07 05:05:00 2023
Response via : Initial Calibration




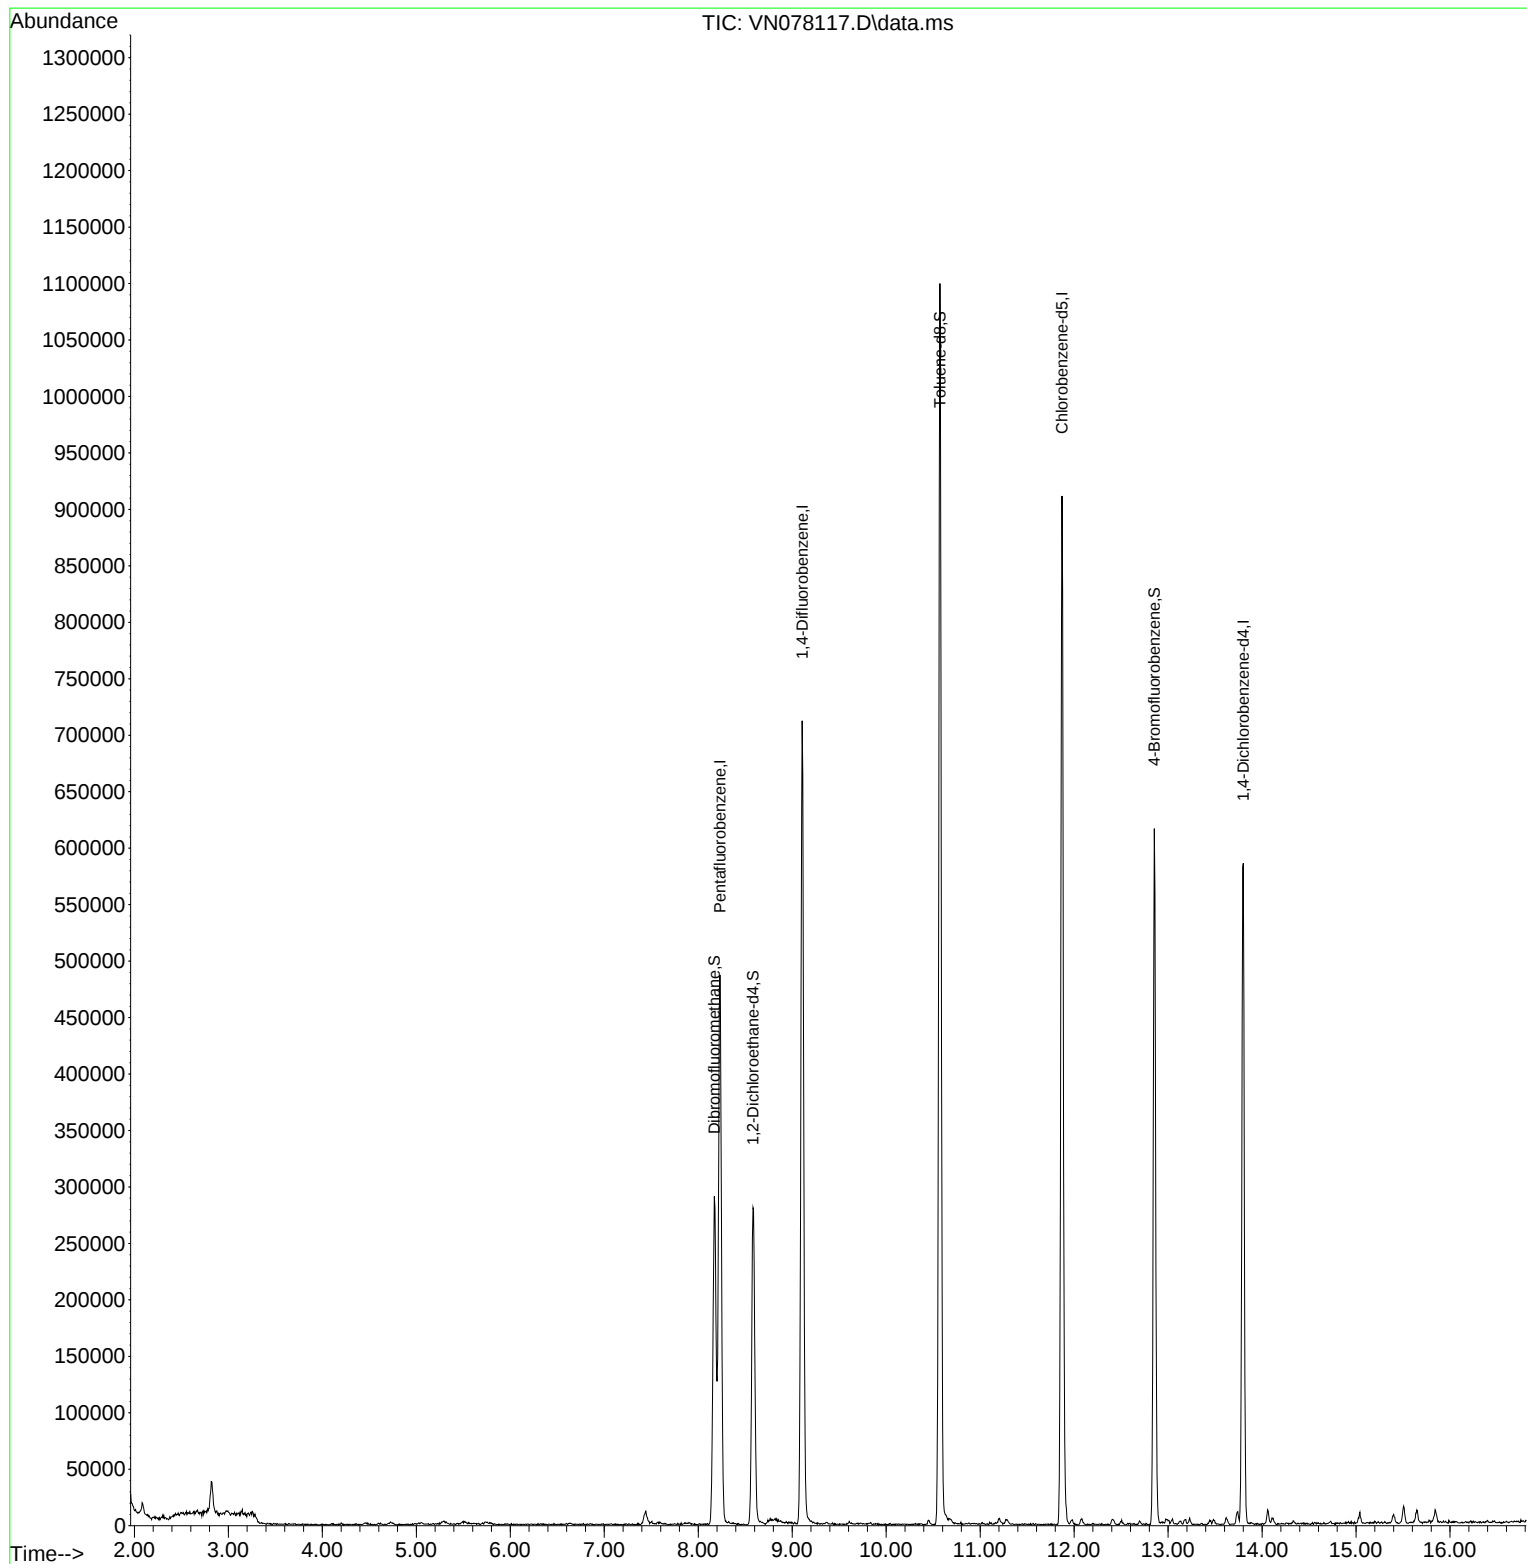




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1068
Delta R.T. -0.005 min
Lab File: VN078117.D
Acq: 08 Jun 2023 09:47




Instrument :
MSVOA_N
ClientSampleId :
VN0608MBL01


Tgt Ion:168 Resp: 348410
Ion Ratio Lower Upper
168 100
99 64.5 53.0 79.6

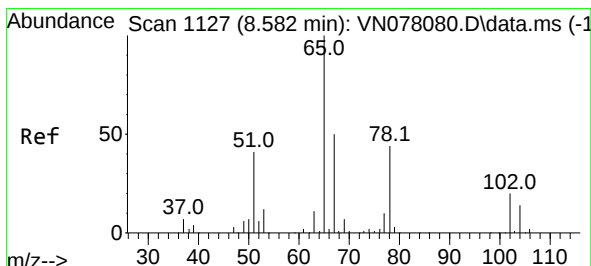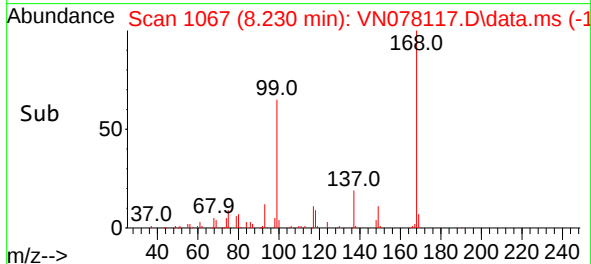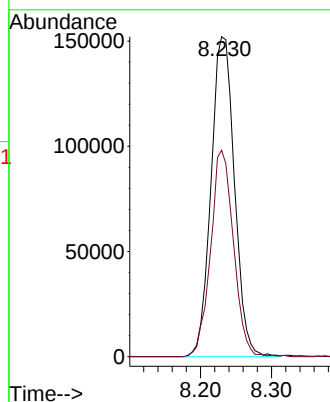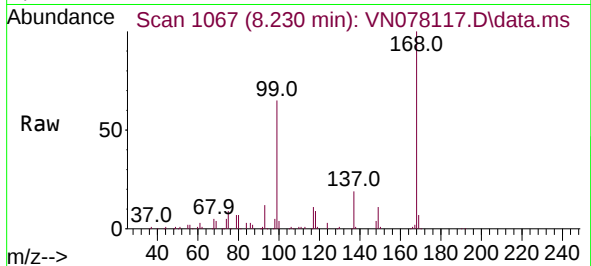

#33
1,2-Dichloroethane-d4
Concen: 51.146 ug/l
RT: 8.583 min Scan# 1127
Delta R.T. 0.000 min
Lab File: VN078117.D
Acq: 08 Jun 2023 09:47

Tgt Ion: 65 Resp: 237590
Ion Ratio Lower Upper
65 100
67 51.6 0.0 106.6


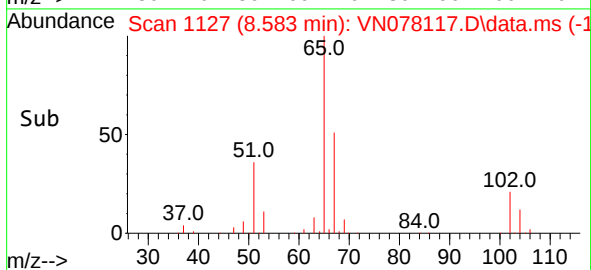
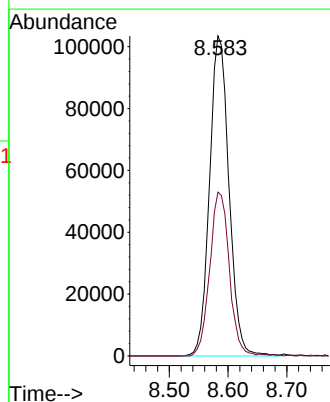
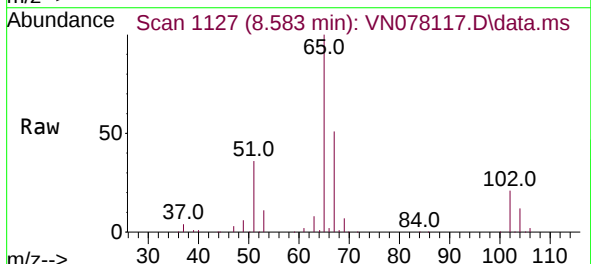


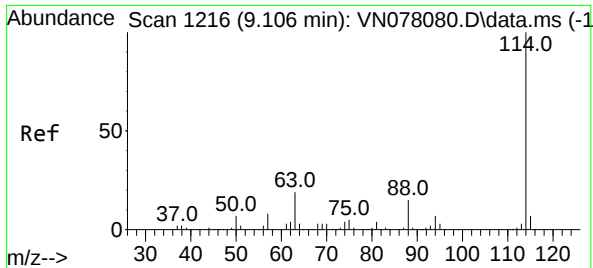

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN078117.D
Acq: 08 Jun 2023 09:47




Instrument :
MSVOA_N
ClientSampleId :
VN0608MBL01


Tgt Ion:114 Resp: 626439
Ion Ratio Lower Upper
114 100
63 21.5 0.0 36.4
88 15.4 0.0 30.6

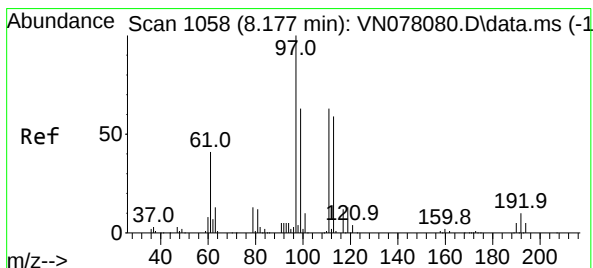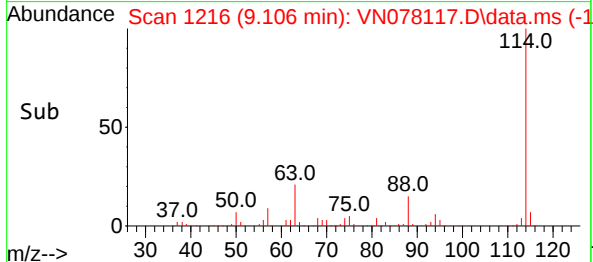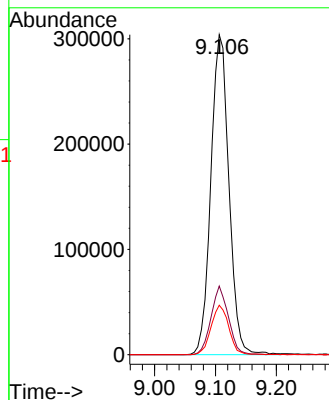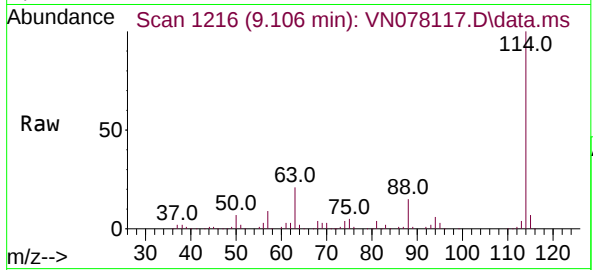

#35
Dibromofluoromethane
Concen: 53.012 ug/l
RT: 8.171 min Scan# 1057
Delta R.T. -0.006 min
Lab File: VN078117.D
Acq: 08 Jun 2023 09:47

Tgt Ion:113 Resp: 209974
Ion Ratio Lower Upper
113 100
111 101.6 82.6 123.8
192 16.4 12.7 19.1


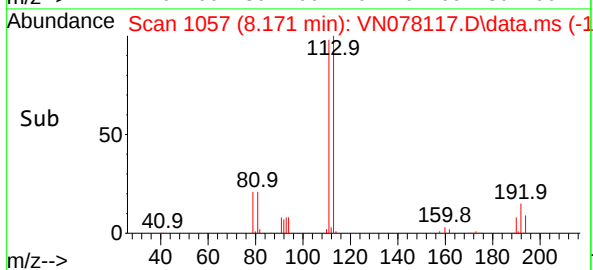
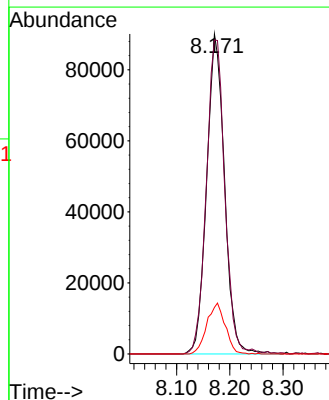
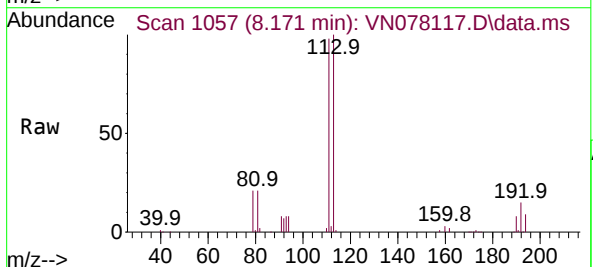


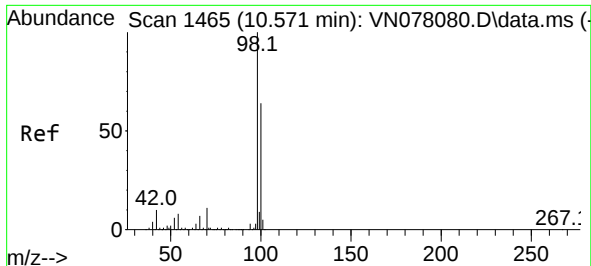

#50
Toluene-d8
Concen: 50.688 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.000 min
Lab File: VN078117.D
Acq: 08 Jun 2023 09:47




Instrument :
MSVOA_N
ClientSampleId :
VN0608MBL01


Tgt Ion: 98 Resp: 773988
Ion Ratio Lower Upper
98 100
100 63.5 52.0 78.0

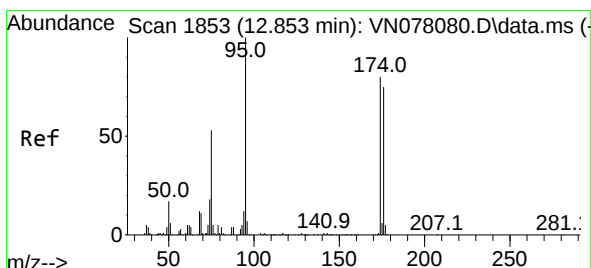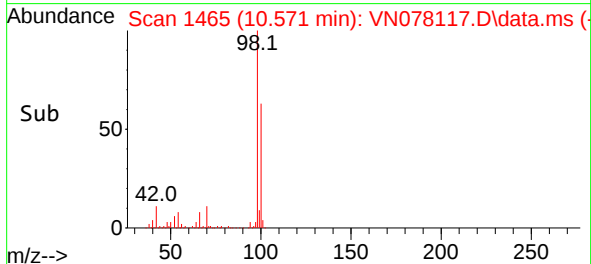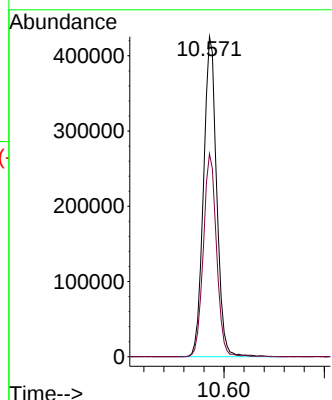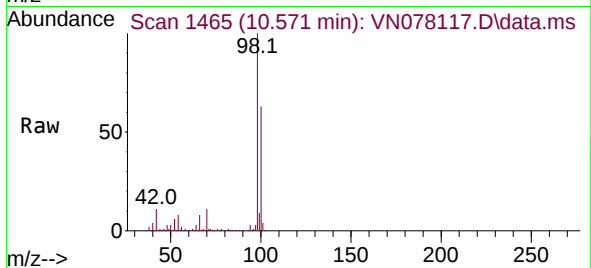

#62
4-Bromofluorobenzene
Concen: 45.832 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.000 min
Lab File: VN078117.D
Acq: 08 Jun 2023 09:47

Tgt Ion: 95 Resp: 217564
Ion Ratio Lower Upper
95 100
174 76.0 0.0 143.8
176 71.4 0.0 135.8

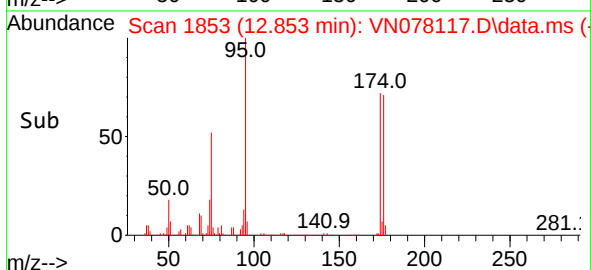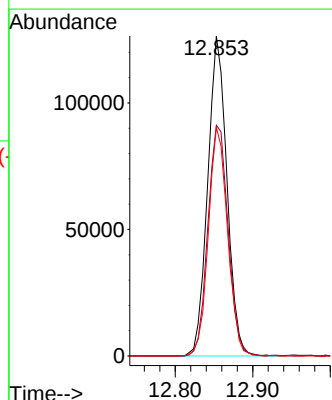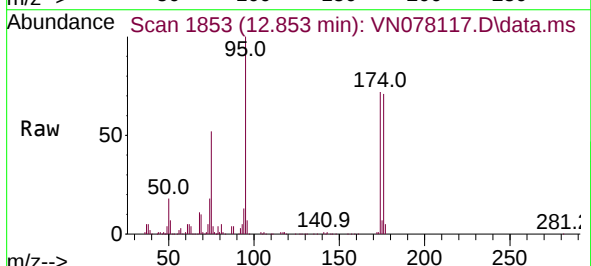

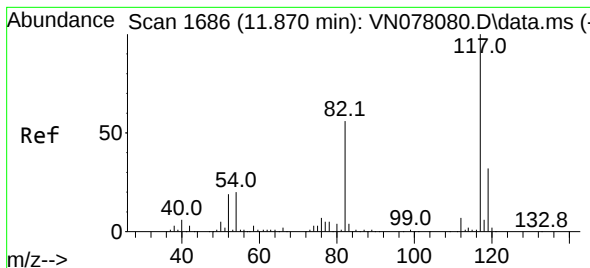

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.871 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN078117.D

Acq: 08 Jun 2023 09:47

Instrument :

MSVOA_N

ClientSampleId :

VN0608MBL01





Tgt Ion:117 Resp: 552987

Ion Ratio Lower Upper

117 100

82 53.2 44.0 66.0

119 30.1 25.6 38.4

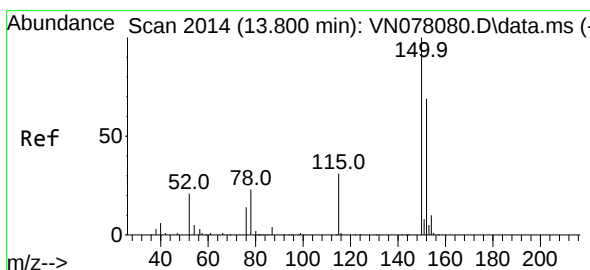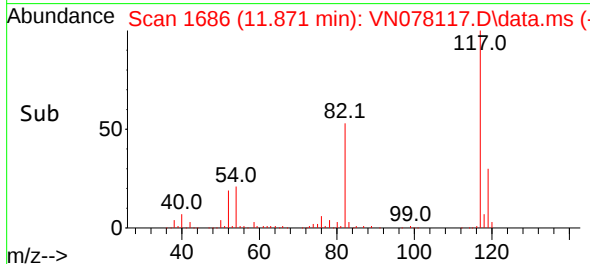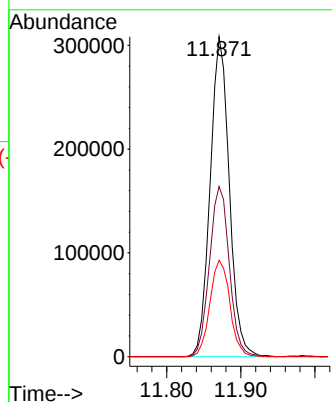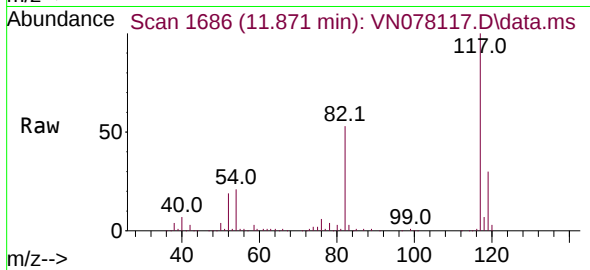

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.800 min Scan# 2014

Delta R.T. 0.000 min

Lab File: VN078117.D

Acq: 08 Jun 2023 09:47

Tgt Ion:152 Resp: 161210

Ion Ratio Lower Upper

152 100

115 63.0 32.3 96.8

150 163.0 0.0 355.8

