
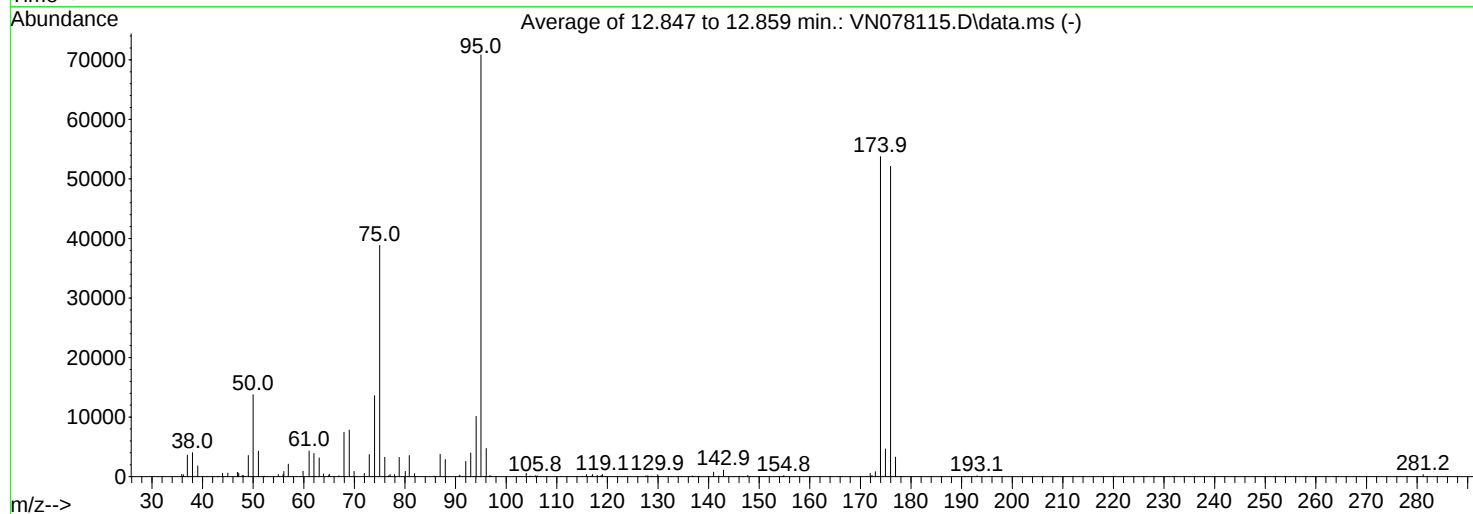


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060823\
Data File : VN078115.D
Acq On : 08 Jun 2023 08:19
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
Title : SW846 8260
Last Update : Wed Jun 07 05:05:00 2023

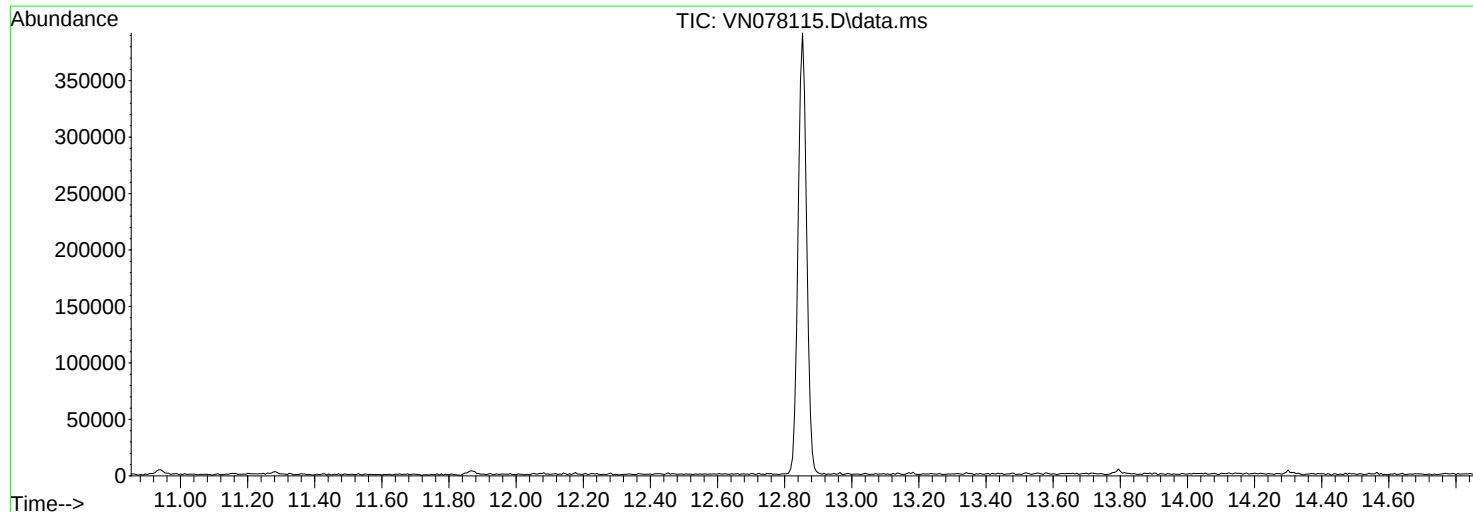

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	13771	PASS
75	95	30	60	54.8	38821	PASS
95	95	100	100	100.0	70843	PASS
96	95	5	9	6.7	4742	PASS
173	174	0.00	2	1.6	846	PASS
174	95	50	100	75.9	53736	PASS
175	174	5	9	8.7	4660	PASS
176	174	95	101	97.0	52107	PASS
177	176	5	9	6.3	3274	PASS

Average of 12.847 to 12.859 min.: VN078115.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	365	47.85	244	59.85	923	71.95	541
36.20	323	48.10	154	61.05	4300	72.95	3701
37.00	3594	49.05	3551	62.00	3910	74.00	1359
38.00	4021	50.00	13771	63.05	3140	75.00	3882
39.05	1815	51.05	4273	63.90	459	76.00	3267
40.90	61	52.20	72	64.90	168	76.80	176
42.90	15	52.80	61	65.05	413	77.05	362
43.95	566	54.95	354	66.95	157	77.95	350
45.00	580	55.90	358	67.95	7435	78.85	3234
46.90	717	56.05	851	69.00	7816	80.05	876
47.15	584	56.95	2086	69.95	892	80.85	3547

Average of 12.847 to 12.859 min.: VN078115.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.90	516	96.80	179	116.80	94	136.75	144
85.90	92	97.00	81	117.05	350	137.00	68
86.95	3770	103.10	59	118.00	218	141.00	748
87.95	2875	103.95	571	118.80	241	142.00	86
90.70	147	104.70	85	119.05	354	142.95	1116
90.85	281	104.90	85	127.60	124	145.00	64
92.00	2553	105.75	175	128.00	160	146.00	88
93.00	3986	106.10	170	128.80	94	146.80	60
94.05	10143	110.70	54	129.95	330	147.75	199
95.00	70843	115.10	62	132.70	54	154.60	54
96.05	4742	115.85	350	134.70	71	154.85	183

Average of 12.847 to 12.859 min.: VN078115.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
171.95	578						
172.30	190						
172.95	846						
173.95	53736						
174.95	4660						
175.95	52107						
176.95	3274						
178.10	58						
190.60	53						
193.05	160						
281.20	353						

Instrument :

MSVOA_N

ClientSampleId :

BFB