

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060922\
 Data File : VN072740.D
 Acq On : 09 Jun 2022 19:07
 Operator : JC\MD
 Sample : N3195-04RE
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 STORAGE-BLANK-SAMPLE-MANAGRE

Quant Time: Jun 10 01:46:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060822W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 09 05:17:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.081	168	158977	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.963	114	305633	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.745	117	279232	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.674	152	97849	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.433	65	258751	60.642	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 121.280%	
35) Dibromofluoromethane	8.016	113	182198	60.247	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 120.500%	
50) Toluene-d8	10.439	98	611215	50.657	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 101.320%	
62) 4-Bromofluorobenzene	12.727	95	212963	51.436	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 102.880%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060922\
Data File : VN072740.D
Acq On : 09 Jun 2022 19:07
Operator : JC\MD
Sample : N3195-04RE
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAGRE

Quant Time: Jun 10 01:46:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060822W.M
Quant Title : SW846 8260
QLast Update : Thu Jun 09 05:17:31 2022
Response via : Initial Calibration




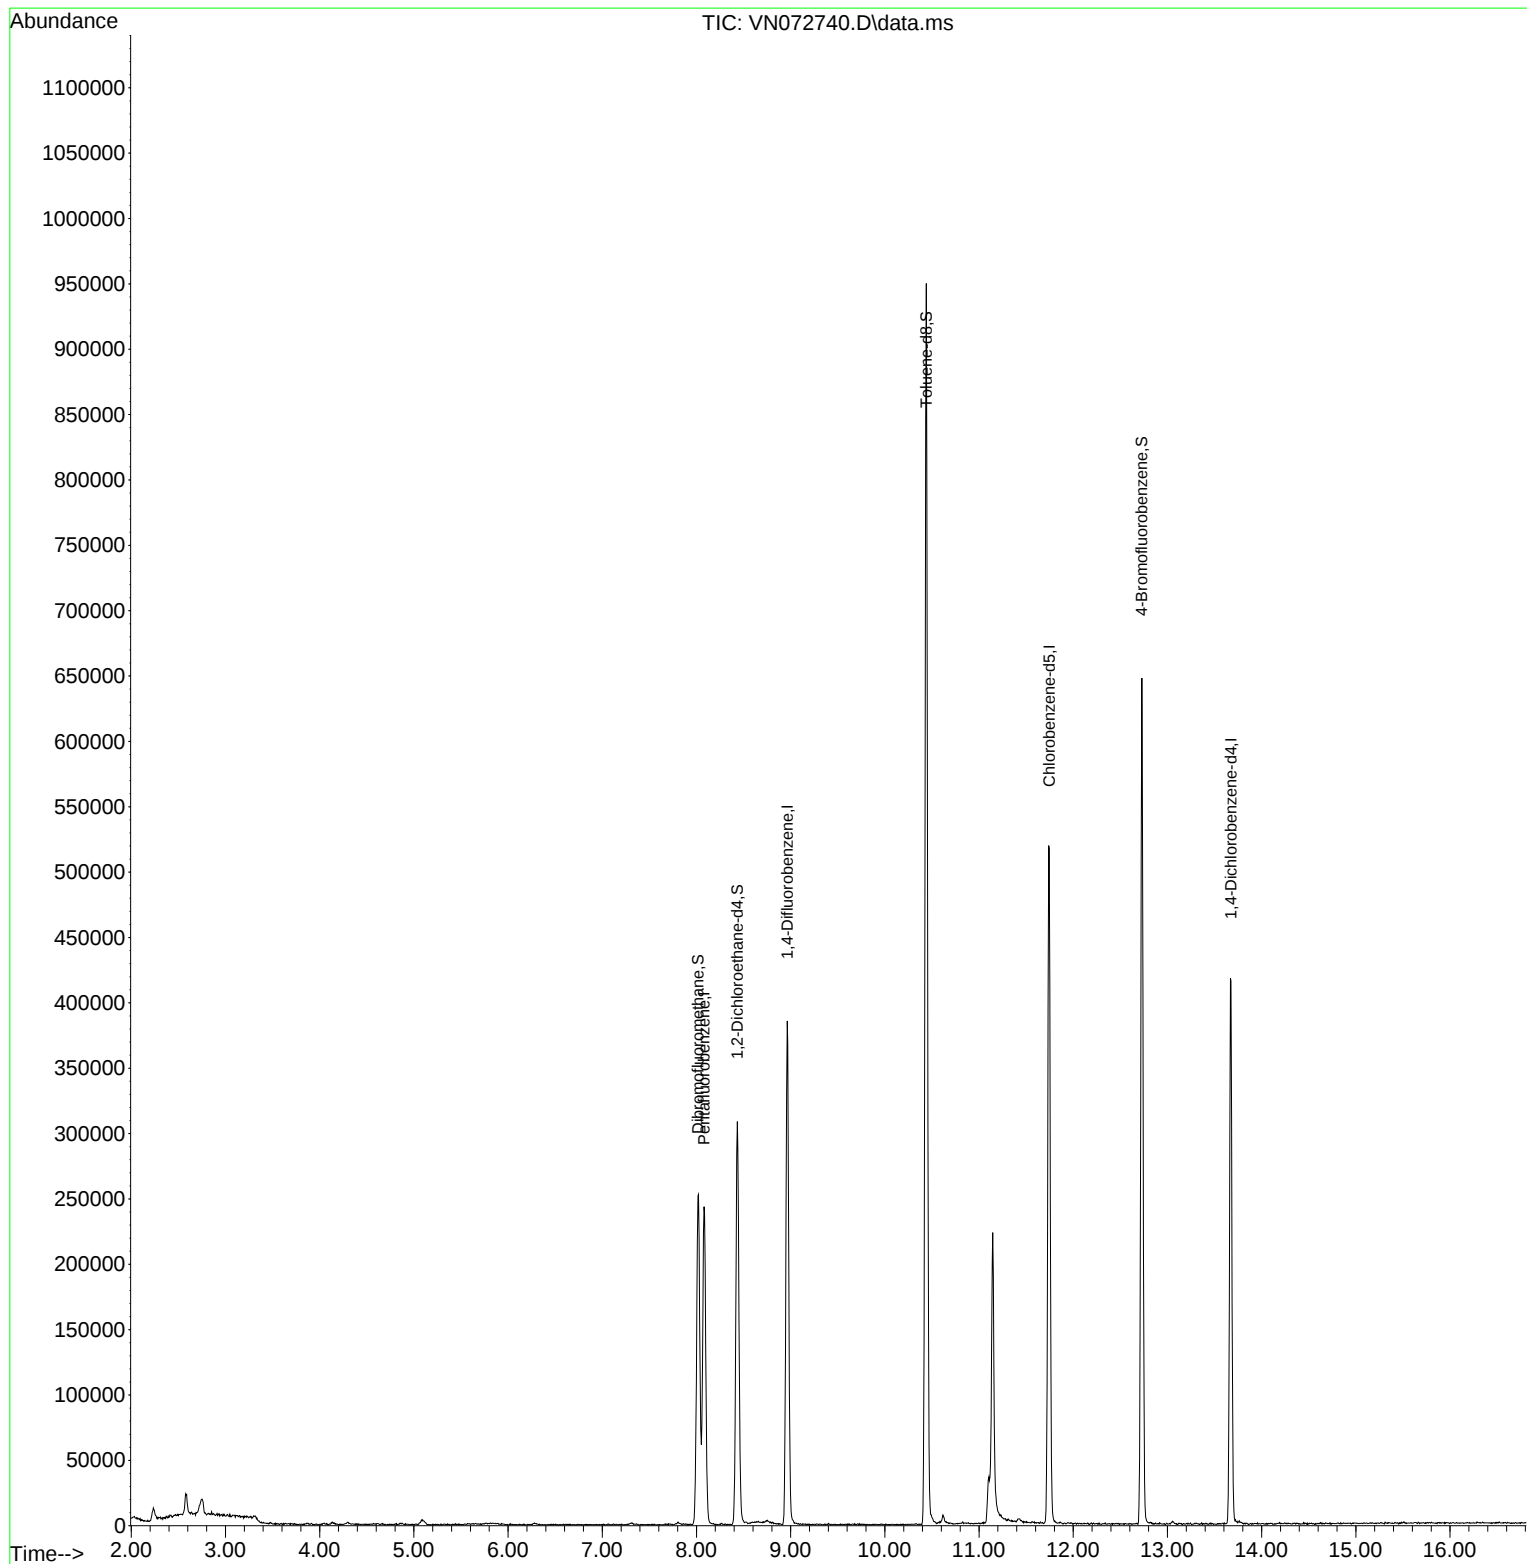


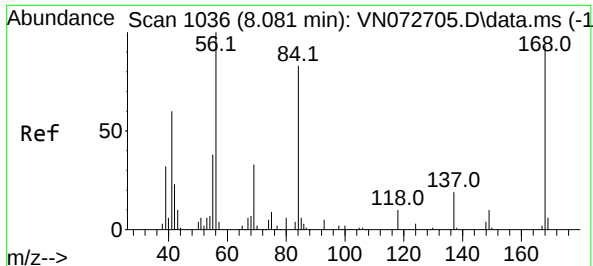

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.000 min
Lab File: VN072740.D
Acq: 09 Jun 2022 19:07




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAGRE


Tgt Ion:168 Resp: 158977
Ion Ratio Lower Upper
168 100
99 71.9 42.3 63.5#

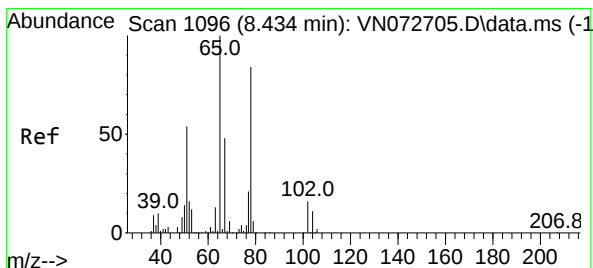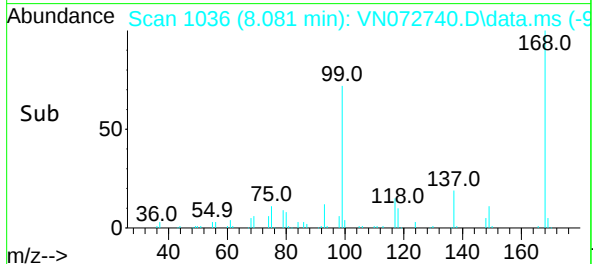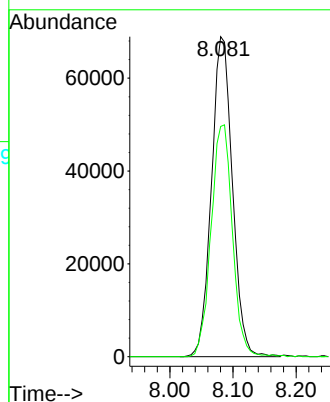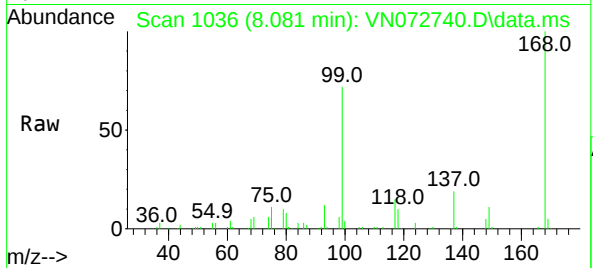

#33
1,2-Dichloroethane-d4
Concen: 60.642 ug/l
RT: 8.433 min Scan# 1096
Delta R.T. -0.001 min
Lab File: VN072740.D
Acq: 09 Jun 2022 19:07

Tgt Ion: 65 Resp: 258751
Ion Ratio Lower Upper
65 100
67 49.5 0.0 104.8

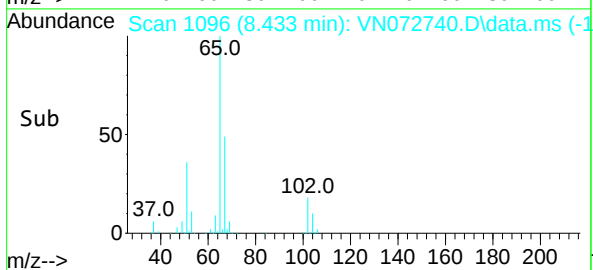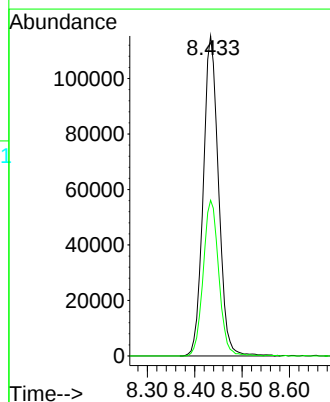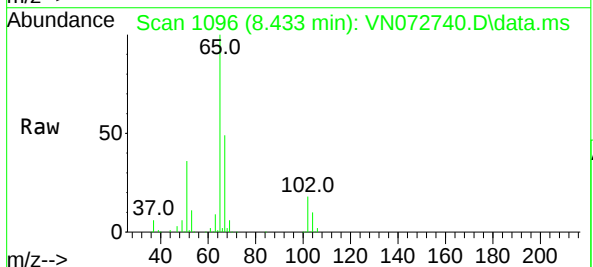

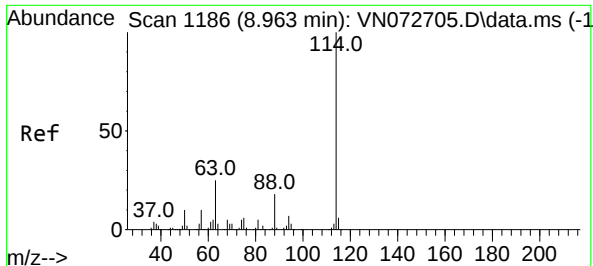

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.963 min Scan# 1186

Delta R.T. -0.000 min

Lab File: VN072740.D

Acq: 09 Jun 2022 19:07

Instrument :

MSVOA_N

ClientSampleId :

STORAGE-BLANK-SAMPLE-MANAGRE





Tgt Ion:114 Resp: 305633

Ion Ratio Lower Upper

114 100

63 25.5 0.0 40.0

88 17.1 0.0 32.6

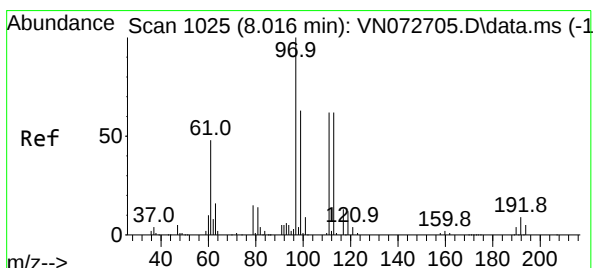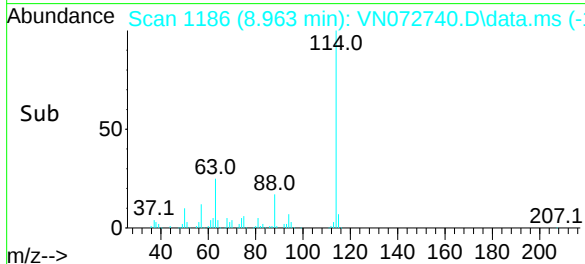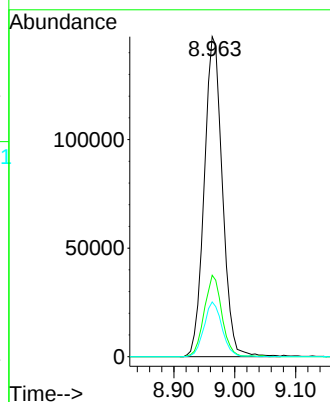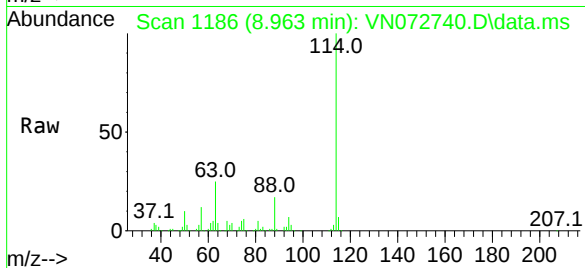

#35

Dibromofluoromethane

Concen: 60.247 ug/l

RT: 8.016 min Scan# 1025

Delta R.T. -0.000 min

Lab File: VN072740.D

Acq: 09 Jun 2022 19:07




Tgt Ion:113 Resp: 182198


Ion Ratio Lower Upper

113 100

111 101.3 81.4 122.0

192 15.0 17.0 25.6#


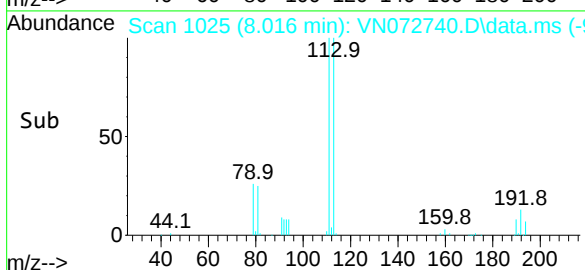
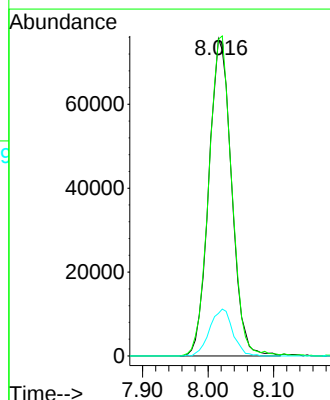
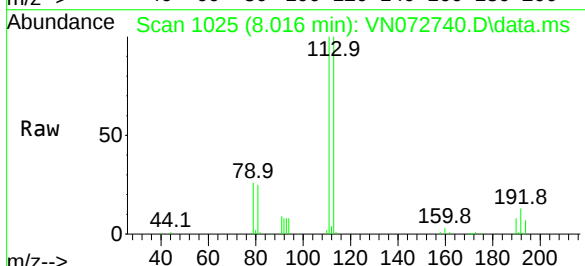


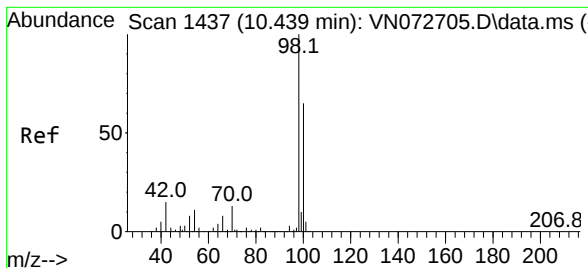

#50
Toluene-d8
Concen: 50.657 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN072740.D
Acq: 09 Jun 2022 19:07




Instrument : MSVOA_N
ClientSampleId : STORAGE-BLANK-SAMPLE-MANAGRE


Tgt Ion: 98 Resp: 611215
Ion Ratio Lower Upper
98 100
100 65.3 52.6 78.8

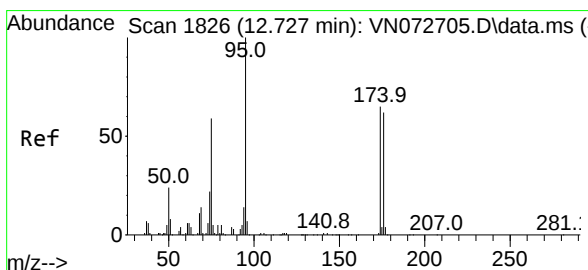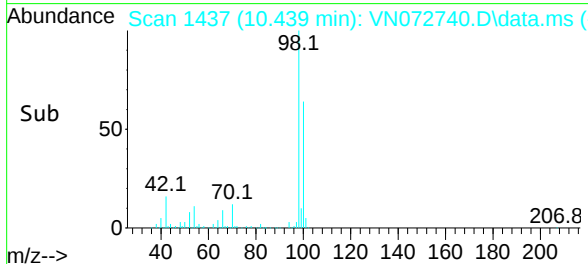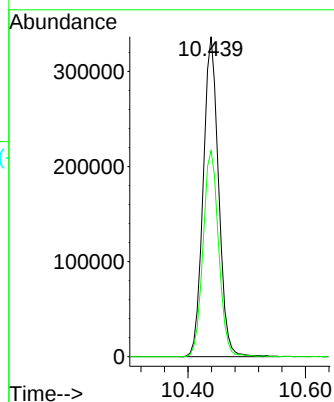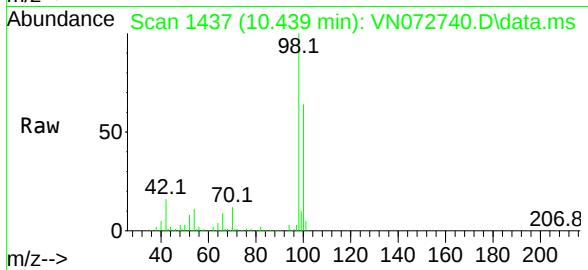

#62
4-Bromofluorobenzene
Concen: 51.436 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN072740.D
Acq: 09 Jun 2022 19:07

Tgt Ion: 95 Resp: 212963
Ion Ratio Lower Upper
95 100
174 63.1 0.0 167.6
176 62.1 0.0 163.4

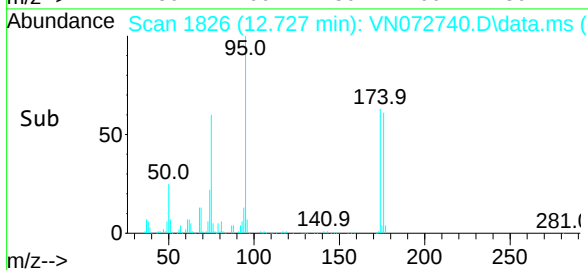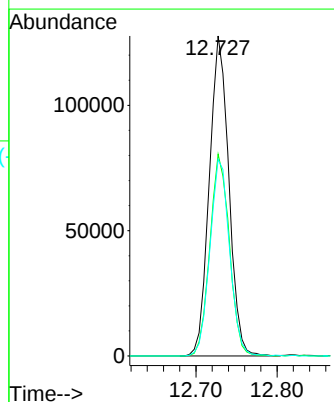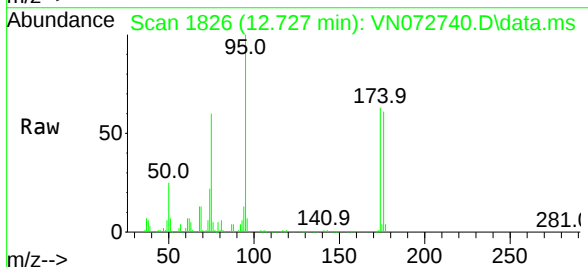

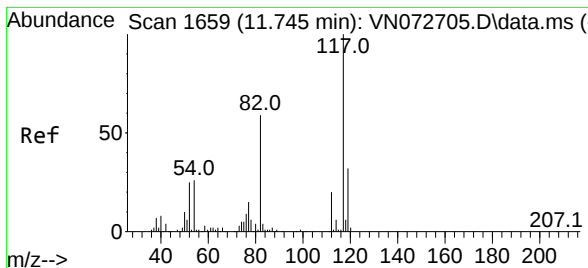

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.745 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN072740.D


Acq: 09 Jun 2022 19:07

Instrument :

MSVOA_N

ClientSampleId :

STORAGE-BLANK-SAMPLE-MANAGRE

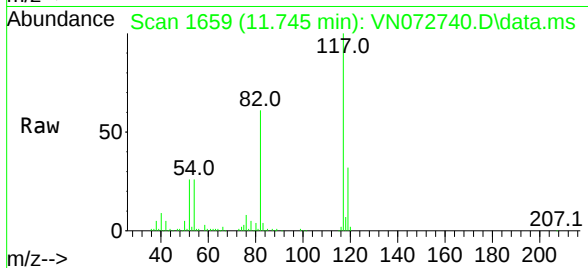




Tgt Ion:117 Resp: 279232

Ion Ratio Lower Upper

117 100

82 61.1 44.2 66.2

119 31.8 25.4 38.0

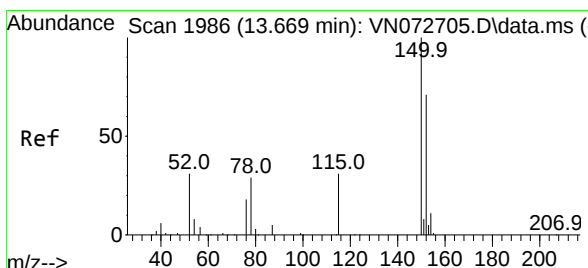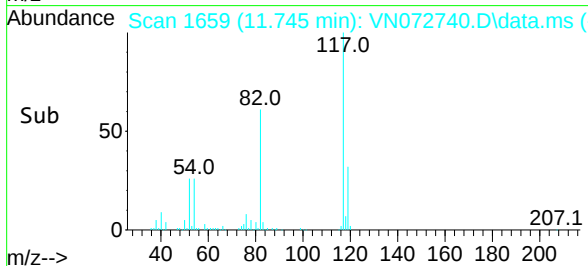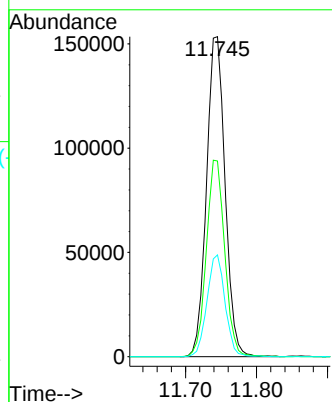

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.674 min Scan# 1987

Delta R.T. 0.005 min

Lab File: VN072740.D

Acq: 09 Jun 2022 19:07

Tgt Ion:152 Resp: 97849

Ion Ratio Lower Upper

152 100

115 69.5 28.9 86.7

150 160.8 0.0 356.2

