
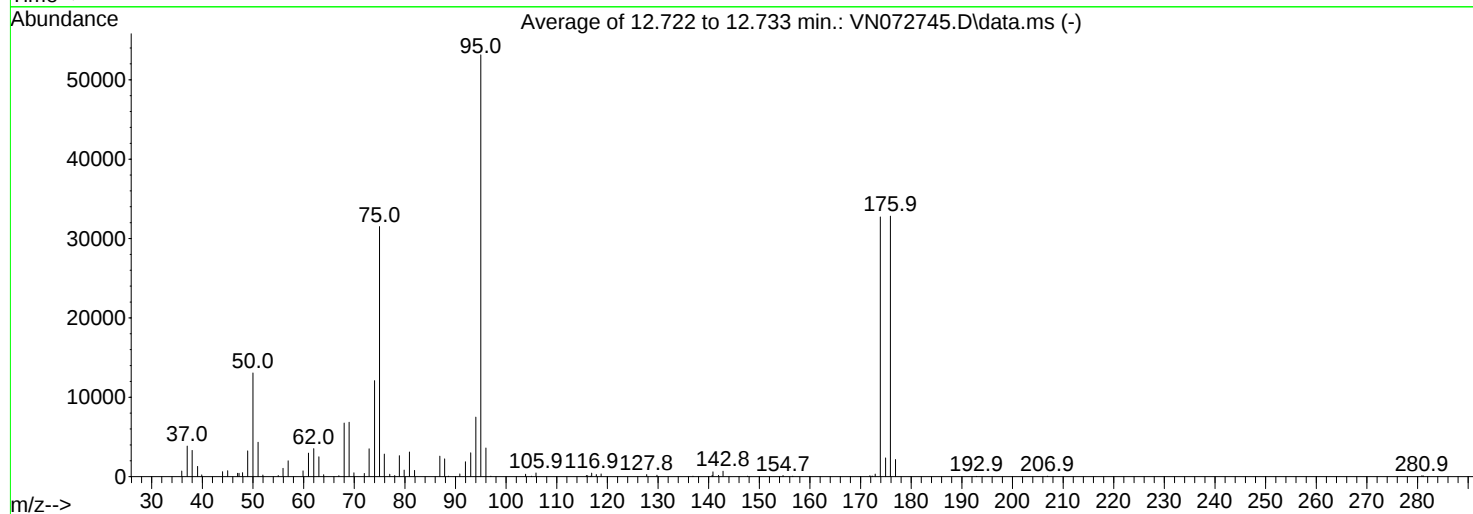


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060922\
Data File : VN072745.D
Acq On : 09 Jun 2022 21:34
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060822W.M
Title : SW846 8260
Last Update : Thu Jun 09 05:17:31 2022

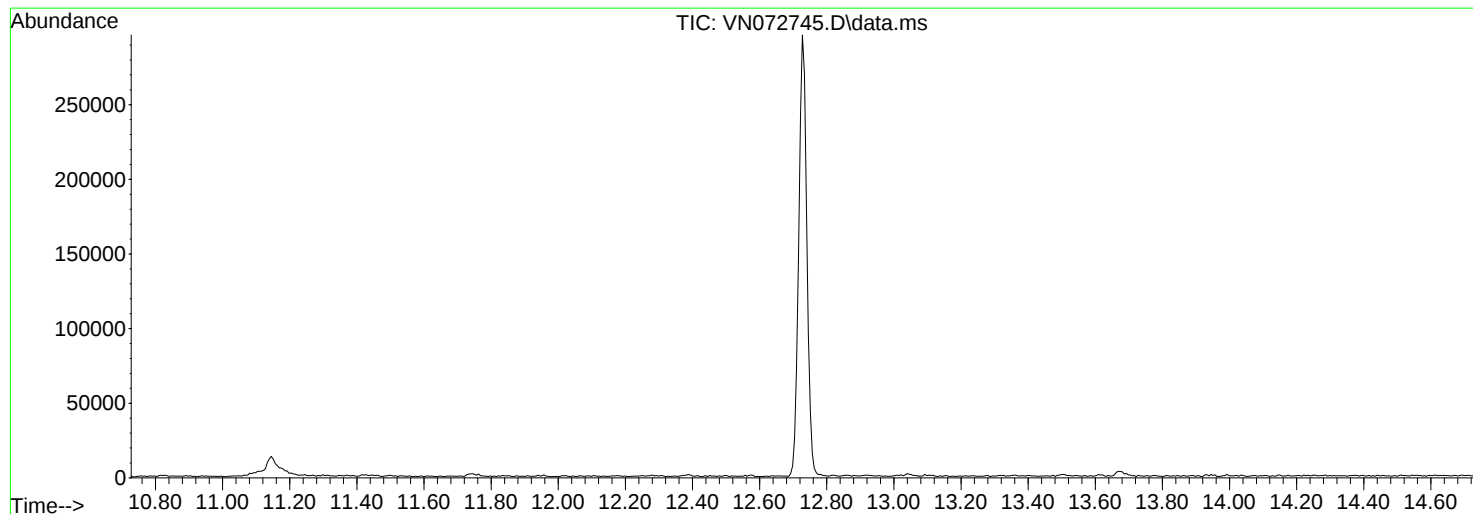

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1817

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.6	13062	PASS
75	95	30	60	59.3	31509	PASS
95	95	100	100	100.0	53141	PASS
96	95	5	9	6.8	3614	PASS
173	174	0.00	2	1.0	333	PASS
174	95	50	100	61.6	32709	PASS
175	174	5	9	7.2	2351	PASS
176	174	95	101	100.3	32811	PASS
177	176	5	9	6.6	2157	PASS