

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060923\
 Data File : VN078138.D
 Acq On : 09 Jun 2023 11:58
 Operator : JC\MD
 Sample : 03123-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :


Quant Time: Jun 09 23:05:58 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 07 05:05:00 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	350243	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	639316	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	542041	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	136032	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.589	65	245563	52.585	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 105.180%			
35) Dibromofluoromethane	8.177	113	208891	51.676	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 103.360%			
50) Toluene-d8	10.571	98	791875	50.815	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 101.620%			
62) 4-Bromofluorobenzene	12.853	95	213779	44.128	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 88.260%			
Target Compounds						Qvalue
3) Chloromethane	2.371	50	1294	Below Cal		92
5) Bromomethane	2.983	94	2463	0.629 ug/l		93
10) Methyl Iodide	4.595	142	1748	0.333 ug/l #		91
11) Tert butyl alcohol	5.548	59	234	0.363 ug/l #		72
13) Acrolein	4.201	56	343	0.483 ug/l		85
15) Acrylonitrile	5.736	53	575	0.346 ug/l #		83
16) Acetone	4.460	43	5827	4.335 ug/l		95
18) Methyl Acetate	5.036	43	1822	0.294 ug/l #		56
25) 2-Butanone	7.495	43	4430	2.143 ug/l		94
29) Tetrahydrofuran	7.842	42	280	0.203 ug/l #		20
31) Cyclohexane	8.236	56	8083	1.349 ug/l #		34
36) 1,1-Dichloropropene	8.230	75	30499	5.260 ug/l #		49
38) Carbon Tetrachloride	8.230	117	39129	6.391 ug/l #		13
43) Isopropyl Acetate	8.742	43	3008	0.347 ug/l #		49
51) 4-Methyl-2-Pentanone	10.453	43	1905	0.418 ug/l #		63
59) 2-Hexanone	11.206	43	2453	0.772 ug/l		63
71) Bromoform	12.859	173	1772	0.643 ug/l #		1
75) 1,1,2,2-Tetrachloroethane	12.935	83	754	Below Cal #		89
76) 1,2,3-Trichloropropane	12.853	75	118728	36.920 ug/l #		1
81) trans-1,4-Dichloro-2-b...	12.853	75	118728	113.429 ug/l #		15
82) 4-Chlorotoluene	13.230	91	2184	0.259 ug/l		90
86) p-Isopropyltoluene	13.741	119	2117	0.220 ug/l		98
87) 1,3-Dichlorobenzene	13.730	146	1408	0.279 ug/l		96
88) 1,4-Dichlorobenzene	13.730	146	1408	0.289 ug/l		94
89) n-Butylbenzene	14.065	91	2923	0.385 ug/l		89
91) 1,2-Dichlorobenzene	14.118	146	1211	0.245 ug/l #		54
92) 1,2-Dibromo-3-Chloropr...	14.729	75	360	0.565 ug/l #		30
93) 1,2,4-Trichlorobenzene	15.394	180	1495	0.850 ug/l		91
94) Hexachlorobutadiene	15.518	225	1175	Below Cal		84
95) Naphthalene	15.647	128	5151	0.871 ug/l		97
96) 1,2,3-Trichlorobenzene	15.847	180	1850	0.940 ug/l		87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jun 09 23:05:58 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 07 05:05:00 2023
Response via : Initial Calibration

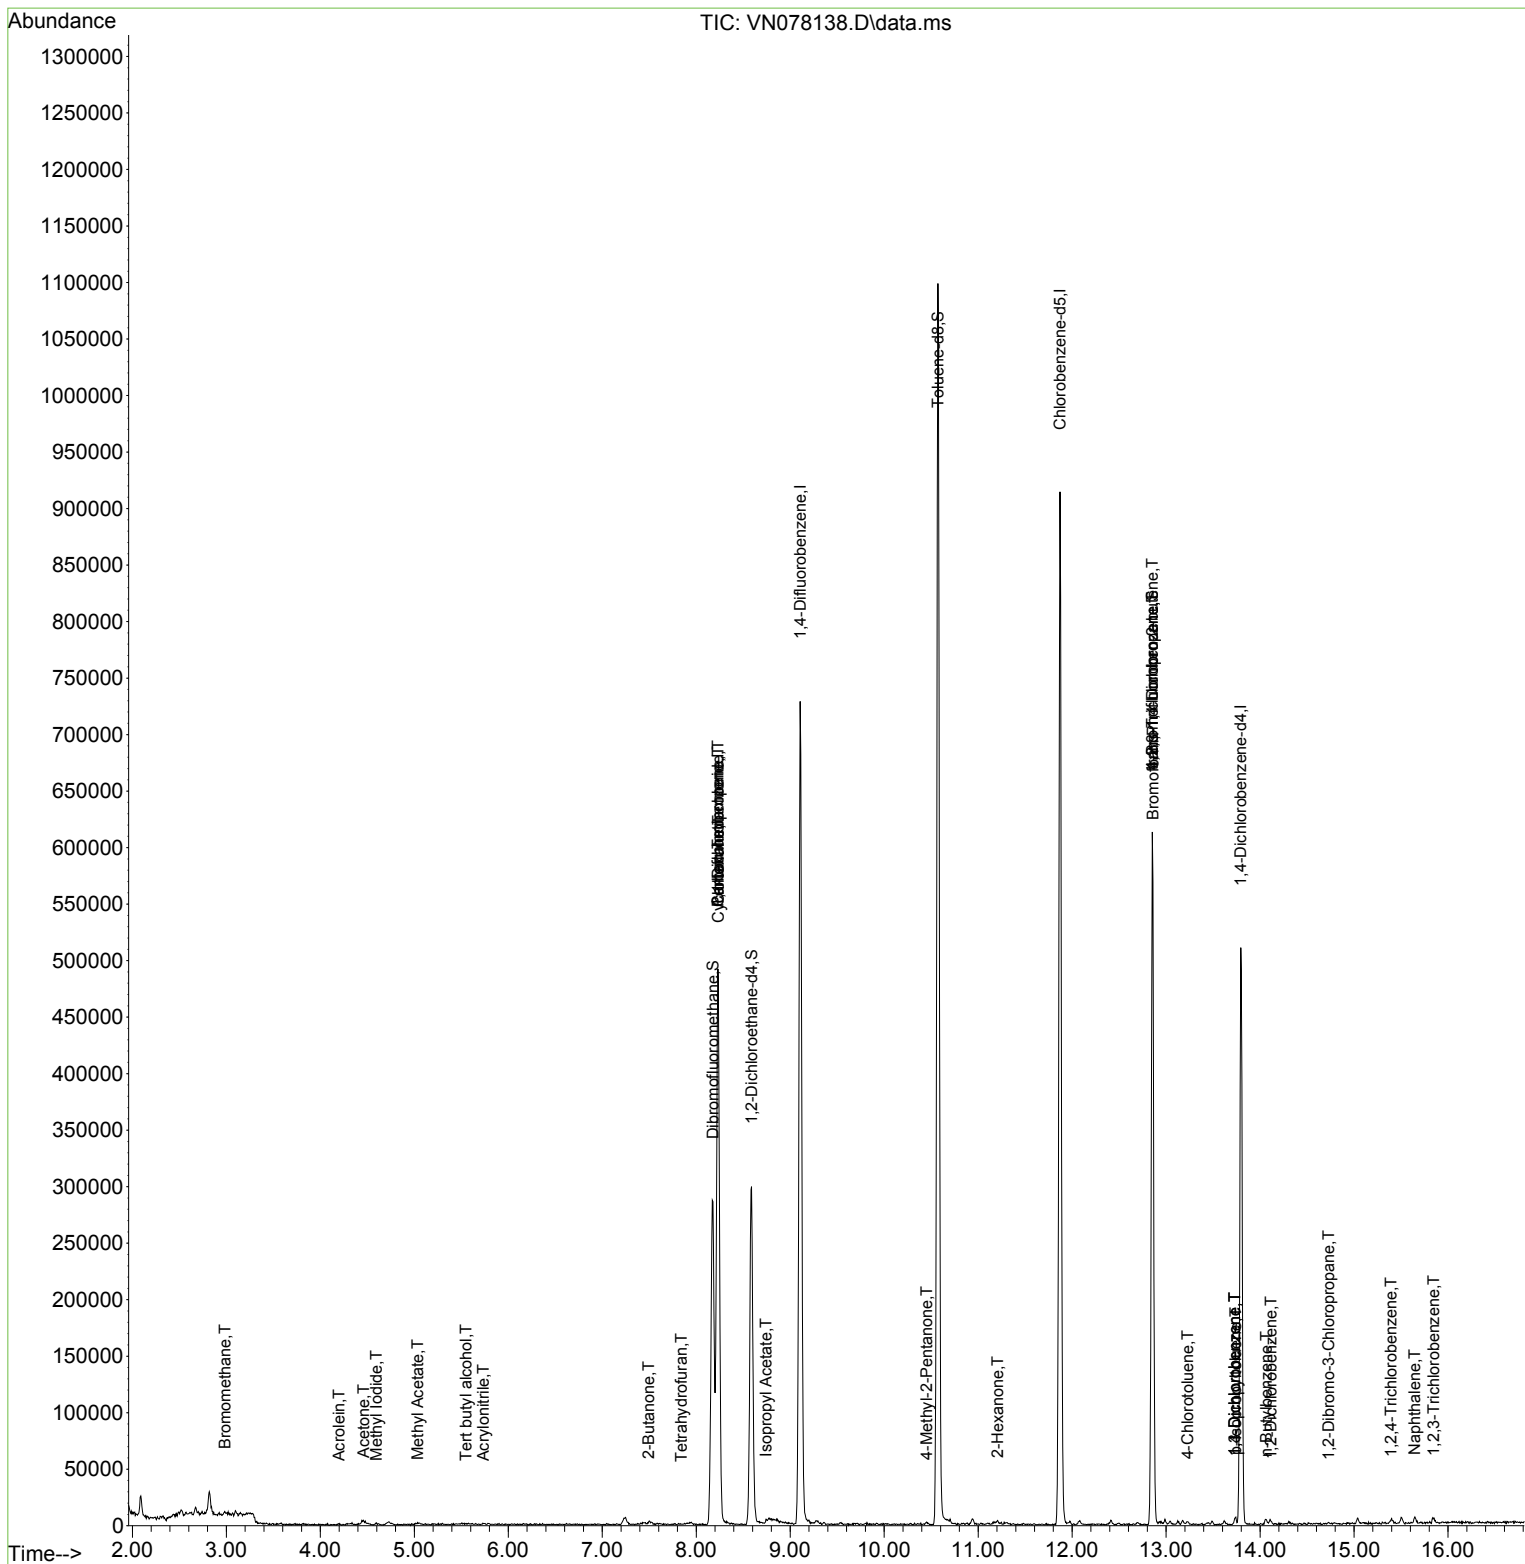




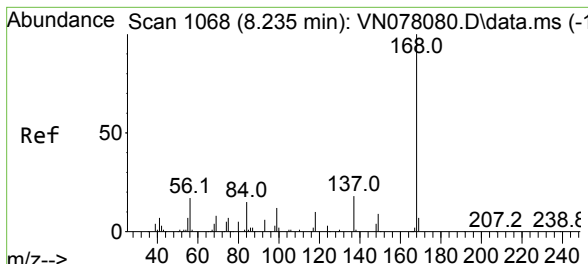


#1
 Pentafluorobenzene
 Concen: 50.000 ug/l
 RT: 8.230 min Scan# 10
 Delta R.T. -0.005 min
 Lab File: VN078138.D
 Acq: 09 Jun 2023 11:58

Instrument :
 MSVOA_N
 ClientSampleId :

Tgt Ion:168 Resp: 350243




Ion	Ratio	Lower	Upper
168	100		
99	61.4	53.0	79.6

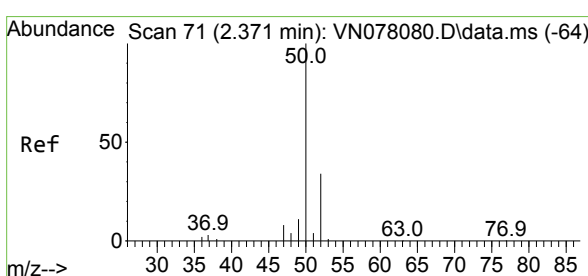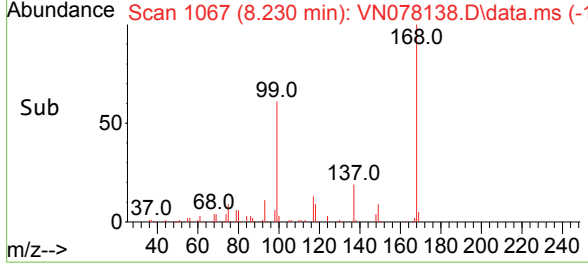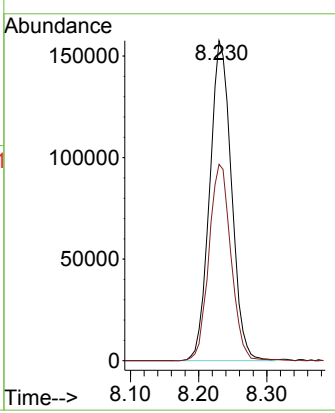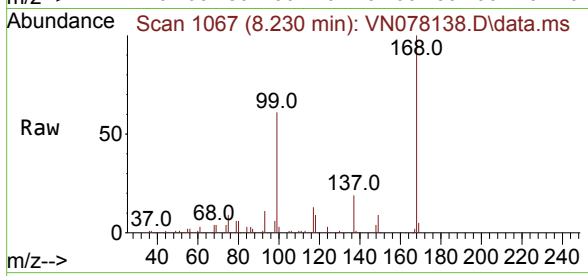


#3
 Chloromethane
 Concen: Below Cal
 RT: 2.371 min Scan# 71
 Delta R.T. 0.000 min
 Lab File: VN078138.D
 Acq: 09 Jun 2023 11:58

Tgt Ion: 50 Resp: 1294

Ion	Ratio	Lower	Upper
50	100		
52	37.4	26.5	39.7


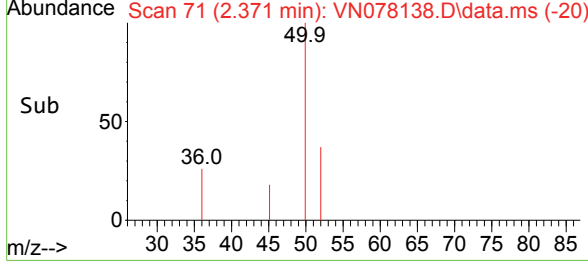
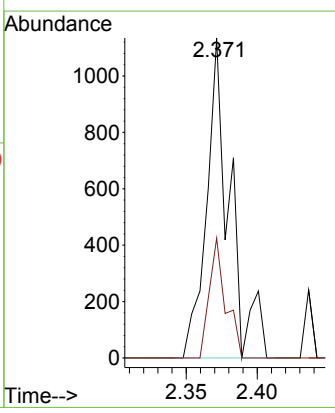
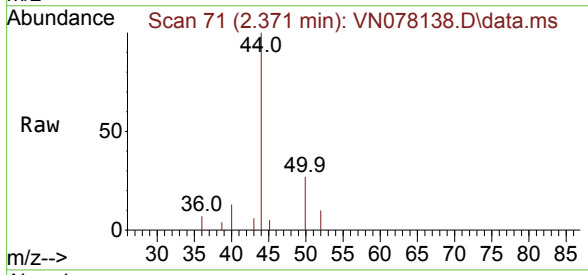




#5
Bromomethane
Concen: 0.629 ug/l
RT: 2.983 min Scan# 11
Delta R.T. 0.030 min
Lab File: VN078138.D
Acq: 09 Jun 2023 11:58




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 94 Resp: 2463
Ion Ratio Lower Upper
94 100
96 84.6 73.1 109.7



#10
Methyl Iodide
Concen: 0.333 ug/l
RT: 4.595 min Scan# 449
Delta R.T. 0.000 min
Lab File: VN078138.D
Acq: 09 Jun 2023 11:58

Tgt Ion: 142 Resp: 1748
Ion Ratio Lower Upper
142 100
127 46.6 37.6 56.4
141 0.0 11.4 17.0#

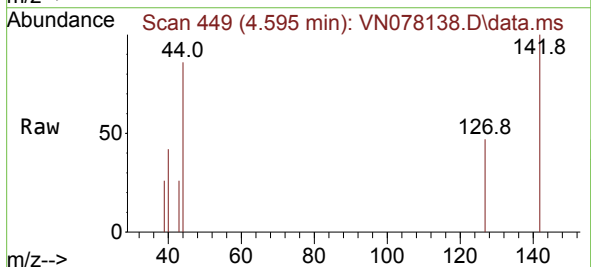



#11

Tert butyl alcohol

Concen: 0.363 ug/l

RT: 5.548 min Scan# 611

Delta R.T. 0.012 min

Lab File: VN078138.D

Acq: 09 Jun 2023 11:58

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 59 Resp: 234

Ion Ratio Lower Upper

59 100

57 0.0 8.2 12.4#

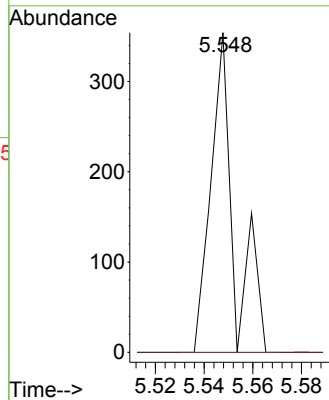

#13

Acrolein

Concen: 0.483 ug/l

RT: 4.201 min Scan# 382

Delta R.T. 0.012 min

Lab File: VN078138.D




Acq: 09 Jun 2023 11:58


Tgt Ion: 56 Resp: 343

Ion Ratio Lower Upper

56 100


55 79.9 54.5 81.7

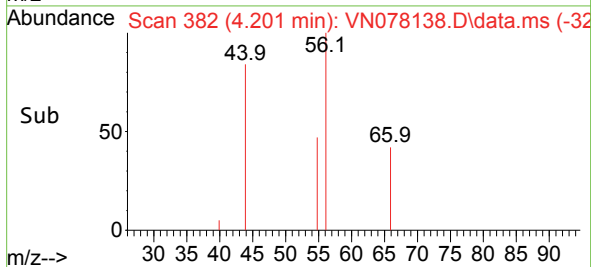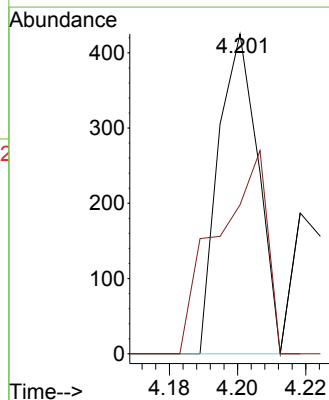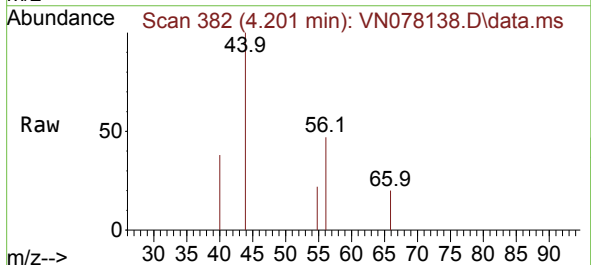






#15
Acrylonitrile
Concen: 0.346 ug/l
RT: 5.736 min Scan# 642
Delta R.T. 0.006 min
Lab File: VN078138.D
Acq: 09 Jun 2023 11:58

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 53 Resp: 575
Ion Ratio Lower Upper
53 100
52 101.9 65.3 97.9#
51 38.3 28.9 43.3



#16
Acetone
Concen: 4.335 ug/l
RT: 4.460 min Scan# 426
Delta R.T. 0.024 min
Lab File: VN078138.D
Acq: 09 Jun 2023 11:58


Tgt Ion: 43 Resp: 5827
Ion Ratio Lower Upper
43 100
58 32.2 28.0 42.0








#18
Methyl Acetate
Concen: 0.294 ug/l
RT: 5.036 min Scan# 51
Delta R.T. 0.000 min
Lab File: VN078138.D
Acq: 09 Jun 2023 11:58

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 43 Resp: 1822
Ion Ratio Lower Upper
43 100
74 8.2 26.2 39.4#

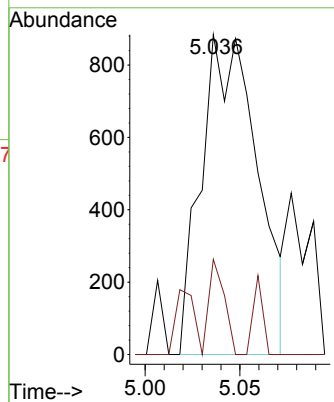

#25
2-Butanone
Concen: 2.143 ug/l
RT: 7.495 min Scan# 942
Delta R.T. 0.000 min
Lab File: VN078138.D
Acq: 09 Jun 2023 11:58

Tgt Ion: 43 Resp: 4430
Ion Ratio Lower Upper
43 100
72 41.3 30.2 45.2

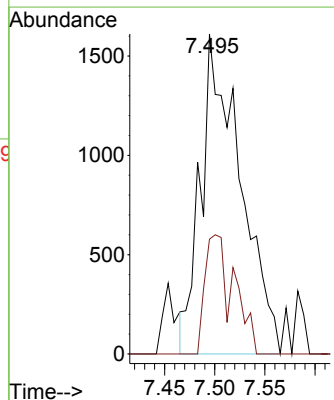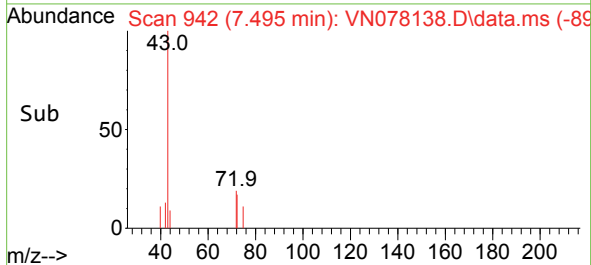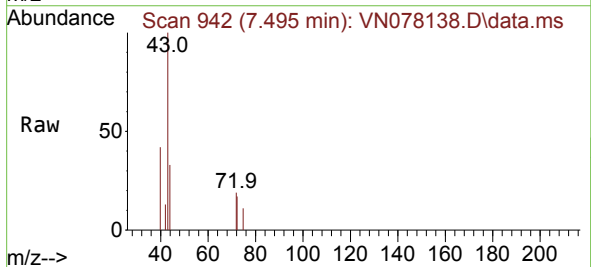



#29

Tetrahydrofuran

Concen: 0.203 ug/l

RT: 7.842 min Scan# 1001

Delta R.T. -0.006 min


Lab File: VN078138.D

Acq: 09 Jun 2023 11:58




Instrument :

MSVOA_N

ClientSampleId :



Tgt Ion:	42	Resp:	280
Ion	Ratio	Lower	Upper
42	100		
72	0.0	49.8	74.6#
71	0.0	47.4	71.2#



#31

Cyclohexane

Concen: 1.349 ug/l




RT: 8.236 min Scan# 1068


Delta R.T. -0.029 min

Lab File: VN078138.D

Acq: 09 Jun 2023 11:58

Tgt Ion:	56	Resp:	8083
Ion	Ratio	Lower	Upper
56	100		
69	153.3	26.8	40.2#
84	120.9	81.8	122.6

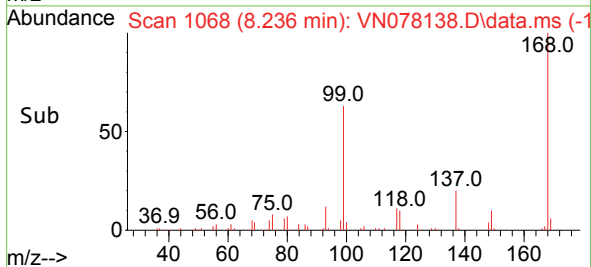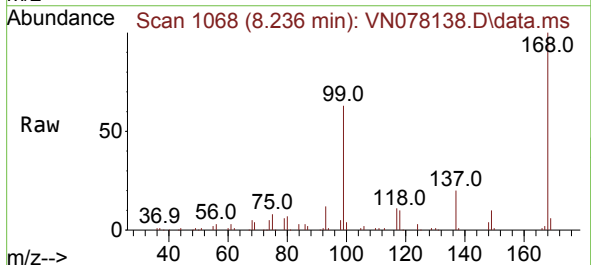



#33

1,2-Dichloroethane-d4

Concen: 52.585 ug/l

RT: 8.589 min Scan# 1128

Delta R.T. 0.006 min

Lab File: VN078138.D

Acq: 09 Jun 2023 11:58

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 65 Resp: 245563

Ion Ratio Lower Upper

65 100

67 50.9 0.0 106.6

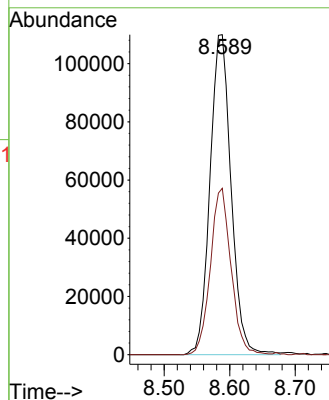

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1216

Delta R.T. 0.000 min

Lab File: VN078138.D

Acq: 09 Jun 2023 11:58




Tgt Ion:114 Resp: 639316


Ion Ratio Lower Upper

114 100

63 19.6 0.0 36.4


88 16.0 0.0 30.6

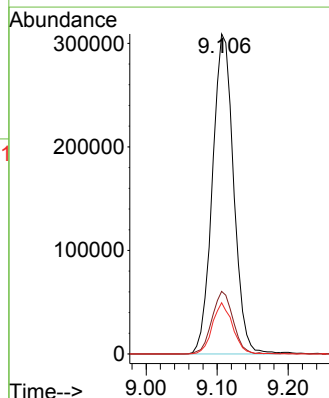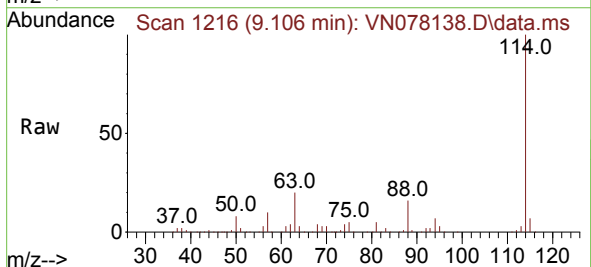






#35
Dibromofluoromethane
Concen: 51.676 ug/l
RT: 8.177 min Scan# 1058
Delta R.T. 0.000 min
Lab File: VN078138.D
Acq: 09 Jun 2023 11:58


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:113 Resp: 208891
Ion Ratio Lower Upper
113 100
111 104.0 82.6 123.8
192 17.2 12.7 19.1




#36
1,1-Dichloropropene
Concen: 5.260 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.147 min
Lab File: VN078138.D
Acq: 09 Jun 2023 11:58

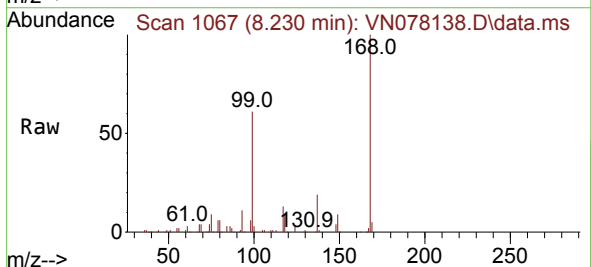

Tgt Ion: 75 Resp: 30499
Ion Ratio Lower Upper
75 100
110 10.4 19.1 57.3#
77 0.0 25.0 37.4#

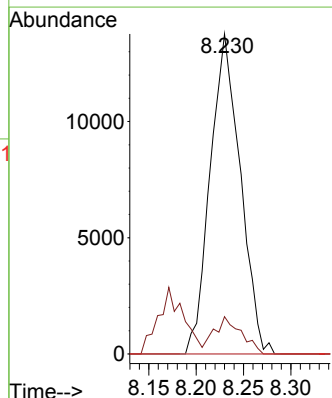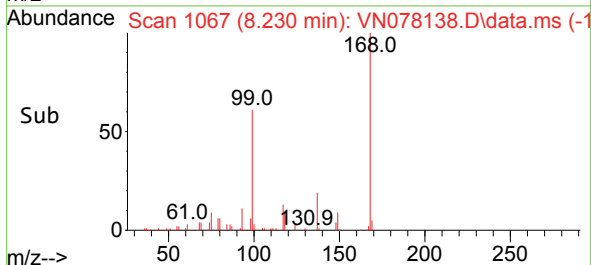



#38

Carbon Tetrachloride

Concen: 6.391 ug/l

RT: 8.230 min Scan# 1067

Delta R.T. -0.141 min


Lab File: VN078138.D

Acq: 09 Jun 2023 11:58

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion:117 Resp: 39129

Ion Ratio Lower Upper

117 100

119 1.9 77.3 115.9#

121 0.0 23.3 34.9#

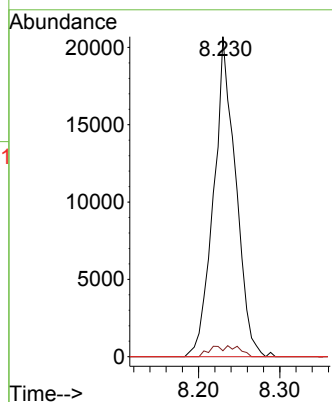

#43

Isopropyl Acetate

Concen: 0.347 ug/l

RT: 8.742 min Scan# 1154

Delta R.T. 0.047 min

Lab File: VN078138.D

Acq: 09 Jun 2023 11:58




Tgt Ion: 43 Resp: 3008


Ion Ratio Lower Upper

43 100

61 0.0 24.7 37.1#

87 0.0 14.6 21.8#



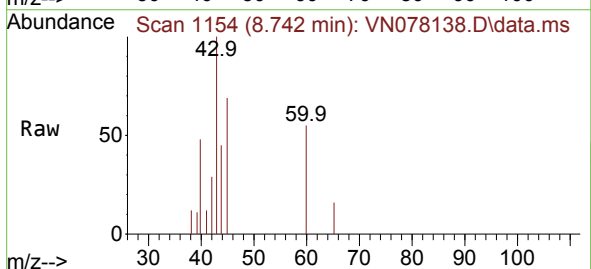





#50
Toluene-d8
Concen: 50.815 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.000 min
Lab File: VN078138.D
Acq: 09 Jun 2023 11:58




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 98 Resp: 791875
Ion Ratio Lower Upper
98 100
100 62.3 52.0 78.0

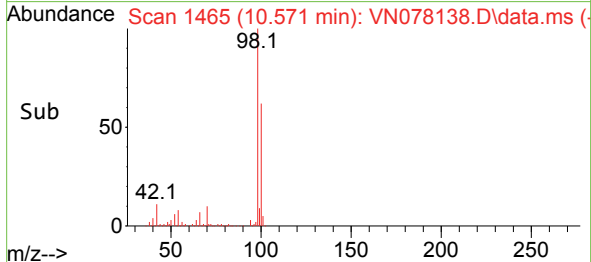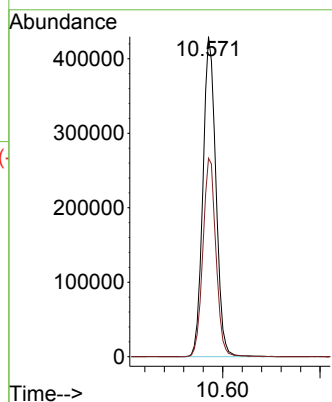

#51
4-Methyl-2-Pentanone
Concen: 0.418 ug/l
RT: 10.453 min Scan# 1445
Delta R.T. 0.000 min
Lab File: VN078138.D
Acq: 09 Jun 2023 11:58

Tgt Ion: 43 Resp: 1905
Ion Ratio Lower Upper
43 100
58 21.1 36.6 54.8#


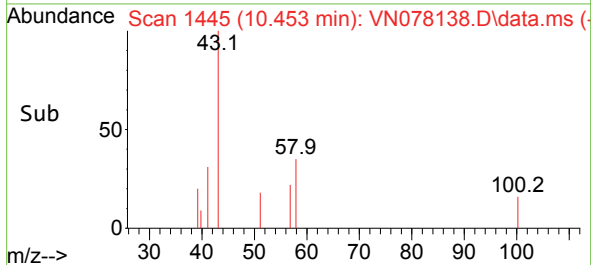

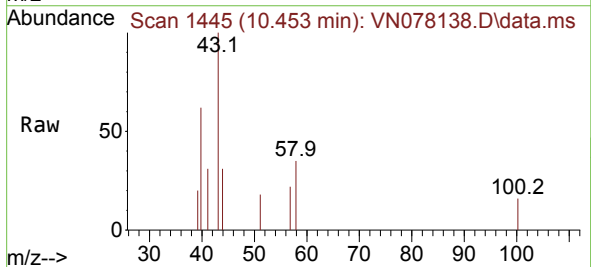




#59
2-Hexanone
Concen: 0.772 ug/l
RT: 11.206 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN078138.D
Acq: 09 Jun 2023 11:58




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 2453
Ion Ratio Lower Upper
43 100
58 34.9 31.7 95.1

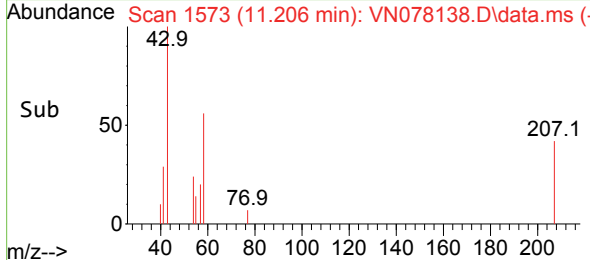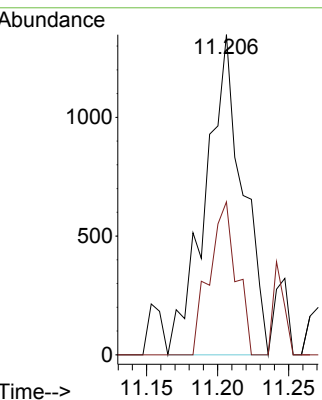

#62
4-Bromofluorobenzene
Concen: 44.128 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.000 min
Lab File: VN078138.D
Acq: 09 Jun 2023 11:58

Tgt Ion: 95 Resp: 213779
Ion Ratio Lower Upper
95 100
174 75.0 0.0 143.8
176 70.2 0.0 135.8

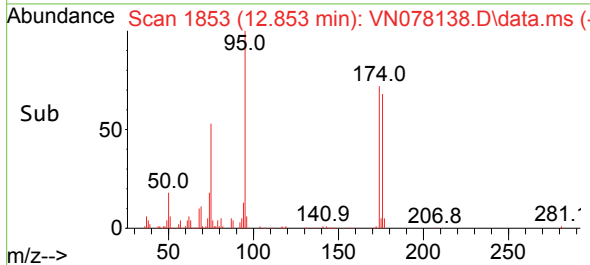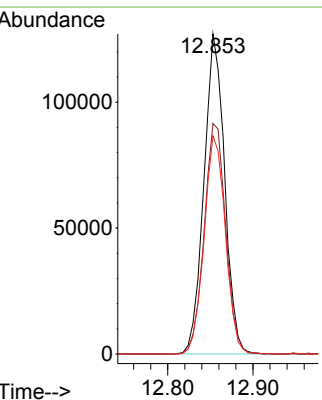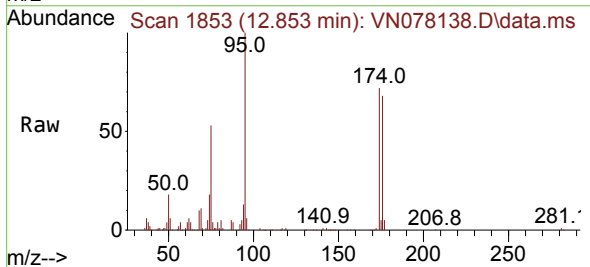



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.871 min Scan# 1

Delta R.T. 0.000 min


Lab File: VN078138.D

Acq: 09 Jun 2023 11:58

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion:117 Resp: 542041

Ion Ratio Lower Upper

117 100

82 54.4 44.0 66.0

119 32.0 25.6 38.4

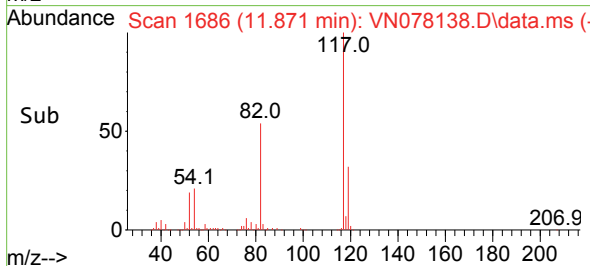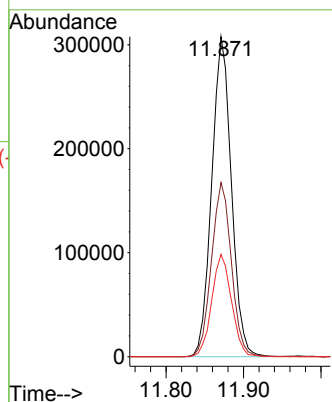

#71

Bromoform

Concen: 0.643 ug/l

RT: 12.859 min Scan# 1854

Delta R.T. 0.271 min

Lab File: VN078138.D

Acq: 09 Jun 2023 11:58




Tgt Ion:173 Resp: 1772


Ion Ratio Lower Upper

173 100

175 603.7 24.3 73.0#

254 0.0 0.0 0.0

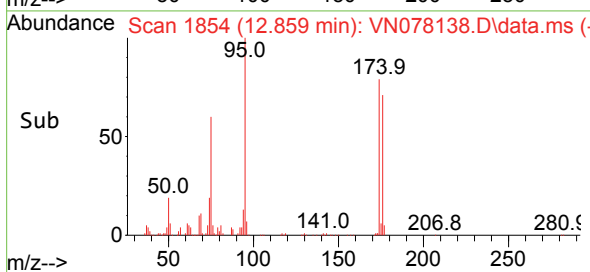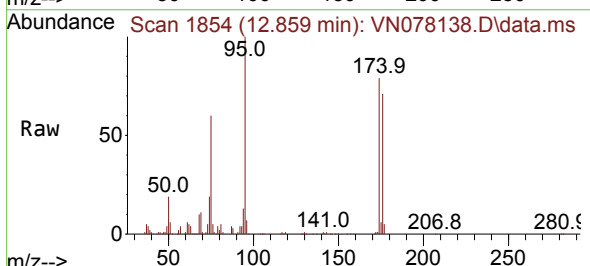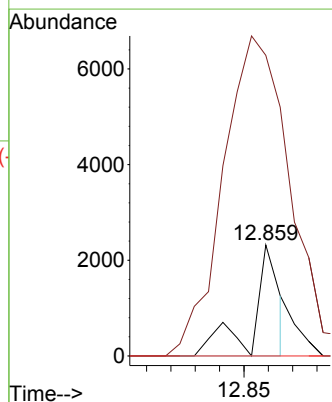



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 20

Delta R.T. -0.006 min


Lab File: VN078138.D

Acq: 09 Jun 2023 11:58

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion:152 Resp: 136032

Ion Ratio Lower Upper

152 100

115 61.3 32.3 96.8

150 161.4 0.0 355.8

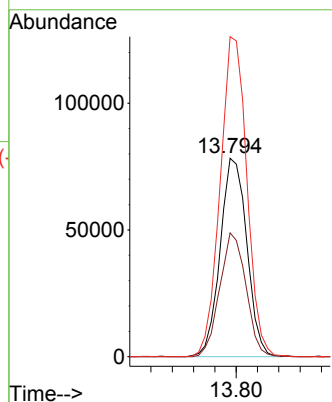

#75

1,1,2,2-Tetrachloroethane

Concen: Below Cal

RT: 12.935 min Scan# 1867

Delta R.T. -0.006 min

Lab File: VN078138.D

Acq: 09 Jun 2023 11:58




Tgt Ion: 83 Resp: 754


Ion Ratio Lower Upper

83 100

131 0.0 5.0 15.0#

85 70.7 31.9 95.7


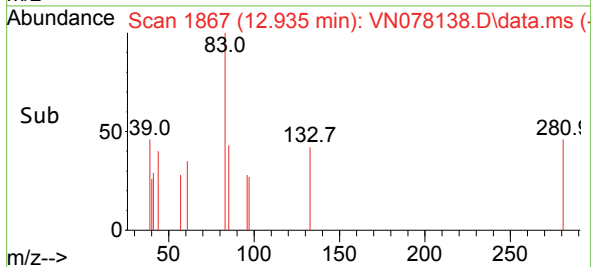
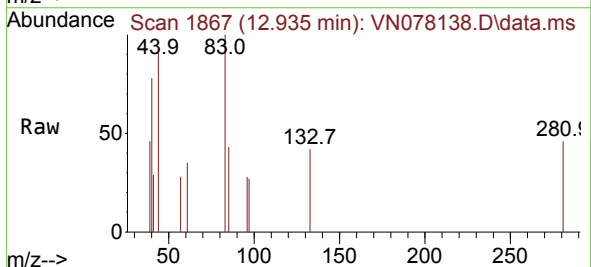
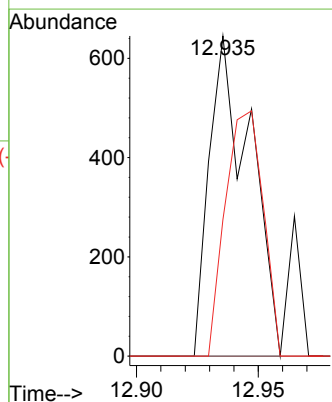


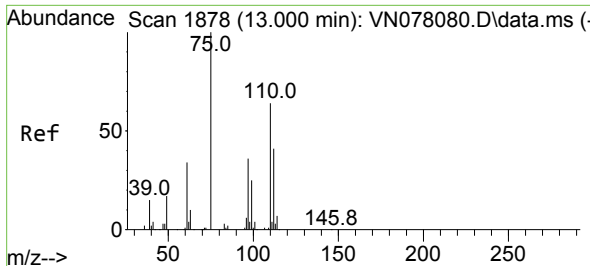

#76
1,2,3-Trichloropropane
Concen: 36.920 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.147 min
Lab File: VN078138.D
Acq: 09 Jun 2023 11:58




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 118728
Ion Ratio Lower Upper
75 100
77 1.1 84.5 253.5#

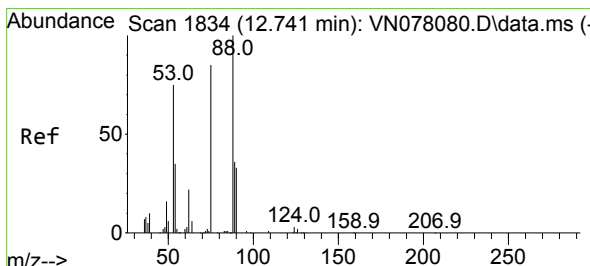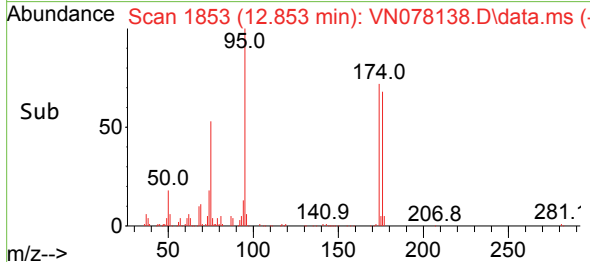

#81
trans-1,4-Dichloro-2-butene
Concen: 113.429 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.112 min
Lab File: VN078138.D
Acq: 09 Jun 2023 11:58

Tgt Ion: 75 Resp: 118728
Ion Ratio Lower Upper
75 100
53 0.1 67.4 101.2#
89 0.1 38.8 58.2#


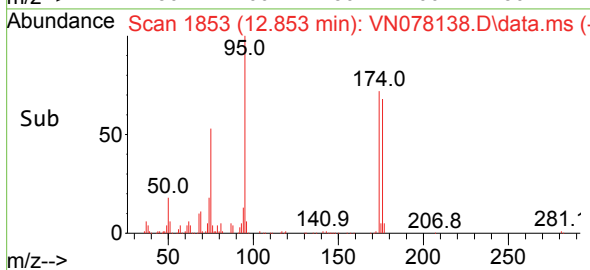

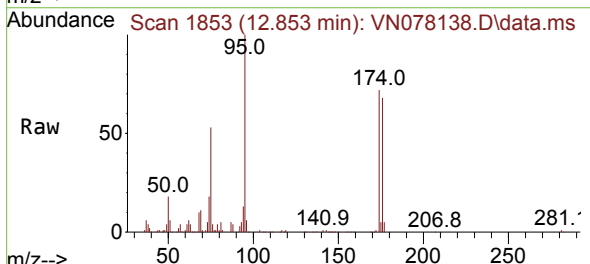




#82
4-Chlorotoluene
Concen: 0.259 ug/l
RT: 13.230 min Scan# 1917
Delta R.T. 0.000 min
Lab File: VN078138.D
Acq: 09 Jun 2023 11:58




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 2184
Ion Ratio Lower Upper
91 100
126 27.7 16.7 50.0

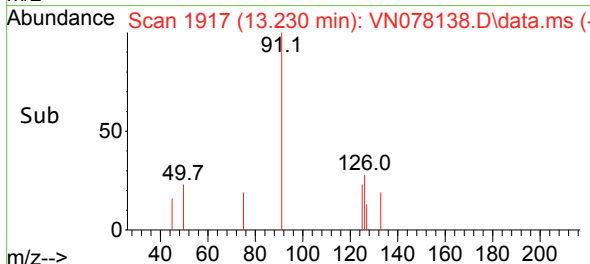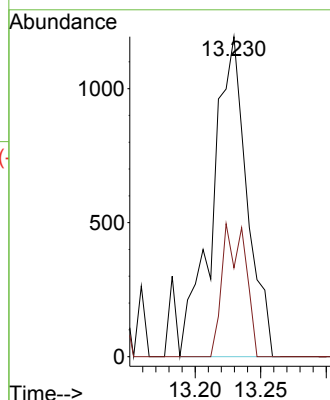

#86
p-Isopropyltoluene
Concen: 0.220 ug/l
RT: 13.741 min Scan# 2004
Delta R.T. 0.006 min
Lab File: VN078138.D
Acq: 09 Jun 2023 11:58

Tgt Ion: 119 Resp: 2117
Ion Ratio Lower Upper
119 100
134 25.9 12.6 37.8
91 25.9 12.4 37.2


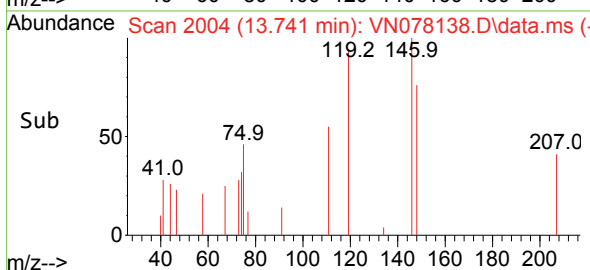
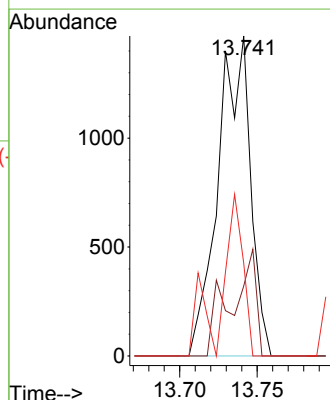
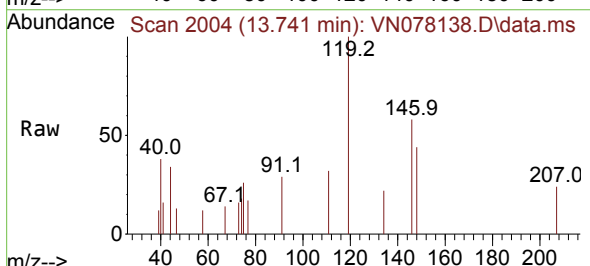


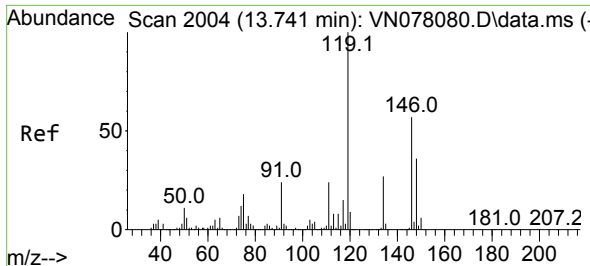

#87
1,3-Dichlorobenzene
Concen: 0.279 ug/l
RT: 13.730 min Scan# 2002
Delta R.T. -0.011 min
Lab File: VN078138.D
Acq: 09 Jun 2023 11:58




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:146 Resp: 1408
Ion Ratio Lower Upper
146 100
111 49.5 22.1 66.3
148 64.6 32.0 96.0

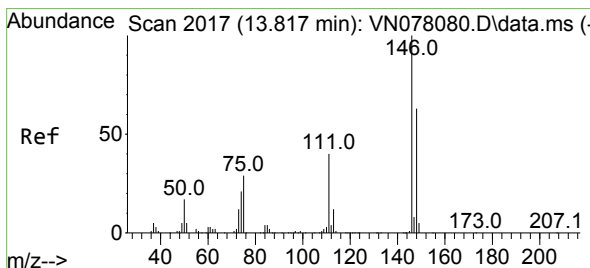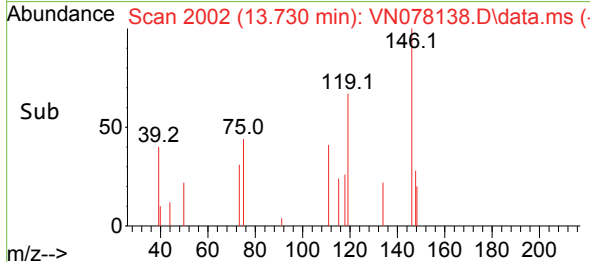

#88
1,4-Dichlorobenzene
Concen: 0.289 ug/l
RT: 13.730 min Scan# 2002
Delta R.T. -0.088 min
Lab File: VN078138.D
Acq: 09 Jun 2023 11:58

Tgt Ion:146 Resp: 1408
Ion Ratio Lower Upper
146 100
111 49.5 20.6 61.8
148 64.6 31.6 94.8

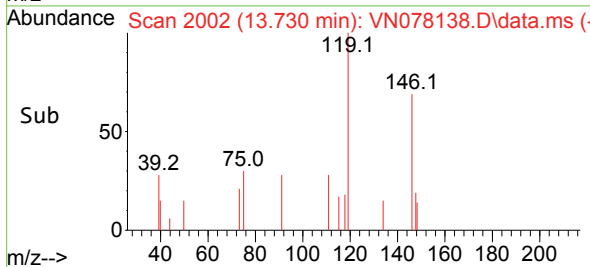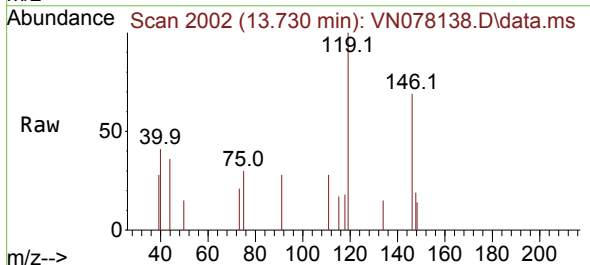



#89

n-Butylbenzene

Concen: 0.385 ug/l

RT: 14.065 min Scan# 2059

Delta R.T. 0.000 min


Lab File: VN078138.D

Acq: 09 Jun 2023 11:58




Instrument :

MSVOA_N

ClientSampleId :



Tgt Ion: 91	Resp: 2923
Ion Ratio	Lower Upper
91	100
92	46.4 26.4 79.0
134	17.1 12.6 37.6

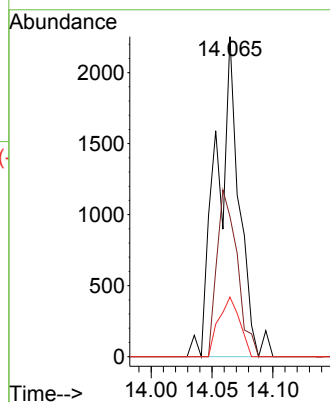

#91

1,2-Dichlorobenzene

Concen: 0.245 ug/l




RT: 14.118 min Scan# 2068


Delta R.T. 0.006 min

Lab File: VN078138.D

Acq: 09 Jun 2023 11:58

Tgt Ion: 146	Resp: 1211
Ion Ratio	Lower Upper
146	100
111	24.0 22.0 66.0
148	107.0 31.8 95.3



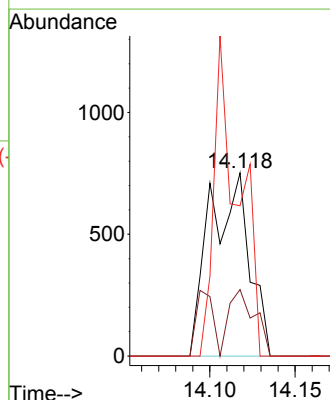
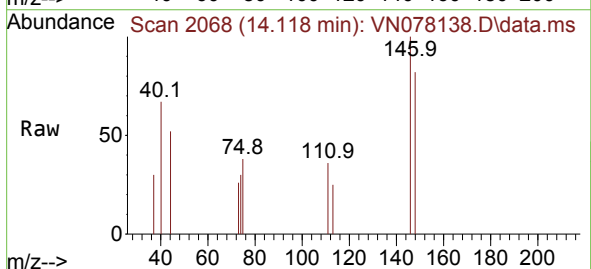




#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.565 ug/l
 RT: 14.729 min Scan# 2171
 Delta R.T. 0.006 min
 Lab File: VN078138.D
 Acq: 09 Jun 2023 11:58




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 75 Resp: 360
 Ion Ratio Lower Upper
 75 100
 155 0.0 39.1 117.2#
 157 46.1 50.3 150.9#



#93
 1,2,4-Trichlorobenzene
 Concen: 0.850 ug/l
 RT: 15.394 min Scan# 2285
 Delta R.T. -0.006 min
 Lab File: VN078138.D
 Acq: 09 Jun 2023 11:58


Tgt Ion: 180 Resp: 1495
 Ion Ratio Lower Upper
 180 100
 182 97.3 46.1 138.2
 145 21.7 16.6 49.8








#94
Hexachlorobutadiene
Concen: Below Cal
RT: 15.518 min Scan# 21
Delta R.T. 0.012 min
Lab File: VN078138.D
Acq: 09 Jun 2023 11:58


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:225 Resp: 1175
Ion Ratio Lower Upper
225 100
223 57.5 31.3 93.8
227 43.6 31.9 95.9

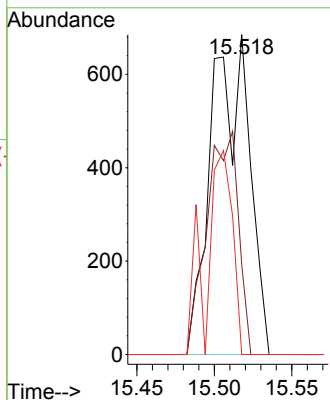


#95
Naphthalene
Concen: 0.871 ug/l
RT: 15.647 min Scan# 2328
Delta R.T. 0.000 min
Lab File: VN078138.D
Acq: 09 Jun 2023 11:58




Tgt Ion:128 Resp: 5151
Ion Ratio Lower Upper
128 100
127 11.2 10.0 15.0
129 9.6 8.7 13.1

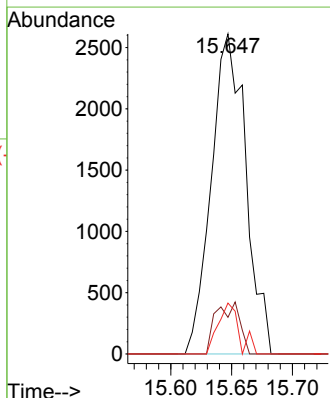



#96
 1,2,3-Trichlorobenzene
 Concen: 0.940 ug/l
 RT: 15.847 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VN078138.D
 Acq: 09 Jun 2023 11:58

Instrument :
 MSVOA_N
 ClientSampleId :



Tgt Ion:	180	Resp:	1850
Ion	Ratio	Lower	Upper
180	100		
182	76.5	46.2	138.6
145	32.4	17.5	52.6

