
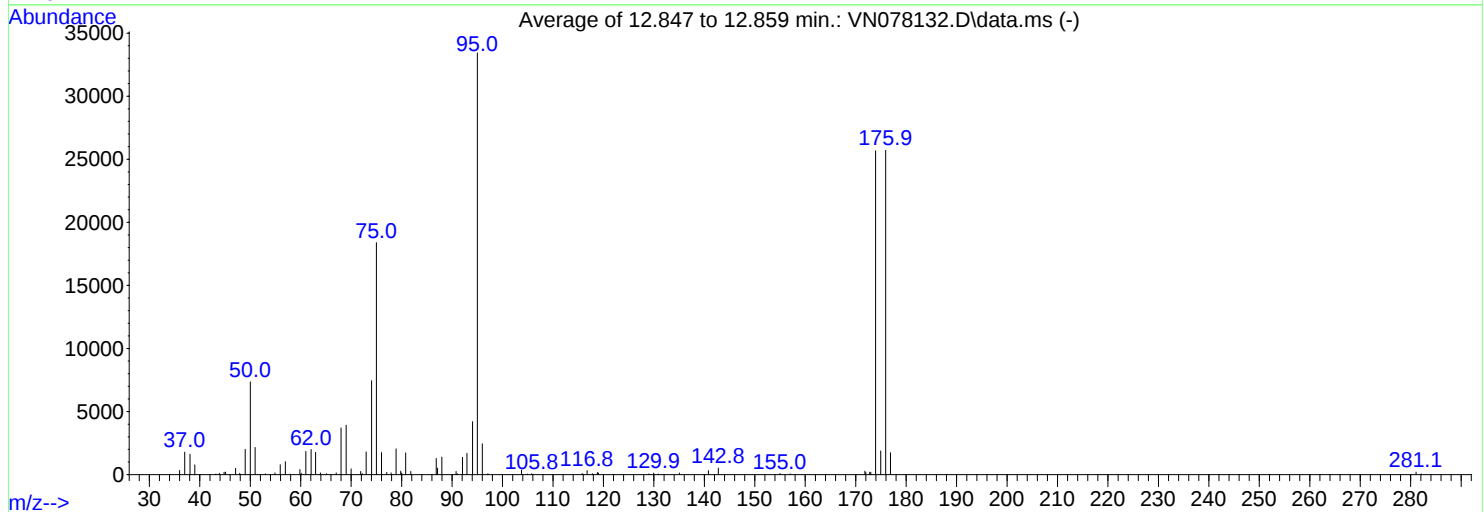


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060923\
 Data File : VN078132.D
 Acq On : 09 Jun 2023 08:08
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060623W.M
 Title : SW846 8260
 Last Update : Wed Jun 07 05:05:00 2023

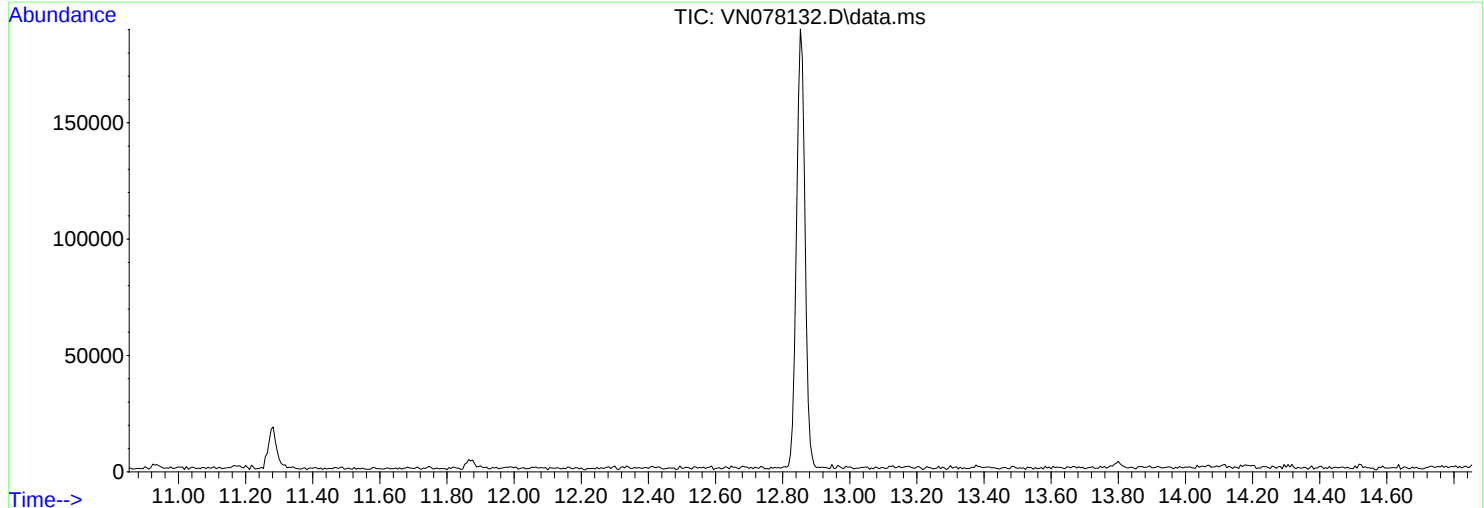

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	7353	PASS
75	95	30	60	55.0	18392	PASS
95	95	100	100	100.0	33437	PASS
96	95	5	9	7.3	2442	PASS
173	174	0.00	2	0.7	190	PASS
174	95	50	100	76.8	25667	PASS
175	174	5	9	7.3	1882	PASS
176	174	95	101	100.2	25715	PASS
177	176	5	9	6.7	1732	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	335	50.00	7353	62.95	1767	75.00	1839
37.00	1793	50.95	2152	63.90	142	76.00	175
38.05	1621	53.00	69	65.10	80	77.05	18
39.00	771	54.90	137	67.05	142	77.90	13
43.20	54	55.95	793	68.00	3709	78.90	2042
43.85	119	56.95	1027	69.00	3918	79.80	279
44.80	196	57.90	52	70.00	462	80.00	127
45.10	200	59.85	400	71.90	250	80.80	1728
47.10	493	60.10	110	72.20	80	81.80	249
47.90	112	61.00	1836	72.95	1796	86.85	1283
49.00	2001	62.05	1993	74.05	7449	87.10	525

Average of 12.847 to 12.859 min.: VN078132.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.95	1390	105.80	78	140.80	315	176.90	1732
90.80	253	115.70	53	142.75	527	281.05	203
91.00	81	115.90	83	155.00	95	282.10	52
92.05	1374	116.75	317	157.00	61		
92.95	1687	117.80	72	171.80	285		
94.05	4198	118.80	182	172.00	183		
95.00	33437	119.00	128	172.75	190		
96.00	2442	129.00	62	173.00	189		
97.10	74	129.95	129	173.95	25667		
103.75	352	130.90	53	174.95	1882		
104.90	56	135.05	126	175.95	25715		

Instrument :

MSVOA_N

ClientSampleId :

BFB