

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060925\
 Data File : VN086889.D
 Acq On : 09 Jun 2025 09:12
 Operator : JC\MD
 Sample : VN0609MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0609MBL01

Quant Time: Jun 10 03:27:54 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060625W.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 07 02:12:50 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	249041	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	437413	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	375931	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	185529	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	144348	43.291	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	86.580%
35) Dibromofluoromethane	8.177	113	125507	48.417	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.840%
50) Toluene-d8	10.565	98	521169	50.787	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	101.580%
62) 4-Bromofluorobenzene	12.847	95	183485	48.126	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	96.260%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN060925\
Data File : VN086889.D
Acq On : 09 Jun 2025 09:12
Operator : JC\MD
Sample : VN0609MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0609MBL01

Quant Time: Jun 10 03:27:54 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060625W.M
Quant Title : SW846 8260
QLast Update : Sat Jun 07 02:12:50 2025
Response via : Initial Calibration




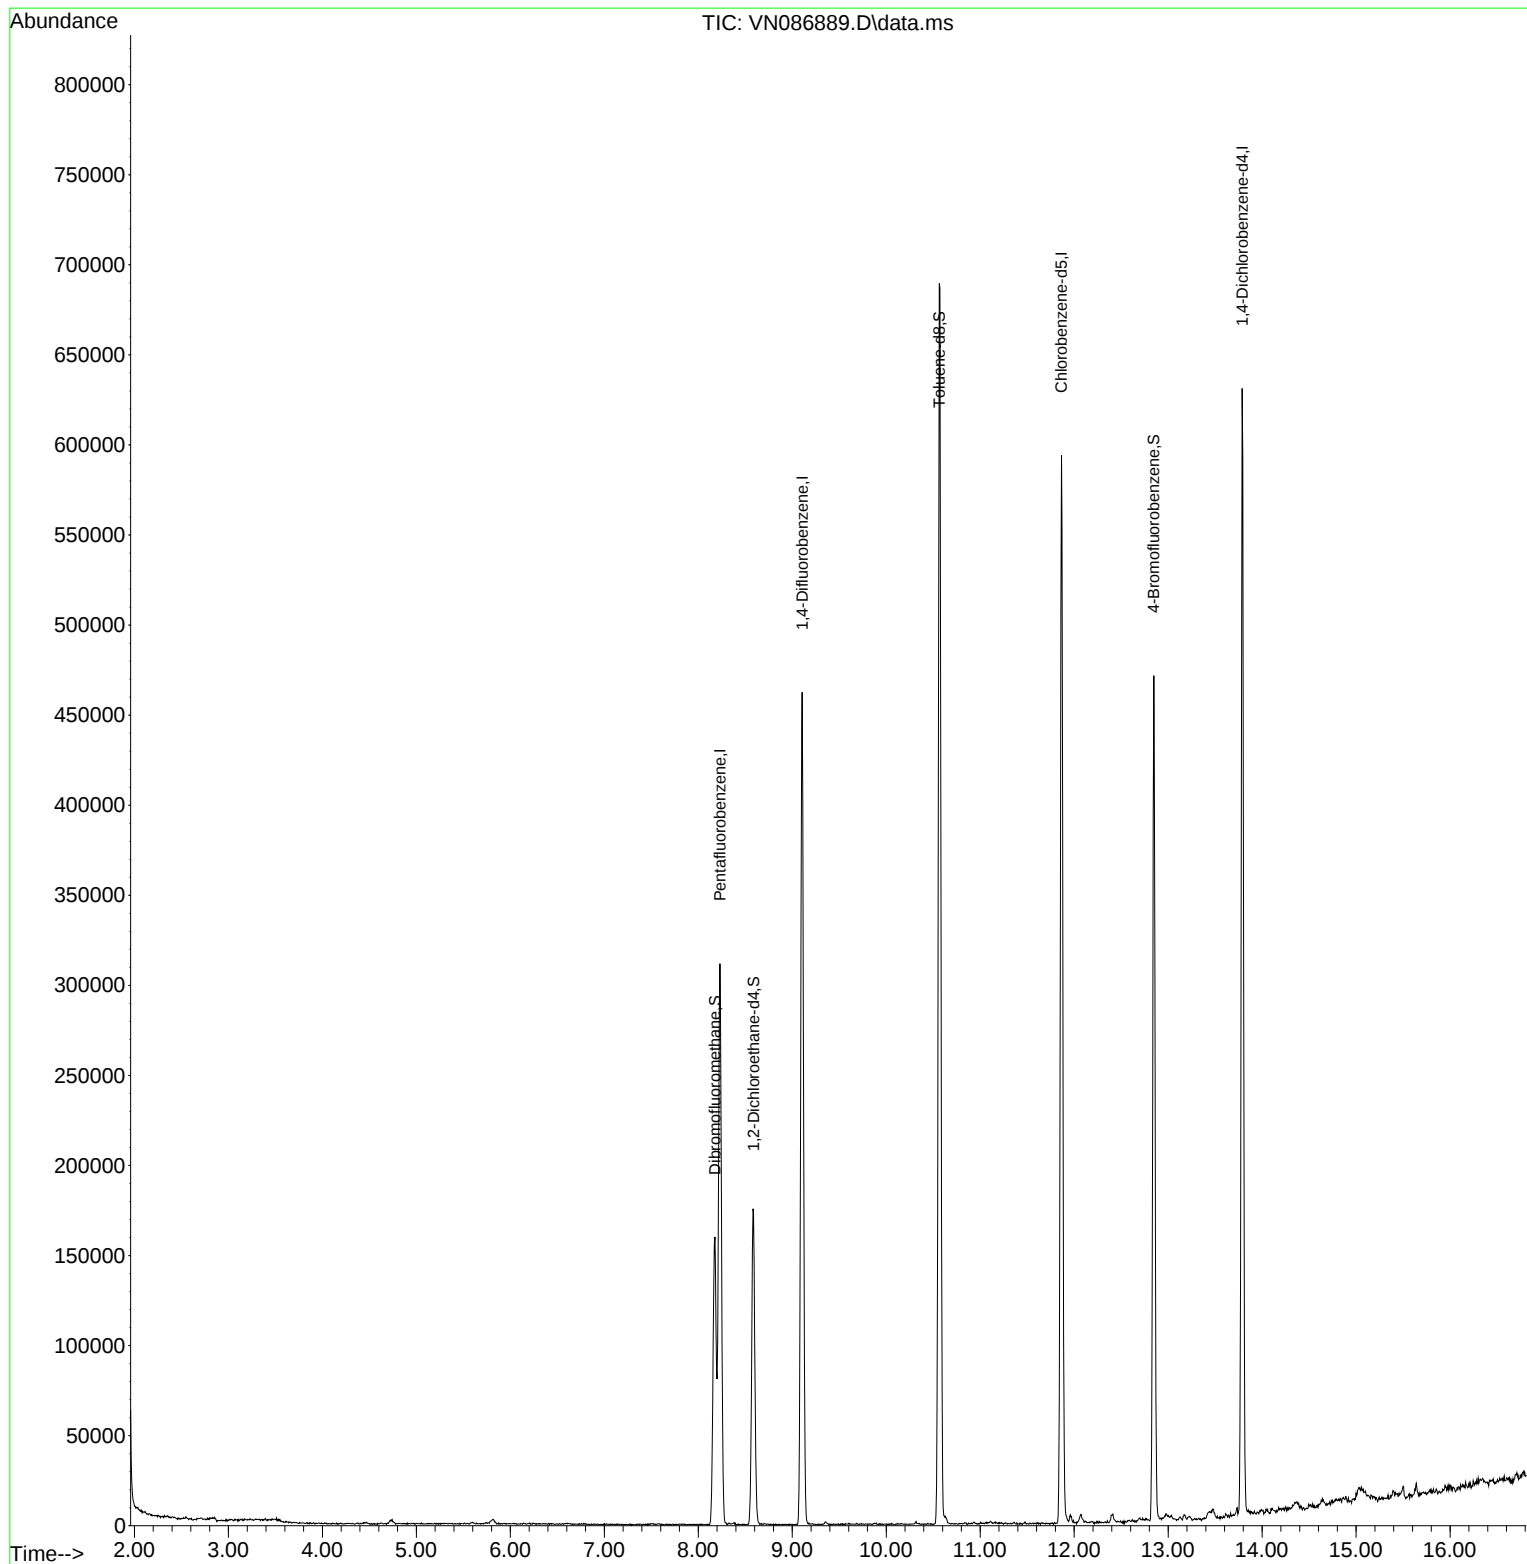




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1068
Delta R.T. -0.006 min
Lab File: VN086889.D
Acq: 09 Jun 2025 09:12




Instrument :
MSVOA_N
ClientSampleId :
VN0609MBL01


Tgt Ion:168 Resp: 249041
Ion Ratio Lower Upper
168 100
99 59.9 49.1 73.7

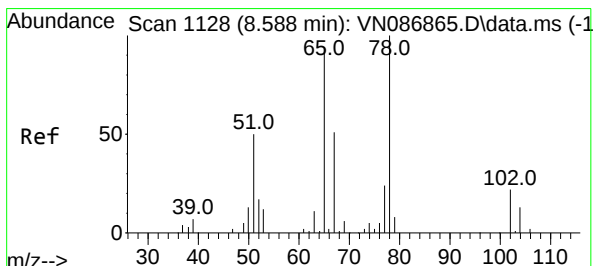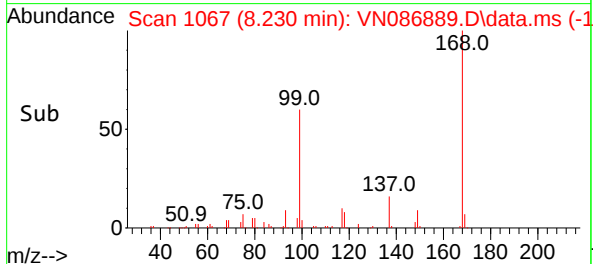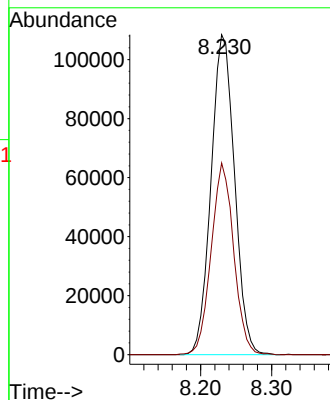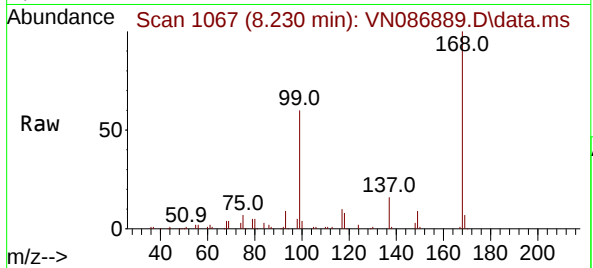

#33
1,2-Dichloroethane-d4
Concen: 43.291 ug/l
RT: 8.588 min Scan# 1128
Delta R.T. -0.000 min
Lab File: VN086889.D
Acq: 09 Jun 2025 09:12

Tgt Ion: 65 Resp: 144348
Ion Ratio Lower Upper
65 100
67 54.7 0.0 105.6


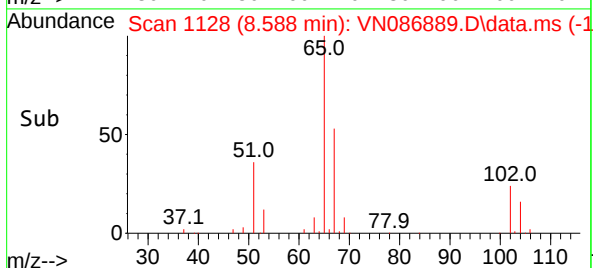
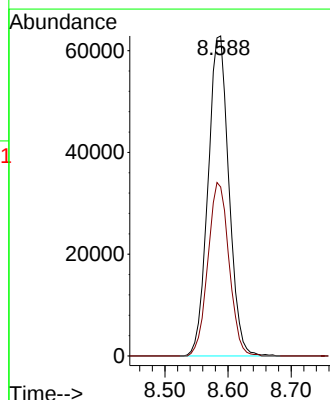
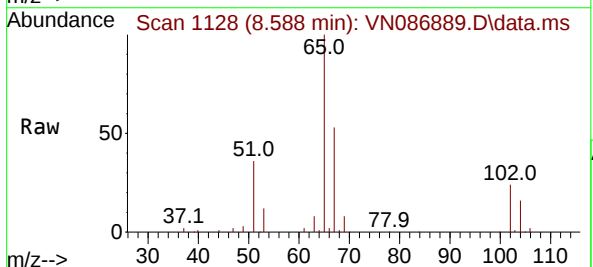


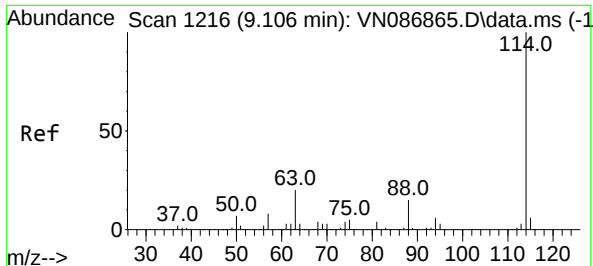

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN086889.D
Acq: 09 Jun 2025 09:12




Instrument :
MSVOA_N
ClientSampleId :
VN0609MBL01


Tgt Ion:114 Resp: 437413
Ion Ratio Lower Upper
114 100
63 19.7 0.0 39.6
88 16.6 0.0 30.2

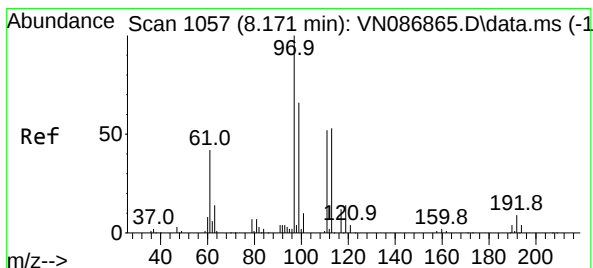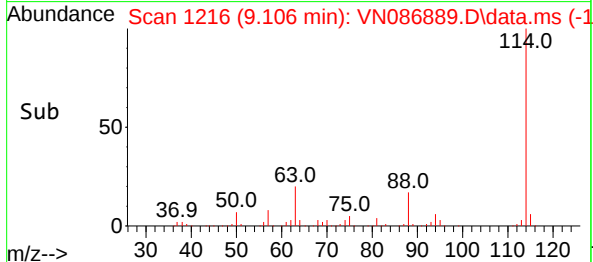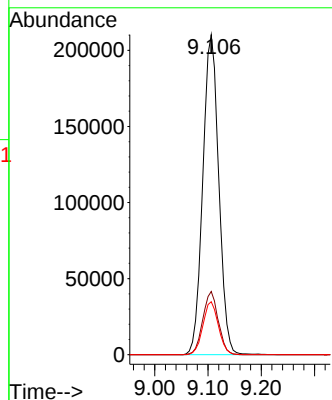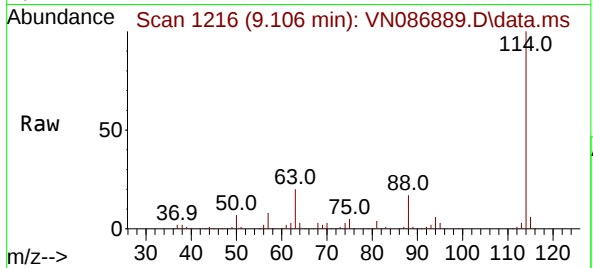

#35
Dibromofluoromethane
Concen: 48.417 ug/l
RT: 8.177 min Scan# 1058
Delta R.T. 0.006 min
Lab File: VN086889.D
Acq: 09 Jun 2025 09:12

Tgt Ion:113 Resp: 125507
Ion Ratio Lower Upper
113 100
111 101.3 84.2 126.2
192 18.2 14.2 21.4


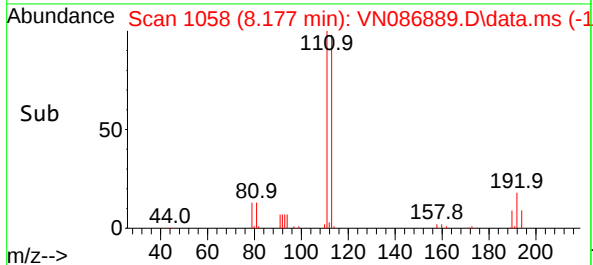
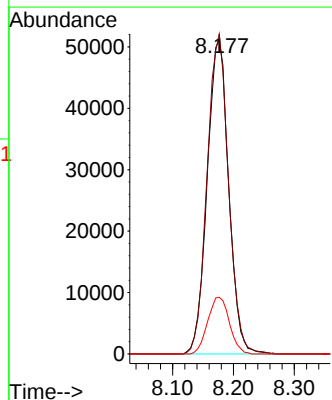
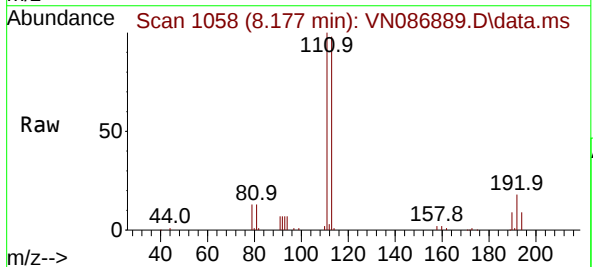


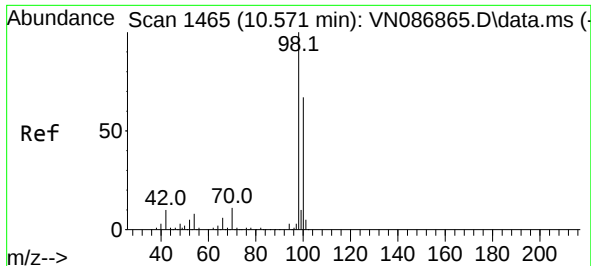

#50
Toluene-d8
Concen: 50.787 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.006 min
Lab File: VN086889.D
Acq: 09 Jun 2025 09:12




Instrument :
MSVOA_N
ClientSampleId :
VN0609MBL01


Tgt Ion: 98 Resp: 521169
Ion Ratio Lower Upper
98 100
100 66.8 53.4 80.0

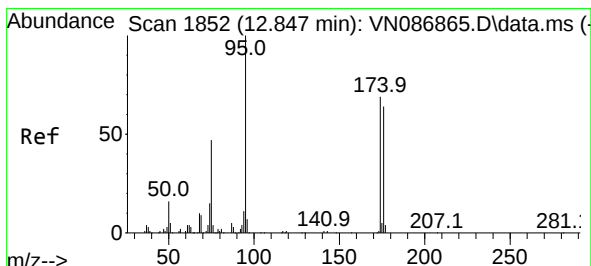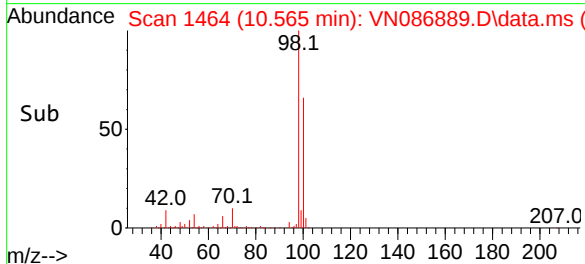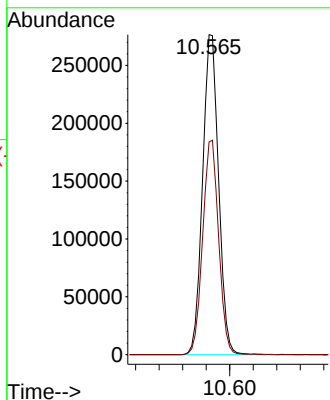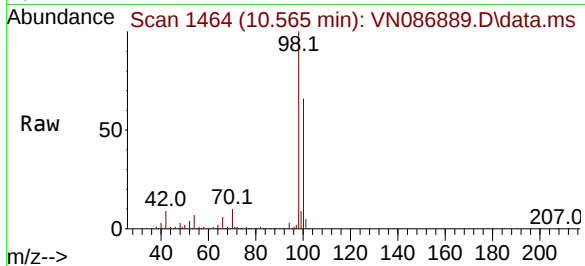

#62
4-Bromofluorobenzene
Concen: 48.126 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN086889.D
Acq: 09 Jun 2025 09:12

Tgt Ion: 95 Resp: 183485
Ion Ratio Lower Upper
95 100
174 73.5 0.0 141.8
176 70.6 0.0 132.6


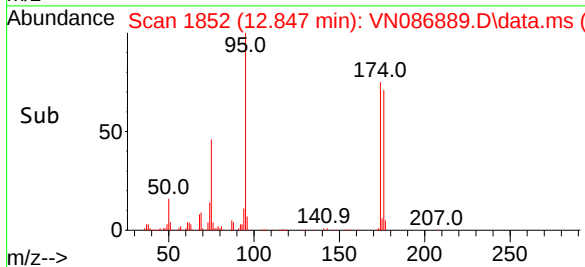
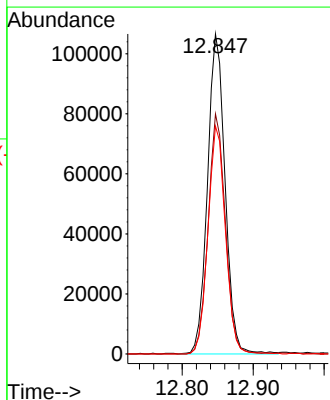
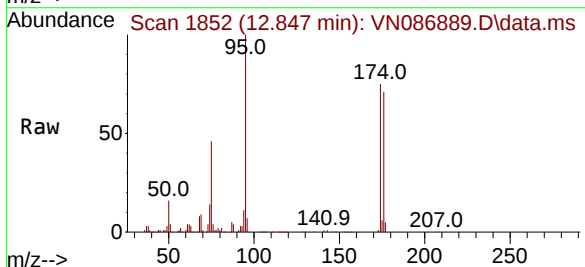


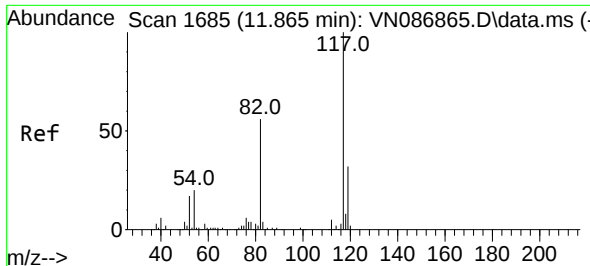

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN086889.D
Acq: 09 Jun 2025 09:12

Instrument :
MSVOA_N
ClientSampleId :
VN0609MBL01

Tgt Ion:117 Resp: 375931
Ion Ratio Lower Upper
117 100
82 54.7 44.6 67.0
119 30.7 25.5 38.3

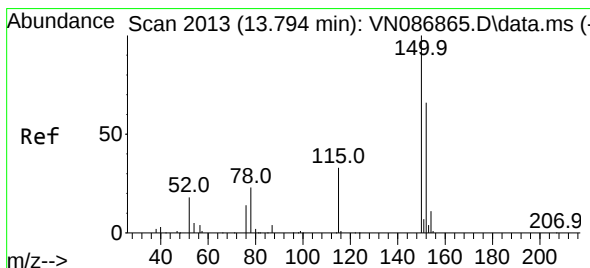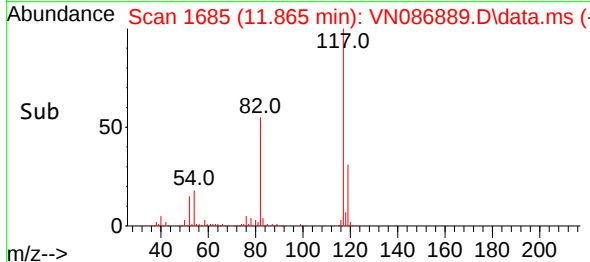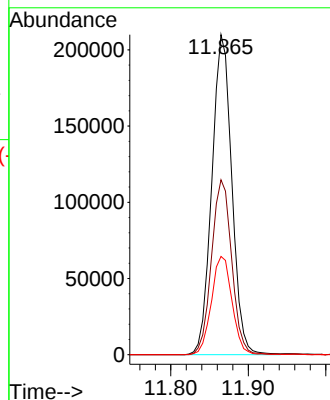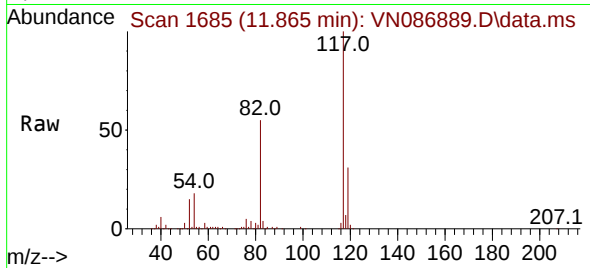

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 2012
Delta R.T. -0.006 min
Lab File: VN086889.D
Acq: 09 Jun 2025 09:12

Tgt Ion:152 Resp: 185529
Ion Ratio Lower Upper
152 100
115 58.9 30.1 90.5
150 157.5 0.0 345.0

