
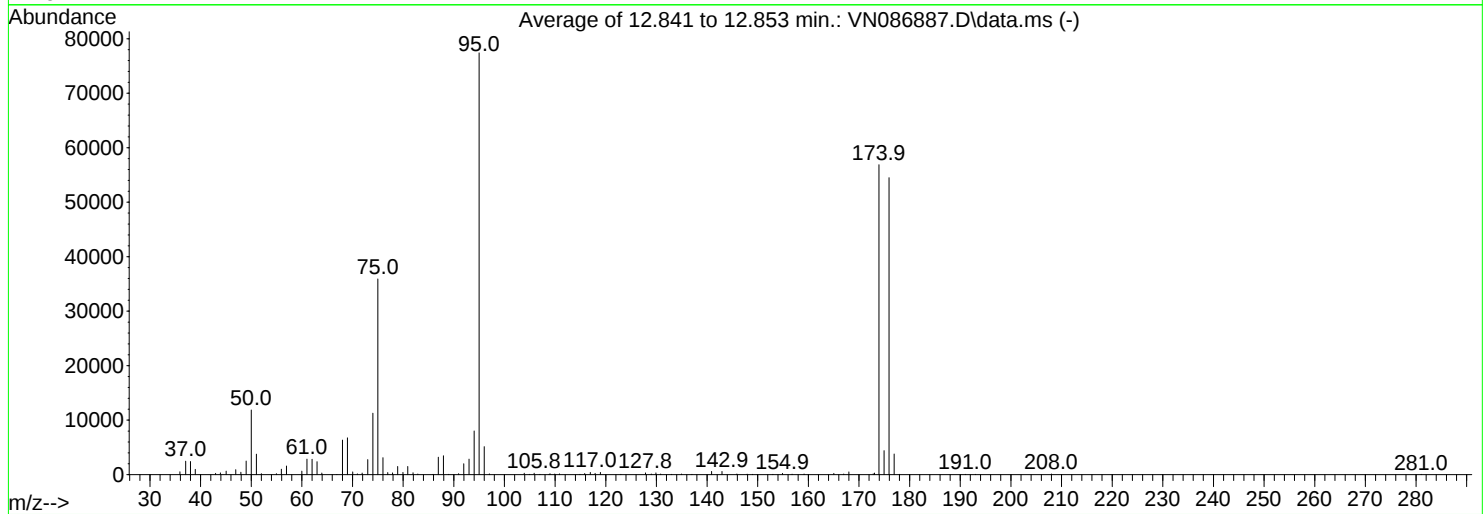


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN060925\  
Data File : VN086887.D  
Acq On : 09 Jun 2025 08:04  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N060625W.M  
Title : SW846 8260  
Last Update : Sat Jun 07 02:12:50 2025

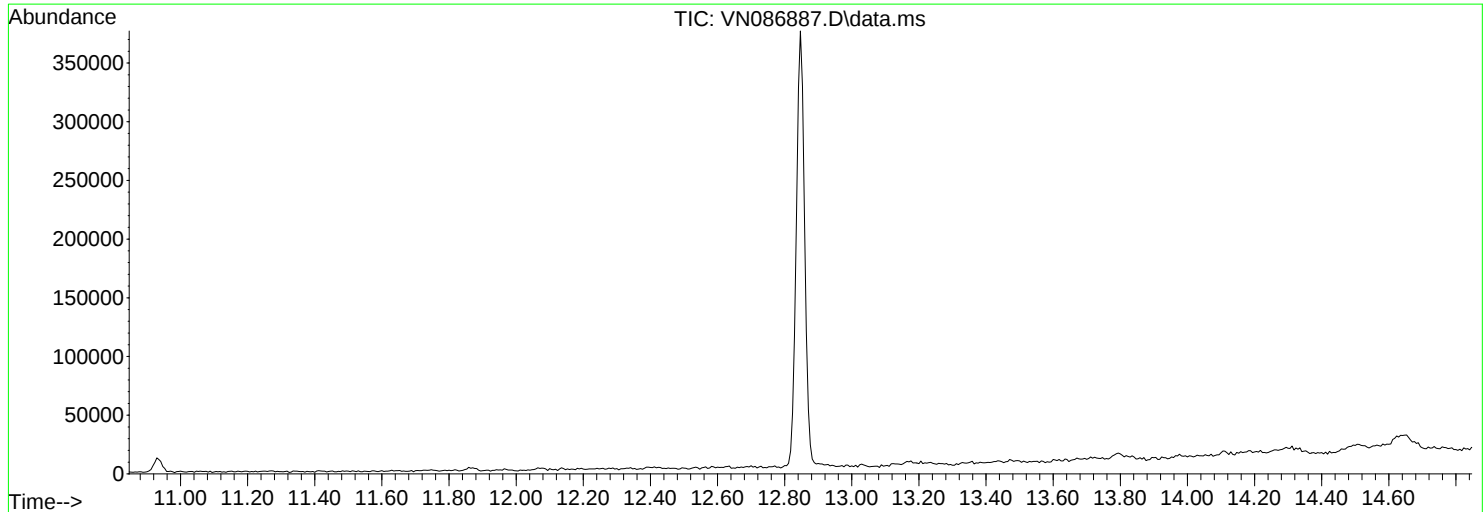

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1840

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 15.3  | 11871 | PASS      |
| 75     | 95      | 30     | 60     | 46.4  | 35931 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 77415 | PASS      |
| 96     | 95      | 5      | 9      | 6.6   | 5148  | PASS      |
| 173    | 174     | 0.00   | 2      | 0.5   | 309   | PASS      |
| 174    | 95      | 50     | 100    | 73.5  | 56888 | PASS      |
| 175    | 174     | 5      | 9      | 7.8   | 4421  | PASS      |
| 176    | 174     | 95     | 101    | 95.8  | 54509 | PASS      |
| 177    | 176     | 5      | 9      | 6.9   | 3785  | PASS      |

Average of 12.841 to 12.853 min.: VN086887.D\data.ms

BFB

Modified:subtracted

| m/z   | abund. | m/z   | abund. | m/z   | abund. | m/z   | abund. |
|-------|--------|-------|--------|-------|--------|-------|--------|
| 35.90 | 535    | 51.00 | 3760   | 68.00 | 6351   | 78.90 | 1481   |
| 37.05 | 2466   | 52.00 | 191    | 69.00 | 6745   | 79.95 | 411    |
| 38.00 | 2416   | 54.95 | 172    | 70.05 | 506    | 80.90 | 149    |
| 38.95 | 974    | 55.95 | 1011   | 70.95 | 137    | 81.95 | 36     |
| 42.95 | 245    | 56.95 | 1580   | 71.90 | 302    | 82.90 | 114    |
| 43.90 | 314    | 60.00 | 650    | 73.00 | 2758   | 85.90 | 50     |
| 45.05 | 641    | 61.00 | 2856   | 74.00 | 11273  | 86.95 | 3209   |
| 46.95 | 922    | 62.00 | 2814   | 75.00 | 35931  | 87.95 | 3465   |
| 47.95 | 453    | 63.00 | 2376   | 76.00 | 3116   | 89.00 | 56     |
| 49.00 | 2498   | 63.95 | 306    | 76.95 | 390    | 90.95 | 172    |
| 50.00 | 11871  | 66.90 | 36     | 77.90 | 336    | 91.95 | 1998   |

Average of 12.841 to 12.853 min.: VN086887.D\data.ms

BFB

Modified:subtracted

| m/z    | abund. | m/z    | abund. | m/z    | abund. | m/z    | abund. |
|--------|--------|--------|--------|--------|--------|--------|--------|
| 93.00  | 2849   | 109.95 | 104    | 130.85 | 116    | 156.80 | 82     |
| 94.00  | 8007   | 110.85 | 138    | 133.00 | 54     | 159.15 | 111    |
| 95.00  | 77415  | 114.90 | 53     | 134.95 | 129    | 165.05 | 238    |
| 96.00  | 5148   | 115.85 | 200    | 137.00 | 64     | 167.00 | 127    |
| 97.00  | 150    | 116.95 | 418    | 140.90 | 576    | 168.00 | 497    |
| 103.90 | 272    | 117.90 | 243    | 142.95 | 587    | 172.80 | 158    |
| 104.90 | 66     | 118.95 | 408    | 145.90 | 124    | 173.05 | 309    |
| 105.85 | 261    | 123.00 | 58     | 147.90 | 102    | 173.95 | 56888  |
| 107.00 | 54     | 127.85 | 331    | 149.00 | 66     | 174.95 | 4421   |
| 108.80 | 60     | 129.00 | 116    | 153.00 | 58     | 175.95 | 54509  |
| 109.00 | 188    | 129.90 | 331    | 154.90 | 229    | 176.95 | 3785   |

Average of 12.841 to 12.853 min.: VN086887.D\data.ms

BFB

Modified:subtracted

| m/z    | abund. | m/z | abund. | m/z | abund. | m/z | abund. |
|--------|--------|-----|--------|-----|--------|-----|--------|
| 178.00 | 62     |     |        |     |        |     |        |
| 191.00 | 71     |     |        |     |        |     |        |
| 193.00 | 59     |     |        |     |        |     |        |
| 208.00 | 120    |     |        |     |        |     |        |
| 281.00 | 51     |     |        |     |        |     |        |

Instrument :

MSVOA\_N

ClientSampleId :

BFB