


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN061019\
 Data File : VN056182.D
 Acq On : 10 Jun 2019 20:49
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N060419W.M
 Title : SW846 8260
 Last Update : Tue Jun 04 11:02:09 2019

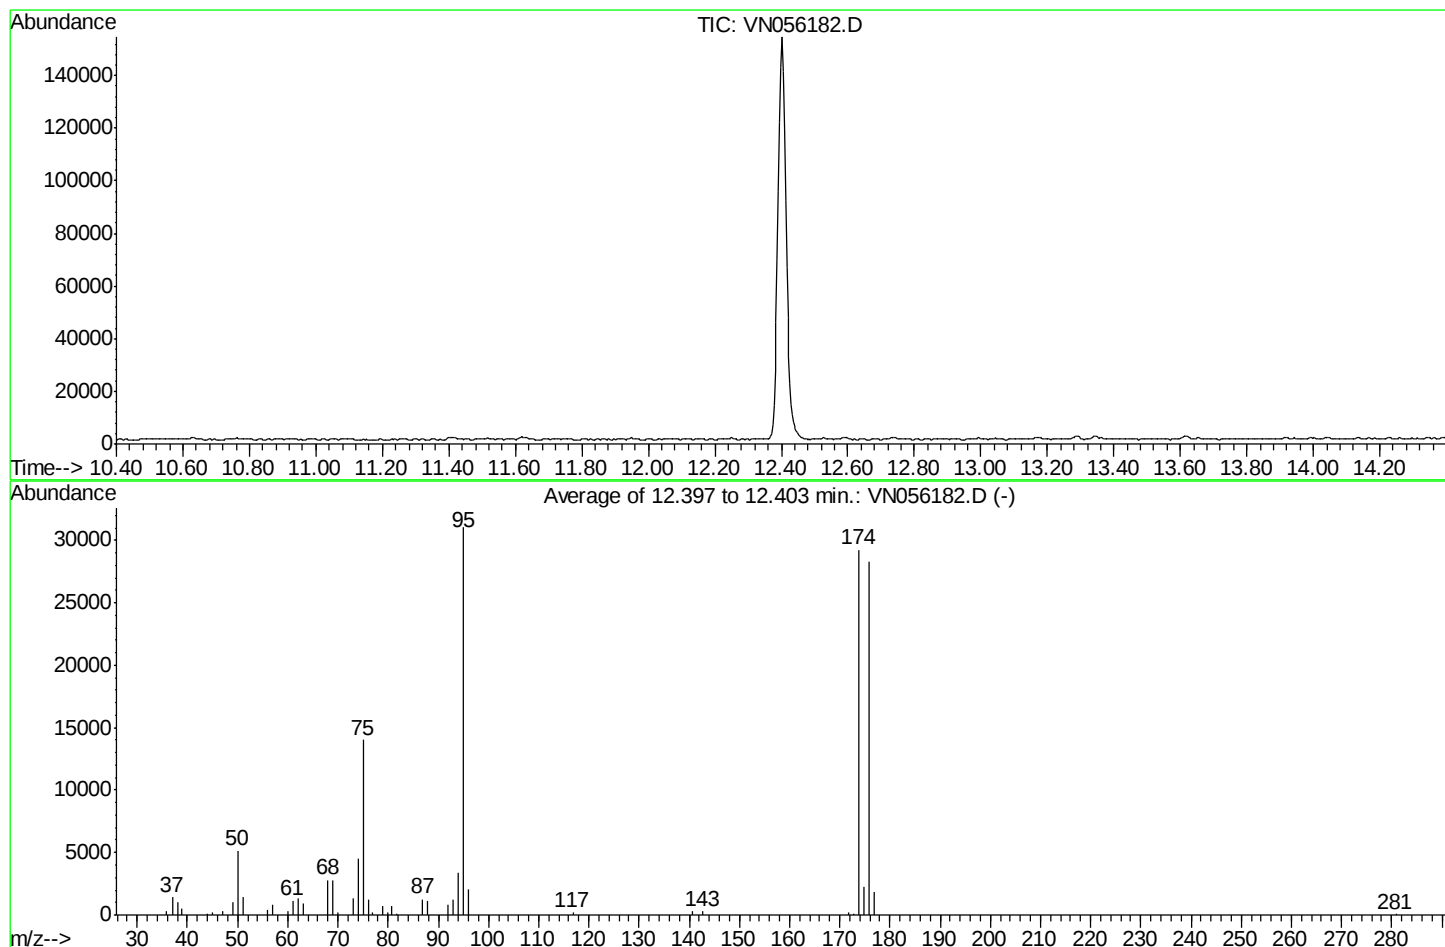

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	5156	PASS
75	95	30	60	45.1	14006	PASS
95	95	100	100	100.0	31040	PASS
96	95	5	9	6.6	2049	PASS
173	174	0.00	2	0.4	103	PASS
174	95	50	100	94.2	29226	PASS
175	174	5	9	7.8	2289	PASS
176	174	95	101	96.9	28322	PASS
177	176	5	9	6.5	1850	PASS