


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN061020\
 Data File : VN061727.D
 Acq On : 10 Jun 2020 9:17
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N061020W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Wed Jun 10 12:28:45 2020

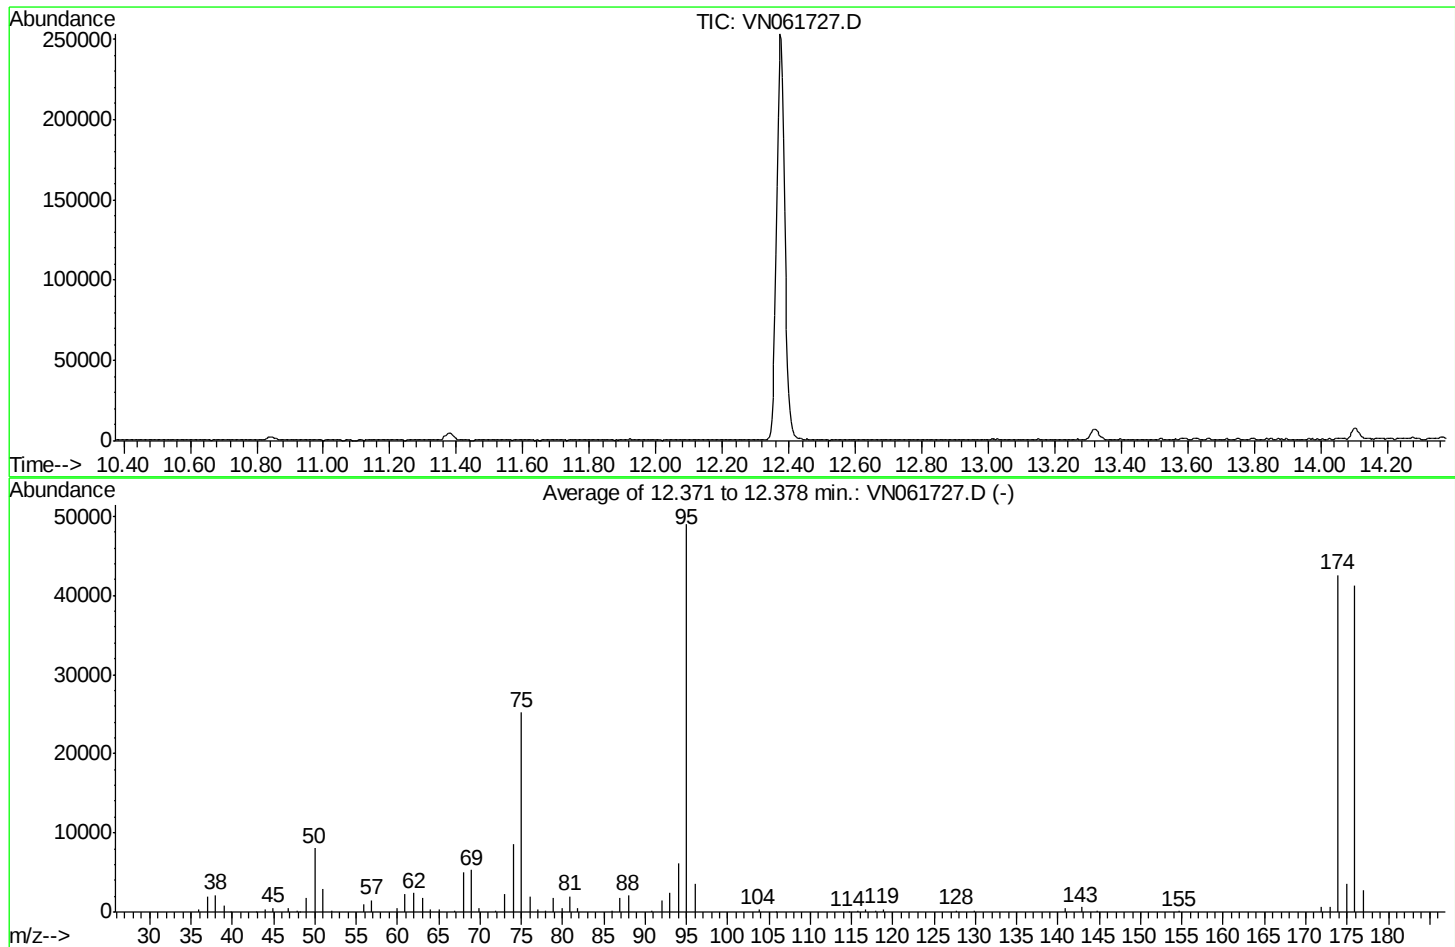

AutoFind: Scans 3296, 3297, 3298; Background Corrected with Scan 3284

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	8038	PASS
75	95	30	60	51.4	25178	PASS
95	95	100	100	100.0	48986	PASS
96	95	5	9	7.3	3563	PASS
173	174	0.00	2	1.6	668	PASS
174	95	50	100	86.9	42592	PASS
175	174	5	9	8.2	3504	PASS
176	174	95	101	96.8	41216	PASS
177	176	5	9	6.8	2811	PASS