

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061021\
 Data File : VN067267.D
 Acq On : 10 Jun 2021 13:08
 Operator : JC/MD
 Sample : VN0610MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :


Quant Time: Jun 11 05:38:34 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061021W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 11 05:27:41 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	397440	50.00	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.971	114	721907	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.749	117	633879	50.00	ug/l	# 0.00
72) 1,4-Dichlorobenzene-d4	13.677	152	245008	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.442	65	349604	46.54	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	93.08%
35) Dibromofluoromethane	8.024	113	225919	49.11	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	98.22%
50) Toluene-d8	10.443	98	922744	51.04	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	102.08%
62) 4-Bromofluorobenzene	12.733	95	356040	47.33	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	94.66%
Target Compounds						
						Qvalue
3) Chloromethane	2.306	50	1506	0.24	ug/l	97
11) Tert butyl alcohol	5.390	59	386	0.30	ug/l	# 36
13) Acrolein	4.036	56	258	0.50	ug/l	# 1
16) Acetone	4.301	43	3900	1.29	ug/l	# 69
20) Methylene Chloride	5.090	84	1906	0.35	ug/l	# 91
25) 2-Butanone	7.353	43	1449	0.31	ug/l	# 78
31) Cyclohexane	8.086	56	12595	1.36	ug/l	# 43
36) 1,1-Dichloropropene	8.083	75	42436	5.55	ug/l	# 40
38) Carbon Tetrachloride	8.088	117	49493	6.21	ug/l	# 14
49) 1,4-Dioxane	9.579	88	172	1.93	ug/l	# 6
51) 4-Methyl-2-Pentanone	10.338	43	6561	0.69	ug/l	# 73
58) 2-Chloroethyl Vinyl ether	10.051	63	169	28.15	ug/l	# 45
59) 2-Hexanone	11.092	43	13157	1.93	ug/l	71
68) m/p-Xylenes	11.950	106	2281	0.24	ug/l	97
74) N-amyl acetate	12.393	43	6719	0.59	ug/l	# 67
76) 1,2,3-Trichloropropane	12.733	75	207761	31.92	ug/l	# 100
79) 2-Chlorotoluene	13.109	91	5283	0.32	ug/l	88
81) trans-1,4-Dichloro-2-b...	12.733	75	207761	81.66	ug/l	# 15
82) 4-Chlorotoluene	13.109	91	5283	0.32	ug/l	90
84) 1,2,4-Trimethylbenzene	13.372	105	4307	0.22	ug/l	100
85) sec-Butylbenzene	13.503	105	4764	0.21	ug/l	96
86) p-Isopropyltoluene	13.618	119	5210	0.27	ug/l	# 82
87) 1,3-Dichlorobenzene	13.621	146	3298	0.39	ug/l	91
88) 1,4-Dichlorobenzene	13.621	146	3298	0.40	ug/l	89
89) n-Butylbenzene	13.946	91	9855	0.56	ug/l	95
91) 1,2-Dichlorobenzene	13.994	146	3357	0.42	ug/l	# 82
92) 1,2-Dibromo-3-Chloropr...	14.597	75	684	0.41	ug/l	# 9
93) 1,2,4-Trichlorobenzene	15.265	180	6969	1.71	ug/l	92
94) Hexachlorobutadiene	15.367	225	997	0.42	ug/l	82
95) Naphthalene	15.509	128	41321	7.43	ug/l	# 91
96) 1,2,3-Trichlorobenzene	15.702	180	8805	2.32	ug/l	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jun 11 05:38:34 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061021W.M
Quant Title : SW846 8260
QLast Update : Fri Jun 11 05:27:41 2021
Response via : Initial Calibration




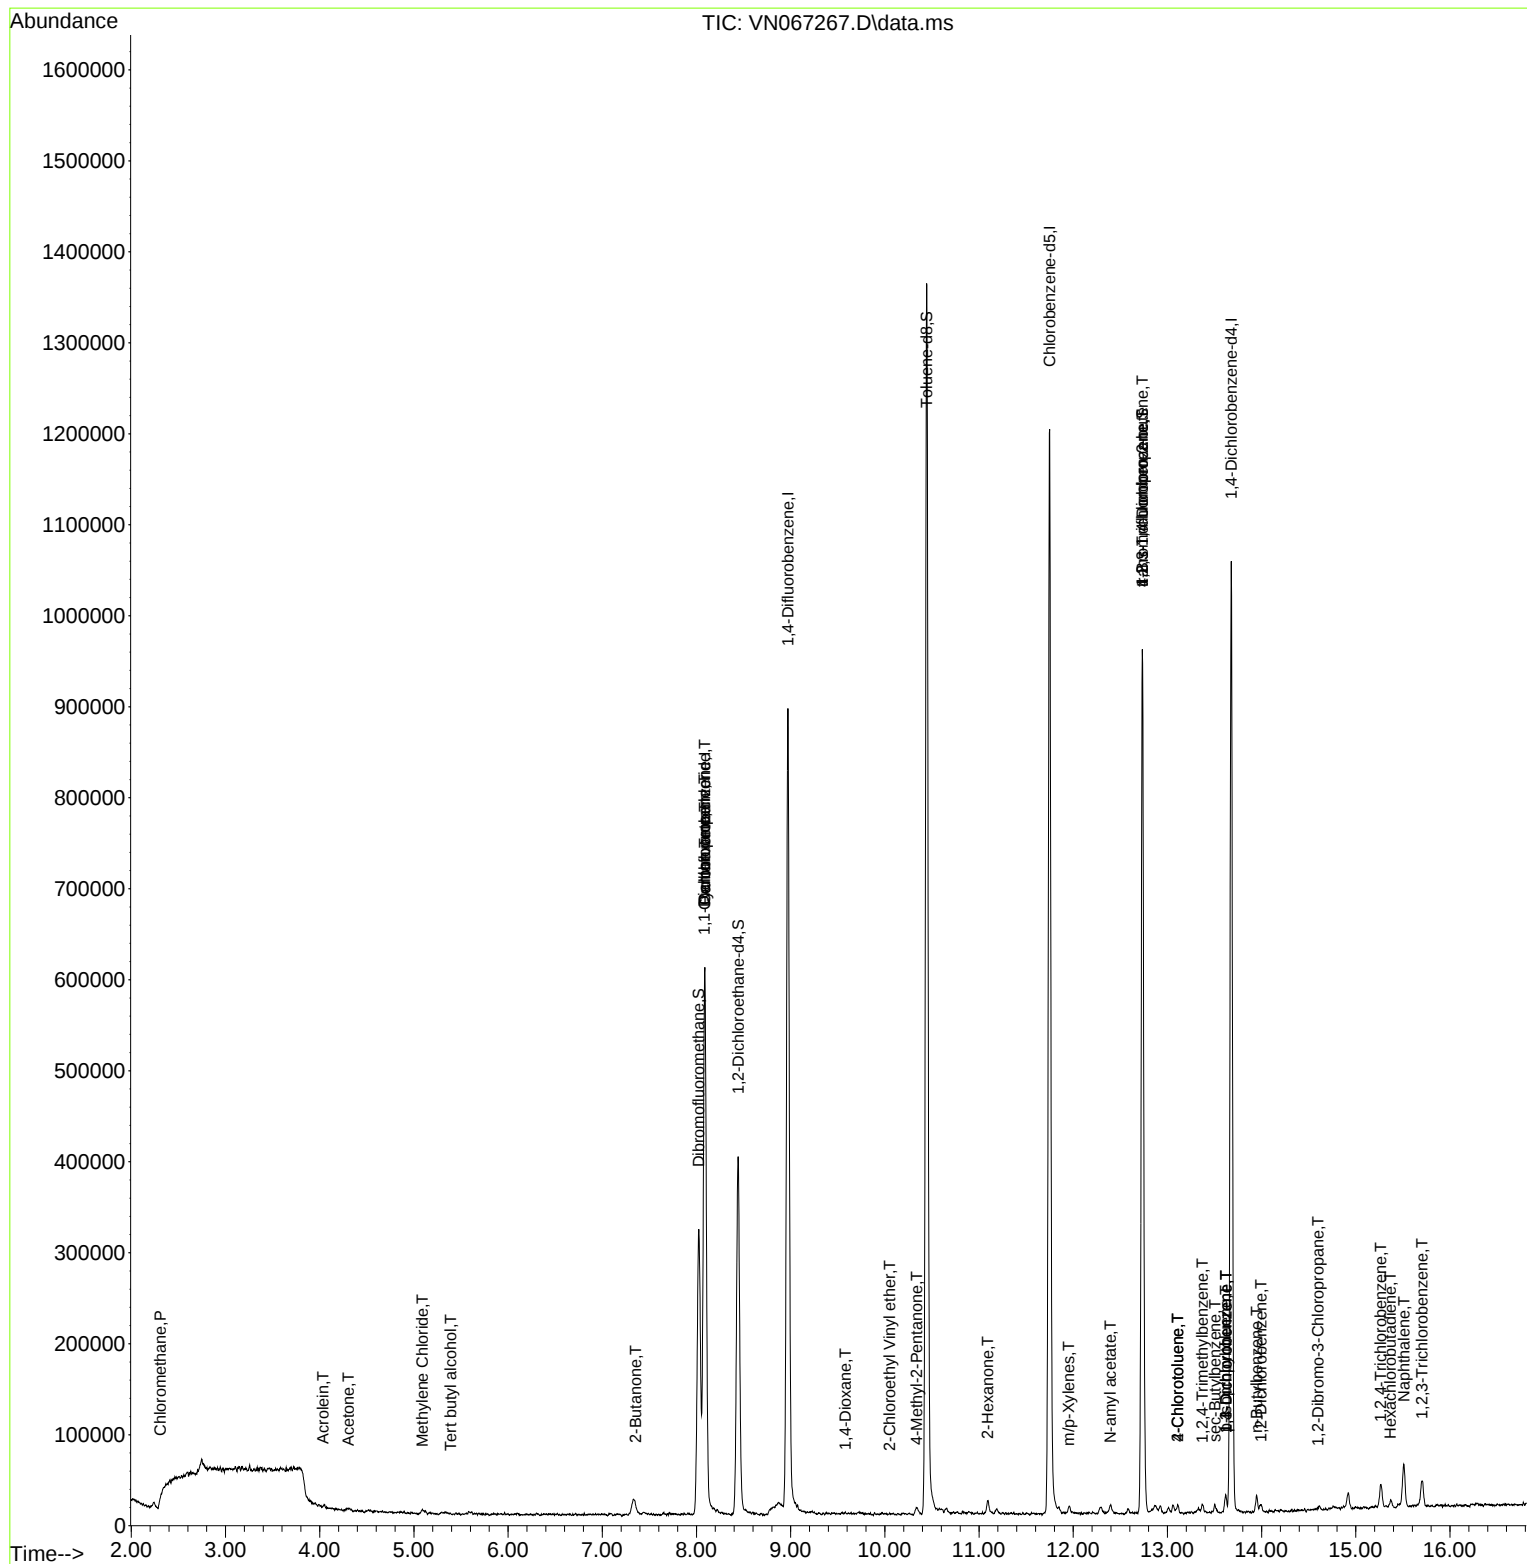




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.000 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:168 Resp: 397440
Ion Ratio Lower Upper
168 100
99 76.0 38.5 57.7#

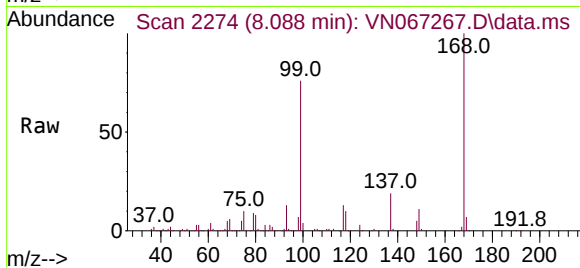

#3
Chloromethane
Concen: 0.24 ug/l
RT: 2.306 min Scan# 118
Delta R.T. 0.003 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08

Tgt Ion: 50 Resp: 1506
Ion Ratio Lower Upper
50 100
52 34.8 26.5 39.7

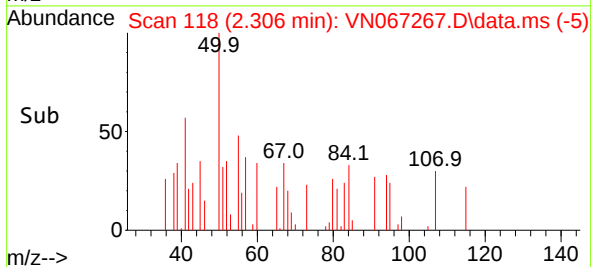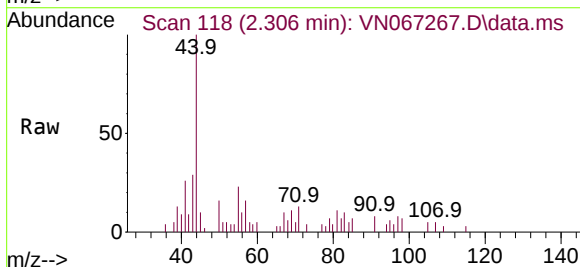







#11

Tert butyl alcohol
Concen: 0.30 ug/l
RT: 5.390 min Scan# 1268
Delta R.T. -0.005 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08

Instrument :
MSVOA_N
ClientSampled :




Tgt Ion: 59 Resp: 386
Ion Ratio Lower Upper
59 100
57 25.6 3.5 5.3#




#13

Acrolein
Concen: 0.50 ug/l
RT: 4.036 min Scan# 763
Delta R.T. -0.003 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08

Tgt Ion: 56 Resp: 258
Ion Ratio Lower Upper
56 100
55 227.9 53.8 80.6#


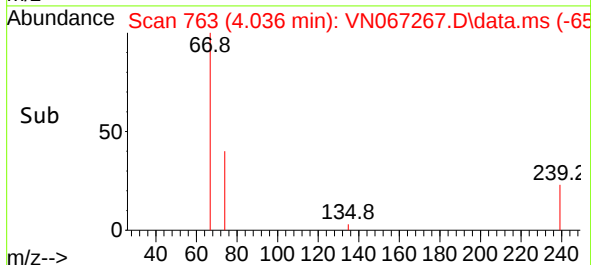

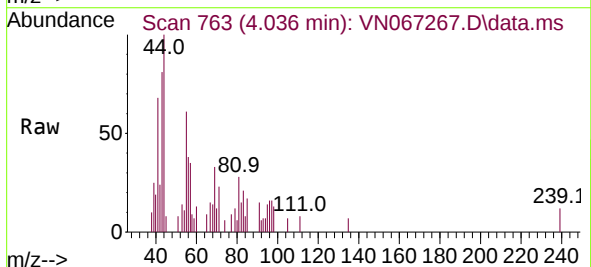




#16
Acetone
Concen: 1.29 ug/l
RT: 4.301 min Scan# 862
Delta R.T. 0.008 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 3900
Ion Ratio Lower Upper
43 100
58 16.4 27.2 40.8#



#20
Methylene Chloride
Concen: 0.35 ug/l
RT: 5.090 min Scan# 1156
Delta R.T. -0.008 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08

Tgt Ion: 84 Resp: 1906
Ion Ratio Lower Upper
84 100
49 106.4 88.3 132.5
51 38.0 26.7 40.1
86 48.2 51.1 76.7#


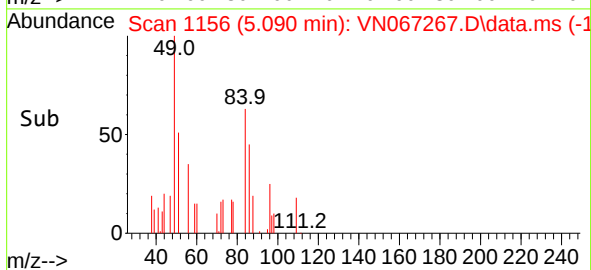






#25
2-Butanone
Concen: 0.31 ug/l
RT: 7.353 min Scan# 2000
Delta R.T. 0.011 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 1449
Ion Ratio Lower Upper
43 100
72 18.5 24.4 36.6#



#31
Cyclohexane
Concen: 1.36 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.008 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08

Tgt Ion: 56 Resp: 12595
Ion Ratio Lower Upper
56 100
69 153.5 28.0 42.0#
84 91.3 74.2 111.2

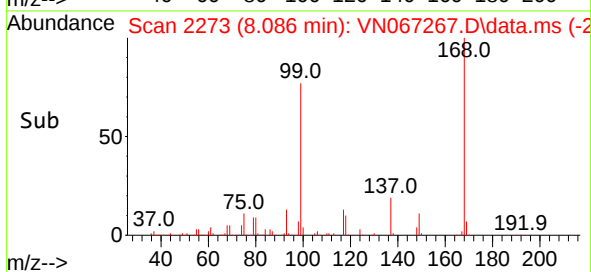



#33

1,2-Dichloroethane-d4

Concen: 46.54 ug/l

RT: 8.442 min Scan# 2406

Delta R.T. 0.005 min

Lab File: VN067267.D





Acq: 10 Jun 2021 13:08

Tgt Ion: 65 Resp: 349604

Ion Ratio Lower Upper

65 100

67 49.9 0.0 110.4

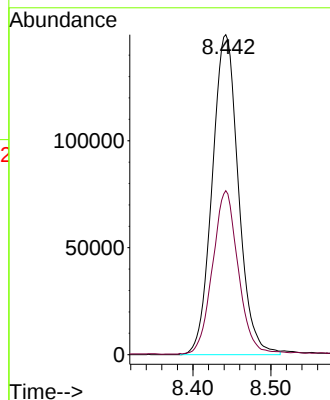

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 8.971 min Scan# 2603

Delta R.T. -0.000 min

Lab File: VN067267.D

Acq: 10 Jun 2021 13:08




Tgt Ion: 114 Resp: 721907


Ion Ratio Lower Upper

114 100

63 25.2 0.0 35.8

88 18.1 0.0 30.4


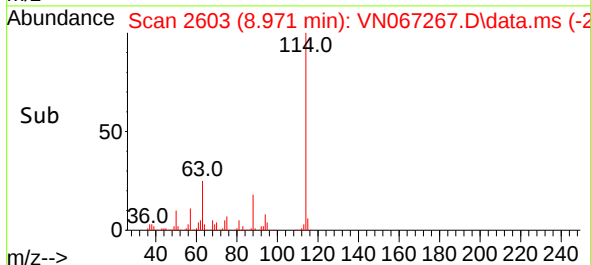
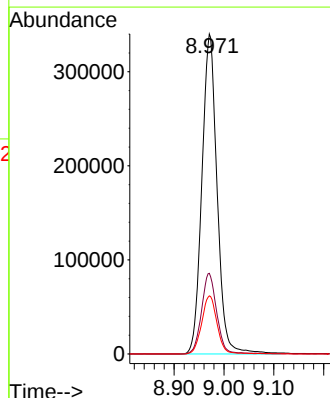
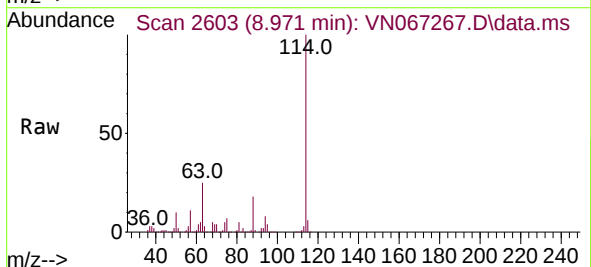




#35
Dibromofluoromethane
Concen: 49.11 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. -0.000 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:113 Resp: 225919
Ion Ratio Lower Upper
113 100
111 105.2 82.6 124.0
192 16.4 18.2 27.4#

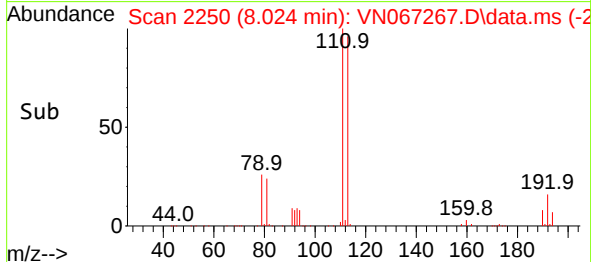

#36
1,1-Dichloropropene
Concen: 5.55 ug/l
RT: 8.083 min Scan# 2272
Delta R.T. -0.140 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08


Tgt Ion: 75 Resp: 42436
Ion Ratio Lower Upper
75 100
110 0.0 19.1 57.3#
77 0.2 24.8 37.2#

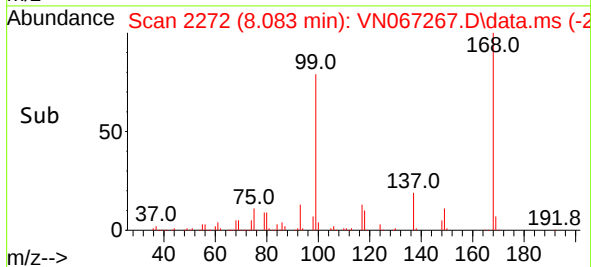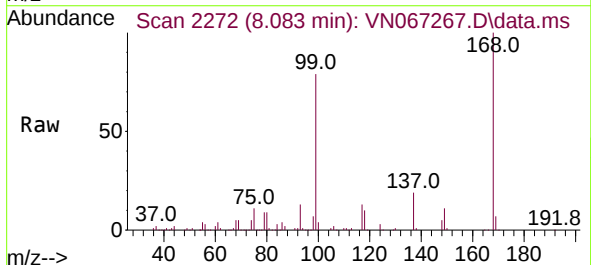



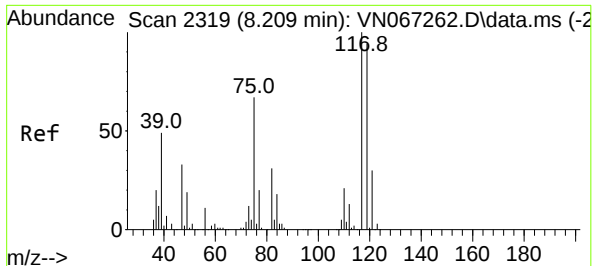


#38
Carbon Tetrachloride
Concen: 6.21 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.121 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08


Instrument :
MSVOA_N
ClientSampled :

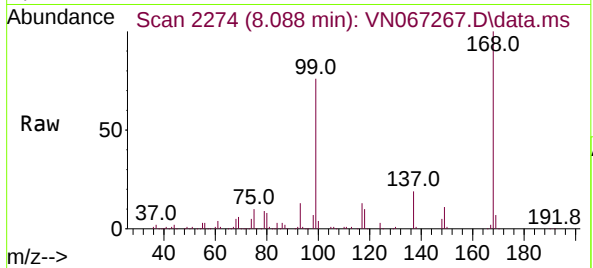



Tgt Ion:117 Resp: 49493
Ion Ratio Lower Upper
117 100
119 4.0 78.2 117.2#
121 0.0 24.7 37.1#

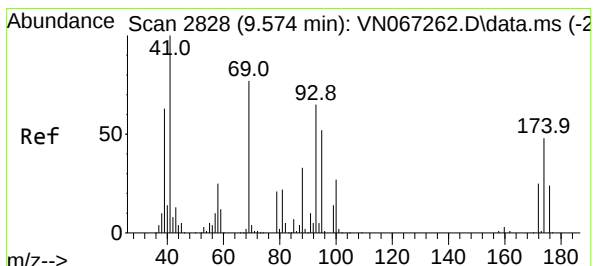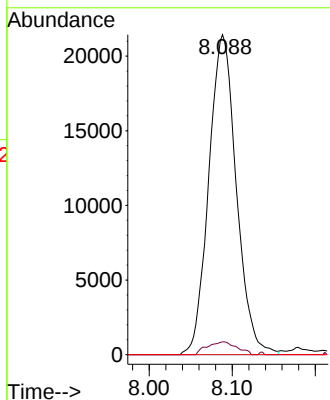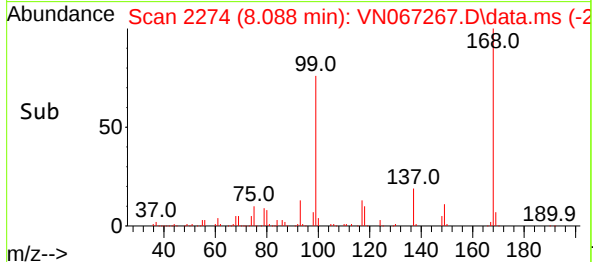


#49
1,4-Dioxane
Concen: 1.93 ug/l
RT: 9.579 min Scan# 2830
Delta R.T. 0.005 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08

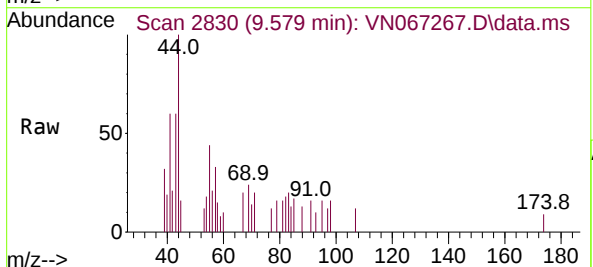

Tgt Ion: 88 Resp: 172
Ion Ratio Lower Upper
88 100
43 0.0 21.8 32.8#
58 150.6 50.8 76.2#



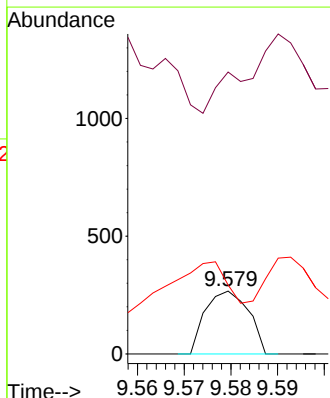
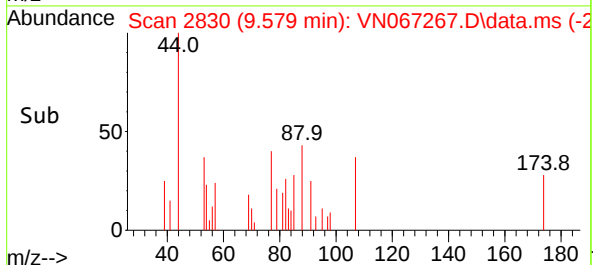


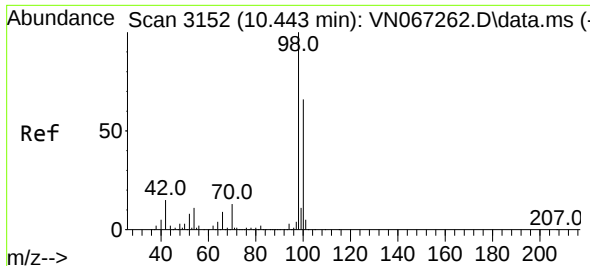

#50
Toluene-d8
Concen: 51.04 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. -0.000 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 98 Resp: 922744
Ion Ratio Lower Upper
98 100
100 65.0 51.8 77.8

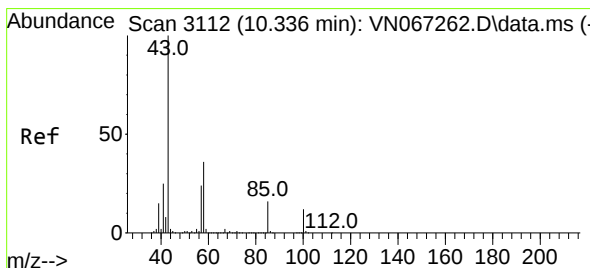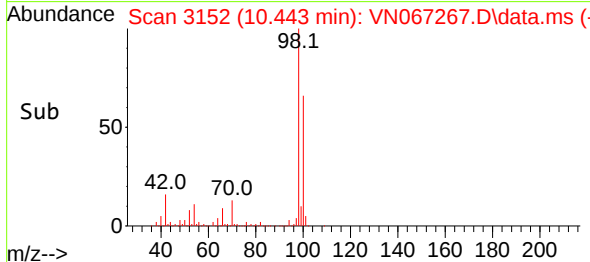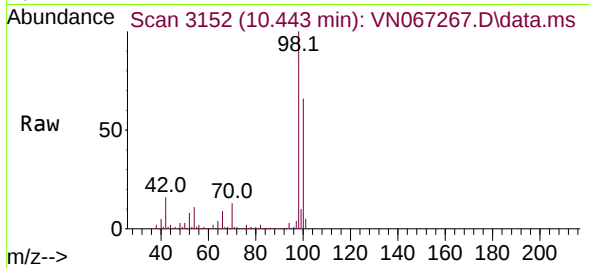

#51
4-Methyl-2-Pentanone
Concen: 0.69 ug/l
RT: 10.338 min Scan# 3113
Delta R.T. 0.002 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08

Tgt Ion: 43 Resp: 6561
Ion Ratio Lower Upper
43 100
58 25.8 34.5 51.7#


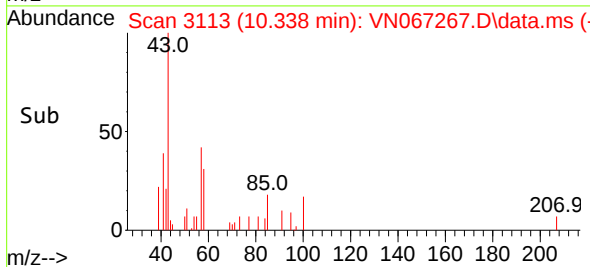

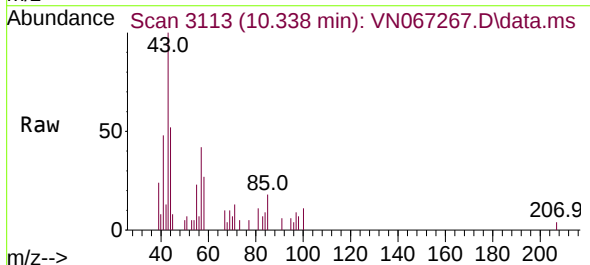


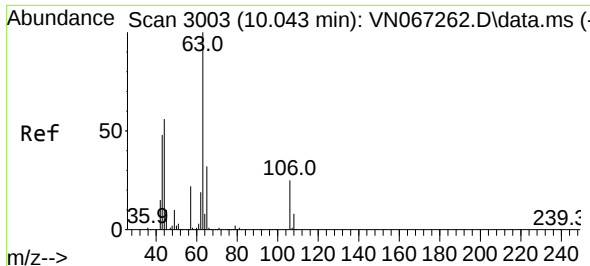

#58
2-Chloroethyl Vinyl ether
Concen: 28.15 ug/l
RT: 10.051 min Scan# 3006
Delta R.T. 0.008 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 63 Resp: 169
Ion Ratio Lower Upper
63 100
106 0.0 23.9 35.9#

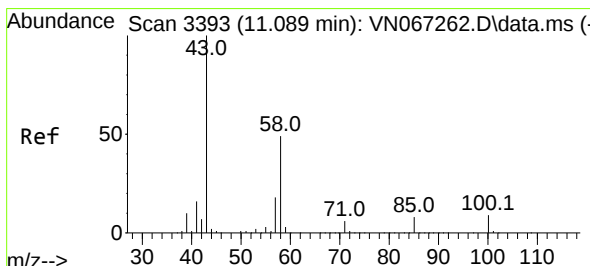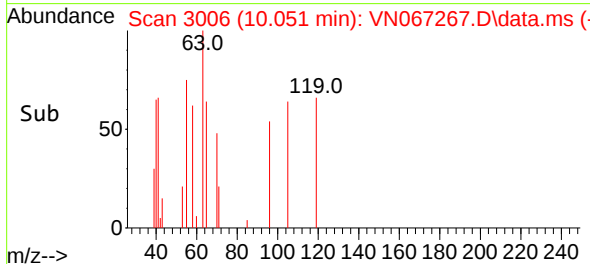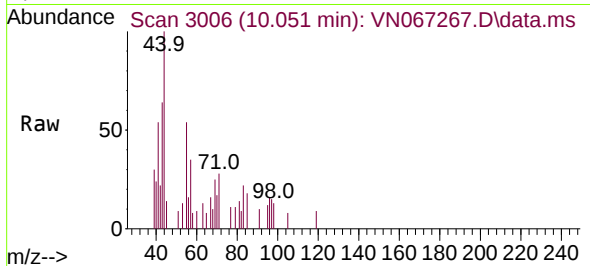

#59
2-Hexanone
Concen: 1.93 ug/l
RT: 11.092 min Scan# 3394
Delta R.T. 0.003 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08

Tgt Ion: 43 Resp: 13157
Ion Ratio Lower Upper
43 100
58 37.9 29.8 89.5


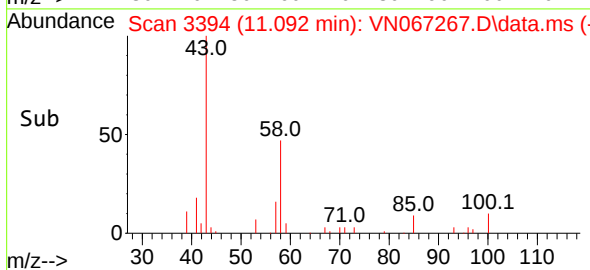

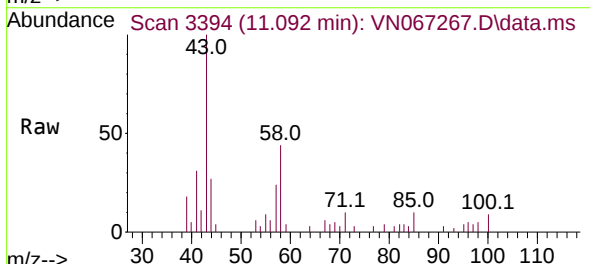


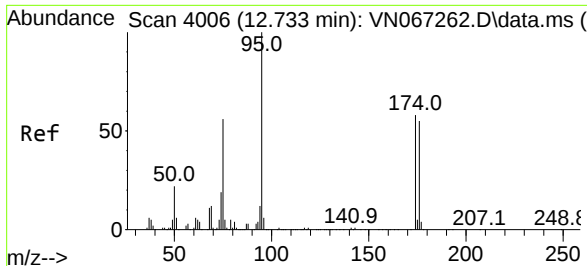

#62
4-Bromofluorobenzene
Concen: 47.33 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.000 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 356040
Ion Ratio Lower Upper
95 100
174 58.9 0.0 182.8
176 57.0 0.0 176.6

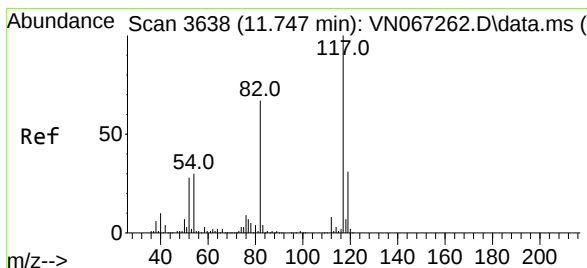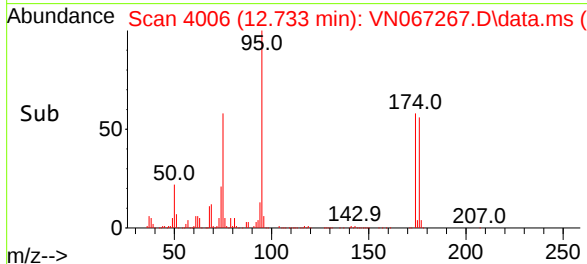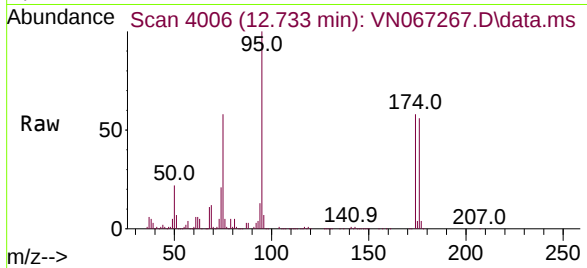

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.749 min Scan# 3639
Delta R.T. 0.003 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08

Tgt Ion:117 Resp: 633879
Ion Ratio Lower Upper
117 100
82 65.9 42.2 63.2#
119 32.0 25.8 38.6


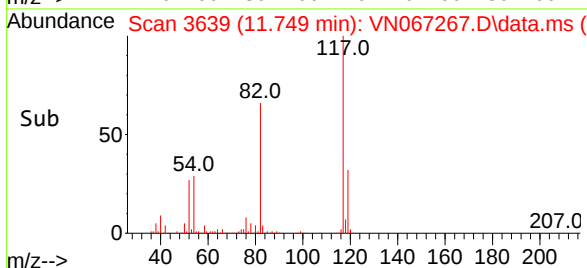

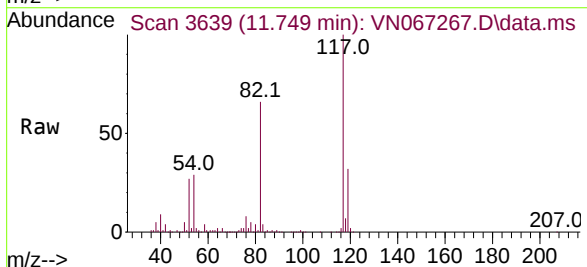


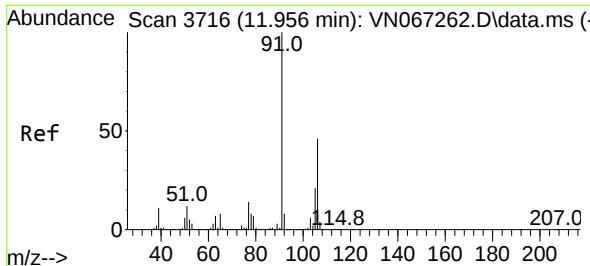

#68
m/p-Xylenes
Concen: 0.24 ug/l
RT: 11.950 min Scan# 3714
Delta R.T. -0.005 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:106 Resp: 2281
Ion Ratio Lower Upper
106 100
91 189.7 155.2 232.8

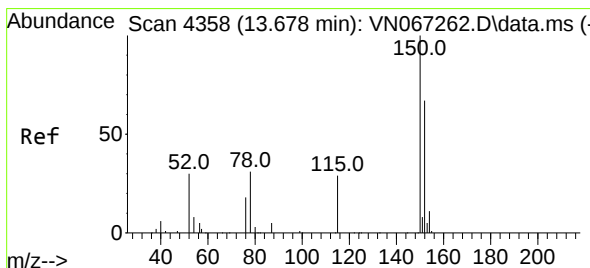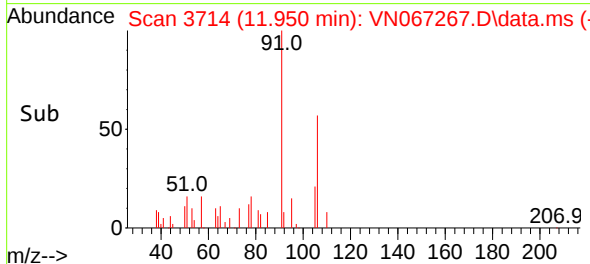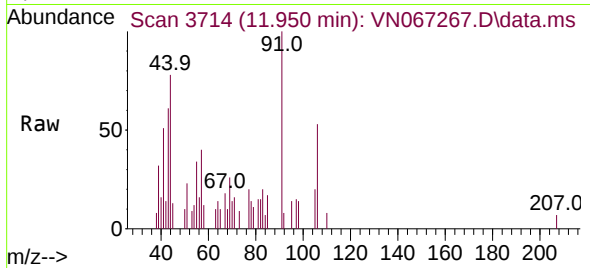

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.677 min Scan# 4358
Delta R.T. -0.001 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08

Tgt Ion:152 Resp: 245008
Ion Ratio Lower Upper
152 100
115 71.0 27.0 80.8
150 157.0 0.0 350.2


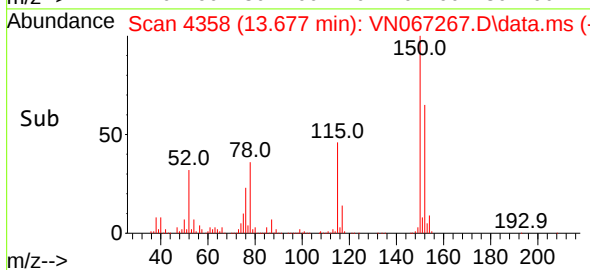

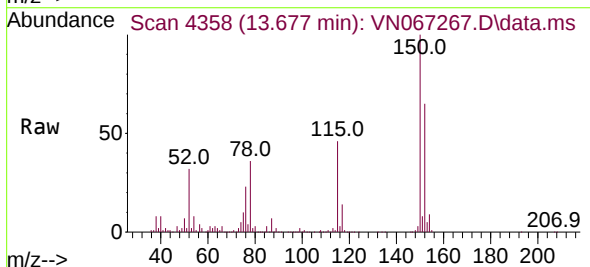


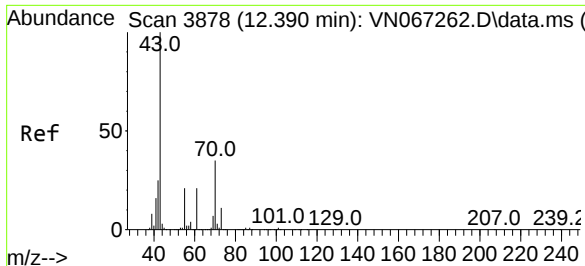

#74
N-amy1 acetate
Concen: 0.59 ug/l
RT: 12.393 min Scan# 3879
Delta R.T. 0.003 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43	Resp: 6719
Ion Ratio	Lower Upper
43 100	
70 8.3	36.7 55.1#
55 25.4	17.6 26.4
61 17.8	18.9 28.3#

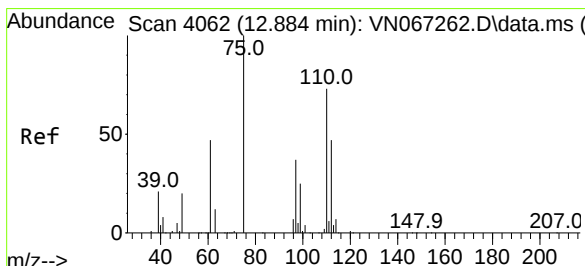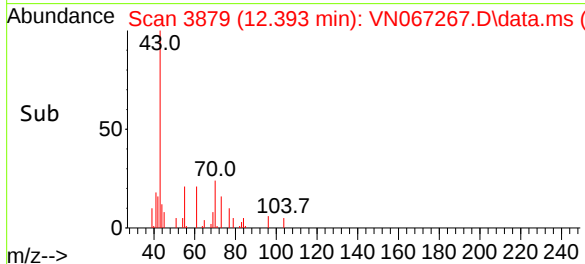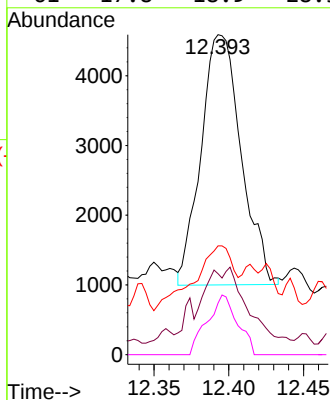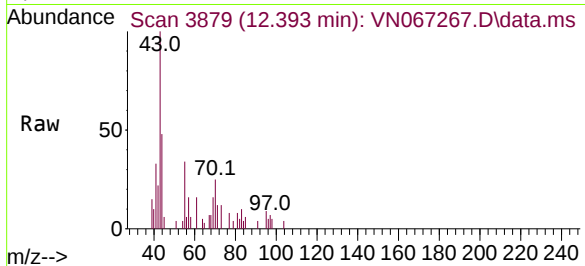

#76
1,2,3-Trichloropropane
Concen: 31.92 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.150 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08

Tgt Ion: 75	Resp: 207761
Ion Ratio	Lower Upper
75 100	
77 1.4	0.0 0.0#


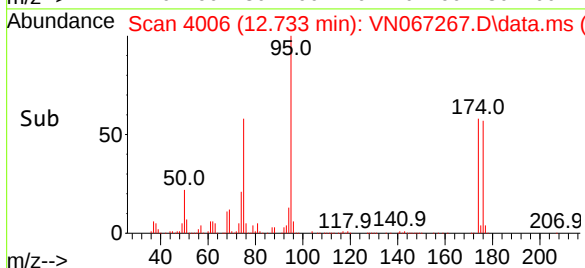
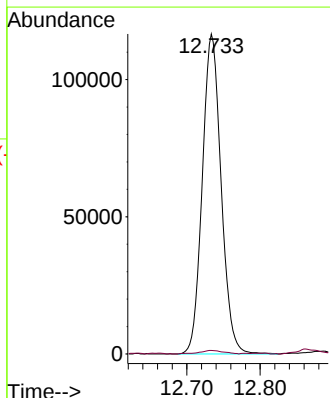
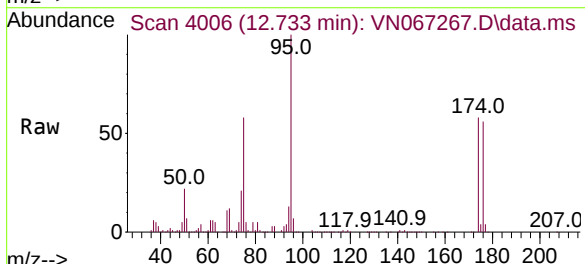




#79
2-Chlorotoluene
Concen: 0.32 ug/l
RT: 13.109 min Scan# 4146
Delta R.T. 0.003 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 5283
Ion Ratio Lower Upper
91 100
126 29.3 18.3 54.8



#81
trans-1,4-Dichloro-2-butene
Concen: 81.66 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.104 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08

Tgt Ion: 75 Resp: 207761
Ion Ratio Lower Upper
75 100
53 0.1 66.3 99.5#
89 0.0 39.5 59.3#



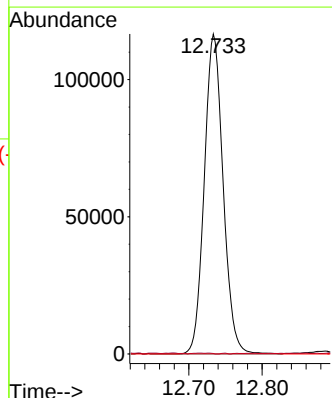





#82
4-Chlorotoluene
Concen: 0.32 ug/l
RT: 13.109 min Scan# 4146
Delta R.T. 0.099 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 5283
Ion Ratio Lower Upper
91 100
126 29.3 17.7 53.1



#84
1,2,4-Trimethylbenzene
Concen: 0.22 ug/l
RT: 13.372 min Scan# 4244
Delta R.T. 0.003 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08

Tgt Ion: 105 Resp: 4307
Ion Ratio Lower Upper
105 100
120 47.4 23.8 71.2


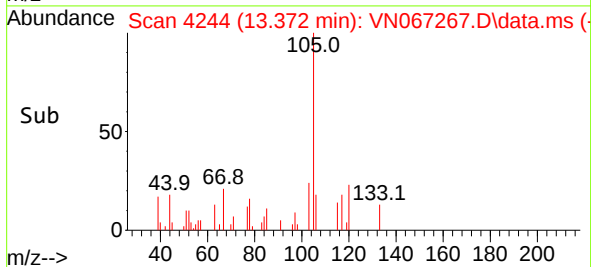

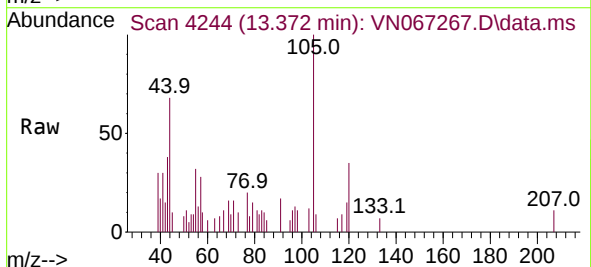




#85
 sec-Butylbenzene
 Concen: 0.21 ug/l
 RT: 13.503 min Scan# 4293
 Delta R.T. -0.000 min
 Lab File: VN067267.D
 Acq: 10 Jun 2021 13:08




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion:105 Resp: 4764
 Ion Ratio Lower Upper
 105 100
 134 19.1 10.5 31.5

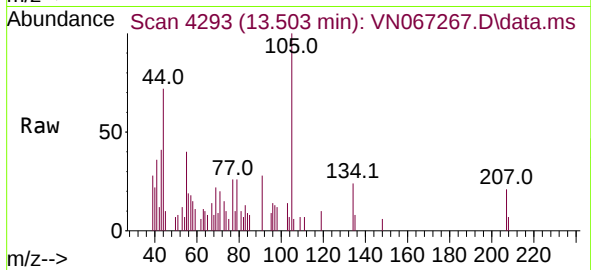

#86
 p-Isopropyltoluene
 Concen: 0.27 ug/l
 RT: 13.618 min Scan# 4336
 Delta R.T. -0.000 min
 Lab File: VN067267.D
 Acq: 10 Jun 2021 13:08

Tgt Ion:119 Resp: 5210
 Ion Ratio Lower Upper
 119 100
 134 27.5 13.3 39.9
 91 39.2 10.7 32.1#

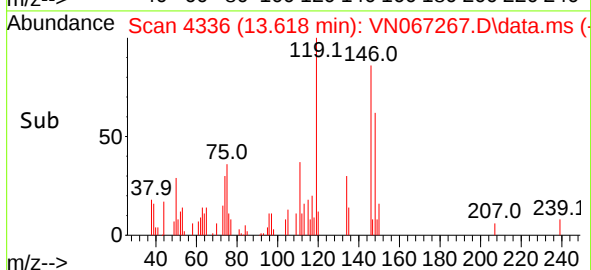







#87

1,3-Dichlorobenzene
Concen: 0.39 ug/l
RT: 13.621 min Scan# 4337
Delta R.T. 0.003 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08

Instrument :
MSVOA_N
ClientSampled :




Tgt Ion:146 Resp: 3298
Ion Ratio Lower Upper
146 100
111 51.9 19.3 57.8
148 65.0 32.0 96.2




#88

1,4-Dichlorobenzene
Concen: 0.40 ug/l
RT: 13.621 min Scan# 4337
Delta R.T. -0.075 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08

Tgt Ion:146 Resp: 3298
Ion Ratio Lower Upper
146 100
111 51.9 18.5 55.5
148 65.0 31.4 94.3


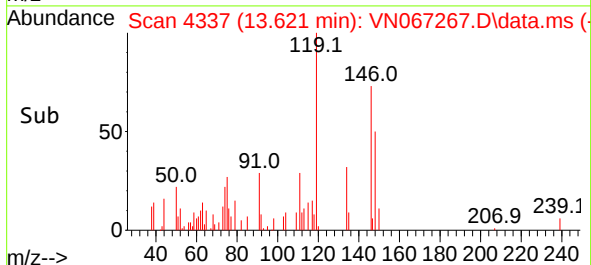
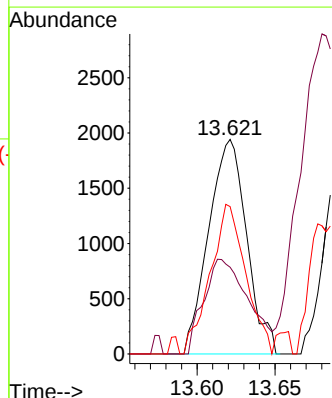
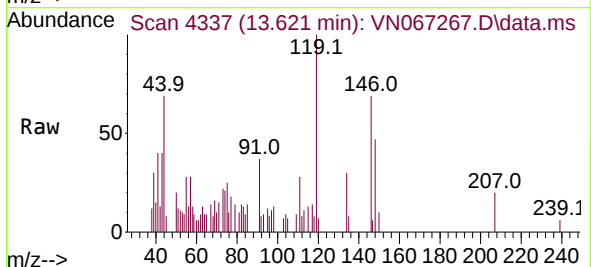




#89
n-Butylbenzene
Concen: 0.56 ug/l
RT: 13.946 min Scan# 4458
Delta R.T. 0.003 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91	Resp:	9855
Ion Ratio	Lower	Upper
91	100	
92	54.2	26.5 79.5
134	23.4	14.3 42.9

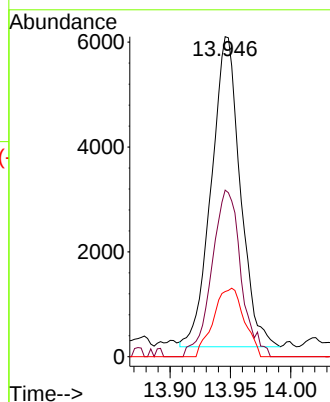

#91
1,2-Dichlorobenzene
Concen: 0.42 ug/l
RT: 13.994 min Scan# 4476
Delta R.T. 0.003 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08

Tgt Ion: 146	Resp:	3357
Ion Ratio	Lower	Upper
146	100	
111	62.4	19.8 59.3#
148	68.3	31.7 95.1


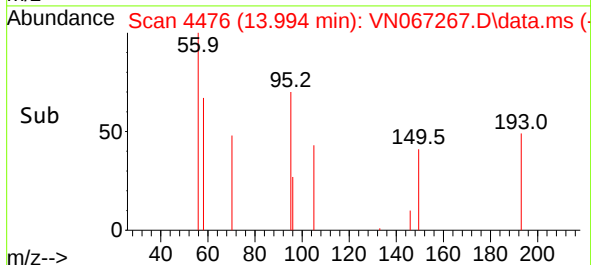
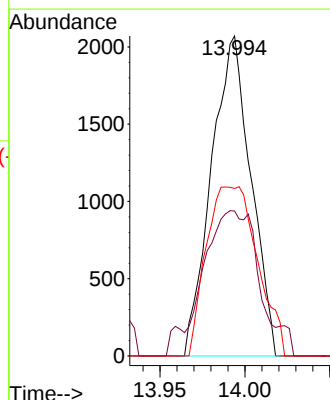
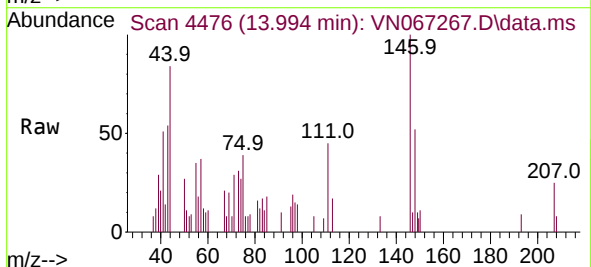


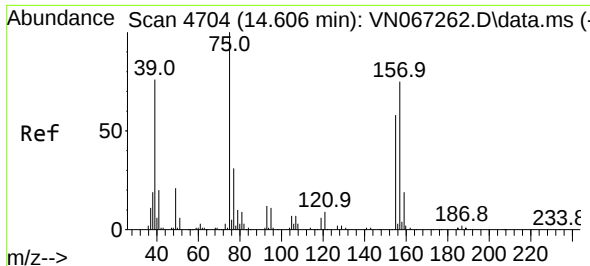

#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.41 ug/l
 RT: 14.597 min Scan# 4701
 Delta R.T. -0.008 min
 Lab File: VN067267.D
 Acq: 10 Jun 2021 13:08




Instrument :
 MSVOA_N
 ClientSampled :


Tgt Ion: 75 Resp: 684
 Ion Ratio Lower Upper
 75 100
 155 34.6 49.9 149.7#
 157 0.0 63.8 191.4#

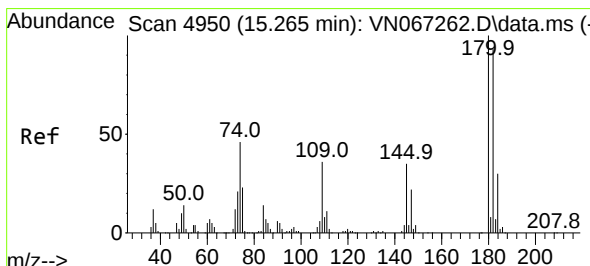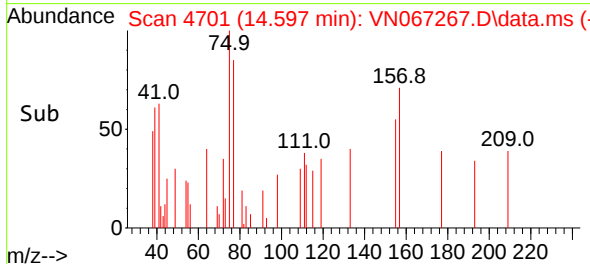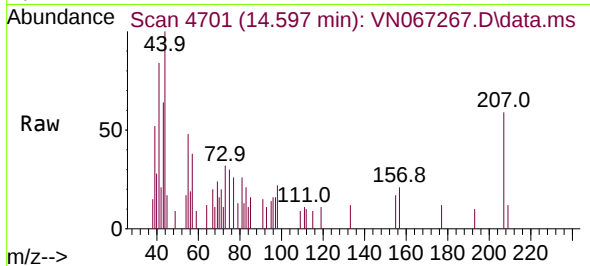

#93
 1,2,4-Trichlorobenzene
 Concen: 1.71 ug/l
 RT: 15.265 min Scan# 4950
 Delta R.T. -0.000 min
 Lab File: VN067267.D
 Acq: 10 Jun 2021 13:08

Tgt Ion:180 Resp: 6969
 Ion Ratio Lower Upper
 180 100
 182 100.9 47.3 141.8
 145 20.8 14.0 42.0


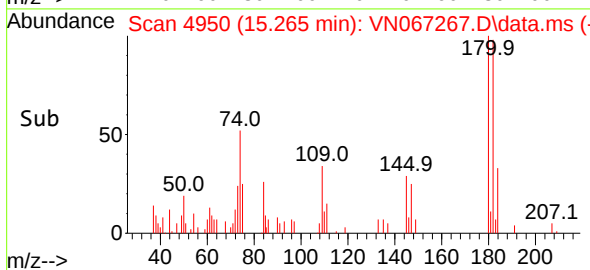

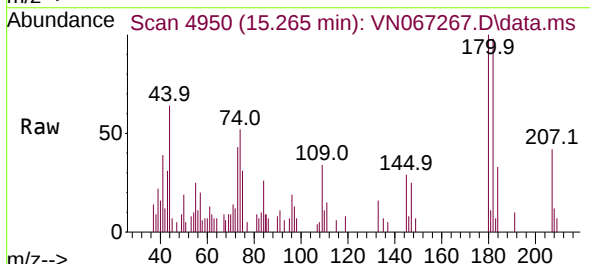




#94
Hexachlorobutadiene
Concen: 0.42 ug/l
RT: 15.367 min Scan# 4988
Delta R.T. -0.005 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:225 Resp: 997
Ion Ratio Lower Upper
225 100
223 46.6 31.7 95.1
227 75.4 31.7 95.1



#95
Naphthalene
Concen: 7.43 ug/l
RT: 15.509 min Scan# 5041
Delta R.T. 0.002 min
Lab File: VN067267.D
Acq: 10 Jun 2021 13:08

Tgt Ion:128 Resp: 41321
Ion Ratio Lower Upper
128 100
127 6.0 10.2 15.2#
129 11.0 8.6 13.0

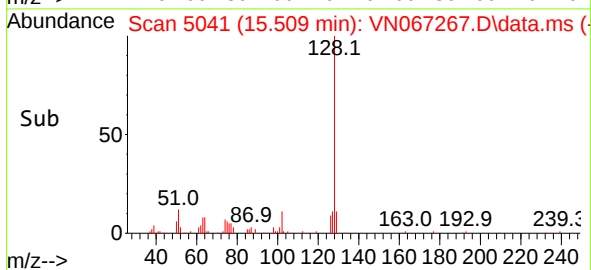

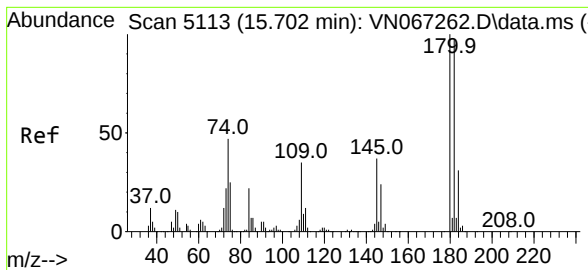

#96
 1,2,3-Trichlorobenzene
 Concen: 2.32 ug/l
 RT: 15.702 min Scan# 5113
 Delta R.T. -0.000 min
 Lab File: VN067267.D
 Acq: 10 Jun 2021 13:08

Instrument :
 MSVOA_N
 ClientSampleId :

Tgt Ion:	180	Resp:	8805
Ion	Ratio	Lower	Upper
180	100		
182	98.4	48.5	145.6
145	36.5	15.4	46.2

