
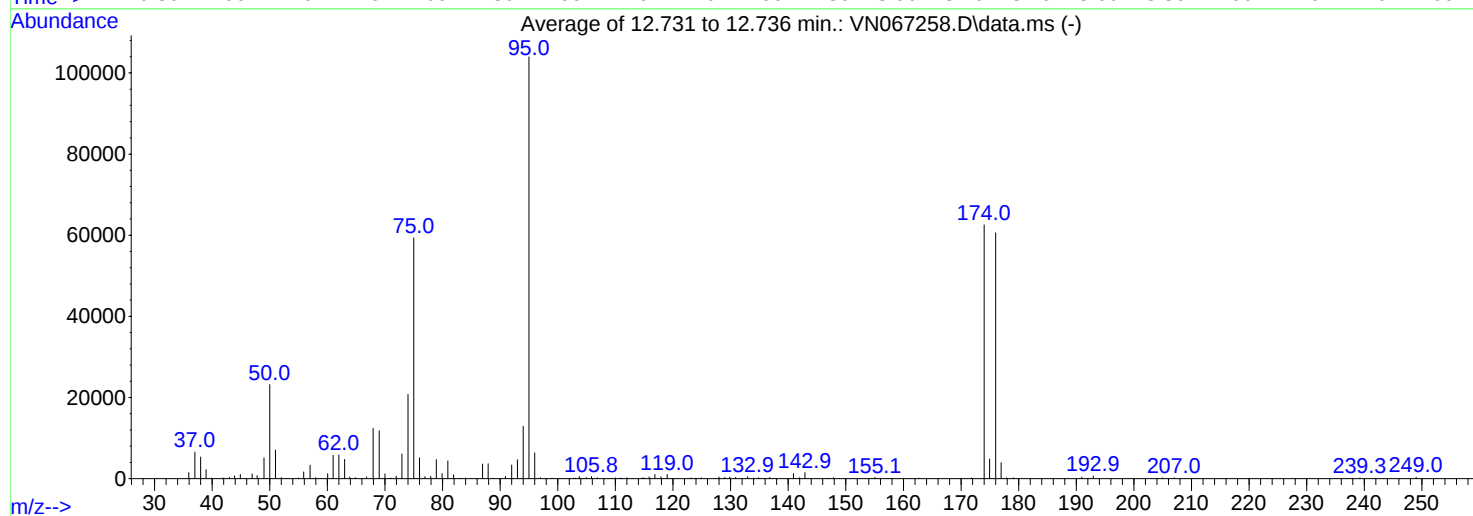


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061021\
 Data File : VN067258.D
 Acq On : 10 Jun 2021 8:50
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N061021W.M
 Title : SW846 8260
 Last Update : Fri Jun 11 05:27:41 2021

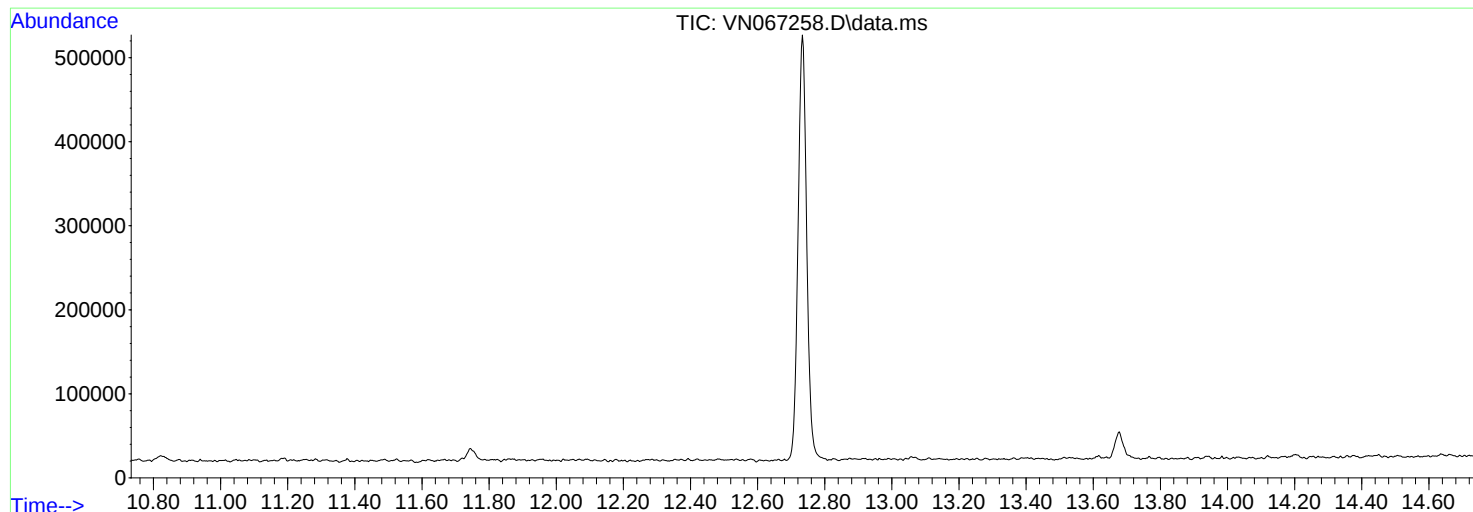

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3989

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	23187	PASS
75	95	30	60	57.1	59368	PASS
95	95	100	100	100.0	103971	PASS
96	95	5	9	6.1	6344	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	60.2	62549	PASS
175	174	5	9	7.8	4860	PASS
176	174	95	101	96.9	60579	PASS
177	176	5	9	6.5	3965	PASS