

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061022\
 Data File : VN072766.D
 Acq On : 10 Jun 2022 15:45
 Operator : JC\MD
 Sample : N3293-15 50X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 40807

Quant Time: Jun 11 01:54:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060822W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 09 05:17:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.081	168	171673	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.963	114	320284	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.745	117	283413	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.674	152	113063	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.433	65	248200	53.868	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 107.740%	
35) Dibromofluoromethane	8.022	113	182313	57.527	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 115.060%	
50) Toluene-d8	10.439	98	575643	45.526	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 91.060%	
62) 4-Bromofluorobenzene	12.727	95	219196	50.519	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 101.040%	


Target Compounds			Qvalue			
3) Chloromethane	2.299	50	656	Below Cal	#	67
5) Bromomethane	2.863	94	279	Below Cal	#	73
6) Chloroethane	3.051	64	218	Below Cal	#	42
11) Tert butyl alcohol	5.316	59	2989	2.719	ug/l	# 72
16) Acetone	4.304	43	11007	4.985	ug/l	# 75
17) Carbon Disulfide	4.534	76	163	0.311	ug/l	# 75
20) Methylene Chloride	5.087	84	485	Below Cal	#	10
25) 2-Butanone	7.334	43	164136	46.215	ug/l	# 89
29) Tetrahydrofuran	7.686	42	581	0.265	ug/l	# 46
31) Cyclohexane	8.081	56	6001	0.527	ug/l	# 55
36) 1,1-Dichloropropene	8.081	75	18596	4.227	ug/l	# 48
37) Ethyl Acetate	7.334	43	164136	24.016	ug/l	# 67
38) Carbon Tetrachloride	8.086	117	20431	4.346	ug/l	# 17
40) Benzene	8.457	78	16798	1.258	ug/l	# 98
52) Toluene	10.504	92	83770	10.051	ug/l	# 99
53) t-1,3-Dichloropropene	10.504	75	1359	0.236	ug/l	# 1
67) Ethyl Benzene	11.839	91	27695	1.950	ug/l	100
68) m/p-Xylenes	11.945	106	37089	7.350	ug/l	85
69) o-Xylene	12.274	106	24341	4.798	ug/l	93
70) Styrene	12.292	104	13440	1.686	ug/l	# 63
73) Isopropylbenzene	12.592	105	3046	0.251	ug/l	79
74) N-amyl acetate	12.457	43	1604	0.285	ug/l	# 63
76) 1,2,3-Trichloropropane	12.727	75	129458	35.483	ug/l	# 1
77) Bromobenzene	12.880	156	533	0.223	ug/l	# 1
78) n-propylbenzene	12.921	91	6009	0.454	ug/l	85
80) 1,3,5-Trimethylbenzene	13.057	105	9220	0.959	ug/l	97
81) trans-1,4-Dichloro-2-b...	12.727	75	129458	92.797	ug/l	# 11
84) 1,2,4-Trimethylbenzene	13.368	105	44106	4.797	ug/l	93
85) sec-Butylbenzene	13.368	105	44106	3.873	ug/l	# 56
86) p-Isopropyltoluene	13.568	119	4643	0.518	ug/l	# 75
90) Hexachloroethane	14.210	117	863	0.445	ug/l	# 9
95) Naphthalene	15.504	128	33174	4.466	ug/l	# 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061022\
Data File : VN072766.D
Acq On : 10 Jun 2022 15:45
Operator : JC\MD
Sample : N3293-15 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
40807


Quant Time: Jun 11 01:54:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060822W.M
Quant Title : SW846 8260
QLast Update : Thu Jun 09 05:17:31 2022
Response via : Initial Calibration

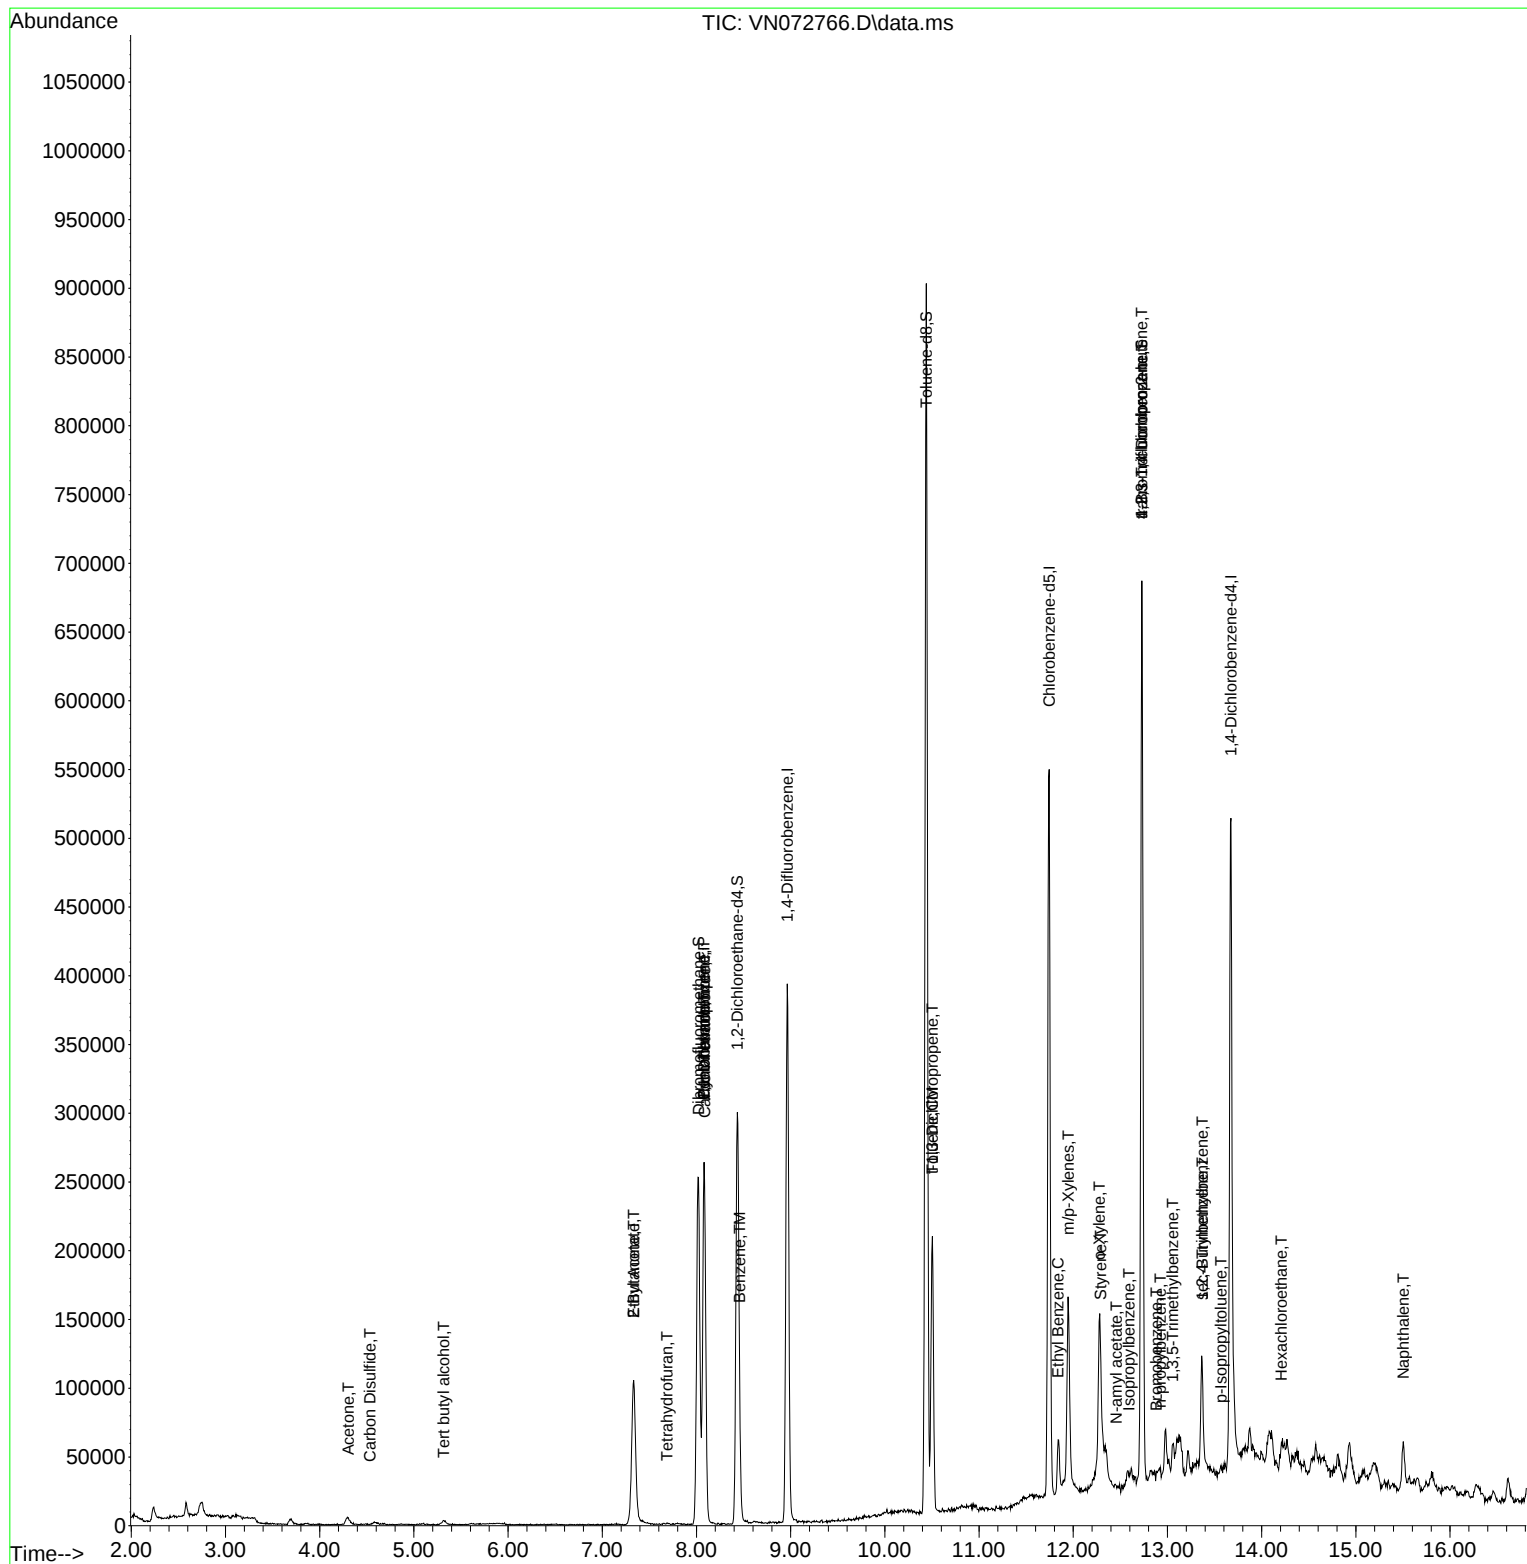



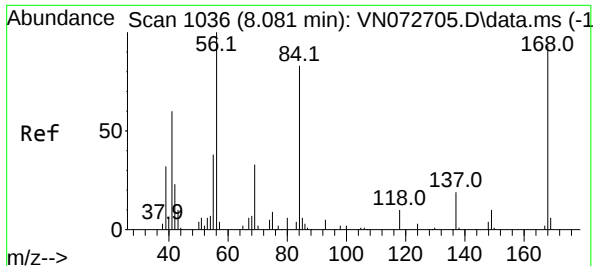


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.081 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN072766.D
Acq: 10 Jun 2022 15:45

Instrument :
MSVOA_N
ClientSampleId :
40807



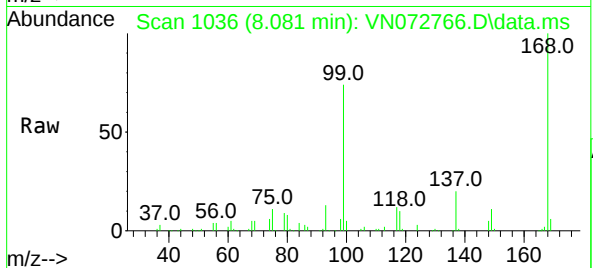



Tgt Ion:168 Resp: 171673
Ion Ratio Lower Upper
168 100
99 74.2 42.3 63.5#

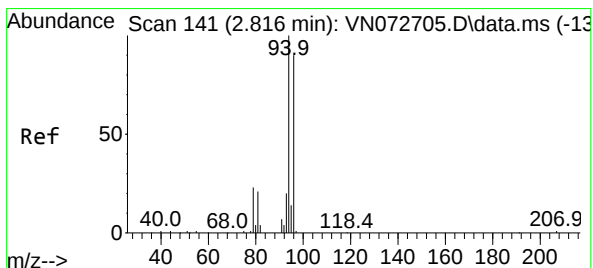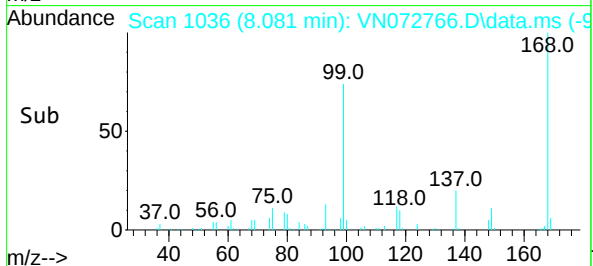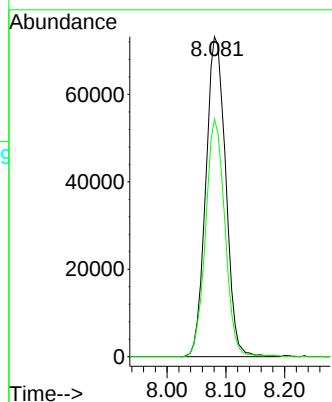

#5
Bromomethane
Concen: Below Cal
RT: 2.863 min Scan# 149
Delta R.T. 0.047 min
Lab File: VN072766.D
Acq: 10 Jun 2022 15:45

Tgt Ion: 94 Resp: 279
Ion Ratio Lower Upper
94 100
96 69.1 76.0 114.0#


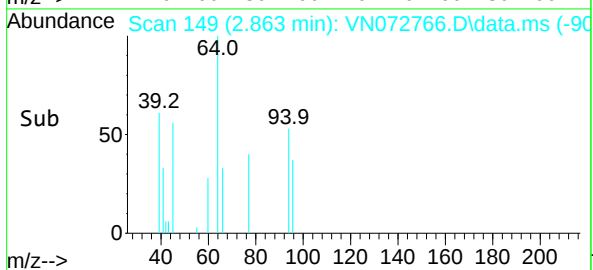
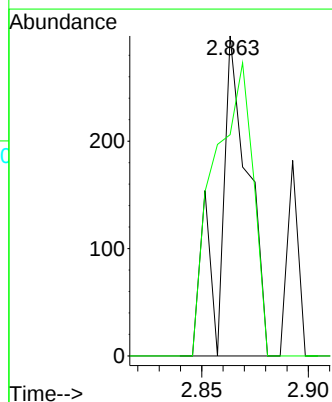
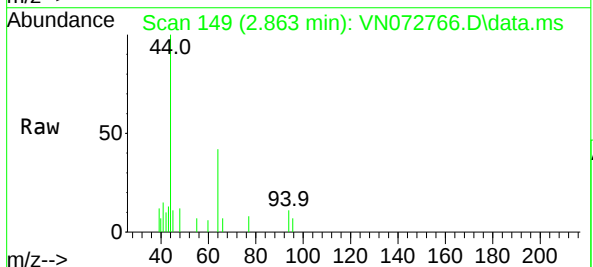


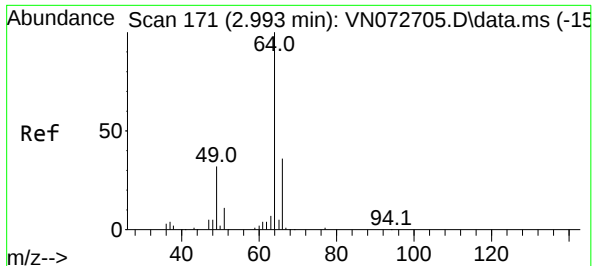

#6
Chloroethane
Concen: Below Cal
RT: 3.051 min Scan# 11
Delta R.T. 0.058 min
Lab File: VN072766.D
Acq: 10 Jun 2022 15:45




Instrument :
MSVOA_N
ClientSampleId :
40807


Tgt Ion: 64 Resp: 218
Ion Ratio Lower Upper
64 100
66 0.0 26.2 39.4#

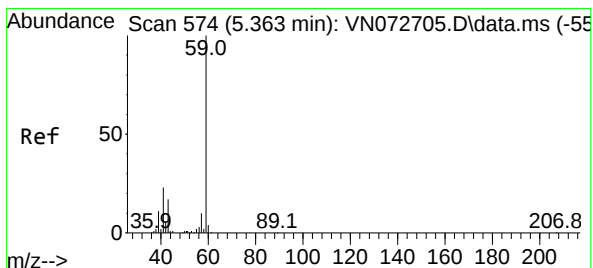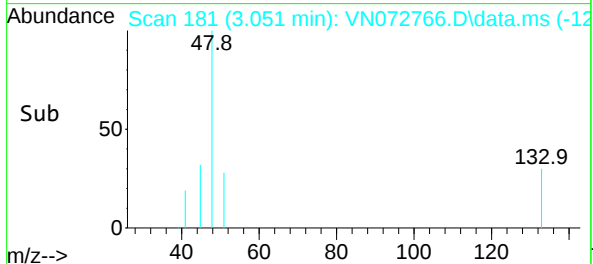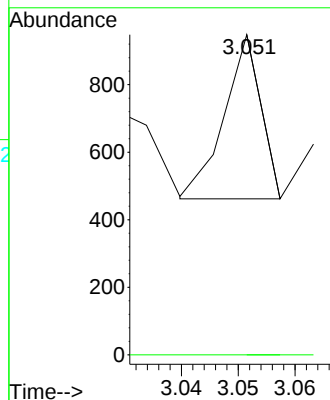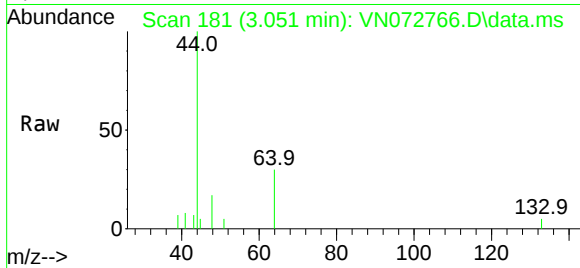

#11
Tert butyl alcohol
Concen: 2.719 ug/l
RT: 5.316 min Scan# 566
Delta R.T. -0.047 min
Lab File: VN072766.D
Acq: 10 Jun 2022 15:45

Tgt Ion: 59 Resp: 2989
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#


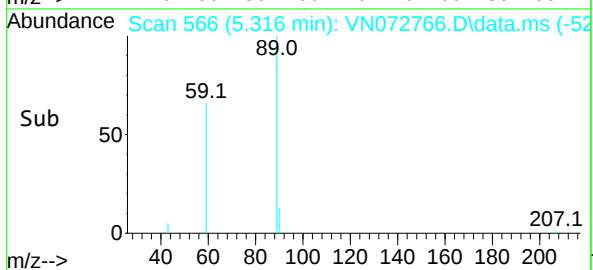
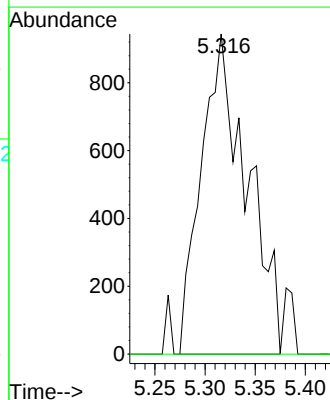
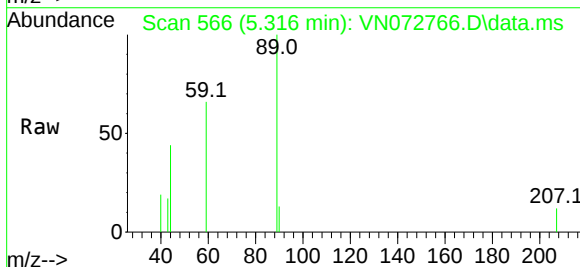


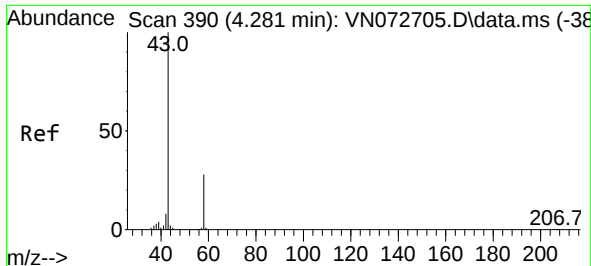

#16
Acetone
Concen: 4.985 ug/l
RT: 4.304 min Scan# 394
Delta R.T. 0.023 min
Lab File: VN072766.D
Acq: 10 Jun 2022 15:45




Instrument :
MSVOA_N
ClientSampleId :
40807


Tgt Ion: 43 Resp: 11007
Ion Ratio Lower Upper
43 100
58 18.4 26.0 39.0#

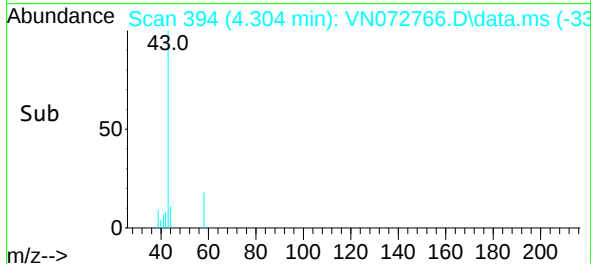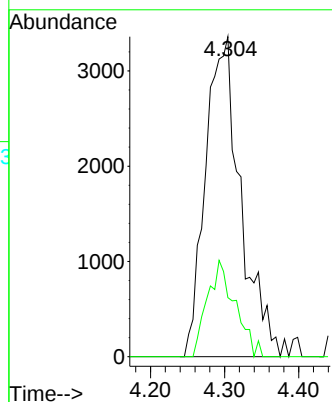

#17
Carbon Disulfide
Concen: 0.311 ug/l
RT: 4.534 min Scan# 433
Delta R.T. 0.012 min
Lab File: VN072766.D
Acq: 10 Jun 2022 15:45

Tgt Ion: 76 Resp: 163
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#


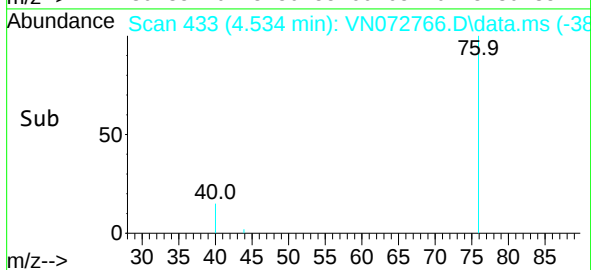
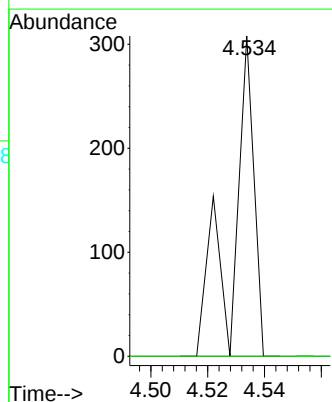
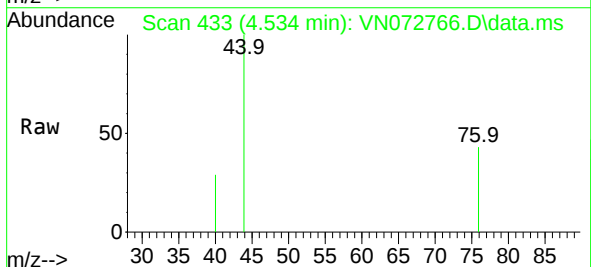




#25
2-Butanone
Concen: 46.215 ug/l
RT: 7.334 min Scan# 908
Delta R.T. 0.006 min
Lab File: VN072766.D
Acq: 10 Jun 2022 15:45




Instrument :
MSVOA_N
ClientSampleId :
40807


Tgt Ion: 43 Resp: 164136
Ion Ratio Lower Upper
43 100
72 23.5 23.7 35.5#

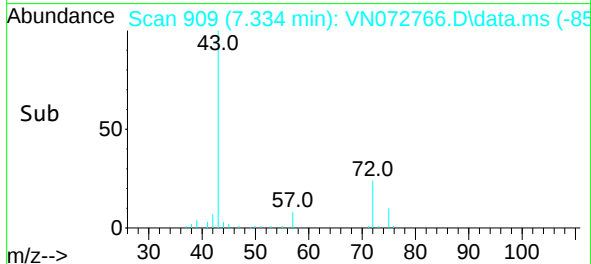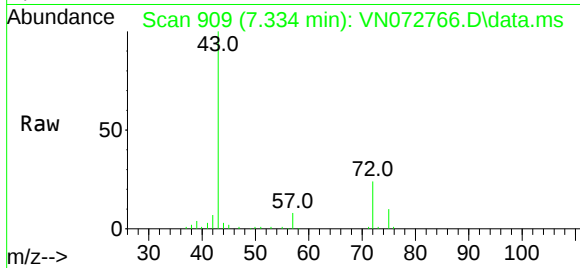

#29
Tetrahydrofuran
Concen: 0.265 ug/l
RT: 7.686 min Scan# 969
Delta R.T. 0.005 min
Lab File: VN072766.D
Acq: 10 Jun 2022 15:45

Tgt Ion: 42 Resp: 581
Ion Ratio Lower Upper
42 100
72 10.8 39.7 59.5#
71 12.0 36.6 55.0#

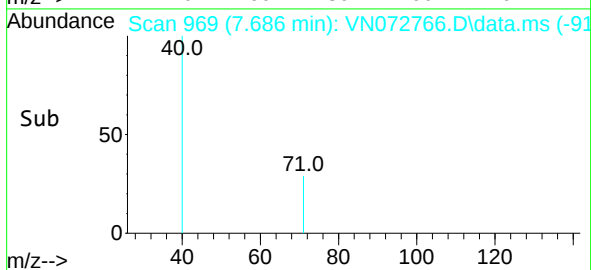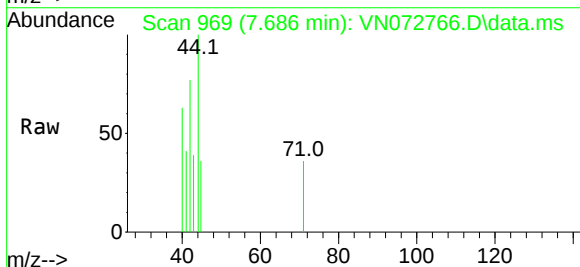

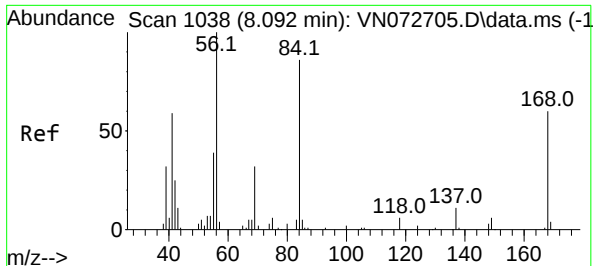

#31

Cyclohexane

Concen: 0.527 ug/l

RT: 8.081 min Scan# 1036

Delta R.T. -0.011 min

Lab File: VN072766.D

Acq: 10 Jun 2022 15:45

Instrument :

MSVOA_N

ClientSampleId :

40807





Tgt Ion: 56 Resp: 6001

Ion Ratio Lower Upper

56 100

69 131.4 27.8 41.8#

84 96.5 76.9 115.3

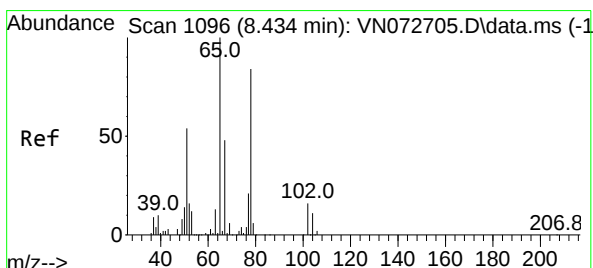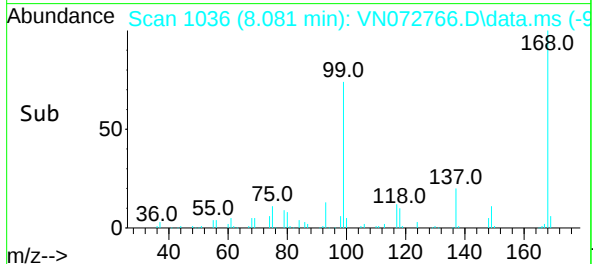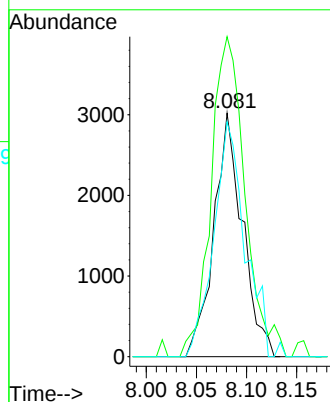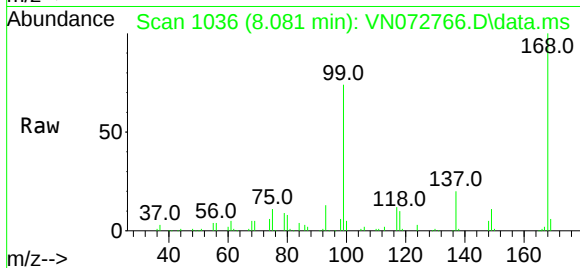

#33

1,2-Dichloroethane-d4

Concen: 53.868 ug/l

RT: 8.433 min Scan# 1096

Delta R.T. -0.001 min

Lab File: VN072766.D




Acq: 10 Jun 2022 15:45


Tgt Ion: 65 Resp: 248200

Ion Ratio Lower Upper

65 100

67 50.2 0.0 104.8

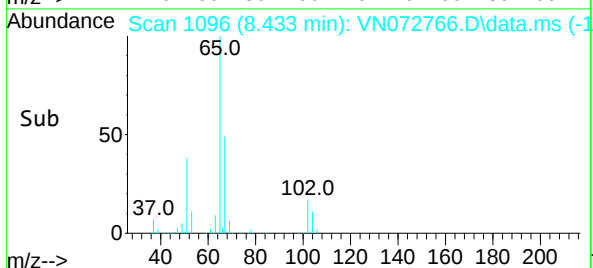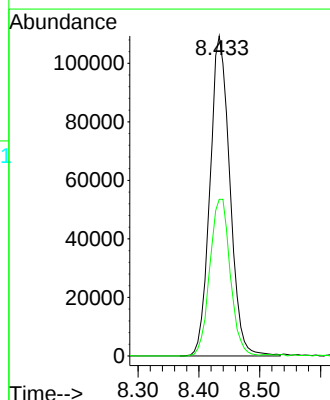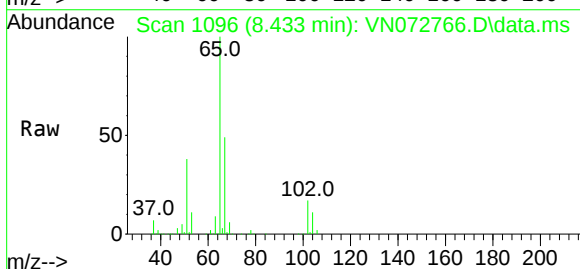

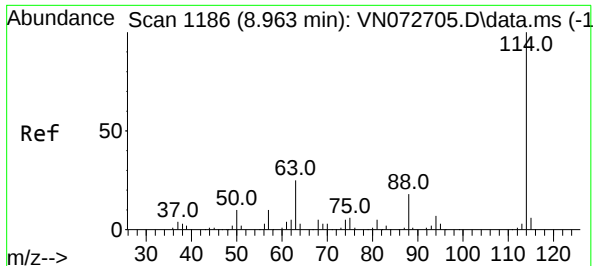

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.963 min Scan# 1186

Delta R.T. -0.000 min

Lab File: VN072766.D

Acq: 10 Jun 2022 15:45

Instrument :

MSVOA_N

ClientSampleId :

40807





Tgt Ion:114 Resp: 320284

Ion Ratio Lower Upper

114 100

63 24.4 0.0 40.0

88 16.9 0.0 32.6

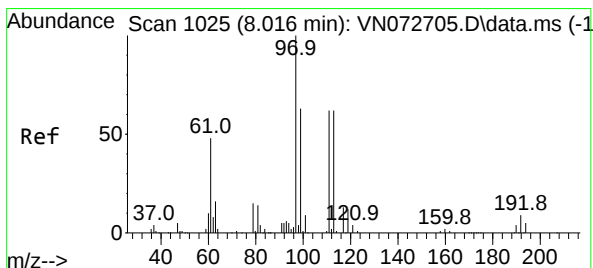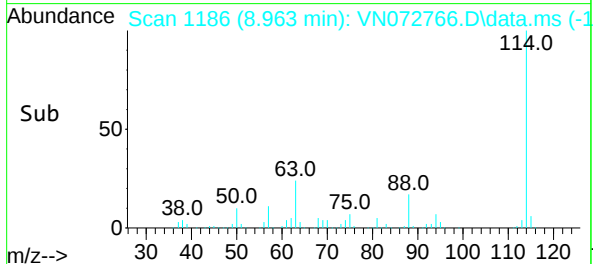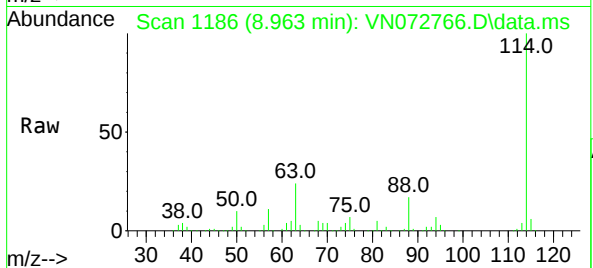

#35

Dibromofluoromethane

Concen: 57.527 ug/l

RT: 8.022 min Scan# 1026

Delta R.T. 0.006 min

Lab File: VN072766.D

Acq: 10 Jun 2022 15:45




Tgt Ion:113 Resp: 182313


Ion Ratio Lower Upper

113 100

111 103.8 81.4 122.0

192 15.4 17.0 25.6#


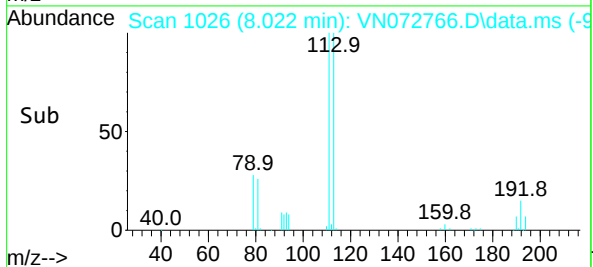

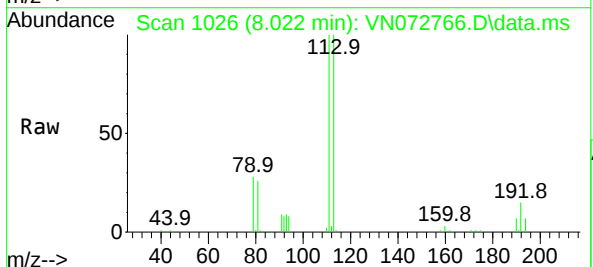


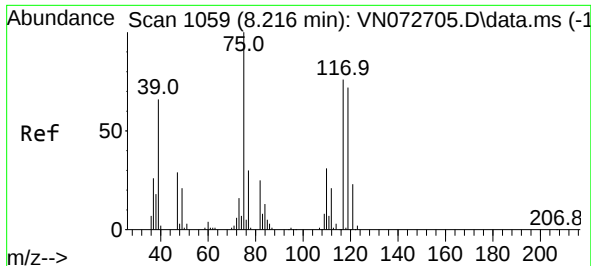

#36
1,1-Dichloropropene
Concen: 4.227 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.135 min
Lab File: VN072766.D
Acq: 10 Jun 2022 15:45




Instrument :
MSVOA_N
ClientSampleId :
40807


Tgt Ion: 75 Resp: 18596
Ion Ratio Lower Upper
75 100
110 7.7 18.3 54.8#
77 0.0 25.1 37.7#

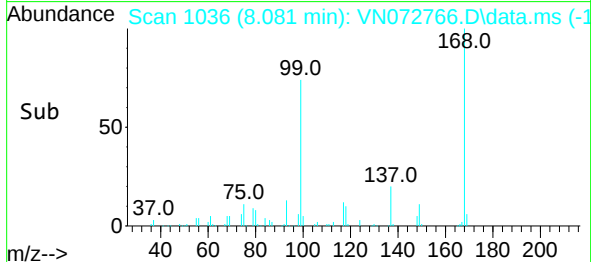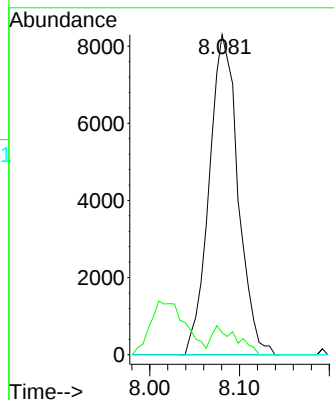

#37
Ethyl Acetate
Concen: 24.016 ug/l
RT: 7.334 min Scan# 909
Delta R.T. -0.076 min
Lab File: VN072766.D
Acq: 10 Jun 2022 15:45

Tgt Ion: 43 Resp: 164136
Ion Ratio Lower Upper
43 100
61 0.3 11.8 17.6#
70 0.0 9.3 13.9#


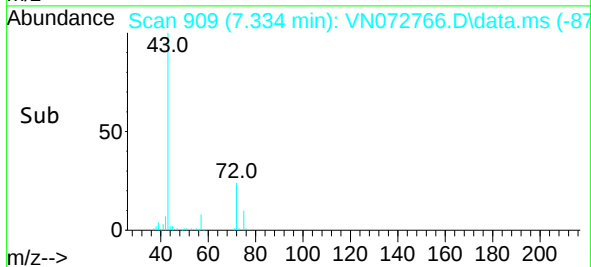
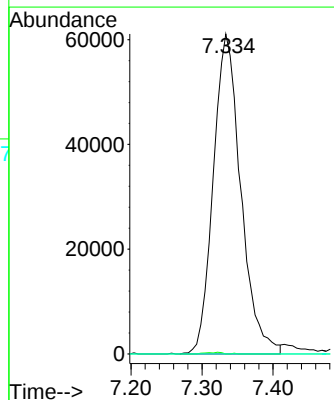
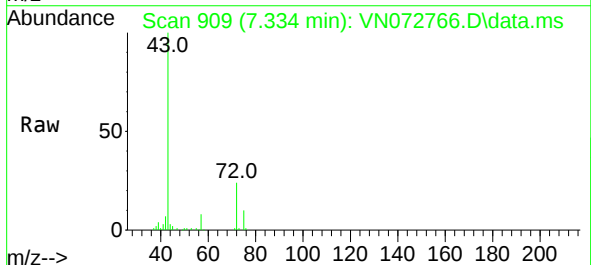


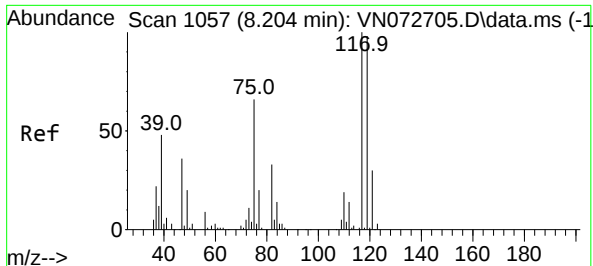

#38
Carbon Tetrachloride
Concen: 4.346 ug/l
RT: 8.086 min Scan# 1107
Delta R.T. -0.118 min
Lab File: VN072766.D
Acq: 10 Jun 2022 15:45




Instrument :
MSVOA_N
ClientSampleId :
40807


Tgt Ion:117 Resp: 20431
Ion Ratio Lower Upper
117 100
119 5.9 75.8 113.8#
121 0.0 24.6 37.0#

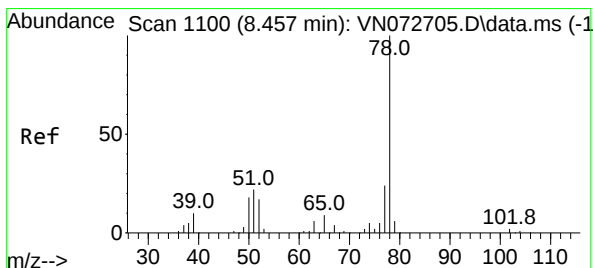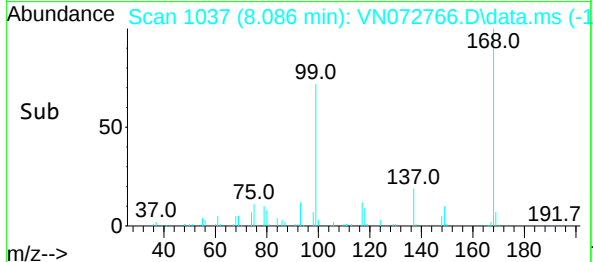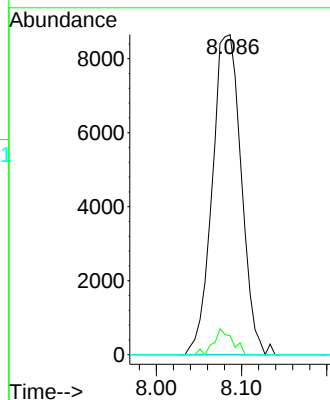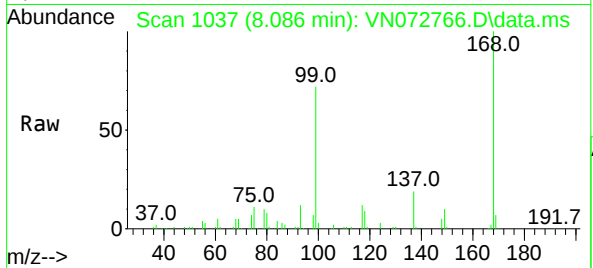

#40
Benzene
Concen: 1.258 ug/l
RT: 8.457 min Scan# 1100
Delta R.T. 0.000 min
Lab File: VN072766.D
Acq: 10 Jun 2022 15:45

Tgt Ion: 78 Resp: 16798
Ion Ratio Lower Upper
78 100
77 23.0 19.4 29.0


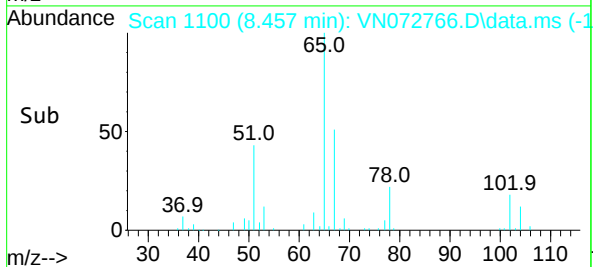
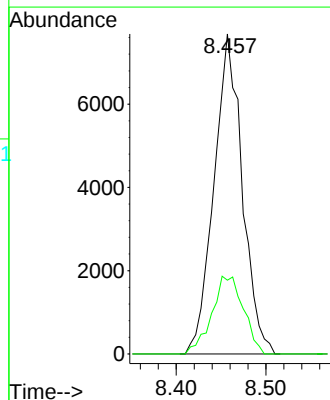
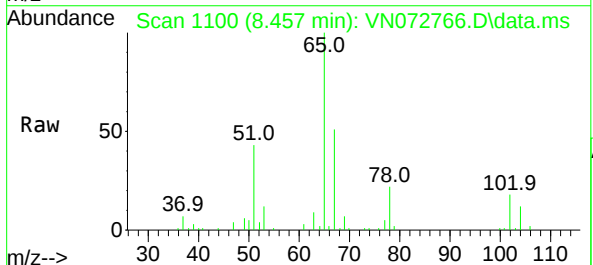


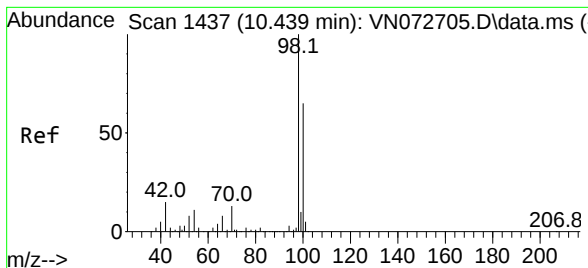

#50
Toluene-d8
Concen: 45.526 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN072766.D
Acq: 10 Jun 2022 15:45




Instrument :
MSVOA_N
ClientSampleId :
40807


Tgt Ion: 98 Resp: 575643
Ion Ratio Lower Upper
98 100
100 64.9 52.6 78.8

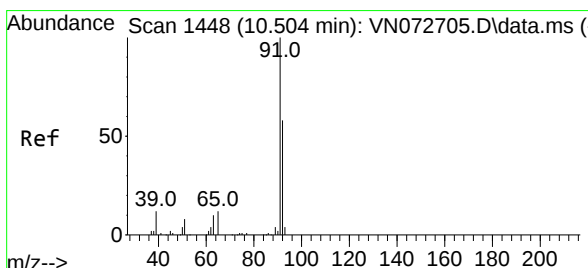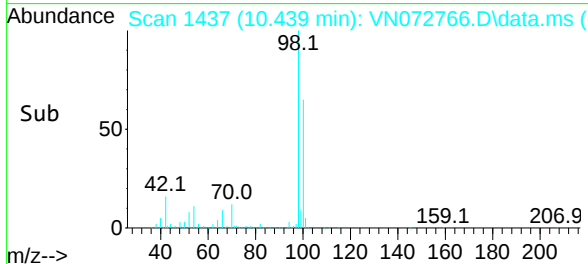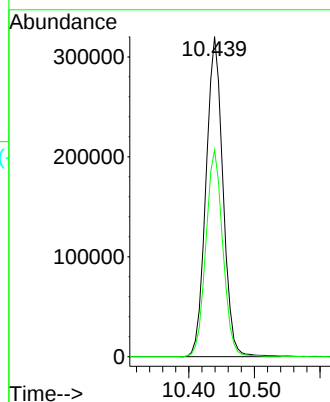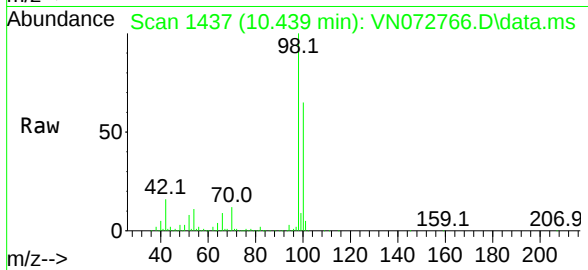

#52
Toluene
Concen: 10.051 ug/l
RT: 10.504 min Scan# 1448
Delta R.T. -0.000 min
Lab File: VN072766.D
Acq: 10 Jun 2022 15:45

Tgt Ion: 92 Resp: 83770
Ion Ratio Lower Upper
92 100
91 171.1 138.6 207.8


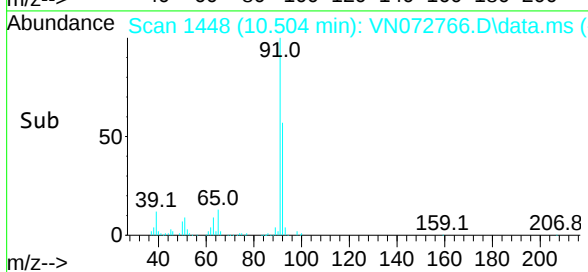
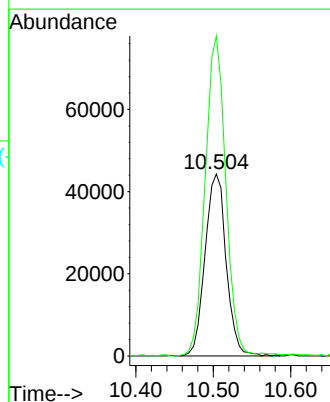
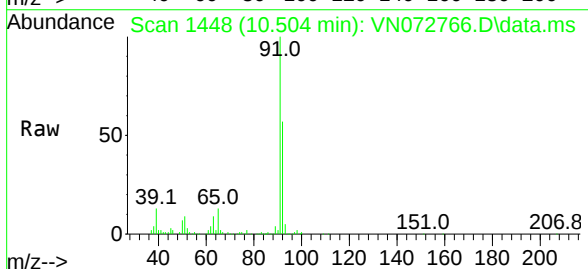


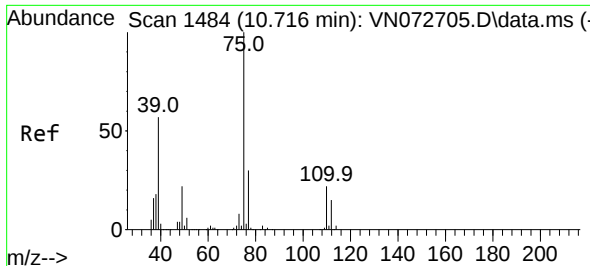

#53
t-1,3-Dichloropropene
Concen: 0.236 ug/l
RT: 10.504 min Scan# 1448
Delta R.T. -0.212 min
Lab File: VN072766.D
Acq: 10 Jun 2022 15:45




Instrument :
MSVOA_N
ClientSampleId :
40807


Tgt Ion: 75 Resp: 1359
Ion Ratio Lower Upper
75 100
77 163.5 25.6 38.4#

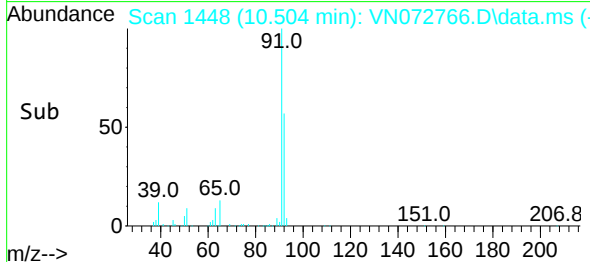

#62
4-Bromofluorobenzene
Concen: 50.519 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN072766.D
Acq: 10 Jun 2022 15:45

Tgt Ion: 95 Resp: 219196
Ion Ratio Lower Upper
95 100
174 63.4 0.0 167.6
176 61.3 0.0 163.4

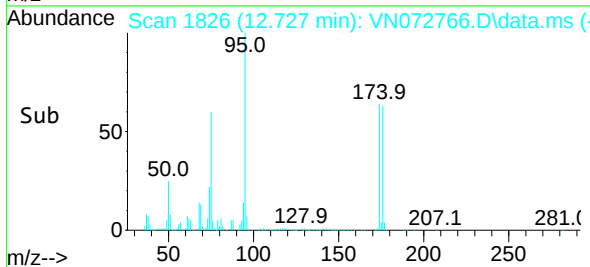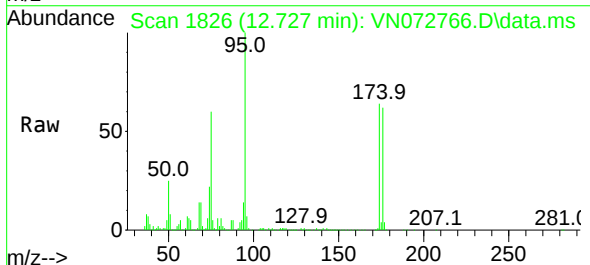



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.745 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN072766.D

Acq: 10 Jun 2022 15:45

Instrument :

MSVOA_N

ClientSampleId :

40807





Tgt Ion:117 Resp: 283413

Ion Ratio Lower Upper

117 100

82 61.7 44.2 66.2

119 32.6 25.4 38.0

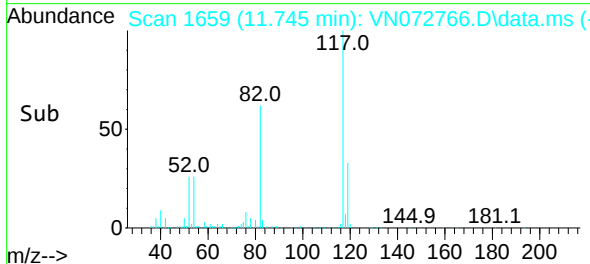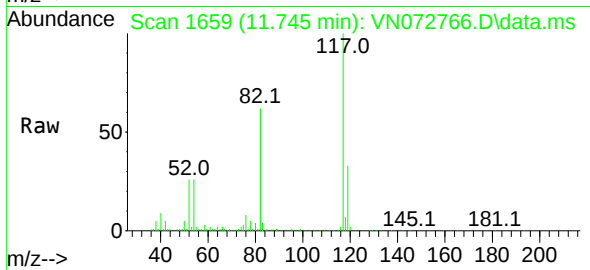

#67

Ethyl Benzene

Concen: 1.950 ug/l

RT: 11.839 min Scan# 1675

Delta R.T. -0.006 min

Lab File: VN072766.D




Acq: 10 Jun 2022 15:45


Tgt Ion: 91 Resp: 27695

Ion Ratio Lower Upper

91 100

106 30.8 24.9 37.3


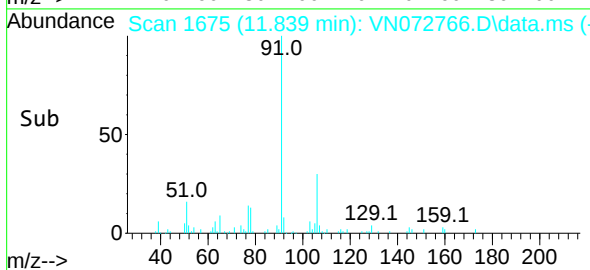

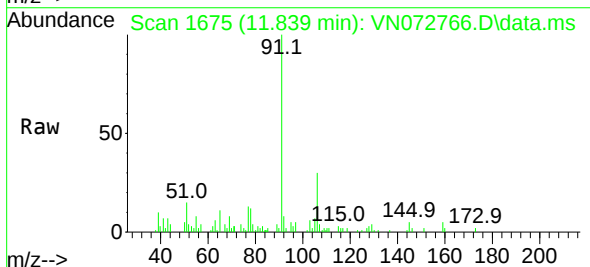


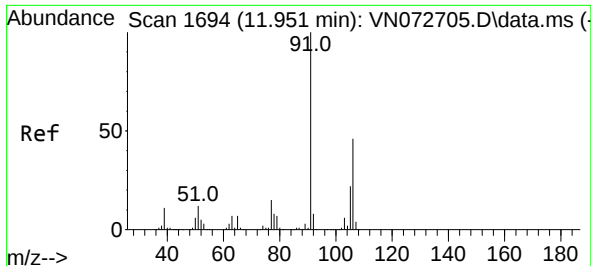

#68
m/p-Xylenes
Concen: 7.350 ug/l
RT: 11.945 min Scan# 1194
Delta R.T. -0.006 min
Lab File: VN072766.D
Acq: 10 Jun 2022 15:45




Instrument :
MSVOA_N
ClientSampleId :
40807


Tgt Ion:106 Resp: 37089
Ion Ratio Lower Upper
106 100
91 221.9 158.9 238.3

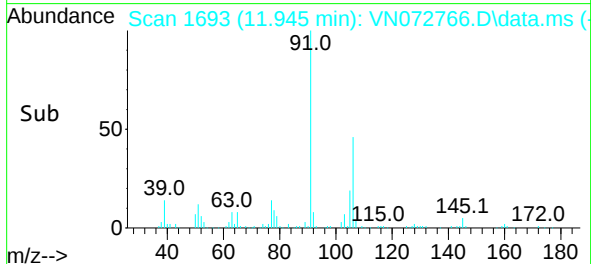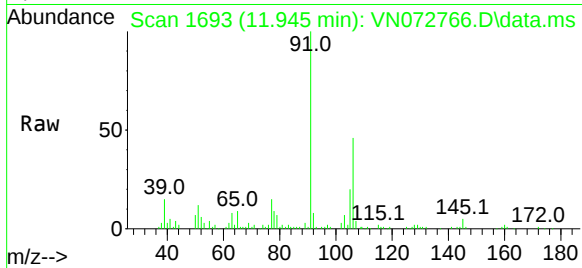

#69
o-Xylene
Concen: 4.798 ug/l
RT: 12.274 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VN072766.D
Acq: 10 Jun 2022 15:45

Tgt Ion:106 Resp: 24341
Ion Ratio Lower Upper
106 100
91 223.6 106.0 318.0



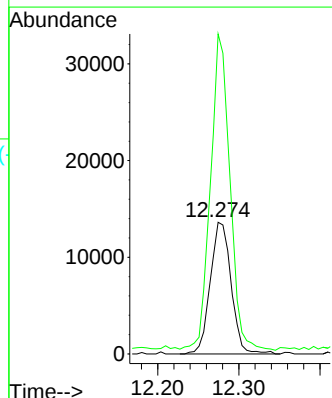
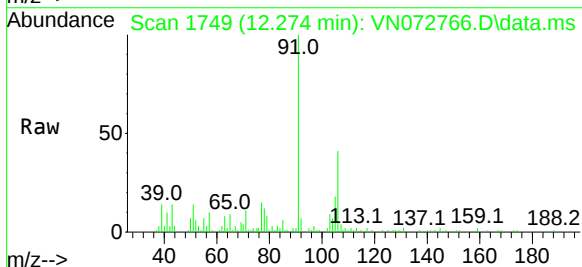


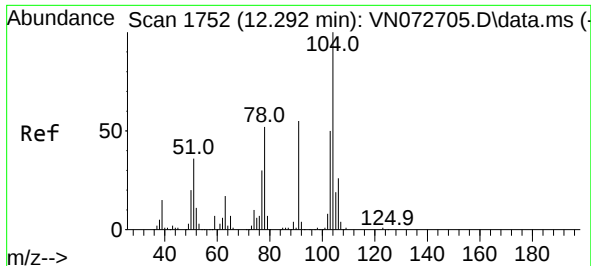

#70
Styrene
Concen: 1.686 ug/l
RT: 12.292 min Scan# 1752
Delta R.T. 0.000 min
Lab File: VN072766.D
Acq: 10 Jun 2022 15:45




Instrument :
MSVOA_N
ClientSampleId :
40807


Tgt Ion	Ratio	Lower	Upper
104	100		
78	80.5	39.5	59.3#
103	76.6	44.0	66.0#

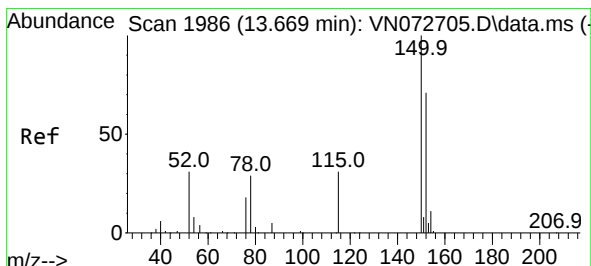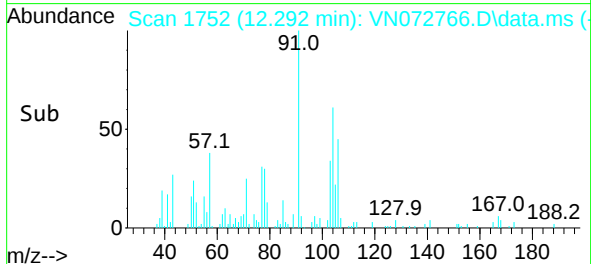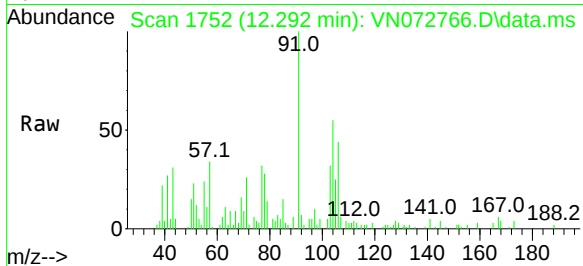

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.674 min Scan# 1987
Delta R.T. 0.005 min
Lab File: VN072766.D
Acq: 10 Jun 2022 15:45

Tgt Ion	Ratio	Lower	Upper
152	100		
115	70.0	28.9	86.7
150	154.9	0.0	356.2

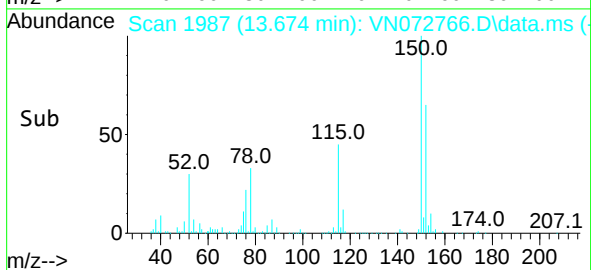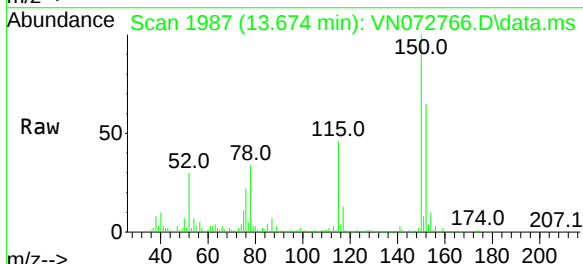



#73

Isopropylbenzene

Concen: 0.251 ug/l

RT: 12.592 min Scan# 11

Delta R.T. 0.018 min

Lab File: VN072766.D

Acq: 10 Jun 2022 15:45

Instrument :

MSVOA_N

ClientSampleId :





40807

Tgt Ion:105 Resp: 3046

Ion Ratio Lower Upper

105 100

120 16.0 13.5 40.4

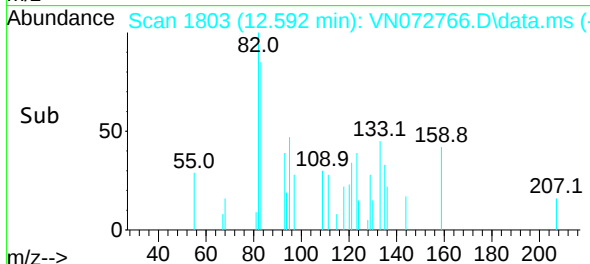

#74

N-ethyl acetate

Concen: 0.285 ug/l

RT: 12.457 min Scan# 1780

Delta R.T. 0.071 min

Lab File: VN072766.D

Acq: 10 Jun 2022 15:45

Tgt Ion: 43 Resp: 1604




Ion Ratio Lower Upper


43 100

70 39.2 39.0 58.4

55 59.6 21.1 31.7#

61 0.0 21.1 31.7#


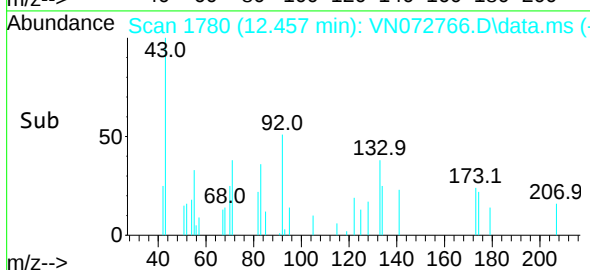

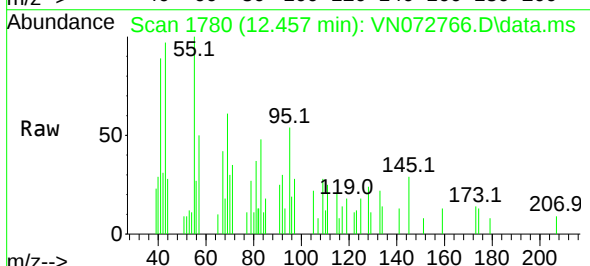


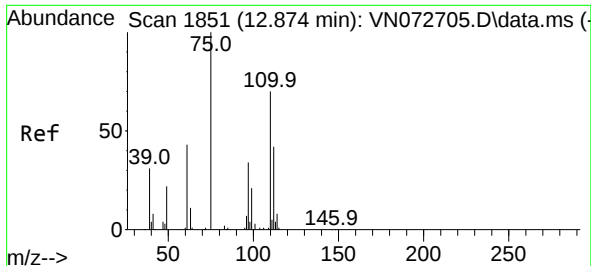

#76
1,2,3-Trichloropropane
Concen: 35.483 ug/l
RT: 12.727 min Scan# 11
Delta R.T. -0.147 min
Lab File: VN072766.D
Acq: 10 Jun 2022 15:45




Instrument :
MSVOA_N
ClientSampleId :
40807


Tgt Ion: 75 Resp: 129458
Ion Ratio Lower Upper
75 100
77 1.6 98.5 295.5#

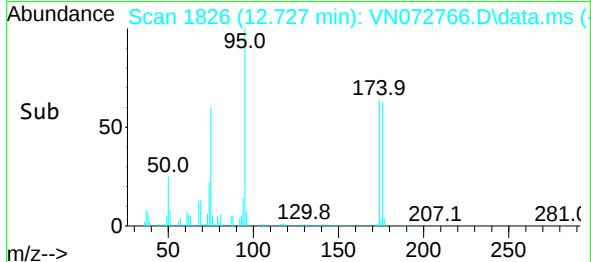

#77
Bromobenzene
Concen: 0.223 ug/l
RT: 12.880 min Scan# 1852
Delta R.T. 0.023 min
Lab File: VN072766.D
Acq: 10 Jun 2022 15:45

Tgt Ion: 156 Resp: 533
Ion Ratio Lower Upper
156 100
77 43.7 100.5 301.5#
158 0.0 48.9 146.6#


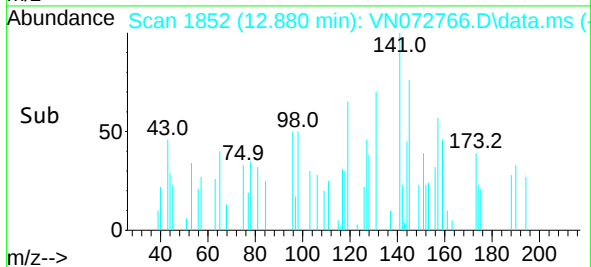

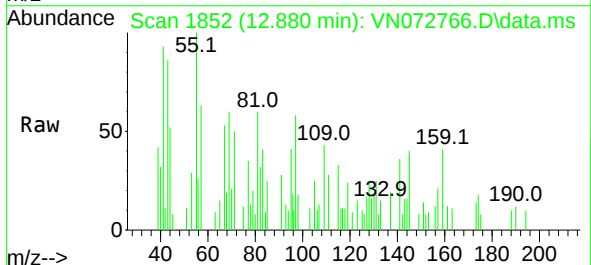


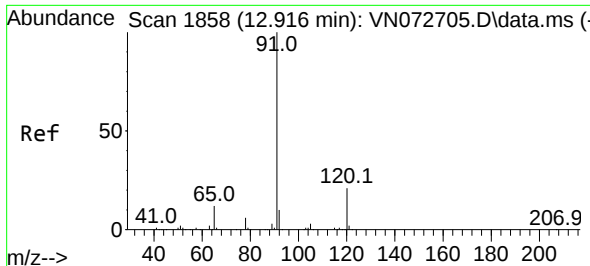

#78
n-propylbenzene
Concen: 0.454 ug/l
RT: 12.921 min Scan# 1859
Delta R.T. 0.005 min
Lab File: VN072766.D
Acq: 10 Jun 2022 15:45




Instrument :
MSVOA_N
ClientSampleId :
40807


Tgt Ion: 91 Resp: 6009
Ion Ratio Lower Upper
91 100
120 30.9 11.9 35.5

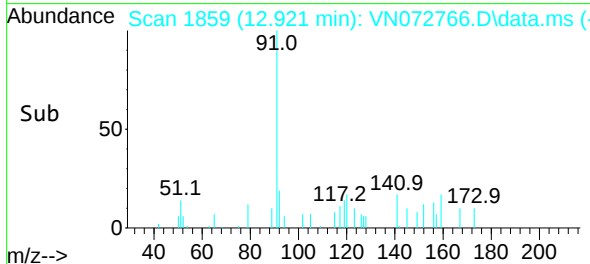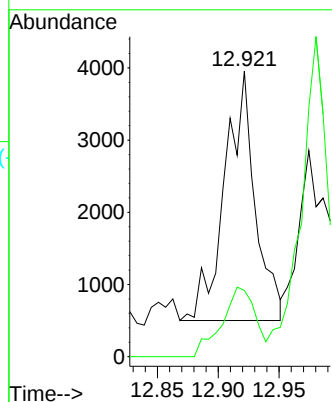

#80
1,3,5-Trimethylbenzene
Concen: 0.959 ug/l
RT: 13.057 min Scan# 1882
Delta R.T. -0.000 min
Lab File: VN072766.D
Acq: 10 Jun 2022 15:45

Tgt Ion: 105 Resp: 9220
Ion Ratio Lower Upper
105 100
120 47.5 24.9 74.7


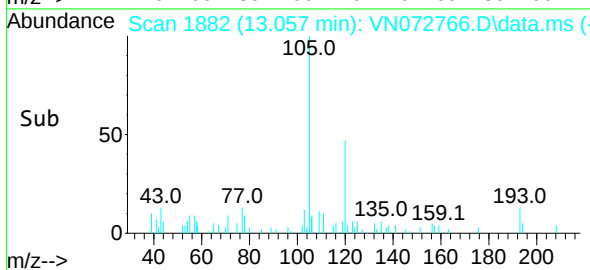
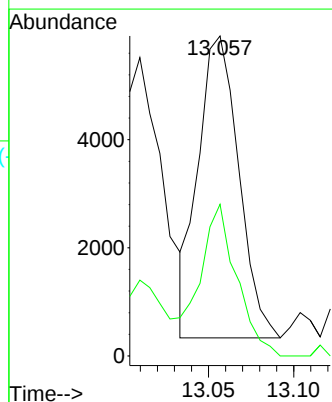
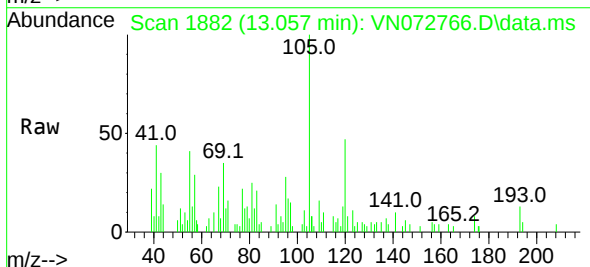


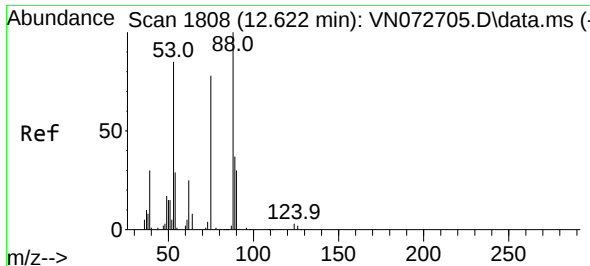

#81
trans-1,4-Dichloro-2-butene
Concen: 92.797 ug/l
RT: 12.727 min Scan# 1808
Delta R.T. 0.105 min
Lab File: VN072766.D
Acq: 10 Jun 2022 15:45




Instrument :
MSVOA_N
ClientSampleId :
40807


Tgt Ion: 75 Resp: 129458
Ion Ratio Lower Upper
75 100
53 0.2 78.0 117.0#
89 0.0 37.2 55.8#

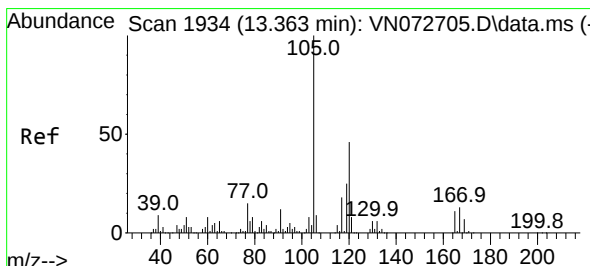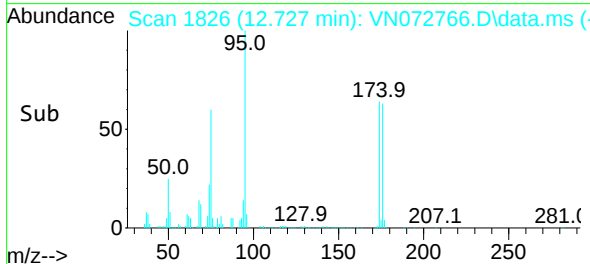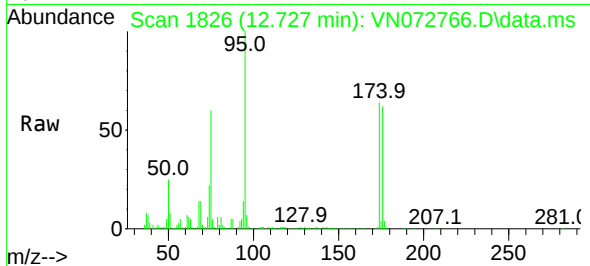

#84
1,2,4-Trimethylbenzene
Concen: 4.797 ug/l
RT: 13.368 min Scan# 1935
Delta R.T. 0.005 min
Lab File: VN072766.D
Acq: 10 Jun 2022 15:45

Tgt Ion: 105 Resp: 44106
Ion Ratio Lower Upper
105 100
120 42.1 23.3 69.8


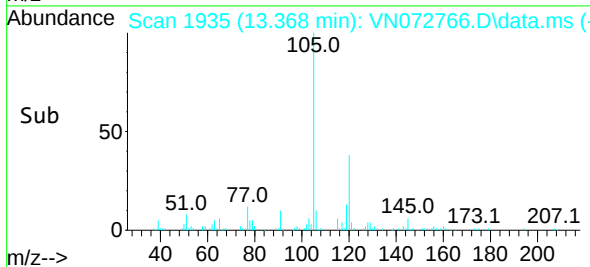

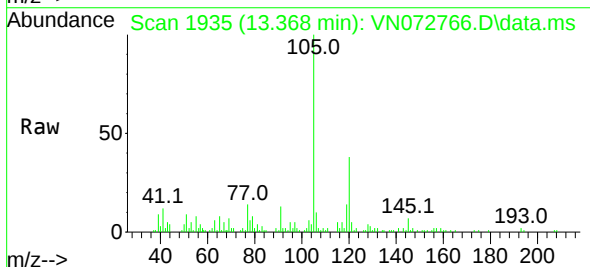


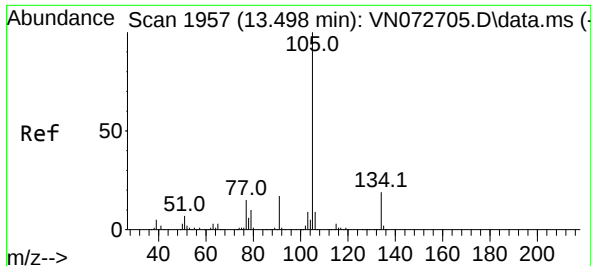

#85
 sec-Butylbenzene
 Concen: 3.873 ug/l
 RT: 13.368 min Scan# 1935
 Delta R.T. -0.130 min
 Lab File: VN072766.D
 Acq: 10 Jun 2022 15:45




Instrument :
 MSVOA_N
 ClientSampleId :
 40807


Tgt Ion:105 Resp: 44106
 Ion Ratio Lower Upper
 105 100
 134 0.1 10.4 31.1#

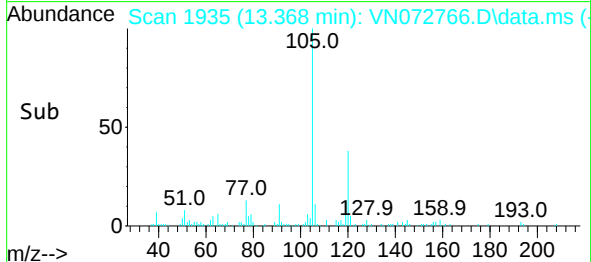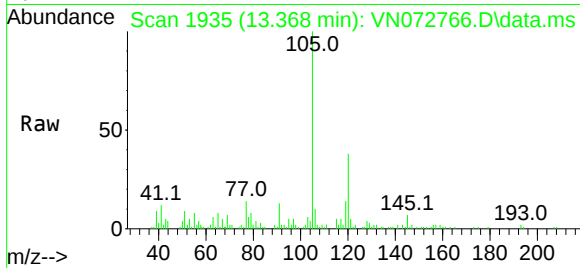

#86
 p-Isopropyltoluene
 Concen: 0.518 ug/l
 RT: 13.568 min Scan# 1969
 Delta R.T. -0.042 min
 Lab File: VN072766.D
 Acq: 10 Jun 2022 15:45

Tgt Ion:119 Resp: 4643
 Ion Ratio Lower Upper
 119 100
 134 9.4 13.3 39.8#
 91 15.4 11.3 33.9

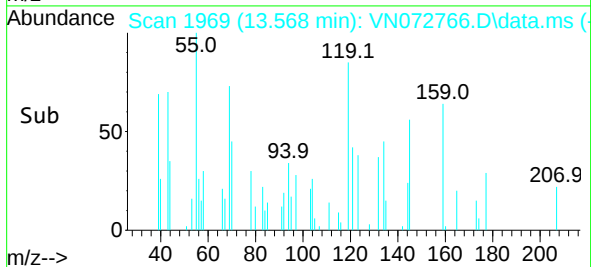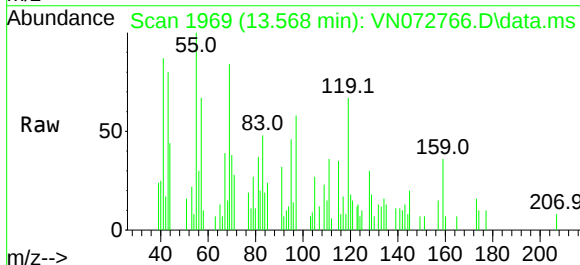



#90

Hexachloroethane

Concen: 0.445 ug/l

RT: 14.210 min Scan# 2078

Delta R.T. -0.000 min

Lab File: VN072766.D

Acq: 10 Jun 2022 15:45

Instrument :

MSVOA_N

ClientSampleId :





40807

Tgt Ion:117 Resp: 863

Ion Ratio Lower Upper

117 100

201 0.0 40.6 122.0#

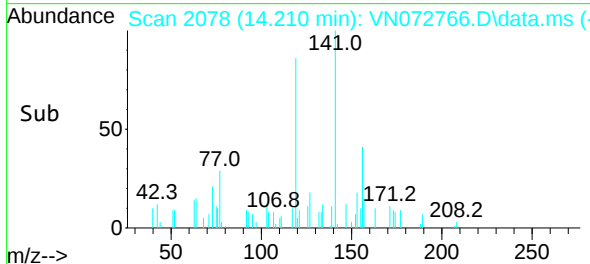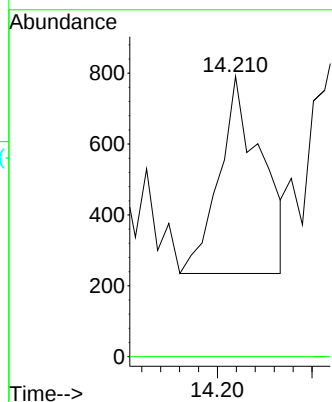

#95

Naphthalene

Concen: 4.466 ug/l

RT: 15.504 min Scan# 2298

Delta R.T. -0.000 min

Lab File: VN072766.D

Acq: 10 Jun 2022 15:45

Tgt Ion:128 Resp: 33174

Ion Ratio Lower Upper

128 100

127 16.2 10.3 15.5#

129 12.1 8.6 13.0

