

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061022\
 Data File : VN072763.D
 Acq On : 10 Jun 2022 14:32
 Operator : JC\MD
 Sample : N3287-03
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-1

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060822W.M

Title : SW846 8260

Signal : TIC: VN072763.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.240	35	43	50	rBV4	10229	27554	1.72%	0.366%
2	2.740	121	128	129	rBV4	10580	17676	1.10%	0.235%
3	4.581	433	441	451	rBV2	7429	22484	1.40%	0.299%
4	8.016	1015	1025	1031	rBV	261953	632792	39.41%	8.416%
5	8.081	1031	1036	1047	rVB	259581	577550	35.97%	7.681%
6	8.433	1086	1096	1108	rBV	304356	684689	42.64%	9.106%
7	8.963	1175	1186	1198	rBV	406399	815443	50.79%	10.845%
8	9.210	1223	1228	1238	rBV3	17780	35307	2.20%	0.470%
9	10.439	1428	1437	1454	rBV	875788	1605672	100.00%	21.356%
10	10.974	1523	1528	1534	rBV4	12070	21098	1.31%	0.281%
11	11.180	1558	1563	1574	rBV3	15667	27934	1.74%	0.372%
12	11.745	1650	1659	1671	rBV	520217	942429	58.69%	12.534%
13	12.727	1818	1826	1841	rBV	593756	1033762	64.38%	13.749%
14	13.274	1907	1919	1920	rBV5	14679	30939	1.93%	0.411%
15	13.298	1920	1923	1933	rVB9	9922	30937	1.93%	0.411%
16	13.668	1971	1986	2000	rBV	425077	841680	52.42%	11.194%
17	13.810	2005	2010	2022	rVB6	18673	58226	3.63%	0.774%
18	14.262	2077	2087	2098	rVB9	9580	39490	2.46%	0.525%
19	14.592	2140	2143	2153	rVB5	7740	18214	1.13%	0.242%
20	16.615	2477	2487	2494	rBV2	22609	54871	3.42%	0.730%




Sum of corrected areas: 7518747

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061022\
Data File : VN072763.D
Acq On : 10 Jun 2022 14:32
Operator : JC\MD
Sample : N3287-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

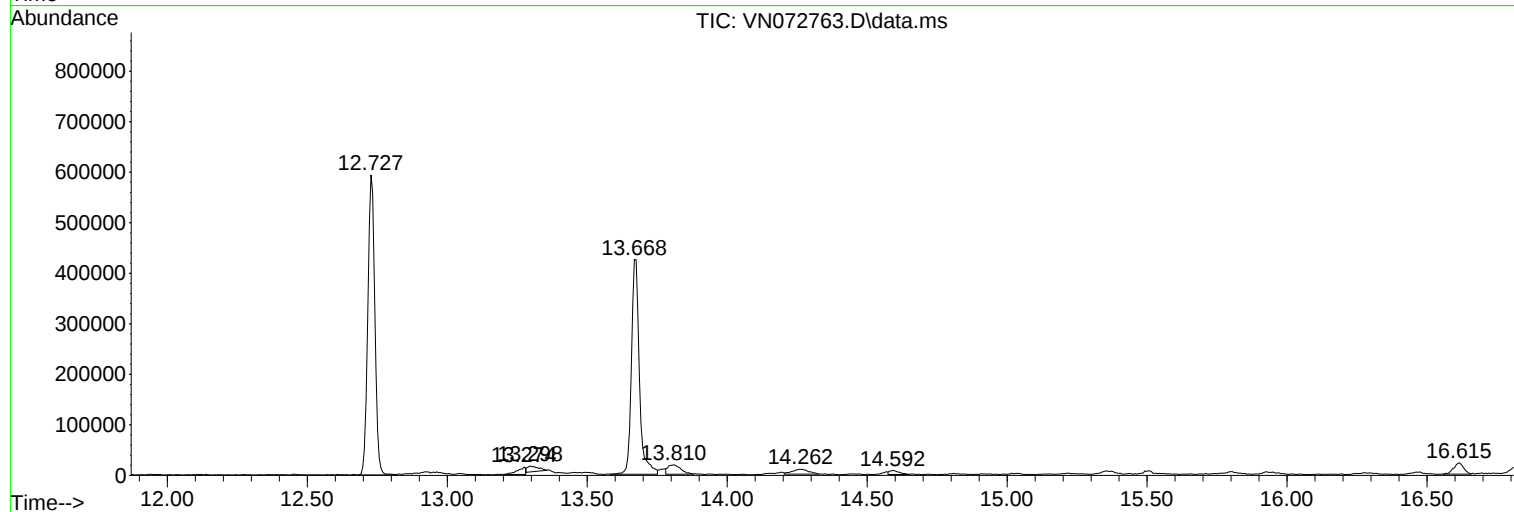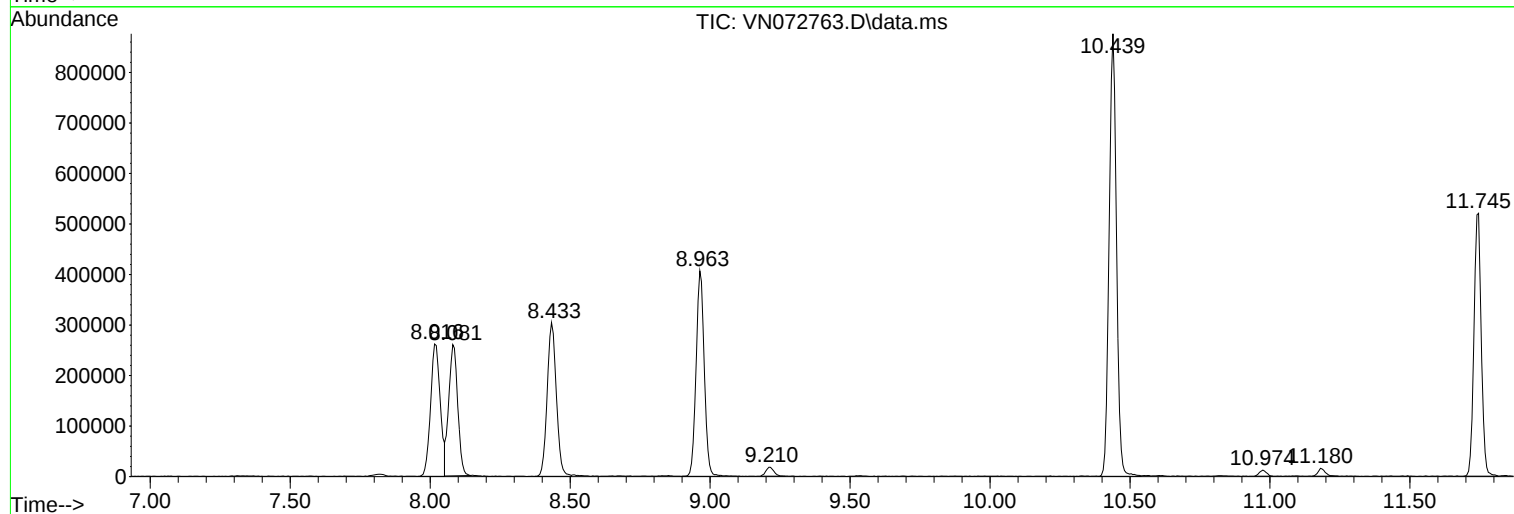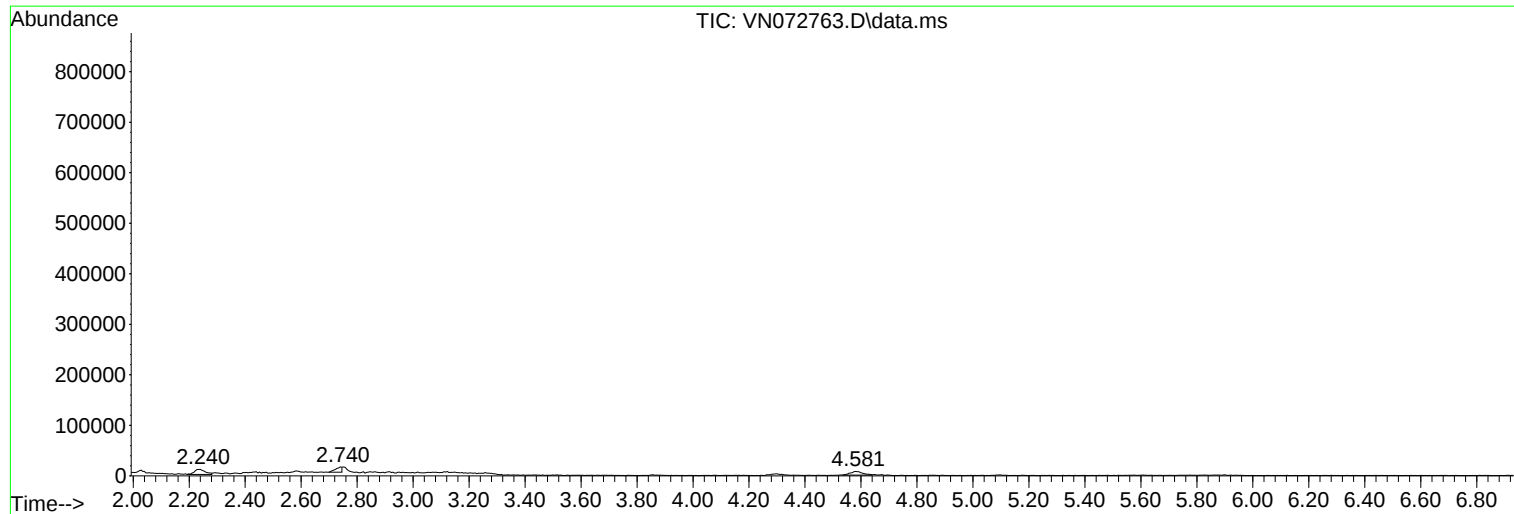

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061022\
Data File : VN072763.D
Acq On : 10 Jun 2022 14:32
Operator : JC\MD
Sample : N3287-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN061022\
Data File : VN072763.D
Acq On : 10 Jun 2022 14:32
Operator : JC\MD
Sample : N3287-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N060822W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc